

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042319\
 Data File : FG004803.D
 Signal(s) : FID1A.ch
 Acq On : 23 Apr 2019 20:42
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 24 01:56:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.399	2080373	20.169 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.624	18587	0.162 ug/ml
12) N-OCTACOSANE	16.576	69165	0.598 ug/ml
13) N-TRIACONTANE	17.466	104522	0.881 ug/ml
14) N-DOTRIACONTANE	18.300	122877	1.048 ug/ml
15) N-TETRATRIACONTANE	19.092	92662	0.832 ug/ml
16) N-HEXATRIACONTANE	19.834	79055	0.709 ug/ml
17) N-OCTATRIACONTANE	20.492f	20959	0.211 ug/ml
18) N-TETRACONTANE	21.373	92698	0.857 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042319\
Data File : FG004803.D
Signal(s) : FID1A.ch
Acq On : 23 Apr 2019 20:42
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 24 01:56:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

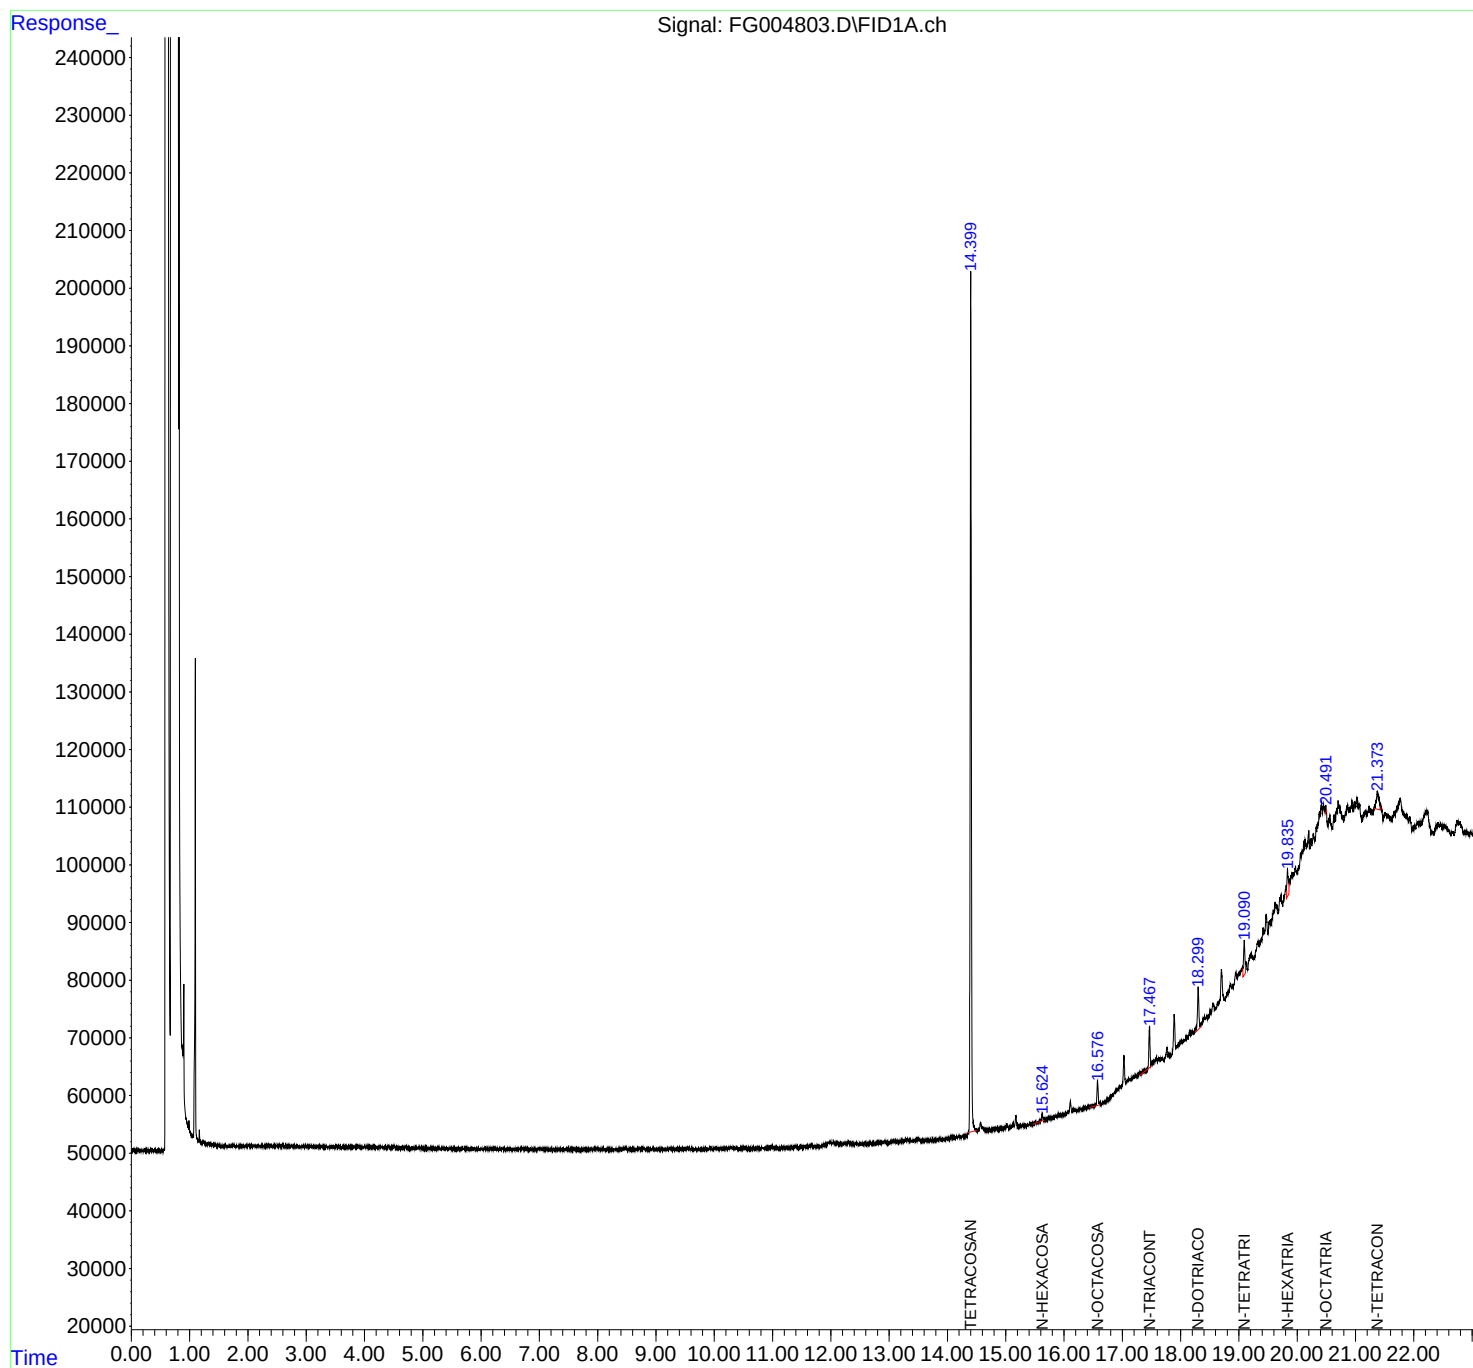


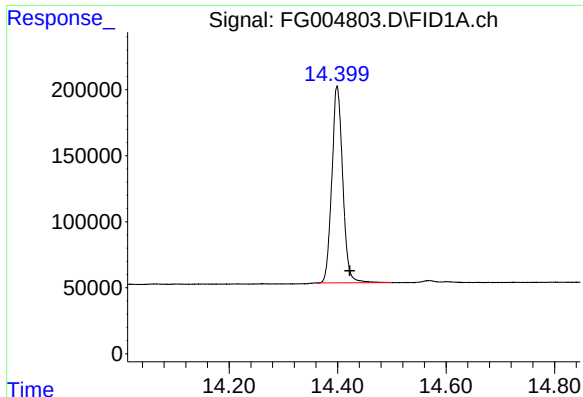

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.399 min
Delta R.T.: -0.023 min
Response: 2080373
Conc: 20.17 ug/ml

Instrument :
FID_G
ClientSampleId :

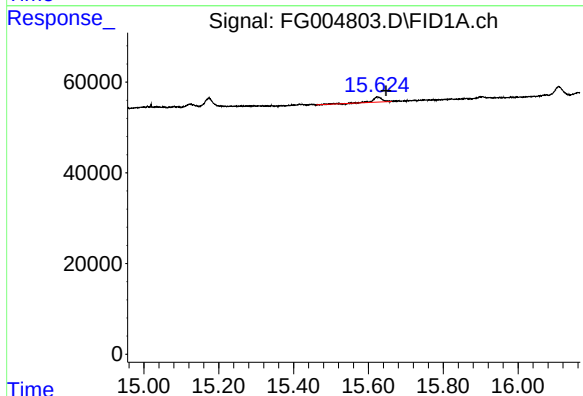


#11 N-HEXACOSANE

R.T.: 15.624 min
Delta R.T.: -0.023 min
Response: 18587
Conc: 0.16 ug/ml

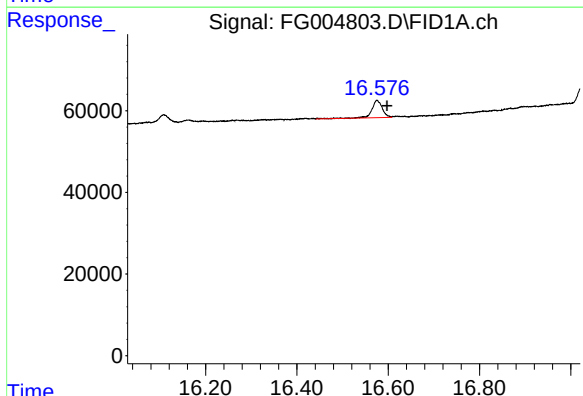


#12 N-OCTACOSANE

R.T.: 16.576 min
Delta R.T.: -0.022 min
Response: 69165
Conc: 0.60 ug/ml

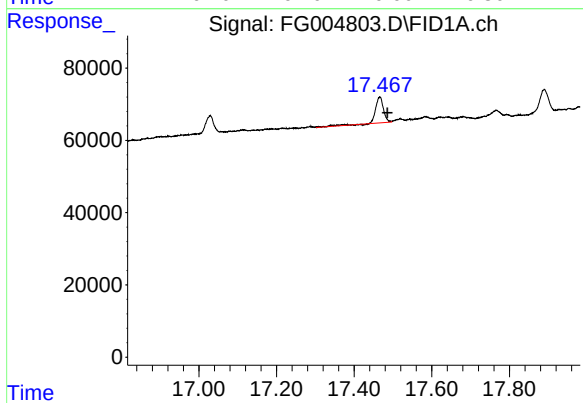

#13 N-TRIACONTANE


R.T.: 17.466 min
Delta R.T.: -0.020 min
Response: 104522
Conc: 0.88 ug/ml

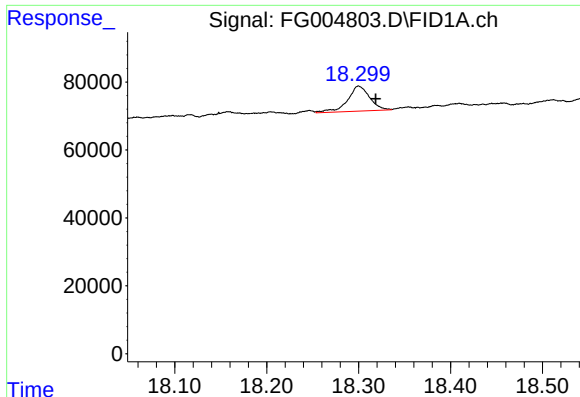

#14 N-DOTRIACONTANE


R.T.: 18.300 min
Delta R.T.: -0.018 min
Response: 122877
Conc: 1.05 ug/ml

Instrument :
FID_G
ClientSampleId :

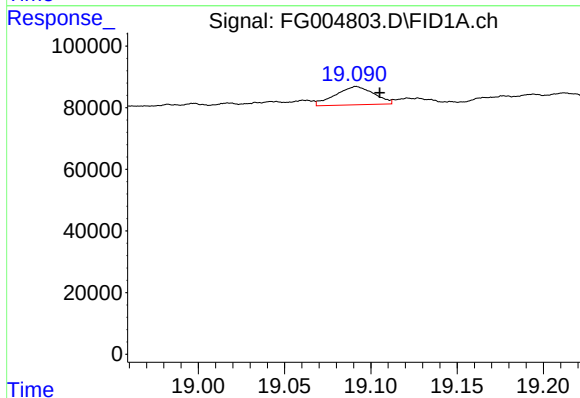


#15 N-TETRATRIACONTANE

R.T.: 19.092 min
Delta R.T.: -0.013 min
Response: 92662
Conc: 0.83 ug/ml

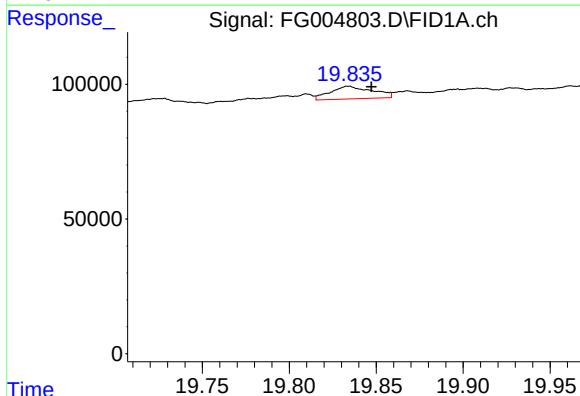


#16 N-HEXATRIACONTANE

R.T.: 19.834 min
Delta R.T.: -0.013 min
Response: 79055
Conc: 0.71 ug/ml

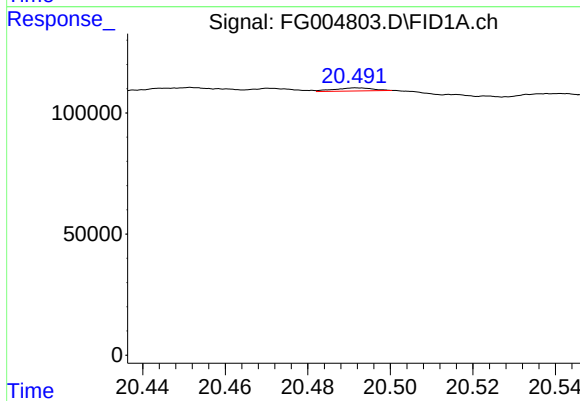

#17 N-OCTATRIACONTANE

R.T.: 20.492 min
Delta R.T.: -0.067 min
Response: 20959
Conc: 0.21 ug/ml

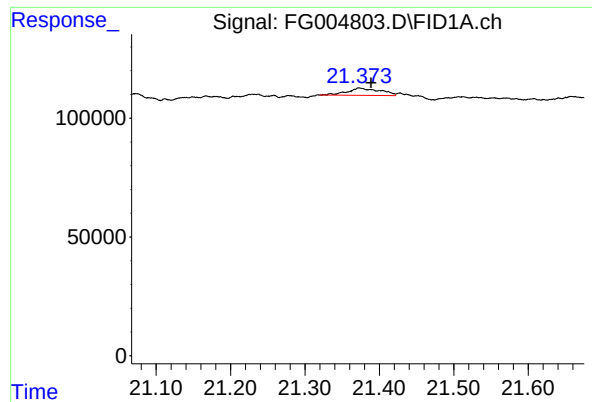

#18 N-TETRACONTANE

R.T.: 21.373 min
Delta R.T.: -0.016 min
Response: 92698
Conc: 0.86 ug/ml

Instrument :
FID_G
ClientSampleId :