

Data Path : P:\HPCHEM1\FID_G\Data\FG042418\
 Data File : FG000813.D
 Signal(s) : FID1A.ch
 Acq On : 24 Apr 2018 12:37
 Operator : UA\AJ
 Sample : J2500-01 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 24 14:08:41 2018
 Quant Method : P:\HPCHEM1\FID_G\Method\FG042318.M
 Quant Title :
 QLast Update : Mon Apr 23 17:37:23 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.541	609708	4.222 ug/ml
Target Compounds			
5) N-HEXADECANE	9.697	178043	1.064 ug/ml
7) N-EICOSANE	12.489	2887004	17.367 ug/ml
10) N-TETRACOSANE	14.702	1154829	7.109 ug/ml
12) N-OCTACOSANE	16.697	356741	2.216 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG042418\
Data File : FG000813.D
Signal(s) : FID1A.ch
Acq On : 24 Apr 2018 12:37
Operator : UA\AJ
Sample : J2500-01 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 24 14:08:41 2018
Quant Method : P:\HPCHEM1\FID_G\Method\FG042318.M
Quant Title :
QLast Update : Mon Apr 23 17:37:23 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

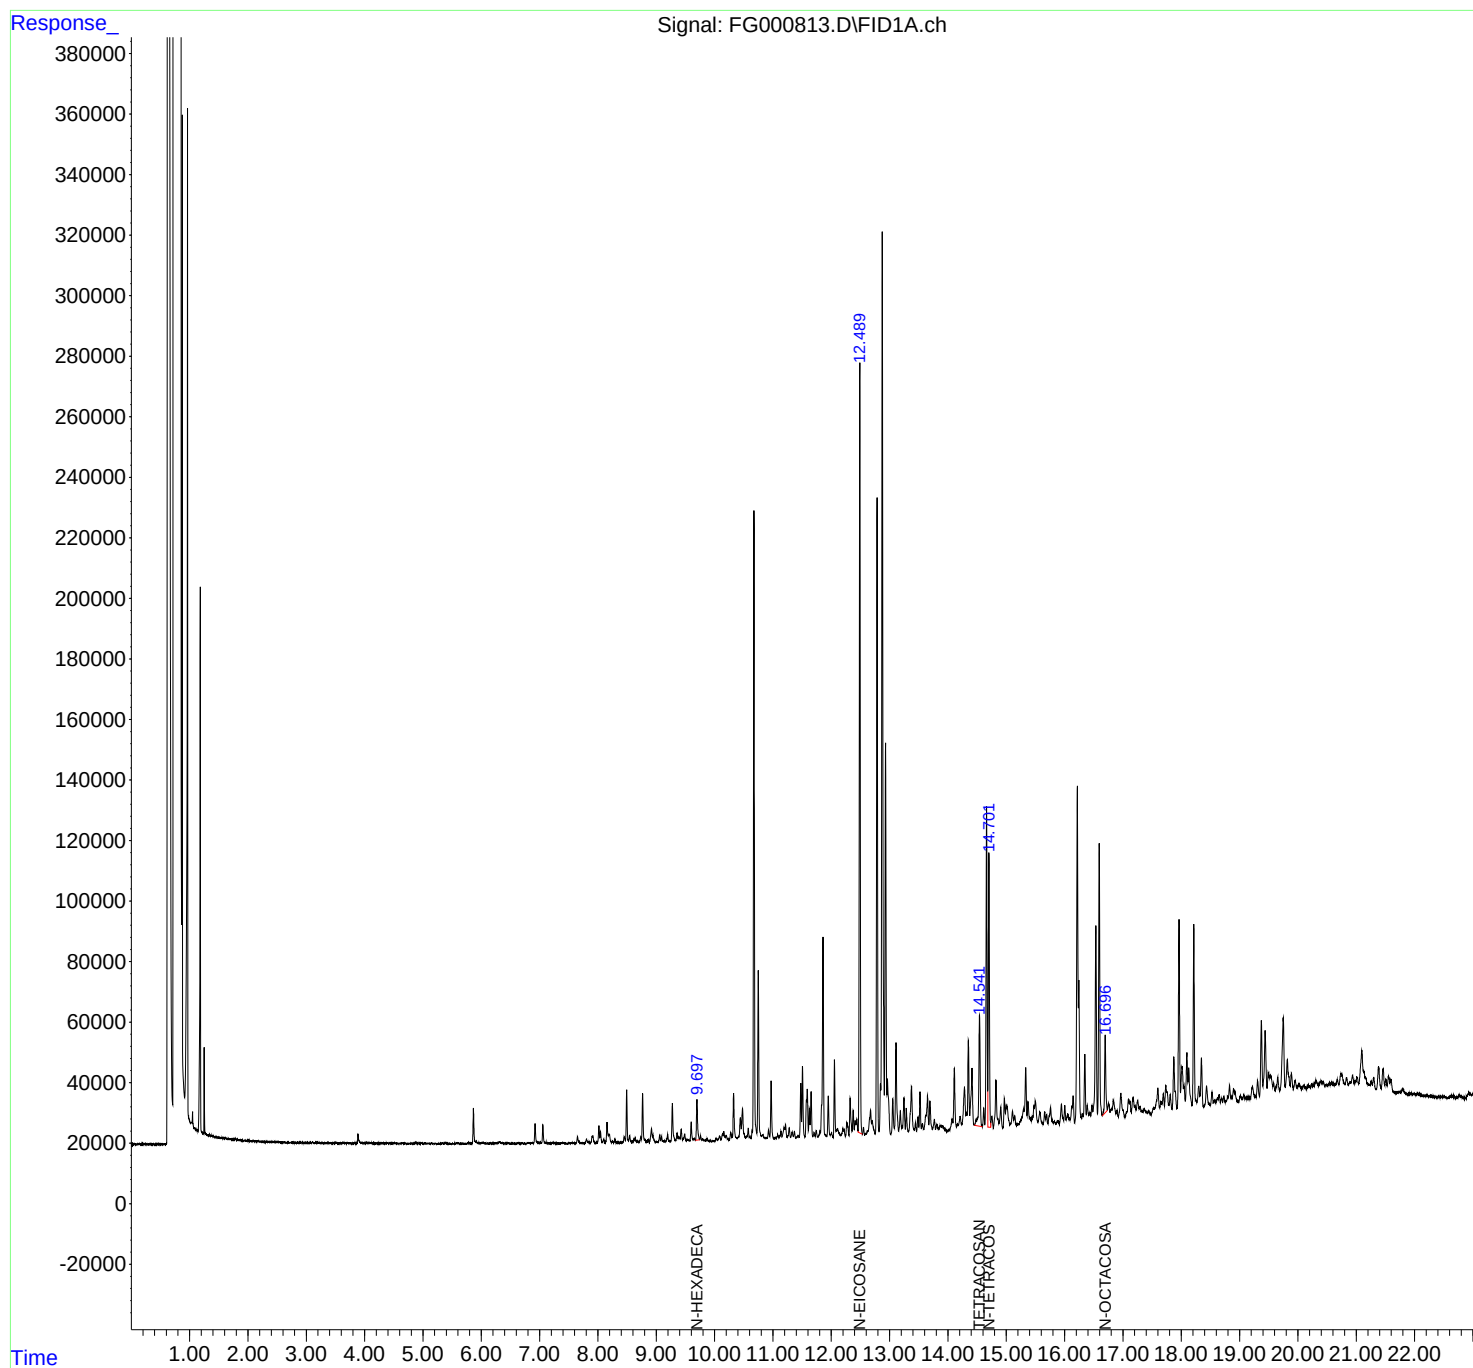


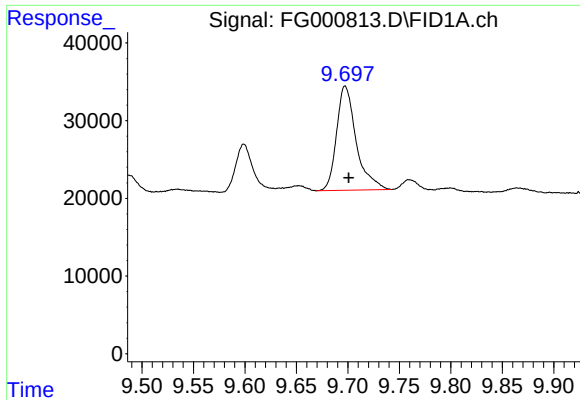

#5 N-HEXADECANE


R.T.: 9.697 min
Delta R.T.: -0.003 min
Response: 178043
Conc: 1.06 ug/ml

Instrument :
FID_G
ClientSampleId :

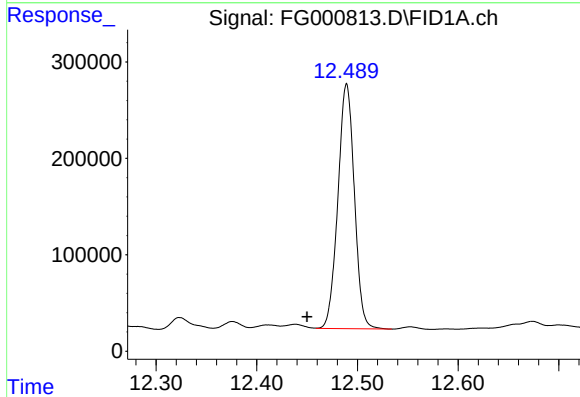


#7 N-EICOSANE

R.T.: 12.489 min
Delta R.T.: 0.039 min
Response: 2887004
Conc: 17.37 ug/ml

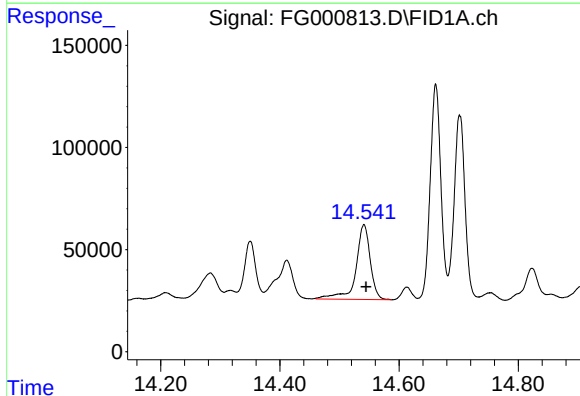


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.541 min
Delta R.T.: -0.004 min
Response: 609708
Conc: 4.22 ug/ml

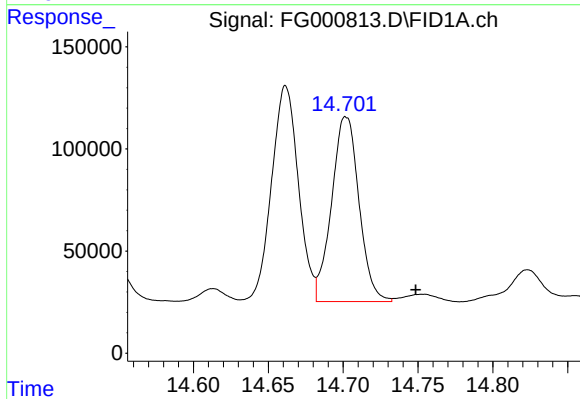

#10 N-TETRACOSANE

R.T.: 14.702 min
Delta R.T.: -0.047 min
Response: 1154829
Conc: 7.11 ug/ml

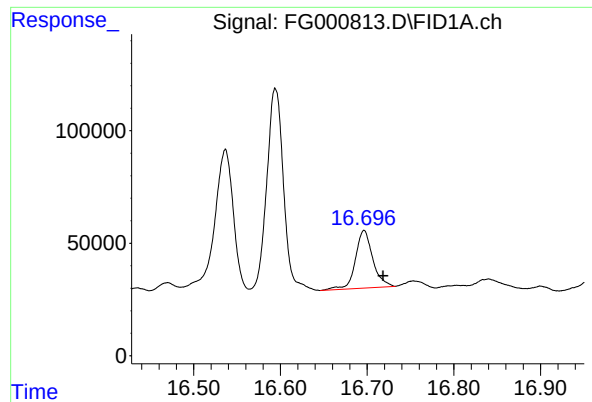

#12 N-OCTACOSANE

R.T.: 16.697 min
Delta R.T.: -0.022 min
Response: 356741
Conc: 2.22 ug/ml

Instrument :
FID_G
ClientSampleId :