

Data Path : P:\HPCHEM1\FID_G\Data\FG042418\
 Data File : FG000816.D
 Signal(s) : FID1A.ch
 Acq On : 24 Apr 2018 14:33
 Operator : UA\AJ
 Sample : J2480-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 24 15:19:31 2018
 Quant Method : P:\HPCHEM1\FID_G\Method\FG042318.M
 Quant Title :
 QLast Update : Mon Apr 23 17:37:23 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.545	4301288	29.787 ug/ml
Target Compounds			
4) N-TETRADECANE	8.156f	807749	4.895 ug/ml
5) N-HEXADECANE	9.698	1937463	11.580 ug/ml
6) N-OCTADECANE	11.141	341325	2.030 ug/ml
7) N-EICOSANE	12.452	929675	5.593 ug/ml
8) N-DOCOSANE	13.660	4296020	26.040 ug/ml
10) N-TETRACOSANE	14.764	564036	3.472 ug/ml
11) N-HEXACOSANE	15.775	885774	5.494 ug/ml
12) N-OCTACOSANE	16.718	3449734	21.430 ug/ml
13) N-TRIACONTANE	17.601	871309	5.396 ug/ml
14) N-DOTRIACONTANE	18.435	284269	1.796 ug/ml
15) N-TETRATRIACONTANE	19.220	272570	1.746 ug/ml
16) N-HEXATRIACONTANE	19.919	1034341	6.944 ug/ml
18) N-TETRACONTANE	21.559	845962	6.511 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG042418\
Data File : FG000816.D
Signal(s) : FID1A.ch
Acq On : 24 Apr 2018 14:33
Operator : UA\AJ
Sample : J2480-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Apr 24 15:19:31 2018
Quant Method : P:\HPCHEM1\FID_G\Method\FG042318.M
Quant Title :
QLast Update : Mon Apr 23 17:37:23 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

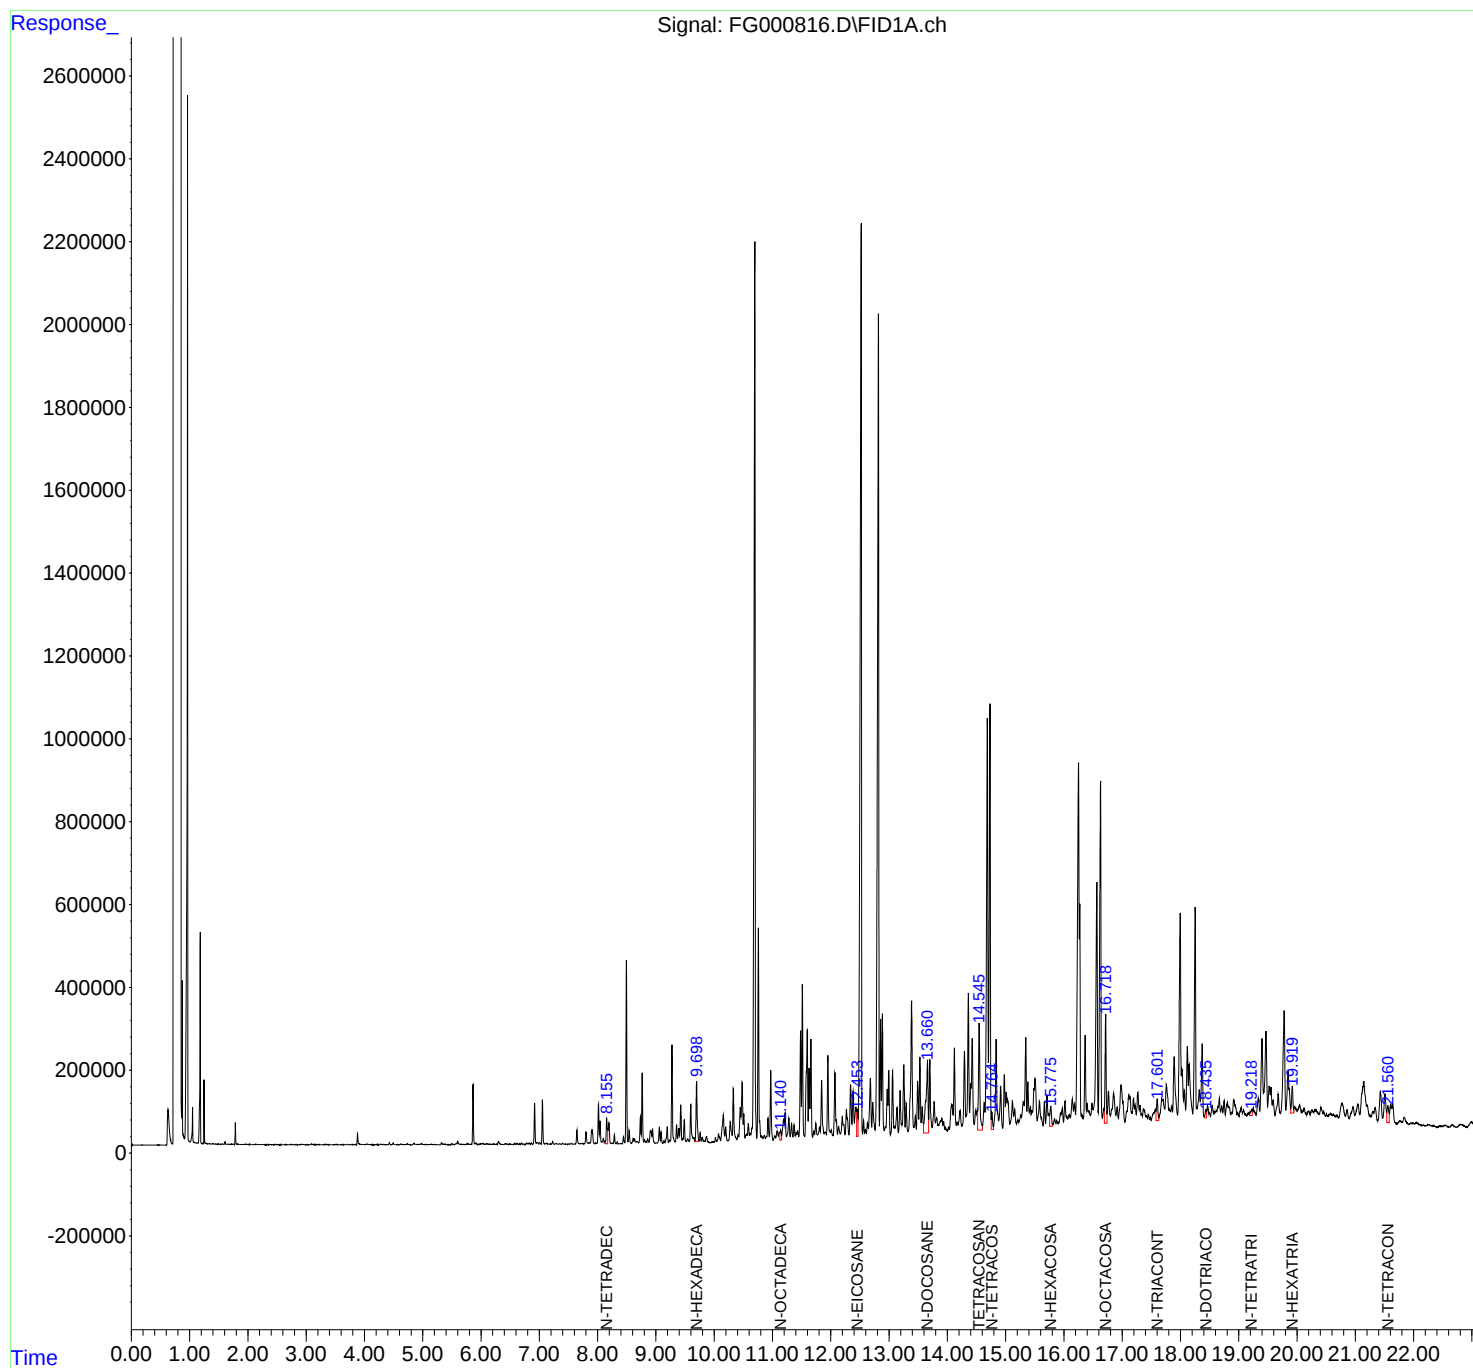


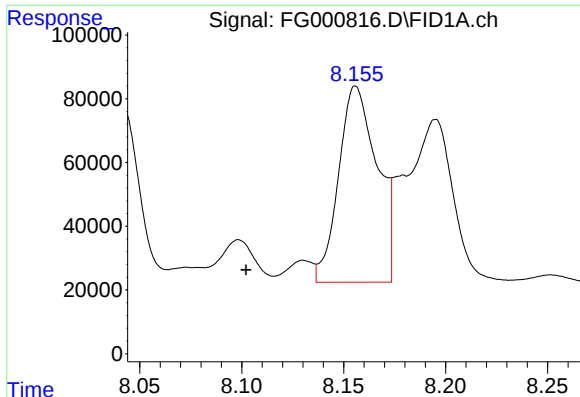

#4 N-TETRADECANE


R.T.: 8.156 min
Delta R.T.: 0.054 min
Response: 807749
Conc: 4.90 ug/ml

Instrument :
FID_G
ClientSampleId :

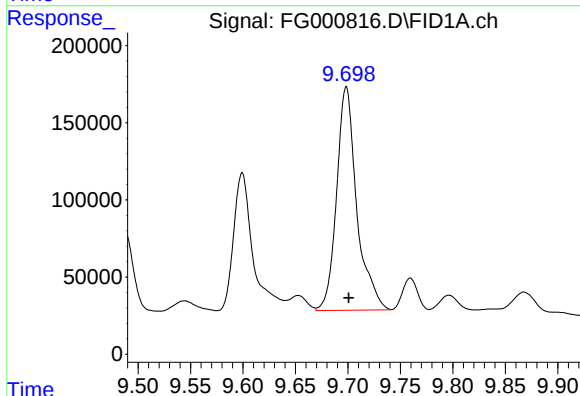


#5 N-HEXADECANE

R.T.: 9.698 min
Delta R.T.: -0.002 min
Response: 1937463
Conc: 11.58 ug/ml

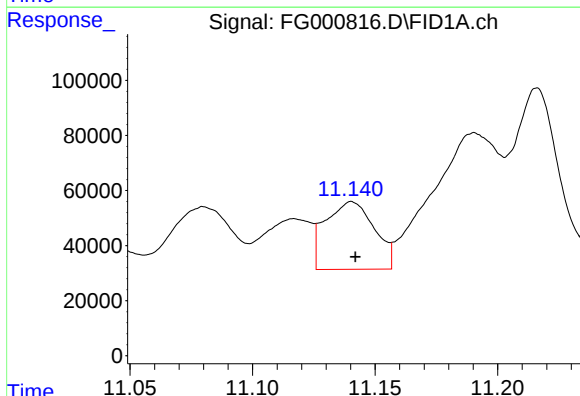


#6 N-OCTADECANE

R.T.: 11.141 min
Delta R.T.: -0.001 min
Response: 341325
Conc: 2.03 ug/ml

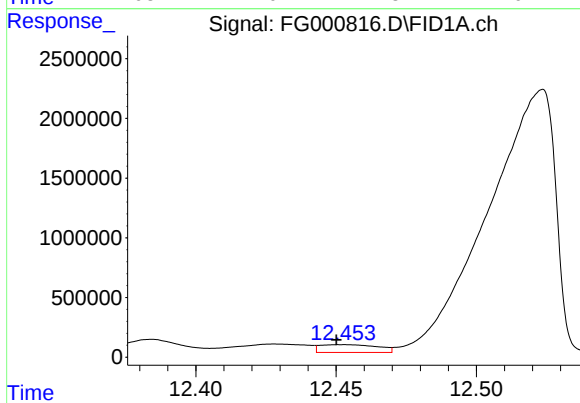

#7 N-EICOSANE


R.T.: 12.452 min
Delta R.T.: 0.002 min
Response: 929675
Conc: 5.59 ug/ml

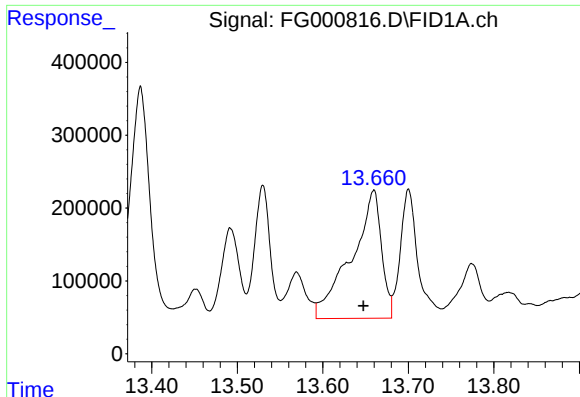

#8 N-DOCOSANE


R.T.: 13.660 min
Delta R.T.: 0.012 min
Response: 4296020
Conc: 26.04 ug/ml

Instrument :
FID_G
ClientSampleId :

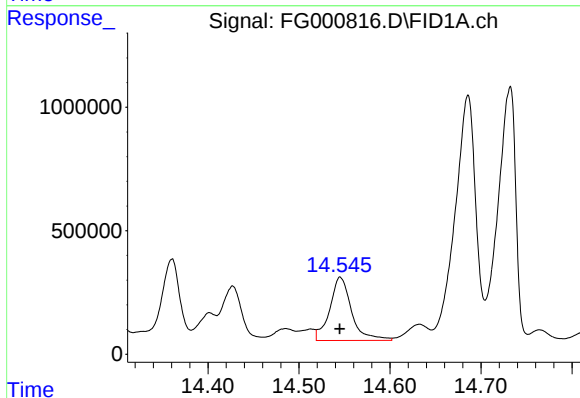


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.545 min
Delta R.T.: 0.000 min
Response: 4301288
Conc: 29.79 ug/ml

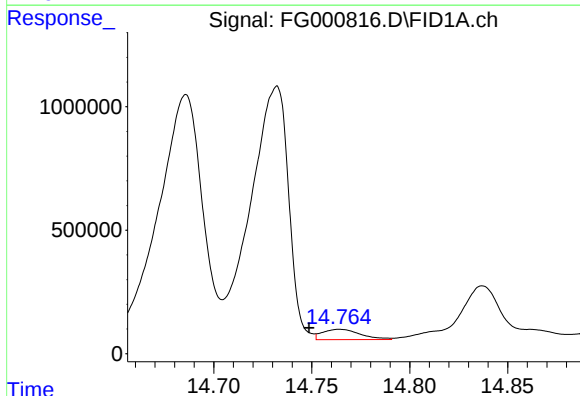


#10 N-TETRACOSANE

R.T.: 14.764 min
Delta R.T.: 0.016 min
Response: 564036
Conc: 3.47 ug/ml

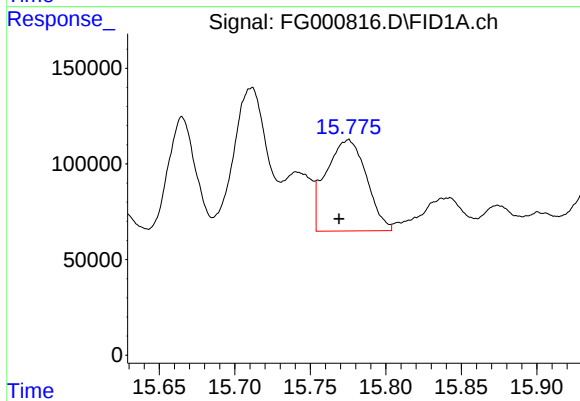

#11 N-HEXACOSANE


R.T.: 15.775 min
Delta R.T.: 0.006 min
Response: 885774
Conc: 5.49 ug/ml

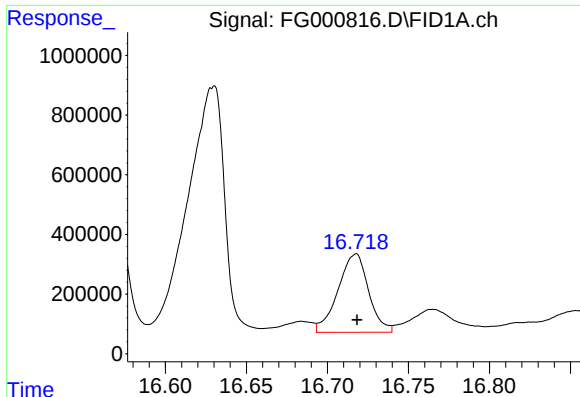

#12 N-OCTACOSANE


R.T.: 16.718 min
Delta R.T.: 0.000 min
Response: 3449734
Conc: 21.43 ug/ml

Instrument :
FID_G
ClientSampleId :

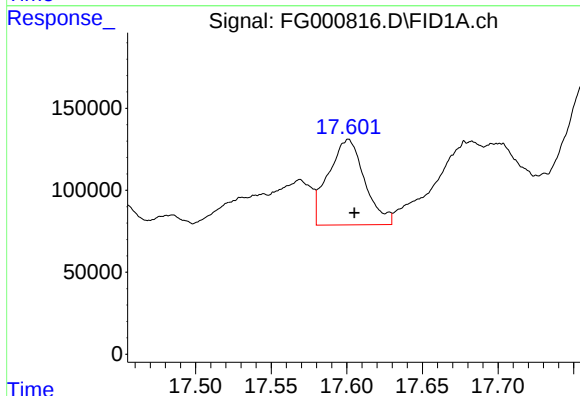


#13 N-TRIACONTANE

R.T.: 17.601 min
Delta R.T.: -0.004 min
Response: 871309
Conc: 5.40 ug/ml

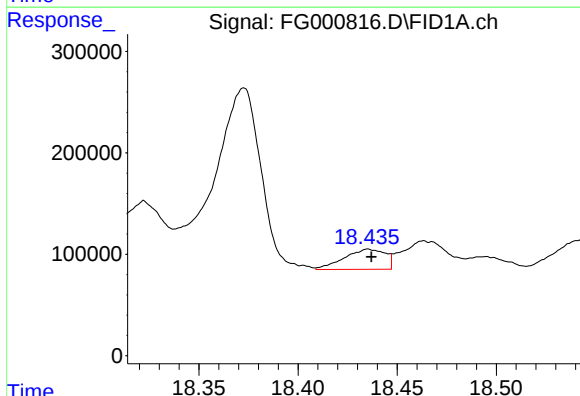


#14 N-DOTRIACONTANE

R.T.: 18.435 min
Delta R.T.: -0.001 min
Response: 284269
Conc: 1.80 ug/ml

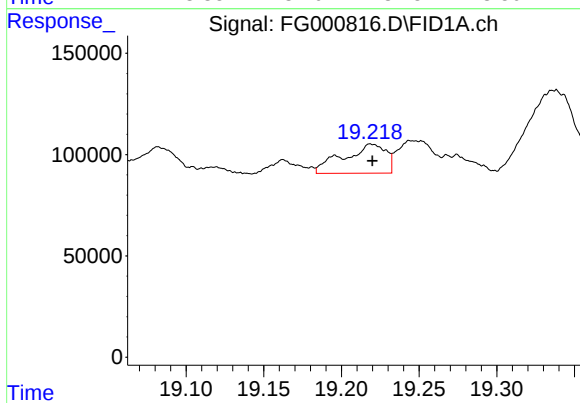

#15 N-TETRATRIACONTANE


R.T.: 19.220 min
Delta R.T.: 0.000 min
Response: 272570
Conc: 1.75 ug/ml

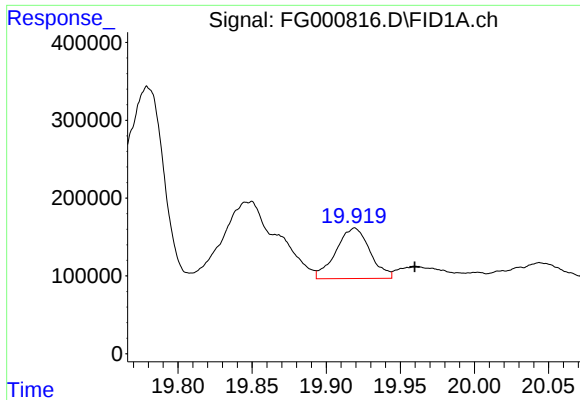

#16 N-HEXATRIACONTANE

R.T.: 19.919 min
Delta R.T.: -0.041 min
Response: 1034341
Conc: 6.94 ug/ml

Instrument :
FID_G
ClientSampleId :

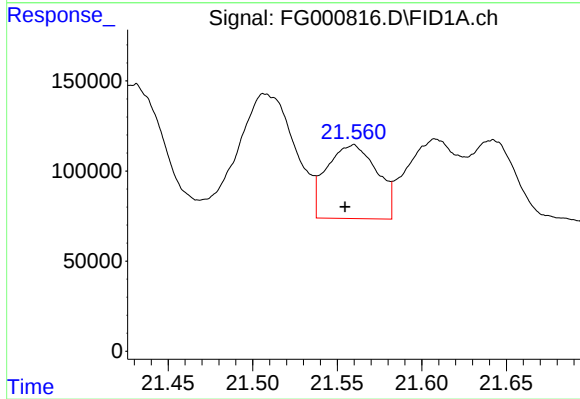

#18 N-TETRACONTANE

R.T.: 21.559 min
Delta R.T.: 0.004 min
Response: 845962
Conc: 6.51 ug/ml