

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062122\
Data File : FG009923.D
Signal(s) : FID1A.ch
Acq On : 21 Jun 2022 16:15
Operator : AJ\MA
Sample : N3383-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 22 01:16:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.830	1429263	13.579 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.076	84862	0.724 ug/ml
13) N-TRIACONTANE	17.901	115499	1.073 ug/ml
14) N-DOTRIACONTANE	18.737	161230	1.532 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062122\
Data File : FG009923.D
Signal(s) : FID1A.ch
Acq On : 21 Jun 2022 16:15
Operator : AJ\MA
Sample : N3383-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 22 01:16:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

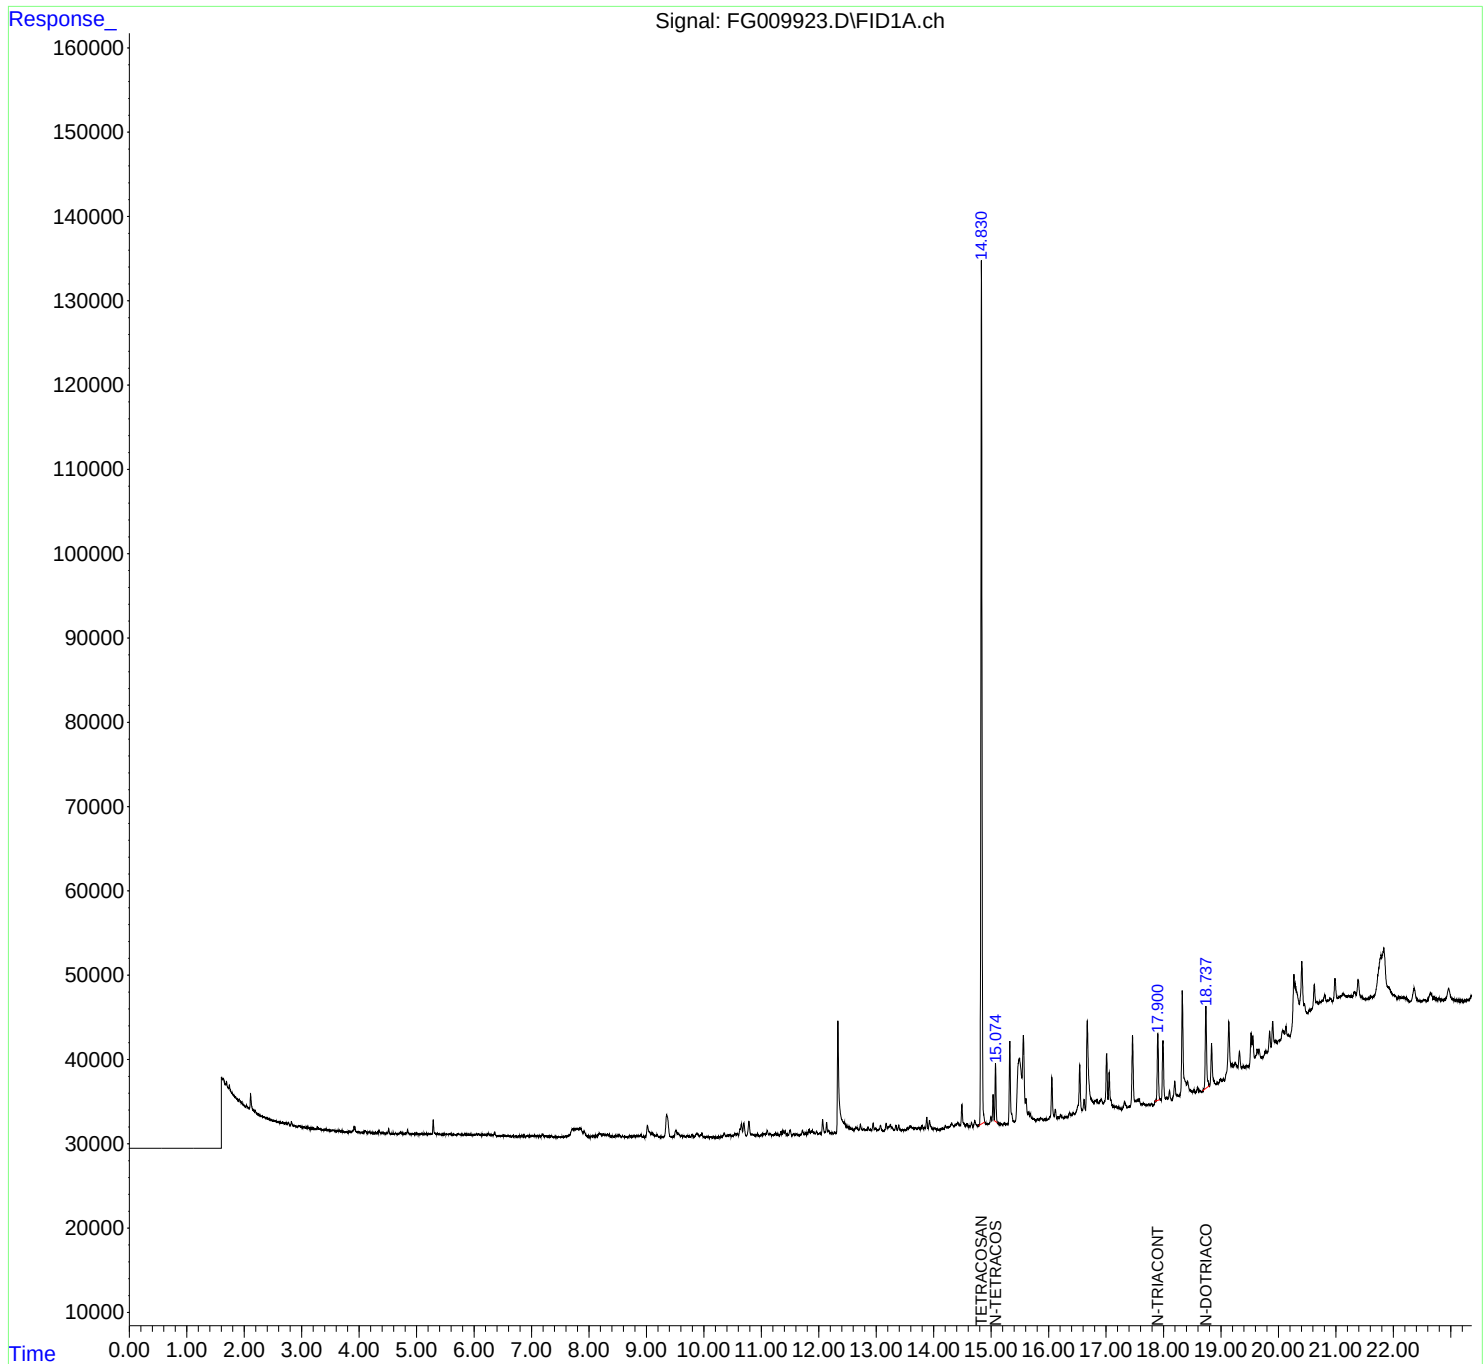


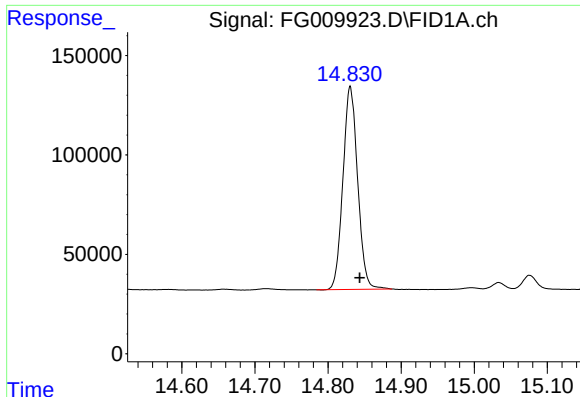

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.830 min
Delta R.T.: -0.013 min
Response: 1429263
Conc: 13.58 ug/ml

Instrument :
FID_G
ClientSampleId :

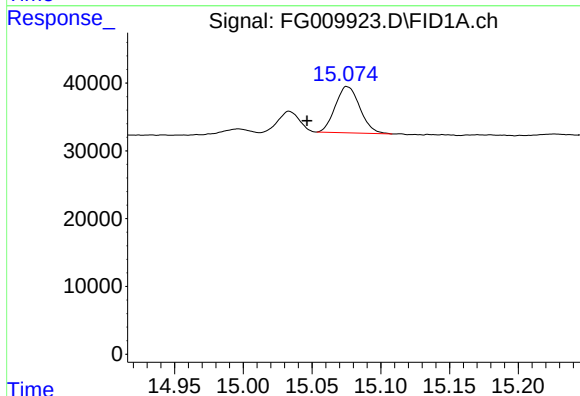


#10 N-TETRACOSANE

R.T.: 15.076 min
Delta R.T.: 0.029 min
Response: 84862
Conc: 0.72 ug/ml

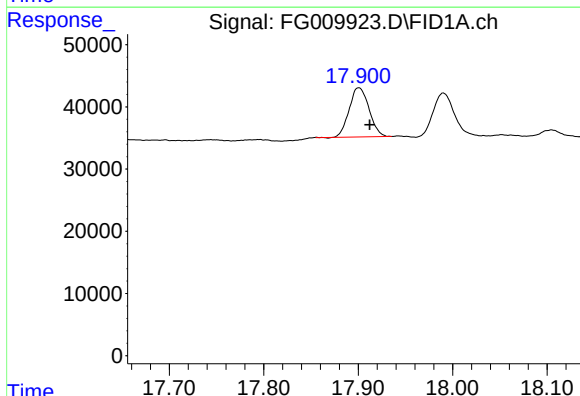

#13 N-TRIACONTANE

R.T.: 17.901 min
Delta R.T.: -0.012 min
Response: 115499
Conc: 1.07 ug/ml

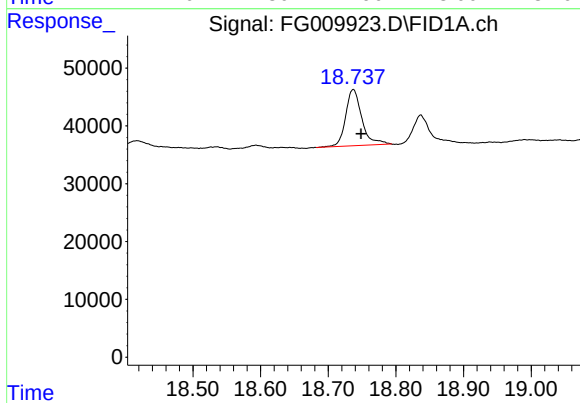

#14 N-DOTRIACONTANE

R.T.: 18.737 min
Delta R.T.: -0.011 min
Response: 161230
Conc: 1.53 ug/ml