

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062122\
Data File : FG009922.D
Signal(s) : FID1A.ch
Acq On : 21 Jun 2022 15:09
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 22 01:15:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.526	2705969	21.449 ug/ml
12)	N-OCTACOSANE	17.011	2550228	22.286 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062122\
Data File : FG009922.D
Signal(s) : FID1A.ch
Acq On : 21 Jun 2022 15:09
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 22 01:15:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

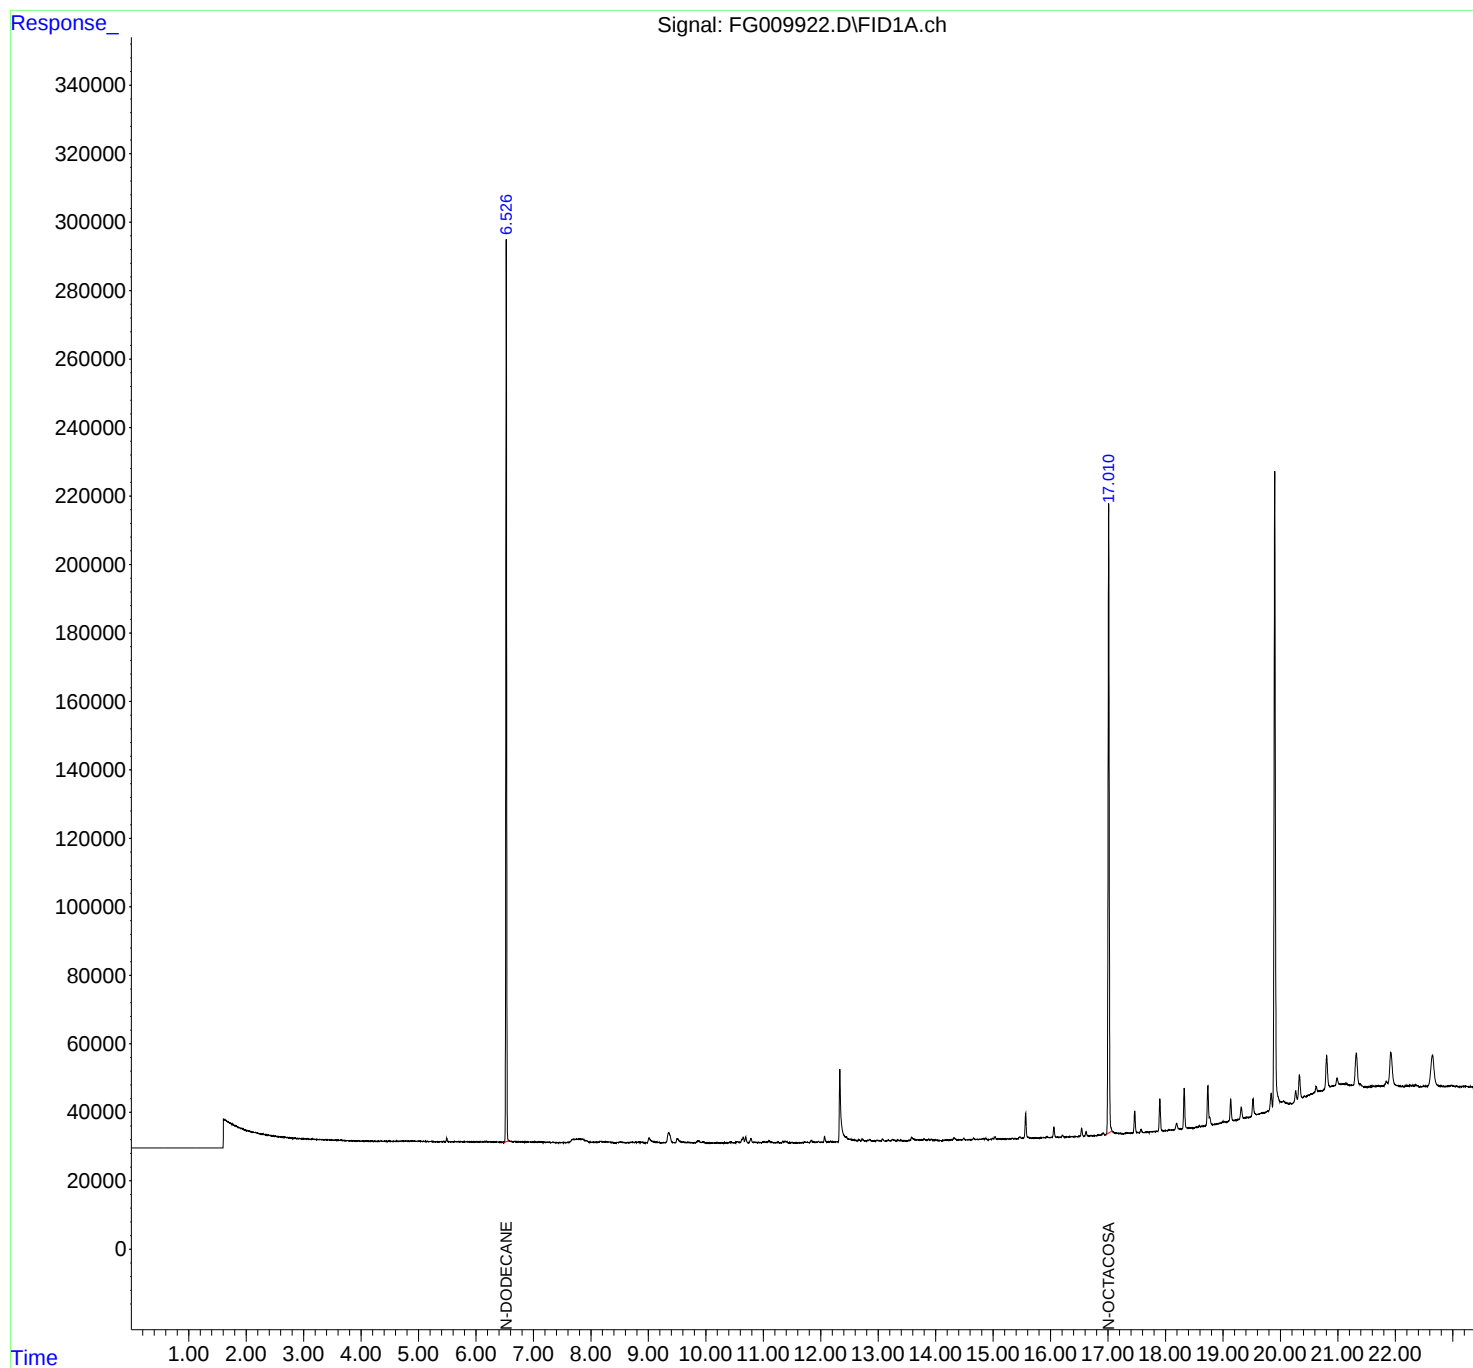


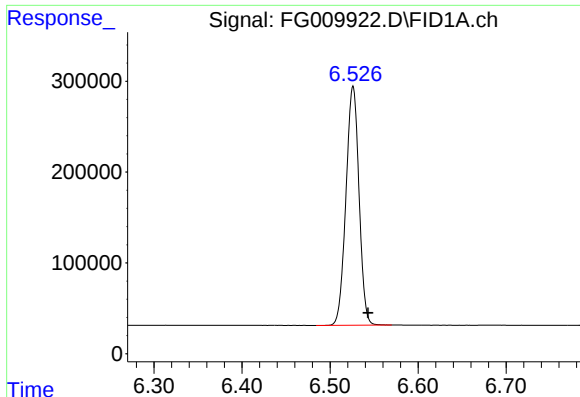

#3 N-DODECANE


R.T.: 6.526 min
Delta R.T.: -0.017 min
Response: 2705969
Conc: 21.45 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

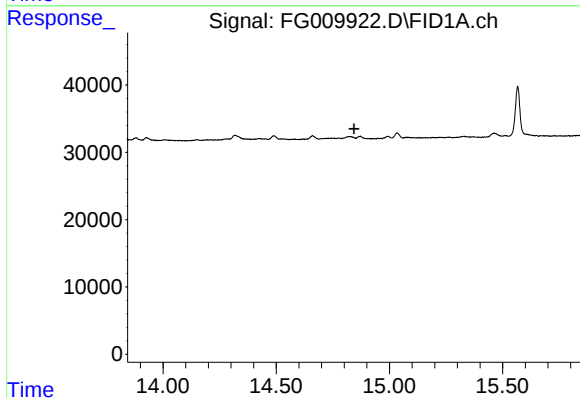

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.843 min
Response: 0
Conc: N.D.

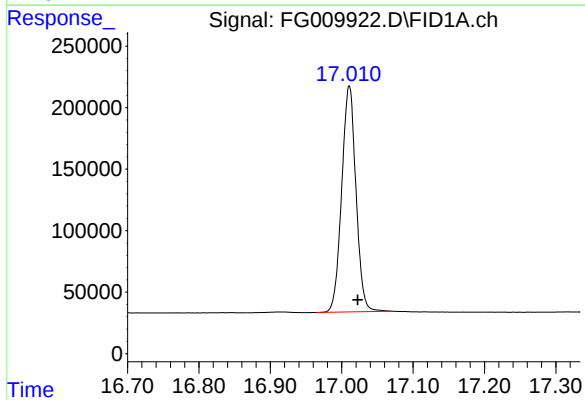

#12 N-OCTACOSANE

R.T.: 17.011 min
Delta R.T.: -0.012 min
Response: 2550228
Conc: 22.29 ug/ml