

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010219\
 Data File : PS002736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2019 16:00
 Operator : EI\SJ
 Sample : J6571-05DL 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 50084-50085-50086DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 16:34:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.389	10.881	134.6E6	80609038	424.181	208.416 #
Target Compounds							
1) T	Dalapon	2.997	2.356	3945757	18829601	8.572	41.372 #
2) T	3,5-DICHL...	9.911	9.123	13852214	8245060	28.991	17.158 #
3) T	4-Nitroph...	11.079	0.000	30259302	0	190.984	N.D. #
5) T	DICAMBA	11.734	11.223	3240.2E6	19555472	2291.559	13.717 #
6) T	MCP	12.069	11.490	27276081	13740608	27.338	14.698 #
10) T	Pentachlo...	13.622	13.305	1309.6E6	1374.2E6	261.158	261.205
11) T	2,4,5-TP ...	14.477	13.958	-302169219	516.1E6	N.D.	245.826
12) T	2,4,5-T	14.904	14.520	229063	358.3E6	0.122	209.429 #
13) T	2,4-DB	15.650	15.160	38380204	1729858	169.701	7.141 #
14) T	DINOSEB	17.077	15.580	9865484	11422536	6.779	7.485
15) T	Picloram	16.921	16.745	253.9E6	317.0E6	100.052	115.238
16) T	DCPA	17.455	0.000	250.9E6	0	103.260	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010219\
Data File : PS002736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2019 16:00
Operator : EI\SJ
Sample : J6571-05DL 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
50084-50085-50086DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 16:34:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

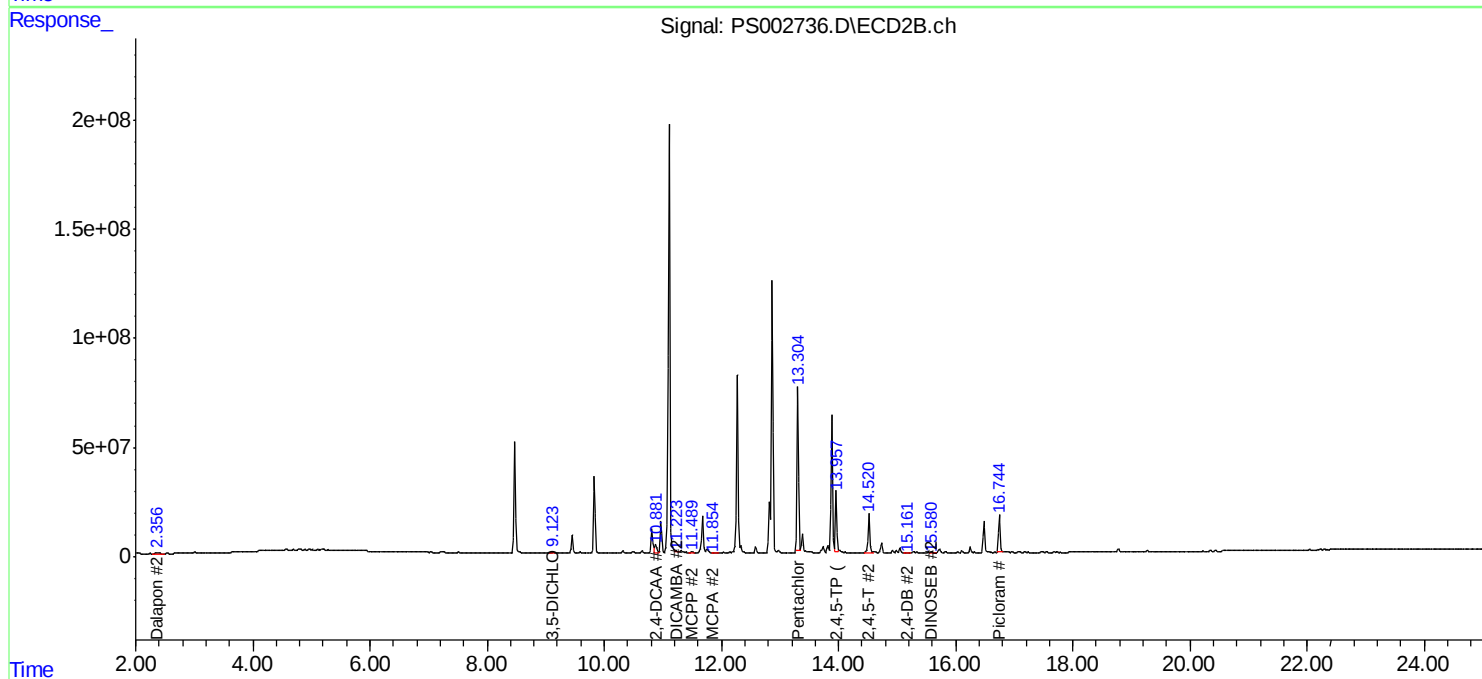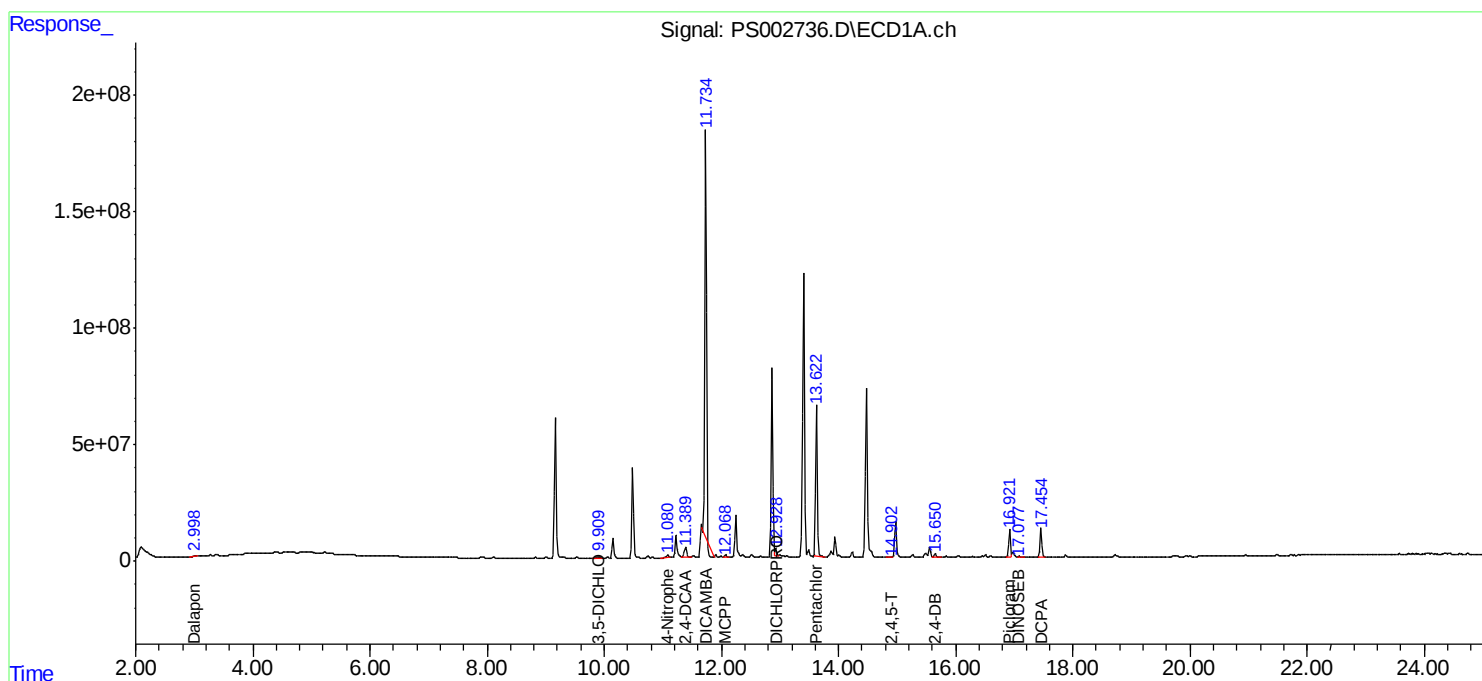


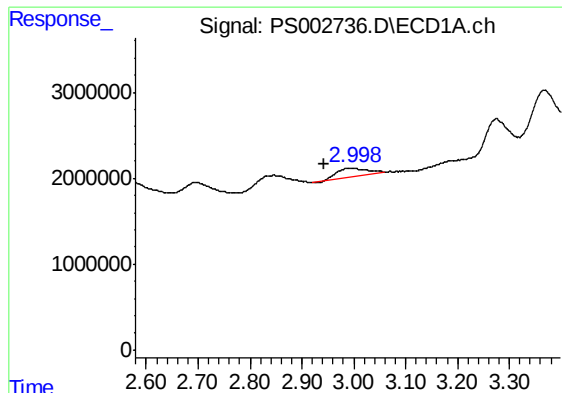

#1 Dalapon


R.T.: 2.997 min
Delta R.T.: 0.053 min
Response: 3945757
Conc: 8.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
50084-50085-50086DL

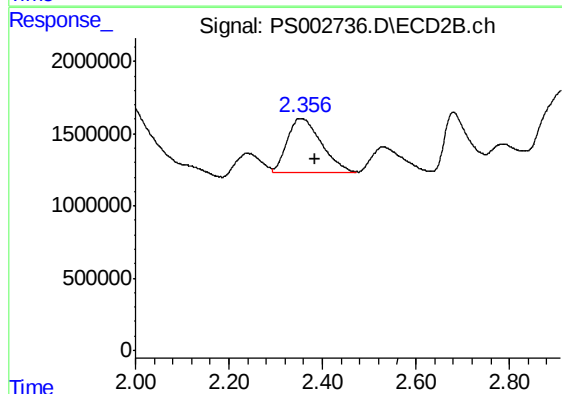


#1 Dalapon

R.T.: 2.356 min
Delta R.T.: -0.029 min
Response: 18829601
Conc: 41.37 ng/ml

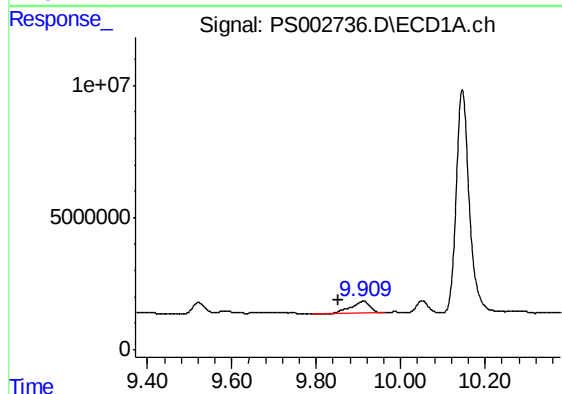


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.911 min
Delta R.T.: 0.060 min
Response: 13852214
Conc: 28.99 ng/ml

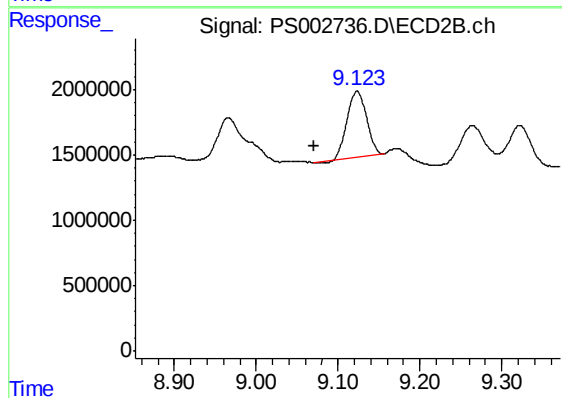

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.123 min
Delta R.T.: 0.053 min
Response: 8245060
Conc: 17.16 ng/ml

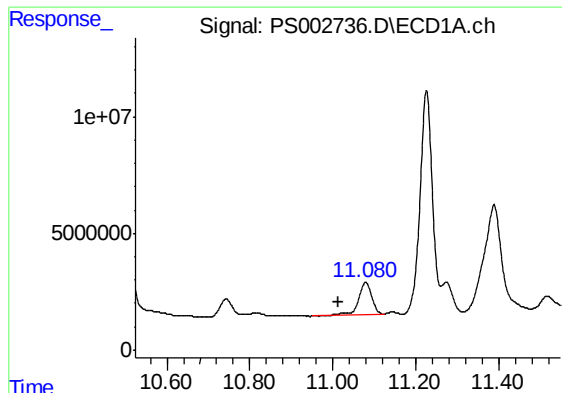

#3 4-Nitrophenol


R.T.: 11.079 min
Delta R.T.: 0.066 min
Response: 30259302
Conc: 190.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
50084-50085-50086DL

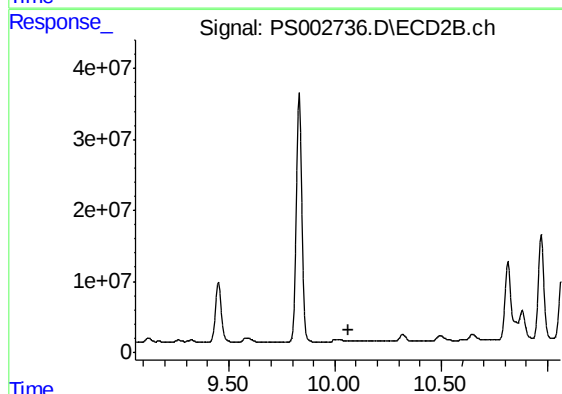


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.061 min
Response: 0
Conc: N.D.

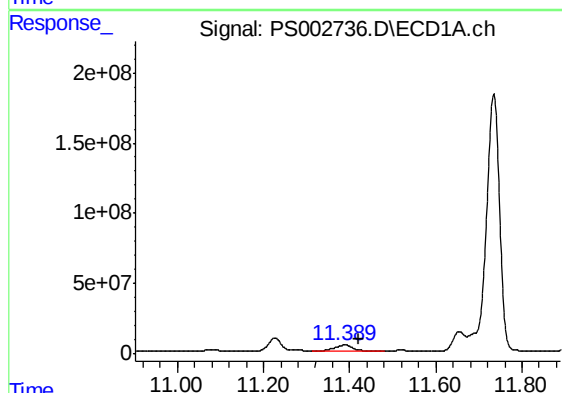


#4 2,4-DCAA

R.T.: 11.389 min
Delta R.T.: -0.031 min
Response: 134643322
Conc: 424.18 ng/ml

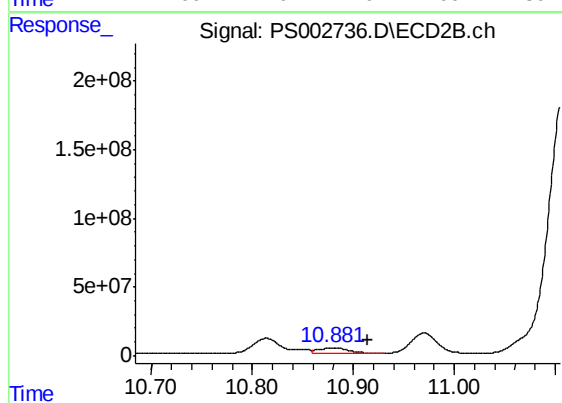

#4 2,4-DCAA


R.T.: 10.881 min
Delta R.T.: -0.034 min
Response: 80609038
Conc: 208.42 ng/ml

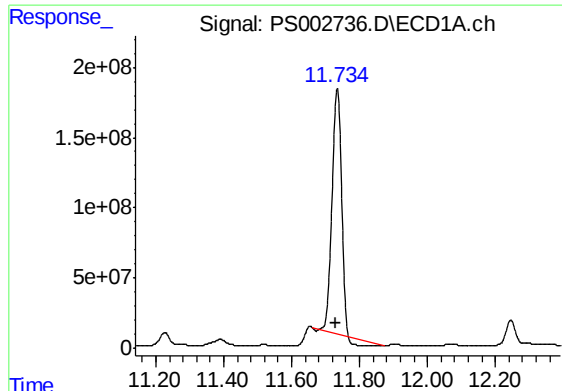

#5 DICAMBA


R.T.: 11.734 min
Delta R.T.: 0.006 min
Response: 3240216702
Conc: 2291.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
50084-50085-50086DL

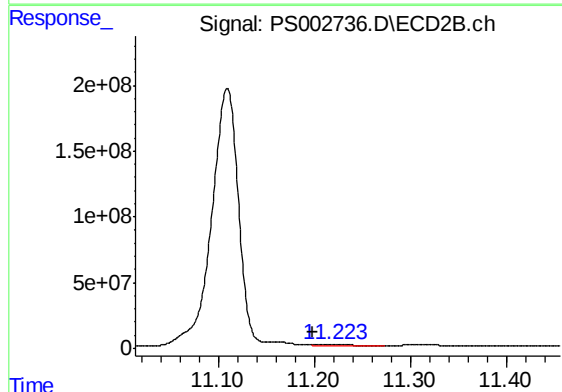


#5 DICAMBA

R.T.: 11.223 min
Delta R.T.: 0.026 min
Response: 19555472
Conc: 13.72 ng/ml

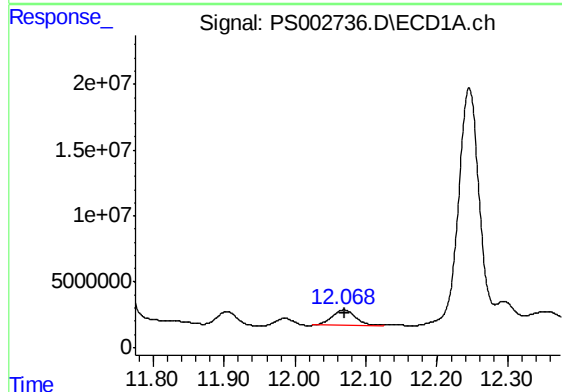


#6 MCPP

R.T.: 12.069 min
Delta R.T.: 0.000 min
Response: 27276081
Conc: 27.34 ug/ml

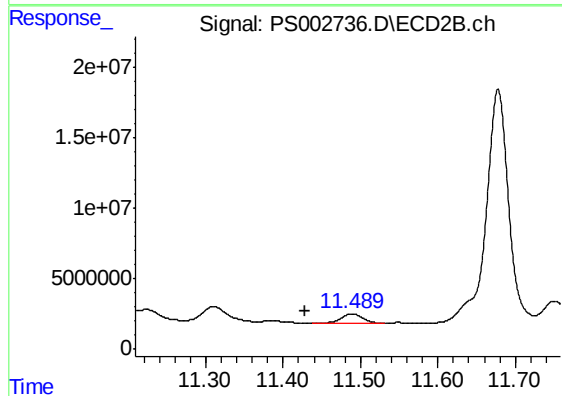

#6 MCPP


R.T.: 11.490 min
Delta R.T.: 0.061 min
Response: 13740608
Conc: 14.70 ug/ml

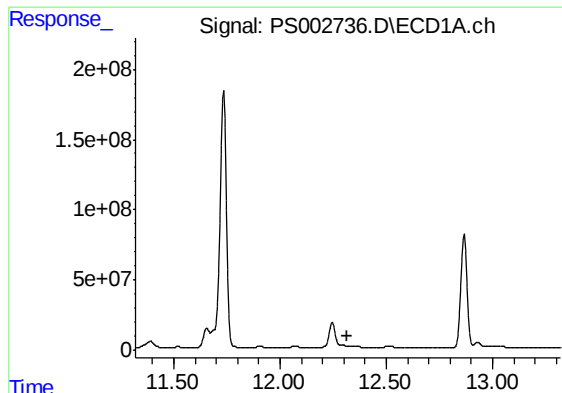

#7 MCPA


R.T.: 12.294 min
Delta R.T.: -0.025 min
Response: -29506825
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
50084-50085-50086DL

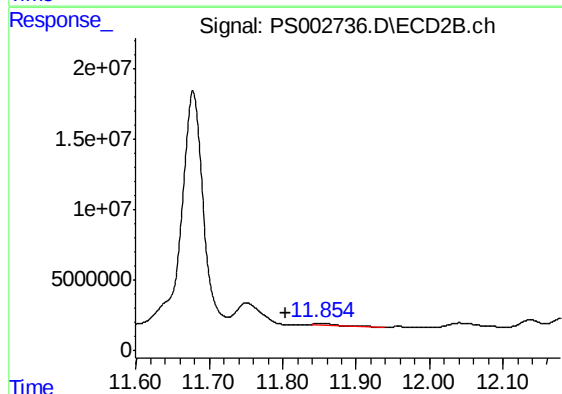


#7 MCPA

R.T.: 11.853 min
Delta R.T.: 0.049 min
Response: 269006
Conc: 0.19 ug/ml

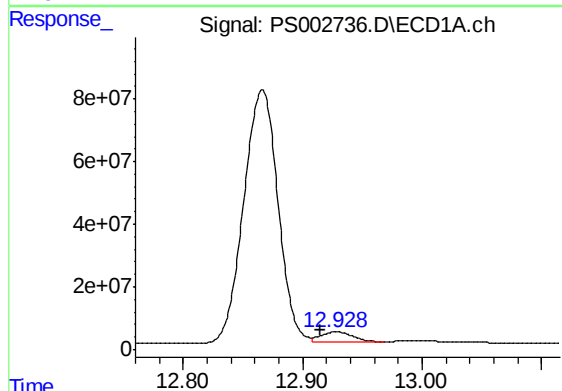


#8 DICHLORPROP

R.T.: 12.929 min
Delta R.T.: 0.013 min
Response: 65005867
Conc: 182.81 ng/ml

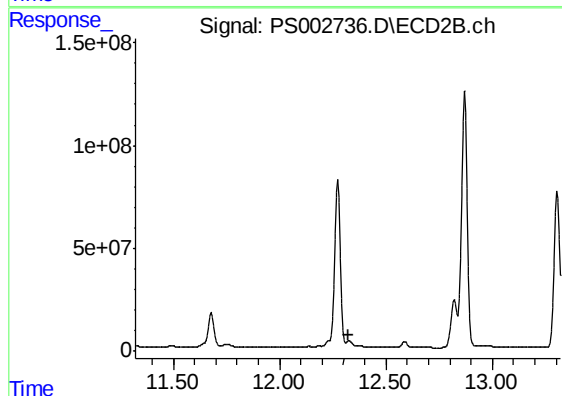

#8 DICHLORPROP


R.T.: 12.326 min
Delta R.T.: 0.004 min
Response: -407880122
Conc: N.D.

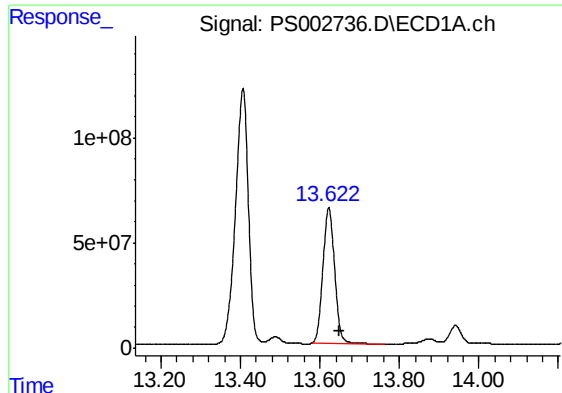

#10 Pentachlorophenol


R.T.: 13.622 min
Delta R.T.: -0.029 min
Response: 1309565965
Conc: 261.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
50084-50085-50086DL

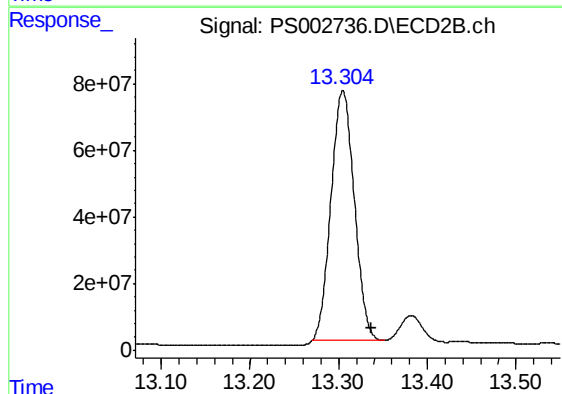


#10 Pentachlorophenol

R.T.: 13.305 min
Delta R.T.: -0.032 min
Response: 1374209424
Conc: 261.20 ng/ml

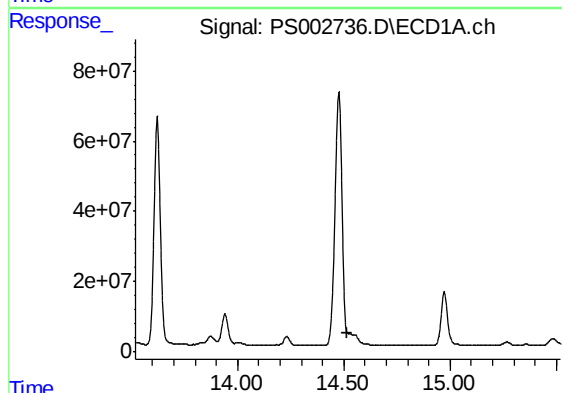


#11 2,4,5-TP (SILVEX)

R.T.: 14.477 min
Delta R.T.: -0.042 min
Response: -302169219
Conc: N.D.

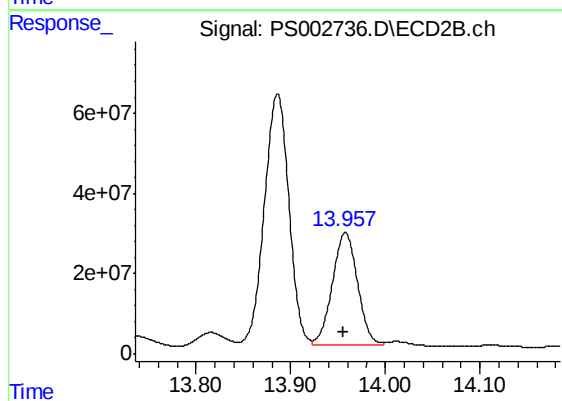

#11 2,4,5-TP (SILVEX)


R.T.: 13.958 min
Delta R.T.: 0.002 min
Response: 516118607
Conc: 245.83 ng/ml

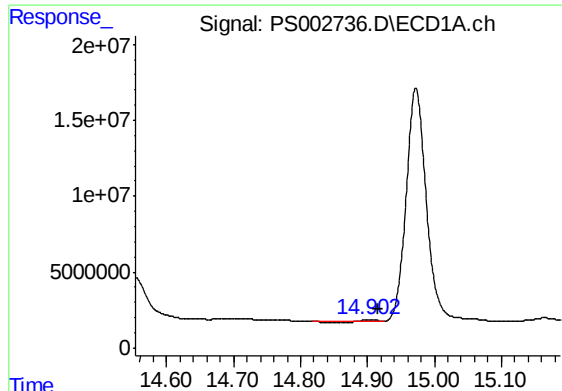

#12 2,4,5-T


R.T.: 14.904 min
Delta R.T.: -0.013 min
Response: 229063
Conc: 0.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
50084-50085-50086DL

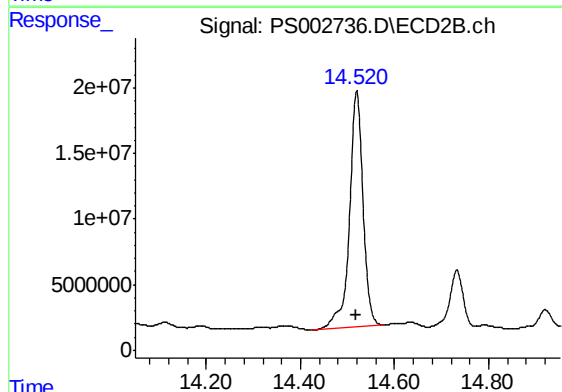


#12 2,4,5-T

R.T.: 14.520 min
Delta R.T.: 0.001 min
Response: 358290679
Conc: 209.43 ng/ml

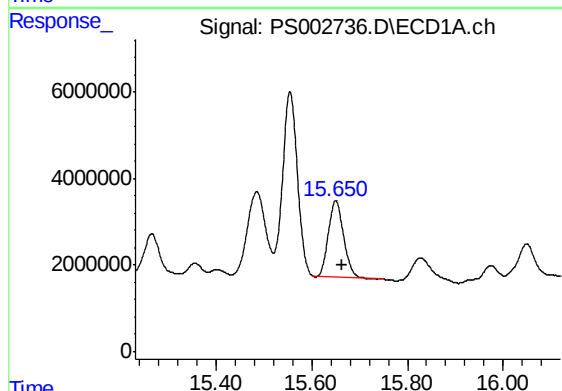


#13 2,4-DB

R.T.: 15.650 min
Delta R.T.: -0.013 min
Response: 38380204
Conc: 169.70 ng/ml

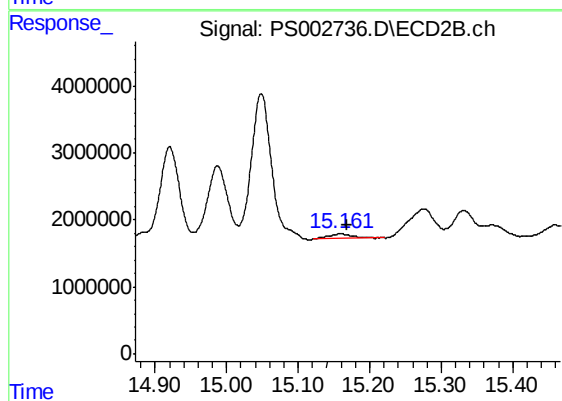

#13 2,4-DB


R.T.: 15.160 min
Delta R.T.: -0.009 min
Response: 1729858
Conc: 7.14 ng/ml

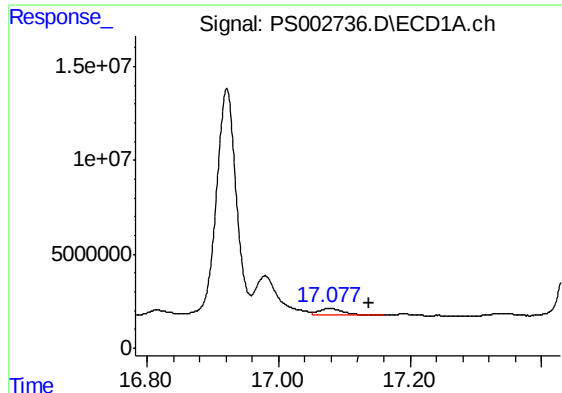

#14 DINOSEB


R.T.: 17.077 min
Delta R.T.: -0.061 min
Response: 9865484
Conc: 6.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
50084-50085-50086DL

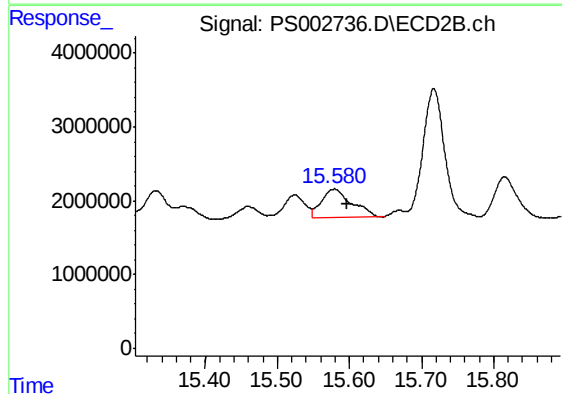


#14 DINOSEB

R.T.: 15.580 min
Delta R.T.: -0.017 min
Response: 11422536
Conc: 7.48 ng/ml

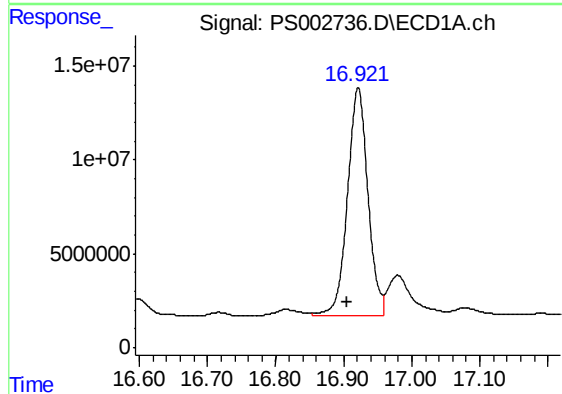


#15 Picloram

R.T.: 16.921 min
Delta R.T.: 0.015 min
Response: 253916124
Conc: 100.05 ng/ml

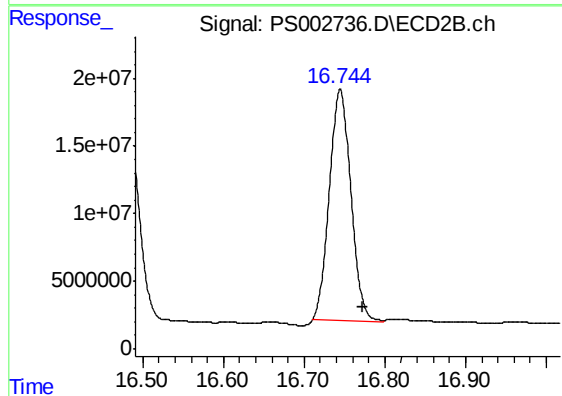

#15 Picloram


R.T.: 16.745 min
Delta R.T.: -0.029 min
Response: 317038839
Conc: 115.24 ng/ml

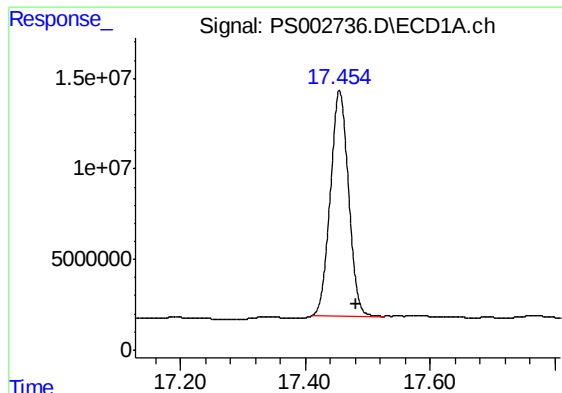

#16 DCPA

R.T.: 17.455 min
Delta R.T.: -0.026 min
Response: 250931011
Conc: 103.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
50084-50085-50086DL

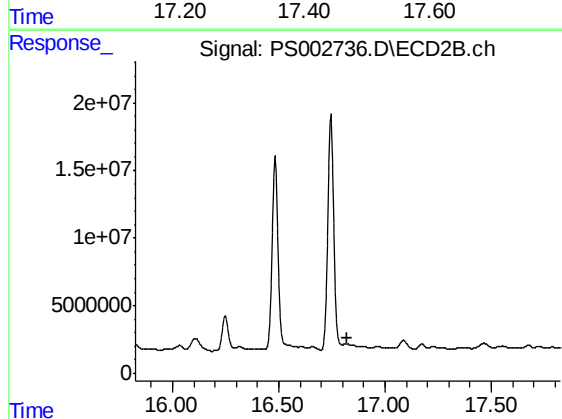

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.825 min
Response: 0
Conc: N.D.