

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010224\
 Data File : PS025386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2024 08:47
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 01:35:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	0.000	2.554	0	3178772	N.D.	2.766
2) T	3,5-DICHL...	5.692	0.000	4740110	0	1.394	N.D. #
3) T	4-Nitroph...	0.000	6.365	0	620123	N.D.	1.248
5) T	DICAMBA	0.000	6.919	0	423717	N.D.	<MDL
6) T	MCP	0.000	6.960f	0	3548604	N.D.	1.778
7) T	MCPA	0.000	7.166f	0	11388389	N.D.	3.623
8) T	DICHLORPROP	0.000	7.550	0	3149224	N.D.	4.071
9) T	2,4-D	7.243	7.764f	22255151	440507	7.184	<MDL #
10) T	Pentachlo...	0.000	8.238	0	464343	N.D.	<MDL
12) T	2,4,5-T	0.000	8.974	0	792635	N.D.	<MDL
14) T	DINOSEB	9.777f	9.796	8074047	740738	<MDL	<MDL #
15) T	Picloram	9.701	10.768	76794679	18114462	3.676	2.659 #
16) T	DCPA	0.000	10.716	0	578747	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010224\
Data File : PS025386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2024 08:47
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 01:35:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

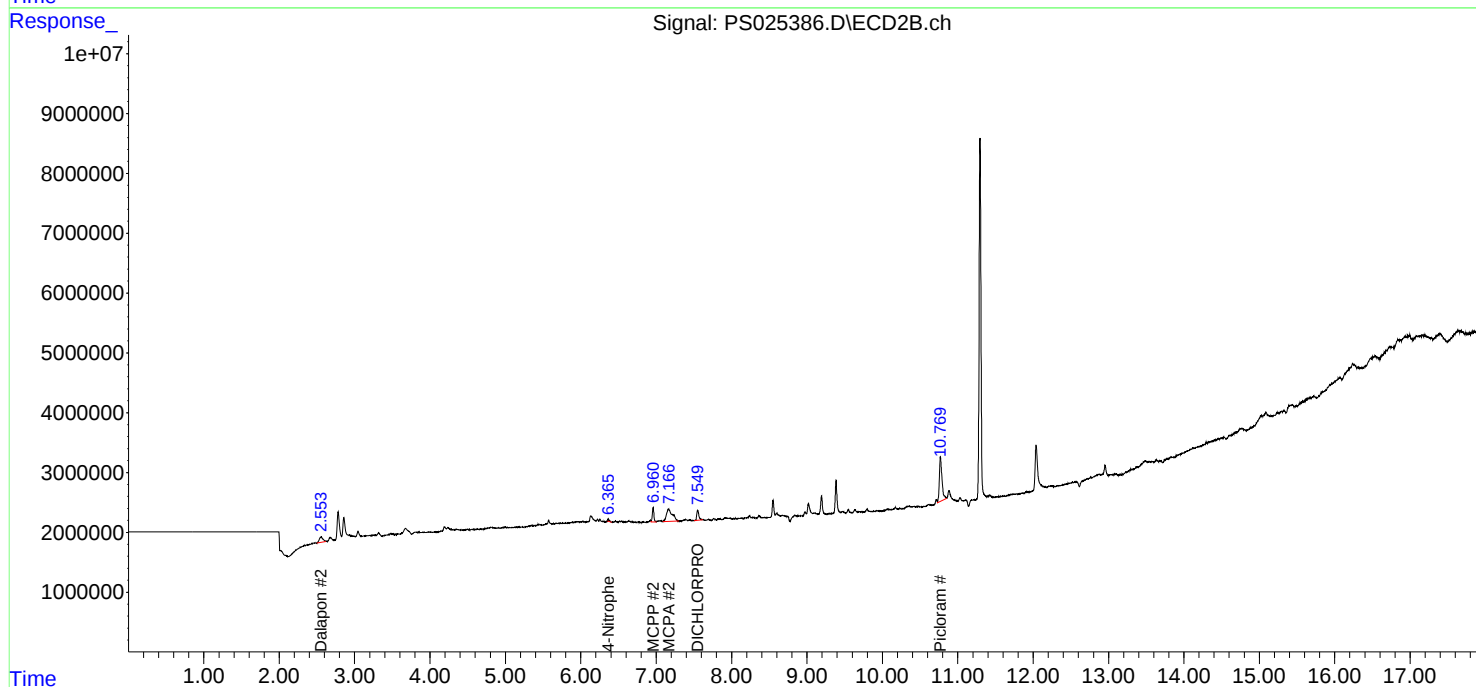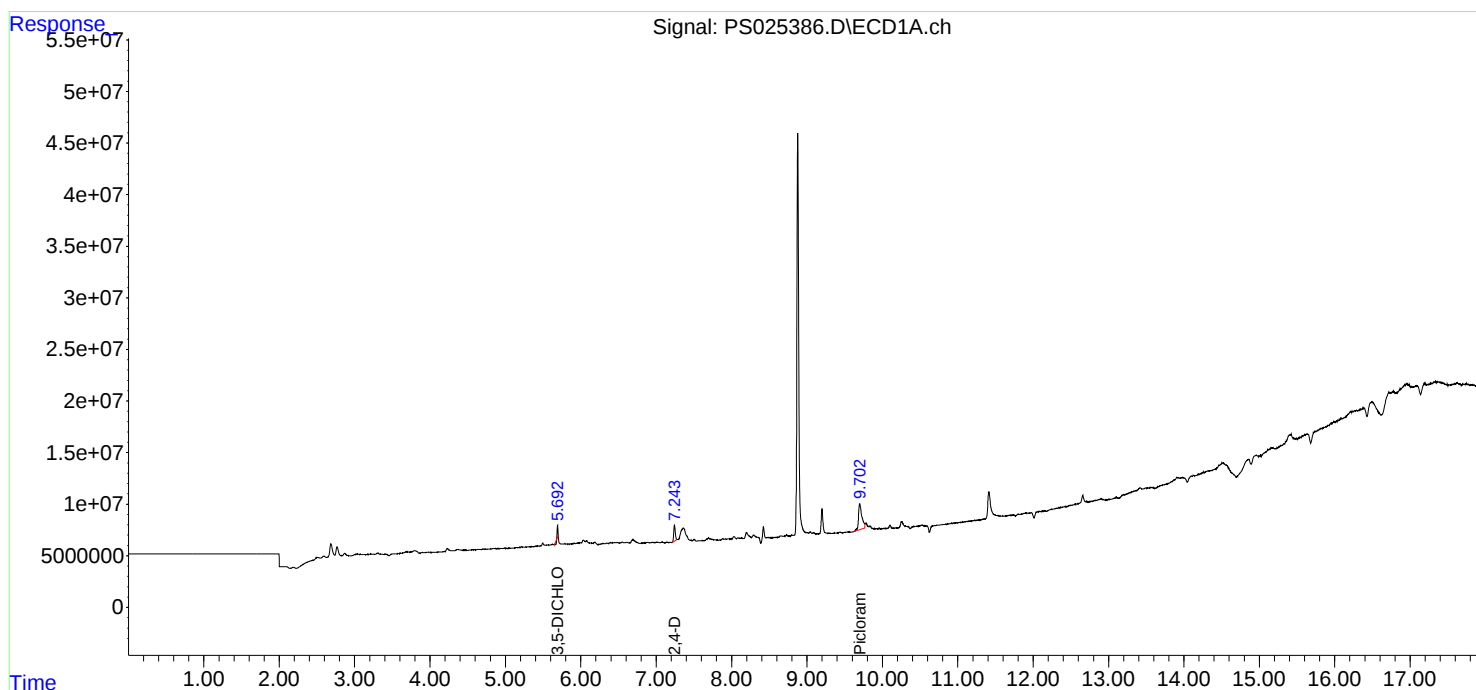


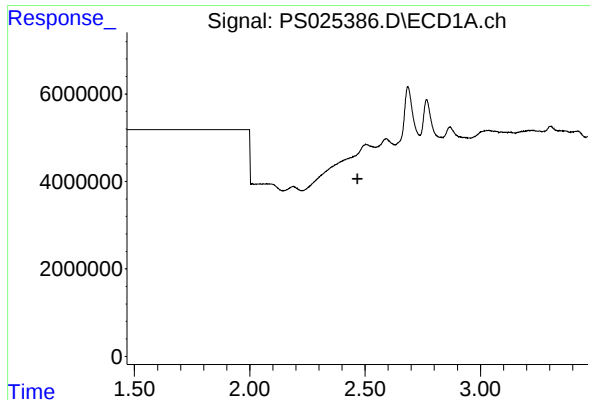

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

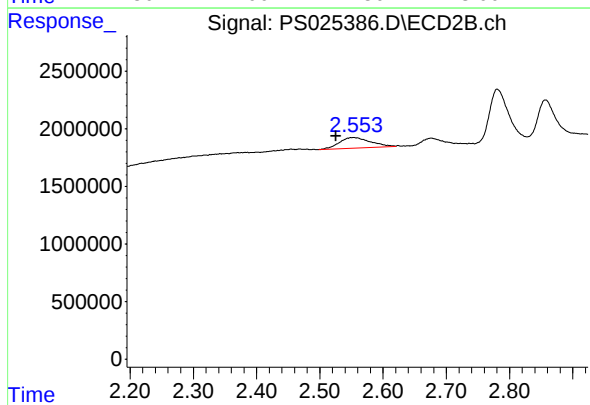


#1 Dalapon

R.T.: 2.554 min
Delta R.T.: 0.028 min
Response: 3178772
Conc: 2.77 ng/ml

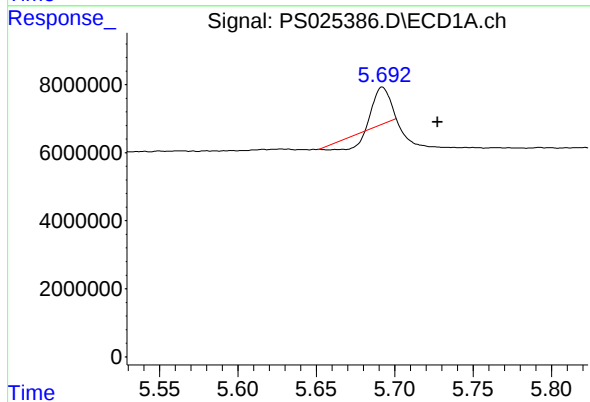


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.692 min
Delta R.T.: -0.035 min
Response: 4740110
Conc: 1.39 ng/ml

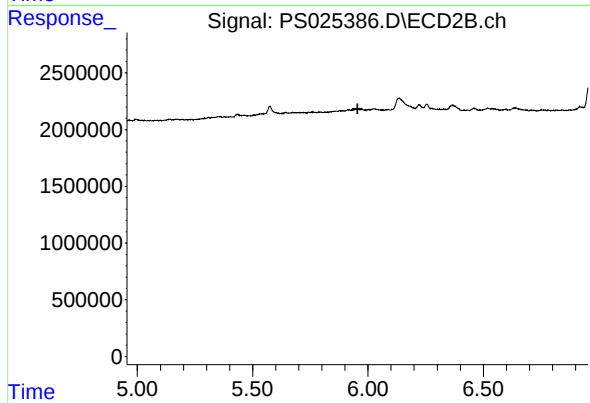

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

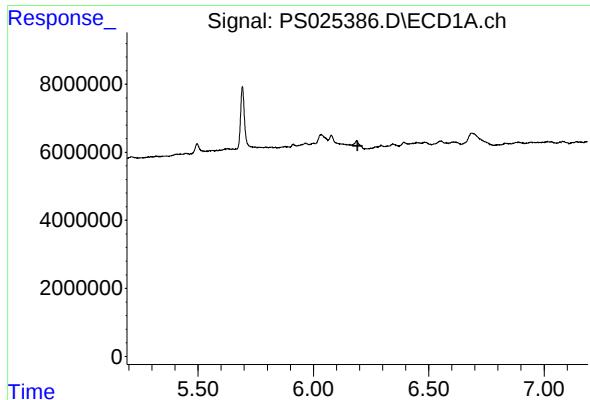

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

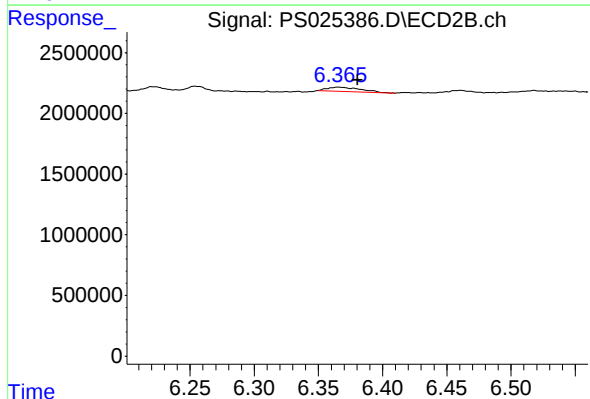


#3 4-Nitrophenol

R.T.: 6.365 min
Delta R.T.: -0.015 min
Response: 620123
Conc: 1.25 ng/ml

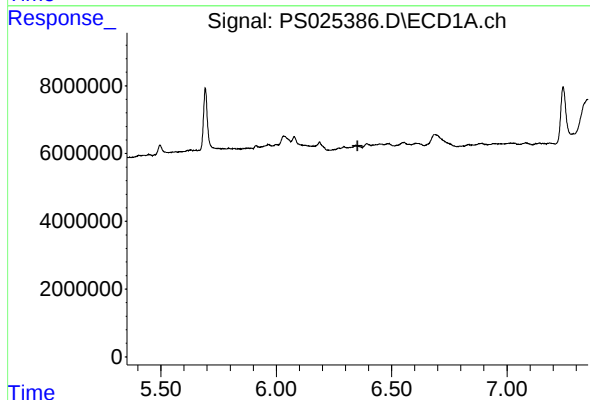


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

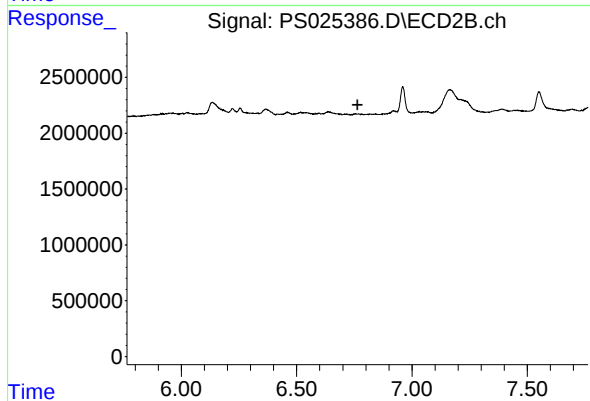

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

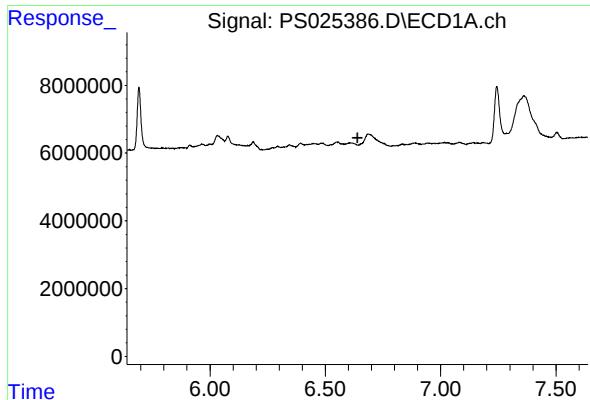


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :


Time

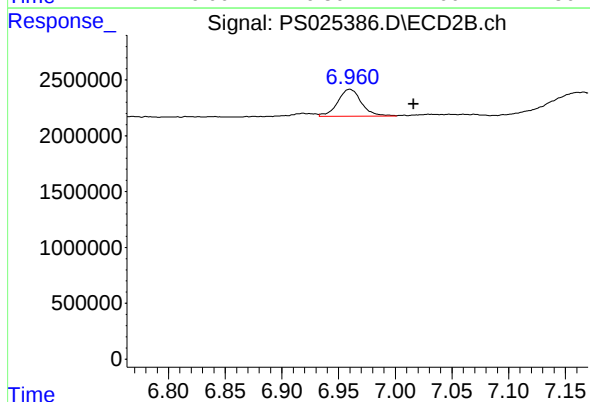

#6 MCPP

R.T.: 6.960 min
Delta R.T.: -0.057 min
Response: 3548604
Conc: 1.78 ug/ml


Time

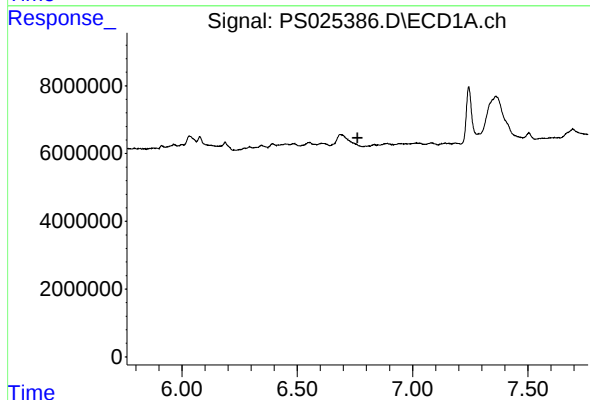

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

Time

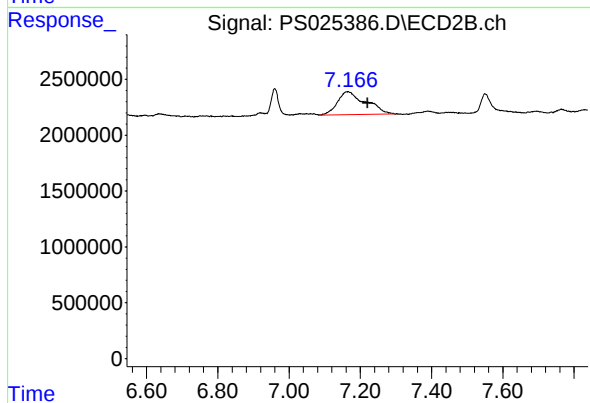

#7 MCPA


R.T.: 7.166 min
Delta R.T.: -0.055 min
Response: 11388389
Conc: 3.62 ug/ml

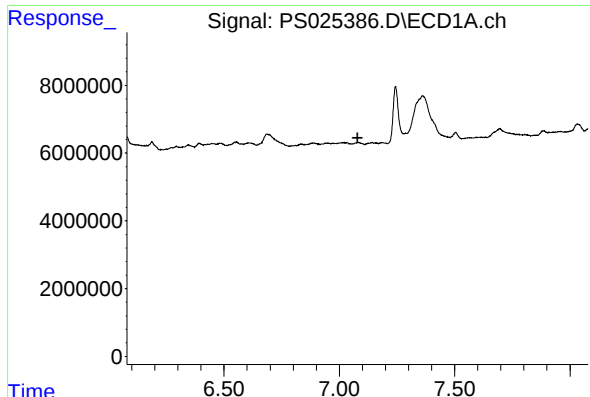

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

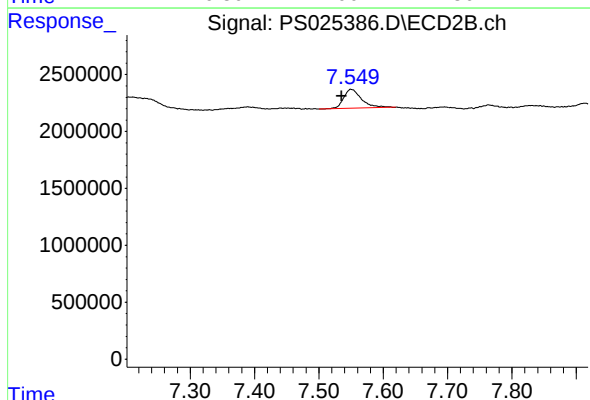


#8 DICHLORPROP

R.T.: 7.550 min
Delta R.T.: 0.015 min
Response: 3149224
Conc: 4.07 ng/ml

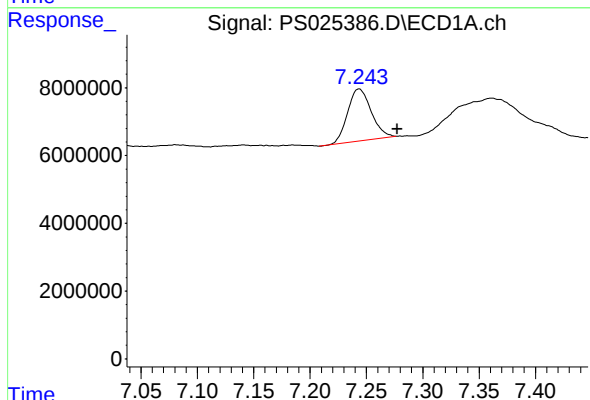


#9 2,4-D

R.T.: 7.243 min
Delta R.T.: -0.034 min
Response: 22255151
Conc: 7.18 ng/ml

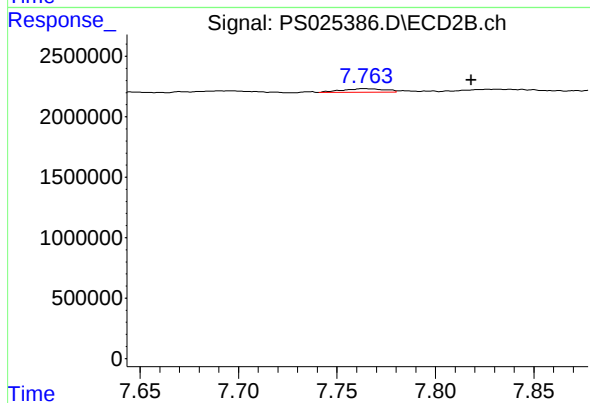

#9 2,4-D


R.T.: 7.764 min
Delta R.T.: -0.055 min
Response: 440507
Conc: N.D.

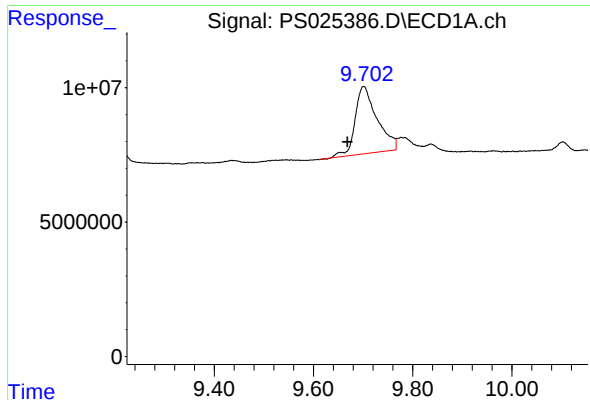

#15 Picloram

R.T.: 9.701 min
Delta R.T.: 0.033 min
Response: 76794679
Conc: 3.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

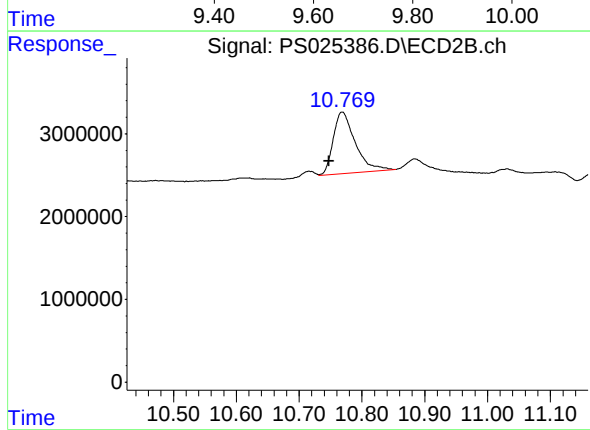

#15 Picloram

R.T.: 10.768 min
Delta R.T.: 0.021 min
Response: 18114462
Conc: 2.66 ng/ml