

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010224\
 Data File : PS025387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2024 09:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 01:35:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.351	6.762	1055.1E6	334.8E6	470.854	471.657
Target Compounds							
1) T	Dalapon	0.000	2.554	0	2669008	N.D.	2.322
3) T	4-Nitroph...	6.191	6.364	10289838	1155416	6.642	2.326 #
5) T	DICAMBA	0.000	6.970f	0	3783950	N.D.	1.250
6) T	MCP	6.682f	6.970f	28176517	3783950	4.188	1.896 #
7) T	MCPA	0.000	7.154f	0	12015641	N.D.	3.823
8) T	DICHLORPROP	0.000	7.551	0	9358372	N.D.	12.098
9) T	2,4-D	7.256	7.763f	19664762	359465	6.348	<MDL #
11) T	2,4,5-TP ...	8.043	8.597	6184172	-1001624	<MDL	N.D. #
12) T	2,4,5-T	0.000	8.974	0	370195	N.D.	<MDL
14) T	DINOSEB	9.782f	0.000	8322193	0	<MDL	N.D. #
15) T	Picloram	9.698	10.765	47514296	12313946	2.274	1.807
16) T	DCPA	0.000	10.716	0	540809	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010224\
Data File : PS025387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2024 09:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 01:35:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

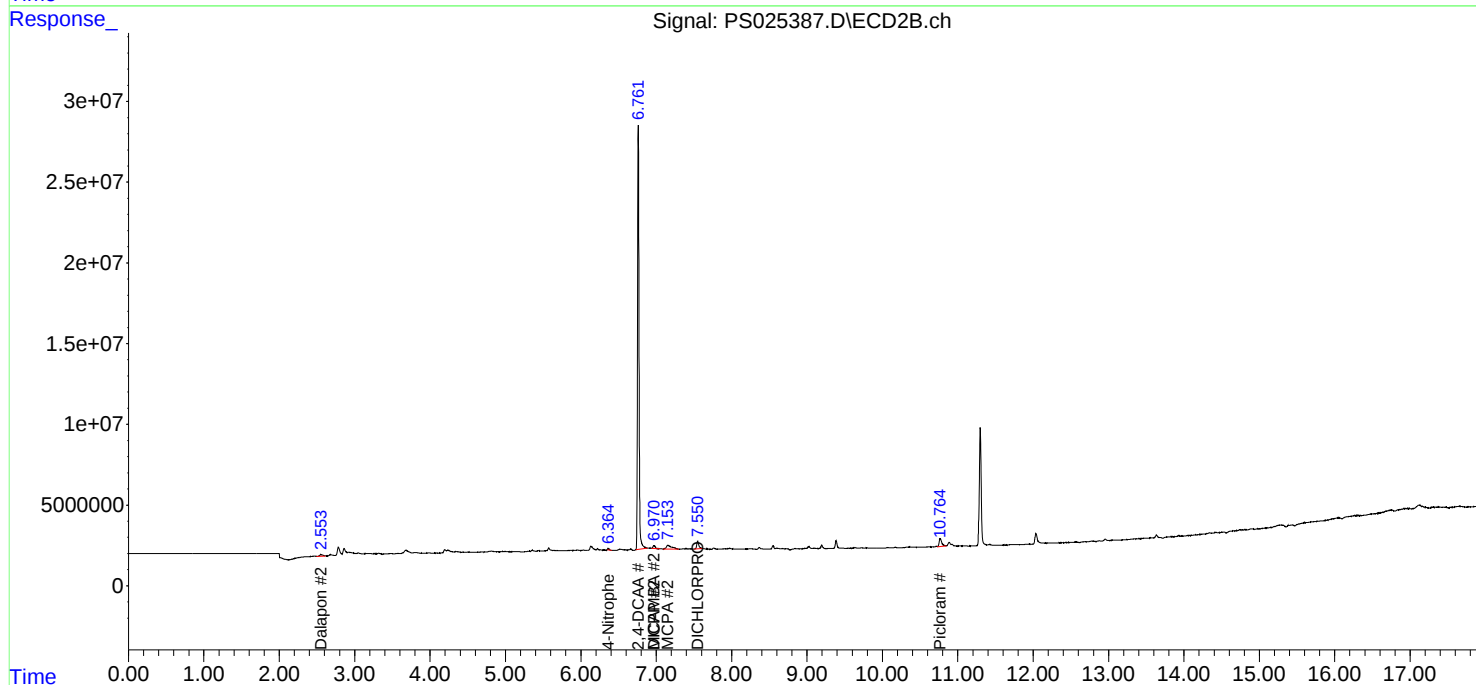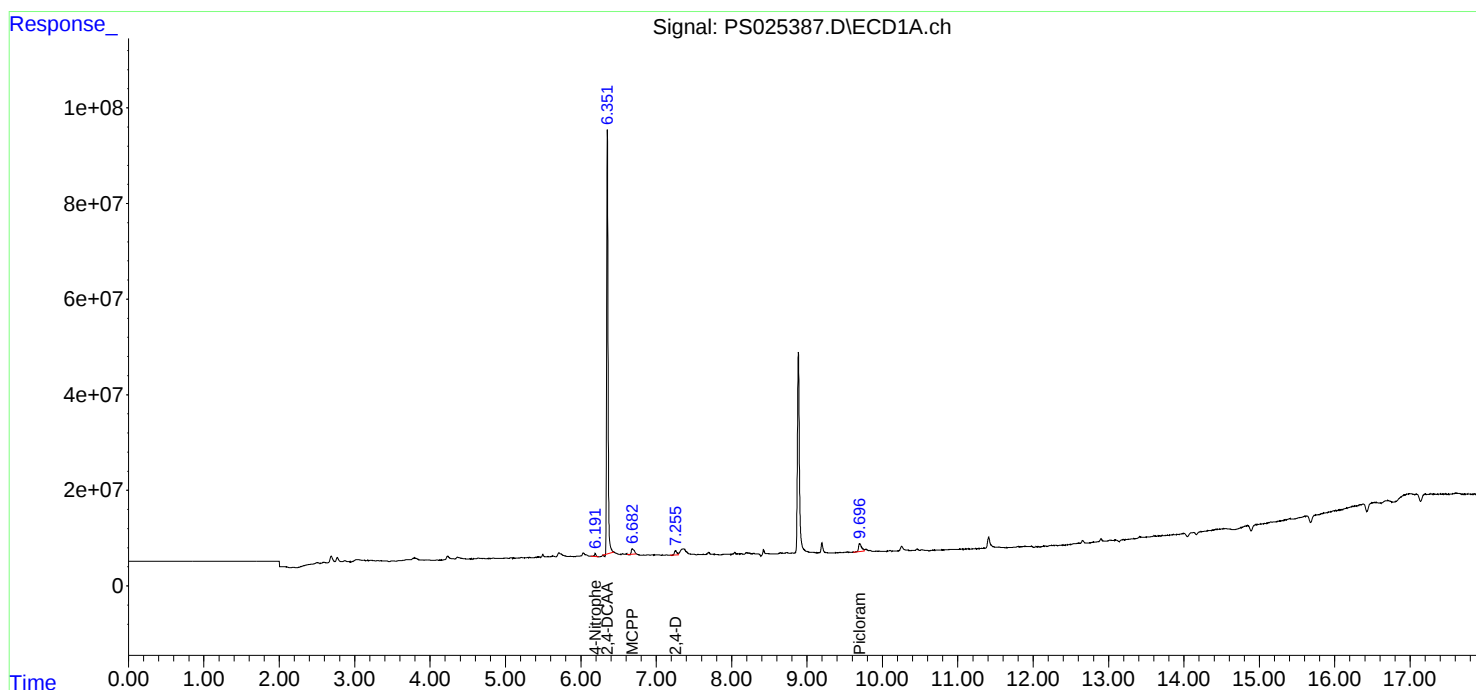


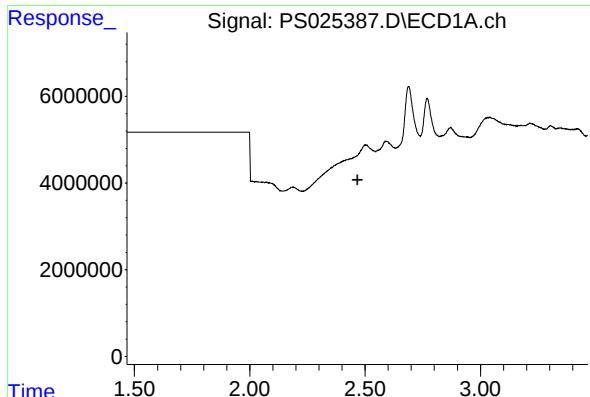

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

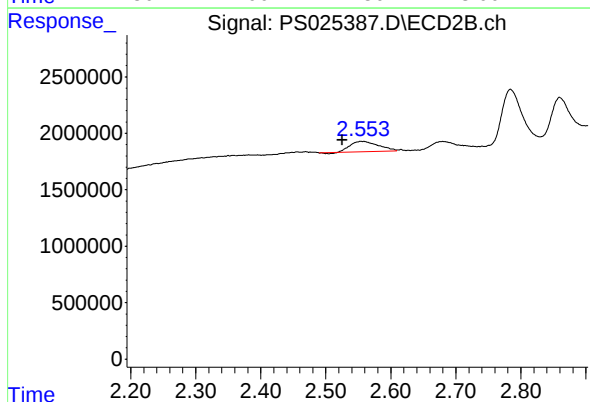


#1 Dalapon

R.T.: 2.554 min
Delta R.T.: 0.028 min
Response: 2669008
Conc: 2.32 ng/ml

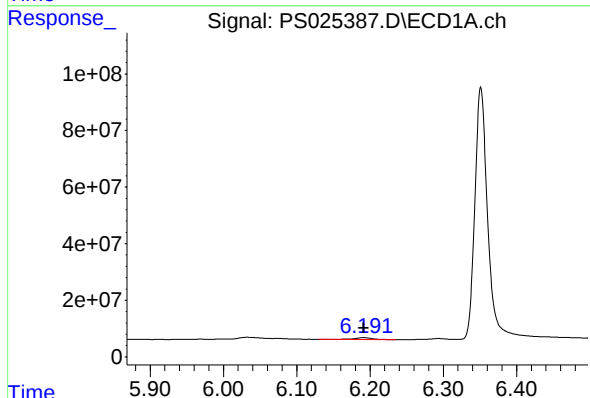


#3 4-Nitrophenol

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 10289838
Conc: 6.64 ng/ml

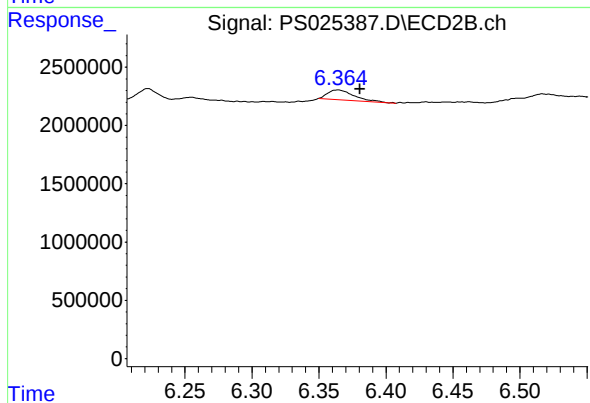

#3 4-Nitrophenol


R.T.: 6.364 min
Delta R.T.: -0.017 min
Response: 1155416
Conc: 2.33 ng/ml

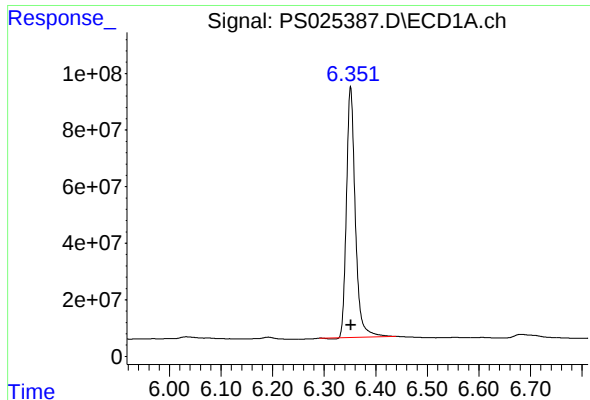

#4 2,4-DCAA


R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 1055092104
Conc: 470.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

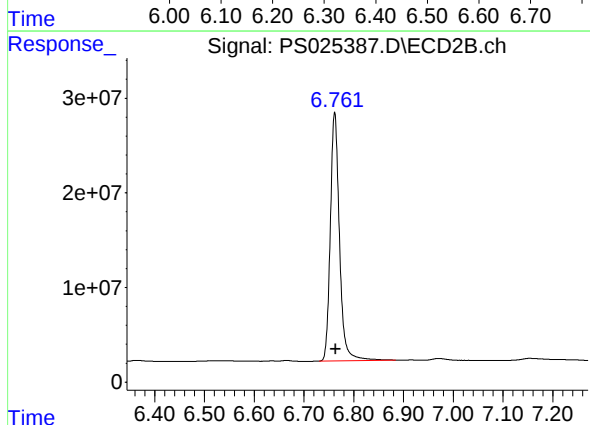


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.002 min
Response: 334769255
Conc: 471.66 ng/ml

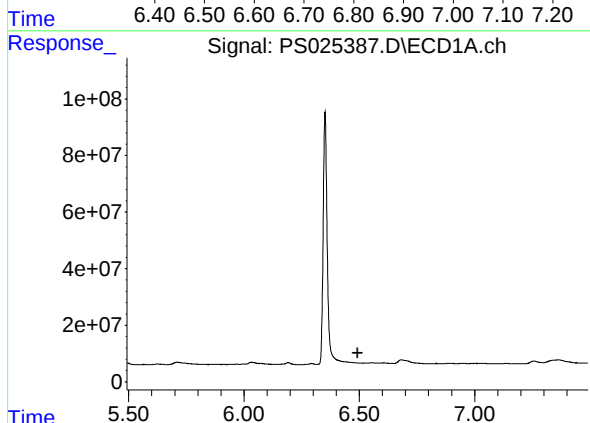


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

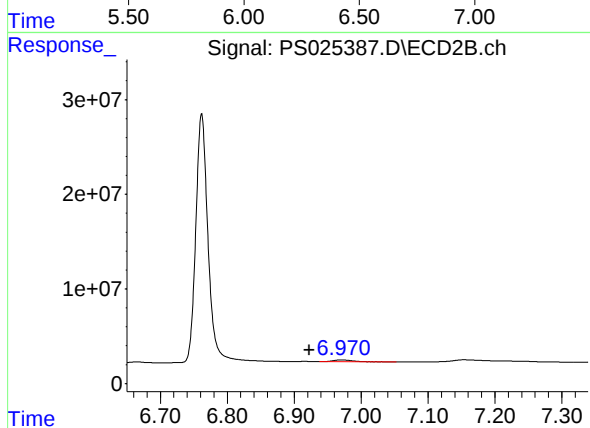

#5 DICAMBA


R.T.: 6.970 min
Delta R.T.: 0.047 min
Response: 3783950
Conc: 1.25 ng/ml

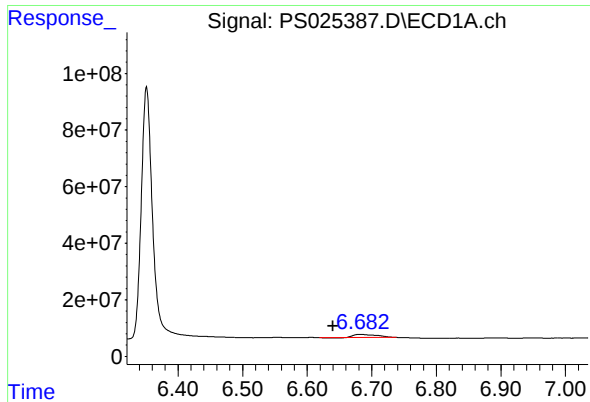

#6 MCPP


R.T.: 6.682 min
Delta R.T.: 0.042 min
Response: 28176517
Conc: 4.19 ug/ml

Instrument :
ECD_S
ClientSampleId :

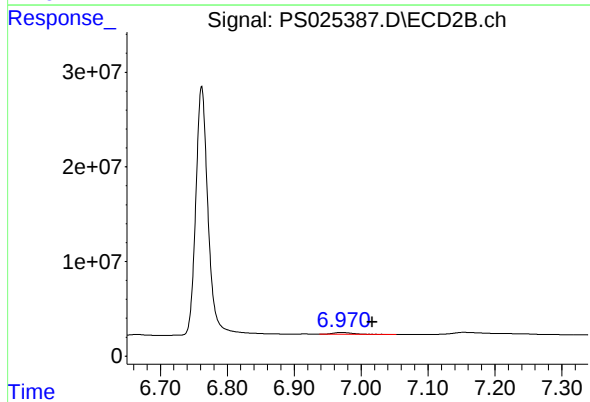


#6 MCPP

R.T.: 6.970 min
Delta R.T.: -0.047 min
Response: 3783950
Conc: 1.90 ug/ml

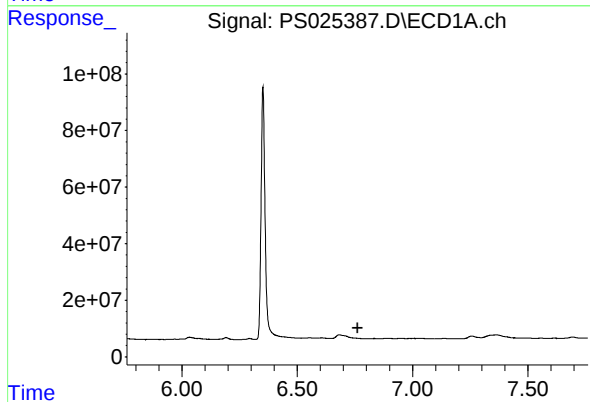


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

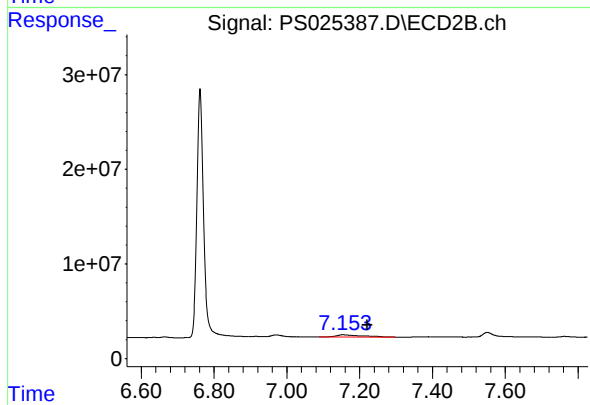

#7 MCPA


R.T.: 7.154 min
Delta R.T.: -0.068 min
Response: 12015641
Conc: 3.82 ug/ml

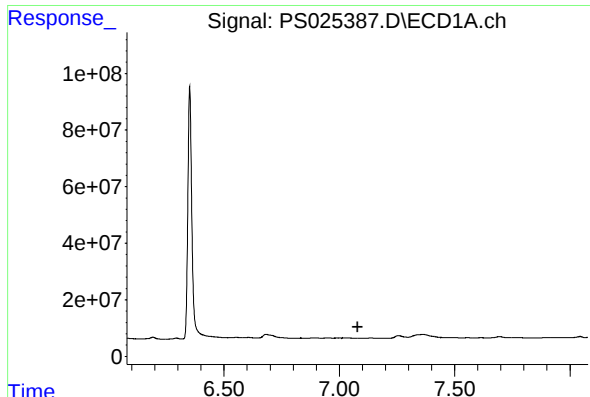

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

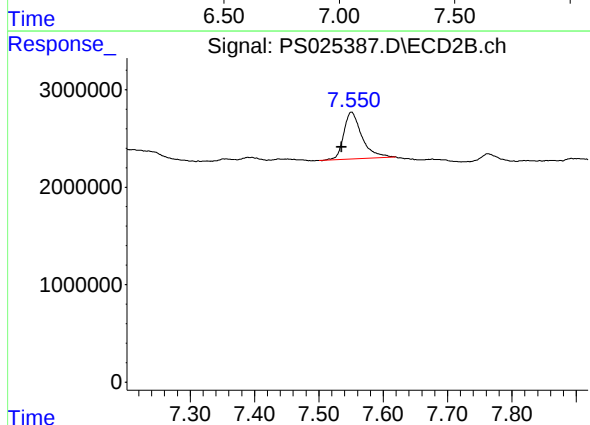


#8 DICHLORPROP

R.T.: 7.551 min
Delta R.T.: 0.016 min
Response: 9358372
Conc: 12.10 ng/ml

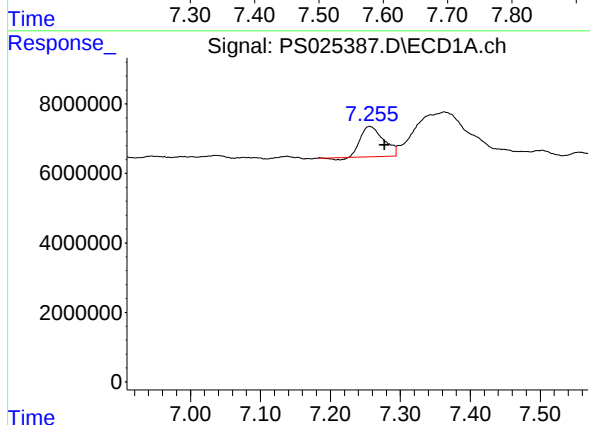


#9 2,4-D

R.T.: 7.256 min
Delta R.T.: -0.021 min
Response: 19664762
Conc: 6.35 ng/ml

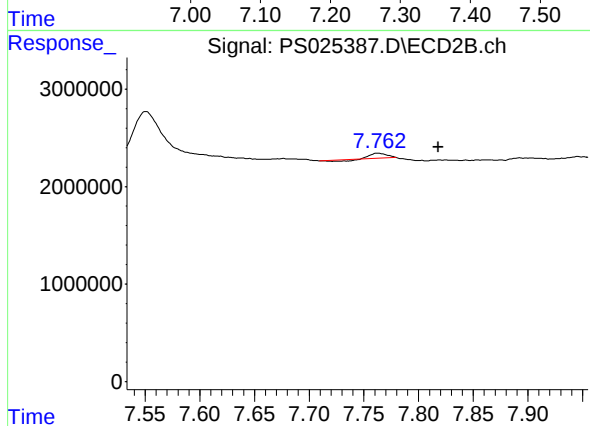

#9 2,4-D


R.T.: 7.763 min
Delta R.T.: -0.056 min
Response: 359465
Conc: N.D.

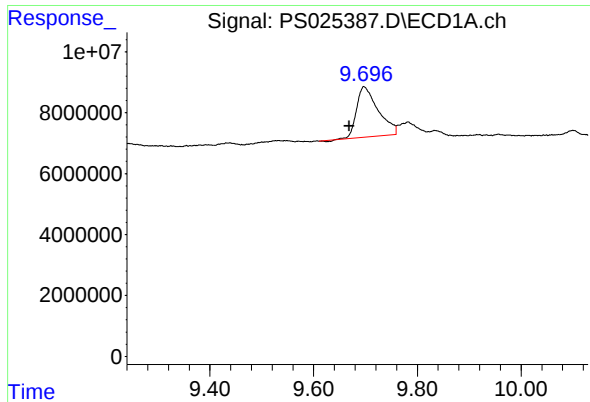

#15 Picloram

R.T.: 9.698 min
Delta R.T.: 0.029 min
Response: 47514296
Conc: 2.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

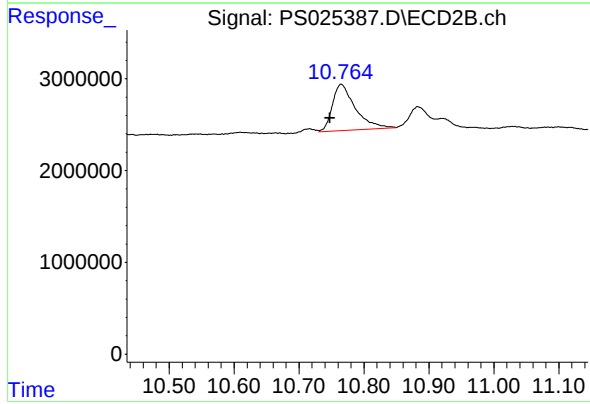

#15 Picloram

R.T.: 10.765 min
Delta R.T.: 0.017 min
Response: 12313946
Conc: 1.81 ng/ml