

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010224\
 Data File : PS025399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2024 15:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 01:38:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.351	6.762	1091.1E6	342.7E6	486.904	482.786
Target Compounds						
1) T Dalapon	0.000	2.556	0	3164336	N.D.	2.753
2) T 3,5-DICHL...	5.692	0.000	245824	0	<MDL	N.D. #
3) T 4-Nitroph...	0.000	6.363	0	634340	N.D.	1.277
5) T DICAMBA	0.000	6.959	0	531828	N.D.	<MDL
6) T MCPP	0.000	6.959f	0	531828	N.D.	<MDL
7) T MCPA	6.712f	7.154f	10846307	14503932	1.144	4.615 #
8) T DICHLORPROP	0.000	7.554	0	4936846	N.D.	6.382
12) T 2,4,5-T	0.000	9.033f	0	945599	N.D.	<MDL
15) T Picloram	9.722f	10.784	12955575	2236590	<MDL	<MDL #
16) T DCPA	0.000	10.784f	0	2236590	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010224\
Data File : PS025399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2024 15:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 01:38:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

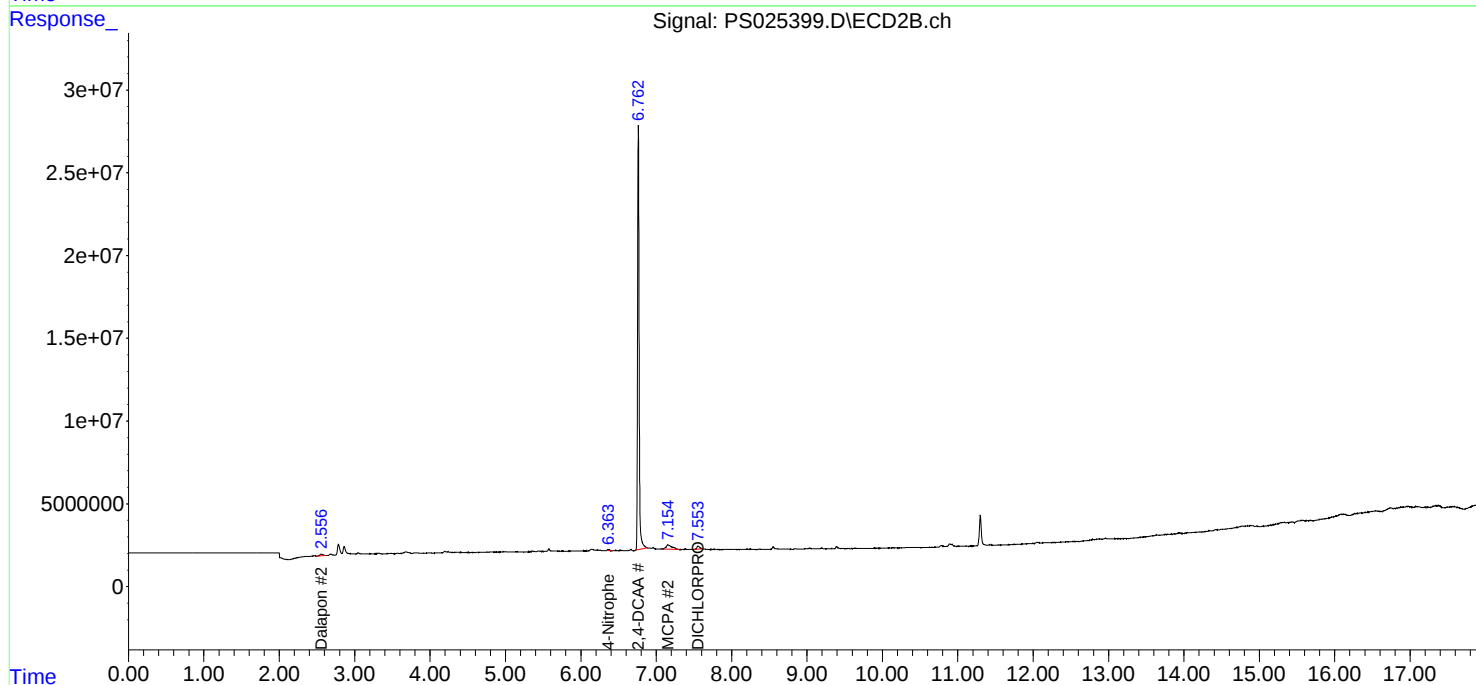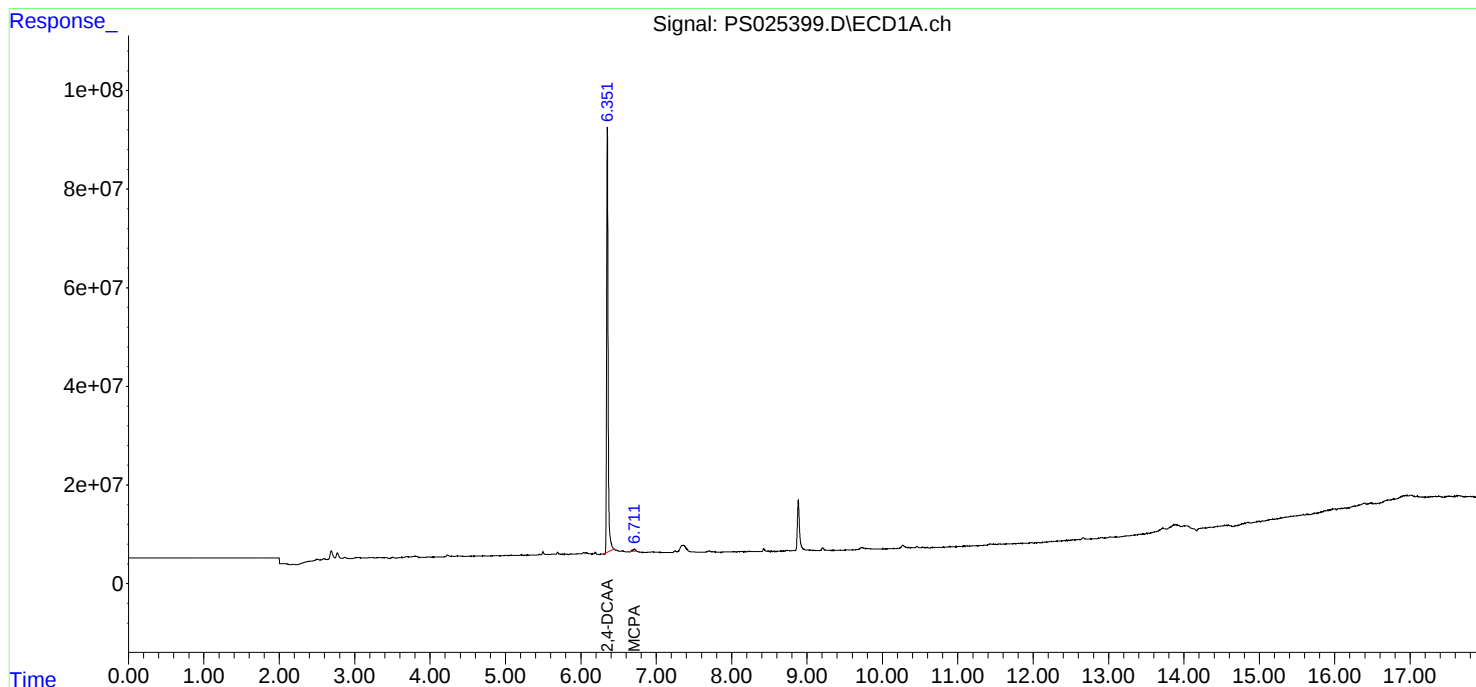


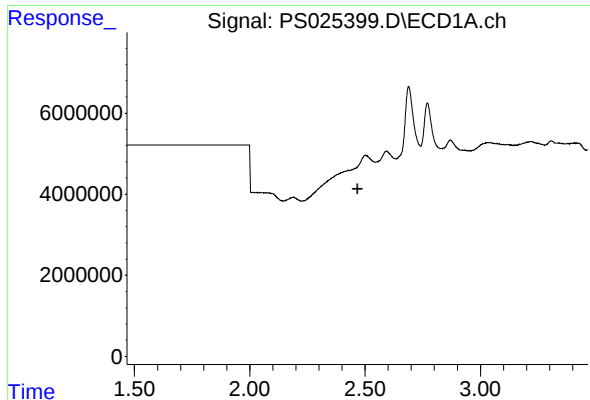

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

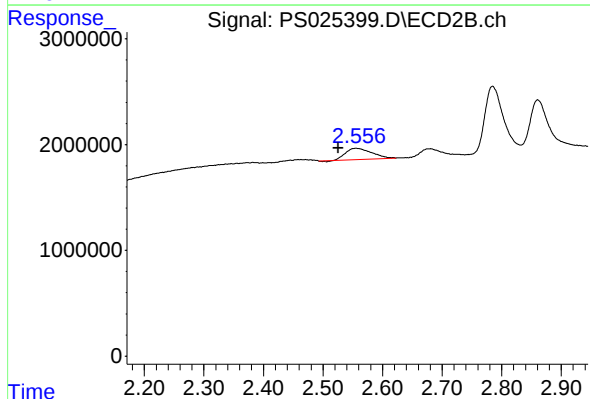


#1 Dalapon

R.T.: 2.556 min
Delta R.T.: 0.030 min
Response: 3164336
Conc: 2.75 ng/ml

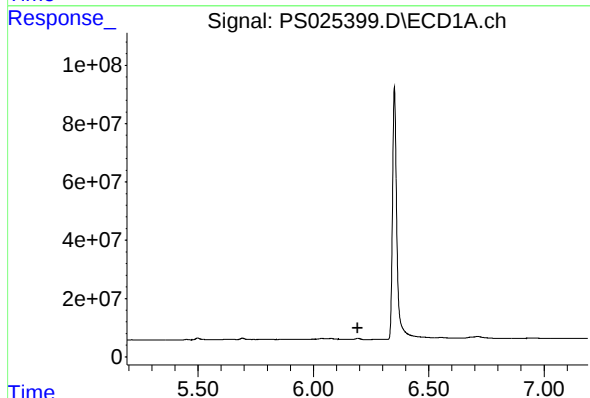


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

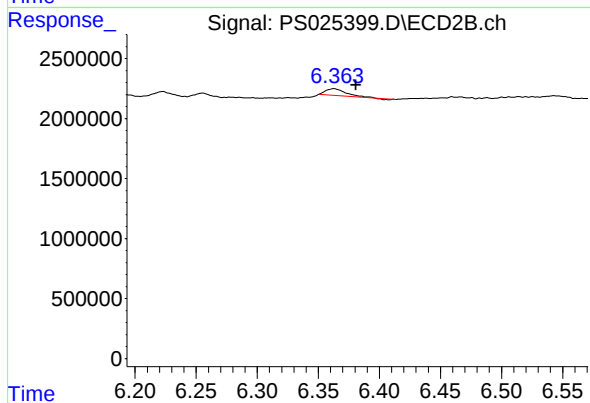

#3 4-Nitrophenol


R.T.: 6.363 min
Delta R.T.: -0.018 min
Response: 634340
Conc: 1.28 ng/ml

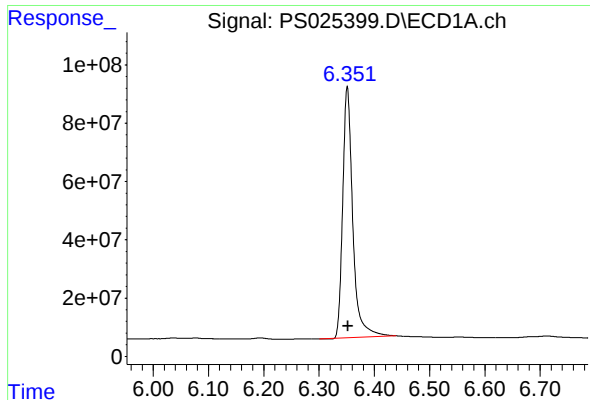

#4 2,4-DCAA


R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 1091055337
Conc: 486.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

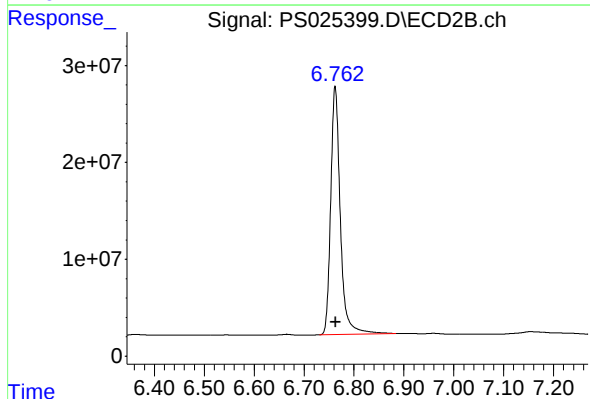


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 342668747
Conc: 482.79 ng/ml

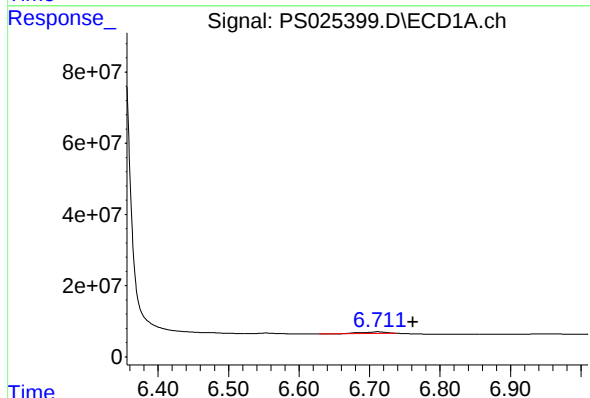


#7 MCPA

R.T.: 6.712 min
Delta R.T.: -0.050 min
Response: 10846307
Conc: 1.14 ug/ml

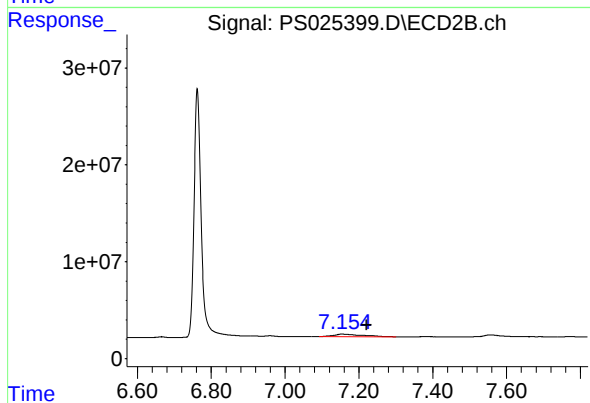

#7 MCPA


R.T.: 7.154 min
Delta R.T.: -0.067 min
Response: 14503932
Conc: 4.61 ug/ml

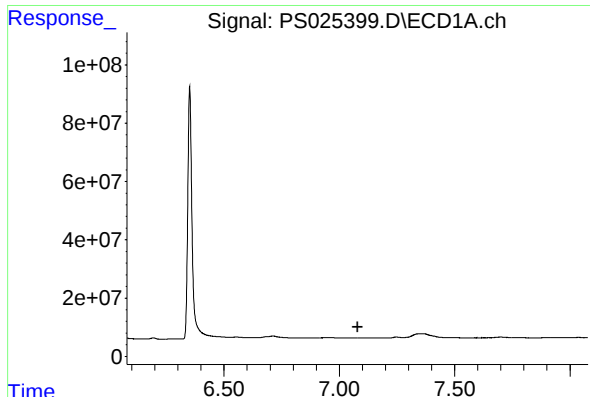

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

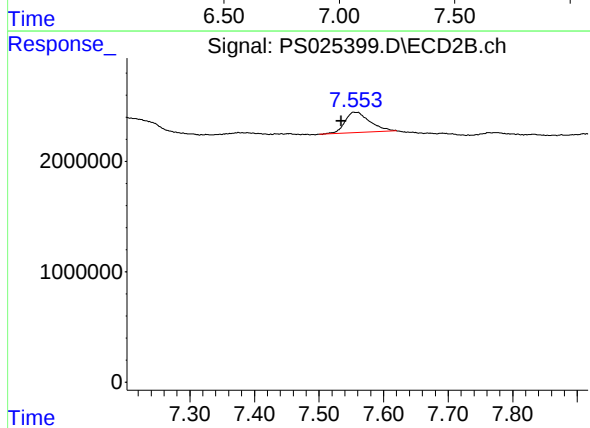

#8 DICHLORPROP

R.T.: 7.554 min
Delta R.T.: 0.019 min
Response: 4936846
Conc: 6.38 ng/ml