

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010224\
 Data File : PS025411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2024 21:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 01:40:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.351	6.762	1094.5E6	345.2E6	488.442	486.352
Target Compounds							
1) T	Dalapon	2.505	2.557	9937990	3927897	3.211	3.418
2) T	3,5-DICHL...	5.693	0.000	1184564	0	<MDL	N.D. #
3) T	4-Nitroph...	6.191	6.364	9210051	1007048	5.945	2.027 #
5) T	DICAMBA	0.000	6.960	0	1682178	N.D.	<MDL
6) T	MCP	6.704f	6.960f	62991845	1682178	9.363	<MDL #
7) T	MCPA	6.704f	7.155f	62991845	13215409	6.642	4.205 #
8) T	DICHLORPROP	0.000	7.560	0	40800039	N.D.	52.745
9) T	2,4-D	7.246	7.770f	11256732	-318126	3.634	N.D. #
12) T	2,4,5-T	0.000	9.031f	0	745616	N.D.	<MDL
15) T	Picloram	0.000	10.776	0	1398437	N.D.	<MDL
16) T	DCPA	0.000	10.776f	0	1398437	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010224\
Data File : PS025411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2024 21:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 01:40:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

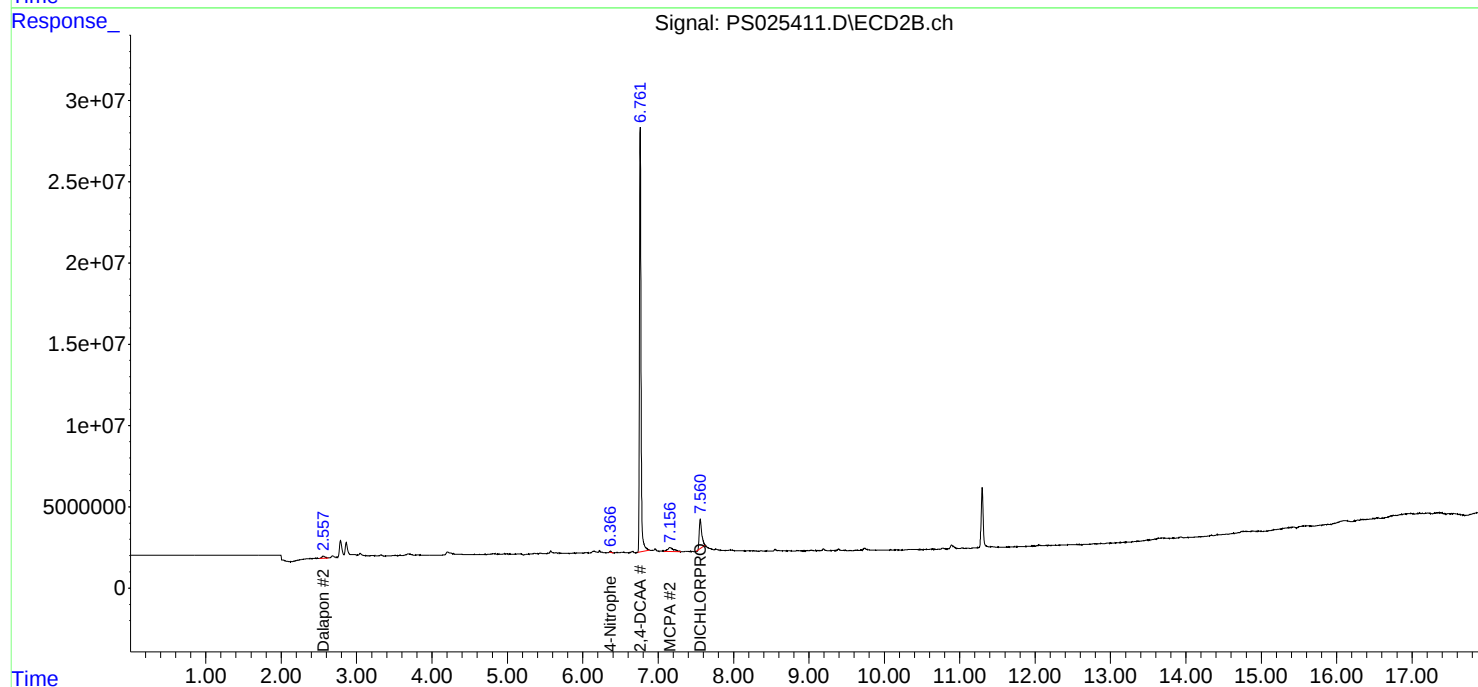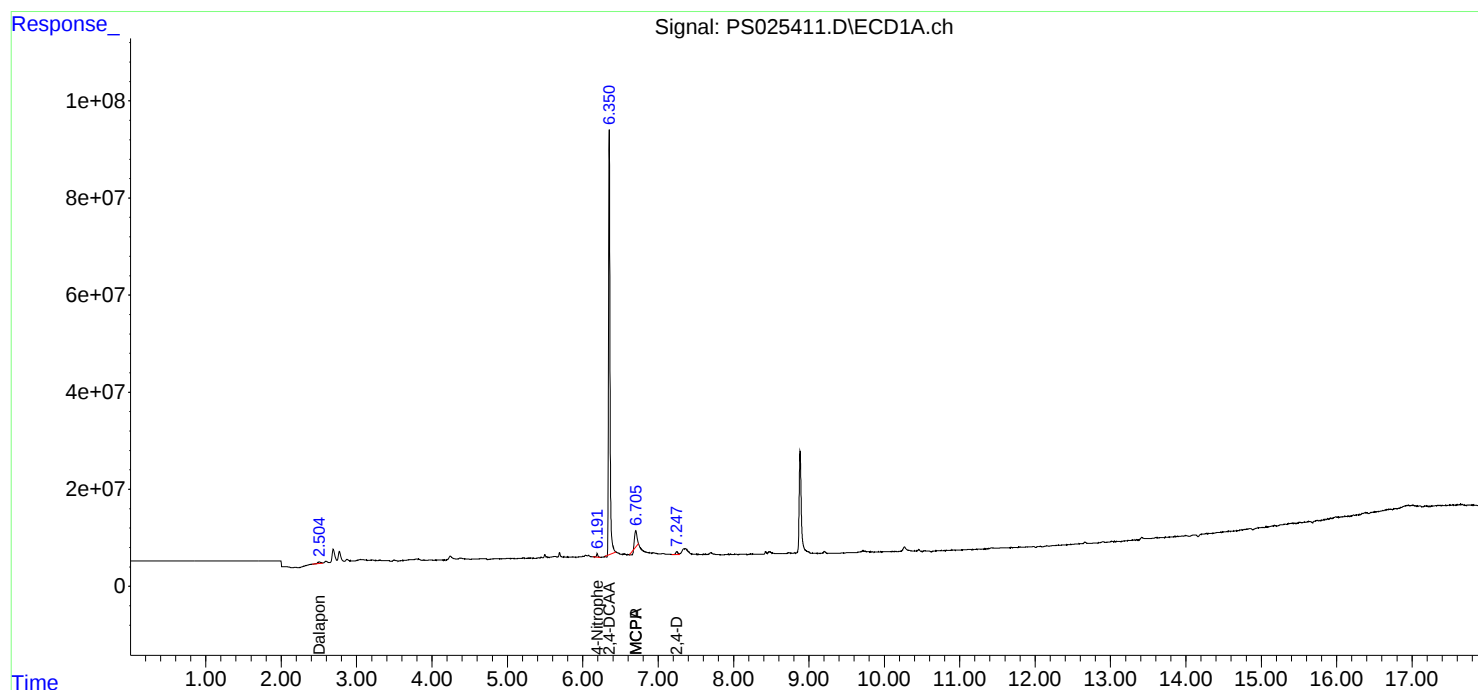


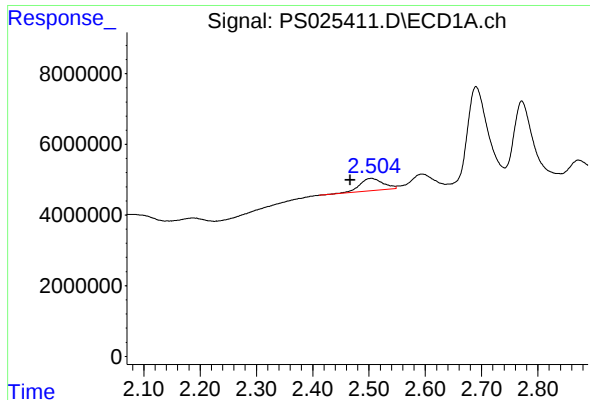

#1 Dalapon


R.T.: 2.505 min
Delta R.T.: 0.038 min
Response: 9937990
Conc: 3.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

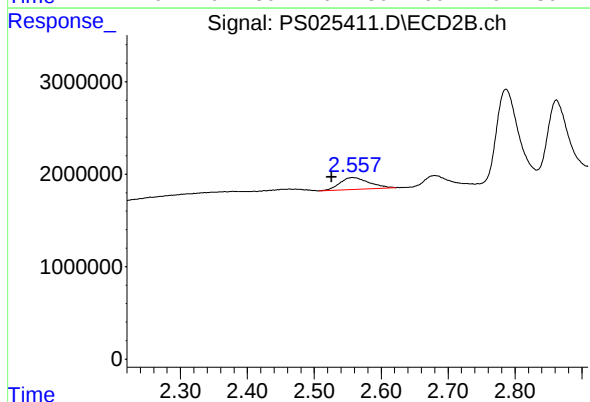


#1 Dalapon

R.T.: 2.557 min
Delta R.T.: 0.031 min
Response: 3927897
Conc: 3.42 ng/ml

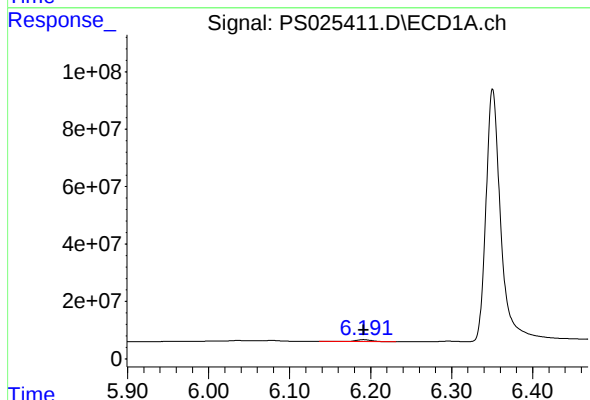


#3 4-Nitrophenol

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 9210051
Conc: 5.95 ng/ml

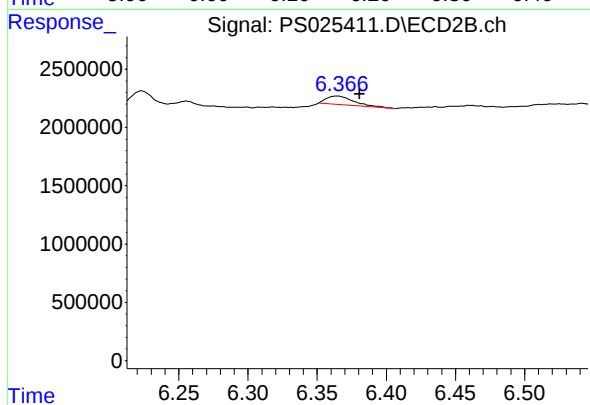

#3 4-Nitrophenol


R.T.: 6.364 min
Delta R.T.: -0.016 min
Response: 1007048
Conc: 2.03 ng/ml

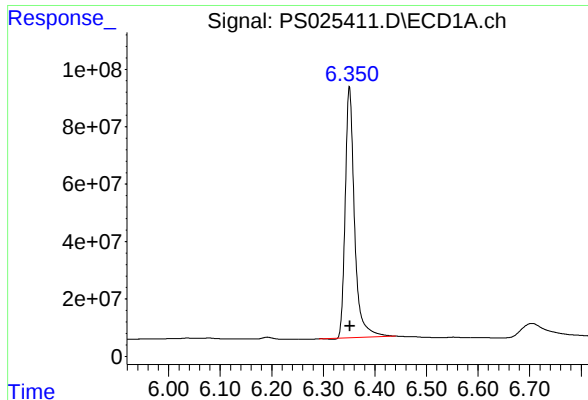

#4 2,4-DCAA


R.T.: 6.351 min
Delta R.T.: -0.001 min
Response: 1094501446
Conc: 488.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

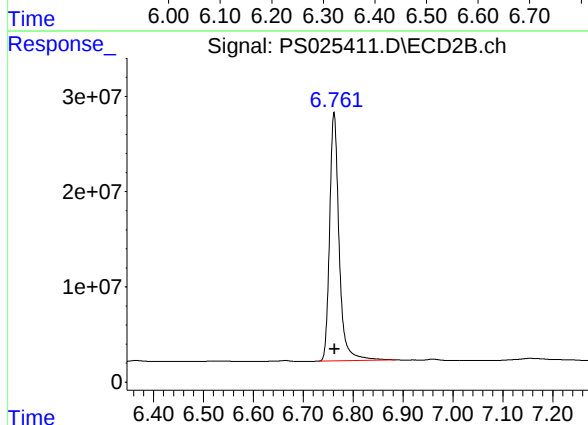


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.002 min
Response: 345199948
Conc: 486.35 ng/ml

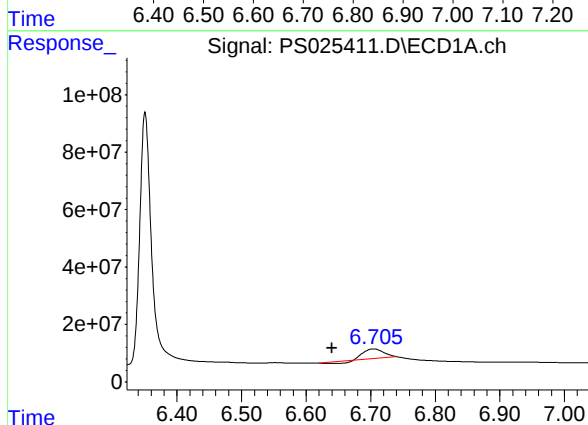


#6 MCPP

R.T.: 6.704 min
Delta R.T.: 0.065 min
Response: 62991845
Conc: 9.36 ug/ml

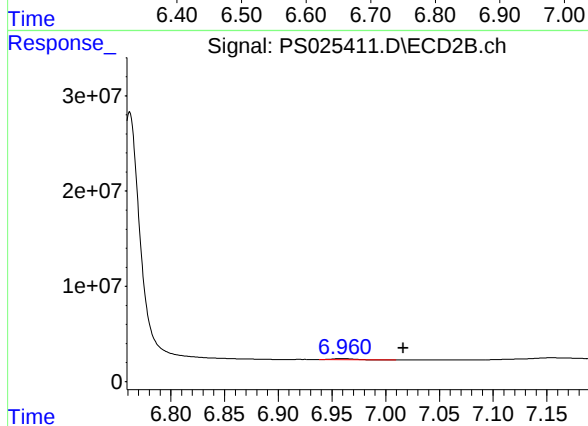

#6 MCPP


R.T.: 6.960 min
Delta R.T.: -0.057 min
Response: 1682178
Conc: N.D.

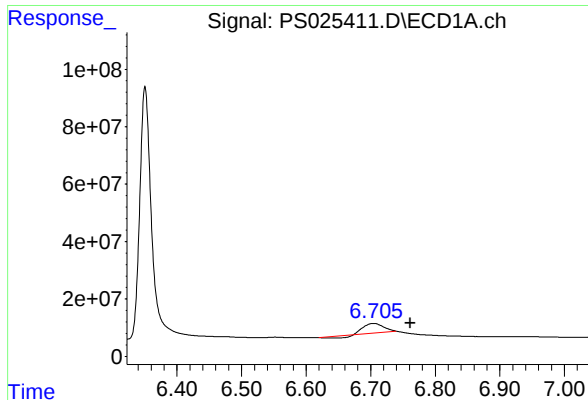

#7 MCPA


R.T.: 6.704 min
Delta R.T.: -0.057 min
Response: 62991845
Conc: 6.64 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

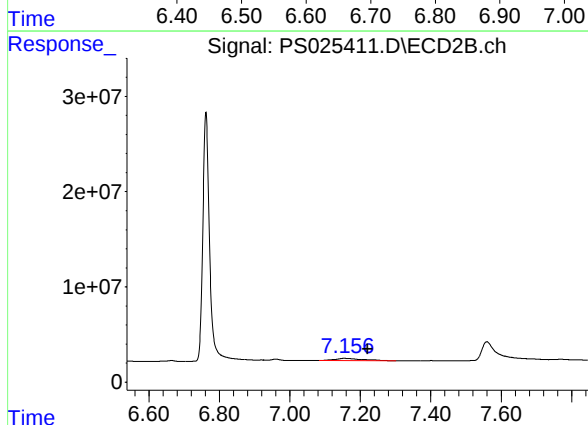


#7 MCPA

R.T.: 7.155 min
Delta R.T.: -0.066 min
Response: 13215409
Conc: 4.20 ug/ml

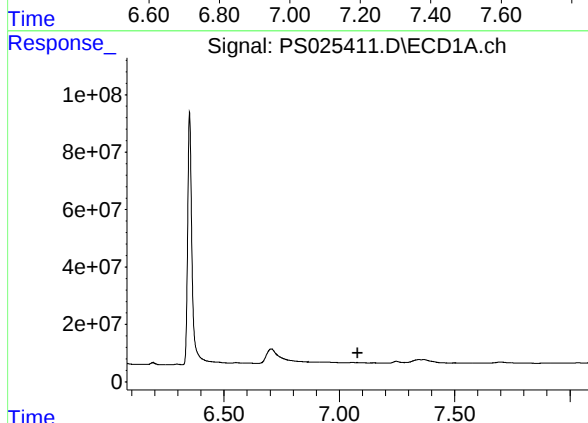


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

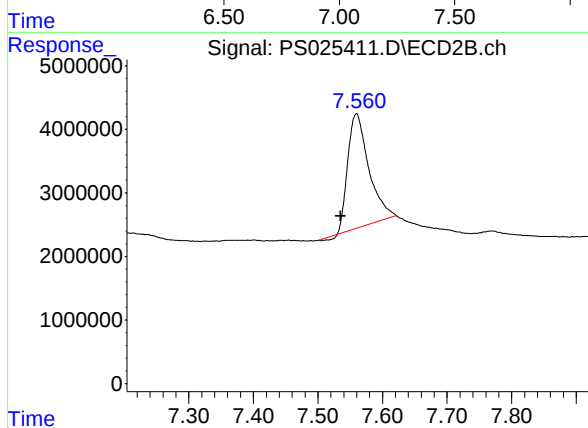

#8 DICHLORPROP


R.T.: 7.560 min
Delta R.T.: 0.025 min
Response: 40800039
Conc: 52.74 ng/ml

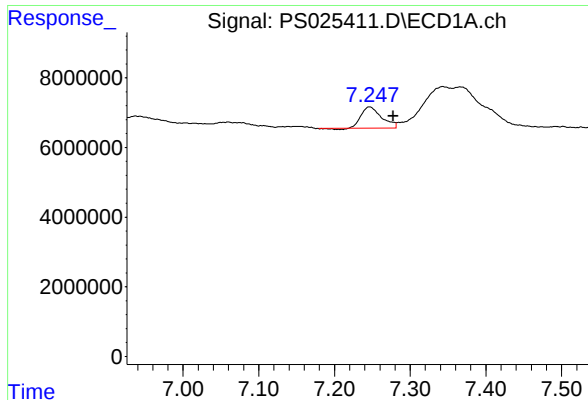

#9 2,4-D

R.T.: 7.246 min
Delta R.T.: -0.031 min
Response: 11256732
Conc: 3.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

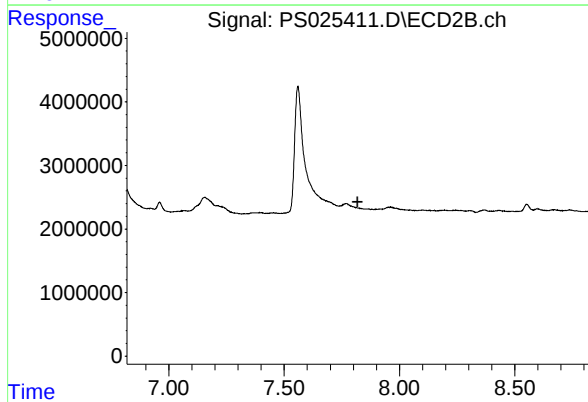

#9 2,4-D

R.T.: 7.770 min
Delta R.T.: -0.049 min
Response: -318126
Conc: N.D.