

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010224\
 Data File : PS025423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2024 02:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 05:05:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.351	6.762	1092.4E6	344.3E6	487.492	485.031
Target Compounds						
1) T Dalapon	0.000	2.554	0	2970723	N.D.	2.585
2) T 3,5-DICHL...	5.693	0.000	1405890	0	<MDL	N.D. #
3) T 4-Nitroph...	0.000	6.361	0	693047	N.D.	1.395
5) T DICAMBA	0.000	6.961	0	1982305	N.D.	<MDL
6) T MCPP	0.000	6.961f	0	1982305	N.D.	<MDL
7) T MCPA	6.713f	7.230	9285274	1299496	<MDL	<MDL #
8) T DICHLORPROP	0.000	7.556	0	4706039	N.D.	6.084
9) T 2,4-D	7.247	0.000	14991232	0	4.839	N.D. #
15) T Picloram	0.000	10.784	0	647212	N.D.	<MDL
16) T DCPA	0.000	10.784f	0	647212	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010224\
Data File : PS025423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2024 02:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 05:05:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

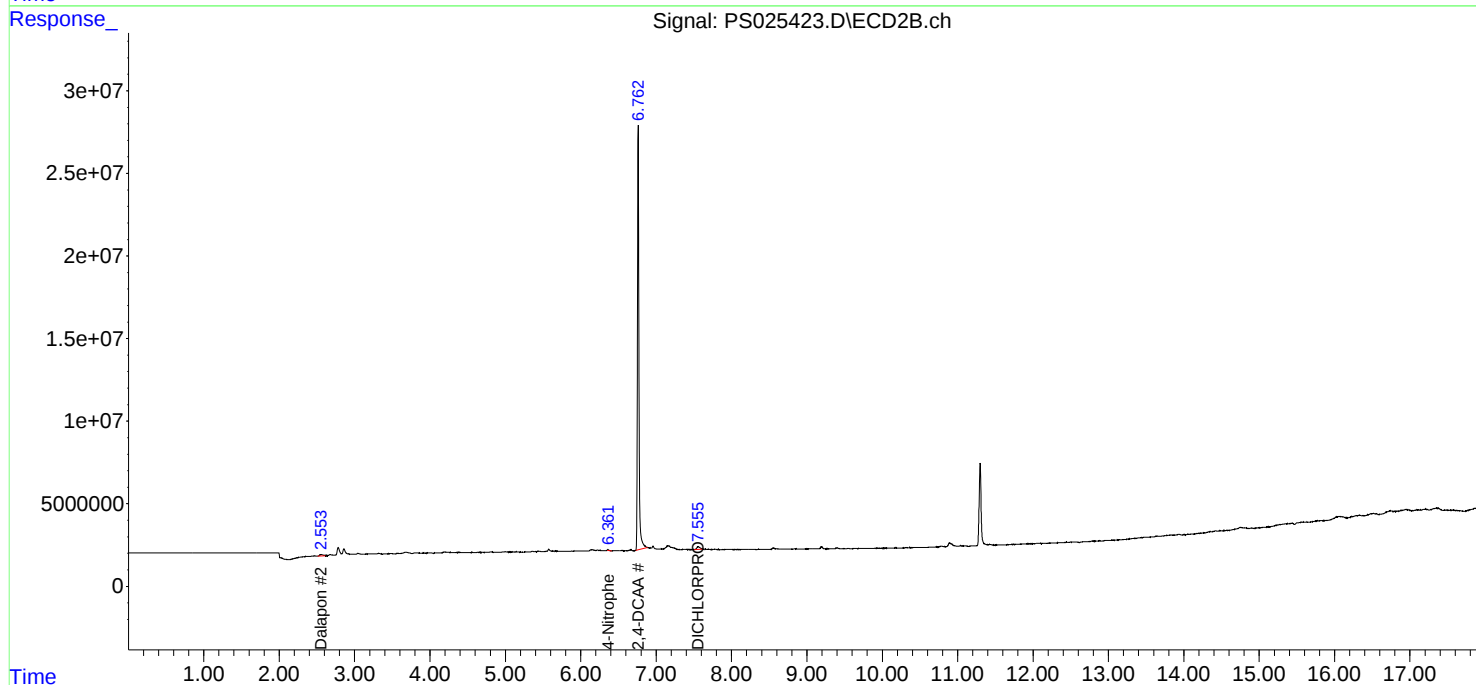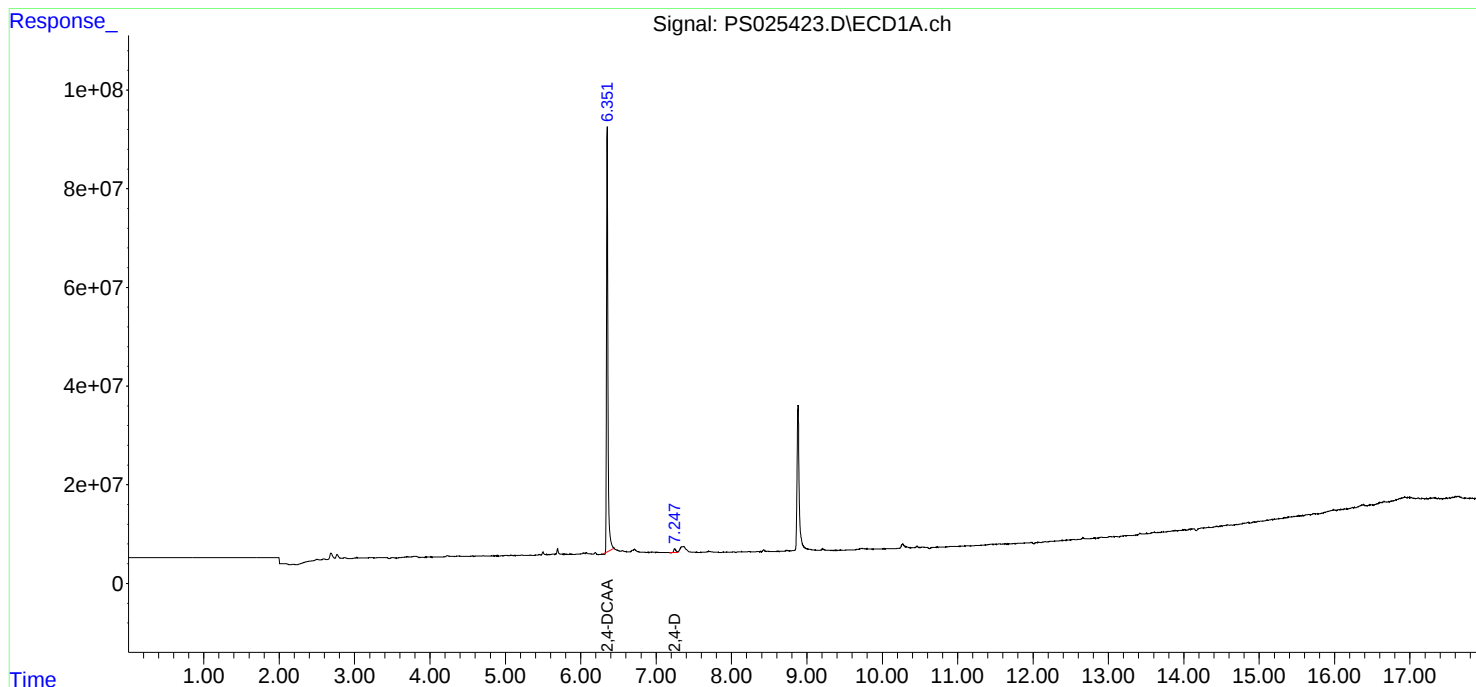


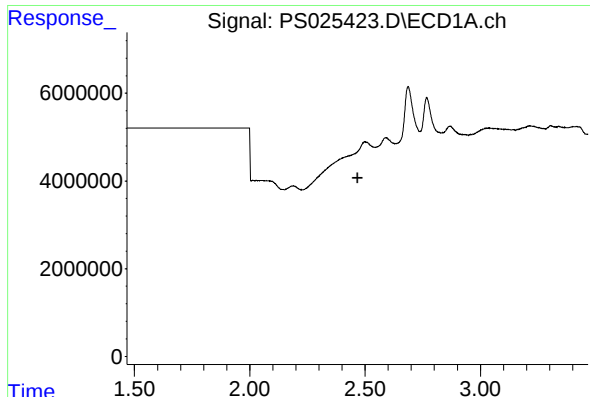

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

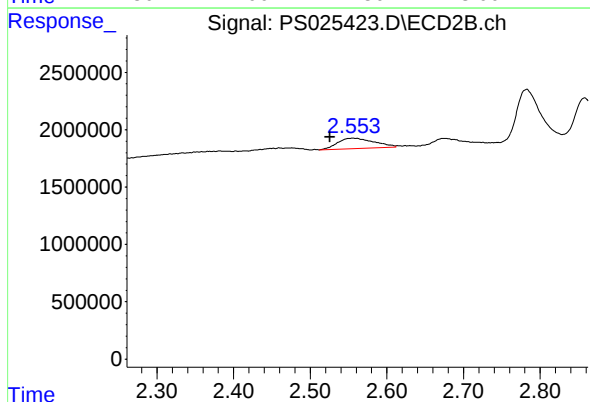


#1 Dalapon

R.T.: 2.554 min
Delta R.T.: 0.028 min
Response: 2970723
Conc: 2.58 ng/ml

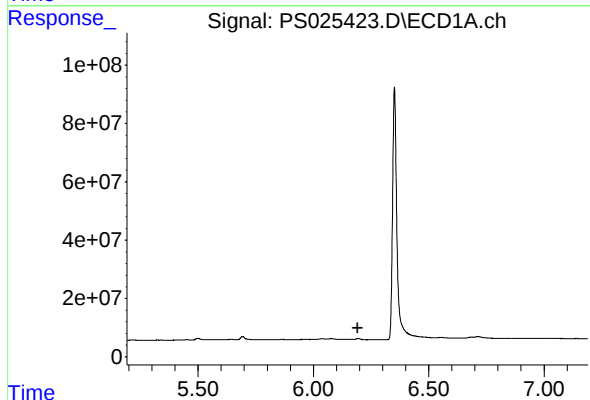


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

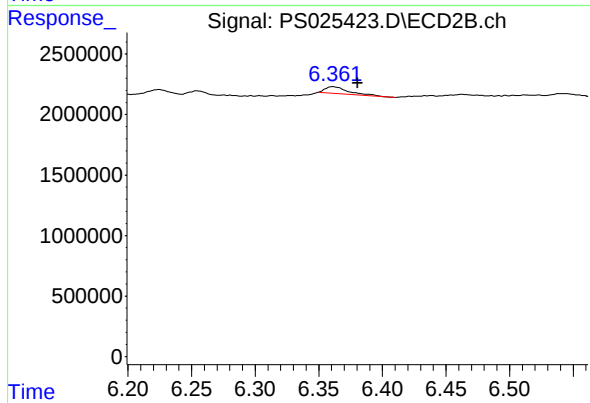

#3 4-Nitrophenol


R.T.: 6.361 min
Delta R.T.: -0.020 min
Response: 693047
Conc: 1.40 ng/ml

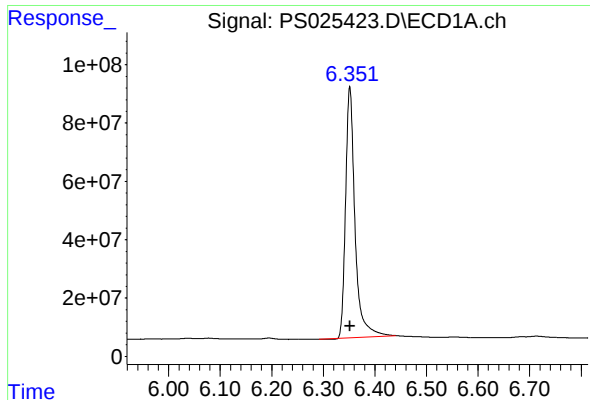

#4 2,4-DCAA


R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 1092373465
Conc: 487.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

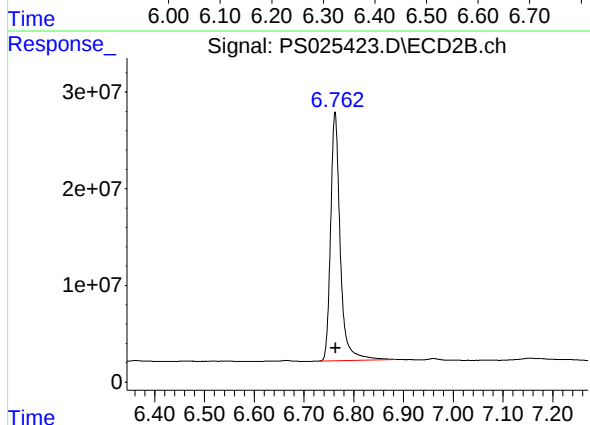


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 344262246
Conc: 485.03 ng/ml

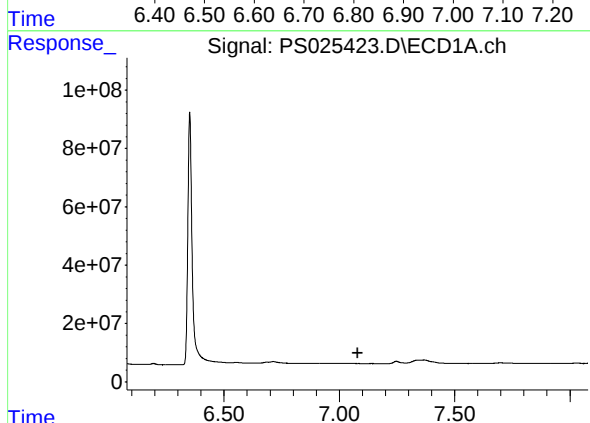


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

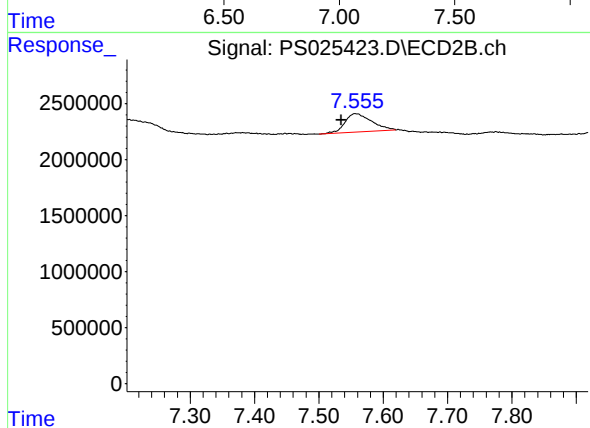

#8 DICHLORPROP


R.T.: 7.556 min
Delta R.T.: 0.021 min
Response: 4706039
Conc: 6.08 ng/ml

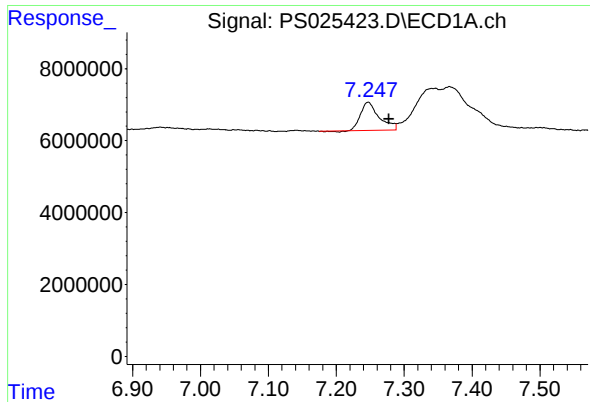

#9 2,4-D

R.T.: 7.247 min
Delta R.T.: -0.031 min
Response: 14991232
Conc: 4.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

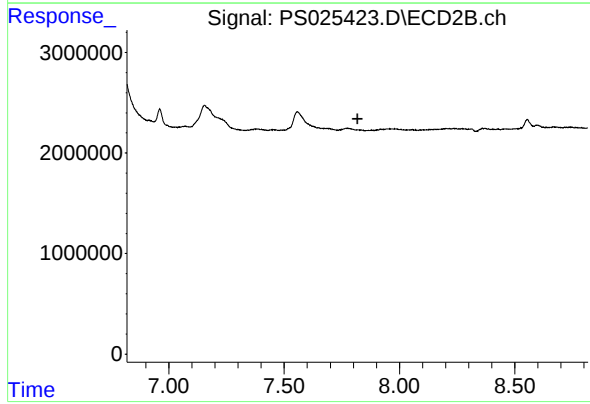

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.818 min
Response: 0
Conc: N.D.