

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS010224\  
 Data File : PS025423.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 03 Jan 2024 02:17  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 03 05:05:30 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS122823.M  
 Quant Title : 8080.M  
 QLast Update : Thu Dec 28 17:23:18 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2    | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|---------|----------|---------|---------|---------|
| -----                       |              |        |         |          |         |         |         |
| System Monitoring Compounds |              |        |         |          |         |         |         |
| 4) S                        | 2,4-DCAA     | 6.351  | 6.762   | 1092.4E6 | 344.3E6 | 487.492 | 485.031 |
| Target Compounds            |              |        |         |          |         |         |         |
| 1) T                        | Dalapon      | 0.000  | 2.554   | 0        | 2970723 | N.D.    | 2.585   |
| 2) T                        | 3,5-DICHL... | 5.693  | 0.000   | 1405890  | 0       | <MDL    | N.D. #  |
| 3) T                        | 4-Nitroph... | 0.000  | 6.361   | 0        | 693047  | N.D.    | 1.395   |
| 5) T                        | DICAMBA      | 0.000  | 6.961   | 0        | 1982305 | N.D.    | <MDL    |
| 6) T                        | MCP          | 0.000  | 6.961f  | 0        | 1982305 | N.D.    | <MDL    |
| 7) T                        | MCPA         | 6.713f | 7.230   | 9285274  | 1299496 | <MDL    | <MDL #  |
| 8) T                        | DICHLORPROP  | 0.000  | 7.556   | 0        | 4706039 | N.D.    | 6.084   |
| 9) T                        | 2,4-D        | 7.247  | 0.000   | 14991232 | 0       | 4.839   | N.D. #  |
| 15) T                       | Picloram     | 0.000  | 10.784  | 0        | 647212  | N.D.    | <MDL    |
| 16) T                       | DCPA         | 0.000  | 10.784f | 0        | 647212  | N.D.    | <MDL    |
| -----                       |              |        |         |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS010224\  
Data File : PS025423.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 03 Jan 2024 02:17  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 03 05:05:30 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS122823.M  
Quant Title : 8080.M  
QLast Update : Thu Dec 28 17:23:18 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

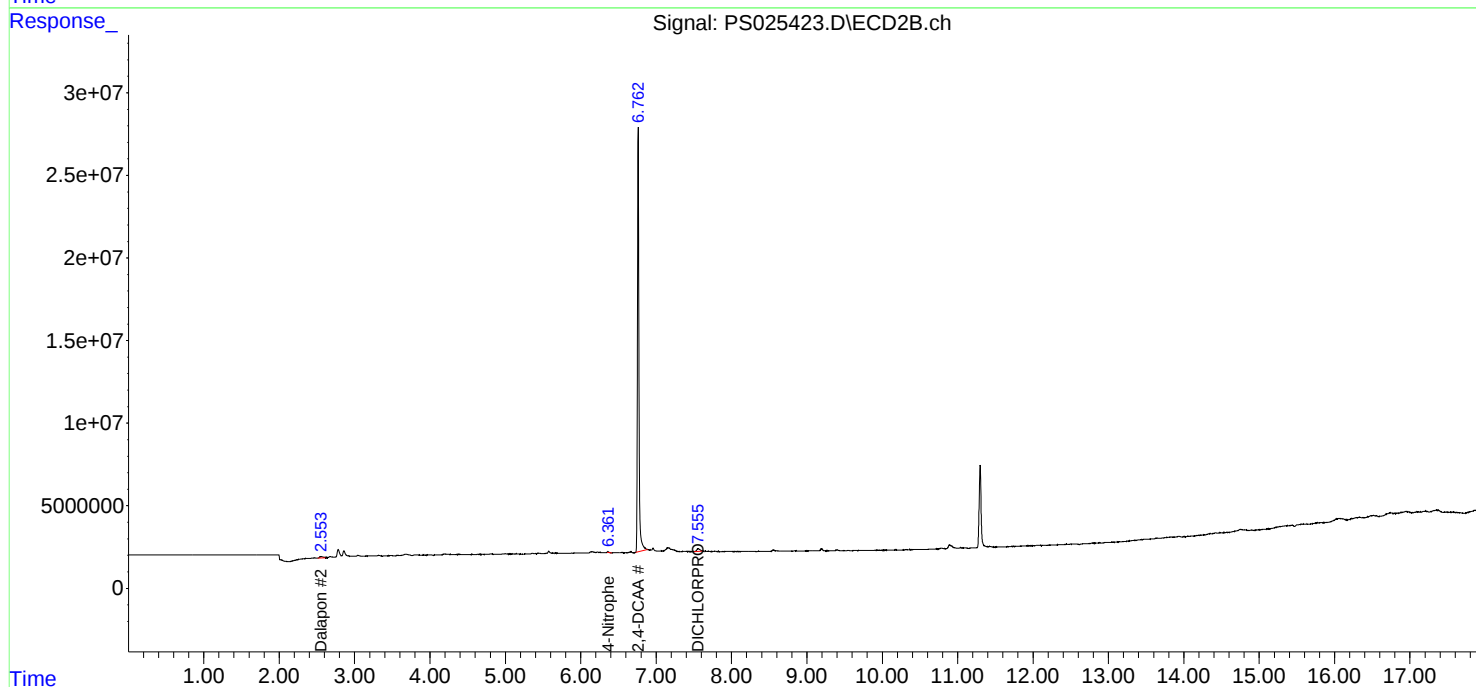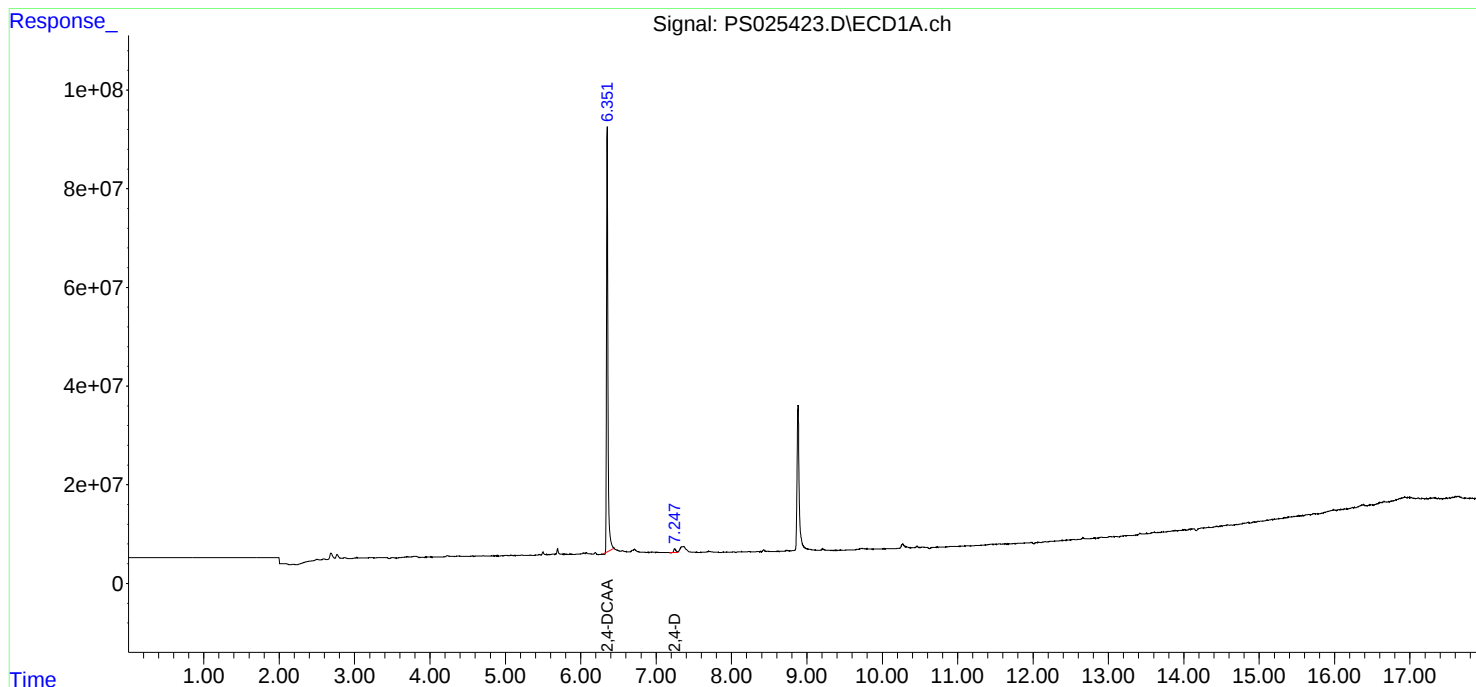


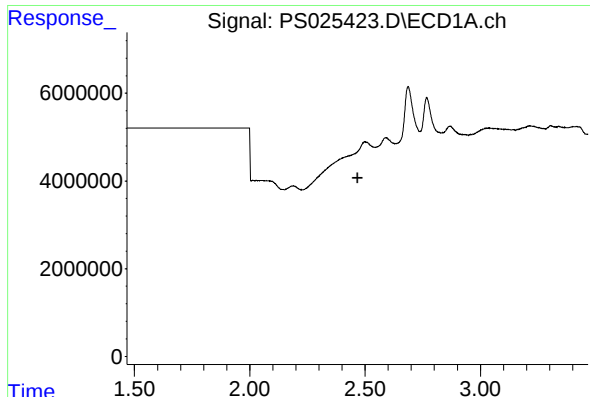

#1 Dalapon


R.T.: 0.000 min  
Exp R.T.: 2.467 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

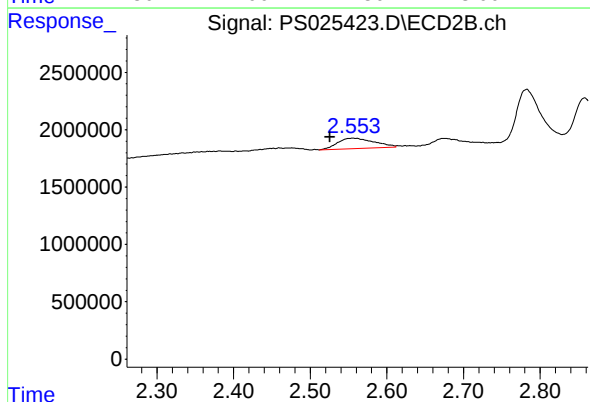


#1 Dalapon

R.T.: 2.554 min  
Delta R.T.: 0.028 min  
Response: 2970723  
Conc: 2.58 ng/ml

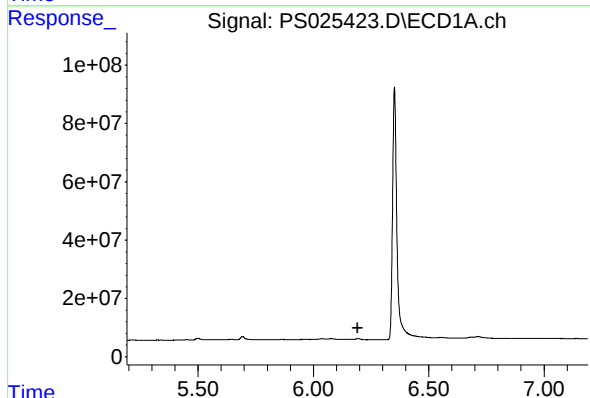


#3 4-Nitrophenol

R.T.: 0.000 min  
Exp R.T.: 6.191 min  
Response: 0  
Conc: N.D.

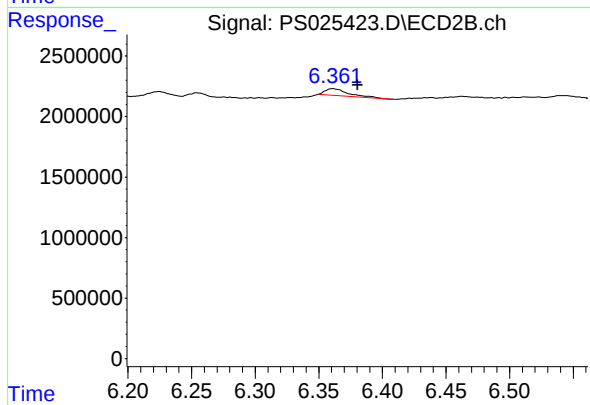

#3 4-Nitrophenol


R.T.: 6.361 min  
Delta R.T.: -0.020 min  
Response: 693047  
Conc: 1.40 ng/ml

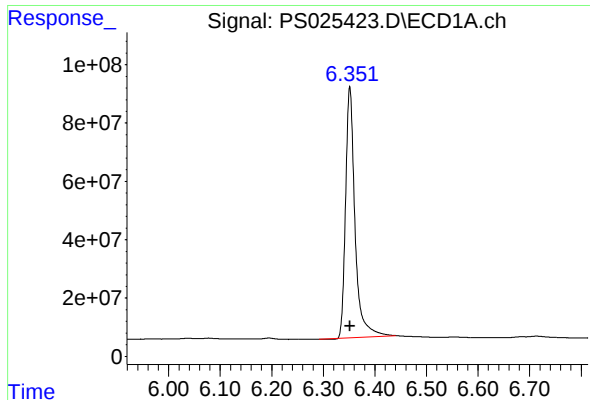

#4 2,4-DCAA


R.T.: 6.351 min  
Delta R.T.: 0.000 min  
Response: 1092373465  
Conc: 487.49 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

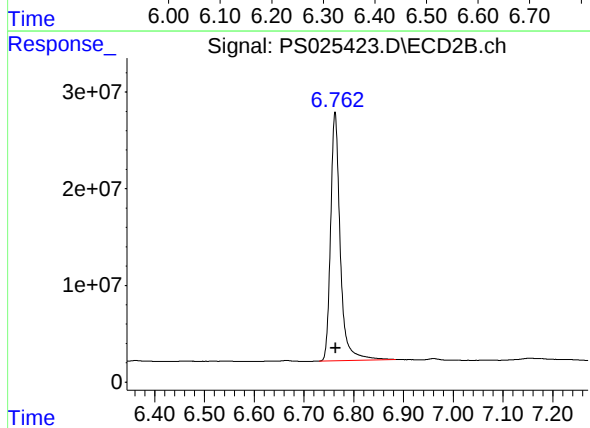


#4 2,4-DCAA

R.T.: 6.762 min  
Delta R.T.: -0.001 min  
Response: 344262246  
Conc: 485.03 ng/ml

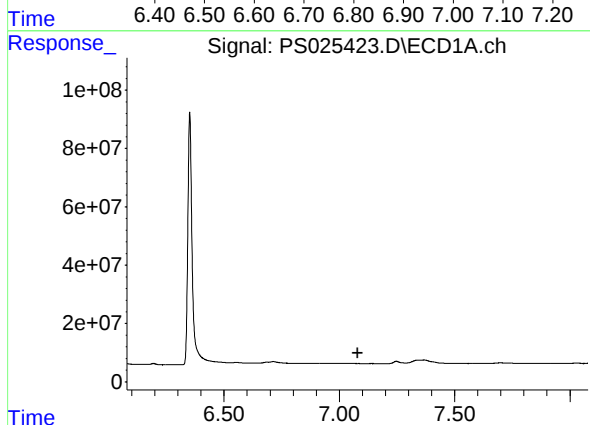


#8 DICHLORPROP

R.T.: 0.000 min  
Exp R.T.: 7.079 min  
Response: 0  
Conc: N.D.

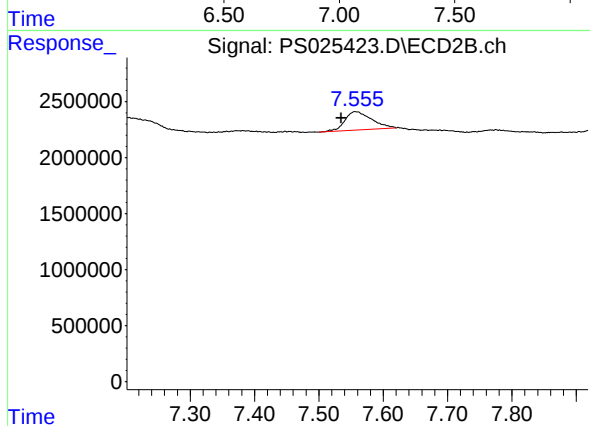

#8 DICHLORPROP


R.T.: 7.556 min  
Delta R.T.: 0.021 min  
Response: 4706039  
Conc: 6.08 ng/ml

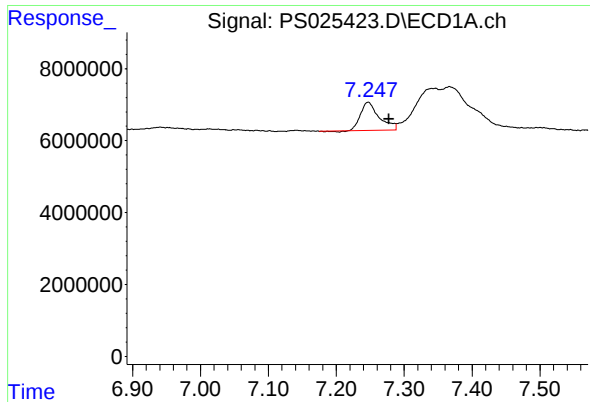

#9 2,4-D

R.T.: 7.247 min  
Delta R.T.: -0.031 min  
Response: 14991232  
Conc: 4.84 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

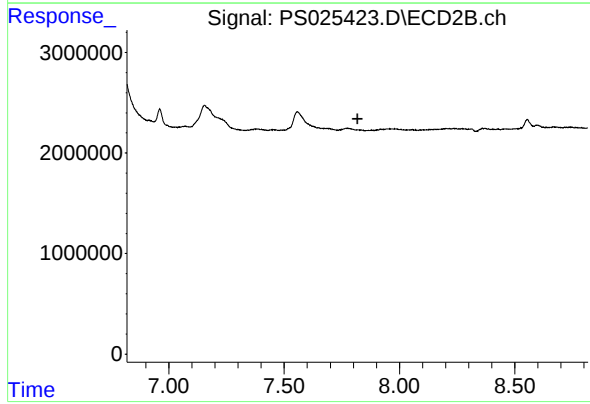

#9 2,4-D

R.T.: 0.000 min  
Exp R.T. : 7.818 min  
Response: 0  
Conc: N.D.