

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010225\
 Data File : PS028866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2025 10:10
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 21:44:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	0.000	2.705f	0	5456939	N.D.	2.772
2) T	3,5-DICHL...	6.402	0.000	537426	0	<MDL	N.D. #
3) T	4-Nitroph...	6.991	0.000	2741188	0	1.825	N.D. #
6) T	MCP	7.569	0.000	134096	0	<MDL	N.D. #
7) T	MCPA	0.000	8.225	0	5823078	N.D.	1.257
8) T	DICHLORPROP	8.121	8.649f	495322	4002524	<MDL	2.901 #
10) T	Pentachlo...	8.667f	0.000	543950	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.169f	0.000	516656	0	<MDL	N.D. #
12) T	2,4,5-T	9.451f	10.243	5207005	3409653	<MDL	<MDL #
13) T	2,4-DB	10.063	0.000	2103337	0	<MDL	N.D. #
14) T	DINOSEB	11.265	0.000	2048793	0	<MDL	N.D. #
15) T	Picloram	11.103	12.286	17407593	10987667	<MDL	<MDL #
16) T	DCPA	11.548	12.286f	1645110	10987667	<MDL	1.023 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010225\
Data File : PS028866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2025 10:10
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 21:44:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

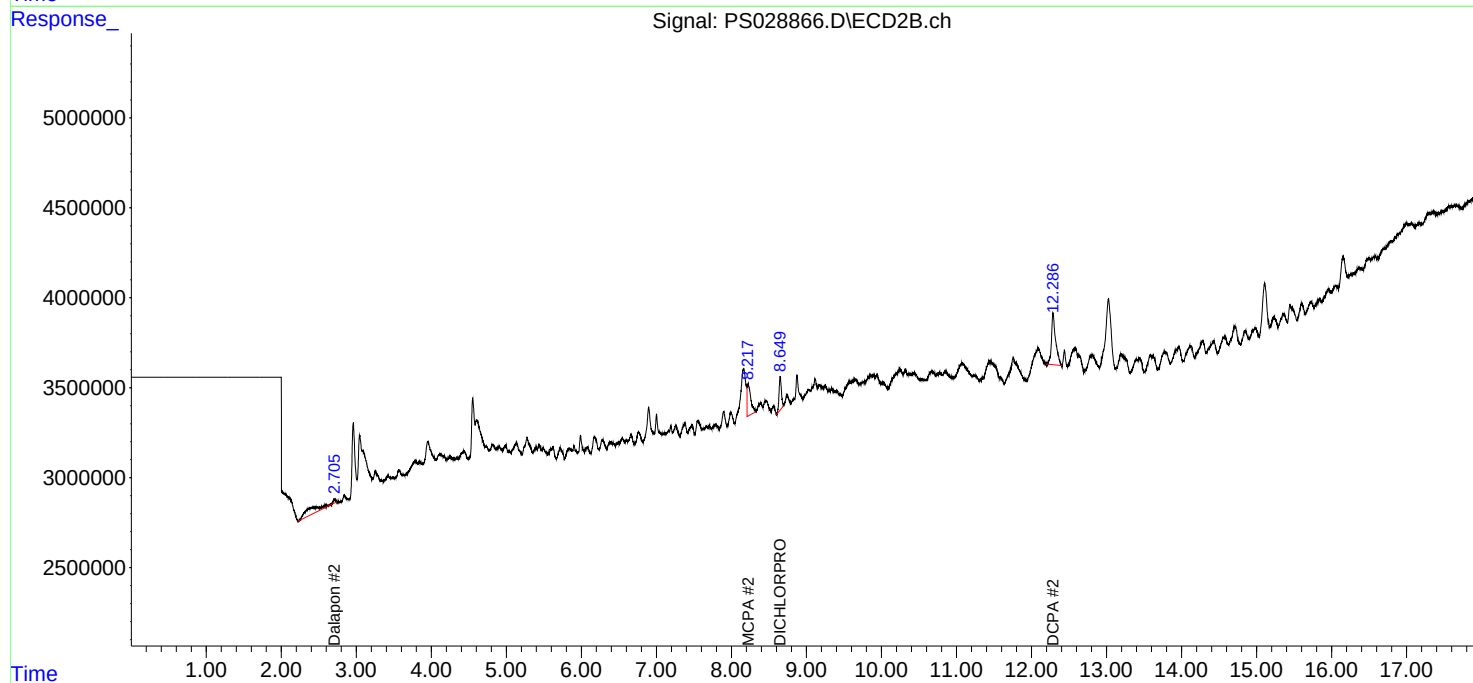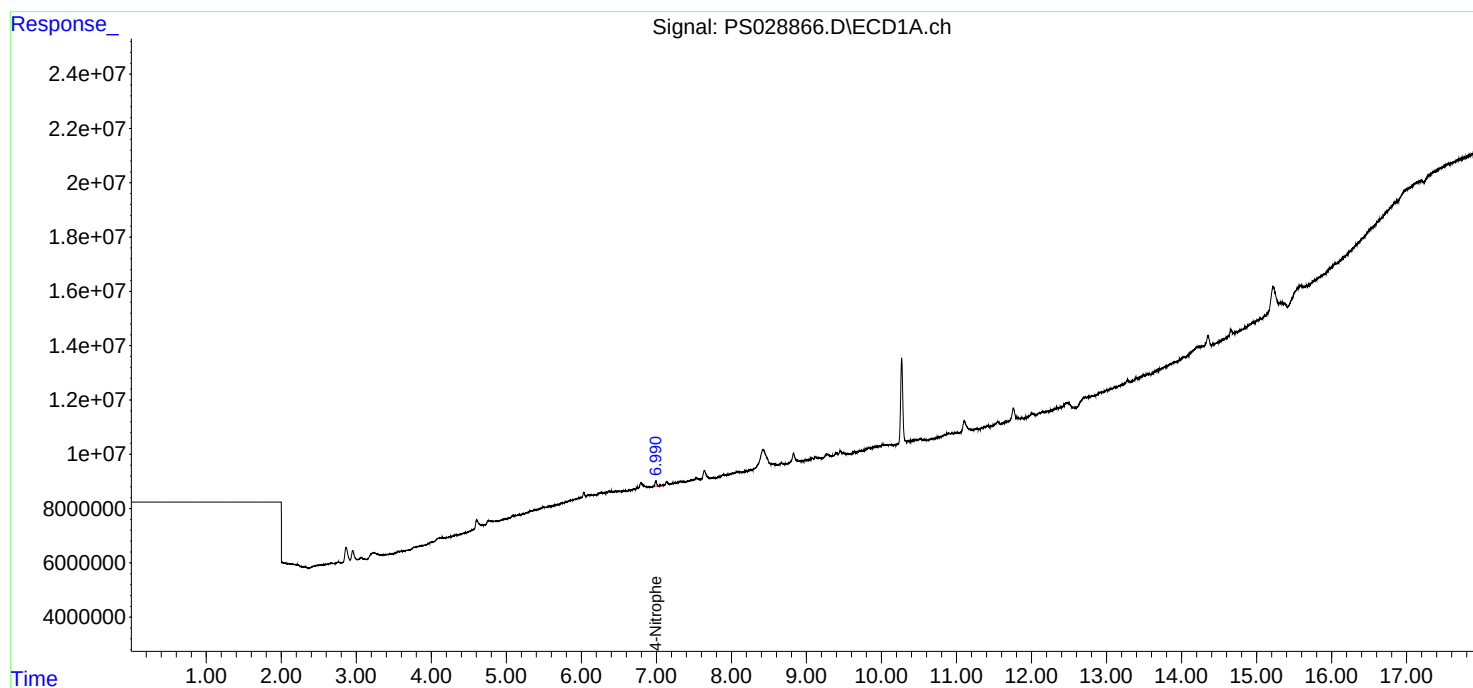


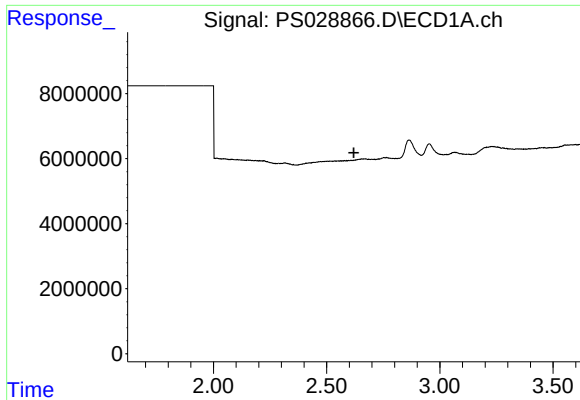

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

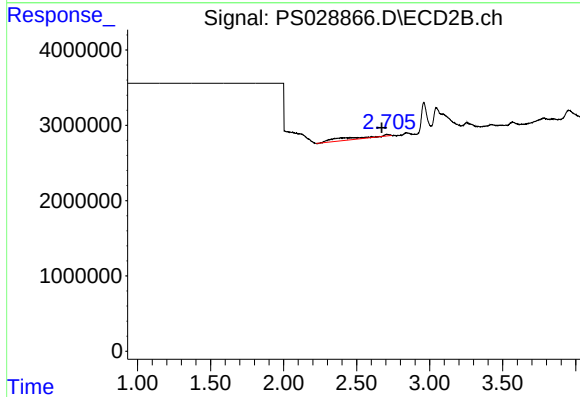


#1 Dalapon

R.T.: 2.705 min
Delta R.T.: 0.033 min
Response: 5456939
Conc: 2.77 ng/ml

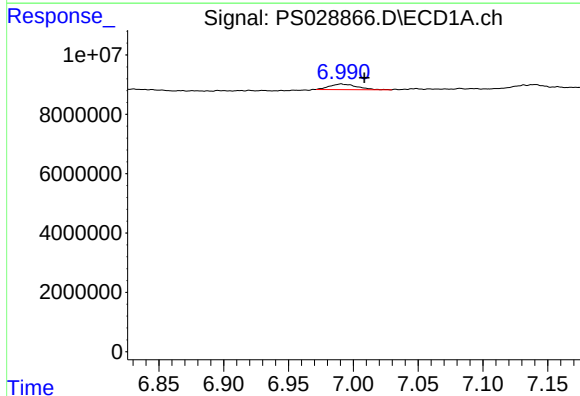


#3 4-Nitrophenol

R.T.: 6.991 min
Delta R.T.: -0.017 min
Response: 2741188
Conc: 1.82 ng/ml

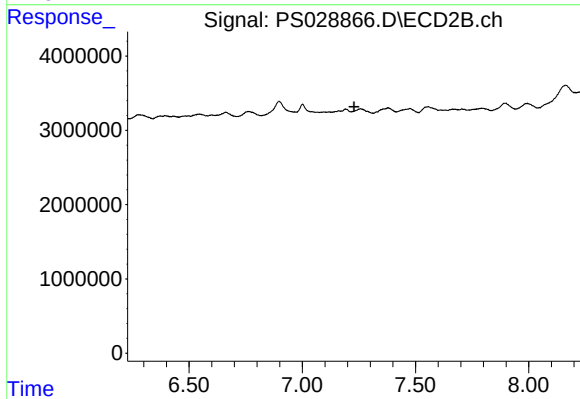

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.228 min
Response: 0
Conc: N.D.

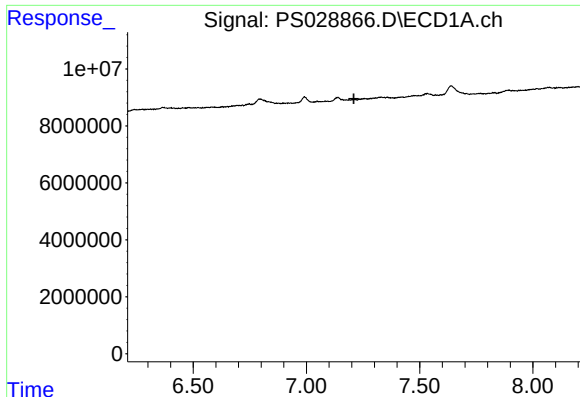

#4 2,4-DCAA


R.T.: 7.255 min
Delta R.T.: 0.045 min
Response: -142057
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

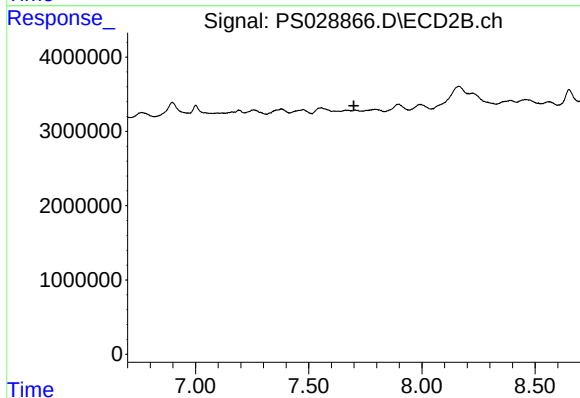


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.699 min
Response: 0
Conc: N.D.

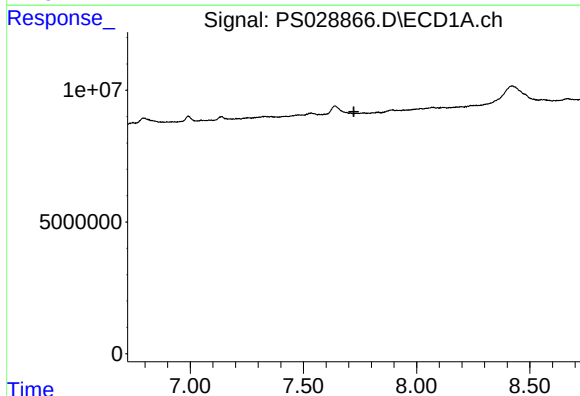


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.723 min
Response: 0
Conc: N.D.

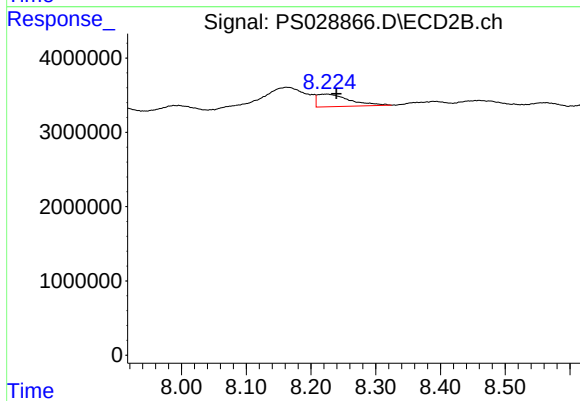

#7 MCPA


R.T.: 8.225 min
Delta R.T.: -0.015 min
Response: 5823078
Conc: 1.26 ug/ml

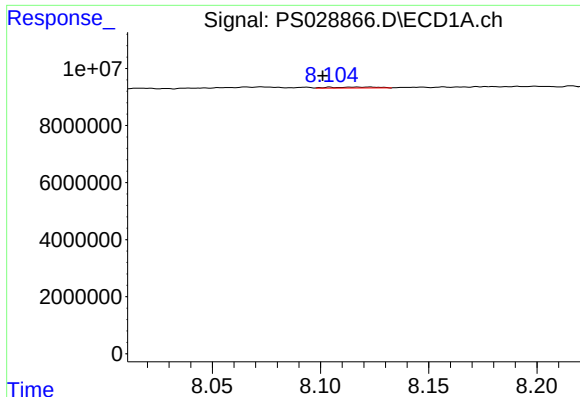

#8 DICHLORPROP


R.T.: 8.121 min
Delta R.T.: 0.020 min
Response: 495322
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

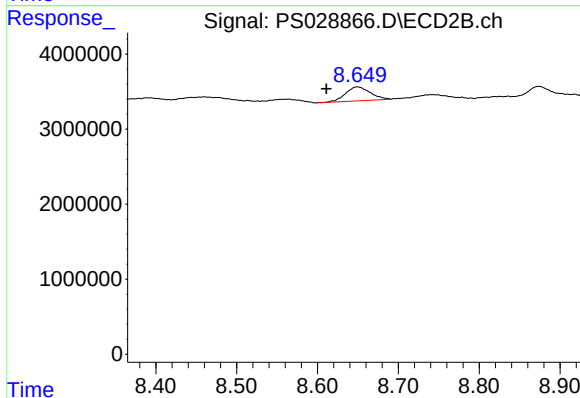


#8 DICHLORPROP

R.T.: 8.649 min
Delta R.T.: 0.038 min
Response: 4002524
Conc: 2.90 ng/ml

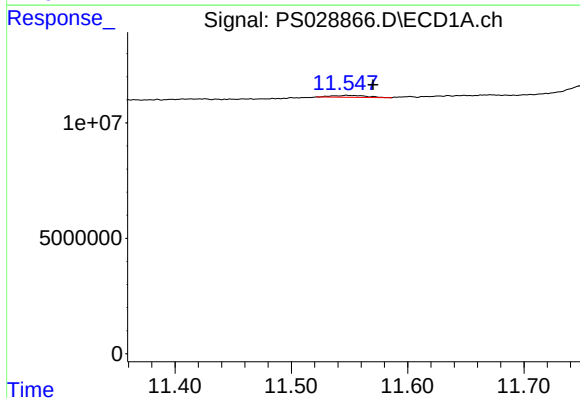

#16 DCPA

R.T.: 11.548 min
Delta R.T.: -0.022 min
Response: 1645110
Conc: N.D.

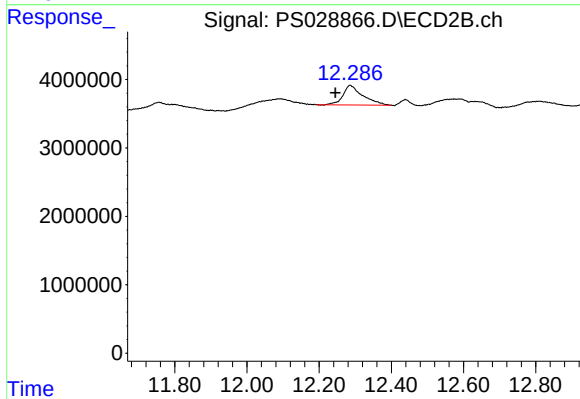

#16 DCPA

R.T.: 12.286 min
Delta R.T.: 0.040 min
Response: 10987667
Conc: 1.02 ng/ml