

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010225\
 Data File : PS028867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2025 10:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 21:45:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.208	7.690	1240.6E6	518.9E6	548.436	461.047
Target Compounds							
1) T	Dalapon	2.668f	0.000	19403085	0	6.889	N.D. #
2) T	3,5-DICHL...	6.402	0.000	740889	0	<MDL	N.D. #
3) T	4-Nitroph...	7.001	0.000	6197596	0	4.126	N.D. #
5) T	DICAMBA	7.391	7.891	-438054	3819172	N.D.	<MDL
6) T	MCP	7.586	0.000	396518	0	<MDL	N.D. #
8) T	DICHLORPROP	8.071f	8.650f	4150348	3431486	1.564	2.487 #
10) T	Pentachlo...	8.624	0.000	1227619	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.188	0.000	892577	0	<MDL	N.D. #
12) T	2,4,5-T	9.451f	0.000	5337600	0	<MDL	N.D. #
13) T	2,4-DB	10.020f	0.000	2155526	0	<MDL	N.D. #
14) T	DINOSEB	11.267	0.000	2030740	0	<MDL	N.D. #
15) T	Picloram	11.103	12.288	13828228	8719334	<MDL	<MDL #
16) T	DCPA	11.560	12.288f	1416530	8719334	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010225\
Data File : PS028867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2025 10:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 21:45:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

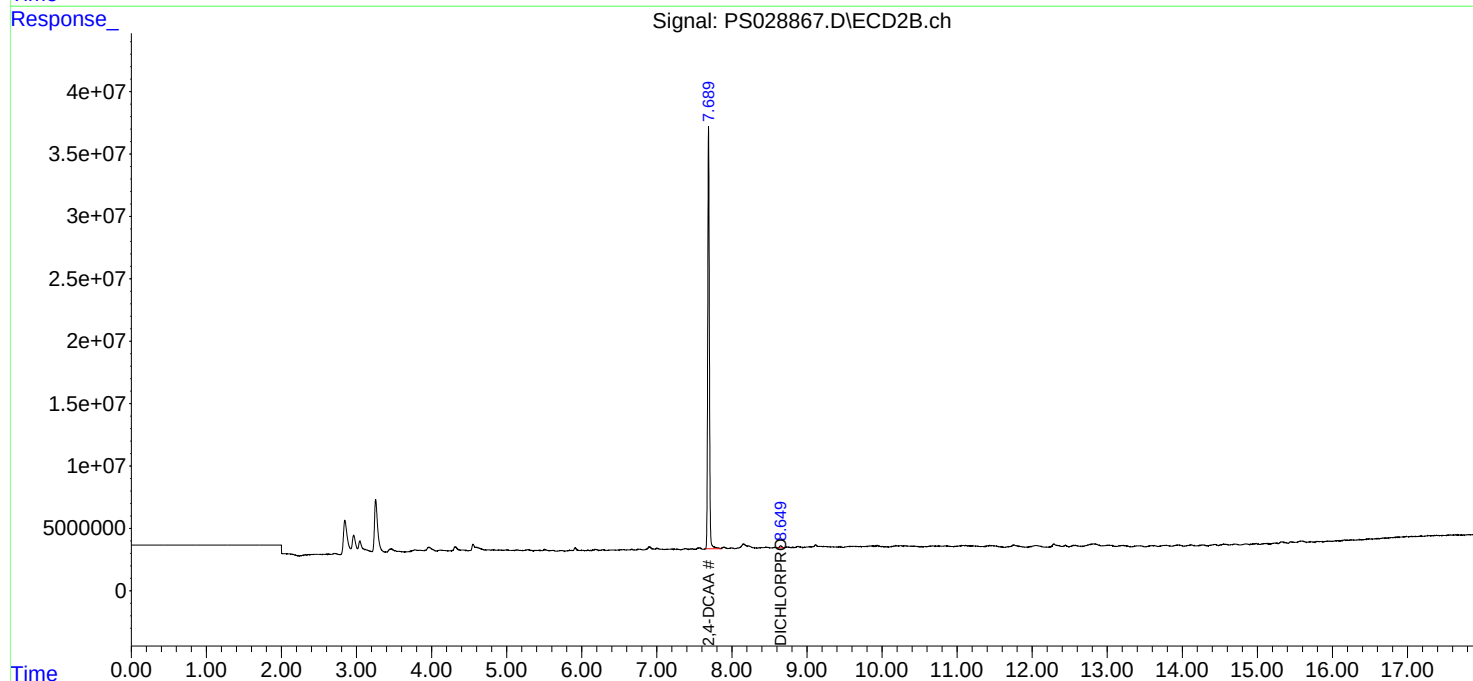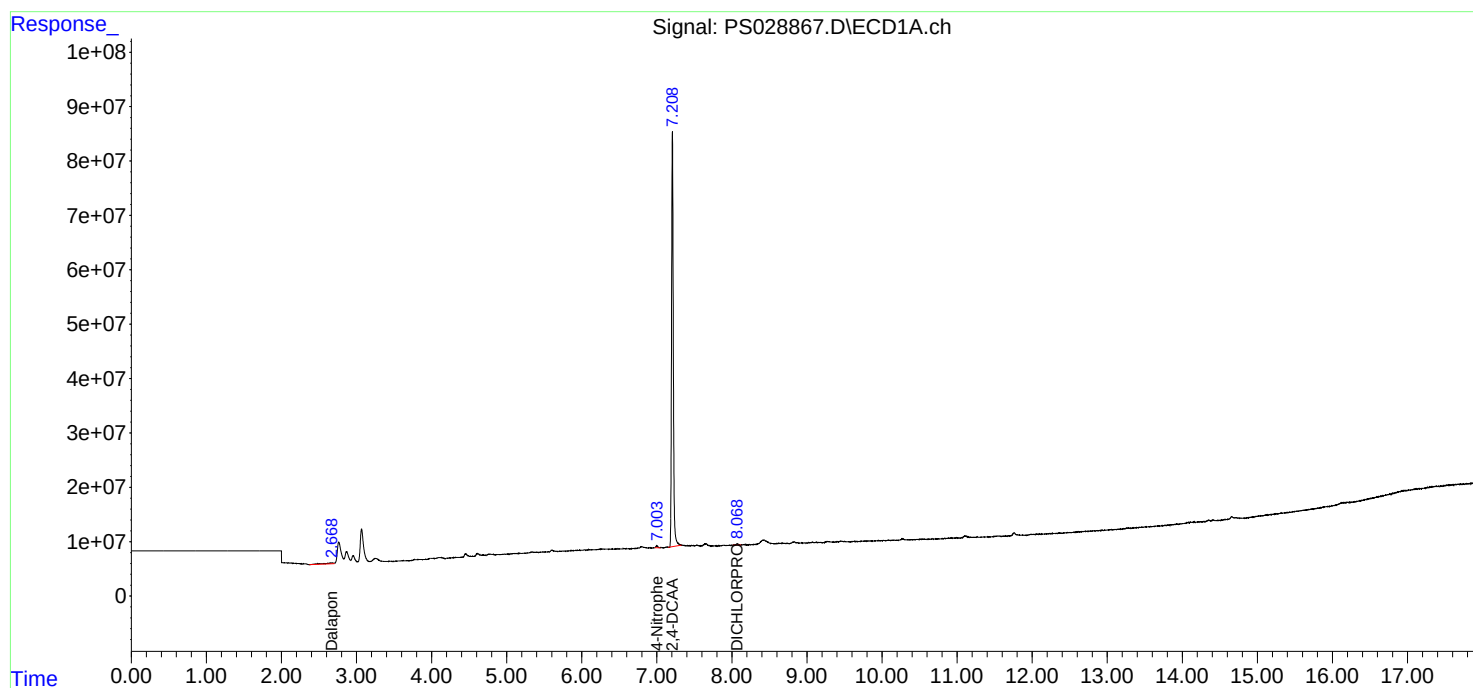


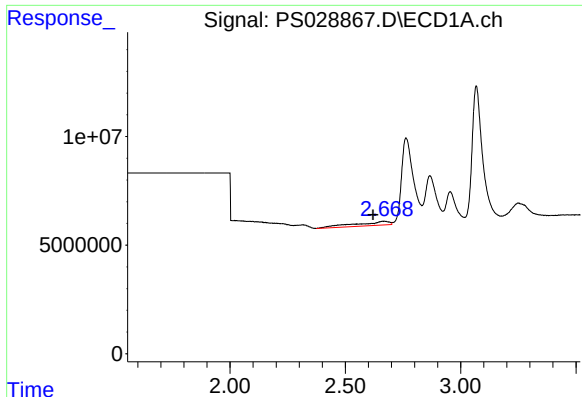

#1 Dalapon


R.T.: 2.668 min
Delta R.T.: 0.048 min
Response: 19403085
Conc: 6.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

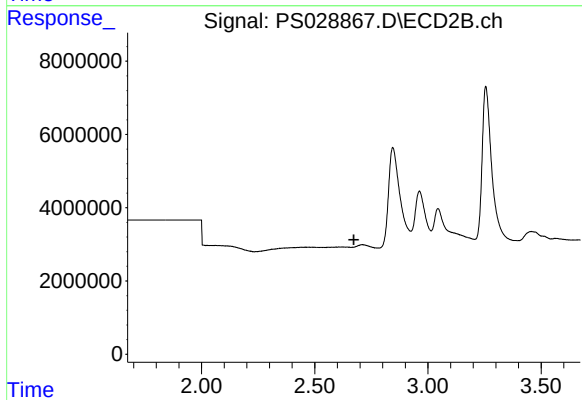


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.673 min
Response: 0
Conc: N.D.

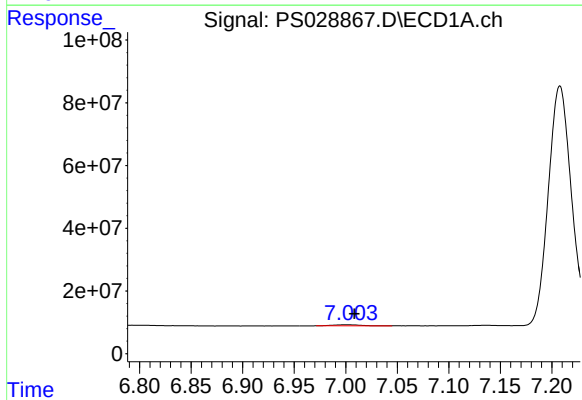


#3 4-Nitrophenol

R.T.: 7.001 min
Delta R.T.: -0.008 min
Response: 6197596
Conc: 4.13 ng/ml

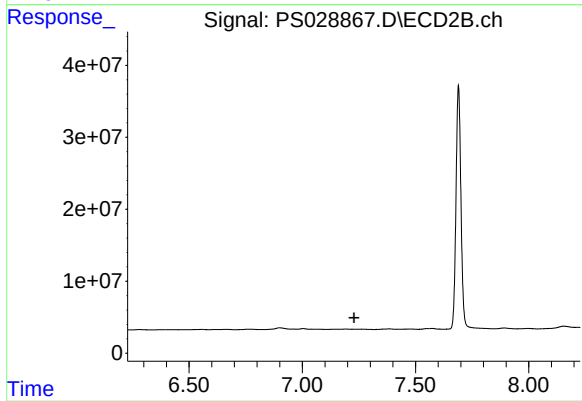

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

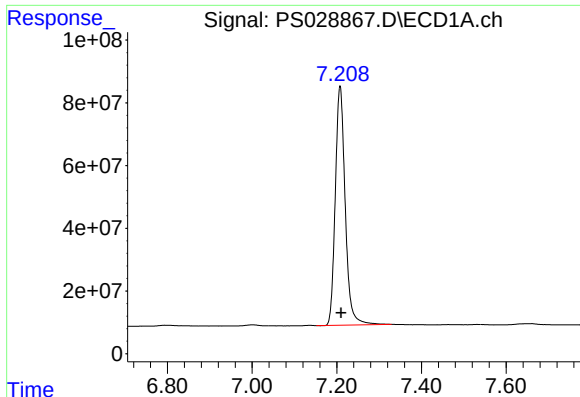

#4 2,4-DCAA


R.T.: 7.208 min
Delta R.T.: -0.002 min
Response: 1240576577
Conc: 548.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

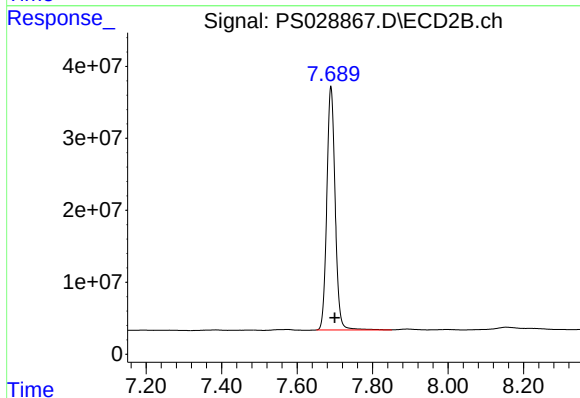


#4 2,4-DCAA

R.T.: 7.690 min
Delta R.T.: -0.010 min
Response: 518925873
Conc: 461.05 ng/ml

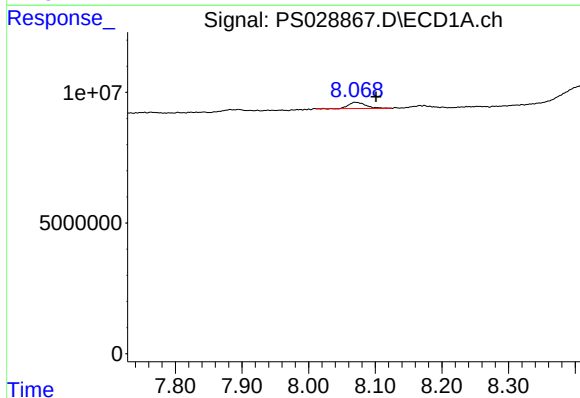

#8 DICHLORPROP

R.T.: 8.071 min
Delta R.T.: -0.030 min
Response: 4150348
Conc: 1.56 ng/ml

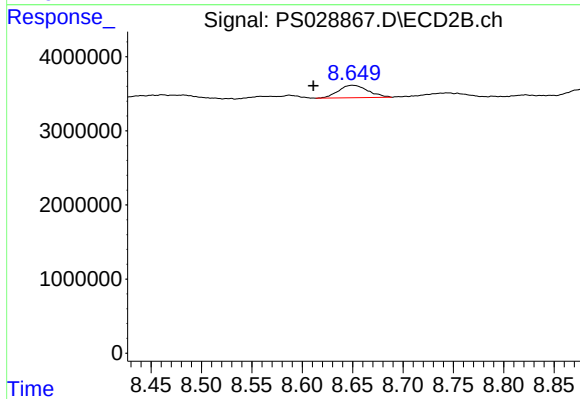

#8 DICHLORPROP

R.T.: 8.650 min
Delta R.T.: 0.039 min
Response: 3431486
Conc: 2.49 ng/ml