

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010320\
 Data File : PS008304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2020 18:27
 Operator : DD\AJ
 Sample : L1009-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 NB-08-010220

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 22:36:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 27 02:43:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.378	5.128	983.4E6	464.7E6	486.728	518.967
Target Compounds							
1) T	Dalapon	1.960	1.675	51350838	32630716	21.391	31.987 #
2) T	3,5-DICHL...	0.000	4.424	0	5562825	N.D.	4.777
3) T	4-Nitroph...	5.274	4.809	23778193	6499991	34.794	13.122 #
5) T	DICAMBA	5.467	0.000	40560370	0	5.578	N.D. #
9) T	2,4-D	0.000	6.020	0	5969146	N.D.	5.879
10) T	Pentachlo...	0.000	6.404	0	7380701	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.707	0	111.2E6	N.D.	22.257
12) T	2,4,5-T	7.435	0.000	30110288	0	2.506	N.D. #
15) T	Picloram	8.814	0.000	74134877	0	141.738	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010320\
Data File : PS008304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2020 18:27
Operator : DD\AJ
Sample : L1009-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
NB-08-010220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 22:36:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
Quant Title : 8080.M
QLast Update : Fri Dec 27 02:43:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

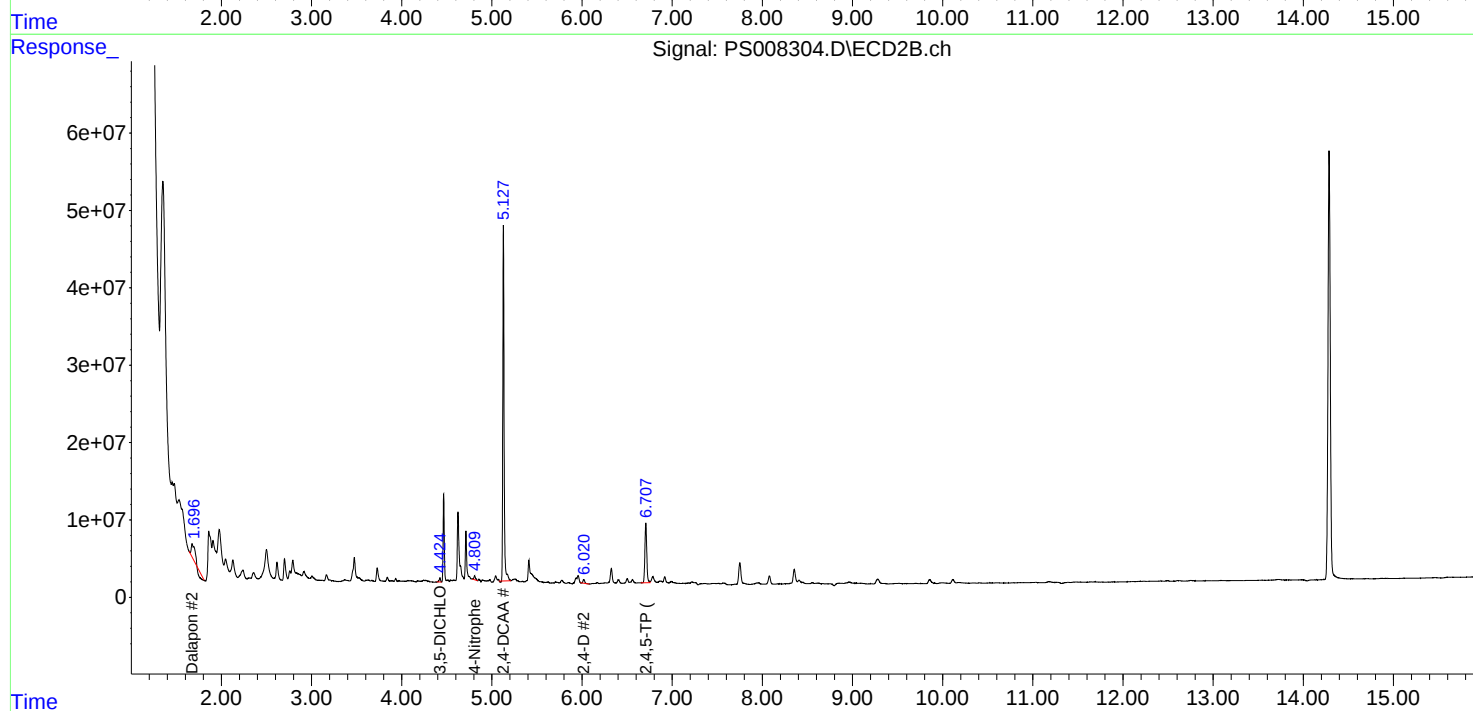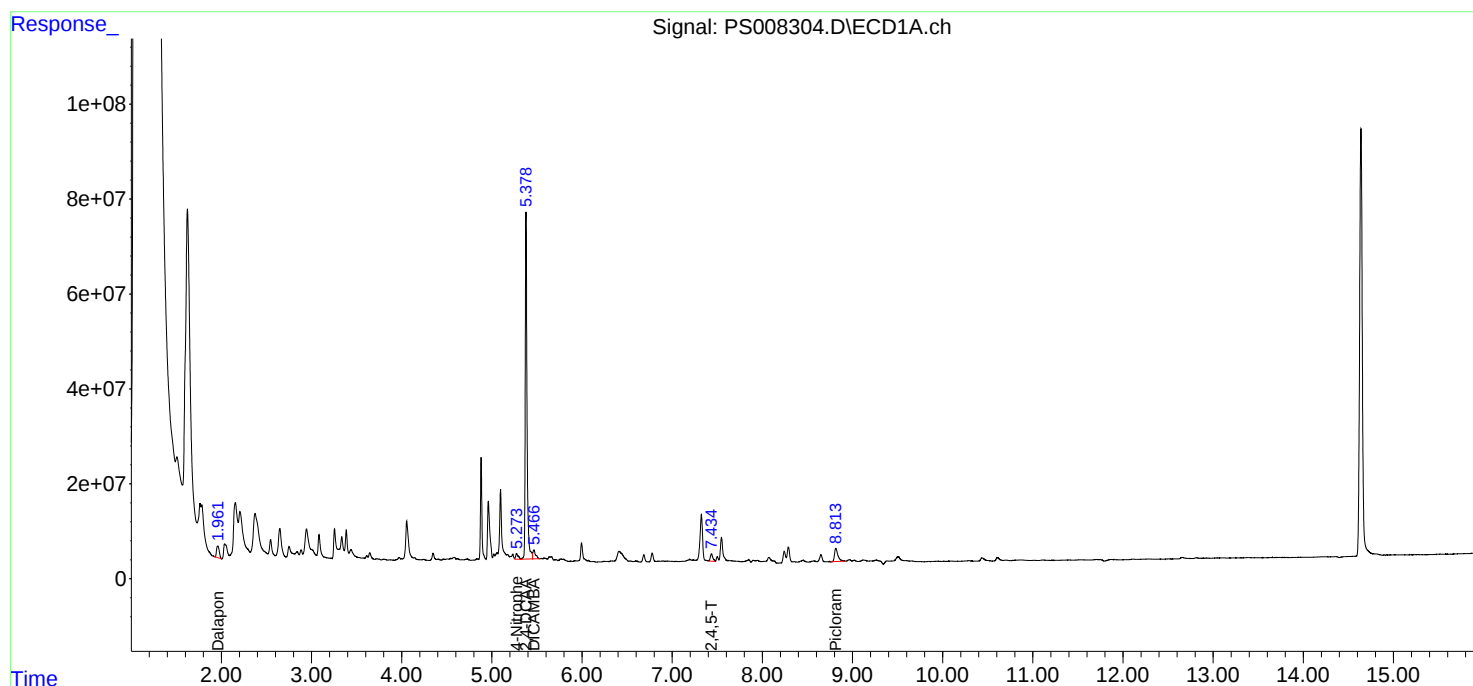


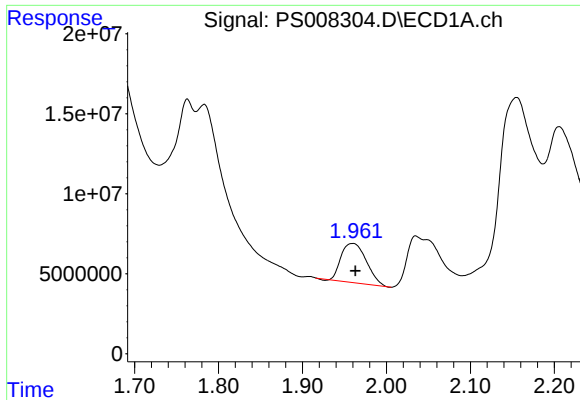

#1 Dalapon


R.T.: 1.960 min
Delta R.T.: -0.003 min
Response: 51350838
Conc: 21.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-08-010220

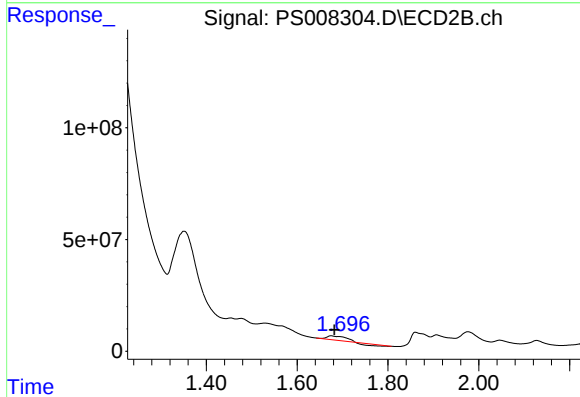


#1 Dalapon

R.T.: 1.675 min
Delta R.T.: -0.007 min
Response: 32630716
Conc: 31.99 ng/ml

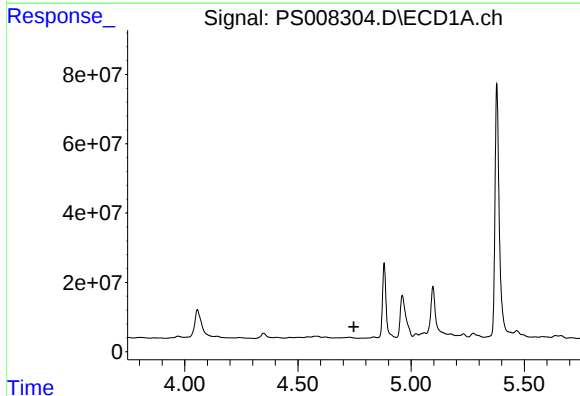


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.747 min
Response: 0
Conc: N.D.

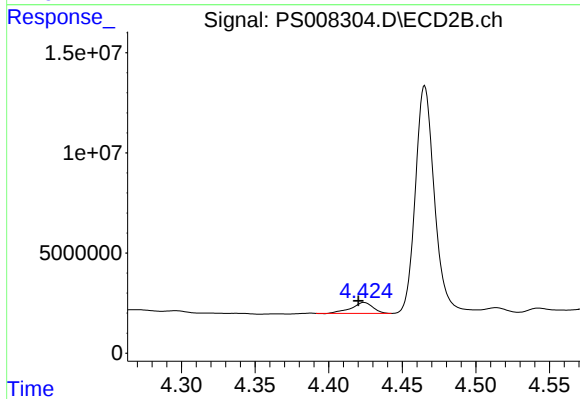

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.424 min
Delta R.T.: 0.004 min
Response: 5562825
Conc: 4.78 ng/ml

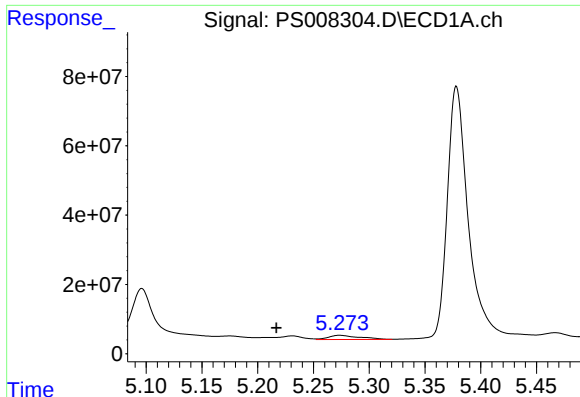

#3 4-Nitrophenol


R.T.: 5.274 min
Delta R.T.: 0.057 min
Response: 23778193
Conc: 34.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-08-010220

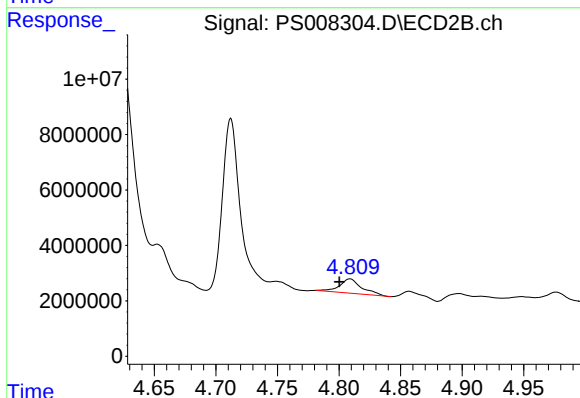


#3 4-Nitrophenol

R.T.: 4.809 min
Delta R.T.: 0.009 min
Response: 6499991
Conc: 13.12 ng/ml

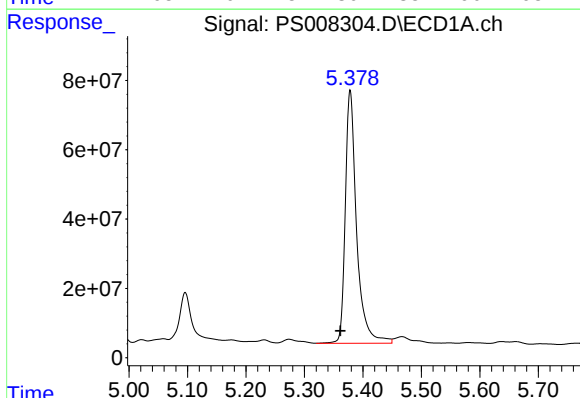


#4 2,4-DCAA

R.T.: 5.378 min
Delta R.T.: 0.017 min
Response: 983356761
Conc: 486.73 ng/ml

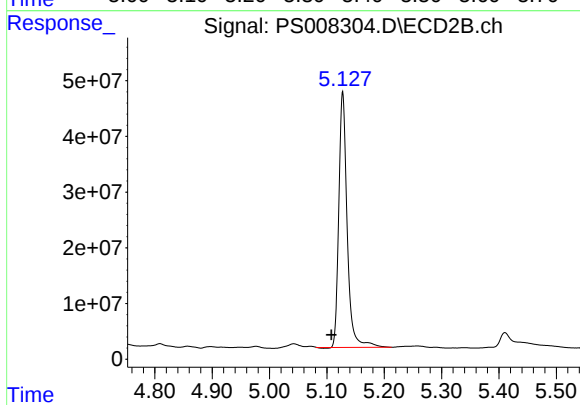

#4 2,4-DCAA


R.T.: 5.128 min
Delta R.T.: 0.020 min
Response: 464674044
Conc: 518.97 ng/ml

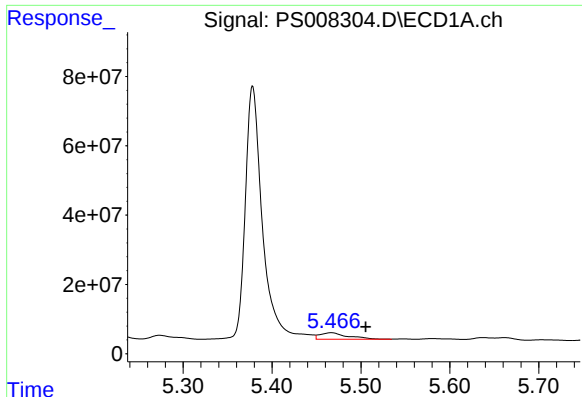

#5 DICAMBA


R.T.: 5.467 min
Delta R.T.: -0.039 min
Response: 40560370
Conc: 5.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-08-010220

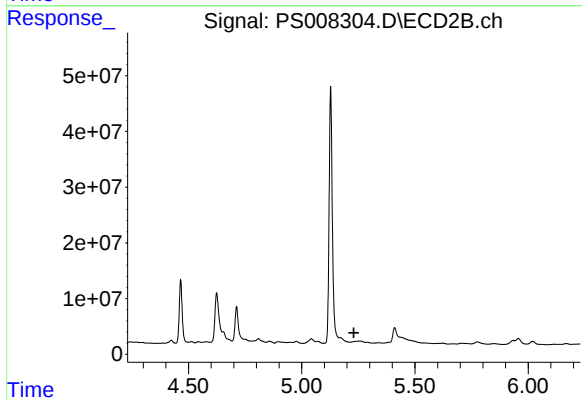


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.230 min
Response: 0
Conc: N.D.

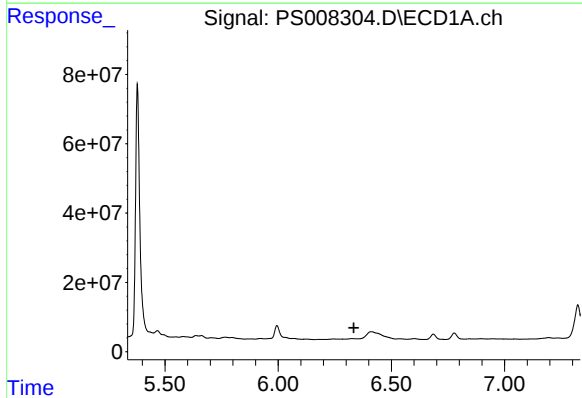


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.334 min
Response: 0
Conc: N.D.

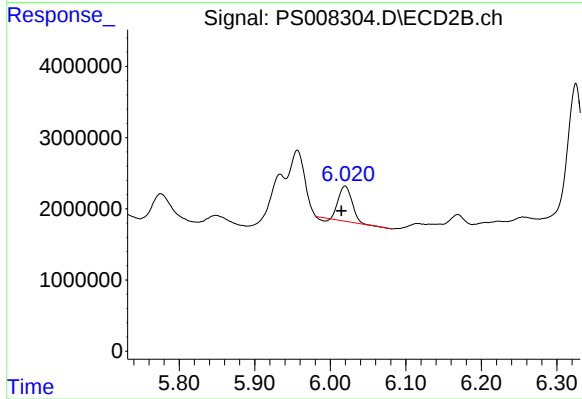

#9 2,4-D


R.T.: 6.020 min
Delta R.T.: 0.005 min
Response: 5969146
Conc: 5.88 ng/ml

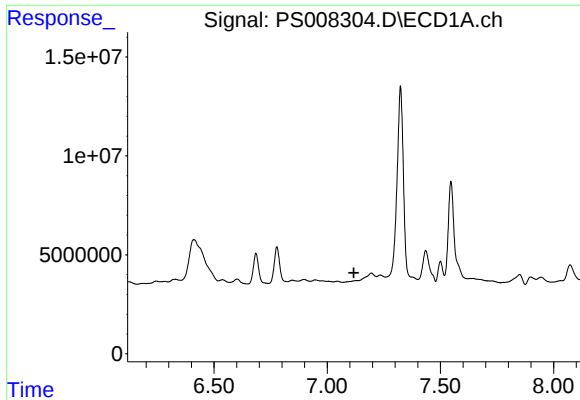

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
NB-08-010220

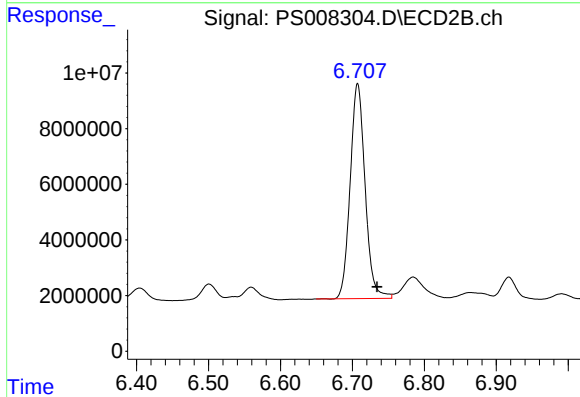


#11 2,4,5-TP (SILVEX)

R.T.: 6.707 min
Delta R.T.: -0.027 min
Response: 111220531
Conc: 22.26 ng/ml

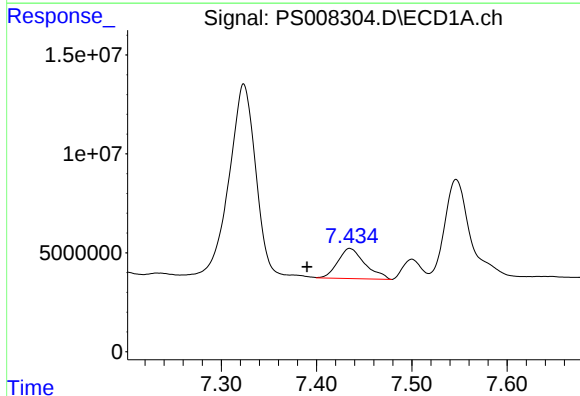


#12 2,4,5-T

R.T.: 7.435 min
Delta R.T.: 0.045 min
Response: 30110288
Conc: 2.51 ng/ml

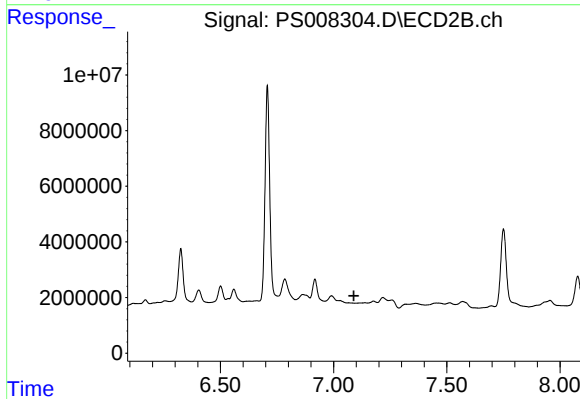

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

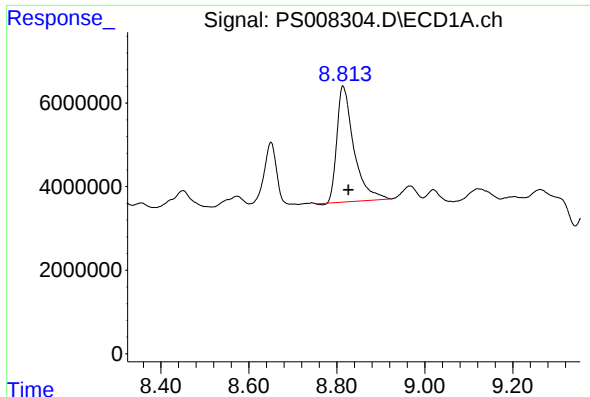

#15 Picloram

R.T.: 8.814 min
Delta R.T.: -0.012 min
Response: 74134877
Conc: 141.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-08-010220

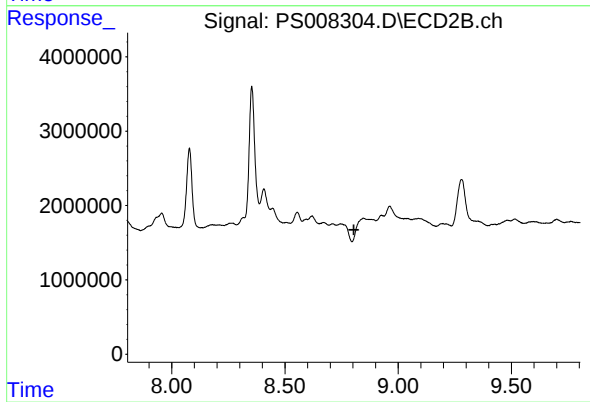

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.805 min
Response: 0
Conc: N.D.