

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010320\
 Data File : PS008305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2020 18:49
 Operator : DD\AJ
 Sample : L1010-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-01-010220

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 22:36:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
 Quant Title : 8080.M
 QLast Update : Fri Dec 27 02:43:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.376	5.111	892.3E6	428.6E6	441.674	478.731
Target Compounds							
1) T	Dalapon	1.959	1.658	62917528	32908901	26.209	32.260
2) T	3,5-DICHL...	0.000	4.448	0	111.1E6	N.D.	95.380
3) T	4-Nitroph...	5.271	4.841	59146857	12687237	86.549	25.612 #
5) T	DICAMBA	5.465	5.241	45575354	12615466	6.268	3.703 #
9) T	2,4-D	0.000	6.001	0	8445586	N.D.	8.318
10) T	Pentachlo...	0.000	6.386	0	7617389	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.767	0	16364326	N.D.	3.275
12) T	2,4,5-T	7.434	0.000	30014087	0	2.498	N.D. #
14) T	DINOSEB	0.000	7.911	0	70018456	N.D.	18.696
15) T	Picloram	8.817	0.000	99751626	0	143.465	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010320\
Data File : PS008305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2020 18:49
Operator : DD\AJ
Sample : L1010-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OK-01-010220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 22:36:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122619.M
Quant Title : 8080.M
QLast Update : Fri Dec 27 02:43:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

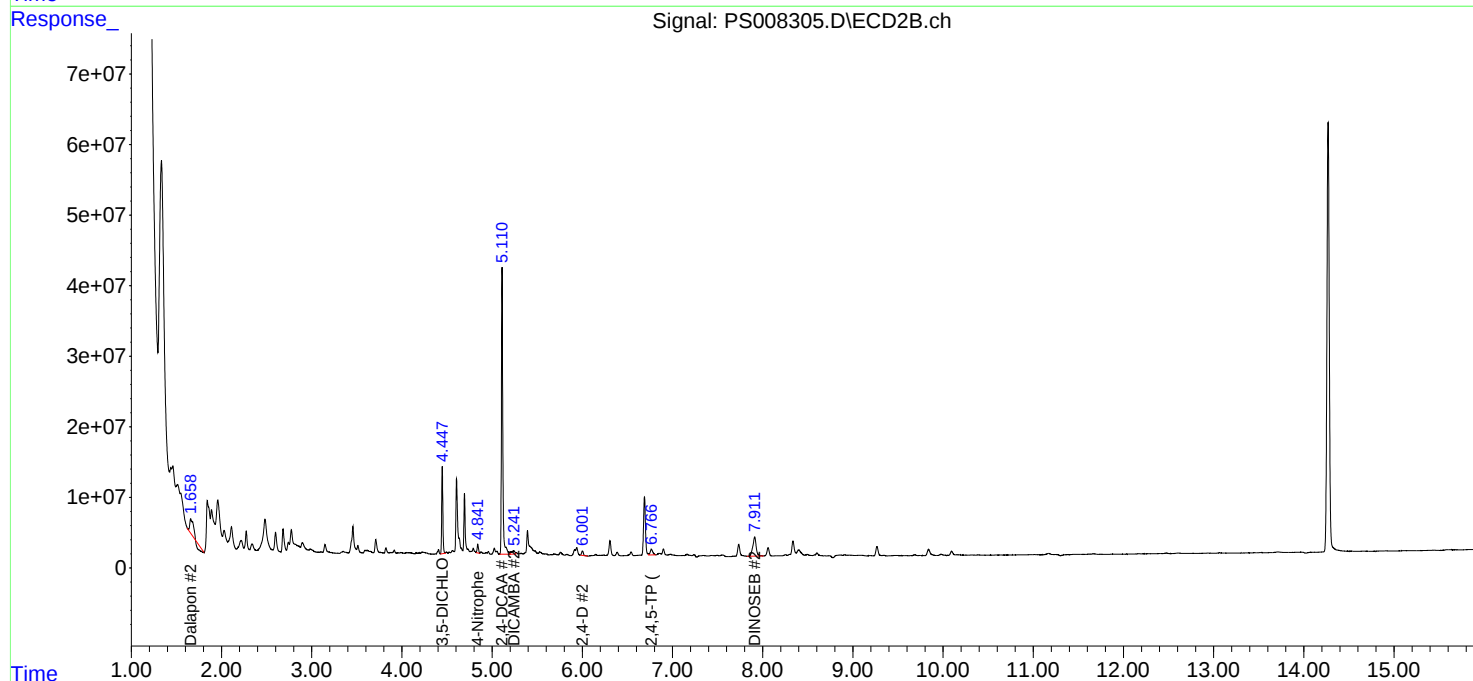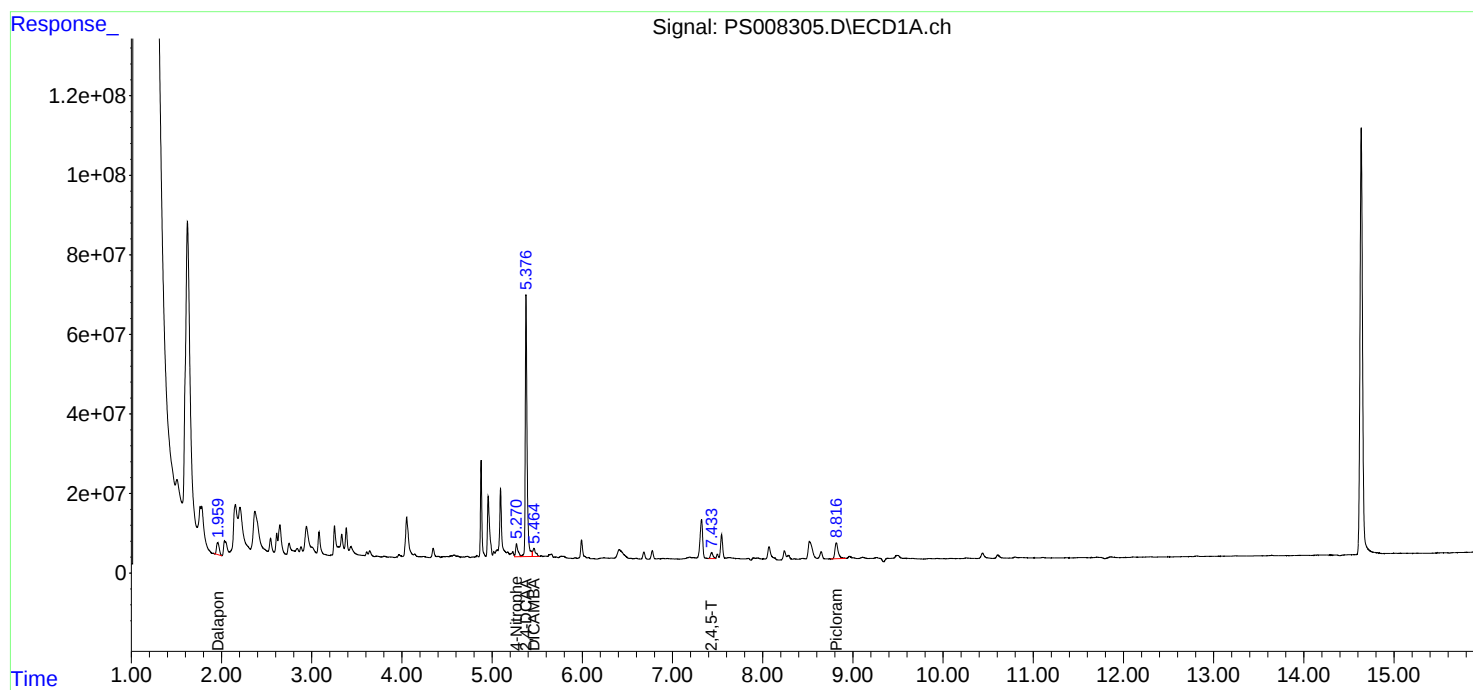


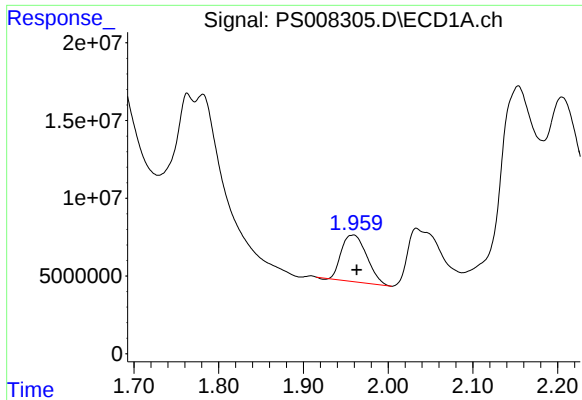

#1 Dalapon


R.T.: 1.959 min
Delta R.T.: -0.004 min
Response: 62917528
Conc: 26.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-01-010220

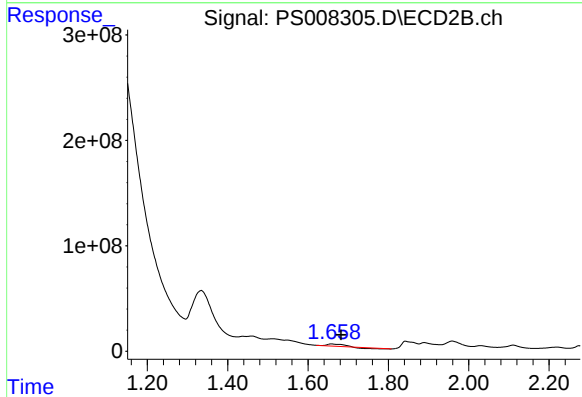


#1 Dalapon

R.T.: 1.658 min
Delta R.T.: -0.024 min
Response: 32908901
Conc: 32.26 ng/ml

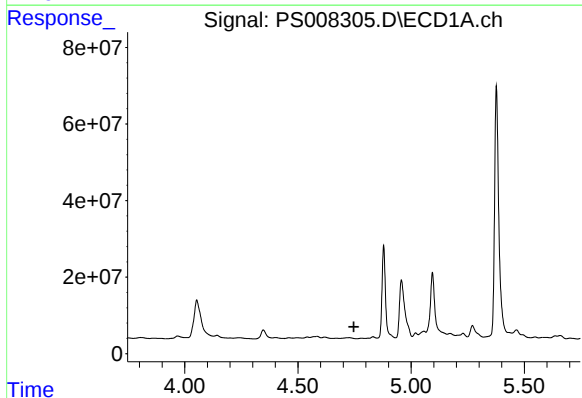


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.747 min
Response: 0
Conc: N.D.

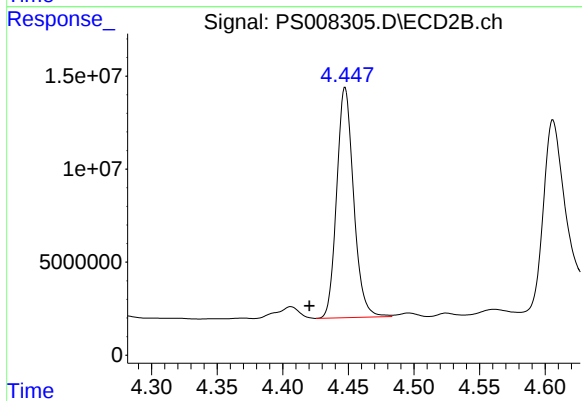

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.448 min
Delta R.T.: 0.027 min
Response: 111061616
Conc: 95.38 ng/ml

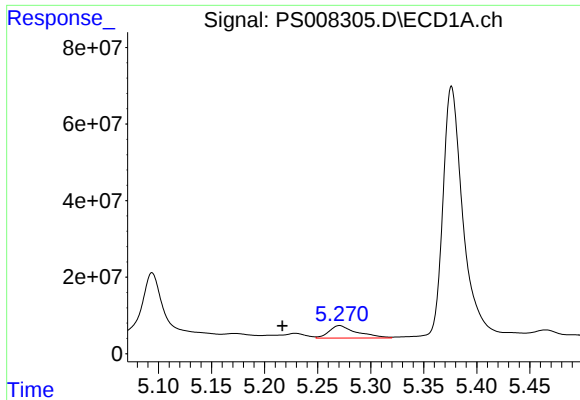

#3 4-Nitrophenol


R.T.: 5.271 min
Delta R.T.: 0.054 min
Response: 59146857
Conc: 86.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-01-010220

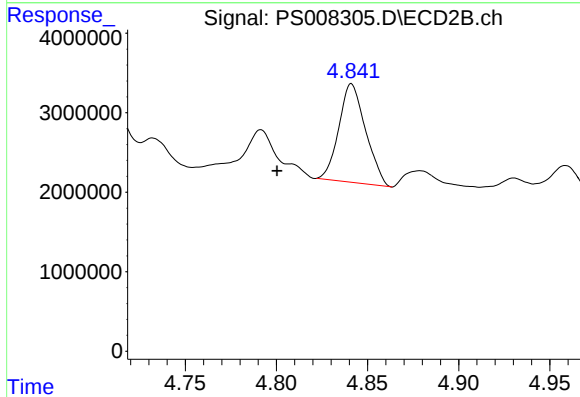


#3 4-Nitrophenol

R.T.: 4.841 min
Delta R.T.: 0.041 min
Response: 12687237
Conc: 25.61 ng/ml

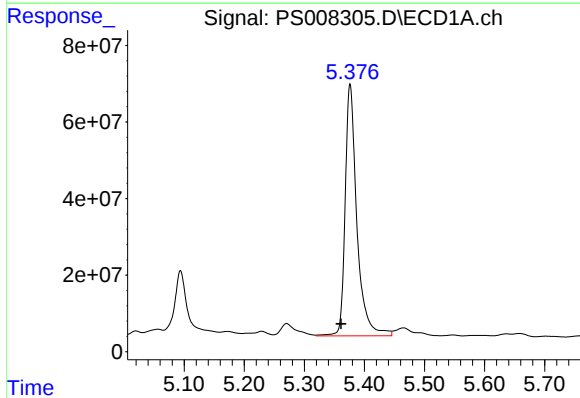


#4 2,4-DCAA

R.T.: 5.376 min
Delta R.T.: 0.015 min
Response: 892333225
Conc: 441.67 ng/ml

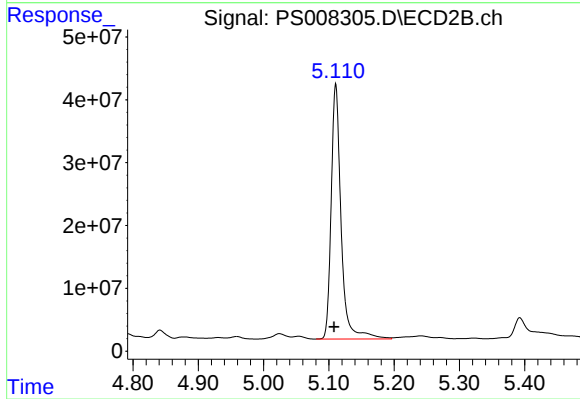

#4 2,4-DCAA


R.T.: 5.111 min
Delta R.T.: 0.002 min
Response: 428647192
Conc: 478.73 ng/ml

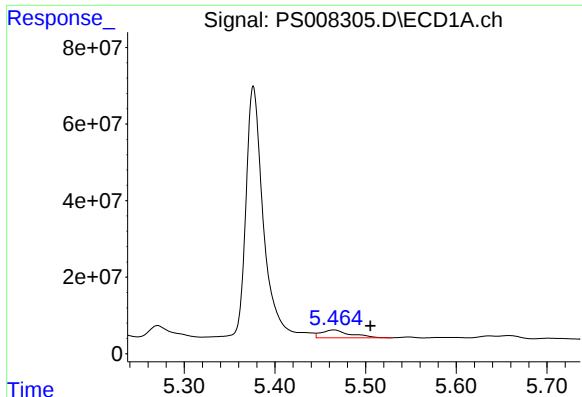

#5 DICAMBA


R.T.: 5.465 min
Delta R.T.: -0.041 min
Response: 45575354
Conc: 6.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-01-010220

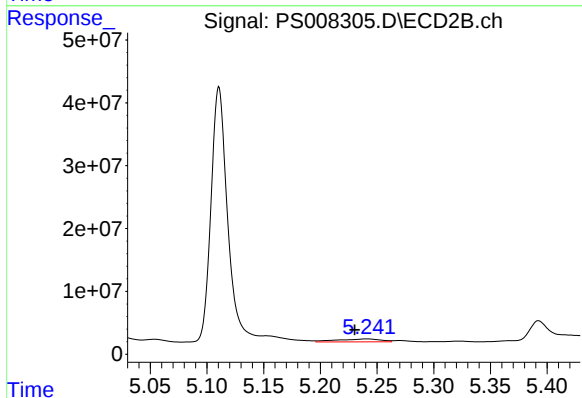


#5 DICAMBA

R.T.: 5.241 min
Delta R.T.: 0.011 min
Response: 12615466
Conc: 3.70 ng/ml

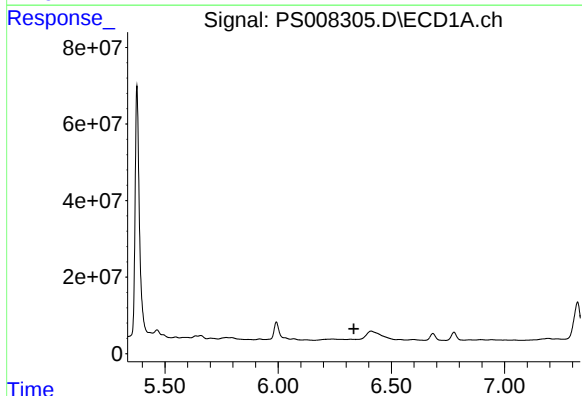


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.334 min
Response: 0
Conc: N.D.

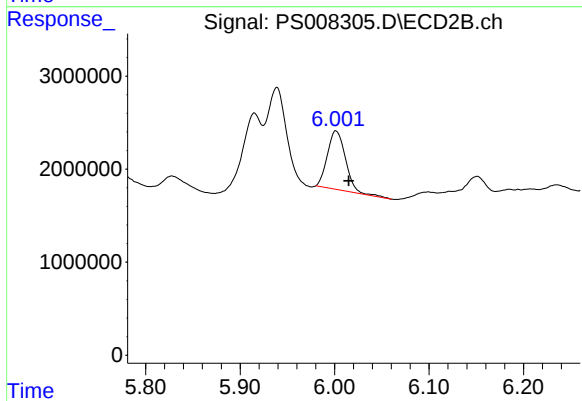

#9 2,4-D


R.T.: 6.001 min
Delta R.T.: -0.013 min
Response: 8445586
Conc: 8.32 ng/ml

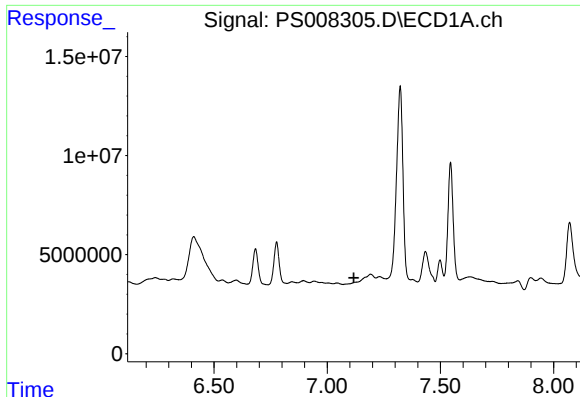

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-01-010220

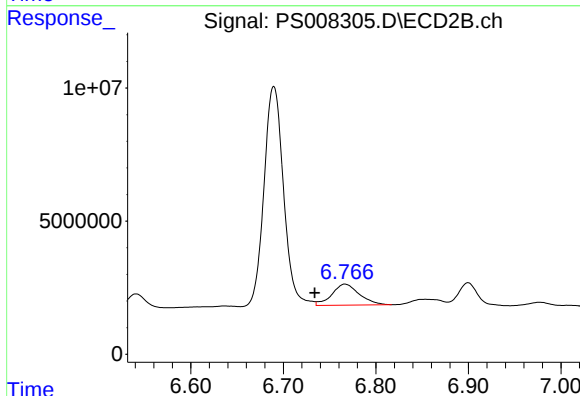


#11 2,4,5-TP (SILVEX)

R.T.: 6.767 min
Delta R.T.: 0.033 min
Response: 16364326
Conc: 3.27 ng/ml

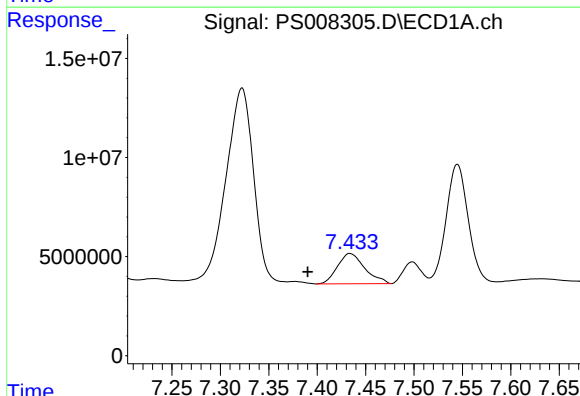


#12 2,4,5-T

R.T.: 7.434 min
Delta R.T.: 0.044 min
Response: 30014087
Conc: 2.50 ng/ml

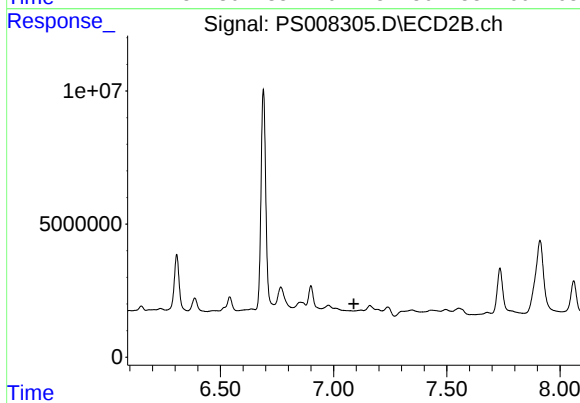

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

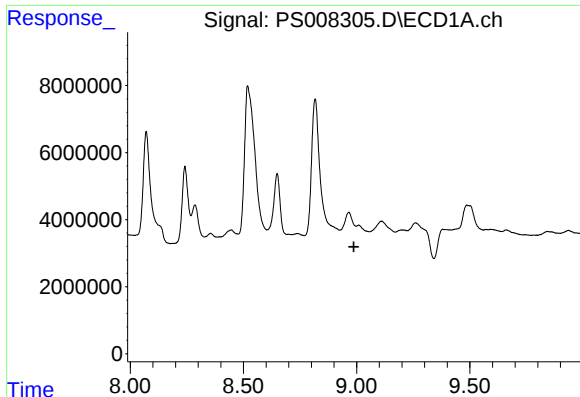

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 8.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-01-010220

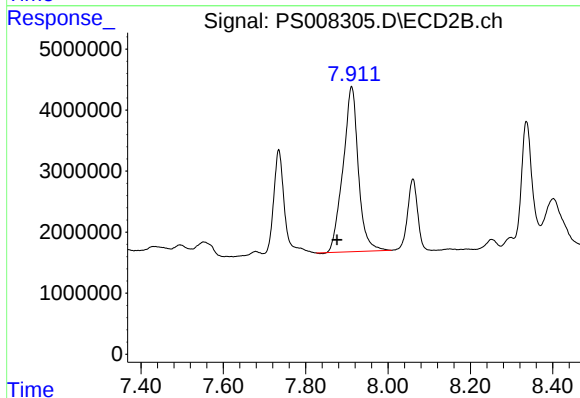


#14 DINOSEB

R.T.: 7.911 min
Delta R.T.: 0.036 min
Response: 70018456
Conc: 18.70 ng/ml

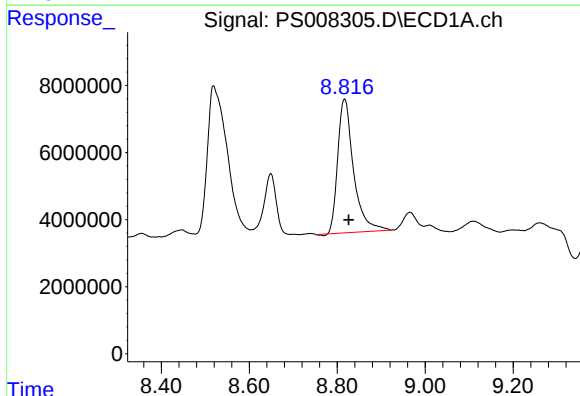

#15 Picloram

R.T.: 8.817 min
Delta R.T.: -0.009 min
Response: 99751626
Conc: 143.46 ng/ml

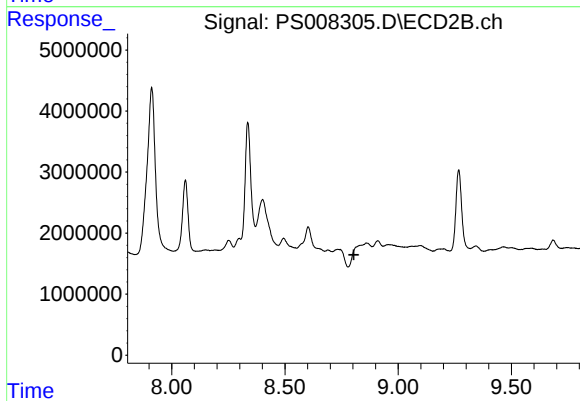

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.805 min
Response: 0
Conc: N.D.