

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010322\
 Data File : PS017895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2022 18:45
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 00:00:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 14 13:29:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.124	6.713	1205.2E6	476.3E6	771.094	799.036
Target Compounds							
1) T	Dalapon	2.976	2.483	1881.4E6	594.6E6	734.166	768.079
2) T	3,5-DICHL...	6.353	5.917	1622.9E6	701.2E6	726.413	773.353
3) T	4-Nitroph...	6.960	6.349	413.3E6	249.3E6	611.206	715.963
5) T	DICAMBA	7.311	6.869	4879.2E6	2105.0E6	771.606	790.175
6) T	MCPD	7.481	6.965	351.5E6	171.7E6	74.558	78.901
7) T	MCPA	7.628	7.176	498.0E6	234.7E6	75.300	76.748
8) T	DICHLORPROP	8.000	7.486	1190.8E6	526.0E6	762.099	771.813
9) T	2,4-D	8.232	7.782	1282.4E6	630.4E6	725.403	775.346
10) T	Pentachlo...	8.531	8.194	16732.8E6	6749.5E6	775.481	787.781
11) T	2,4,5-TP ...	9.081	8.558	6590.4E6	2920.7E6	774.710	803.421
12) T	2,4,5-T	9.366	8.935	6592.9E6	2626.4E6	757.864	768.041
13) T	2,4-DB	9.916	9.439	983.9E6	339.8E6	666.256	749.925
14) T	DINOSEB	11.060	9.758	5169.7E6	1986.9E6	756.035	769.066
15) T	Picloram	10.889	10.746	7158.3E6	3400.1E6	659.682	692.283
16) T	DCPA	11.328	10.684	8392.3E6	3597.2E6	772.737	803.134



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS017895.D
Data File : PS017895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2022 18:45
Operator : AJ\MA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 00:00:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121421.M
Quant Title : 8080.M
QLast Update : Tue Dec 14 13:29:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

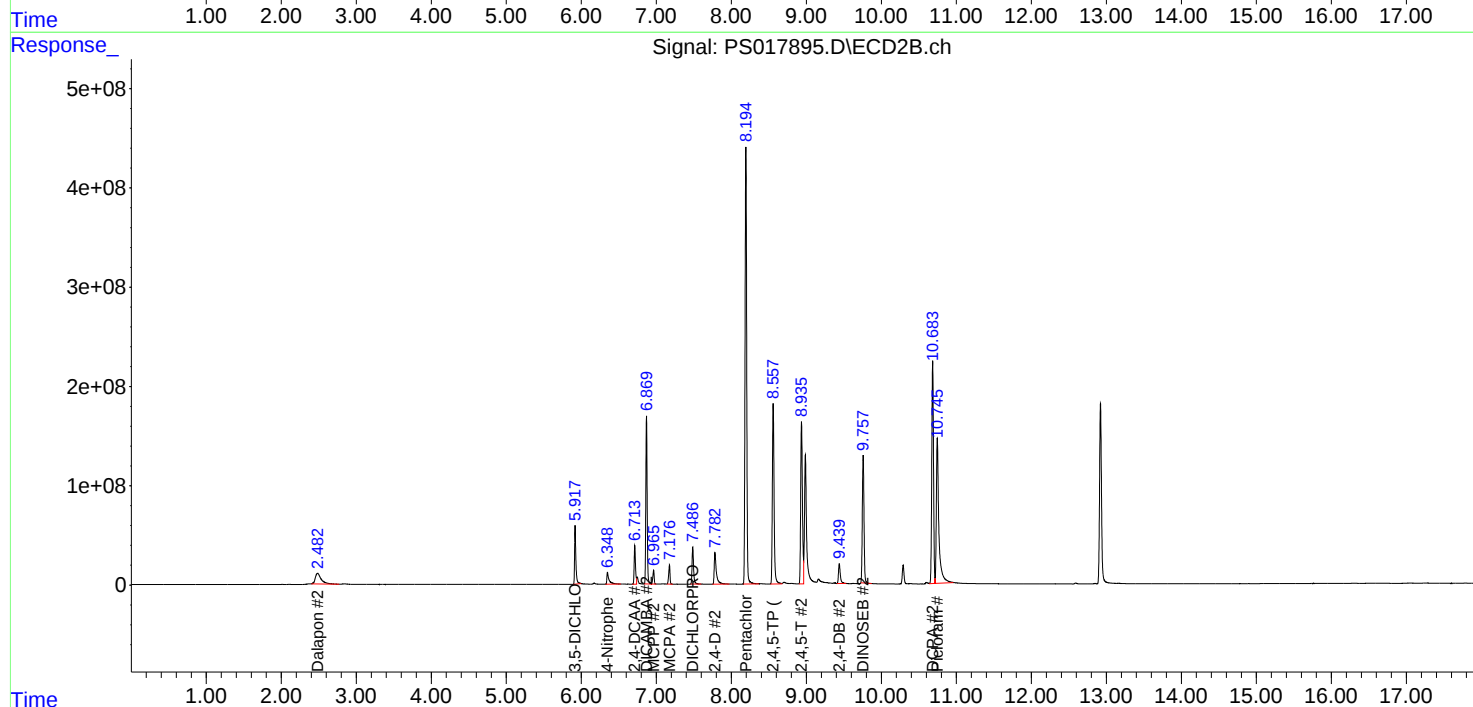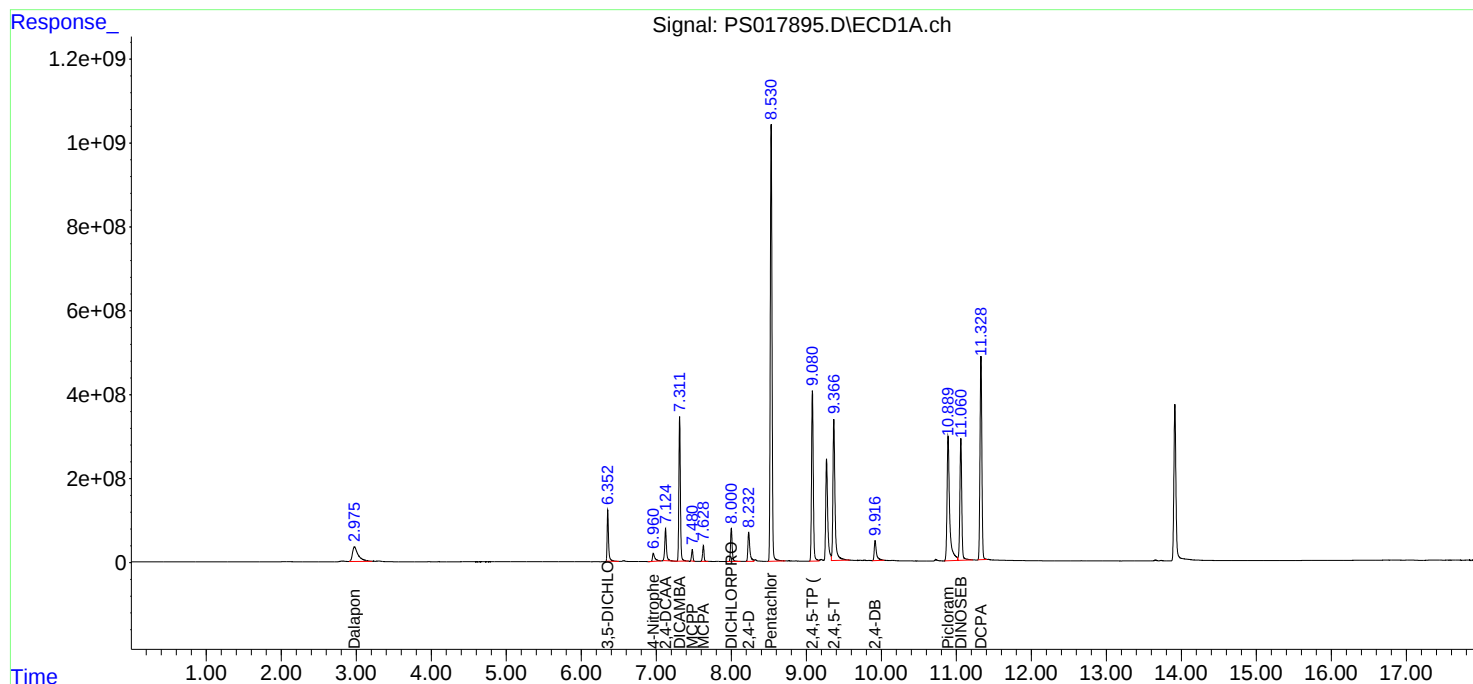


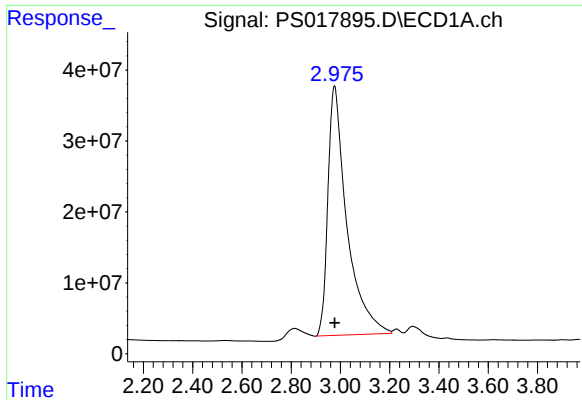

#1 Dalapon


R.T.: 2.976 min
Delta R.T.: -0.001 min
Response: 1881376004
Conc: 734.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

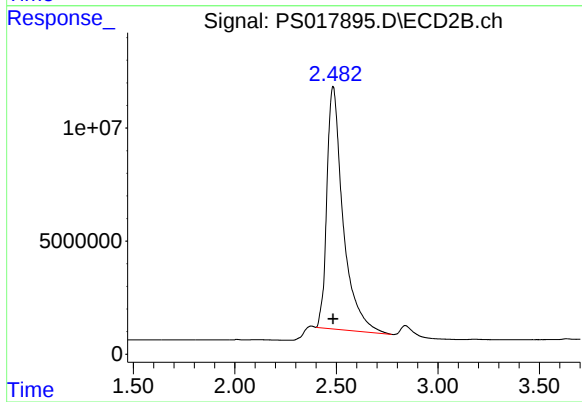


#1 Dalapon

R.T.: 2.483 min
Delta R.T.: 0.000 min
Response: 594568360
Conc: 768.08 ng/ml

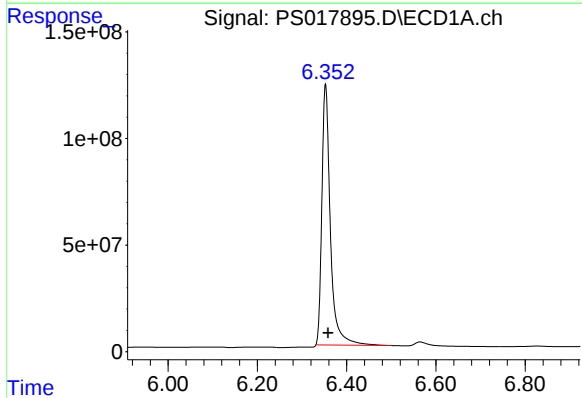


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.353 min
Delta R.T.: -0.005 min
Response: 1622908559
Conc: 726.41 ng/ml

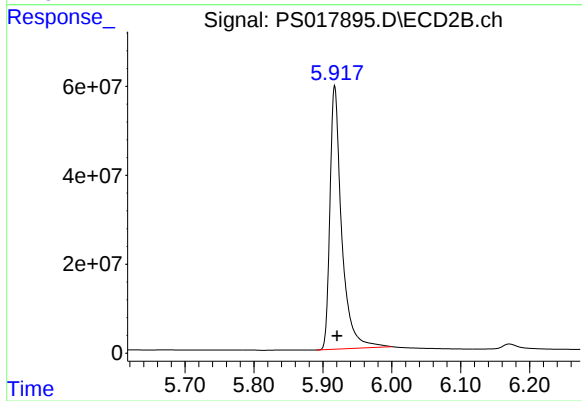

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.917 min
Delta R.T.: -0.003 min
Response: 701166033
Conc: 773.35 ng/ml

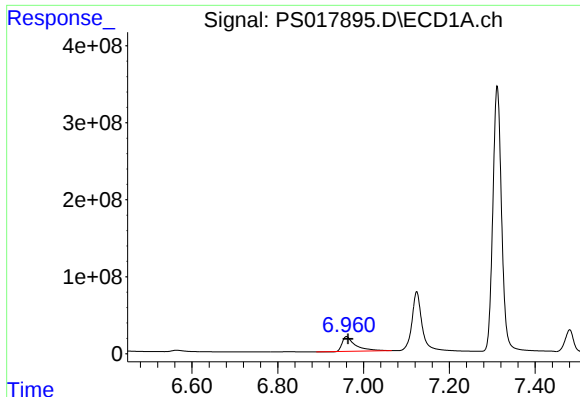

#3 4-Nitrophenol


R.T.: 6.960 min
Delta R.T.: -0.004 min
Response: 413311310
Conc: 611.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

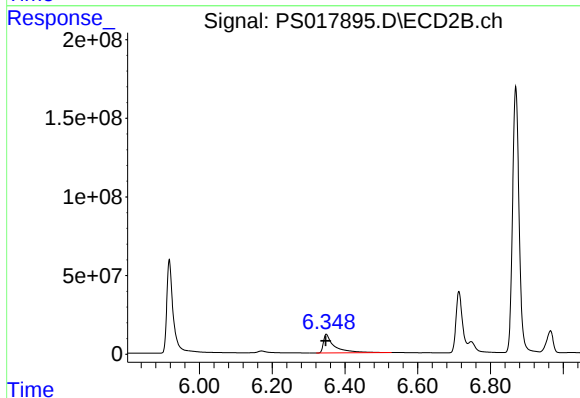


#3 4-Nitrophenol

R.T.: 6.349 min
Delta R.T.: 0.001 min
Response: 249328782
Conc: 715.96 ng/ml

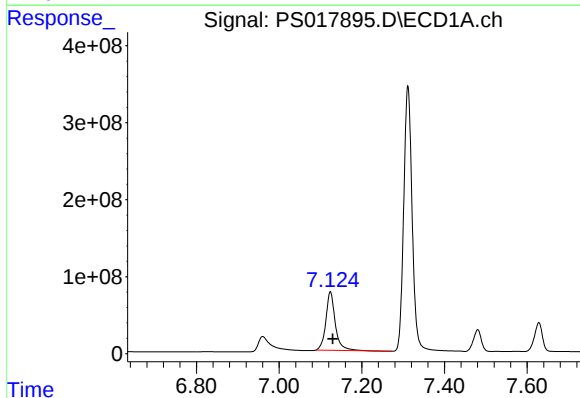


#4 2,4-DCAA

R.T.: 7.124 min
Delta R.T.: -0.006 min
Response: 1205178526
Conc: 771.09 ng/ml

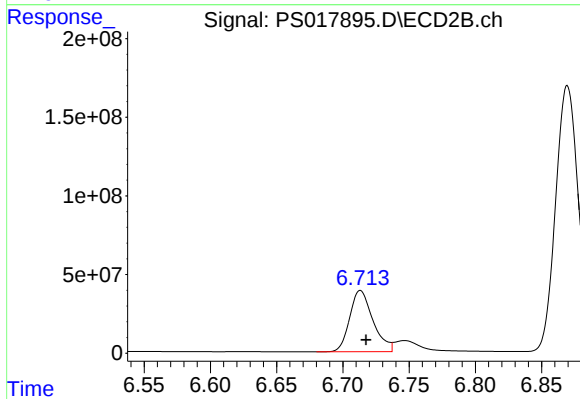

#4 2,4-DCAA


R.T.: 6.713 min
Delta R.T.: -0.004 min
Response: 476306591
Conc: 799.04 ng/ml

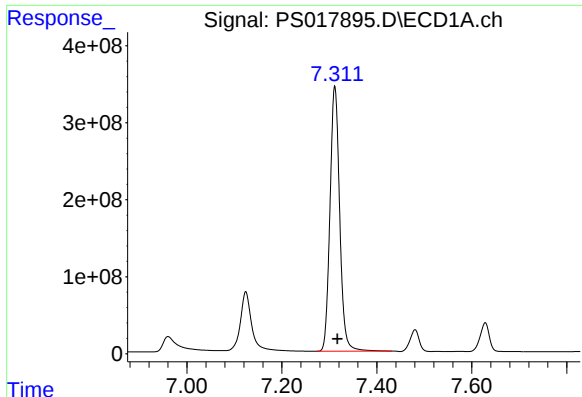

#5 DICAMBA


R.T.: 7.311 min
Delta R.T.: -0.006 min
Response: 4879198054
Conc: 771.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

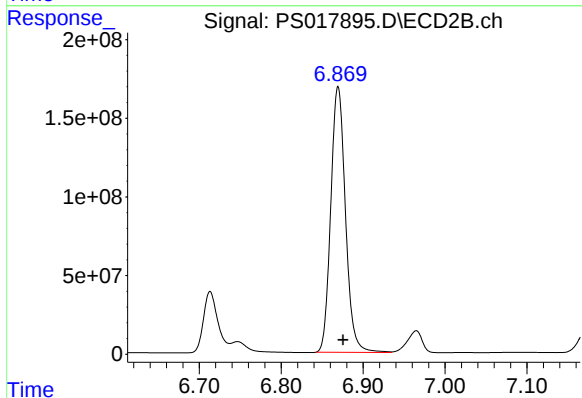


#5 DICAMBA

R.T.: 6.869 min
Delta R.T.: -0.006 min
Response: 2104986397
Conc: 790.17 ng/ml

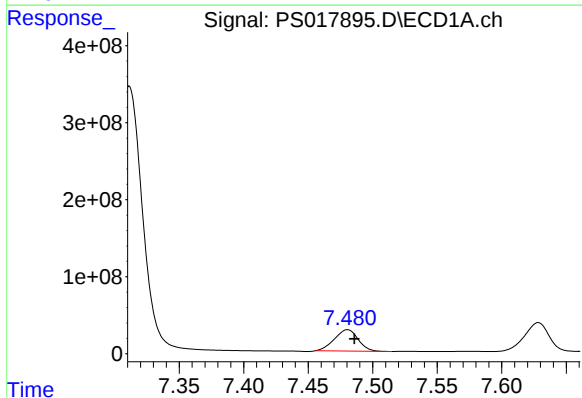


#6 MCP

R.T.: 7.481 min
Delta R.T.: -0.005 min
Response: 351464877
Conc: 74.56 ug/ml

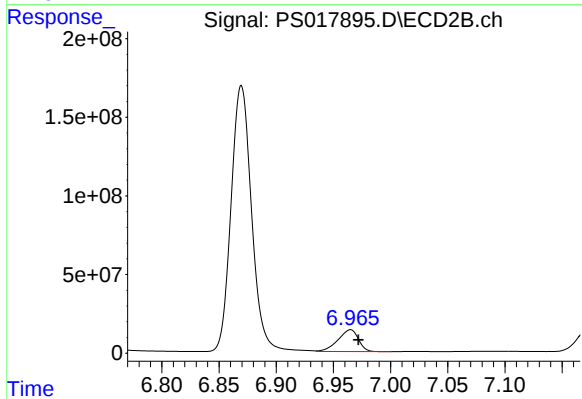

#6 MCP


R.T.: 6.965 min
Delta R.T.: -0.007 min
Response: 171735648
Conc: 78.90 ug/ml

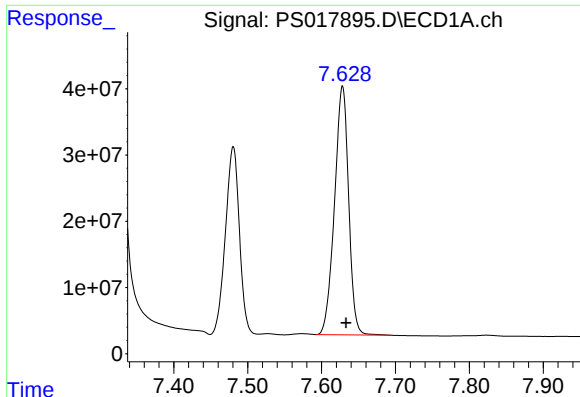

#7 MCPA


R.T.: 7.628 min
Delta R.T.: -0.005 min
Response: 498015522
Conc: 75.30 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

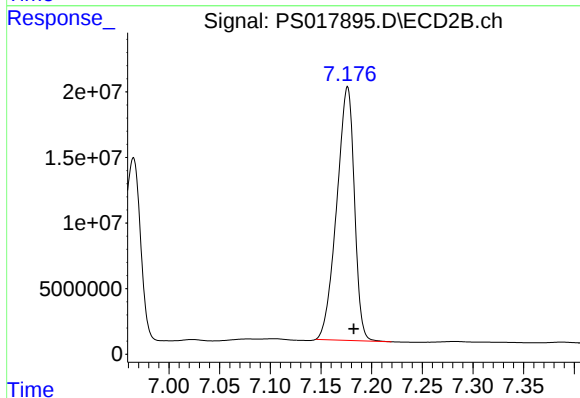


#7 MCPA

R.T.: 7.176 min
Delta R.T.: -0.006 min
Response: 234682272
Conc: 76.75 ug/ml

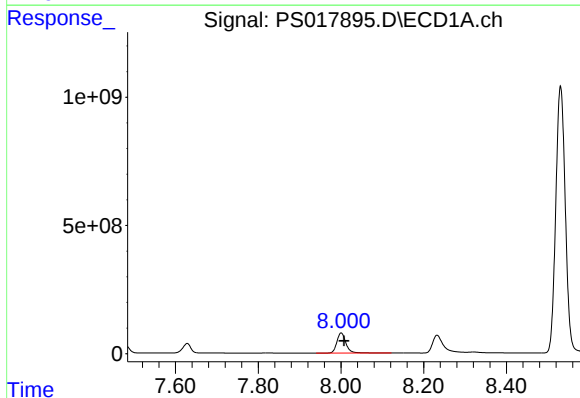


#8 DICHLORPROP

R.T.: 8.000 min
Delta R.T.: -0.007 min
Response: 1190784411
Conc: 762.10 ng/ml

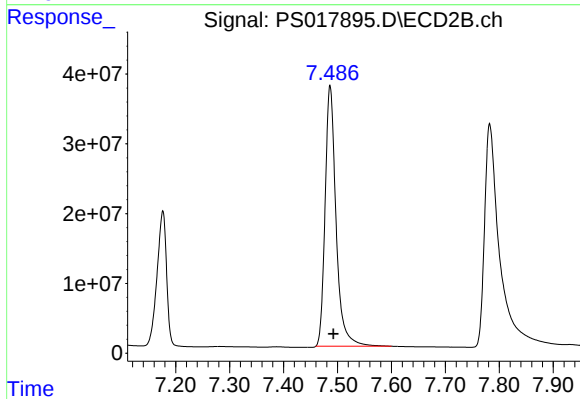

#8 DICHLORPROP


R.T.: 7.486 min
Delta R.T.: -0.006 min
Response: 526005586
Conc: 771.81 ng/ml

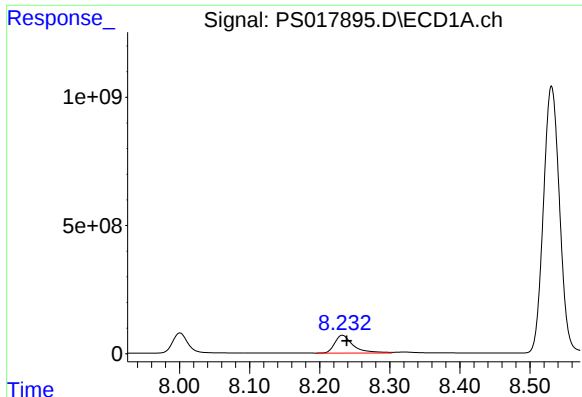

#9 2,4-D


R.T.: 8.232 min
Delta R.T.: -0.006 min
Response: 1282423292
Conc: 725.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

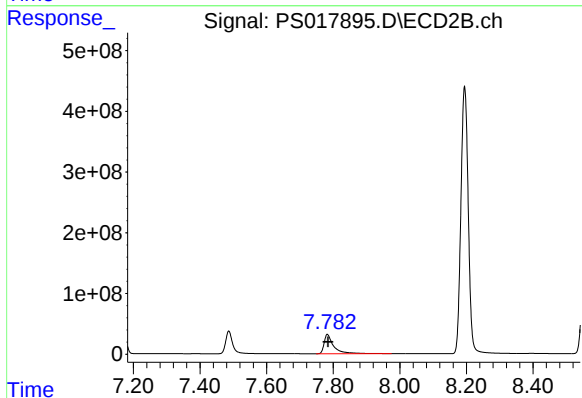


#9 2,4-D

R.T.: 7.782 min
Delta R.T.: -0.002 min
Response: 630390566
Conc: 775.35 ng/ml

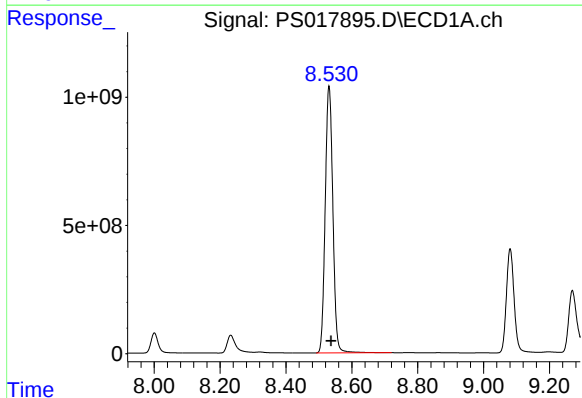


#10 Pentachlorophenol

R.T.: 8.531 min
Delta R.T.: -0.007 min
Response: 16732807740
Conc: 775.48 ng/ml

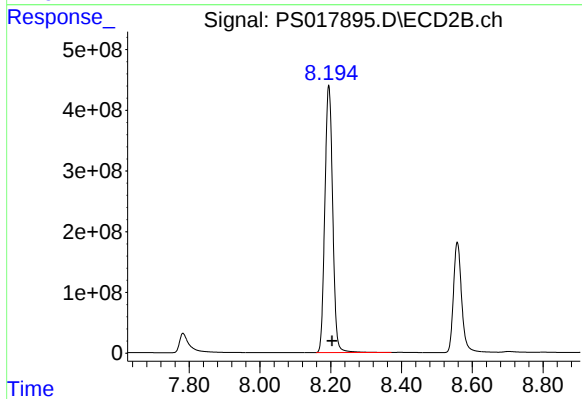

#10 Pentachlorophenol


R.T.: 8.194 min
Delta R.T.: -0.009 min
Response: 6749533823
Conc: 787.78 ng/ml

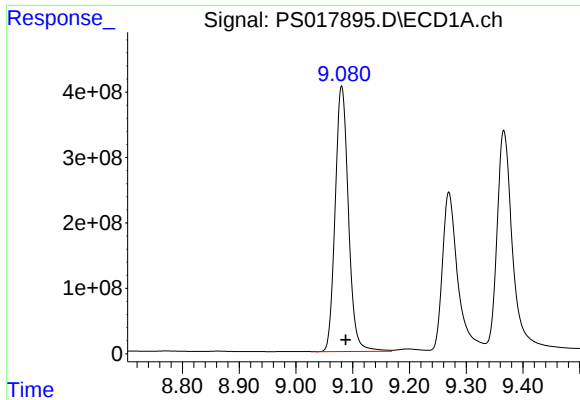

#11 2,4,5-TP (SILVEX)


R.T.: 9.081 min
Delta R.T.: -0.008 min
Response: 6590351429
Conc: 774.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

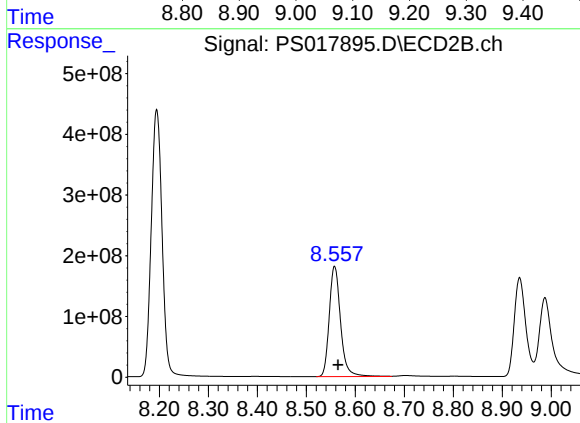


#11 2,4,5-TP (SILVEX)

R.T.: 8.558 min
Delta R.T.: -0.007 min
Response: 2920667691
Conc: 803.42 ng/ml

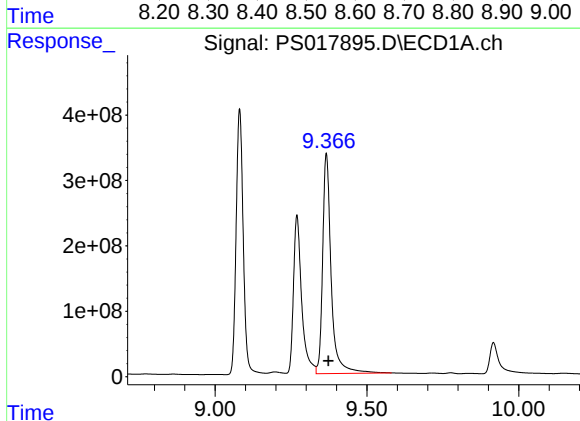


#12 2,4,5-T

R.T.: 9.366 min
Delta R.T.: -0.007 min
Response: 6592881769
Conc: 757.86 ng/ml

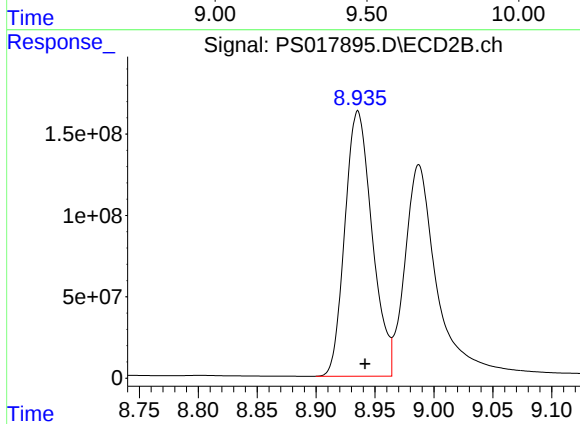

#12 2,4,5-T


R.T.: 8.935 min
Delta R.T.: -0.006 min
Response: 2626434990
Conc: 768.04 ng/ml

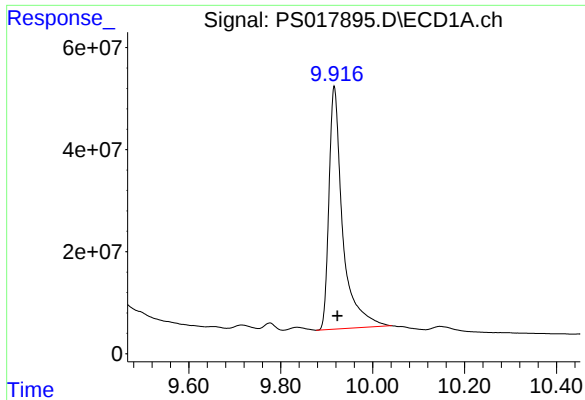

#13 2,4-DB


R.T.: 9.916 min
Delta R.T.: -0.007 min
Response: 983856560
Conc: 666.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

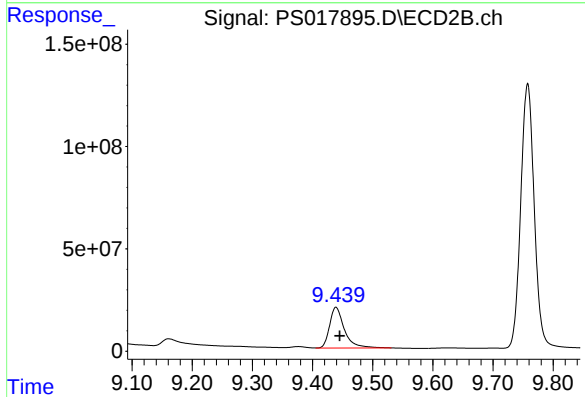


#13 2,4-DB

R.T.: 9.439 min
Delta R.T.: -0.006 min
Response: 339761532
Conc: 749.93 ng/ml

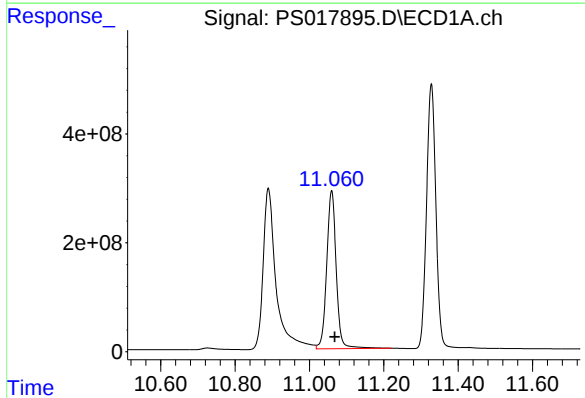


#14 DINOSEB

R.T.: 11.060 min
Delta R.T.: -0.008 min
Response: 5169674809
Conc: 756.04 ng/ml

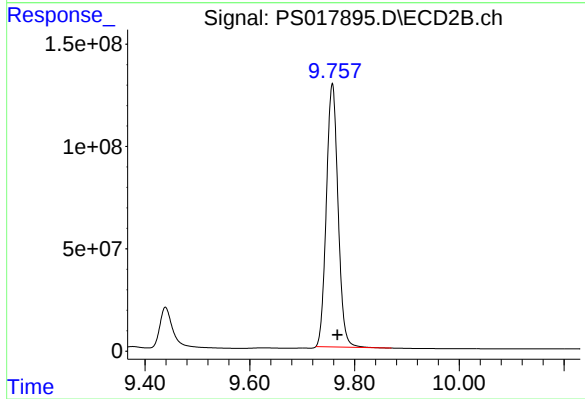

#14 DINOSEB


R.T.: 9.758 min
Delta R.T.: -0.010 min
Response: 1986919909
Conc: 769.07 ng/ml

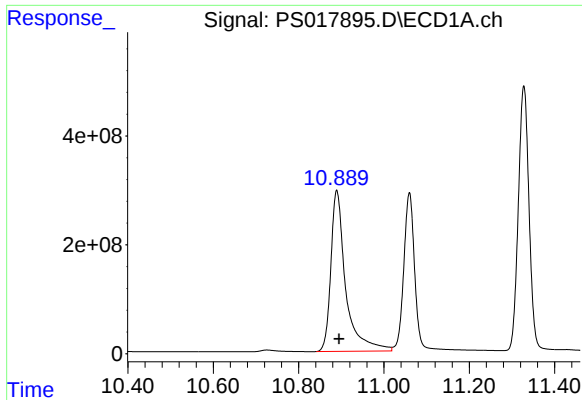

#15 Picloram


R.T.: 10.889 min
Delta R.T.: -0.006 min
Response: 7158325144
Conc: 659.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

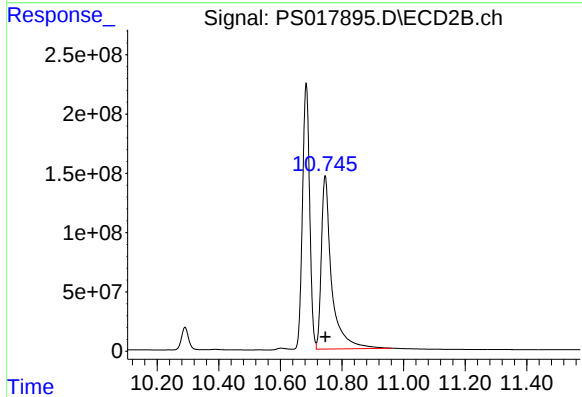


#15 Picloram

R.T.: 10.746 min
Delta R.T.: -0.001 min
Response: 3400125140
Conc: 692.28 ng/ml

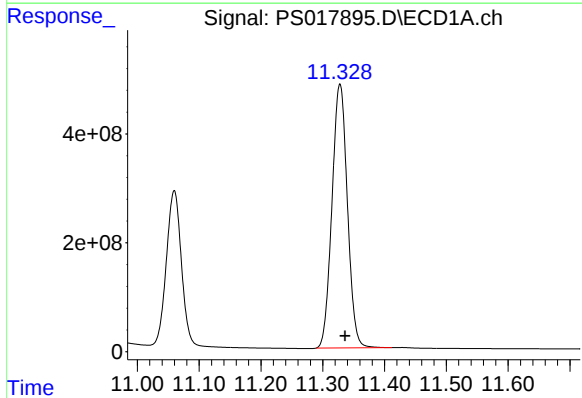

#16 DCPA

R.T.: 11.328 min
Delta R.T.: -0.008 min
Response: 8392317572
Conc: 772.74 ng/ml

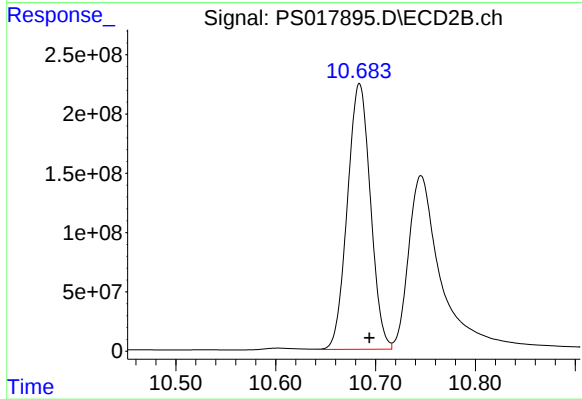

#16 DCPA

R.T.: 10.684 min
Delta R.T.: -0.010 min
Response: 3597160888
Conc: 803.13 ng/ml