

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010324\
 Data File : PS025431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2024 10:20
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 23:24:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	2.506	2.554	5233100	3524378	1.691 3.066 #
5) T	DICAMBA	0.000	6.961	0	13762744	N.D. 4.547
6) T	MCP	0.000	6.961f	0	13762744	N.D. 6.895
7) T	MCPA	0.000	7.218	0	2575201	N.D. <MDL
8) T	DICHLORPROP	0.000	7.563	0	2496231	N.D. 3.227
9) T	2,4-D	7.247	0.000	118.8E6	0	38.341 N.D. #
12) T	2,4,5-T	0.000	9.037f	0	1987697	N.D. <MDL
15) T	Picloram	9.666	10.783	11209937	7396478	<MDL 1.086 #
16) T	DCPA	0.000	10.783f	0	7396478	N.D. 1.385



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010324\
Data File : PS025431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2024 10:20
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 23:24:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

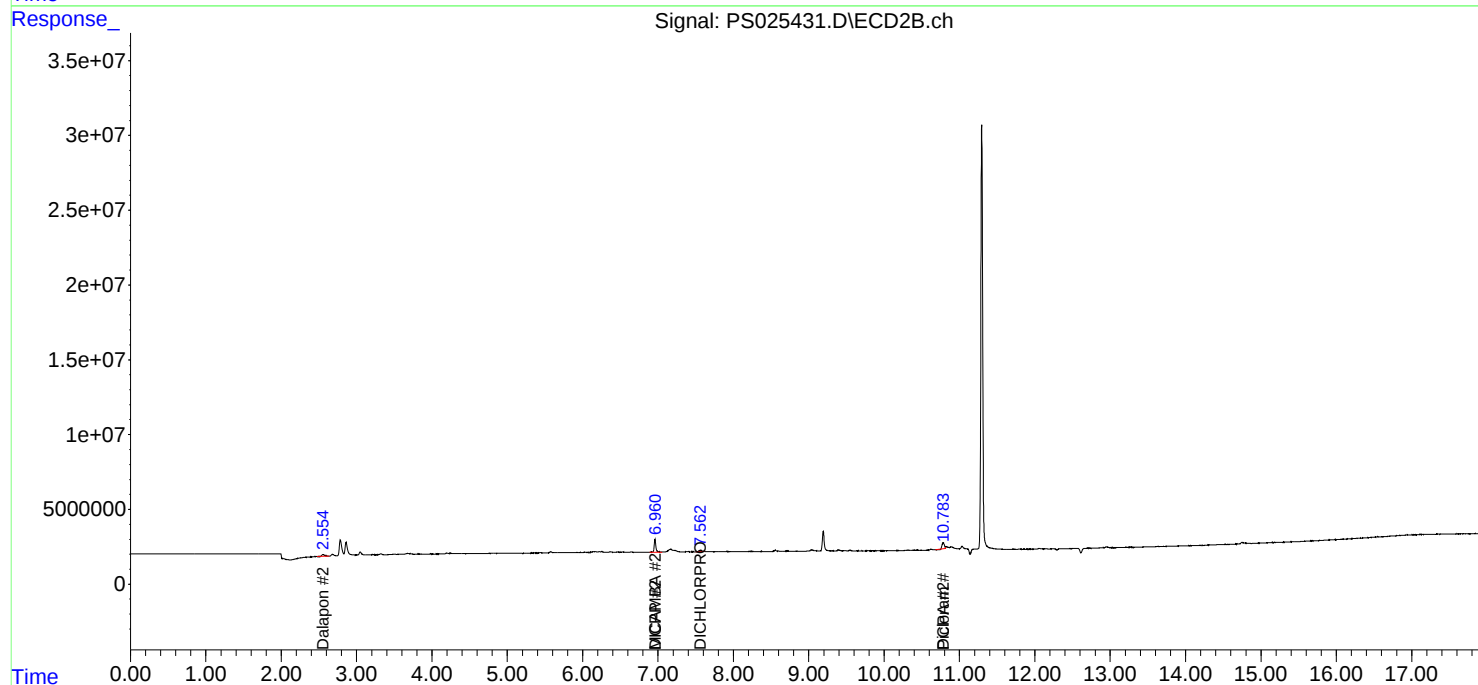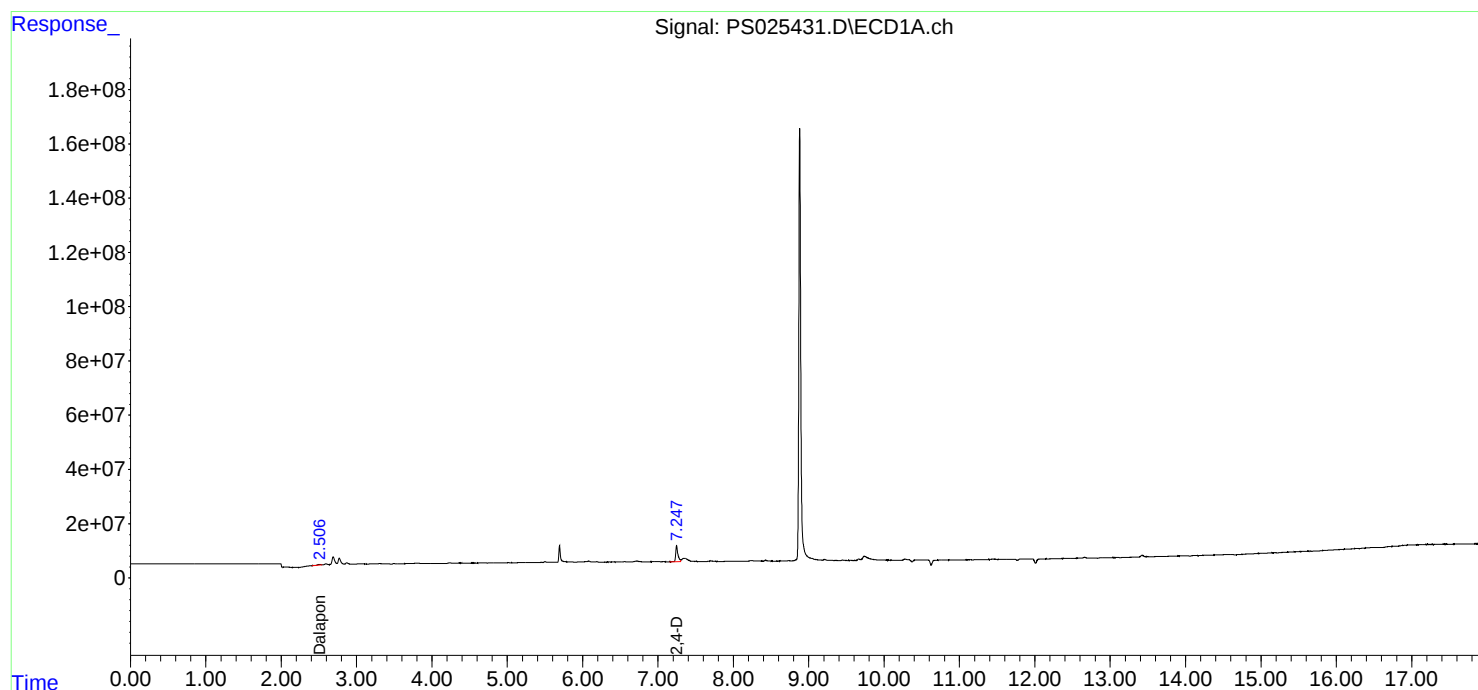


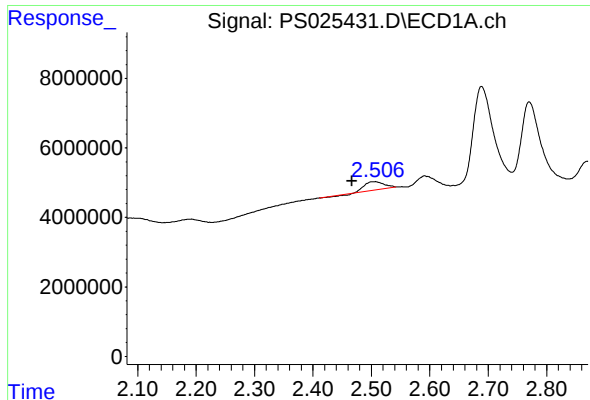

#1 Dalapon


R.T.: 2.506 min
Delta R.T.: 0.039 min
Response: 5233100
Conc: 1.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

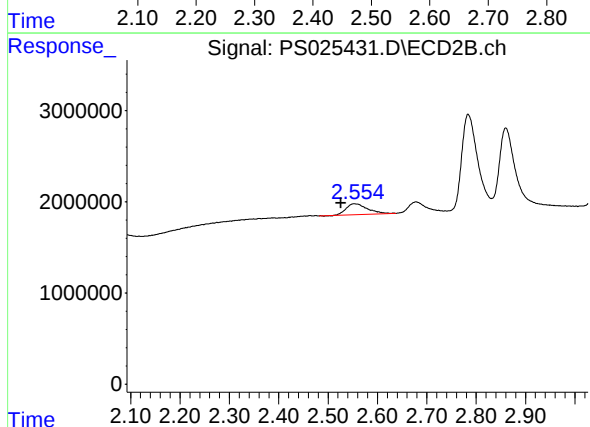


#1 Dalapon

R.T.: 2.554 min
Delta R.T.: 0.028 min
Response: 3524378
Conc: 3.07 ng/ml

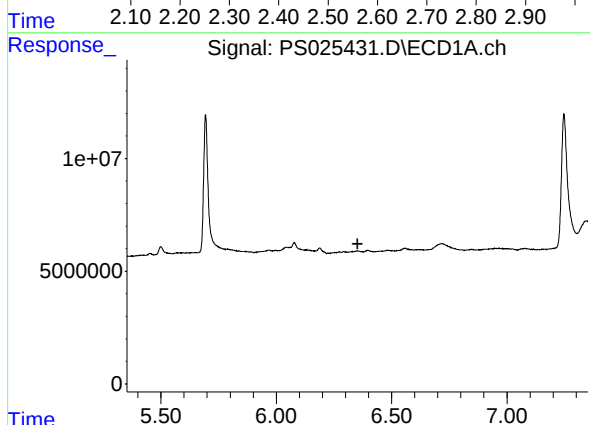


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

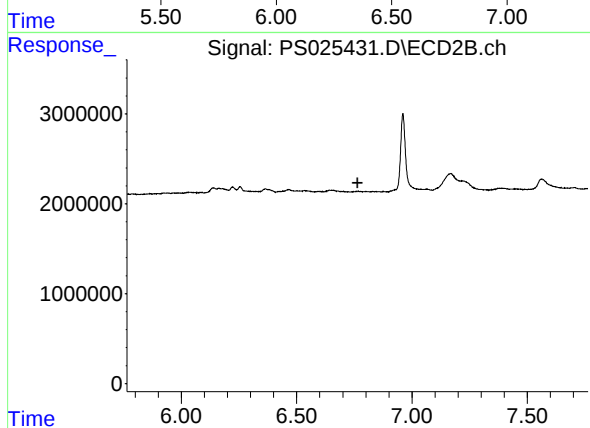

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

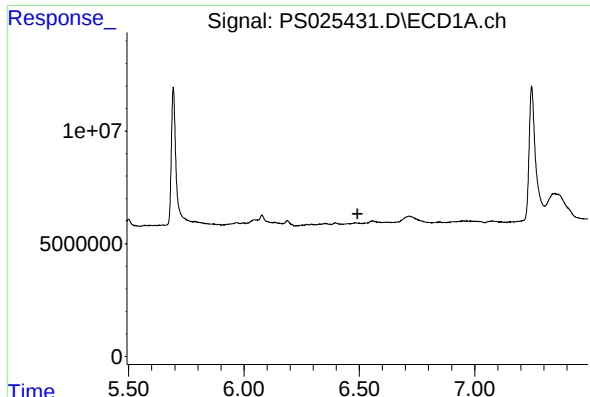

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

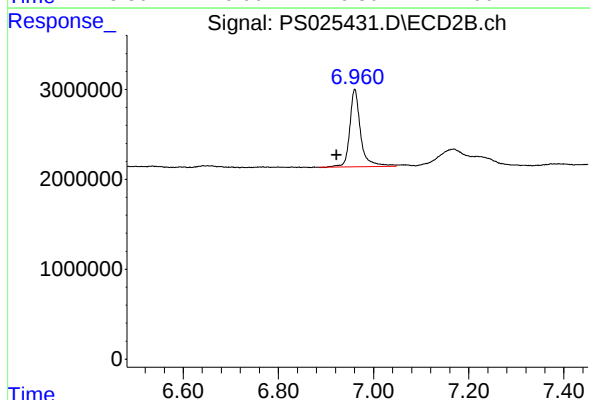


#5 DICAMBA

R.T.: 6.961 min
Delta R.T.: 0.038 min
Response: 13762744
Conc: 4.55 ng/ml

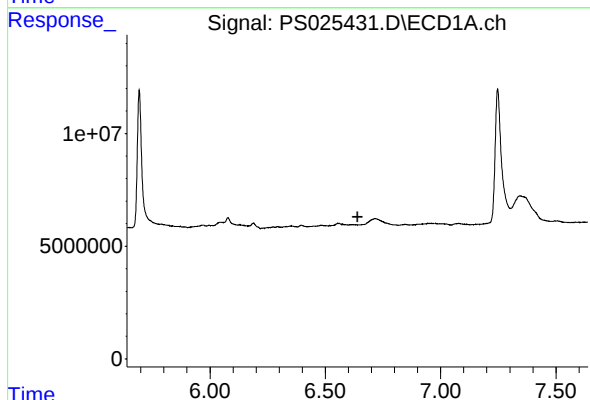


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

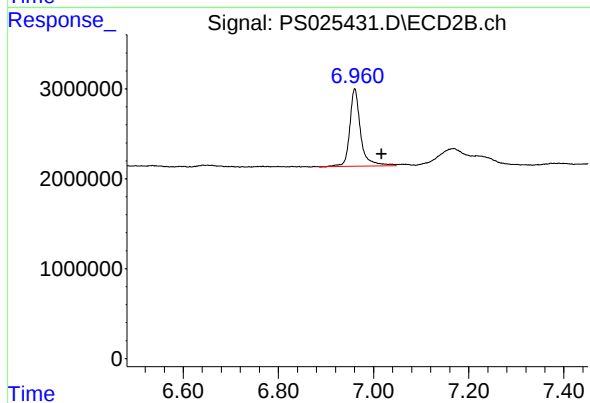

#6 MCPP


R.T.: 6.961 min
Delta R.T.: -0.056 min
Response: 13762744
Conc: 6.89 ug/ml

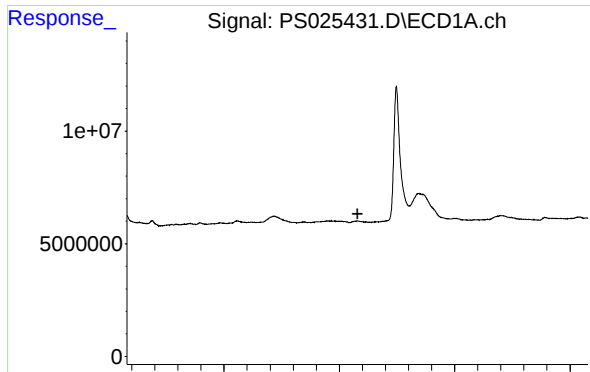

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

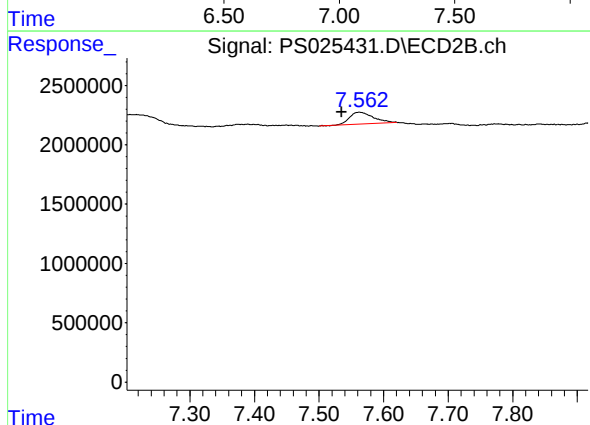


#8 DICHLORPROP

R.T.: 7.563 min
Delta R.T.: 0.028 min
Response: 2496231
Conc: 3.23 ng/ml

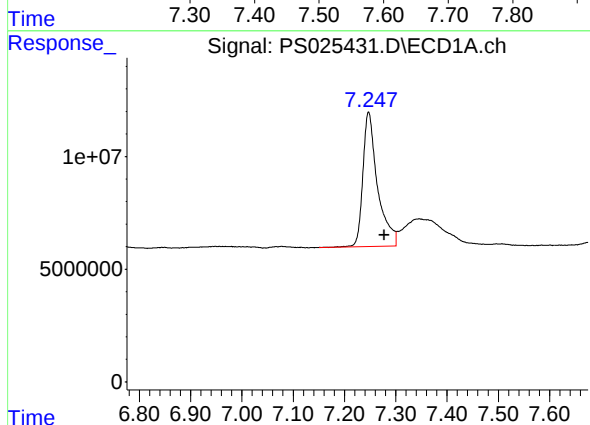


#9 2,4-D

R.T.: 7.247 min
Delta R.T.: -0.031 min
Response: 118777783
Conc: 38.34 ng/ml

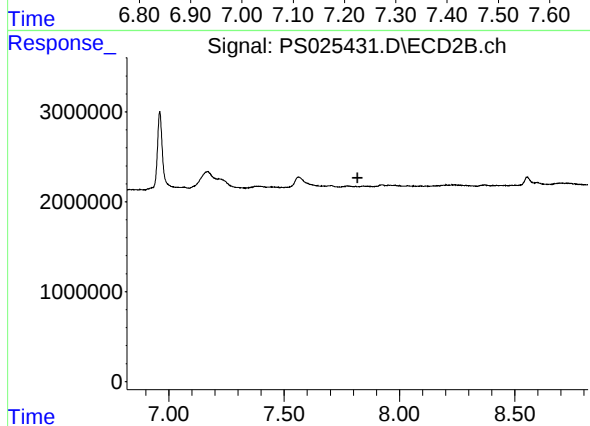

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.818 min
Response: 0
Conc: N.D.

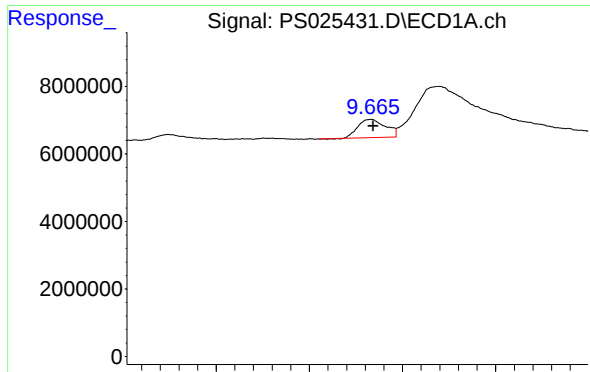

#15 Picloram


R.T.: 9.666 min
Delta R.T.: -0.003 min
Response: 11209937
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

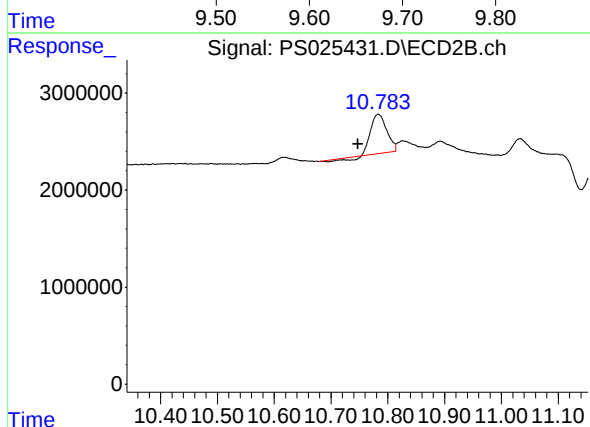


#15 Picloram

R.T.: 10.783 min
Delta R.T.: 0.035 min
Response: 7396478
Conc: 1.09 ng/ml

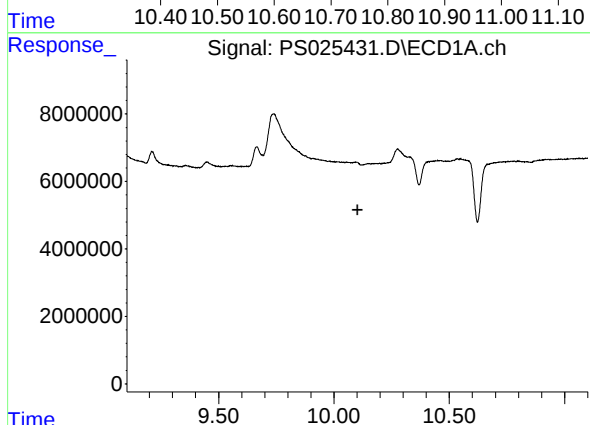

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.102 min
Response: 0
Conc: N.D.

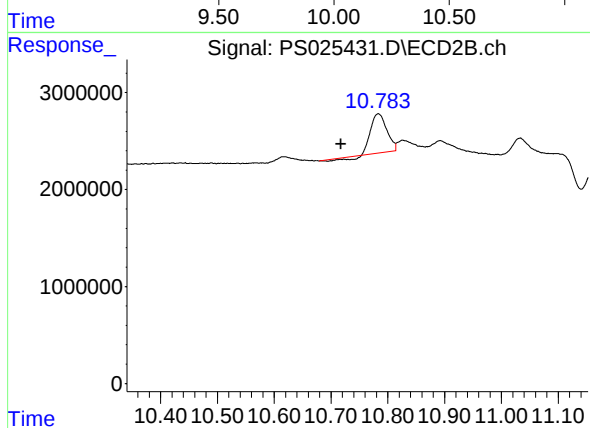

#16 DCPA

R.T.: 10.783 min
Delta R.T.: 0.066 min
Response: 7396478
Conc: 1.39 ng/ml