

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010324\
 Data File : PS025432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2024 10:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 23:24:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.352	6.762	1088.5E6	343.8E6	485.771	484.439
Target Compounds							
1) T	Dalapon	0.000	2.558	0	3327296	N.D.	2.895
3) T	4-Nitroph...	0.000	6.362	0	754947	N.D.	1.520
5) T	DICAMBA	0.000	6.960	0	2329561	N.D.	<MDL
6) T	MCP	0.000	6.960f	0	2329561	N.D.	1.167
7) T	MCPA	0.000	7.156f	0	9873146	N.D.	3.141
8) T	DICHLORPROP	0.000	7.567	0	2118124	N.D.	2.738
9) T	2,4-D	7.249	0.000	19119468	0	6.172	N.D. #
15) T	Picloram	0.000	10.792f	0	7071133	N.D.	1.038



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010324\
Data File : PS025432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2024 10:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 23:24:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

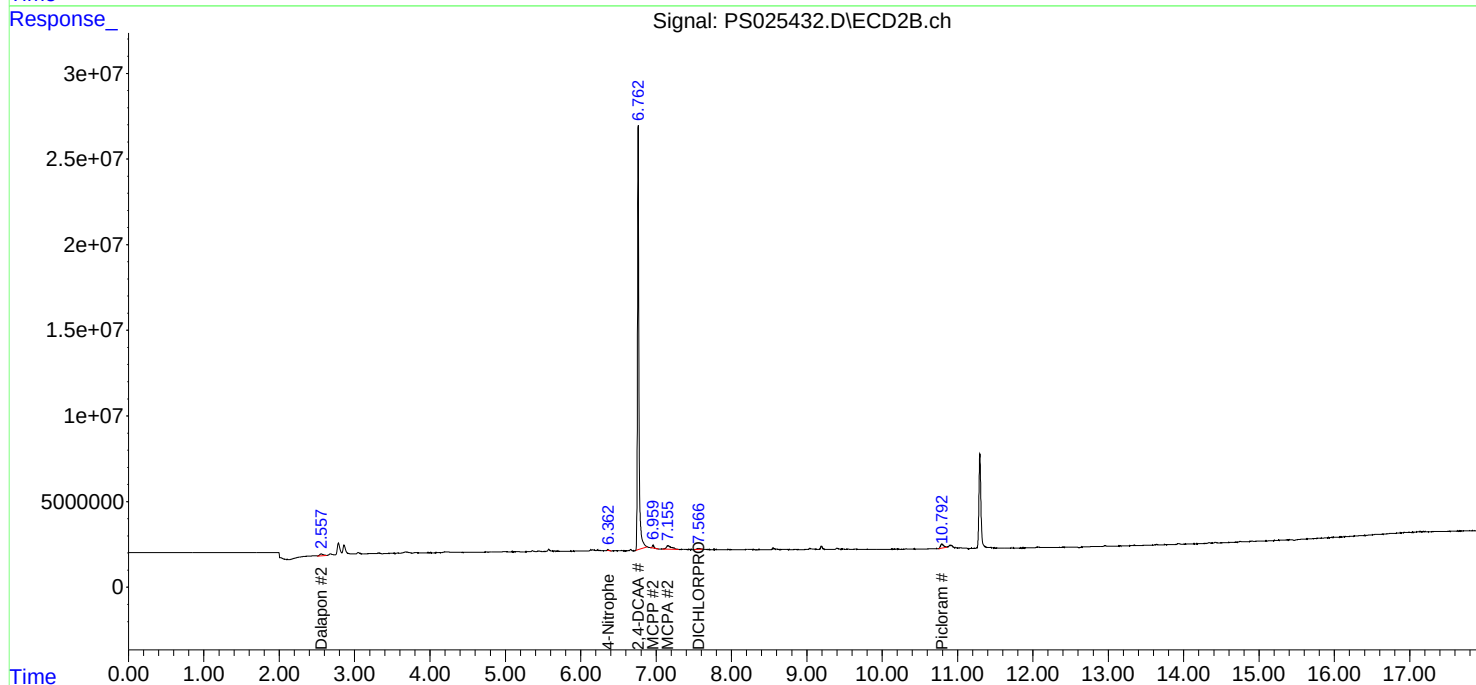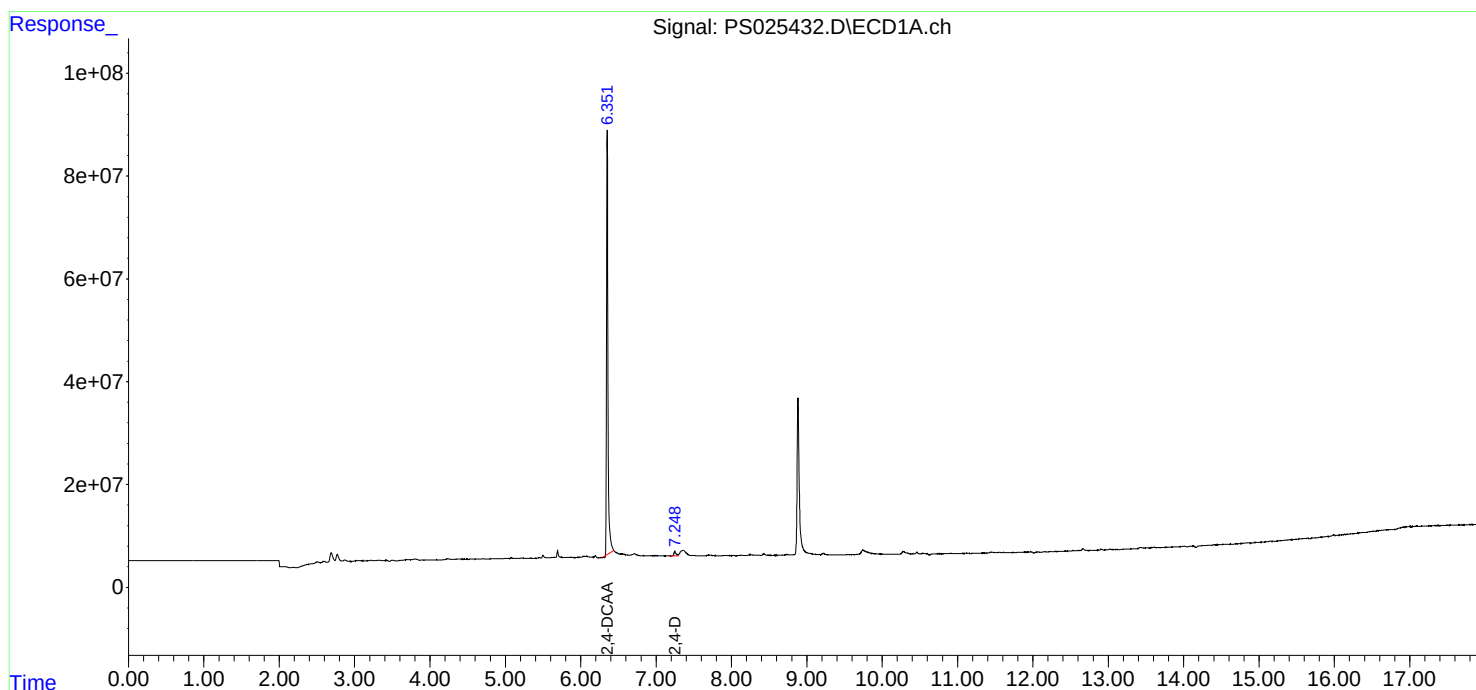


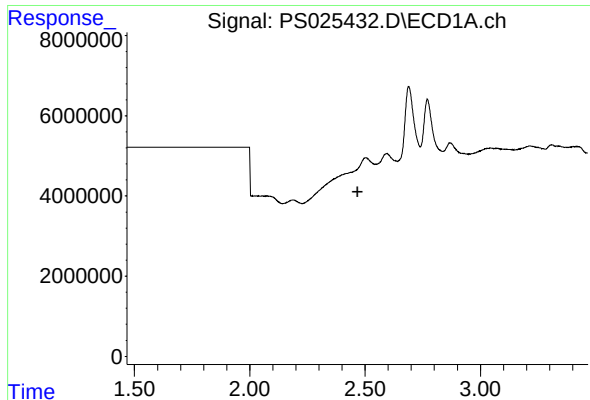

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

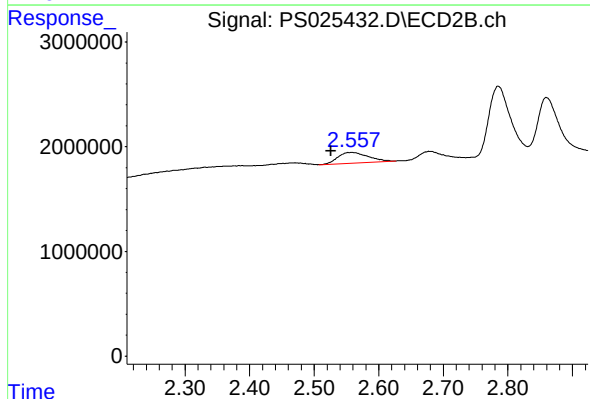


#1 Dalapon

R.T.: 2.558 min
Delta R.T.: 0.032 min
Response: 3327296
Conc: 2.90 ng/ml

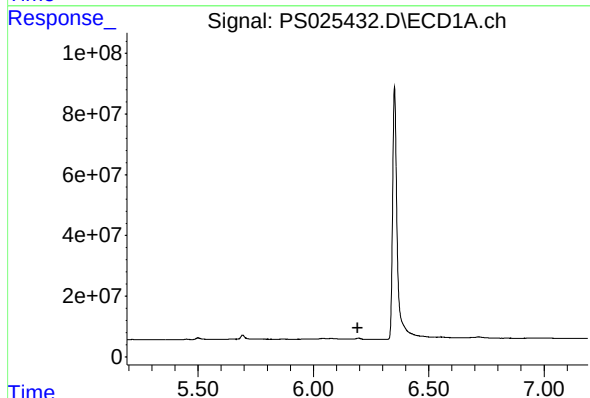


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

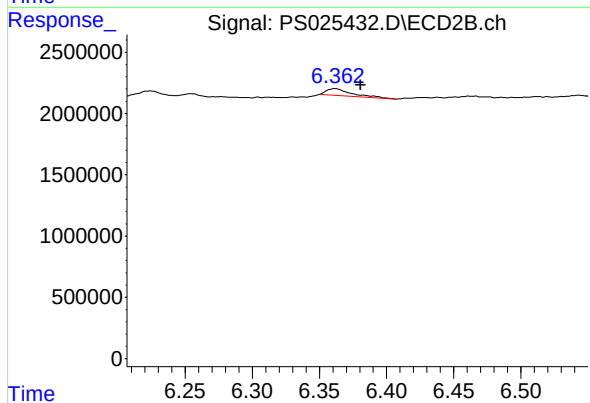

#3 4-Nitrophenol


R.T.: 6.362 min
Delta R.T.: -0.019 min
Response: 754947
Conc: 1.52 ng/ml

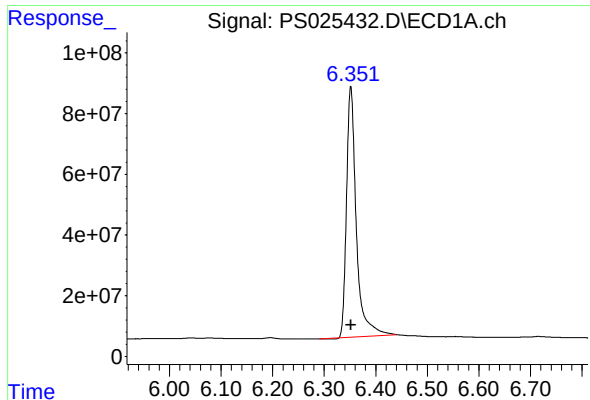

#4 2,4-DCAA


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 1088517403
Conc: 485.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

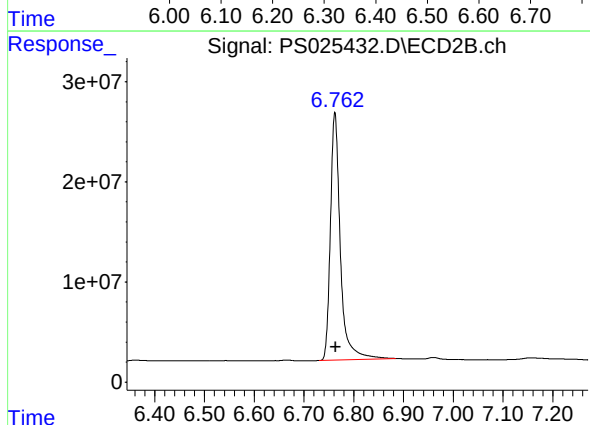


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 343841680
Conc: 484.44 ng/ml

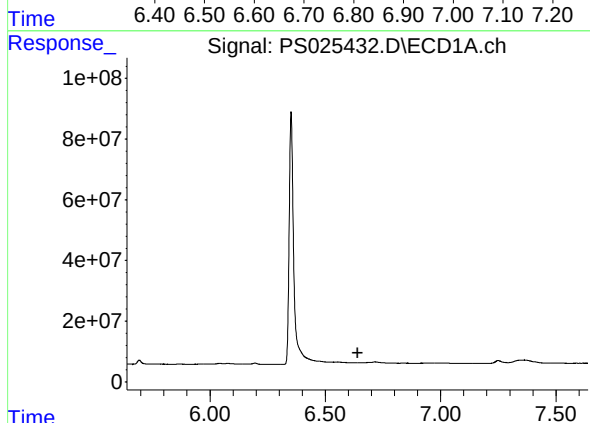


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

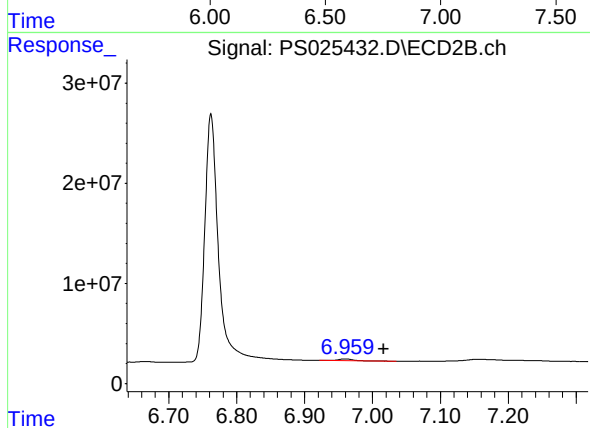

#6 MCPP


R.T.: 6.960 min
Delta R.T.: -0.005 min
Response: 2329561
Conc: 1.17 ug/ml

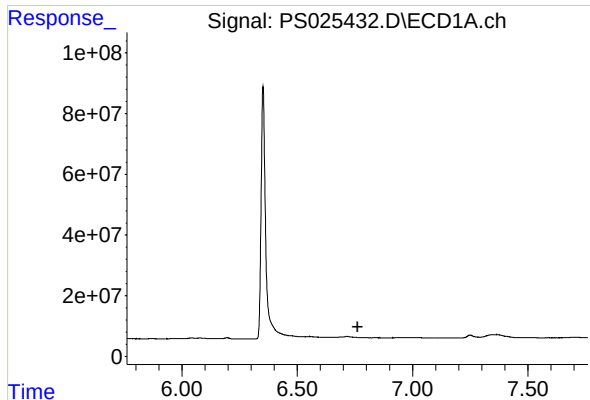

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

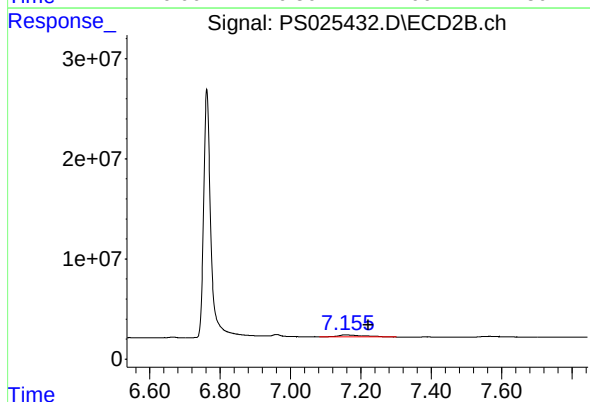


#7 MCPA

R.T.: 7.156 min
Delta R.T.: -0.065 min
Response: 9873146
Conc: 3.14 ug/ml

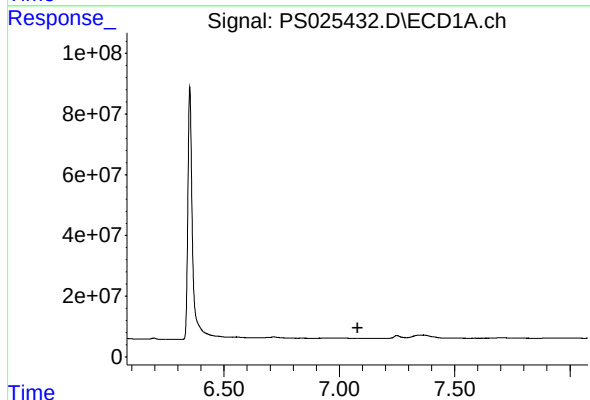


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

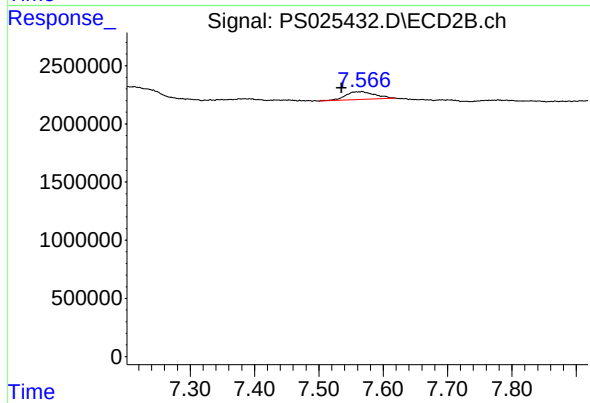

#8 DICHLORPROP


R.T.: 7.567 min
Delta R.T.: 0.032 min
Response: 2118124
Conc: 2.74 ng/ml

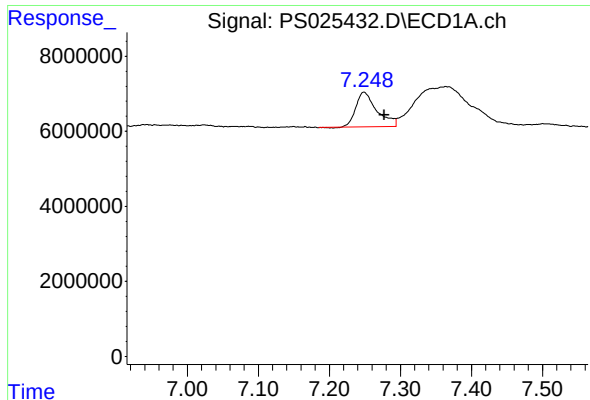

#9 2,4-D


R.T.: 7.249 min
Delta R.T.: -0.029 min
Response: 19119468
Conc: 6.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

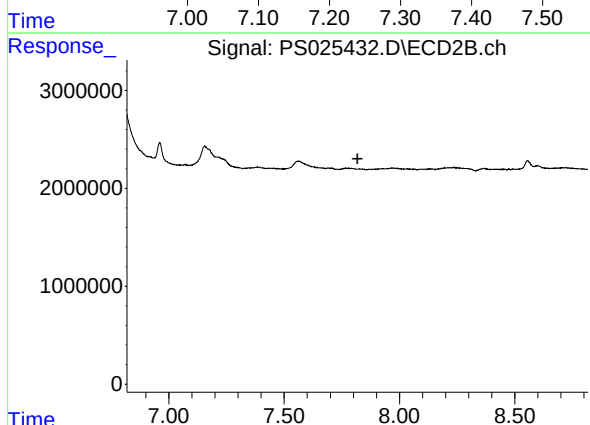


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.818 min
Response: 0
Conc: N.D.

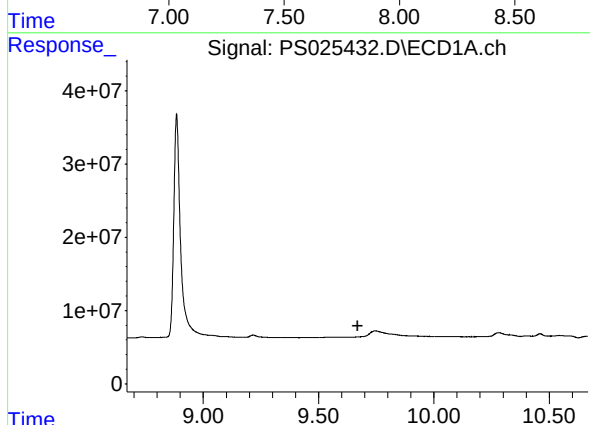

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.668 min
Response: 0
Conc: N.D.

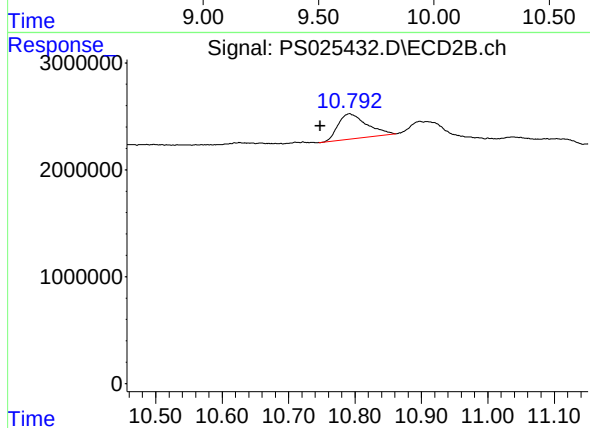

#15 Picloram

R.T.: 10.792 min
Delta R.T.: 0.044 min
Response: 7071133
Conc: 1.04 ng/ml