

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010324\
 Data File : PS025436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2024 13:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 23:25:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.352	6.761	1100.7E6	346.3E6	491.215	487.861
Target Compounds						
1) T Dalapon	0.000	2.552	0	3116542	N.D.	2.712
2) T 3,5-DICHL...	5.693	0.000	961968	0	<MDL	N.D. #
3) T 4-Nitroph...	0.000	6.362	0	834995	N.D.	1.681
5) T DICAMBA	0.000	6.959	0	1778597	N.D.	<MDL
6) T MCPP	0.000	6.959f	0	1778597	N.D.	<MDL
7) T MCPA	6.715f	7.155f	6564130	11905616	<MDL	3.788 #
8) T DICHLORPROP	0.000	7.558	0	4359181	N.D.	5.635
9) T 2,4-D	7.248	0.000	14968885	0	4.832	N.D. #
15) T Picloram	0.000	10.785	0	1751357	N.D.	<MDL
16) T DCPA	0.000	10.785f	0	1751357	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010324\
Data File : PS025436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2024 13:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 23:25:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

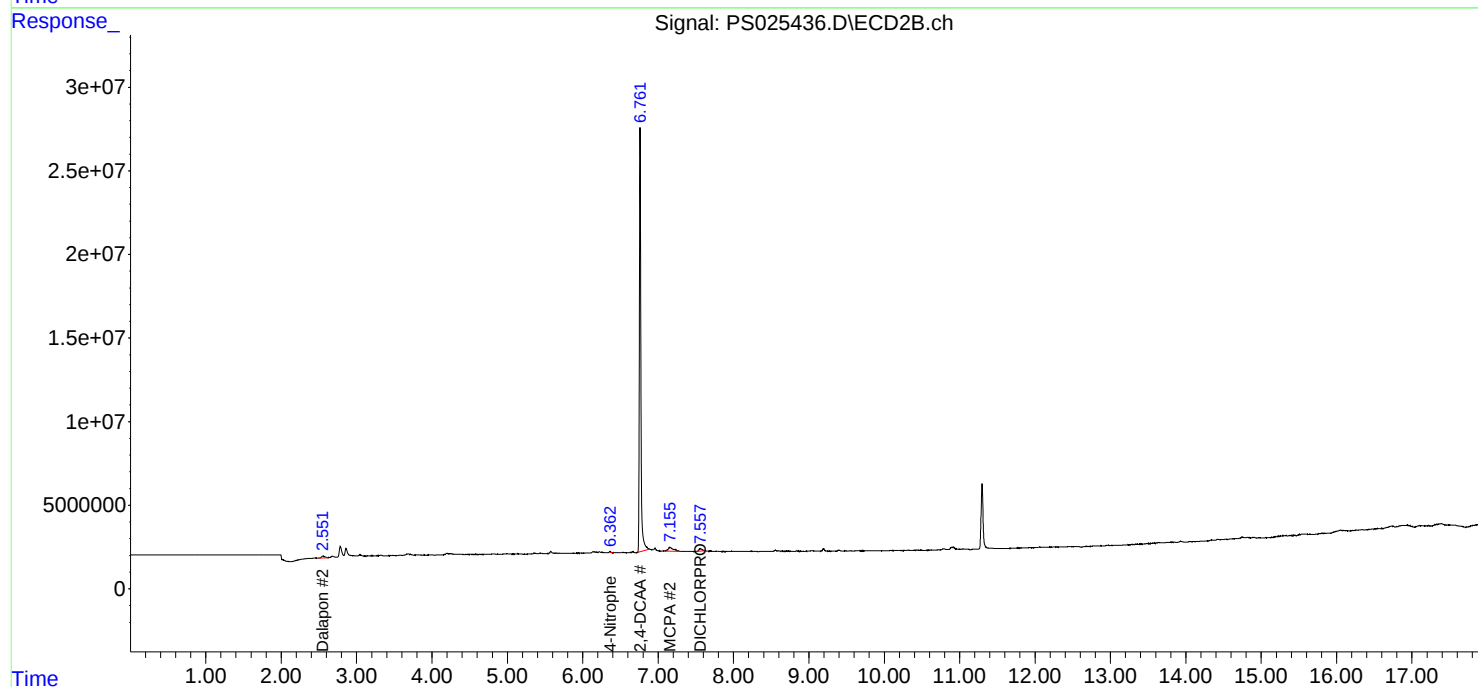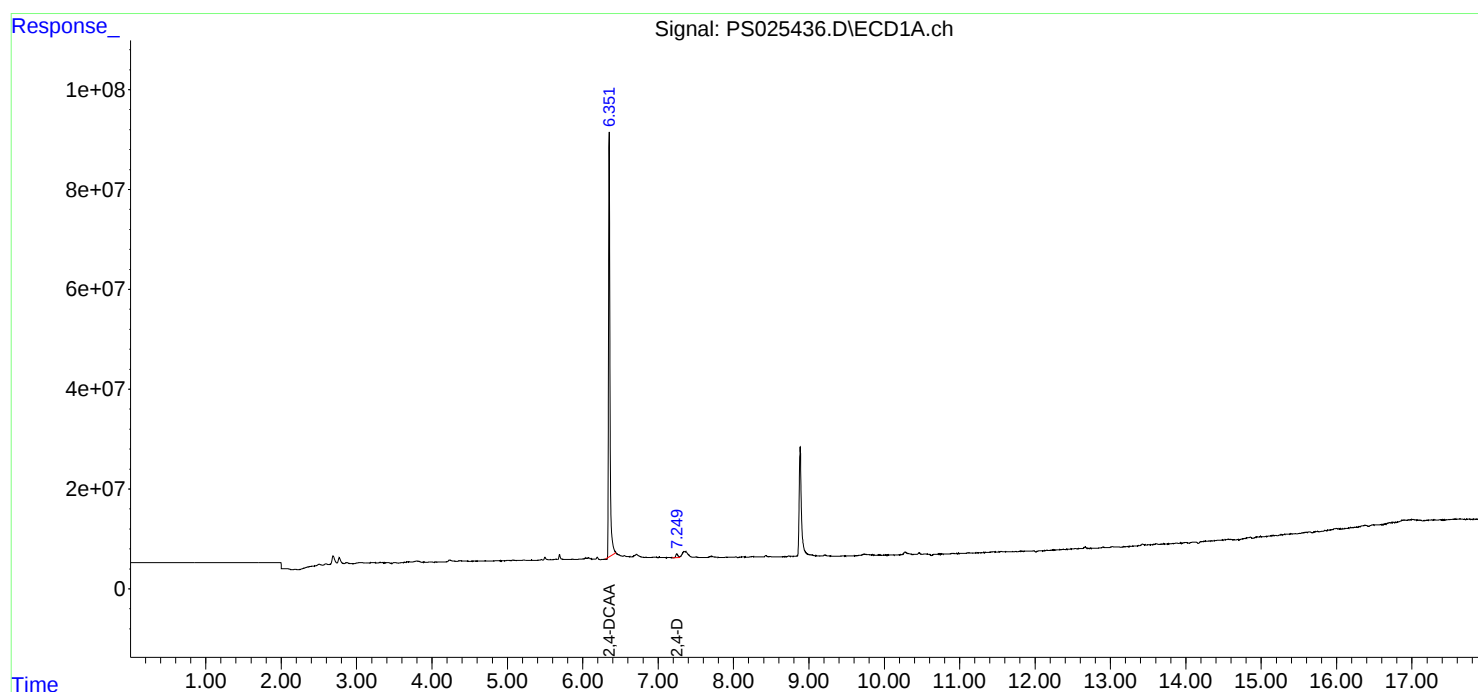


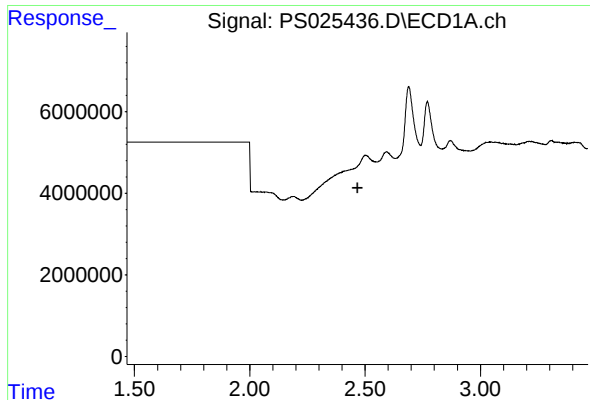

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

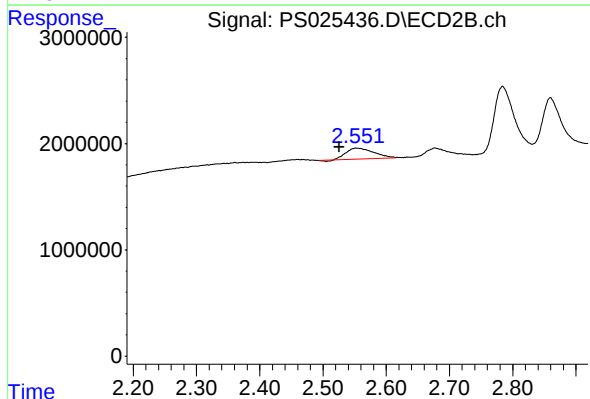


#1 Dalapon

R.T.: 2.552 min
Delta R.T.: 0.026 min
Response: 3116542
Conc: 2.71 ng/ml

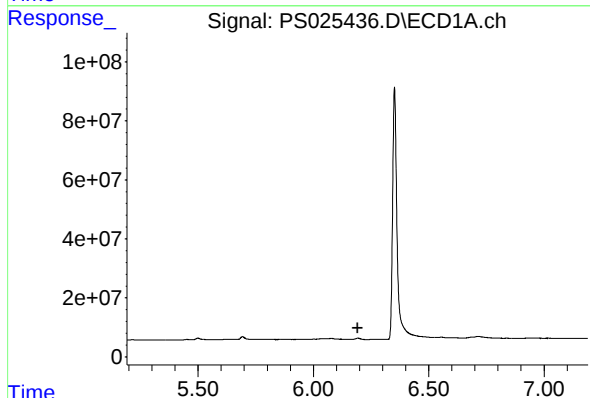


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

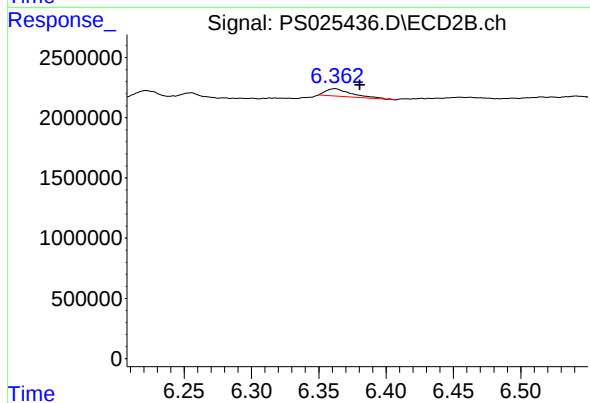

#3 4-Nitrophenol


R.T.: 6.362 min
Delta R.T.: -0.019 min
Response: 834995
Conc: 1.68 ng/ml

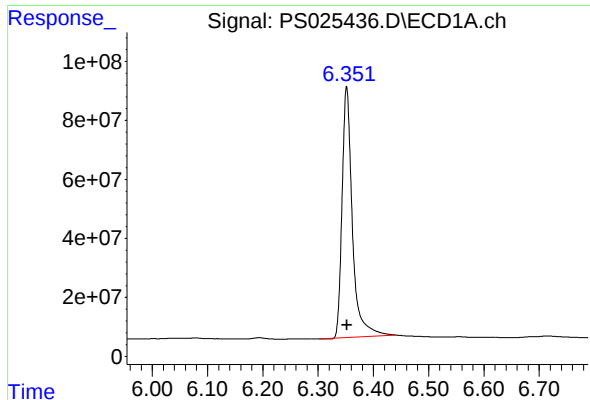

#4 2,4-DCAA


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 1100716563
Conc: 491.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

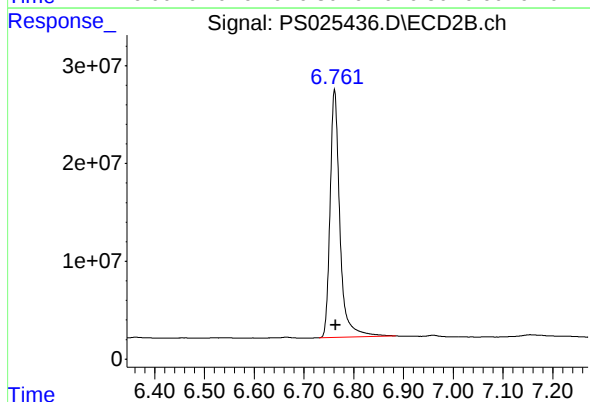


#4 2,4-DCAA

R.T.: 6.761 min
Delta R.T.: -0.002 min
Response: 346270796
Conc: 487.86 ng/ml

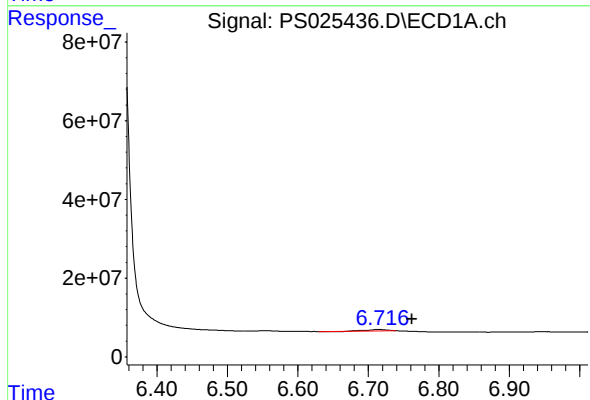


#7 MCPA

R.T.: 6.715 min
Delta R.T.: -0.046 min
Response: 6564130
Conc: N.D.

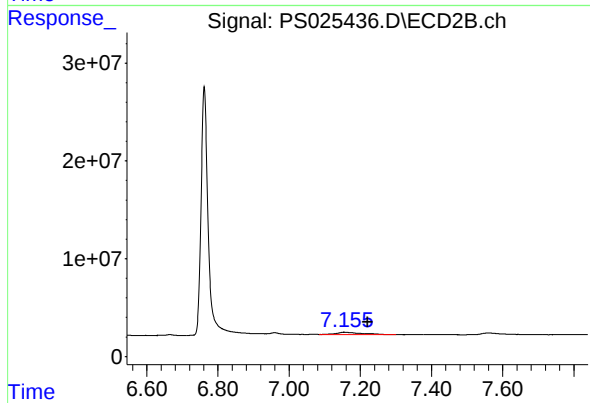

#7 MCPA


R.T.: 7.155 min
Delta R.T.: -0.066 min
Response: 11905616
Conc: 3.79 ug/ml

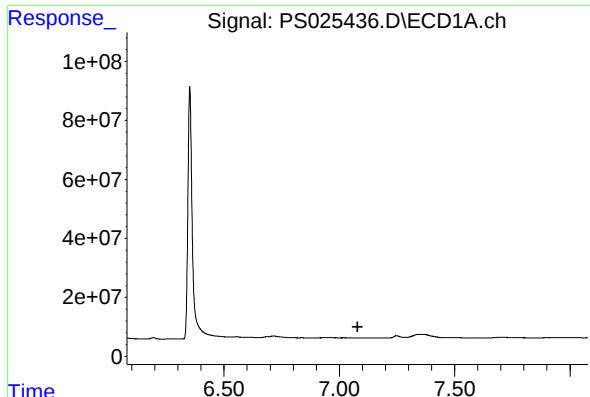

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

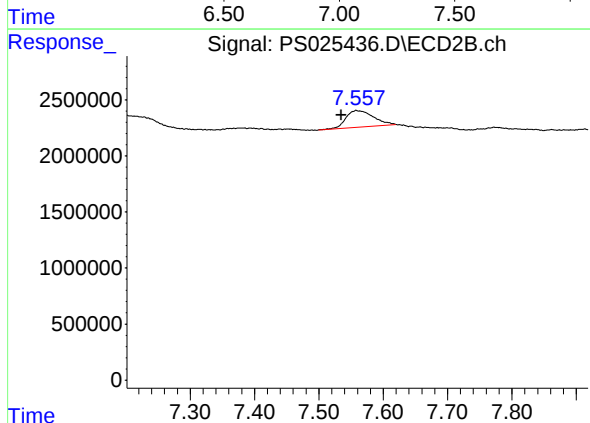


#8 DICHLORPROP

R.T.: 7.558 min
Delta R.T.: 0.023 min
Response: 4359181
Conc: 5.64 ng/ml

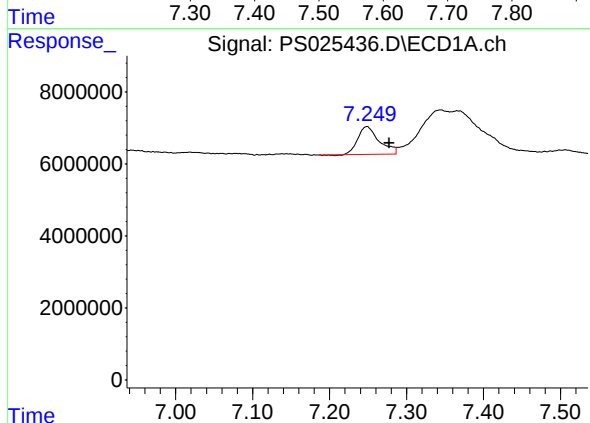

#9 2,4-D

R.T.: 7.248 min
Delta R.T.: -0.029 min
Response: 14968885
Conc: 4.83 ng/ml

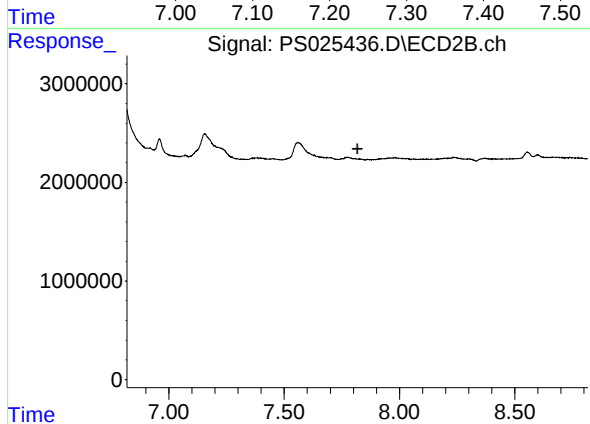

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.818 min
Response: 0
Conc: N.D.