

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010324\
 Data File : PS025447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2024 20:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 23:28:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.351	6.762	1101.1E6	347.3E6	491.388	489.258
Target Compounds						
1) T Dalapon	2.505	2.558	10084468	4181938	3.259	3.639
2) T 3,5-DICHL...	5.693	0.000	1799759	0	<MDL	N.D. #
3) T 4-Nitroph...	0.000	6.361	0	454823	N.D.	<MDL
5) T DICAMBA	0.000	6.960	0	3463139	N.D.	1.144
6) T MCPP	0.000	6.960f	0	3463139	N.D.	1.735
7) T MCPA	6.714f	7.153f	8552062	14601344	<MDL	4.646 #
8) T DICHLORPROP	0.000	7.561	0	5843845	N.D.	7.555
9) T 2,4-D	7.248	0.000	21871365	0	7.060	N.D. #
15) T Picloram	0.000	10.793f	0	501865	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010324\
Data File : PS025447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2024 20:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 23:28:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

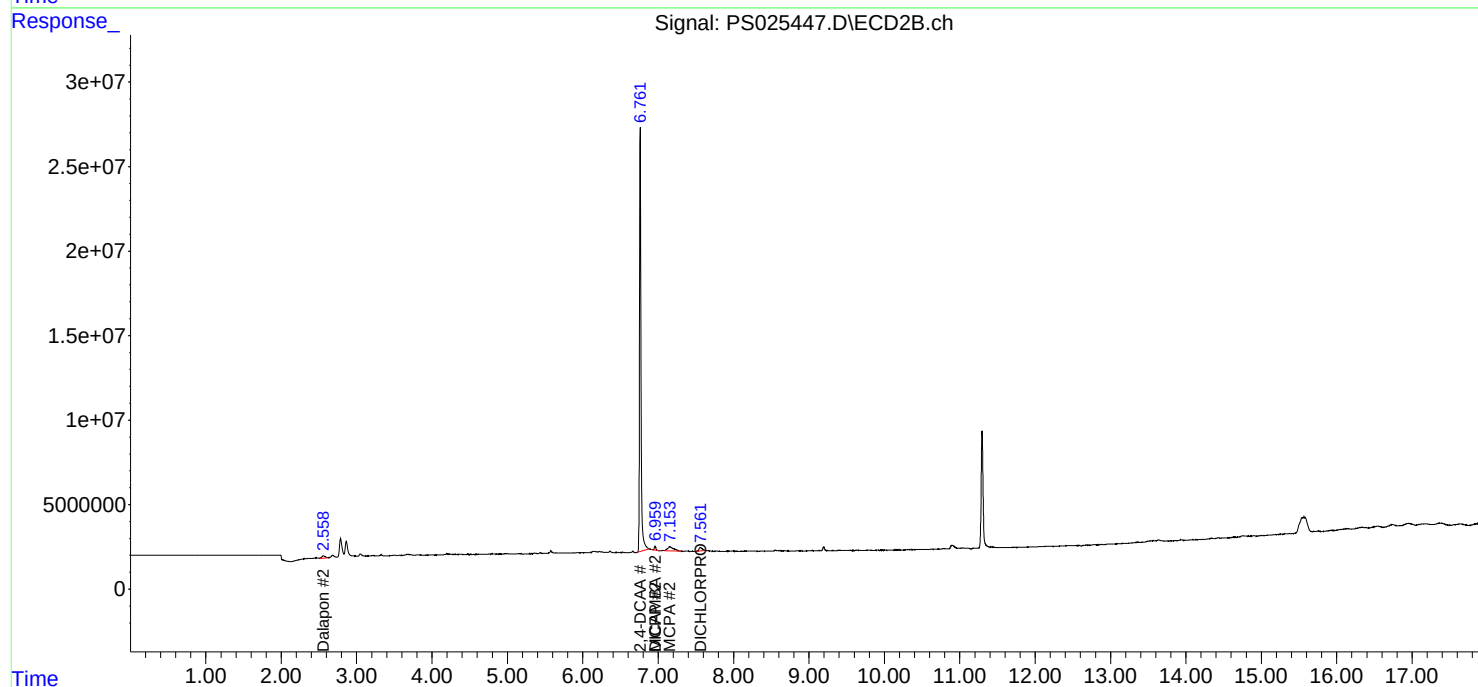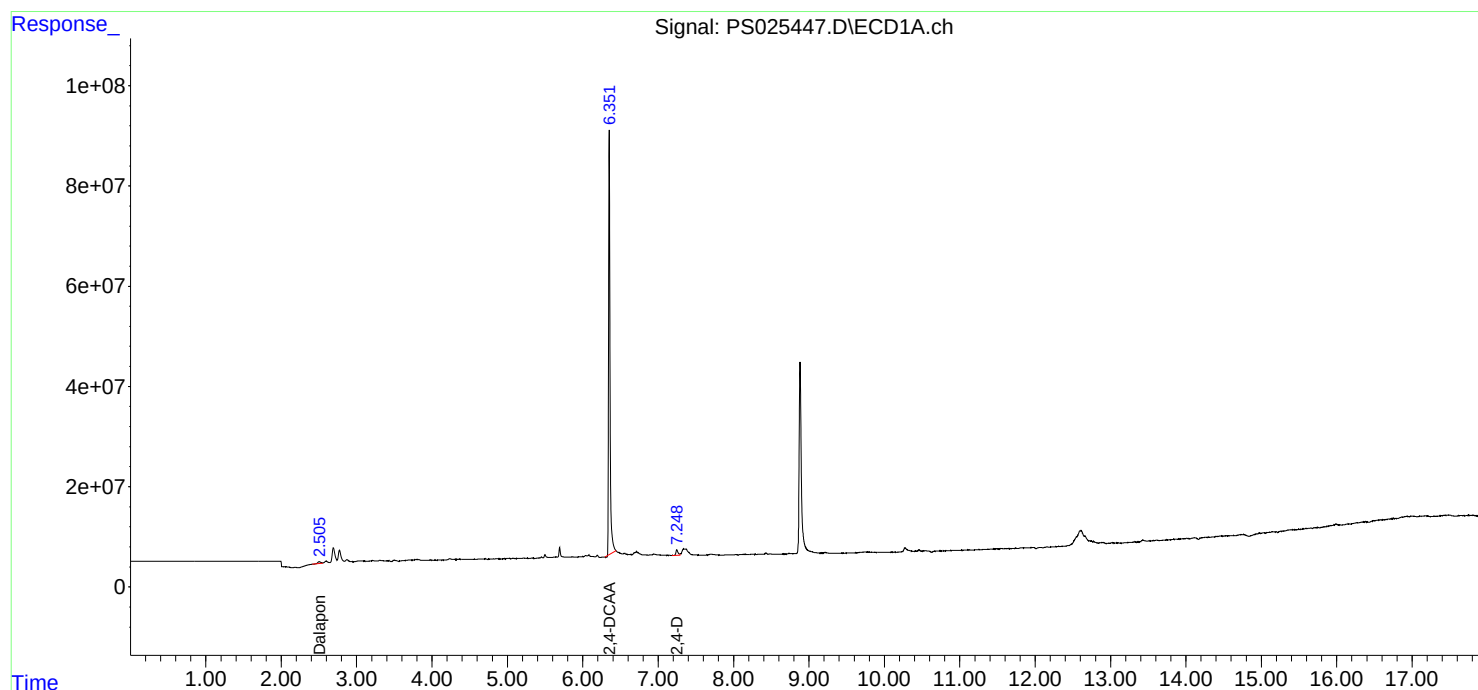


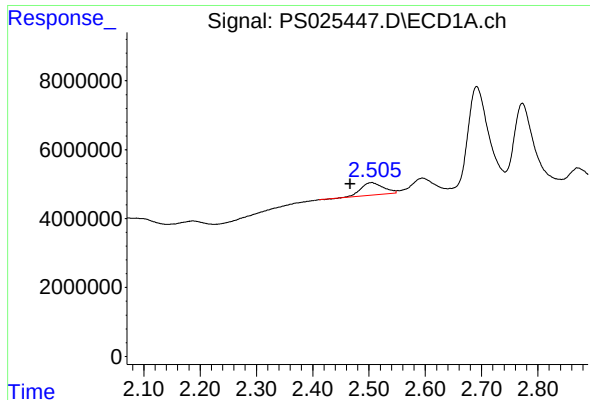

#1 Dalapon


R.T.: 2.505 min
Delta R.T.: 0.038 min
Response: 10084468
Conc: 3.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

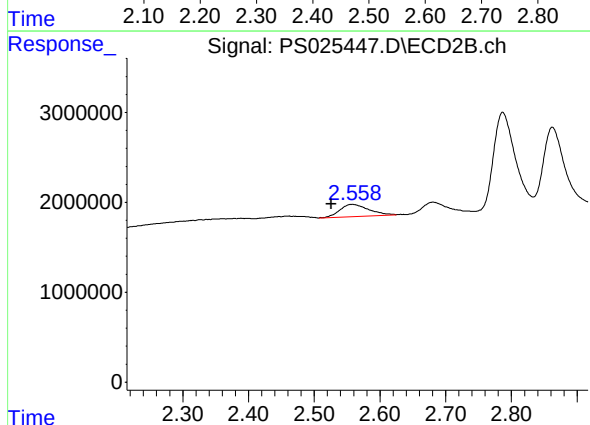


#1 Dalapon

R.T.: 2.558 min
Delta R.T.: 0.032 min
Response: 4181938
Conc: 3.64 ng/ml

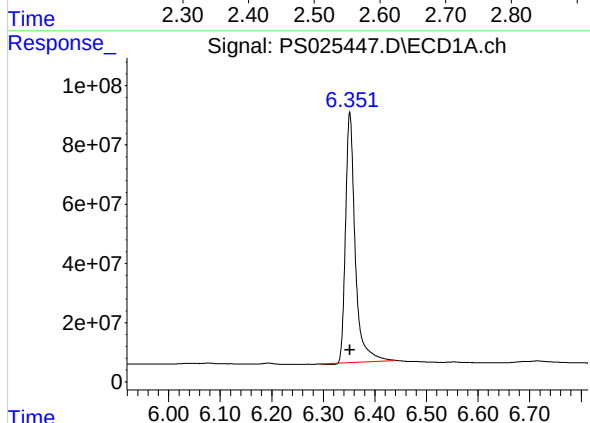


#4 2,4-DCAA

R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 1101103311
Conc: 491.39 ng/ml

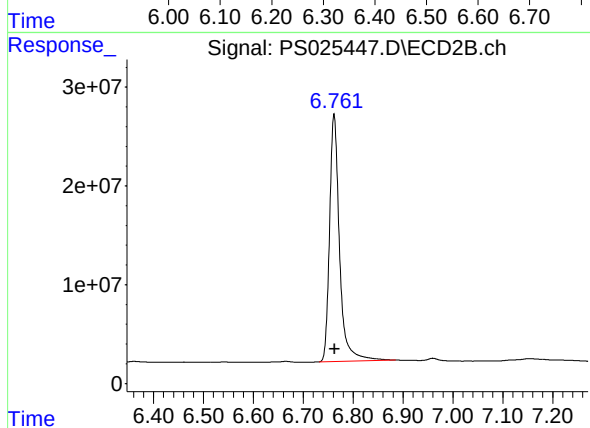

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: -0.002 min
Response: 347262351
Conc: 489.26 ng/ml

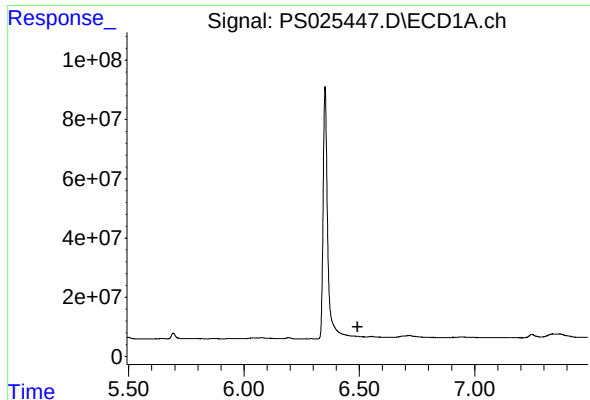

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

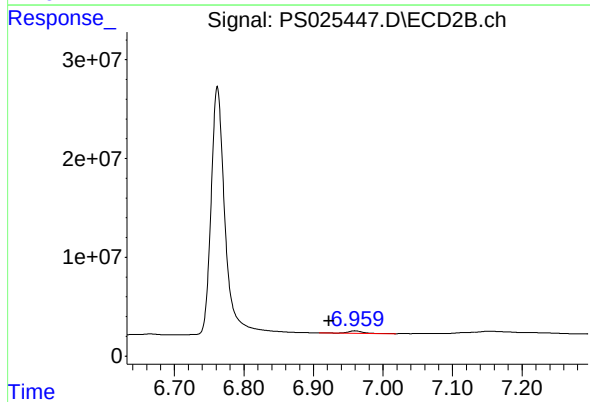


#5 DICAMBA

R.T.: 6.960 min
Delta R.T.: 0.037 min
Response: 3463139
Conc: 1.14 ng/ml

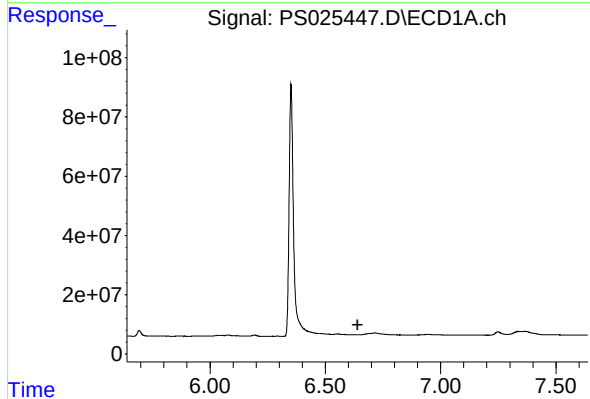


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

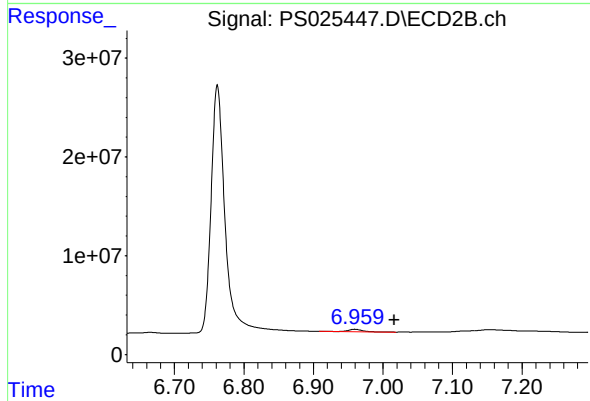

#6 MCPP


R.T.: 6.960 min
Delta R.T.: -0.057 min
Response: 3463139
Conc: 1.73 ug/ml

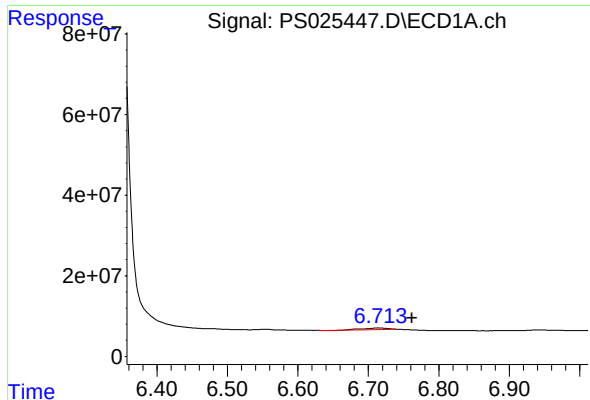

#7 MCPA


R.T.: 6.714 min
Delta R.T.: -0.047 min
Response: 8552062
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

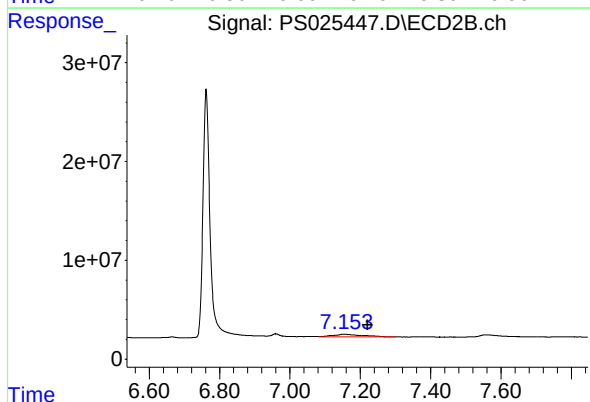


#7 MCPA

R.T.: 7.153 min
Delta R.T.: -0.068 min
Response: 14601344
Conc: 4.65 ug/ml

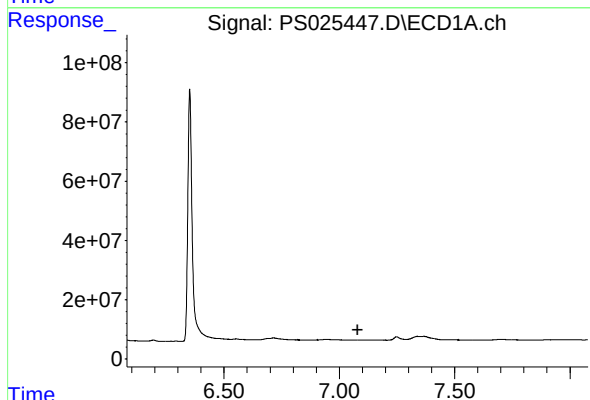


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

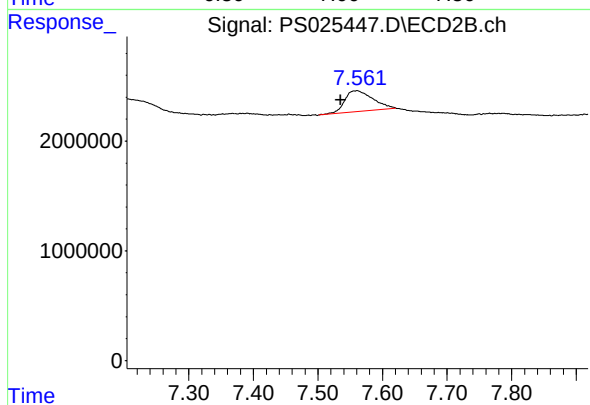

#8 DICHLORPROP


R.T.: 7.561 min
Delta R.T.: 0.026 min
Response: 5843845
Conc: 7.55 ng/ml

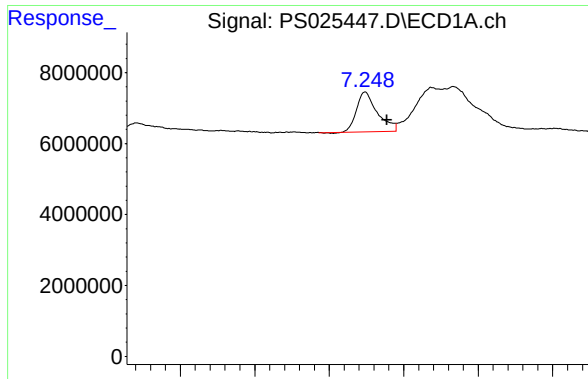

#9 2,4-D

R.T.: 7.248 min
Delta R.T.: -0.030 min
Response: 21871365
Conc: 7.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

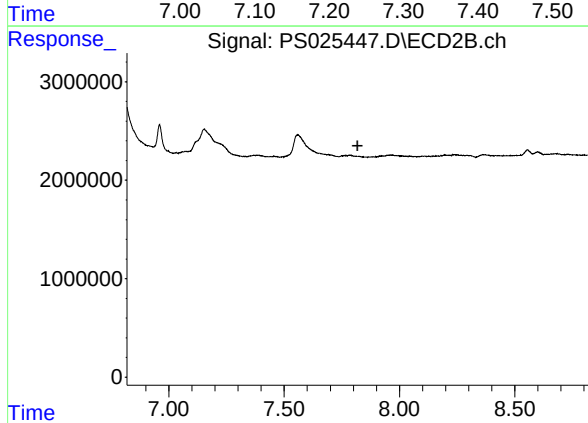

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.818 min
Response: 0
Conc: N.D.