

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010419\
 Data File : PS002751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2019 18:05
 Operator : EI\SJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 06:10:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010419.M
 Quant Title : 8080.M
 QLast Update : Sat Jan 05 06:08:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.389	10.888	239.7E6	290.2E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.882	2.330	244.3E6	215.6E6	682.500	682.500
2) T	3,5-DICHL...	9.817	9.042	358.3E6	348.8E6	697.500	697.500
3) T	4-Nitroph...	10.989	10.041	84734770	122.4E6	682.500	682.500
5) T	DICAMBA	11.696	11.170	1051.7E6	1044.1E6	705.000	705.000
6) T	MCPD	12.036	11.400	71002392	67562345	70.500	70.500
7) T	MCPA	12.286	11.776	107.8E6	97020770	69.750	69.750
8) T	DICHLORPROP	12.884	12.295	252.5E6	257.6E6	705.000	705.000
9) T	2,4-D	13.246	12.769	231.5E6	289.9E6	705.000	705.000
10) T	Pentachlo...	13.618	13.309	3843.2E6	4059.9E6	712.500	712.500
11) T	2,4,5-TP ...	14.490	13.931	1394.5E6	1523.2E6	712.500	712.500
12) T	2,4,5-T	14.892	14.512	1303.3E6	1483.5E6	712.500	712.500
13) T	2,4-DB	15.645	15.159	128.1E6	149.8E6	712.500	712.500
14) T	DINOSEB	17.107	15.574	828.7E6	768.0E6	705.000	705.000
15) T	Picloram	16.932	16.750	1017.9E6	1959.2E6	712.500	712.500
16) T	DCPA	17.451	16.850	1747.9E6	1999.5E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010419\
Data File : PS002751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2019 18:05
Operator : EI\SJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 06:10:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010419.M
Quant Title : 8080.M
QLast Update : Sat Jan 05 06:08:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

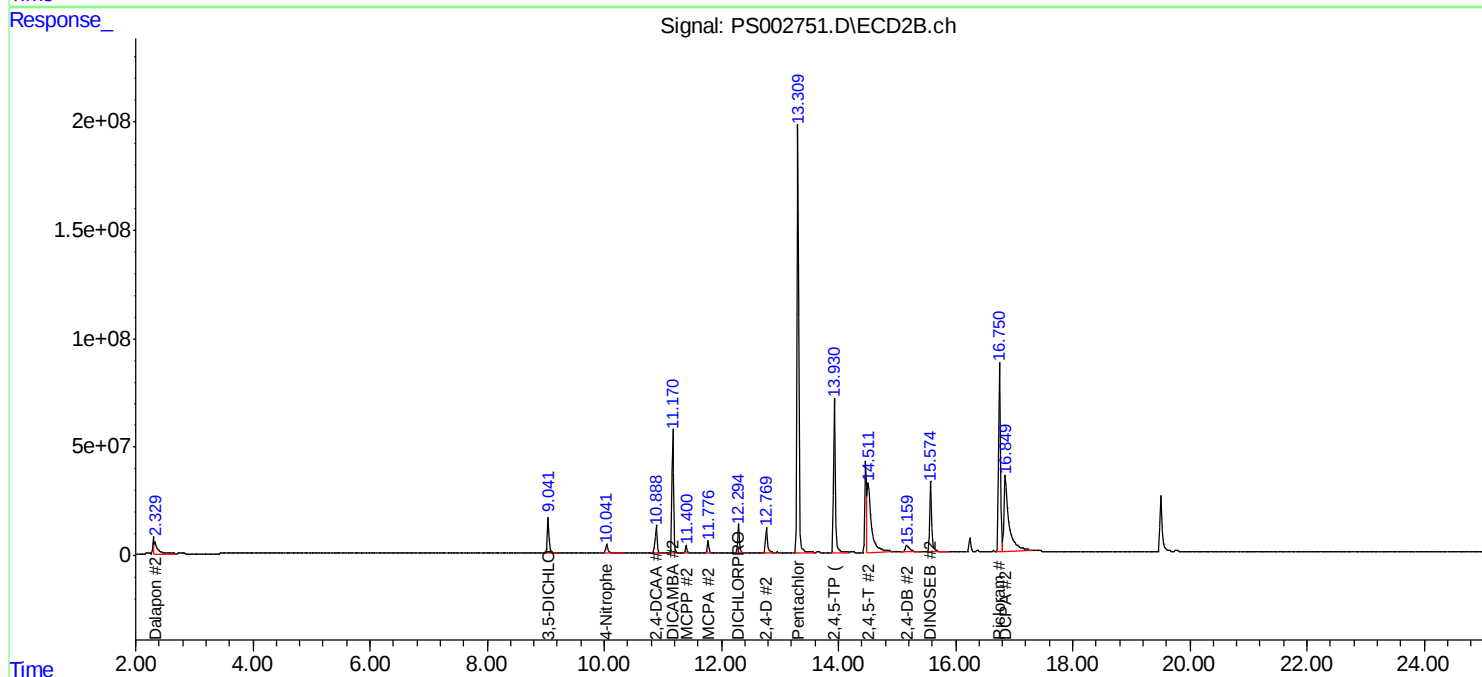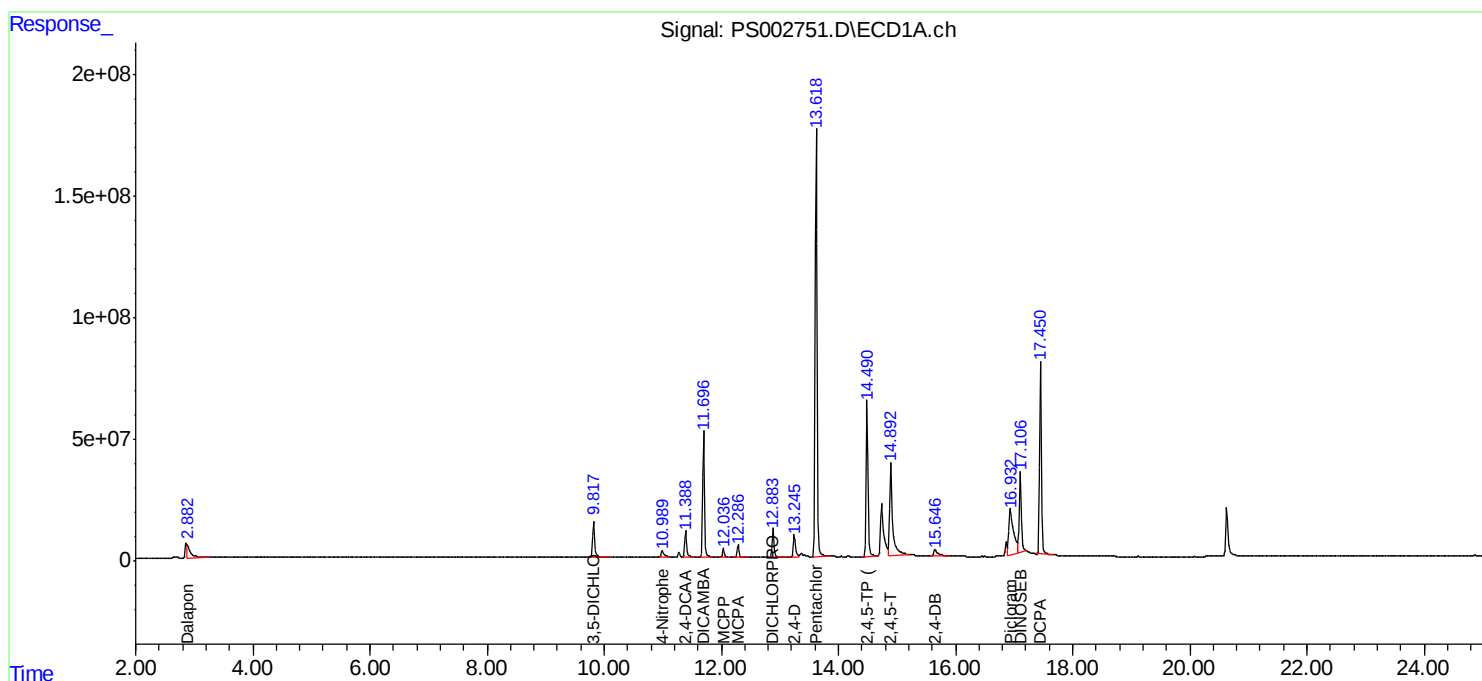


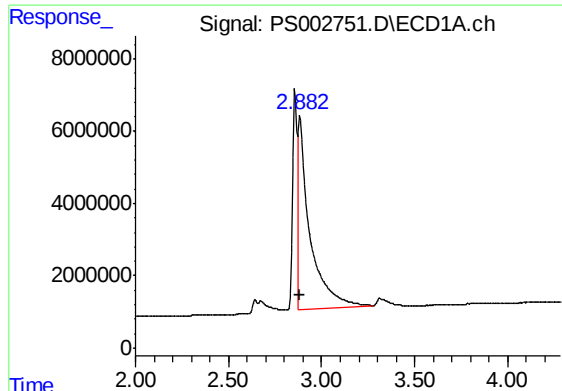

#1 Dalapon


R.T.: 2.882 min
Delta R.T.: 0.000 min
Response: 244328338
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

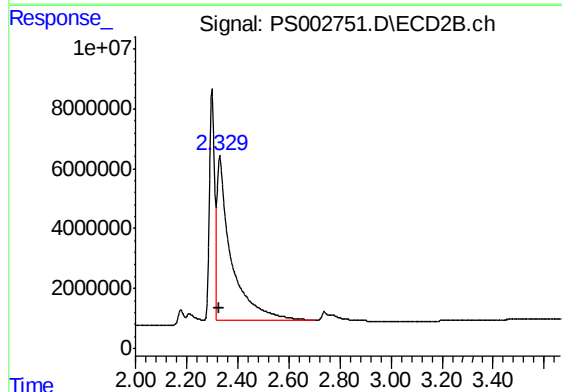


#1 Dalapon

R.T.: 2.330 min
Delta R.T.: 0.000 min
Response: 215618492
Conc: 682.50 ng/ml

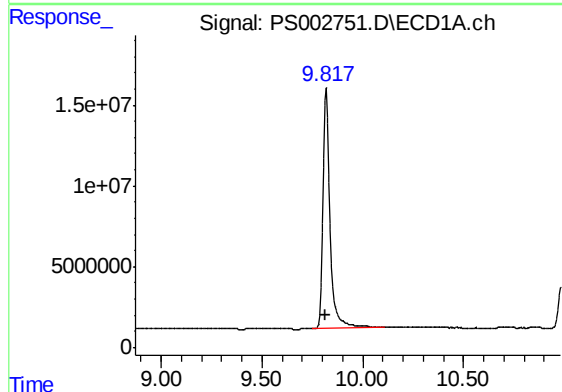


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.817 min
Delta R.T.: 0.000 min
Response: 358293435
Conc: 697.50 ng/ml

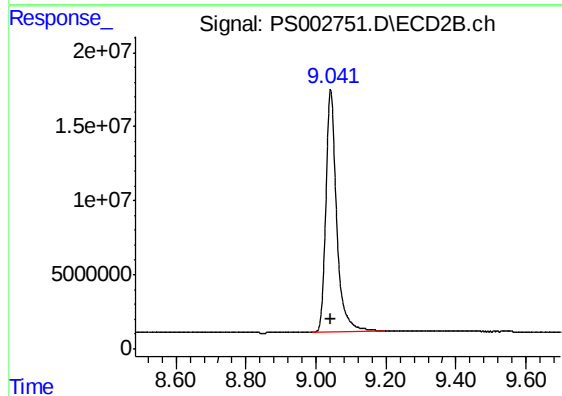

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 348826410
Conc: 697.50 ng/ml

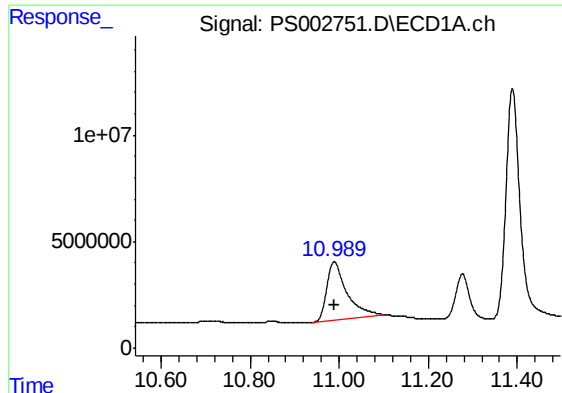

#3 4-Nitrophenol


R.T.: 10.989 min
Delta R.T.: 0.000 min
Response: 84734770
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

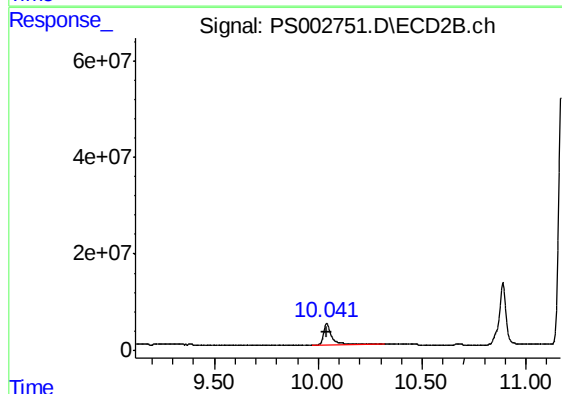


#3 4-Nitrophenol

R.T.: 10.041 min
Delta R.T.: 0.000 min
Response: 122441650
Conc: 682.50 ng/ml

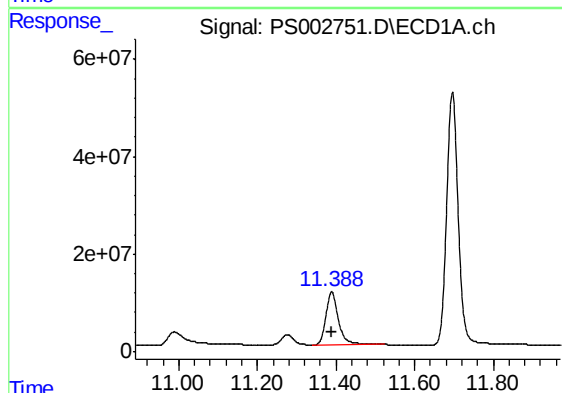


#4 2,4-DCAA

R.T.: 11.389 min
Delta R.T.: 0.000 min
Response: 239740772
Conc: 750.00 ng/ml

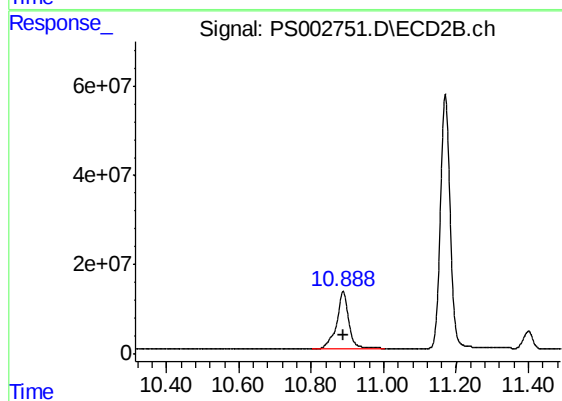

#4 2,4-DCAA


R.T.: 10.888 min
Delta R.T.: 0.000 min
Response: 290228321
Conc: 750.00 ng/ml

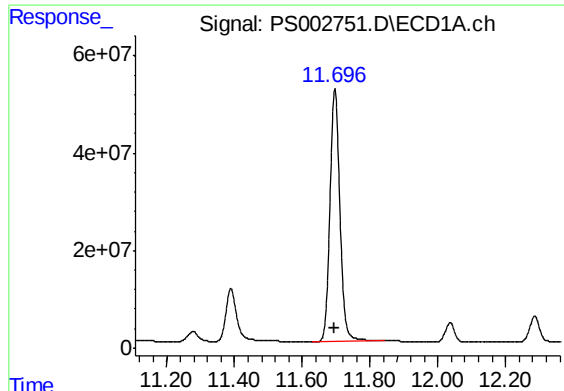

#5 DICAMBA


R.T.: 11.696 min
Delta R.T.: 0.000 min
Response: 1051664521
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

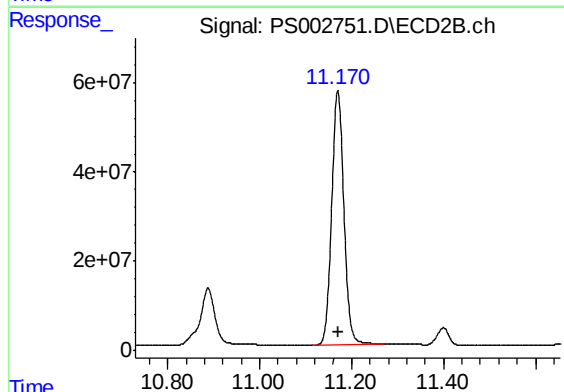


#5 DICAMBA

R.T.: 11.170 min
Delta R.T.: 0.000 min
Response: 1044104346
Conc: 705.00 ng/ml

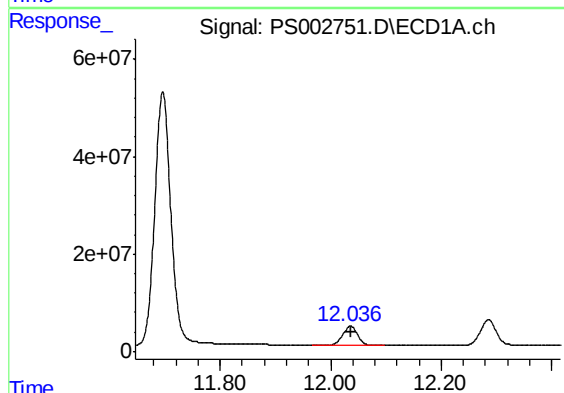


#6 MCPP

R.T.: 12.036 min
Delta R.T.: 0.000 min
Response: 71002392
Conc: 70.50 ug/ml

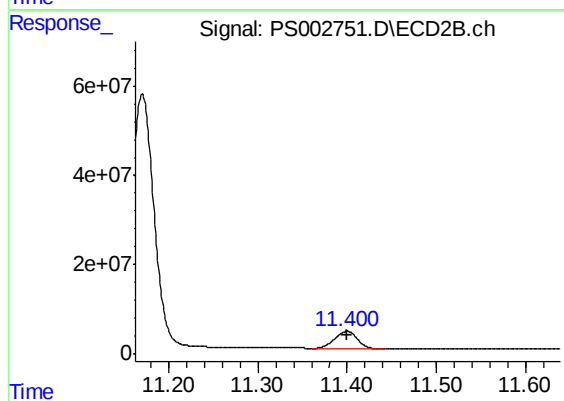

#6 MCPP


R.T.: 11.400 min
Delta R.T.: 0.000 min
Response: 67562345
Conc: 70.50 ug/ml

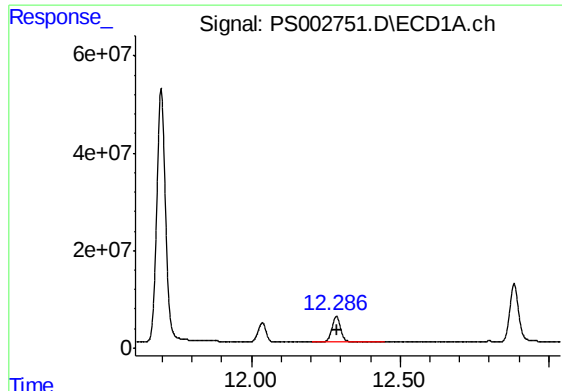

#7 MCPA


R.T.: 12.286 min
Delta R.T.: 0.000 min
Response: 107783930
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

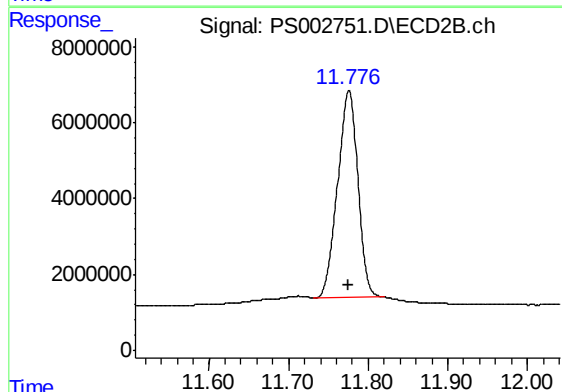


#7 MCPA

R.T.: 11.776 min
Delta R.T.: 0.000 min
Response: 97020770
Conc: 69.75 ug/ml

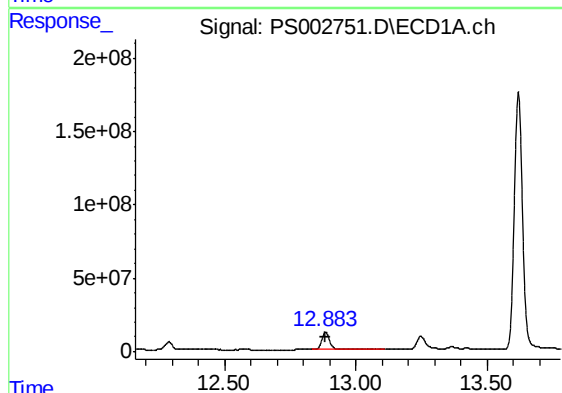


#8 DICHLORPROP

R.T.: 12.884 min
Delta R.T.: 0.000 min
Response: 252530932
Conc: 705.00 ng/ml

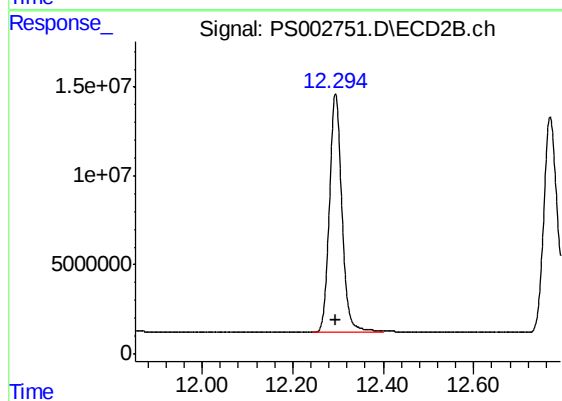

#8 DICHLORPROP


R.T.: 12.295 min
Delta R.T.: 0.000 min
Response: 257625096
Conc: 705.00 ng/ml

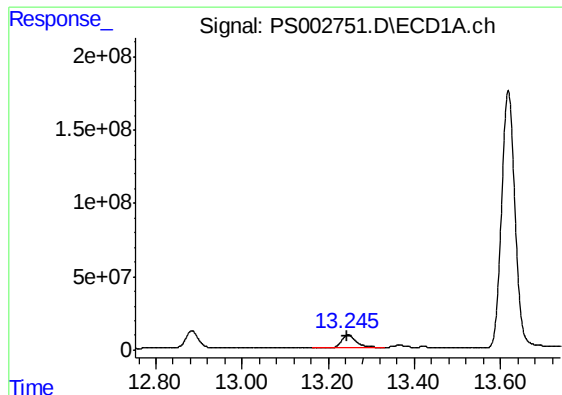

#9 2,4-D


R.T.: 13.246 min
Delta R.T.: 0.000 min
Response: 231521859
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

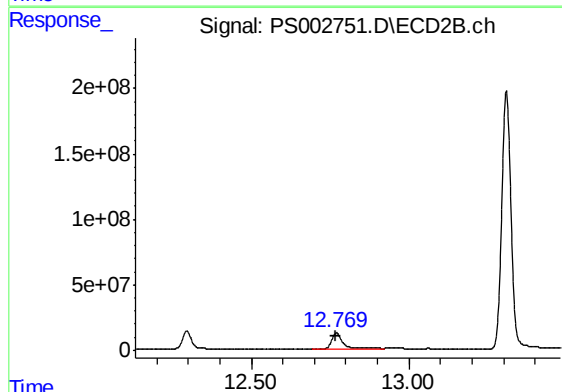


#9 2,4-D

R.T.: 12.769 min
Delta R.T.: 0.000 min
Response: 289904139
Conc: 705.00 ng/ml

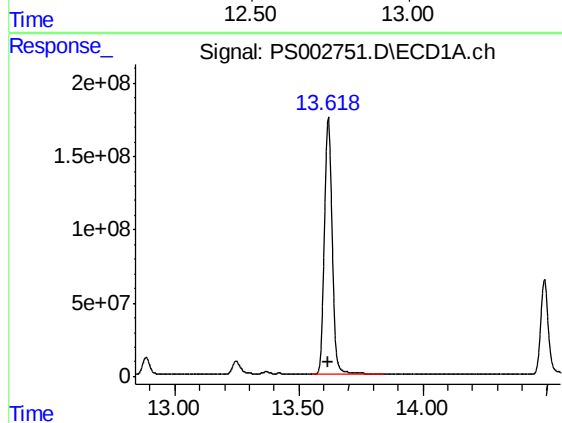


#10 Pentachlorophenol

R.T.: 13.618 min
Delta R.T.: 0.000 min
Response: 3843162220
Conc: 712.50 ng/ml

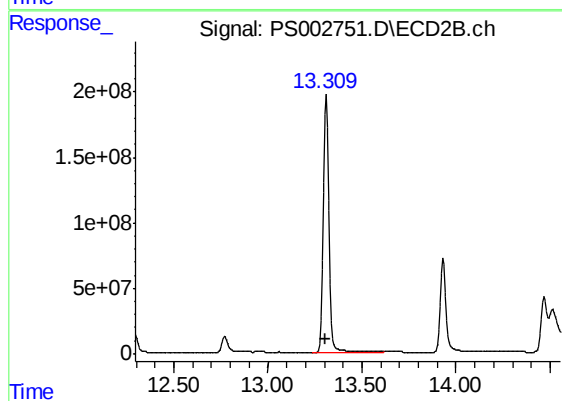

#10 Pentachlorophenol


R.T.: 13.309 min
Delta R.T.: 0.000 min
Response: 4059934822
Conc: 712.50 ng/ml

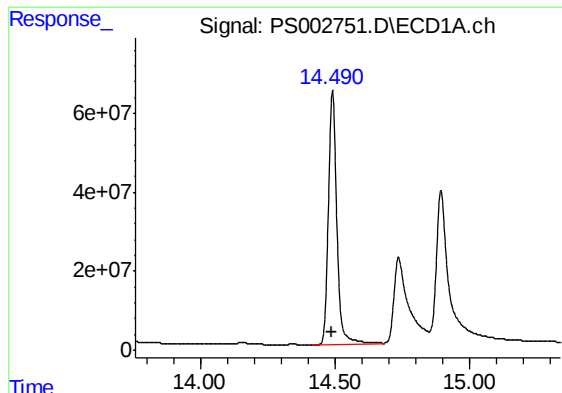

#11 2,4,5-TP (SILVEX)


R.T.: 14.490 min
Delta R.T.: 0.000 min
Response: 1394495774
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

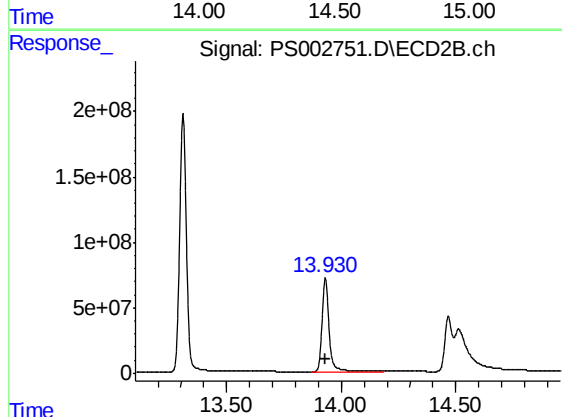


#11 2,4,5-TP (SILVEX)

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 1523248785
Conc: 712.50 ng/ml

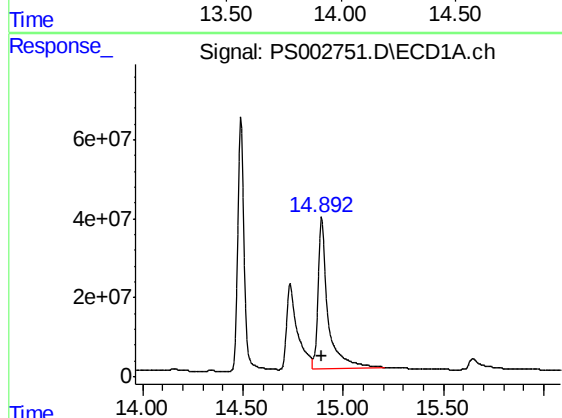


#12 2,4,5-T

R.T.: 14.892 min
Delta R.T.: 0.000 min
Response: 1303278115
Conc: 712.50 ng/ml

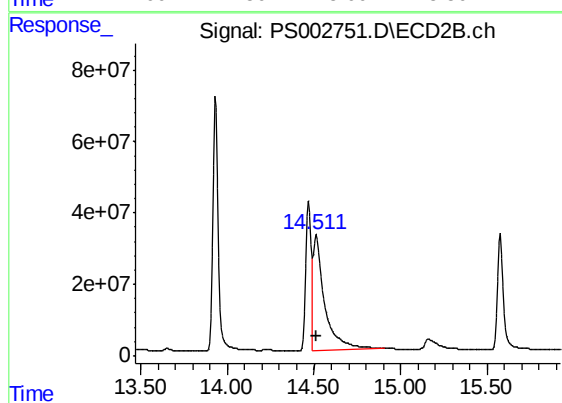

#12 2,4,5-T


R.T.: 14.512 min
Delta R.T.: 0.000 min
Response: 1483508398
Conc: 712.50 ng/ml

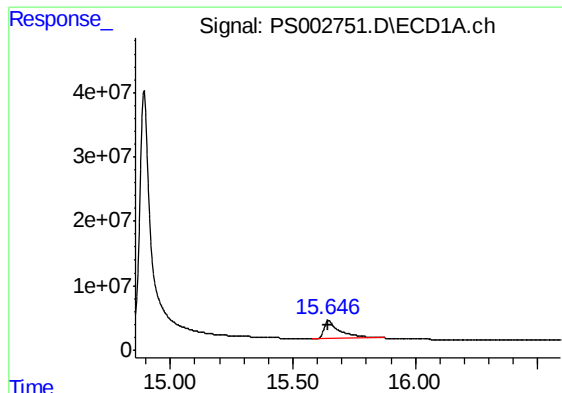

#13 2,4-DB


R.T.: 15.645 min
Delta R.T.: 0.000 min
Response: 128128075
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

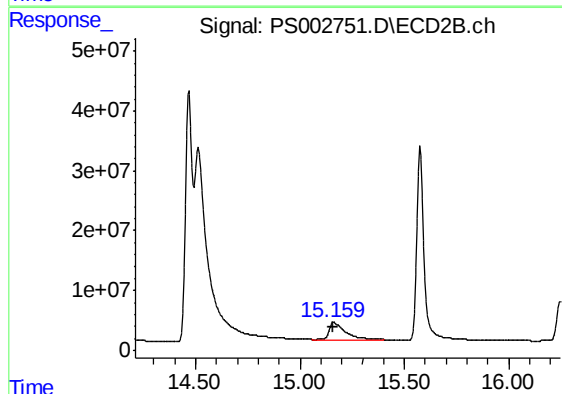


#13 2,4-DB

R.T.: 15.159 min
Delta R.T.: 0.000 min
Response: 149759952
Conc: 712.50 ng/ml

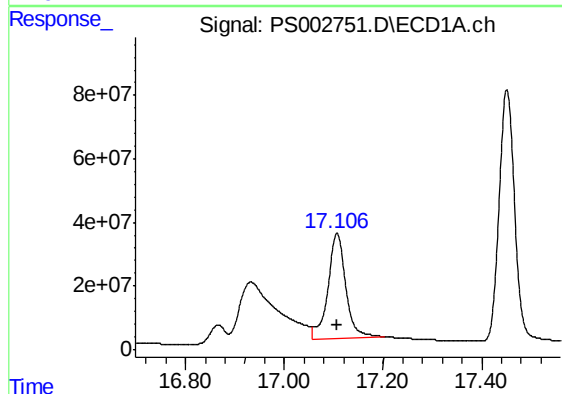


#14 DINOSEB

R.T.: 17.107 min
Delta R.T.: 0.000 min
Response: 828688417
Conc: 705.00 ng/ml

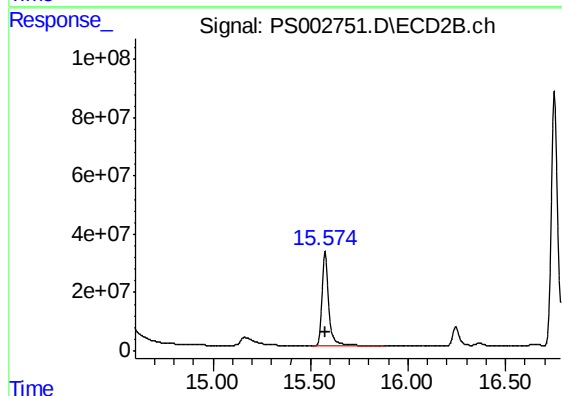

#14 DINOSEB


R.T.: 15.574 min
Delta R.T.: 0.000 min
Response: 767955899
Conc: 705.00 ng/ml

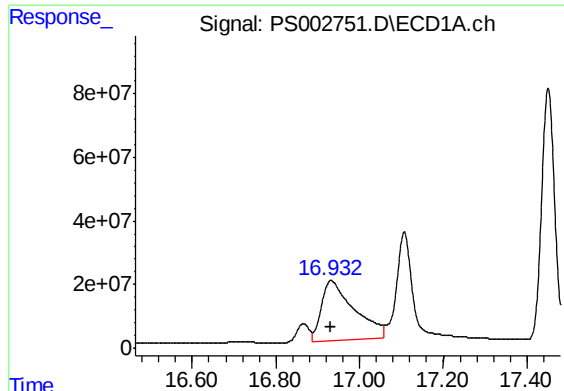

#15 Picloram


R.T.: 16.932 min
Delta R.T.: 0.000 min
Response: 1017897229
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

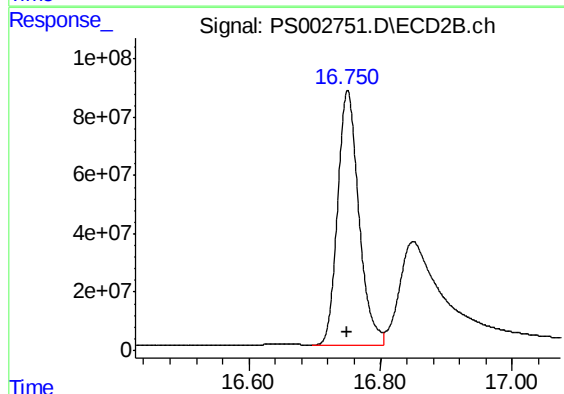


#15 Picloram

R.T.: 16.750 min
Delta R.T.: 0.000 min
Response: 1959164129
Conc: 712.50 ng/ml

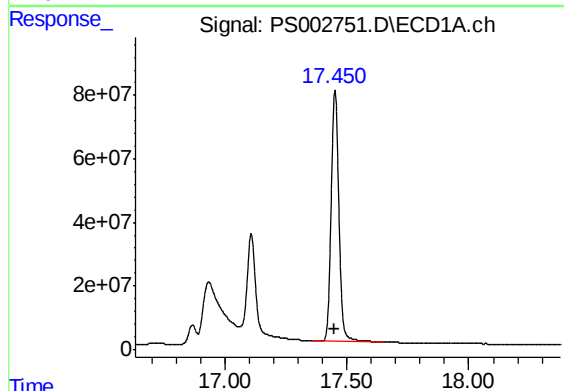

#16 DCPA

R.T.: 17.451 min
Delta R.T.: 0.000 min
Response: 1747930652
Conc: 720.00 ng/ml

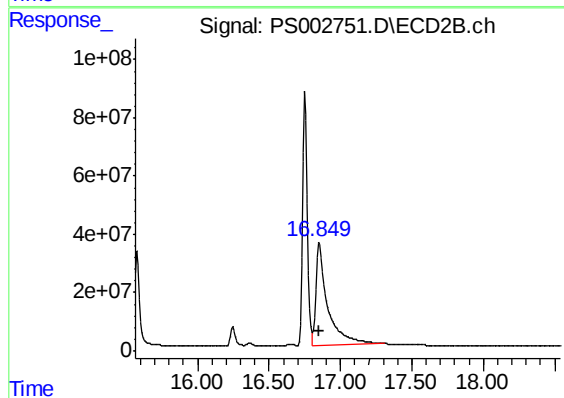

#16 DCPA

R.T.: 16.850 min
Delta R.T.: 0.000 min
Response: 1999458613
Conc: 720.00 ng/ml