

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2021 17:13
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 01:34:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:31:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.208	6.909	703.8E6	295.1E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.029	2.621	731.5E6	346.6E6	682.500	682.500
2) T	3,5-DICHL...	6.425	6.064	909.1E6	432.4E6	697.500	697.500
3) T	4-Nitroph...	7.042	6.523	321.3E6	173.3E6	682.500	682.500
5) T	DICAMBA	7.397	7.076	2689.0E6	1202.2E6	705.000	705.000
6) T	MCPD	7.564	7.170	201.7E6	98292464	70.500	70.500
7) T	MCPA	7.713	7.385	284.6E6	138.1E6	69.750	69.750
8) T	DICHLORPROP	8.088	7.701	667.4E6	307.5E6	705.000	705.000
9) T	2,4-D	8.321	7.999	752.6E6	385.3E6	705.000	705.000
10) T	Pentachlo...	8.626	8.422	9982.0E6	4070.2E6	712.500	712.500
11) T	2,4,5-TP ...	9.175	8.784	3915.9E6	1679.9E6	712.500	712.500
12) T	2,4,5-T	9.463	9.165	3984.8E6	1636.8E6	712.500	712.500
13) T	2,4-DB	10.017	9.672	693.5E6	216.6E6	712.500	712.500
14) T	DINOSEB	11.168	9.999	3017.4E6	1159.2E6	705.000	705.000
15) T	Picloram	11.004	10.995	5267.0E6	2488.4E6	712.500	712.500
16) T	DCPA	11.433	10.925	5001.1E6	2194.0E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2021 17:13
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 01:34:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:31:32 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

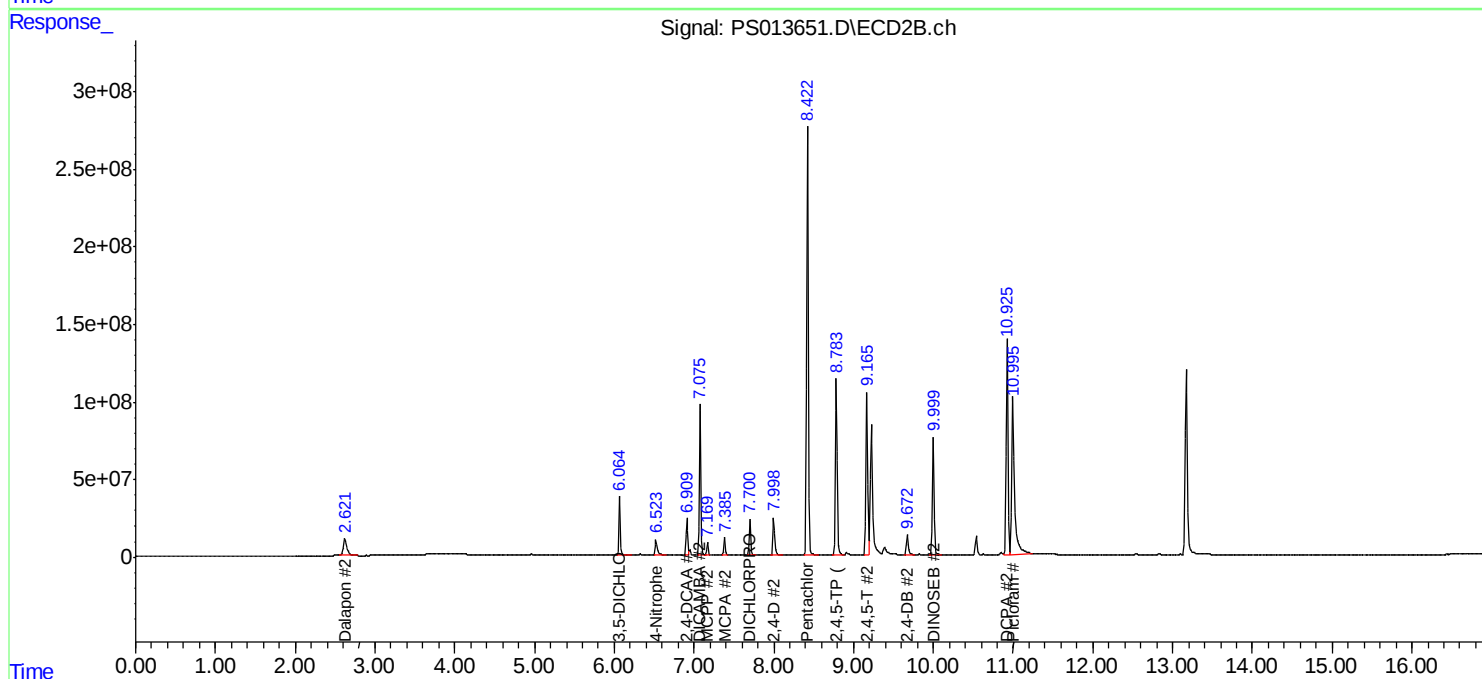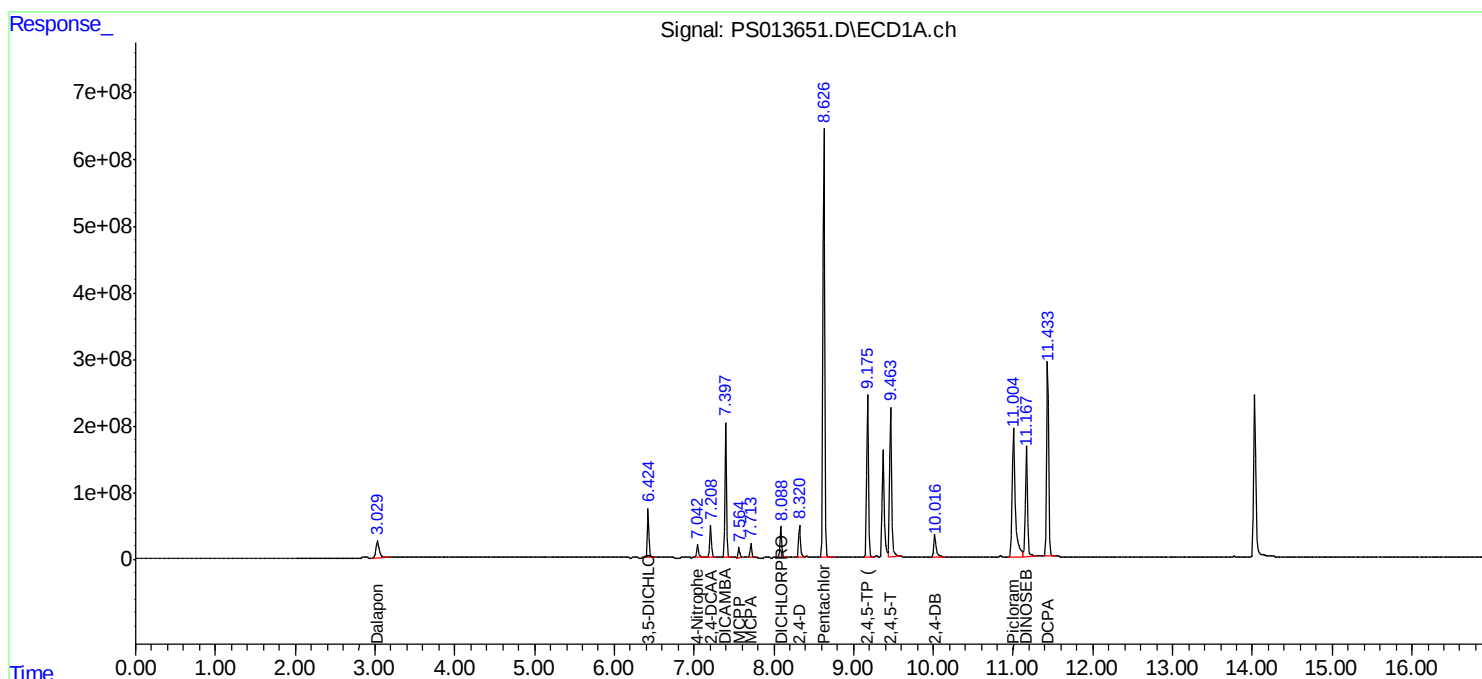


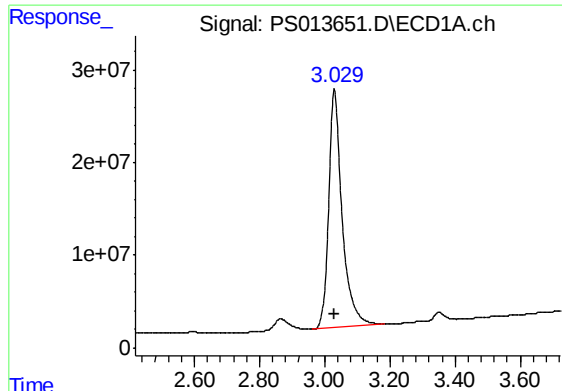

#1 Dalapon


R.T.: 3.029 min
Delta R.T.: 0.000 min
Response: 731528263
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

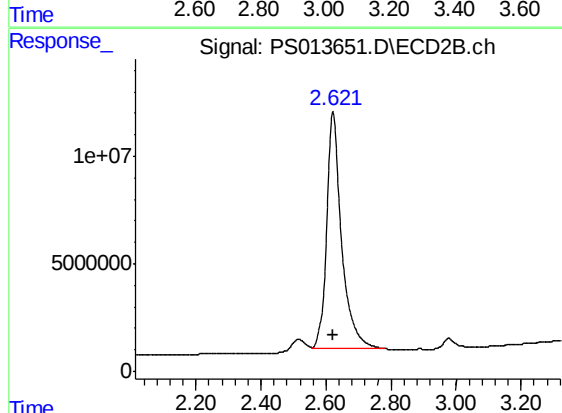


#1 Dalapon

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 346555823
Conc: 682.50 ng/ml

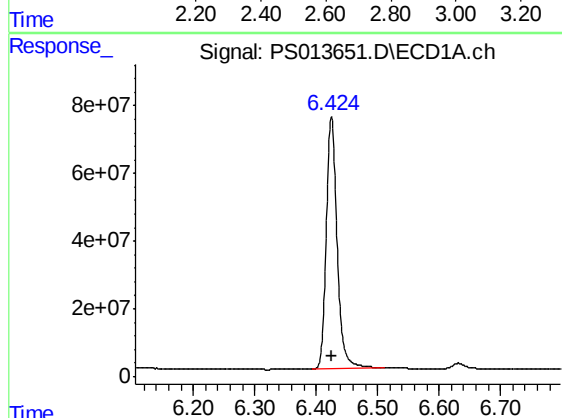


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.425 min
Delta R.T.: 0.000 min
Response: 909140588
Conc: 697.50 ng/ml

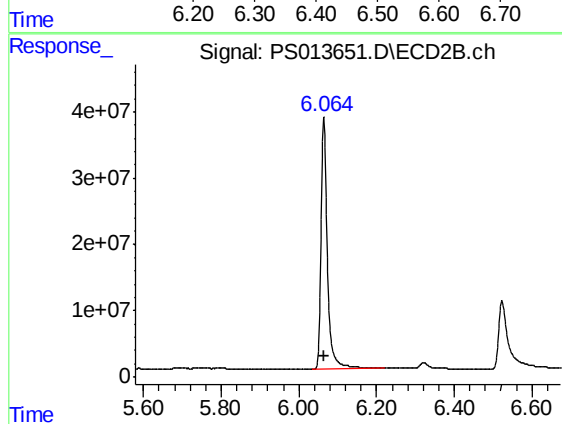

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 432390084
Conc: 697.50 ng/ml

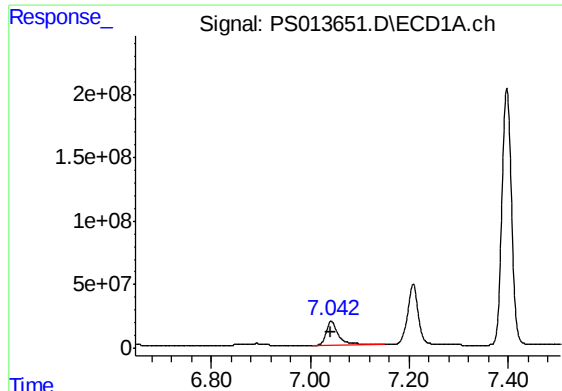

#3 4-Nitrophenol


R.T.: 7.042 min
Delta R.T.: 0.000 min
Response: 321277879
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

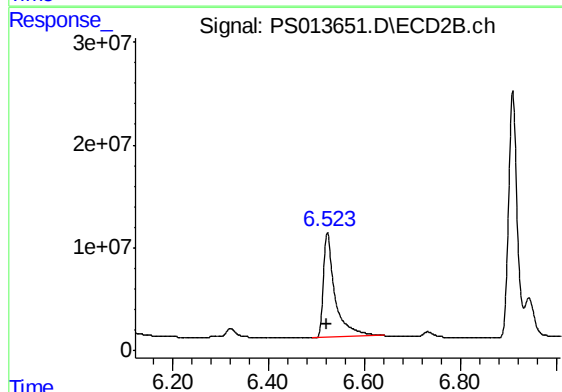


#3 4-Nitrophenol

R.T.: 6.523 min
Delta R.T.: 0.000 min
Response: 173344524
Conc: 682.50 ng/ml

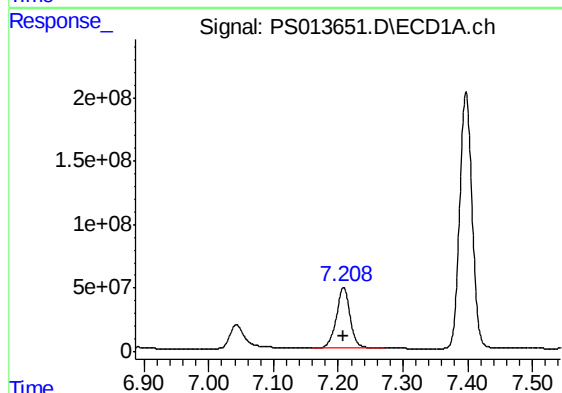


#4 2,4-DCAA

R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 703753418
Conc: 750.00 ng/ml

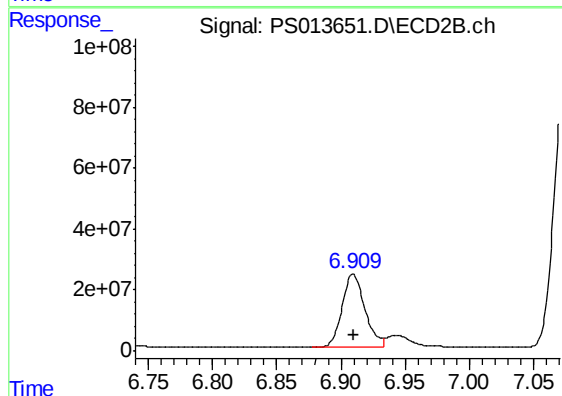

#4 2,4-DCAA


R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 295110786
Conc: 750.00 ng/ml

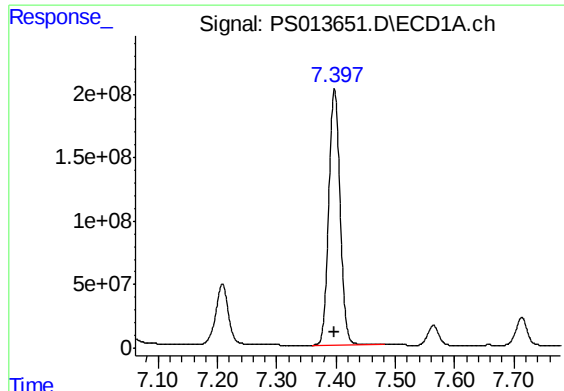

#5 DICAMBA


R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 2688990213
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

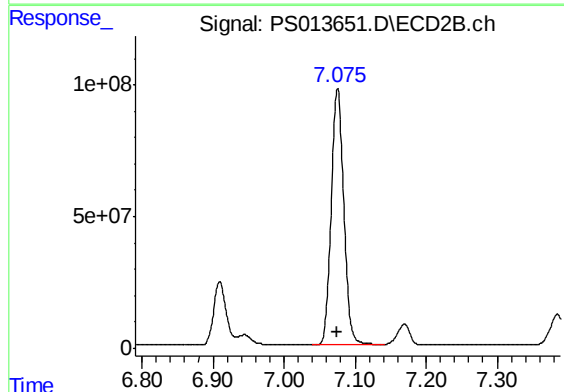


#5 DICAMBA

R.T.: 7.076 min
Delta R.T.: 0.000 min
Response: 1202186524
Conc: 705.00 ng/ml

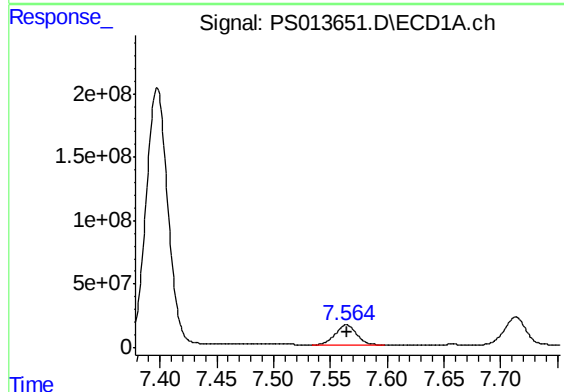


#6 MCPP

R.T.: 7.564 min
Delta R.T.: 0.000 min
Response: 201679566
Conc: 70.50 ug/ml

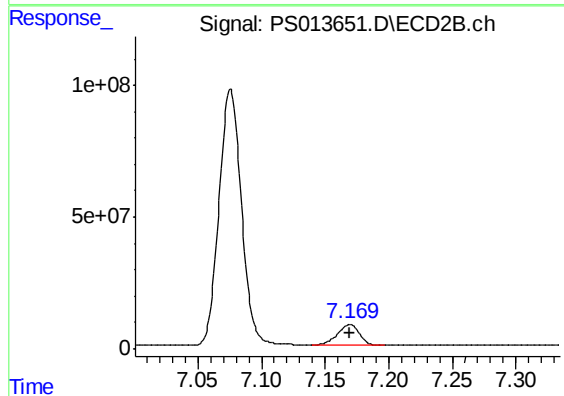

#6 MCPP


R.T.: 7.170 min
Delta R.T.: 0.000 min
Response: 98292464
Conc: 70.50 ug/ml

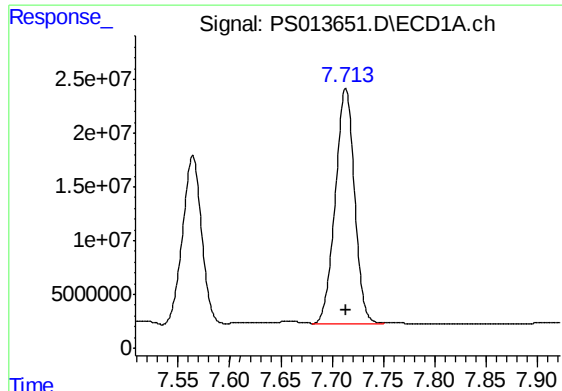

#7 MCPA


R.T.: 7.713 min
Delta R.T.: 0.000 min
Response: 284631970
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

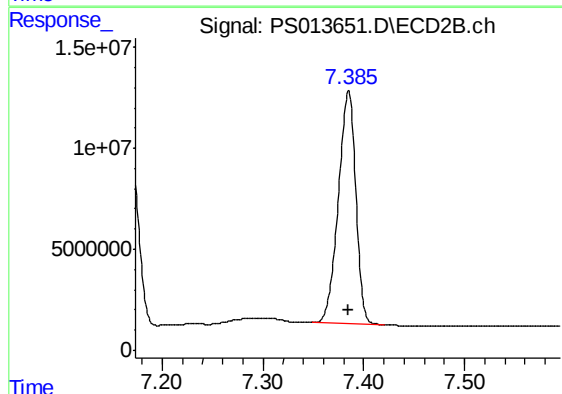


#7 MCPA

R.T.: 7.385 min
Delta R.T.: 0.000 min
Response: 138106655
Conc: 69.75 ug/ml

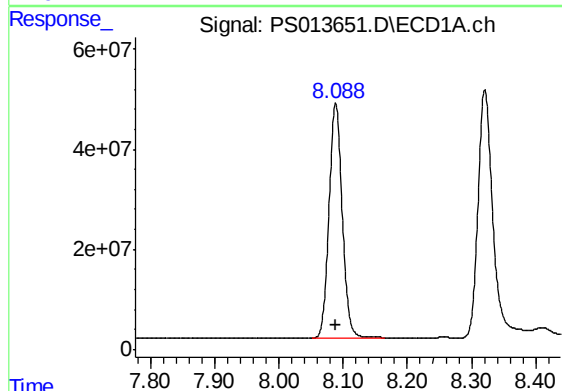


#8 DICHLORPROP

R.T.: 8.088 min
Delta R.T.: 0.000 min
Response: 667433787
Conc: 705.00 ng/ml

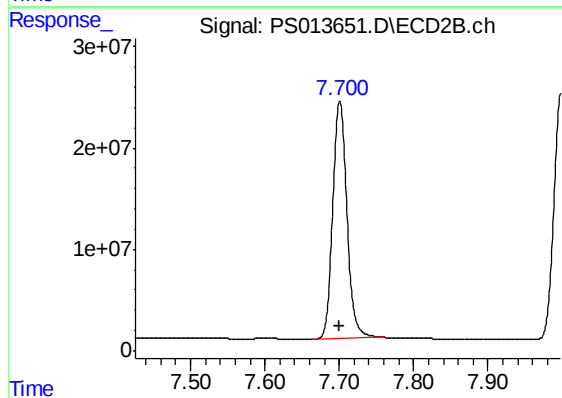

#8 DICHLORPROP


R.T.: 7.701 min
Delta R.T.: 0.000 min
Response: 307486037
Conc: 705.00 ng/ml

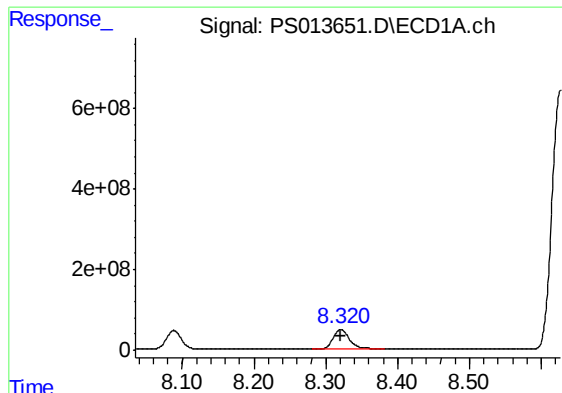

#9 2,4-D


R.T.: 8.321 min
Delta R.T.: 0.000 min
Response: 752553388
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

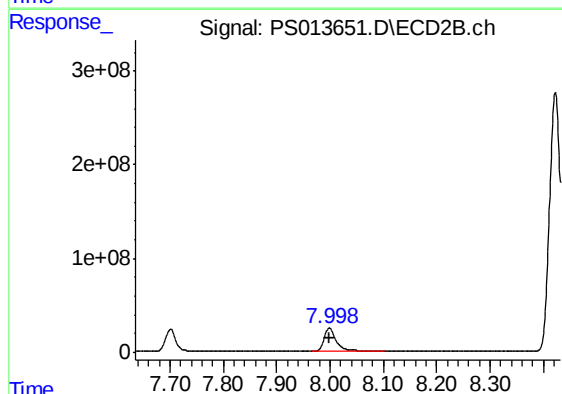


#9 2,4-D

R.T.: 7.999 min
Delta R.T.: 0.000 min
Response: 385267072
Conc: 705.00 ng/ml

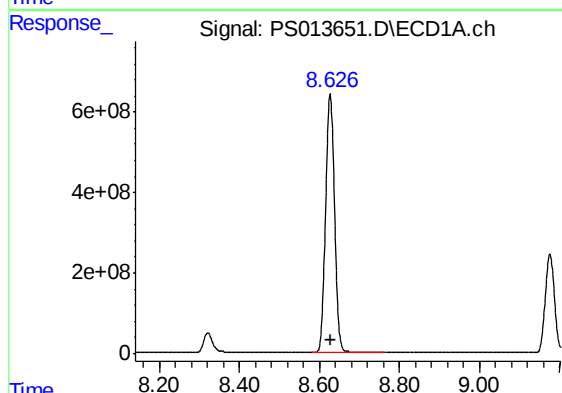


#10 Pentachlorophenol

R.T.: 8.626 min
Delta R.T.: 0.000 min
Response: 9982047249
Conc: 712.50 ng/ml

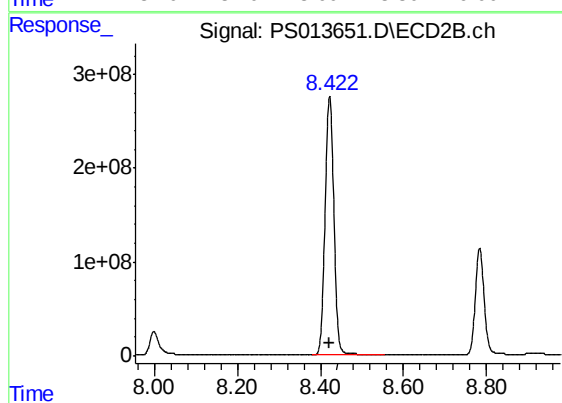

#10 Pentachlorophenol


R.T.: 8.422 min
Delta R.T.: 0.000 min
Response: 4070172017
Conc: 712.50 ng/ml

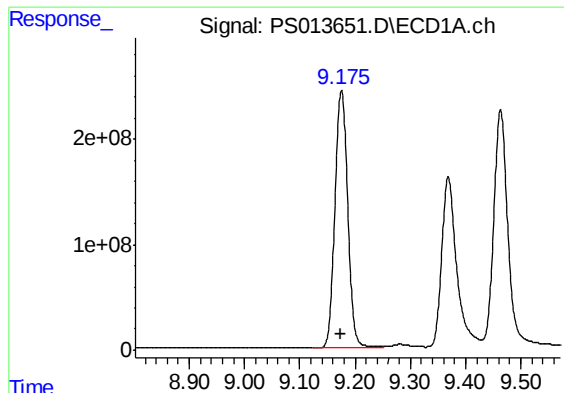

#11 2,4,5-TP (SILVEX)


R.T.: 9.175 min
Delta R.T.: 0.000 min
Response: 3915894028
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

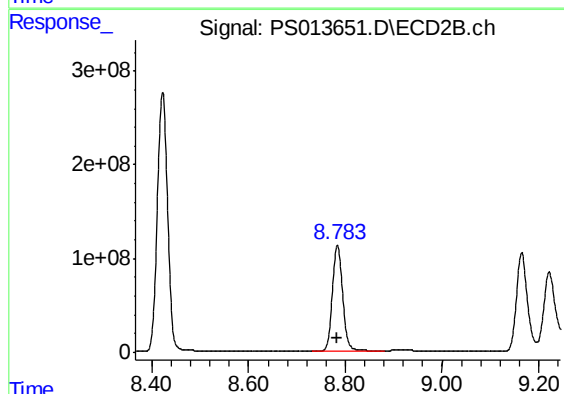


#11 2,4,5-TP (SILVEX)

R.T.: 8.784 min
Delta R.T.: 0.000 min
Response: 1679898233
Conc: 712.50 ng/ml

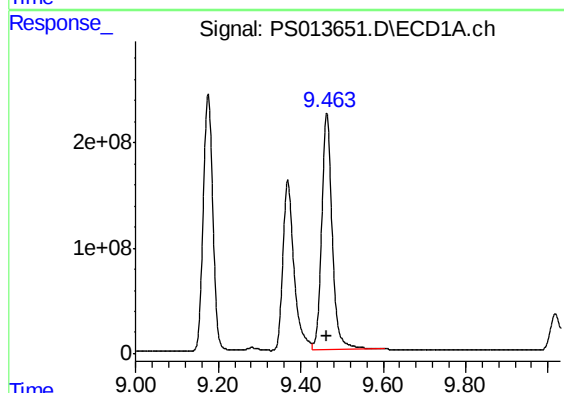


#12 2,4,5-T

R.T.: 9.463 min
Delta R.T.: 0.000 min
Response: 3984840739
Conc: 712.50 ng/ml

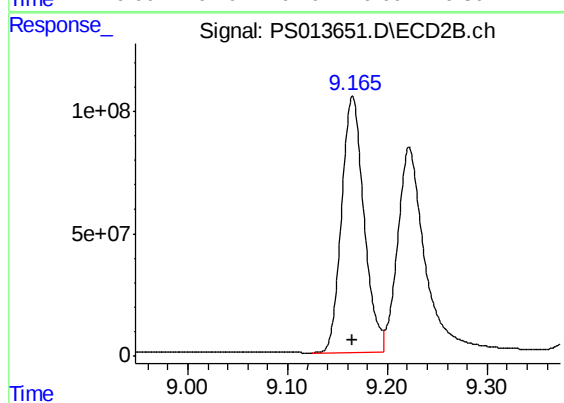

#12 2,4,5-T


R.T.: 9.165 min
Delta R.T.: 0.000 min
Response: 1636846252
Conc: 712.50 ng/ml

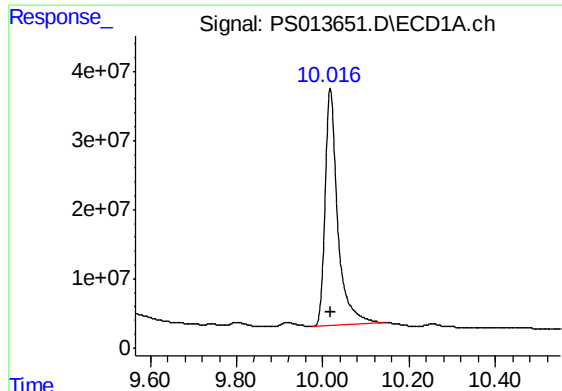

#13 2,4-DB


R.T.: 10.017 min
Delta R.T.: 0.000 min
Response: 693516486
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

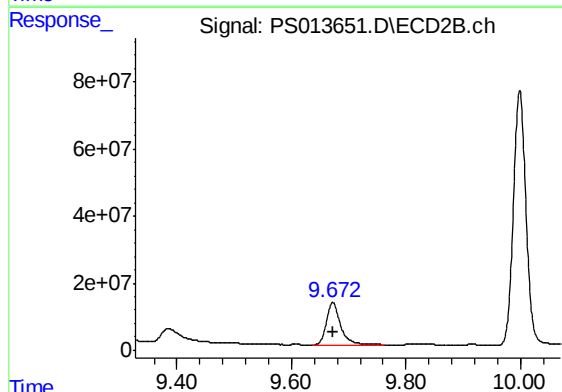


#13 2,4-DB

R.T.: 9.672 min
Delta R.T.: 0.000 min
Response: 216574803
Conc: 712.50 ng/ml

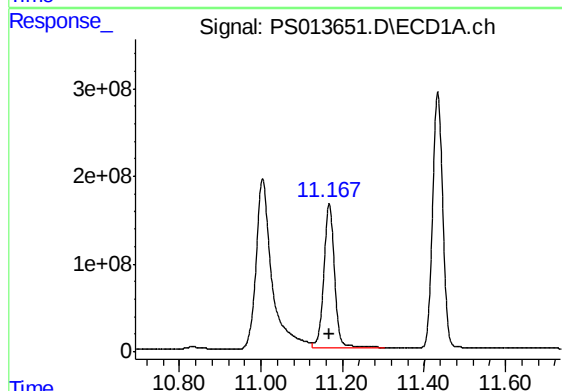


#14 DINOSEB

R.T.: 11.168 min
Delta R.T.: 0.000 min
Response: 3017355708
Conc: 705.00 ng/ml

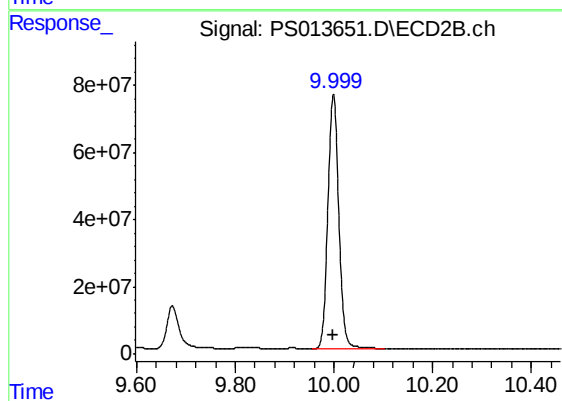

#14 DINOSEB


R.T.: 9.999 min
Delta R.T.: 0.000 min
Response: 1159236843
Conc: 705.00 ng/ml

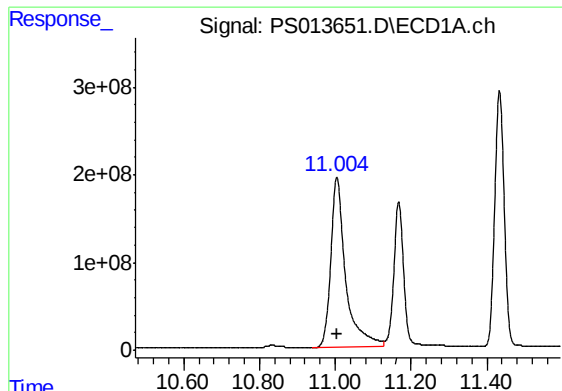

#15 Picloram


R.T.: 11.004 min
Delta R.T.: 0.000 min
Response: 5267014409
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

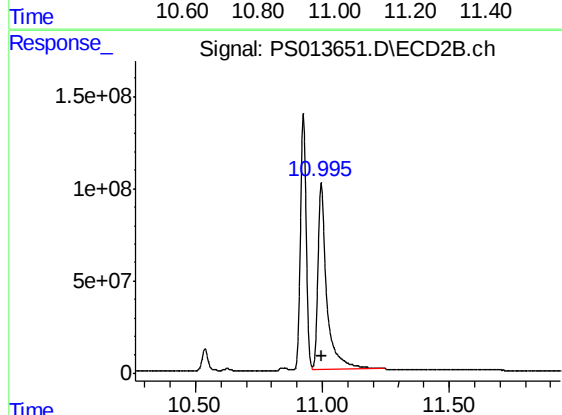


#15 Picloram

R.T.: 10.995 min
Delta R.T.: 0.000 min
Response: 2488397862
Conc: 712.50 ng/ml

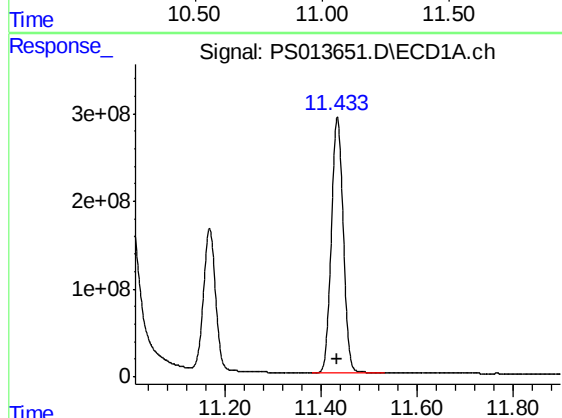

#16 DCPA

R.T.: 11.433 min
Delta R.T.: 0.000 min
Response: 5001085548
Conc: 720.00 ng/ml

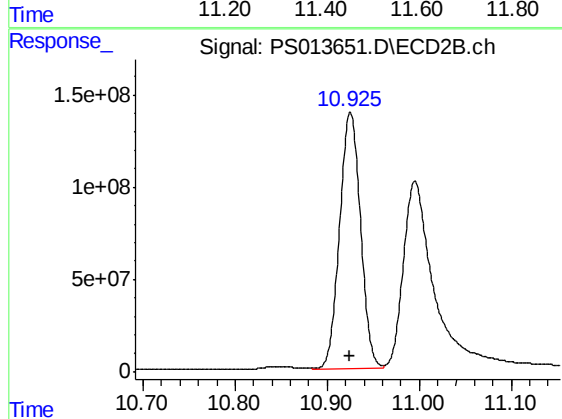

#16 DCPA

R.T.: 10.925 min
Delta R.T.: 0.000 min
Response: 2193974653
Conc: 720.00 ng/ml