

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2021 18:45
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:29:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.213	6.914	371.9E6	208.2E6	389.194	517.819 #
Target Compounds							
5) T	DICAMBA	0.000	7.080	0	2915490	N.D.	1.698
10) T	Pentachlo...	8.637	8.436	9286180	4641801	<MDL	<MDL #
12) T	2,4,5-T	9.447	0.000	36506937	0	6.456	N.D. #
15) T	Picloram	0.000	10.937f	0	4624323	N.D.	1.331
16) T	DCPA	11.442	10.937	8751575	4624323	1.239	1.494



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2021 18:45
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:29:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

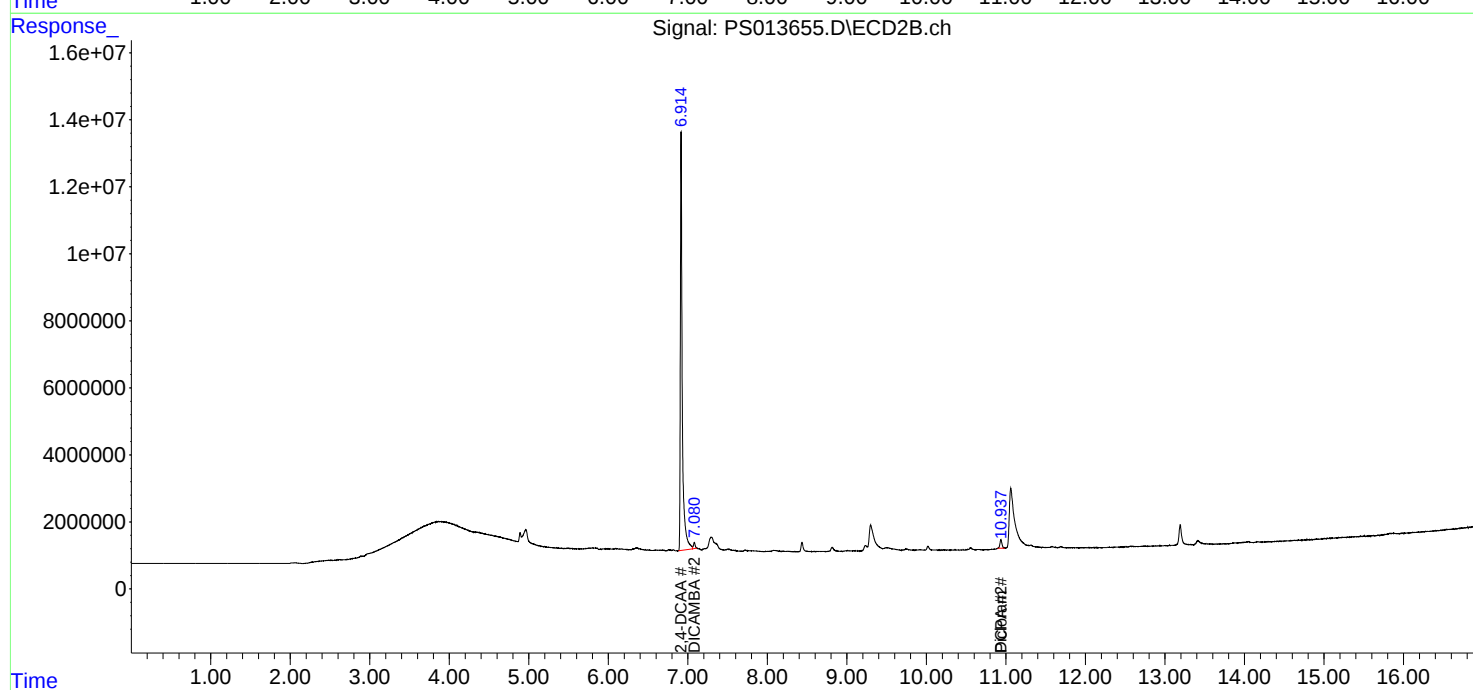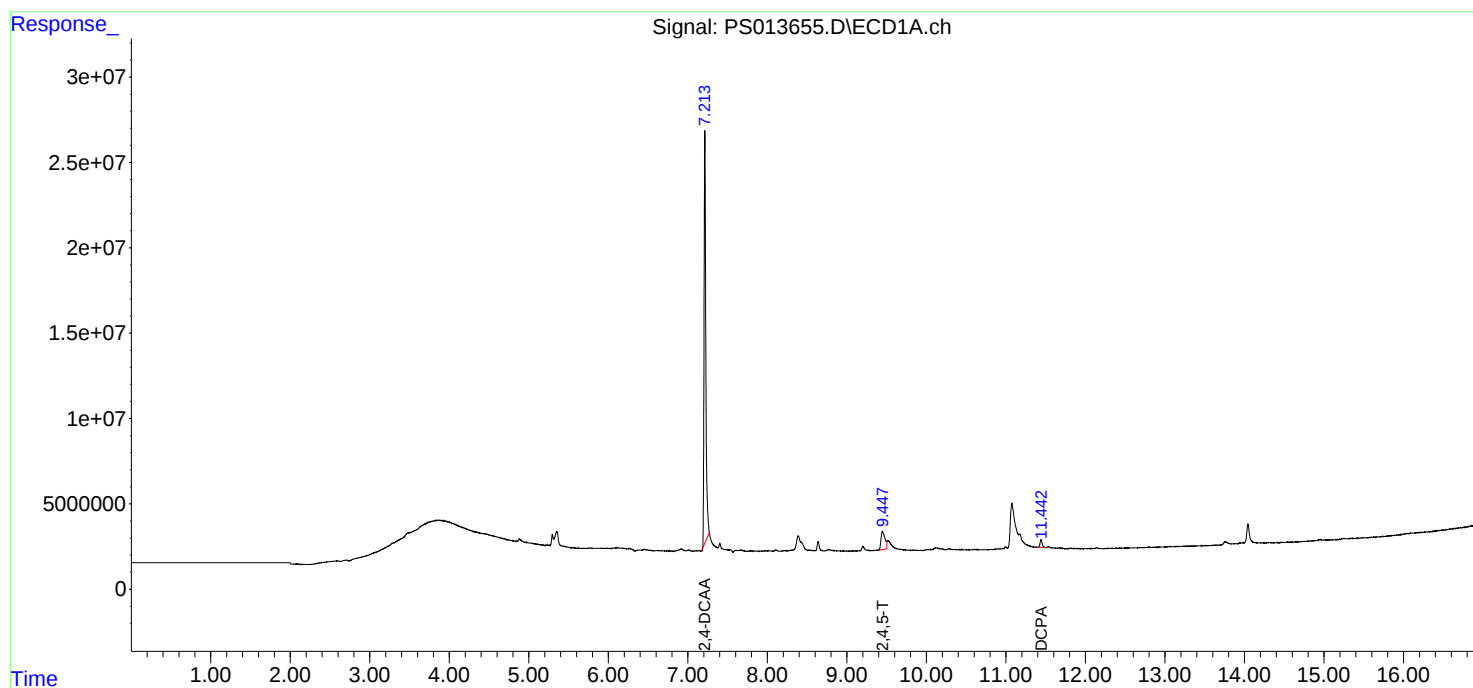


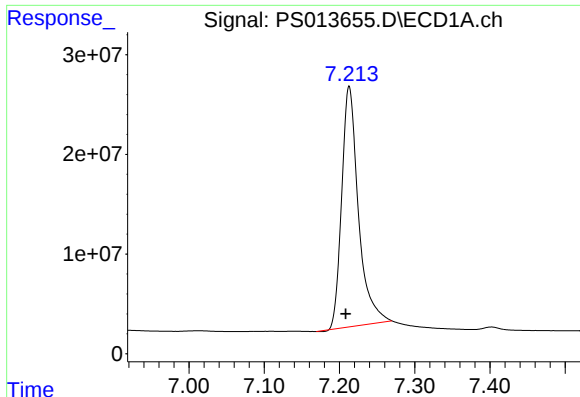

#4 2,4-DCAA


R.T.: 7.213 min
Delta R.T.: 0.005 min
Response: 371911236
Conc: 389.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

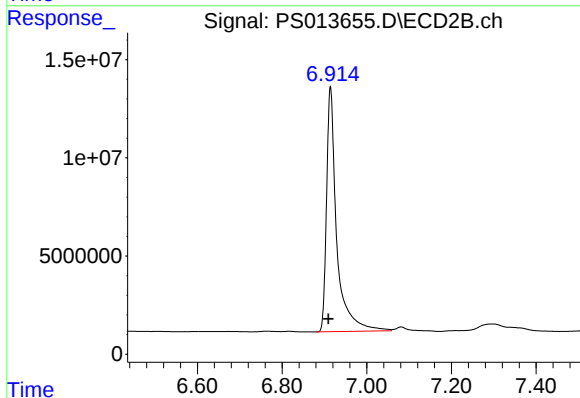


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.005 min
Response: 208222580
Conc: 517.82 ng/ml

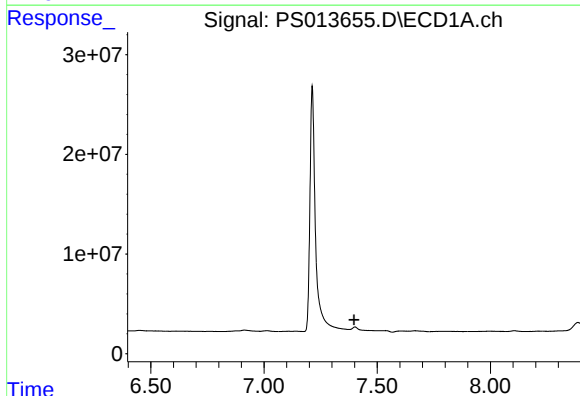


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.397 min
Response: 0
Conc: N.D.

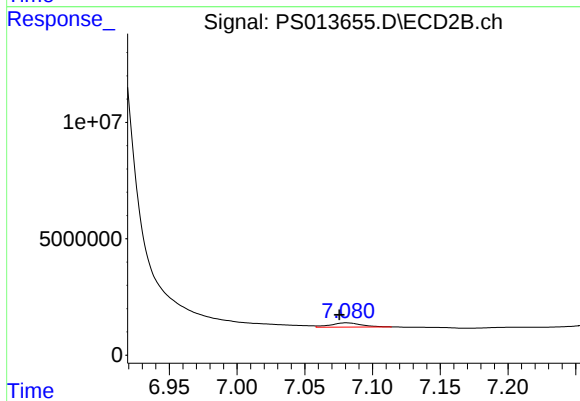

#5 DICAMBA


R.T.: 7.080 min
Delta R.T.: 0.005 min
Response: 2915490
Conc: 1.70 ng/ml

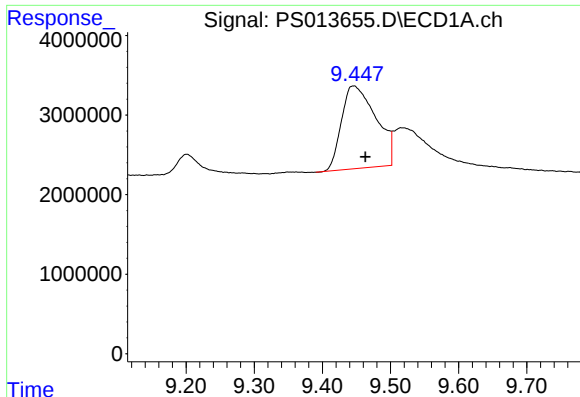

#12 2,4,5-T


R.T.: 9.447 min
Delta R.T.: -0.016 min
Response: 36506937
Conc: 6.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

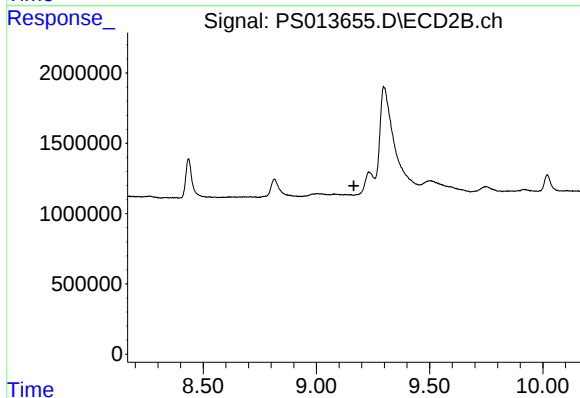


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.165 min
Response: 0
Conc: N.D.

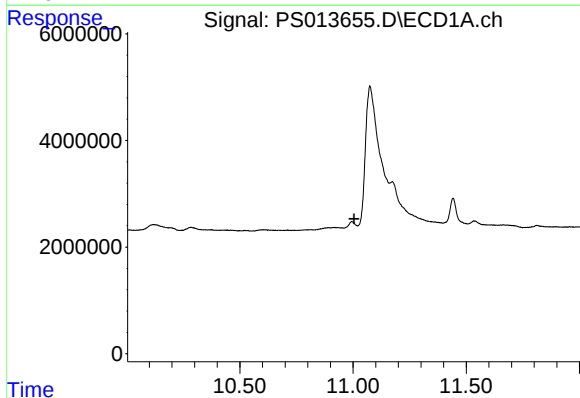


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.004 min
Response: 0
Conc: N.D.

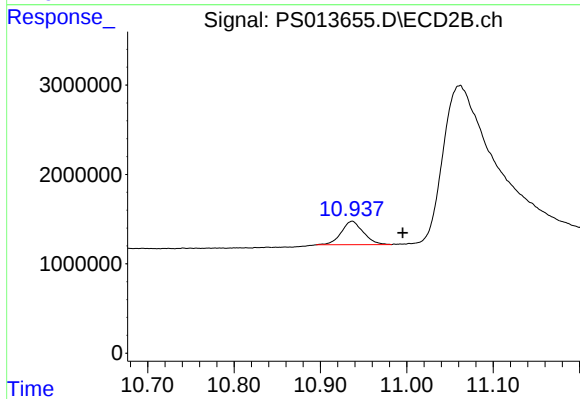

#15 Picloram


R.T.: 10.937 min
Delta R.T.: -0.058 min
Response: 4624323
Conc: 1.33 ng/ml

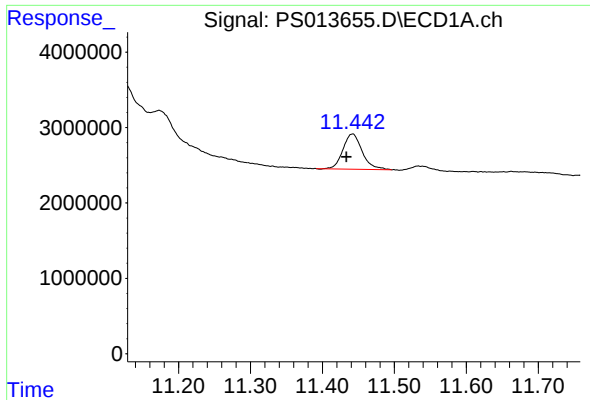

#16 DCPA

R.T.: 11.442 min
Delta R.T.: 0.009 min
Response: 8751575
Conc: 1.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

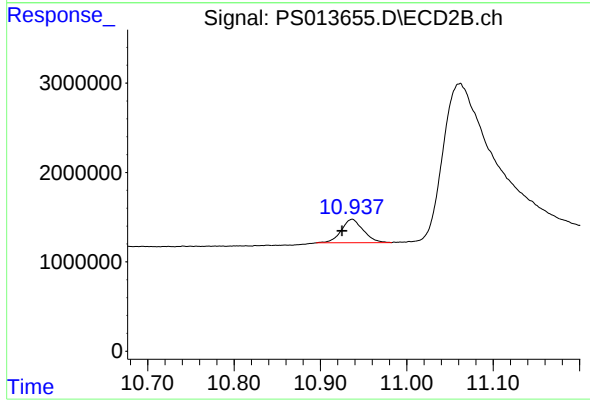

#16 DCPA

R.T.: 10.937 min
Delta R.T.: 0.012 min
Response: 4624323
Conc: 1.49 ng/ml