

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2021 19:31
 Operator : DD\AJ
 Sample : PB133887BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:30:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.210	6.911	490.6E6	239.0E6	513.369	594.390
Target Compounds							
1) T	Dalapon	2.985f	2.588	70602671	180.8E6	64.915	347.635 #
2) T	3,5-DICHL...	0.000	6.094	0	20774082	N.D.	32.975
3) T	4-Nitroph...	6.983f	0.000	5422698	0	11.406	N.D. #
5) T	DICAMBA	0.000	7.045	0	1543744	N.D.	<MDL
7) T	MCPA	0.000	7.368	0	24177155	N.D.	11.959
10) T	Pentachlo...	8.631	8.426	6598189	6097427	<MDL	1.055 #
11) T	2,4,5-TP ...	0.000	8.759	0	14771483	N.D.	6.184
12) T	2,4,5-T	9.481	0.000	12022638	0	2.126	N.D. #
13) T	2,4-DB	9.980	0.000	5207611	0	5.329	N.D. #
14) T	DINOSEB	11.140	10.013	41769570	5457206	9.468	3.261 #
15) T	Picloram	10.983	11.025	7488018	137.9E6	1.037	39.688 #
16) T	DCPA	11.438	10.927	1302351	8783365	<MDL	2.838 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2021 19:31
Operator : DD\AJ
Sample : PB133887BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:30:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

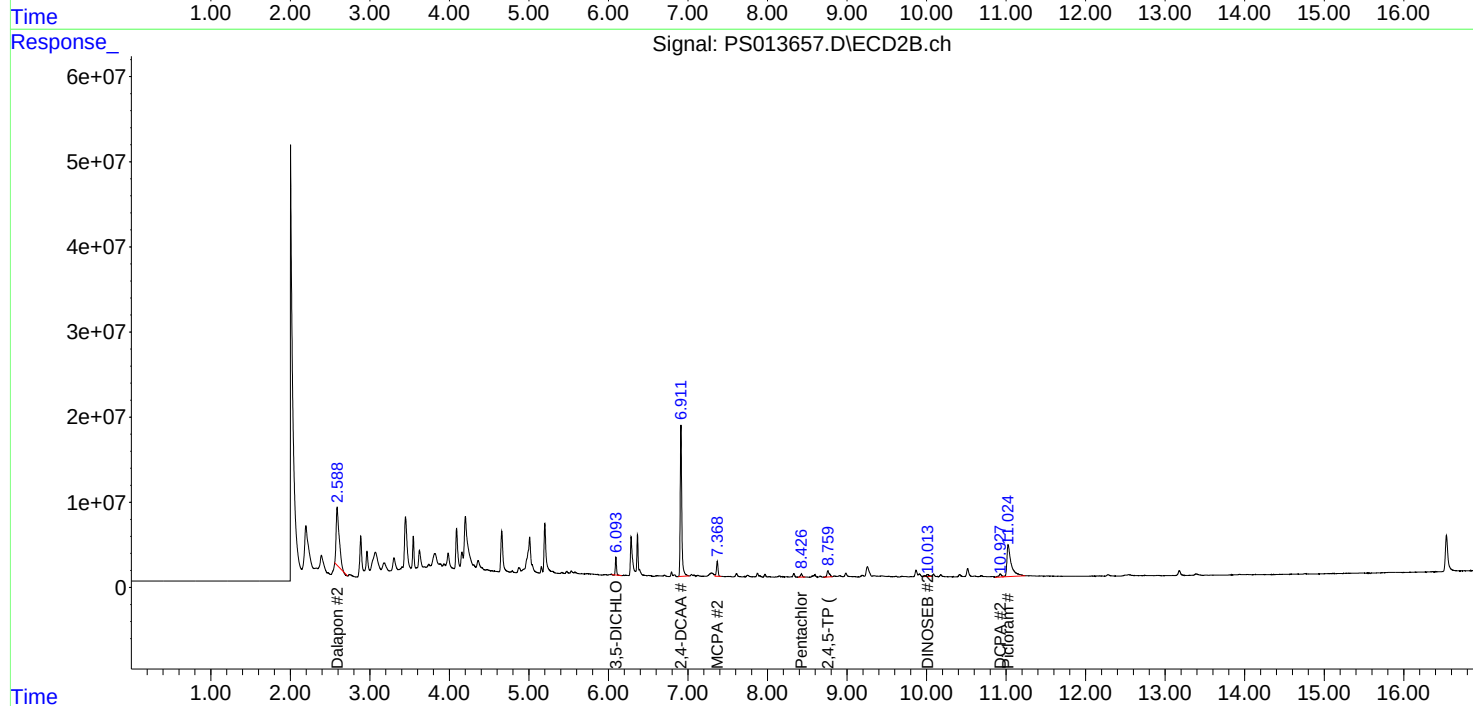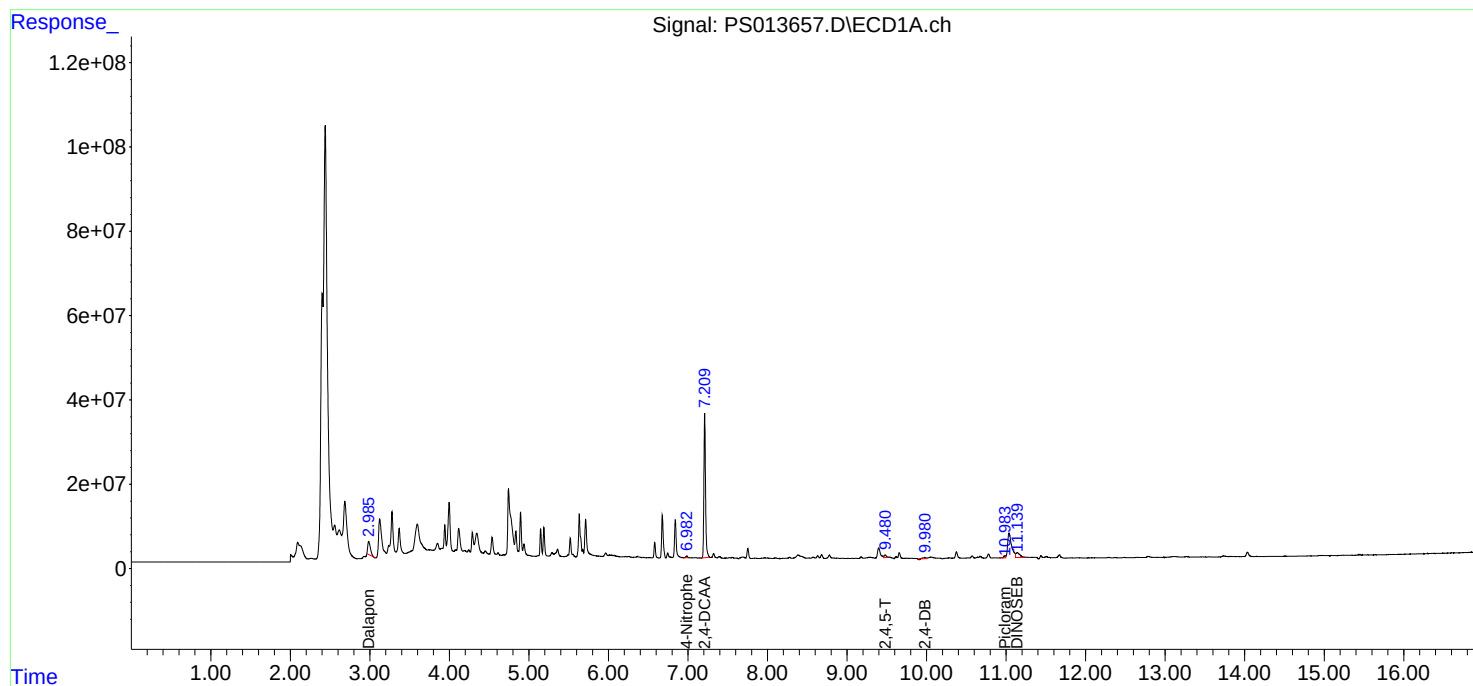


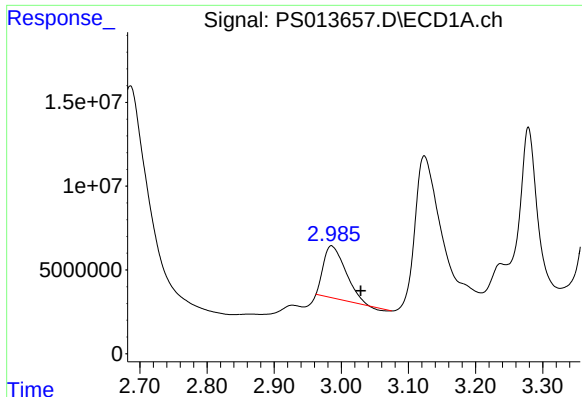

#1 Dalapon


R.T.: 2.985 min
Delta R.T.: -0.044 min
Response: 70602671
Conc: 64.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

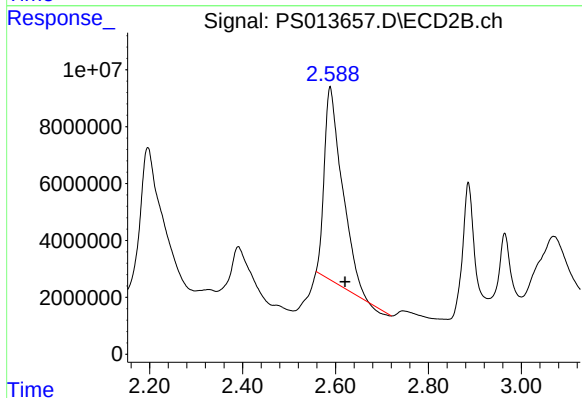


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.032 min
Response: 180752380
Conc: 347.63 ng/ml

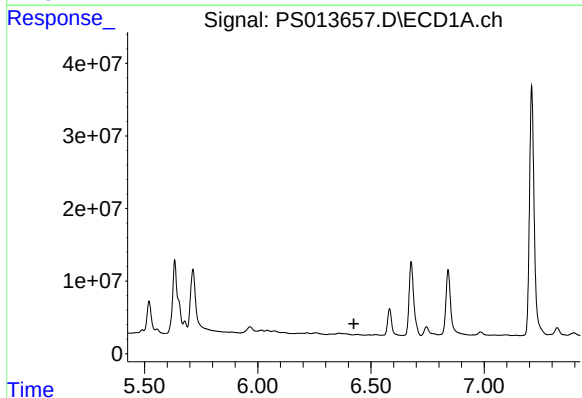


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

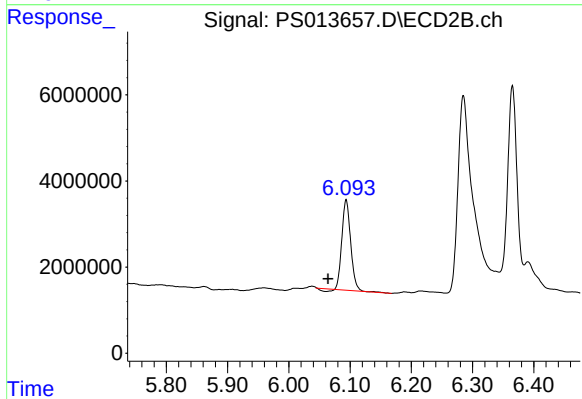

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 20774082
Conc: 32.97 ng/ml

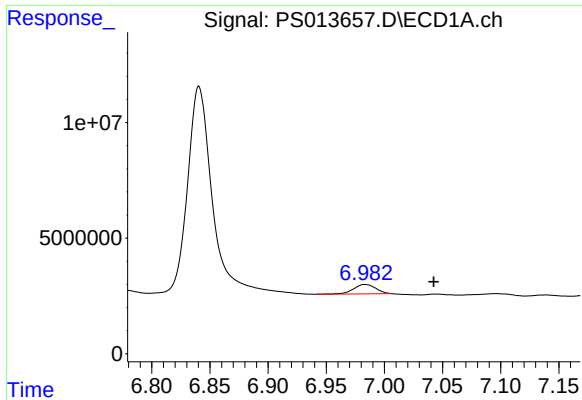

#3 4-Nitrophenol


R.T.: 6.983 min
Delta R.T.: -0.059 min
Response: 5422698
Conc: 11.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

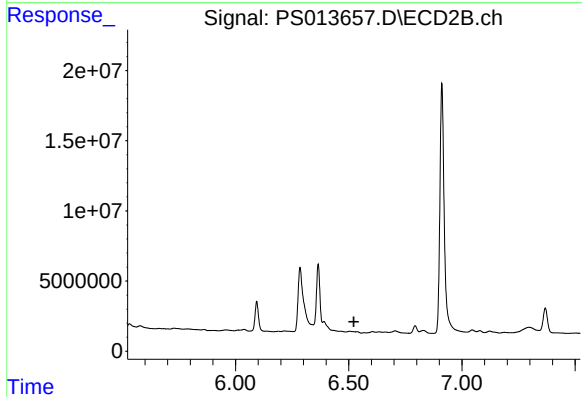


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.523 min
Response: 0
Conc: N.D.

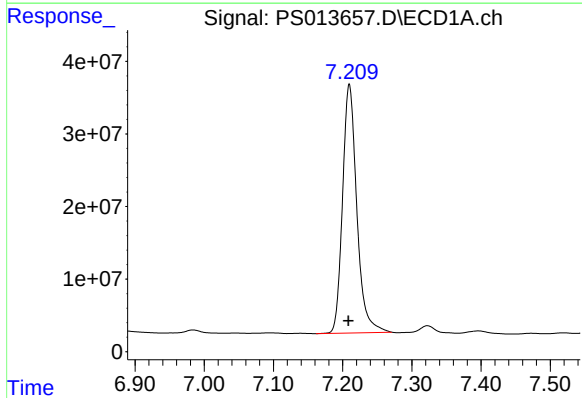


#4 2,4-DCAA

R.T.: 7.210 min
Delta R.T.: 0.001 min
Response: 490571429
Conc: 513.37 ng/ml



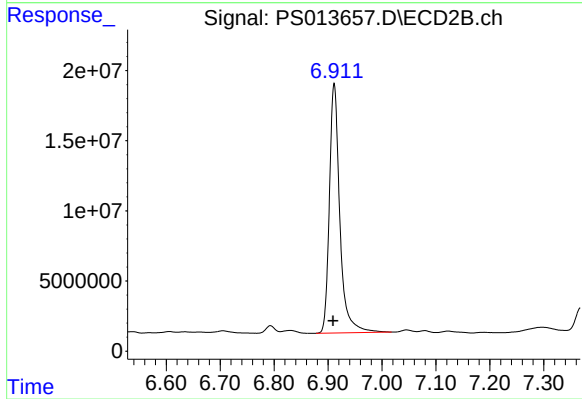



#4 2,4-DCAA

R.T.: 6.911 min
Delta R.T.: 0.002 min
Response: 239013238
Conc: 594.39 ng/ml

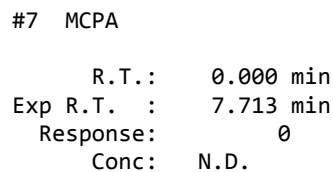

Instrument :
ECD_S
ClientSampleId :

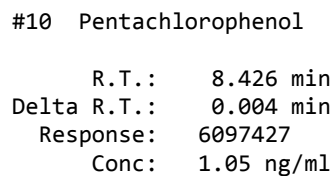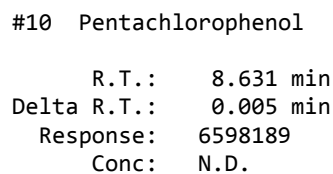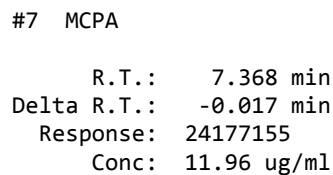


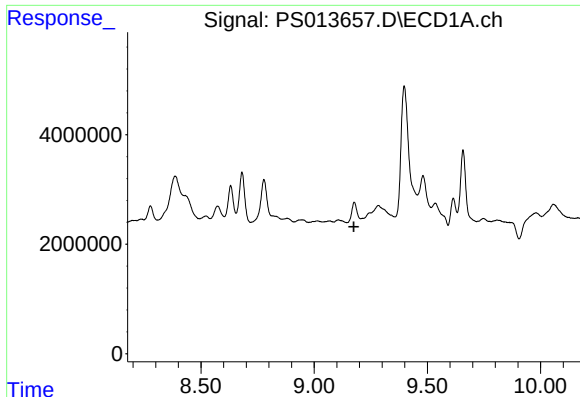

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

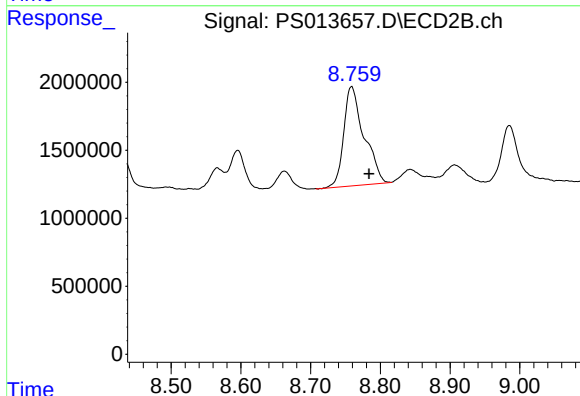


#11 2,4,5-TP (SILVEX)

R.T.: 8.759 min
Delta R.T.: -0.025 min
Response: 14771483
Conc: 6.18 ng/ml

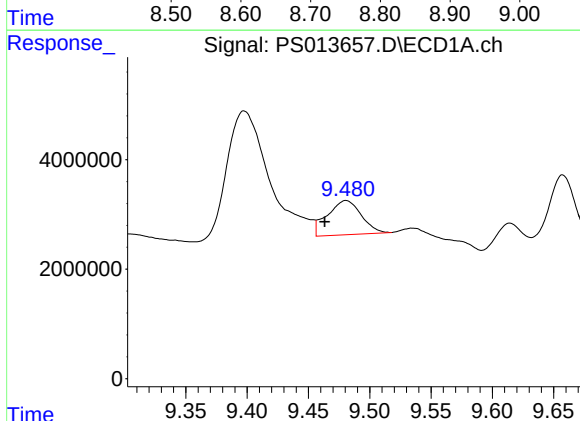


#12 2,4,5-T

R.T.: 9.481 min
Delta R.T.: 0.017 min
Response: 12022638
Conc: 2.13 ng/ml

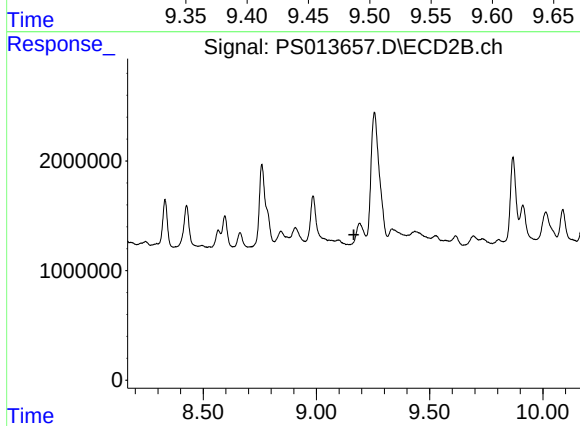

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.165 min
Response: 0
Conc: N.D.

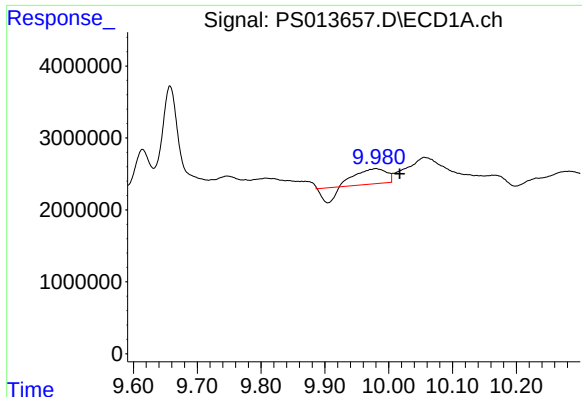

#13 2,4-DB


R.T.: 9.980 min
Delta R.T.: -0.037 min
Response: 5207611
Conc: 5.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

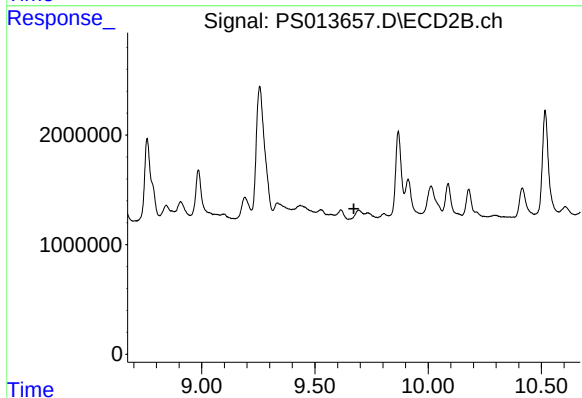


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

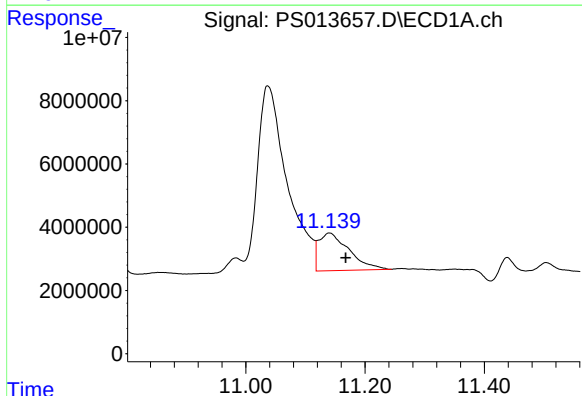


#14 DINOSEB

R.T.: 11.140 min
Delta R.T.: -0.027 min
Response: 41769570
Conc: 9.47 ng/ml

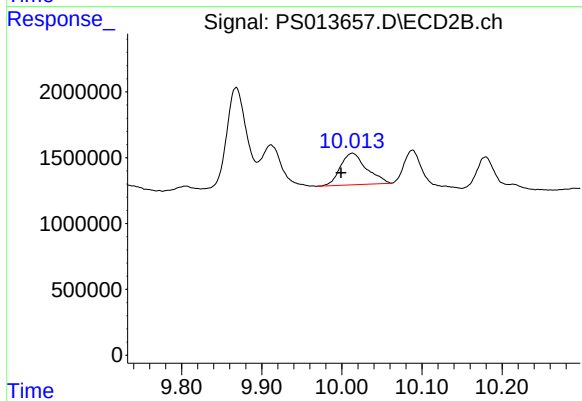

#14 DINOSEB


R.T.: 10.013 min
Delta R.T.: 0.014 min
Response: 5457206
Conc: 3.26 ng/ml

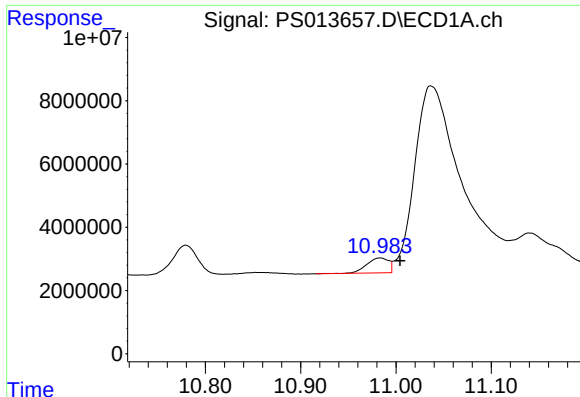

#15 Picloram


R.T.: 10.983 min
Delta R.T.: -0.021 min
Response: 7488018
Conc: 1.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

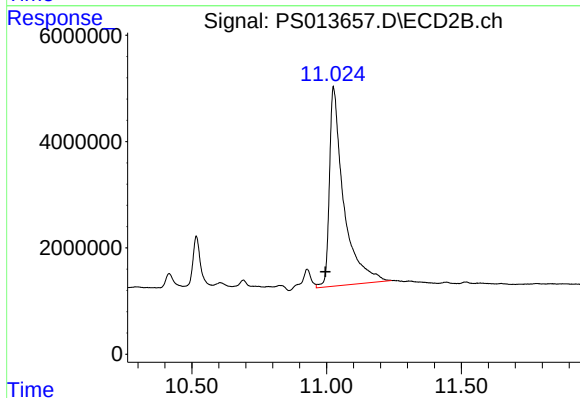


#15 Picloram

R.T.: 11.025 min
Delta R.T.: 0.030 min
Response: 137937793
Conc: 39.69 ng/ml

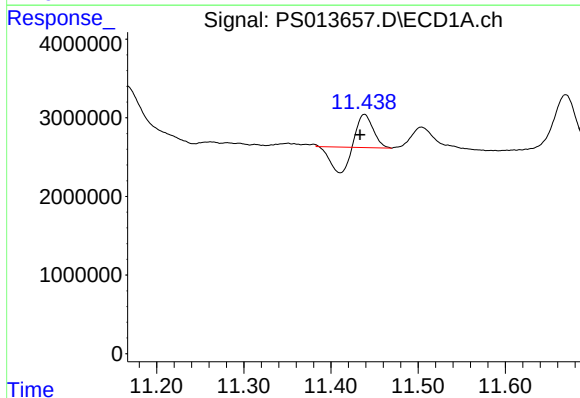

#16 DCPA

R.T.: 11.438 min
Delta R.T.: 0.005 min
Response: 1302351
Conc: N.D.

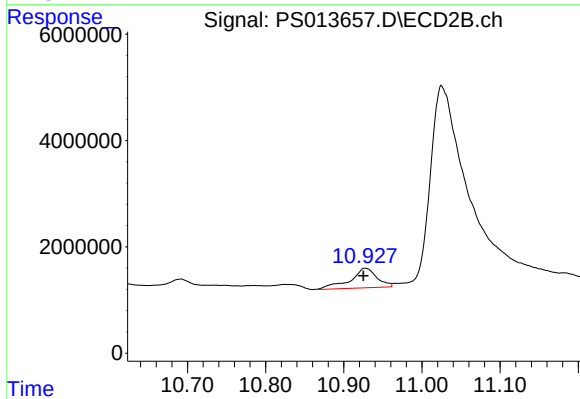

#16 DCPA

R.T.: 10.927 min
Delta R.T.: 0.002 min
Response: 8783365
Conc: 2.84 ng/ml