

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2021 22:12
 Operator : DD\AJ
 Sample : L5241-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:32:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.208	6.910	350.5E6	168.8E6	366.797	419.757
Target Compounds							
1) T	Dalapon	2.987f	2.591	75232306	138.5E6	69.171	266.344 #
2) T	3,5-DICHL...	6.426	6.093	6804826	50745872	5.146	80.549 #
5) T	DICAMBA	0.000	7.042	0	2991987	N.D.	1.742
6) T	MCP	7.617f	0.000	5141563	0	1.795	N.D. #
7) T	MCPA	7.691	0.000	88753771	0	21.594	N.D. #
8) T	DICHLORPROP	0.000	7.735	0	8504228	N.D.	19.097
11) T	2,4,5-TP ...	0.000	8.754	0	18626617	N.D.	7.798
12) T	2,4,5-T	9.397f	0.000	28584538	0	5.055	N.D. #
13) T	2,4-DB	9.974f	0.000	12362639	0	12.652	N.D. #
14) T	DINOSEB	11.138	0.000	14131003	0	3.203	N.D. #
15) T	Picloram	10.970	11.046f	19155692	4041451	2.652	1.163 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2021 22:12
Operator : DD\AJ
Sample : L5241-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:32:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

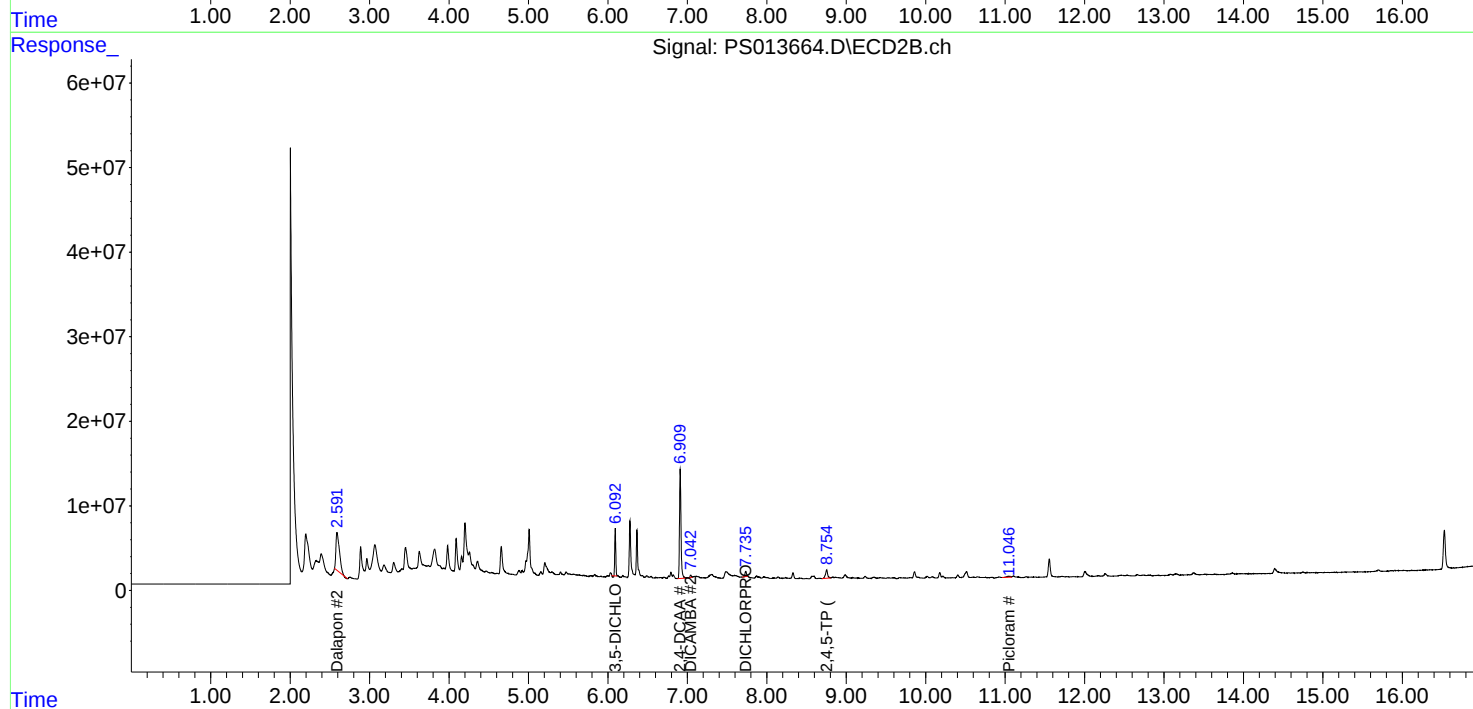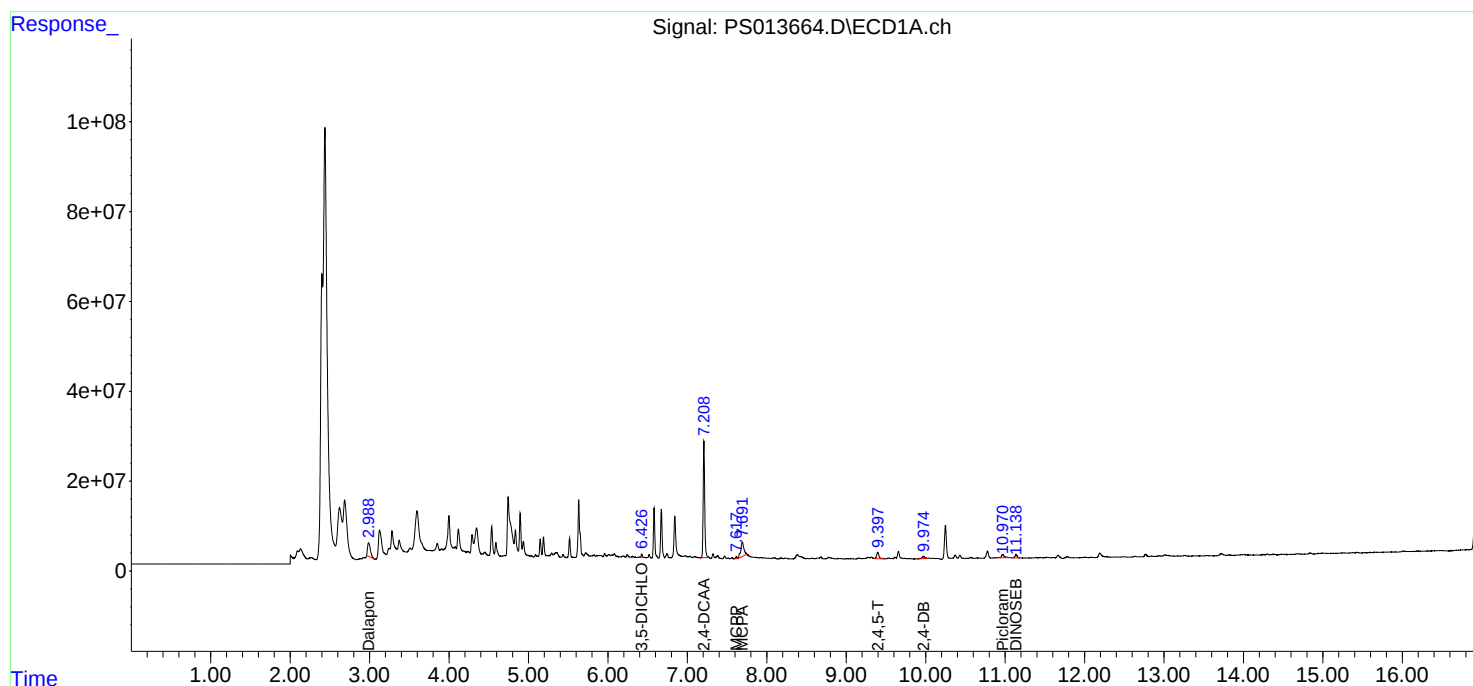


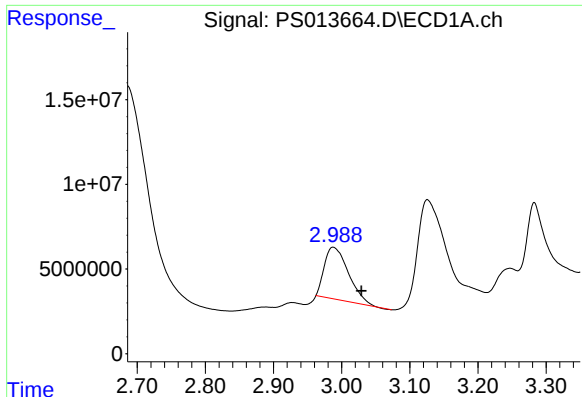

#1 Dalapon


R.T.: 2.987 min
Delta R.T.: -0.042 min
Response: 75232306
Conc: 69.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

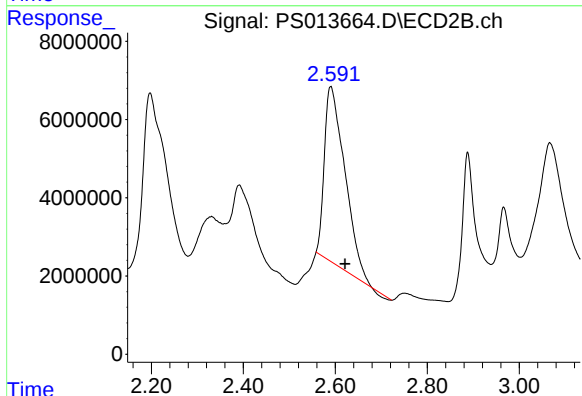


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.030 min
Response: 138485224
Conc: 266.34 ng/ml

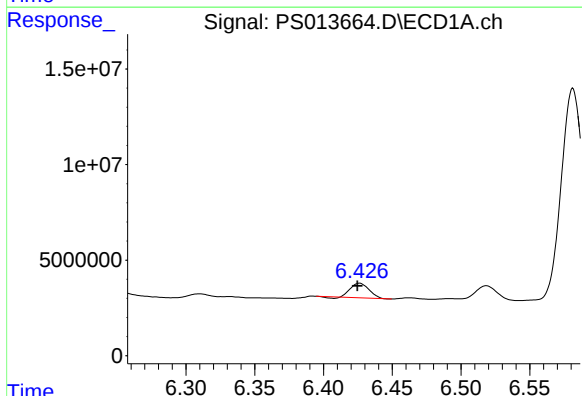


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.426 min
Delta R.T.: 0.002 min
Response: 6804826
Conc: 5.15 ng/ml

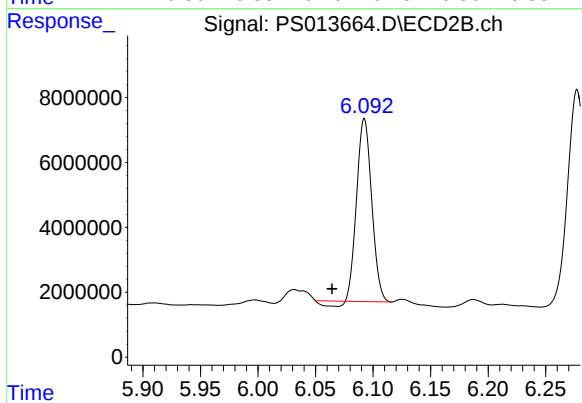

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.093 min
Delta R.T.: 0.028 min
Response: 50745872
Conc: 80.55 ng/ml

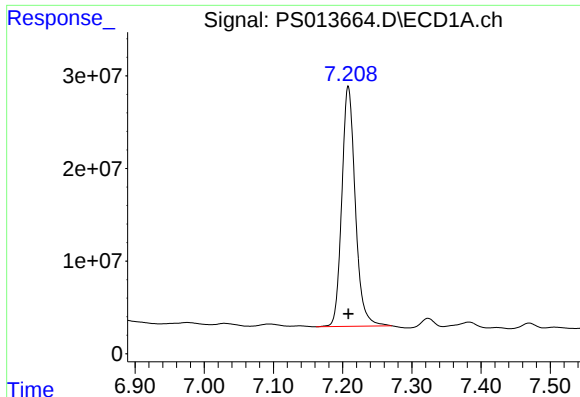

#4 2,4-DCAA


R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 350508347
Conc: 366.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

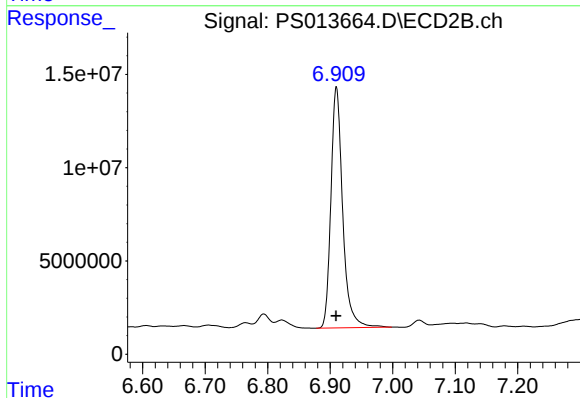


#4 2,4-DCAA

R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 168790412
Conc: 419.76 ng/ml

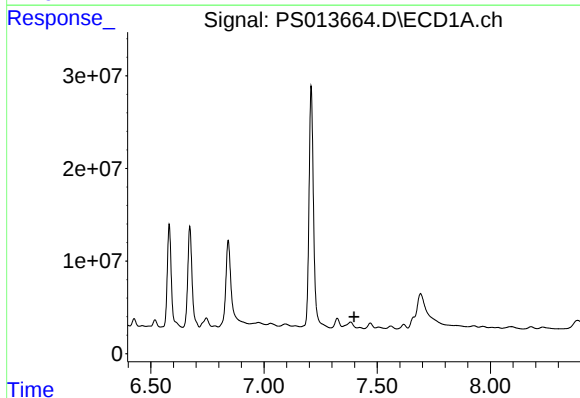


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.397 min
Response: 0
Conc: N.D.

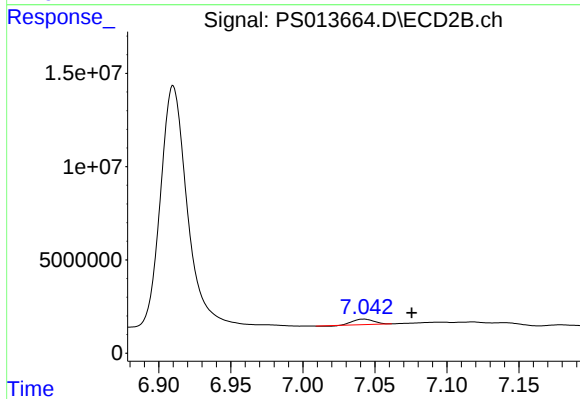

#5 DICAMBA


R.T.: 7.042 min
Delta R.T.: -0.033 min
Response: 2991987
Conc: 1.74 ng/ml

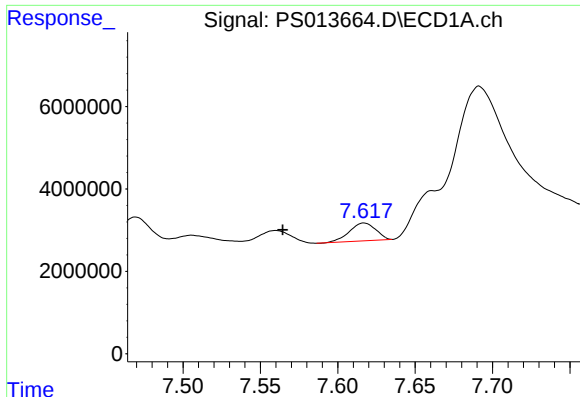

#6 MCPP


R.T.: 7.617 min
Delta R.T.: 0.053 min
Response: 5141563
Conc: 1.79 ug/ml

Instrument :
ECD_S
ClientSampleId :

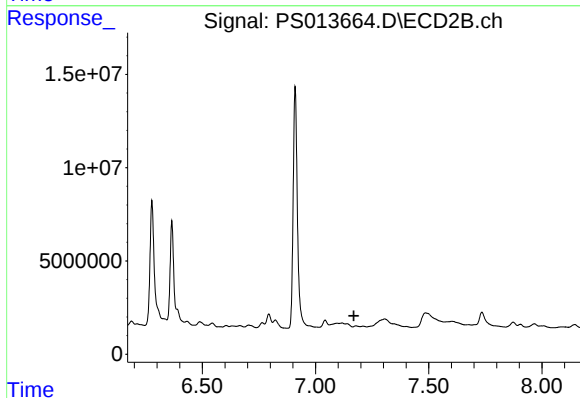


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.170 min
Response: 0
Conc: N.D.

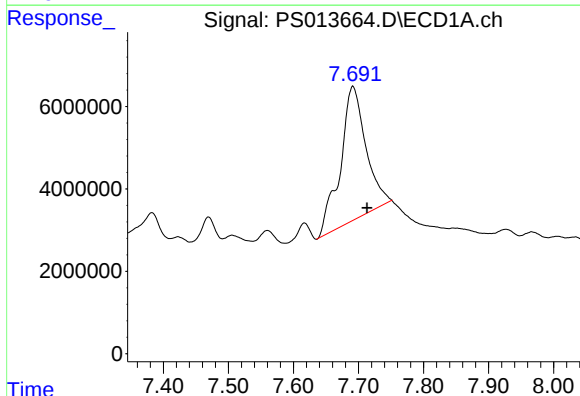


#7 MCPA

R.T.: 7.691 min
Delta R.T.: -0.022 min
Response: 88753771
Conc: 21.59 ug/ml

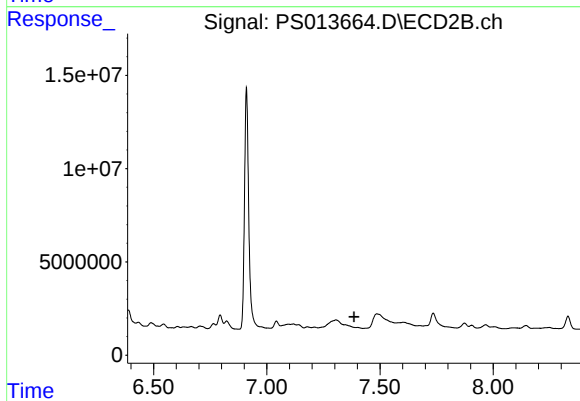

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

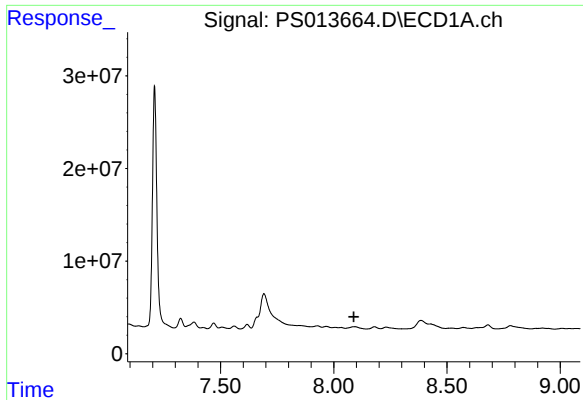

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

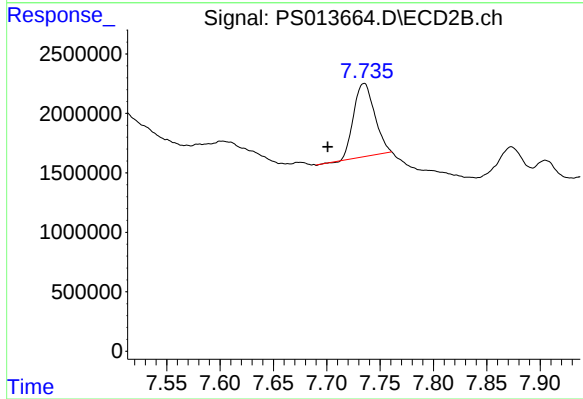


#8 DICHLORPROP

R.T.: 7.735 min
Delta R.T.: 0.034 min
Response: 8504228
Conc: 19.10 ng/ml

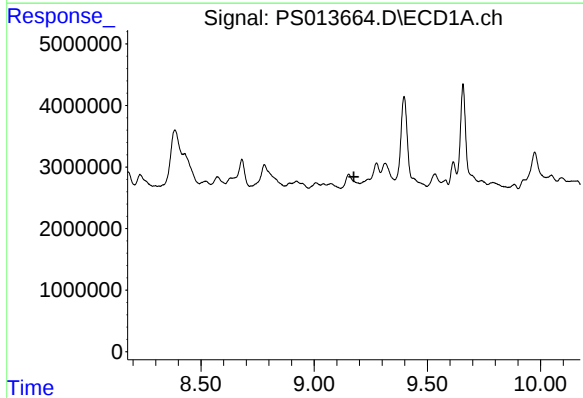


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.175 min
Response: 0
Conc: N.D.

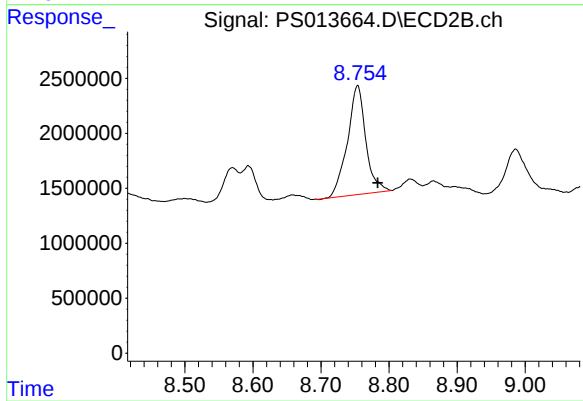

#11 2,4,5-TP (SILVEX)


R.T.: 8.754 min
Delta R.T.: -0.030 min
Response: 18626617
Conc: 7.80 ng/ml

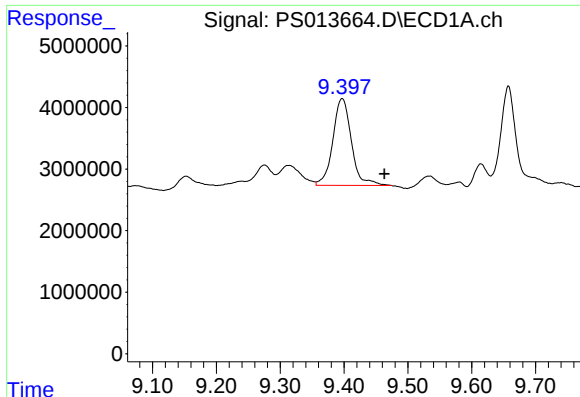

#12 2,4,5-T


R.T.: 9.397 min
Delta R.T.: -0.066 min
Response: 28584538
Conc: 5.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

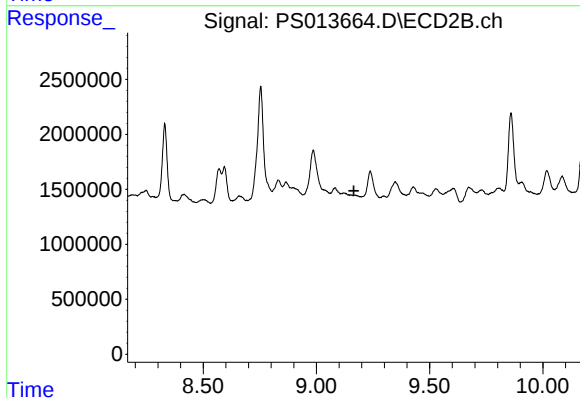


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.165 min
Response: 0
Conc: N.D.

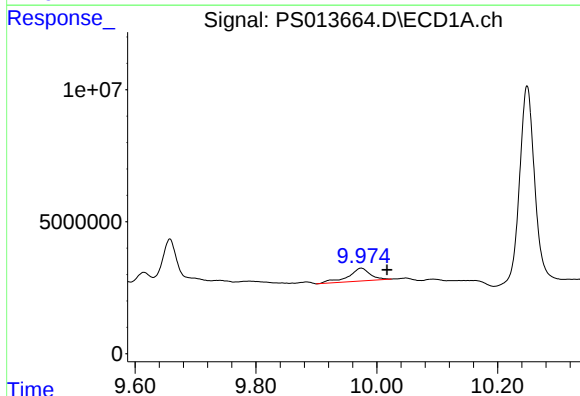


#13 2,4-DB

R.T.: 9.974 min
Delta R.T.: -0.043 min
Response: 12362639
Conc: 12.65 ng/ml

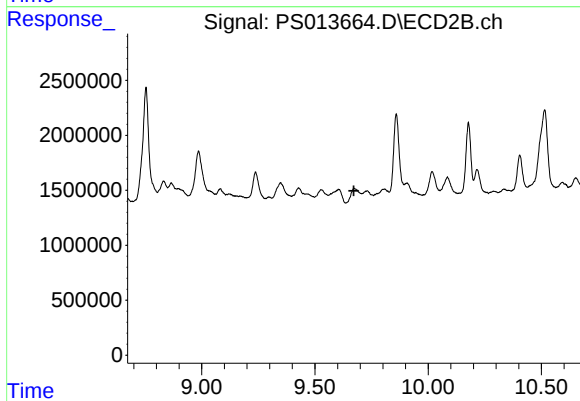

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

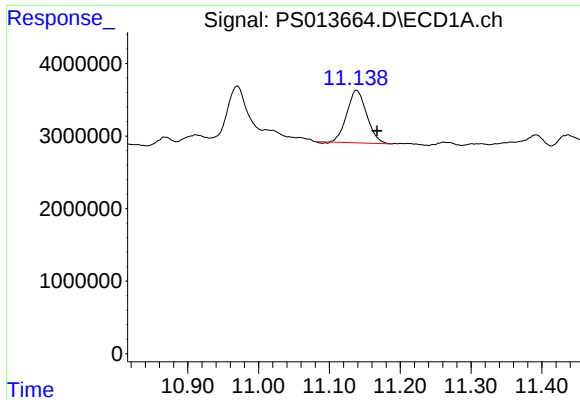

#14 DINOSEB


R.T.: 11.138 min
Delta R.T.: -0.029 min
Response: 14131003
Conc: 3.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

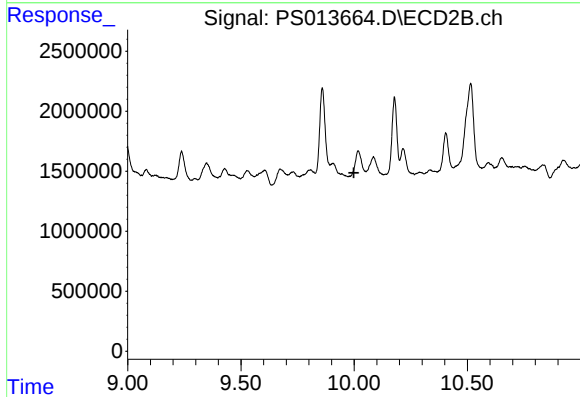


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.999 min
Response: 0
Conc: N.D.

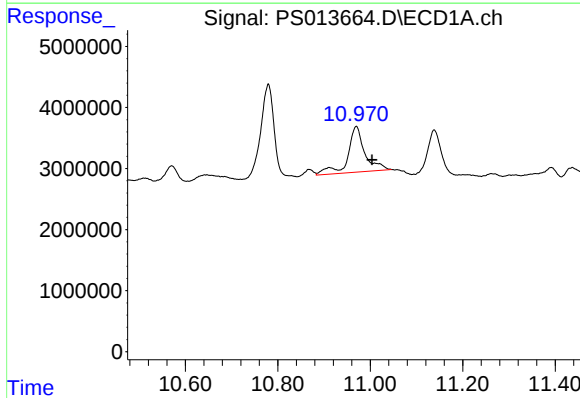

#15 Picloram

R.T.: 10.970 min
Delta R.T.: -0.034 min
Response: 19155692
Conc: 2.65 ng/ml

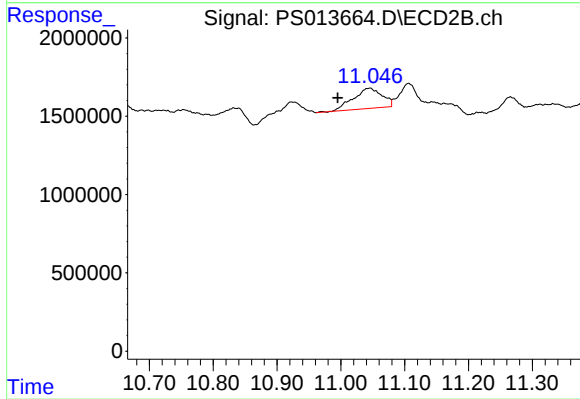

#15 Picloram

R.T.: 11.046 min
Delta R.T.: 0.050 min
Response: 4041451
Conc: 1.16 ng/ml