

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 00:07
 Operator : DD\AJ
 Sample : L5246-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:34:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.209	6.910	341.0E6	168.4E6	356.846	418.786
Target Compounds							
1) T	Dalapon	2.988f	2.589	80149494	147.2E6	73.692	283.049 #
2) T	3,5-DICHL...	0.000	6.093	0	44516324	N.D.	70.661
5) T	DICAMBA	7.385	7.042	10124407	3823489	2.629	2.226
7) T	MCPA	7.713	0.000	15093640	0	3.672	N.D. #
10) T	Pentachlo...	8.681f	8.424	6760442	3760538	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.756	0	17136011	N.D.	7.174
12) T	2,4,5-T	9.396f	0.000	34181595	0	6.045	N.D. #
13) T	2,4-DB	9.979	0.000	8426425	0	8.624	N.D. #
14) T	DINOSEB	11.141	0.000	22652698	0	5.135	N.D. #
15) T	Picloram	10.978	11.026	14122943	45776845	1.955	13.171 #
16) T	DCPA	0.000	10.929	0	2020559	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 00:07
Operator : DD\AJ
Sample : L5246-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:34:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

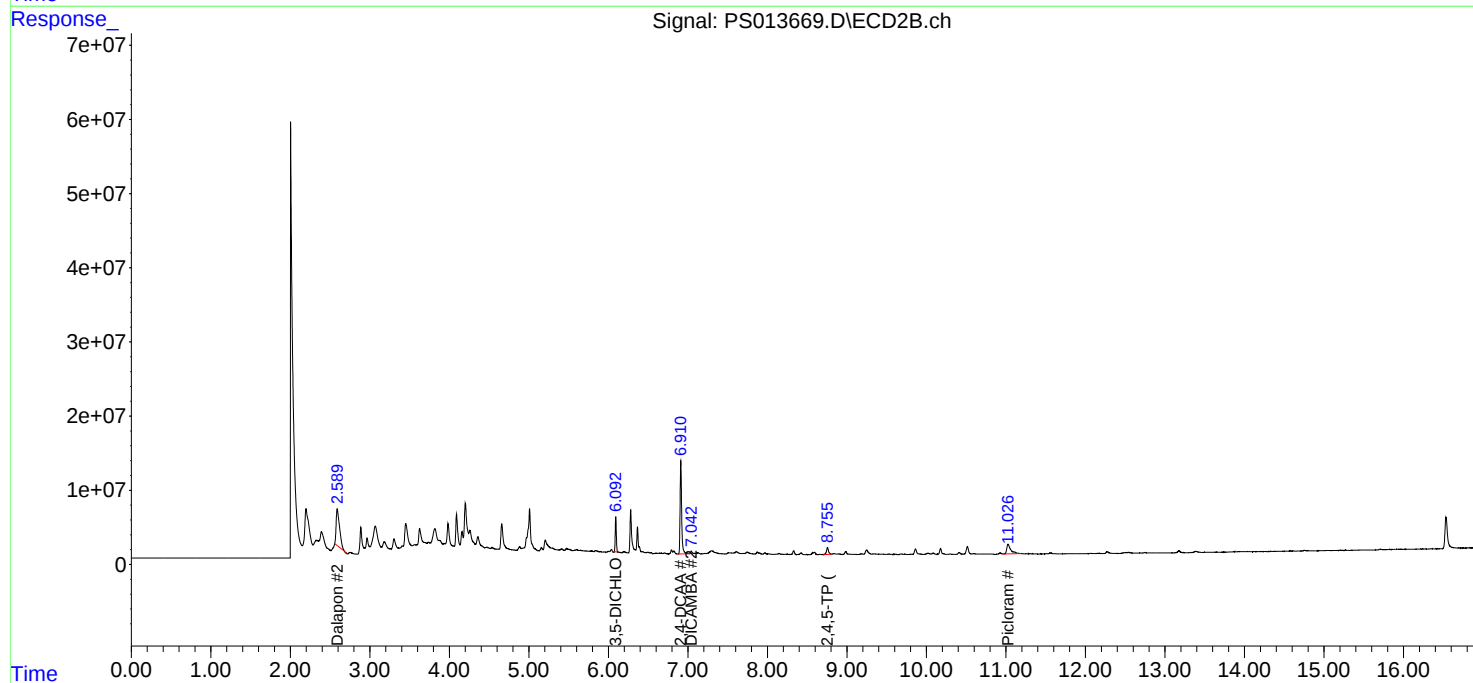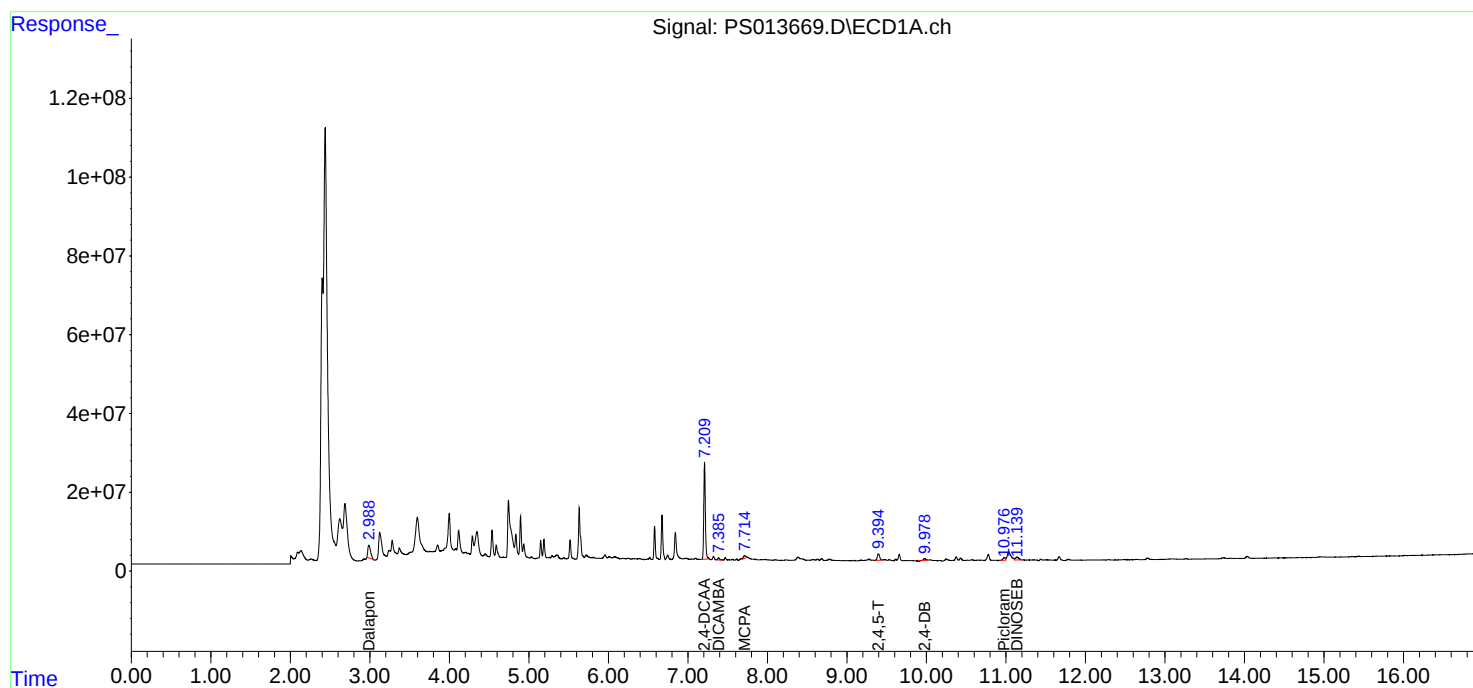


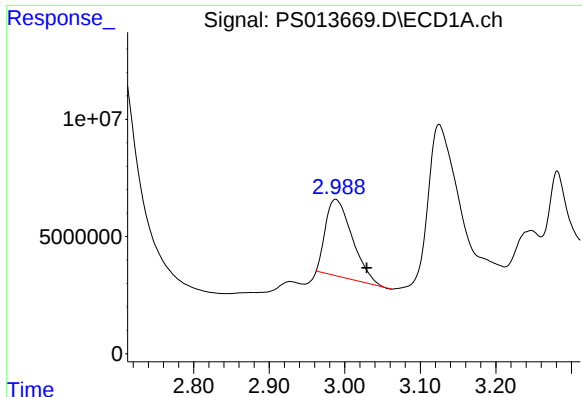

#1 Dalapon


R.T.: 2.988 min
Delta R.T.: -0.041 min
Response: 80149494
Conc: 73.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

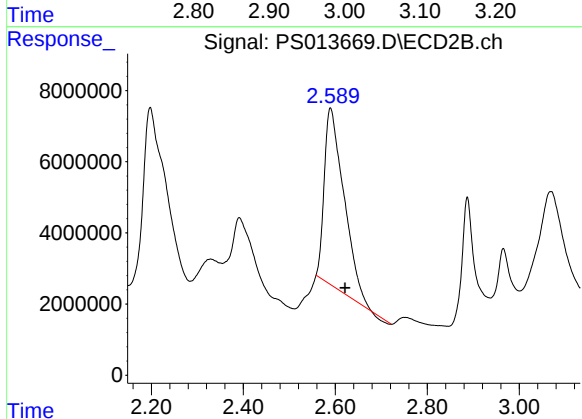


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.032 min
Response: 147170894
Conc: 283.05 ng/ml

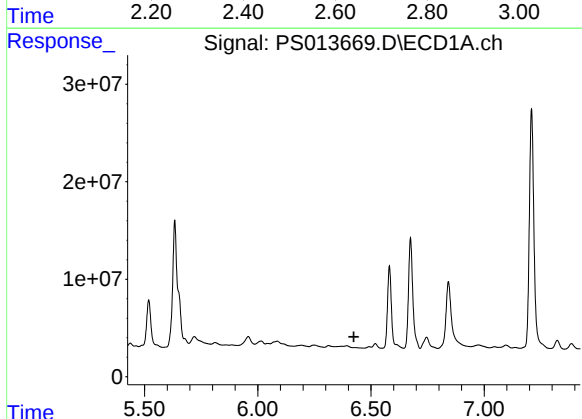


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

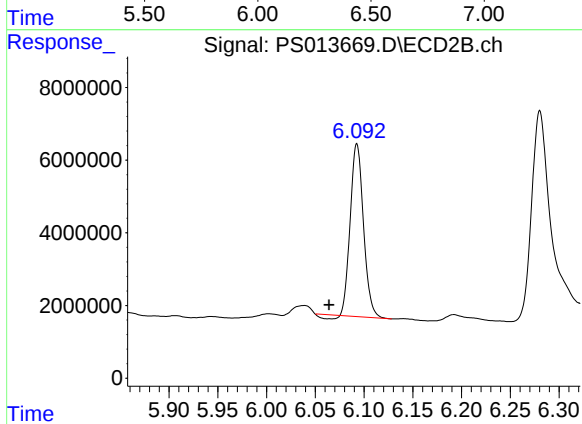

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.093 min
Delta R.T.: 0.028 min
Response: 44516324
Conc: 70.66 ng/ml

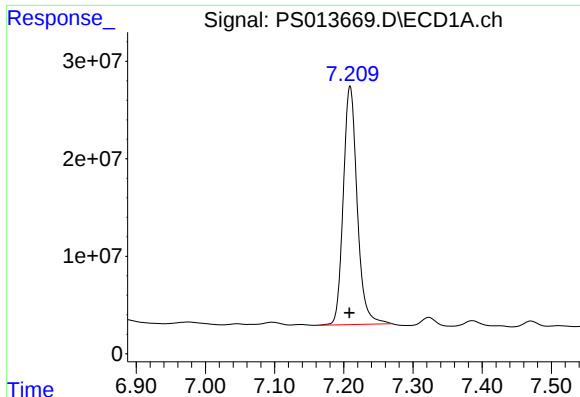

#4 2,4-DCAA


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 340999349
Conc: 356.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

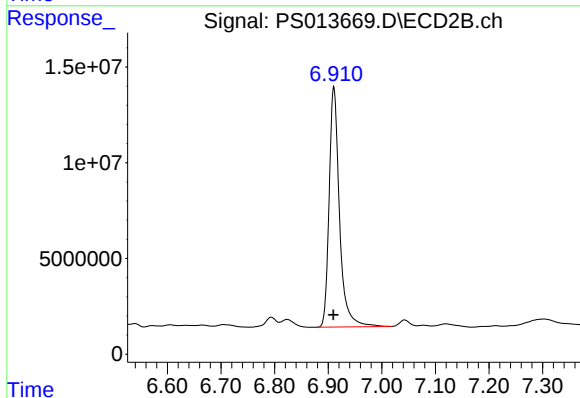


#4 2,4-DCAA

R.T.: 6.910 min
Delta R.T.: 0.001 min
Response: 168399936
Conc: 418.79 ng/ml

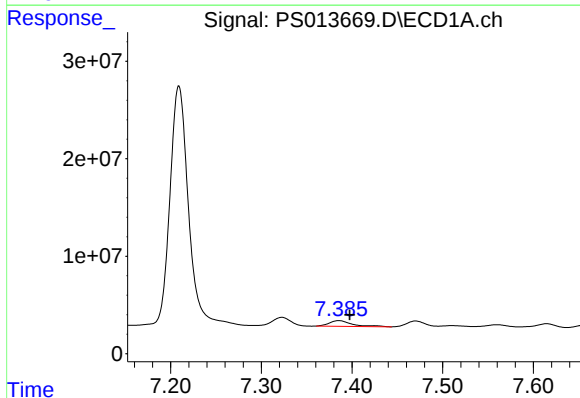


#5 DICAMBA

R.T.: 7.385 min
Delta R.T.: -0.012 min
Response: 10124407
Conc: 2.63 ng/ml

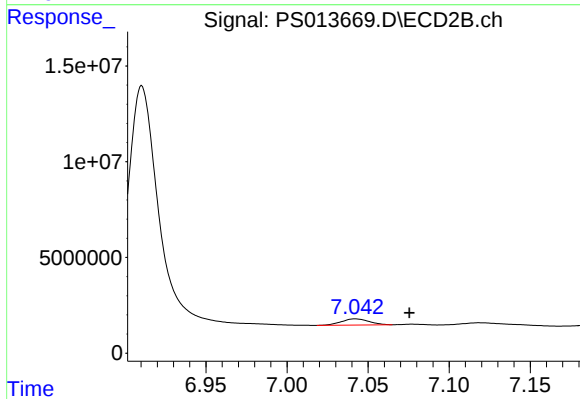

#5 DICAMBA


R.T.: 7.042 min
Delta R.T.: -0.033 min
Response: 3823489
Conc: 2.23 ng/ml

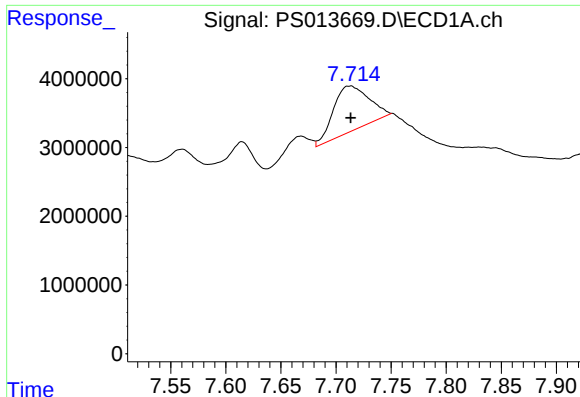

#7 MCPA


R.T.: 7.713 min
Delta R.T.: 0.000 min
Response: 15093640
Conc: 3.67 ug/ml

Instrument :
ECD_S
ClientSampleId :

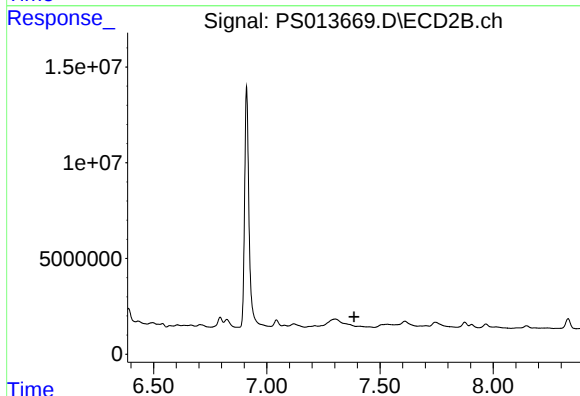


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

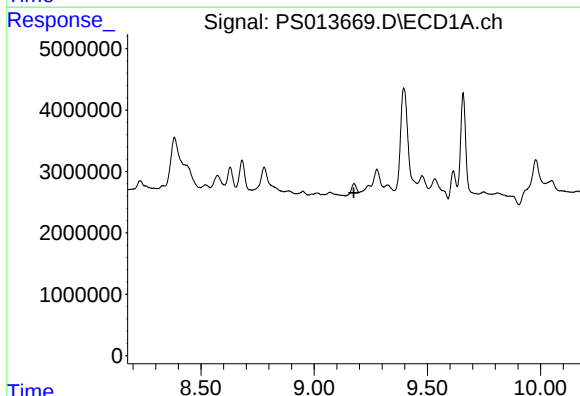


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.175 min
Response: 0
Conc: N.D.

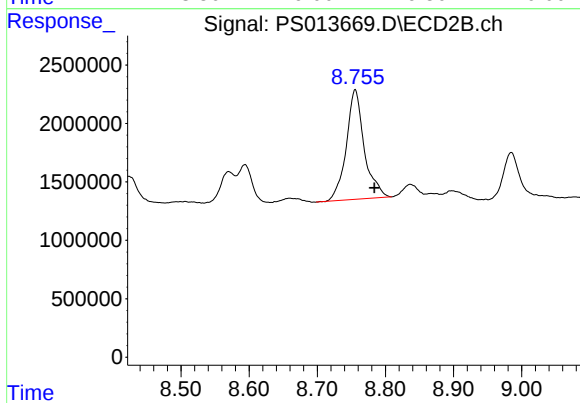

#11 2,4,5-TP (SILVEX)


R.T.: 8.756 min
Delta R.T.: -0.028 min
Response: 17136011
Conc: 7.17 ng/ml

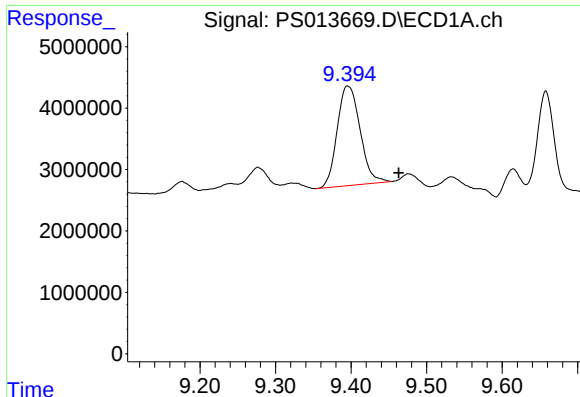

#12 2,4,5-T


R.T.: 9.396 min
Delta R.T.: -0.068 min
Response: 34181595
Conc: 6.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

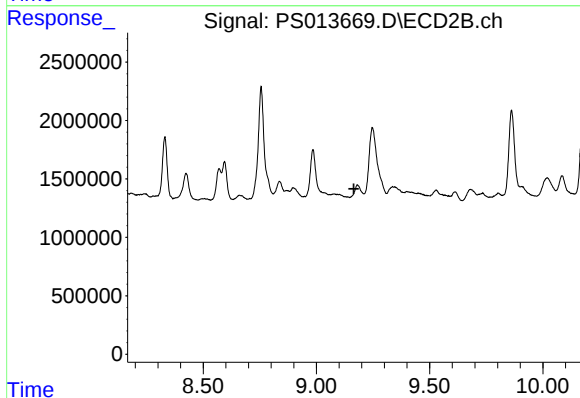


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.165 min
Response: 0
Conc: N.D.

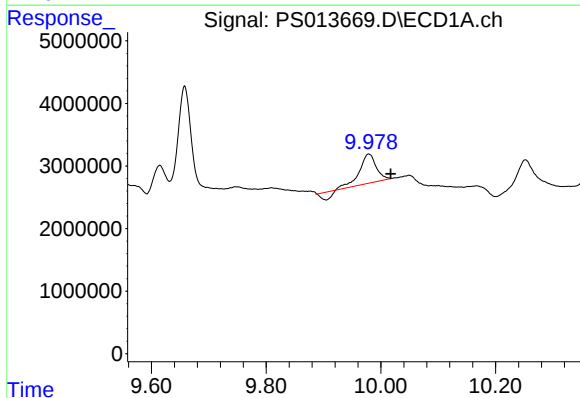


#13 2,4-DB

R.T.: 9.979 min
Delta R.T.: -0.038 min
Response: 8426425
Conc: 8.62 ng/ml

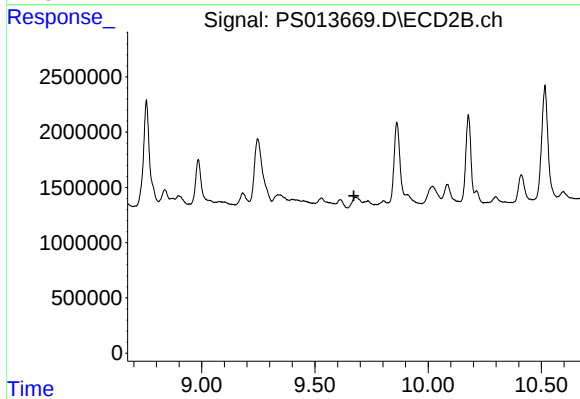

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

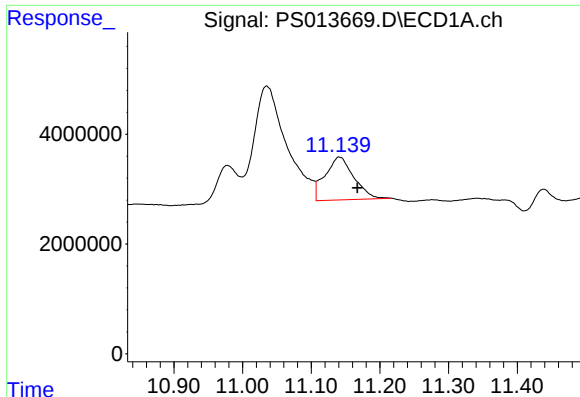

#14 DINOSEB


R.T.: 11.141 min
Delta R.T.: -0.026 min
Response: 22652698
Conc: 5.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

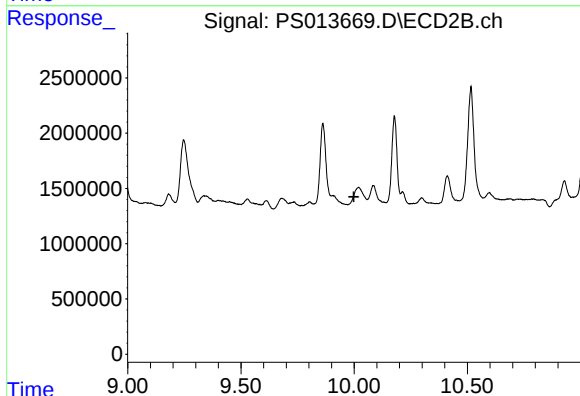


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.999 min
Response: 0
Conc: N.D.

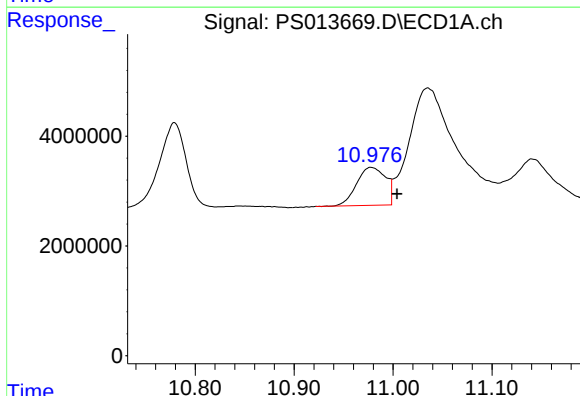

#15 Picloram

R.T.: 10.978 min
Delta R.T.: -0.026 min
Response: 14122943
Conc: 1.96 ng/ml

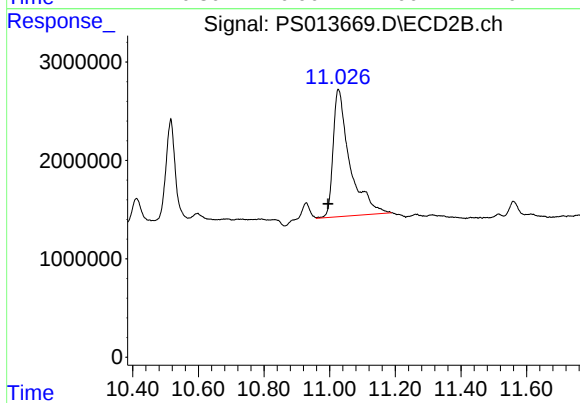

#15 Picloram

R.T.: 11.026 min
Delta R.T.: 0.031 min
Response: 45776845
Conc: 13.17 ng/ml