

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 00:30
 Operator : DD\AJ
 Sample : L5242-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:34:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.208	6.910	357.8E6	175.7E6	374.384	436.835
Target Compounds							
1) T	Dalapon	2.986f	2.588	73545622	149.8E6	67.620	288.087 #
2) T	3,5-DICHL...	0.000	6.093	0	50881081	N.D.	80.763
5) T	DICAMBA	0.000	7.043	0	4048632	N.D.	2.357
6) T	MCP	7.616f	0.000	4835862	0	1.688	N.D. #
7) T	MCPA	7.698	0.000	54739377	0	13.318	N.D. #
8) T	DICHLORPROP	0.000	7.739	0	3109985	N.D.	6.984
10) T	Pentachlo...	8.593	8.434	6549408	11555458	<MDL	1.999 #
11) T	2,4,5-TP ...	0.000	8.754	0	18430703	N.D.	7.716
12) T	2,4,5-T	9.396f	0.000	268.0E6	0	47.392	N.D. #
13) T	2,4-DB	9.973f	0.000	23876017	0	24.435	N.D. #
14) T	DINOSEB	11.139	0.000	16917971	0	3.835	N.D. #
15) T	Picloram	10.968	0.000	24098970	0	3.337	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 00:30
Operator : DD\AJ
Sample : L5242-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:34:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

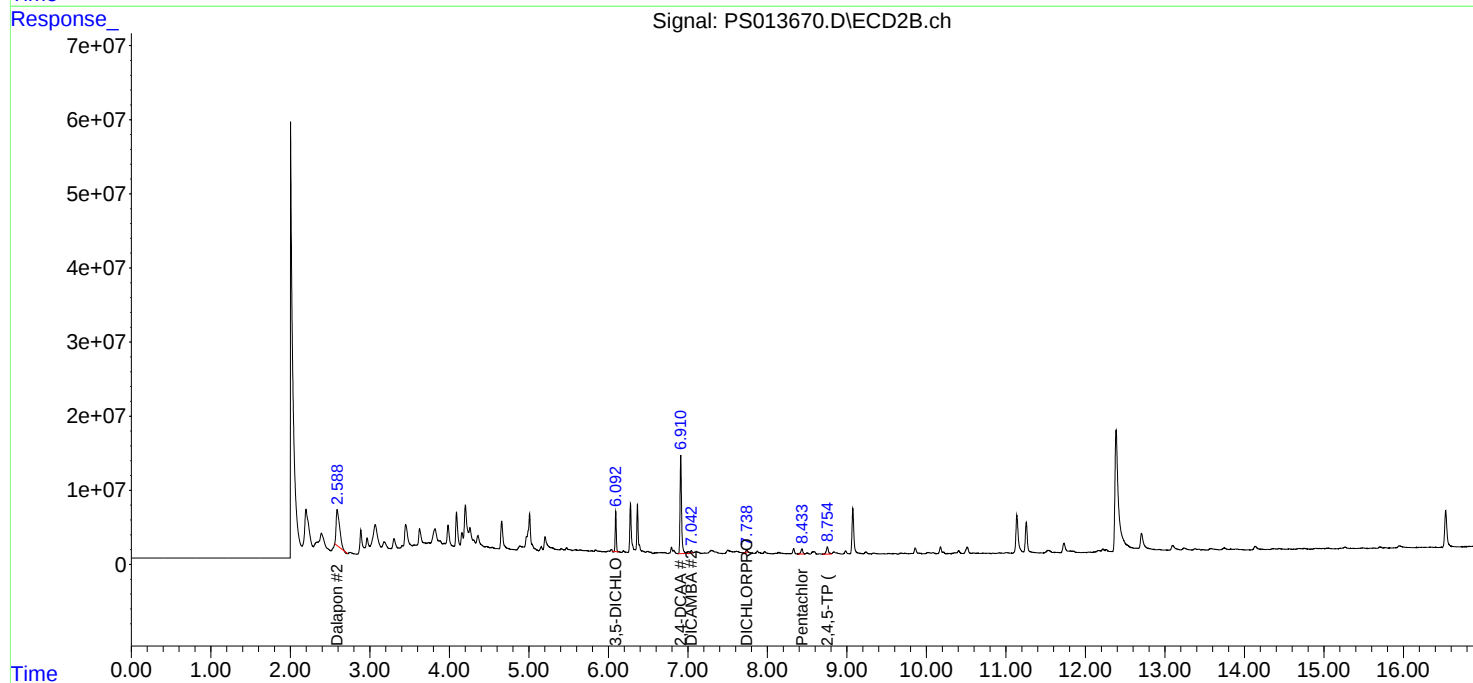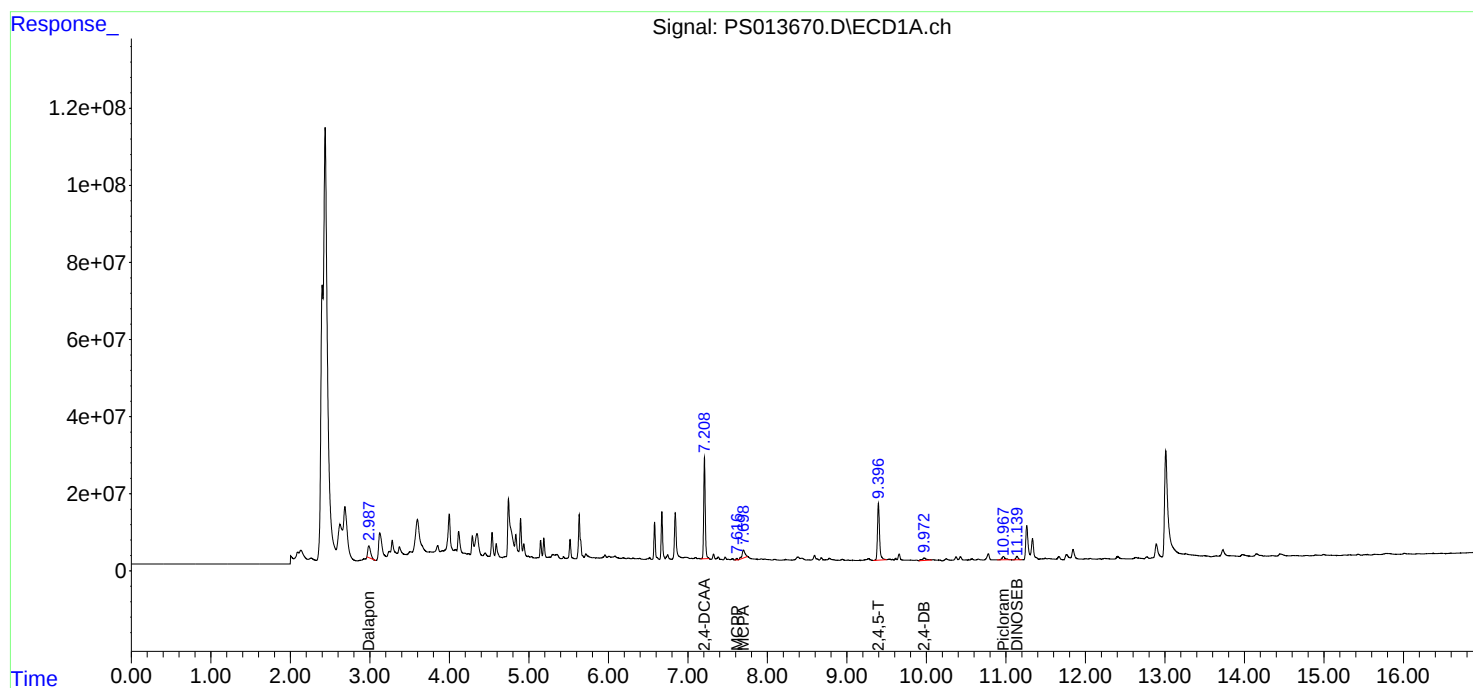


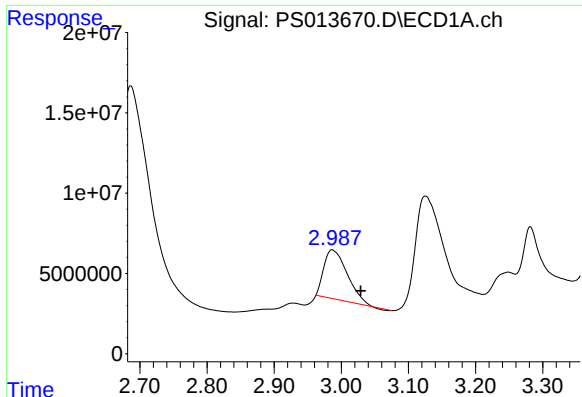

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: -0.043 min
Response: 73545622
Conc: 67.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

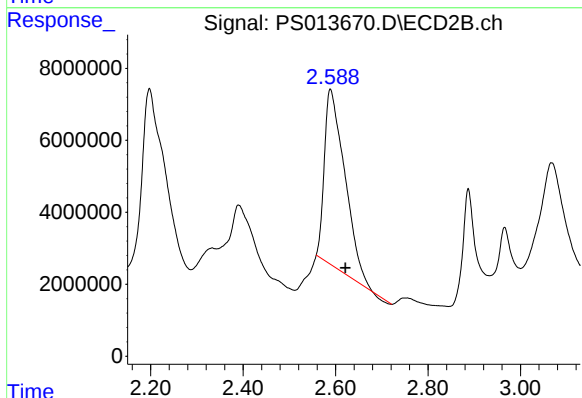


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.032 min
Response: 149790793
Conc: 288.09 ng/ml

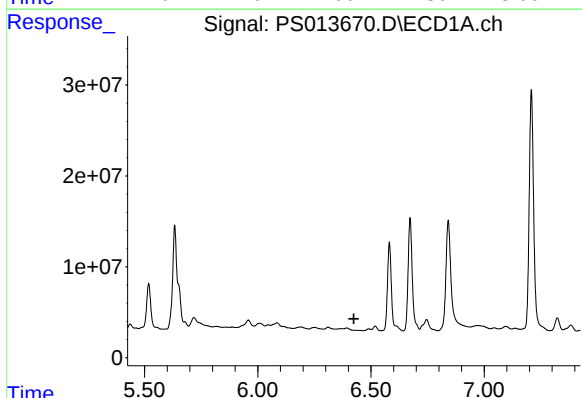


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

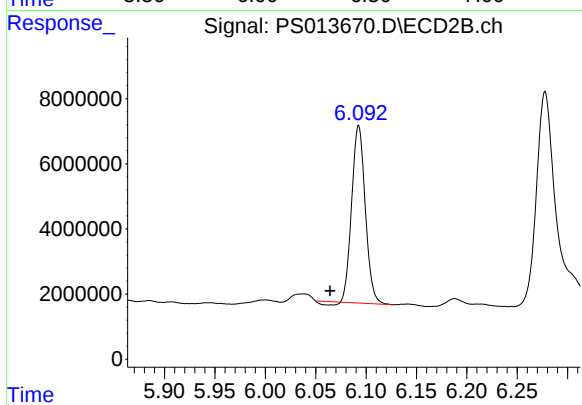

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.093 min
Delta R.T.: 0.028 min
Response: 50881081
Conc: 80.76 ng/ml

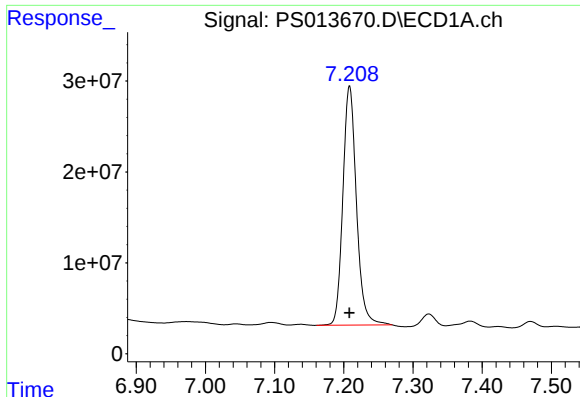

#4 2,4-DCAA


R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 357758990
Conc: 374.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

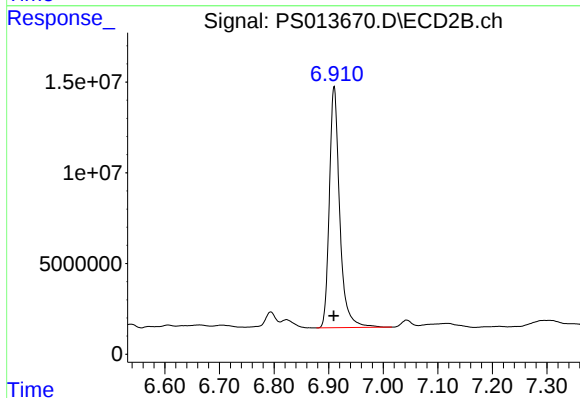


#4 2,4-DCAA

R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 175657800
Conc: 436.83 ng/ml

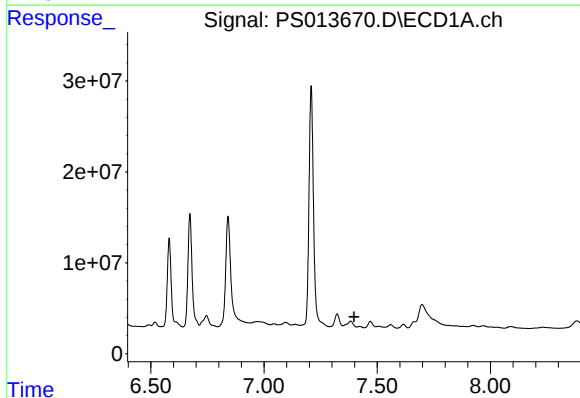


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.397 min
Response: 0
Conc: N.D.

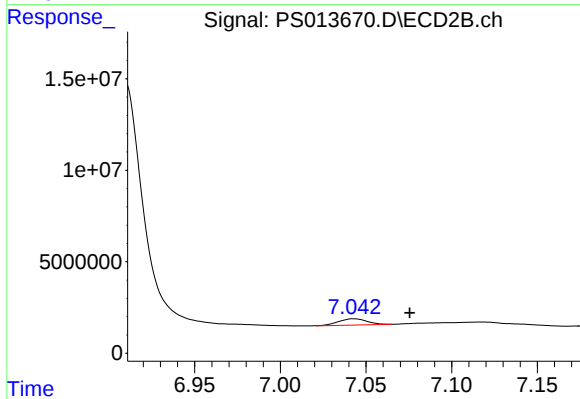

#5 DICAMBA


R.T.: 7.043 min
Delta R.T.: -0.033 min
Response: 4048632
Conc: 2.36 ng/ml

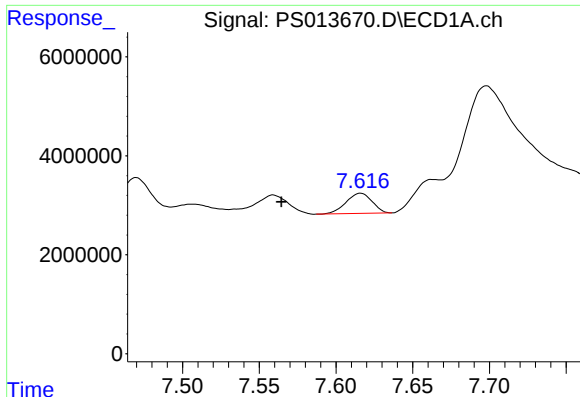

#6 MCPP


R.T.: 7.616 min
Delta R.T.: 0.052 min
Response: 4835862
Conc: 1.69 ug/ml

Instrument :
ECD_S
ClientSampleId :

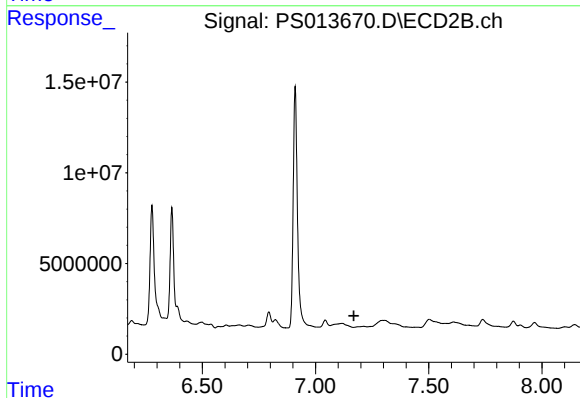


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.170 min
Response: 0
Conc: N.D.

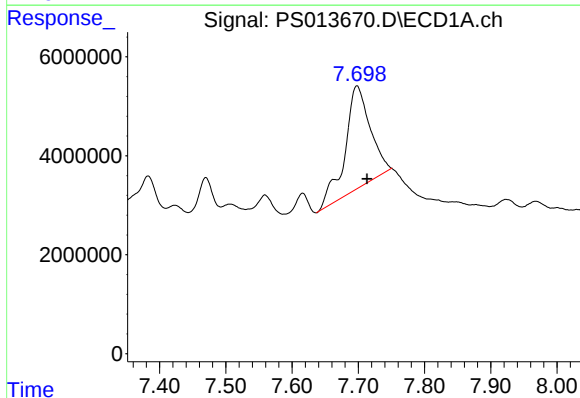


#7 MCPA

R.T.: 7.698 min
Delta R.T.: -0.015 min
Response: 54739377
Conc: 13.32 ug/ml

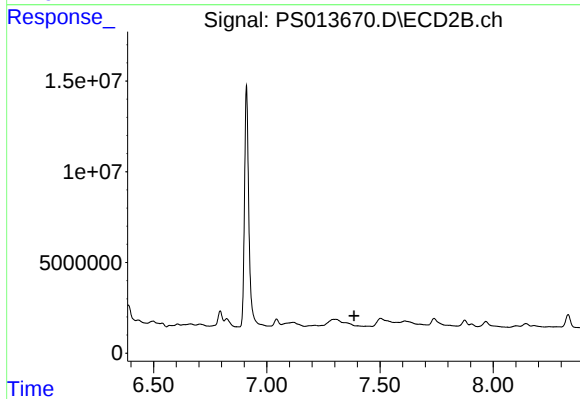

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

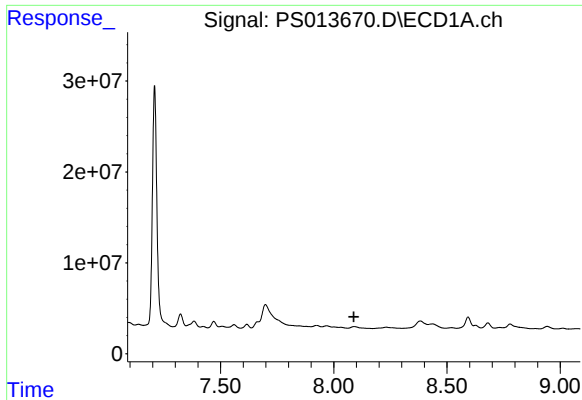

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

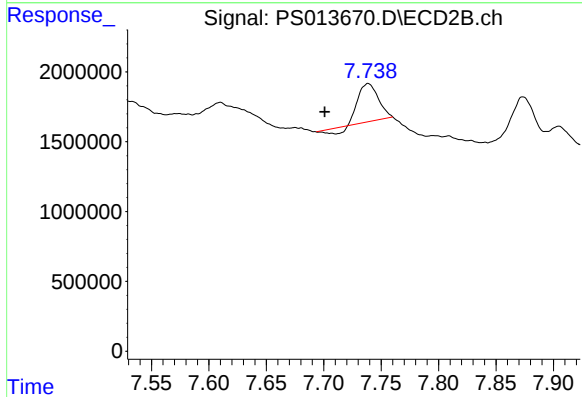


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.038 min
Response: 3109985
Conc: 6.98 ng/ml

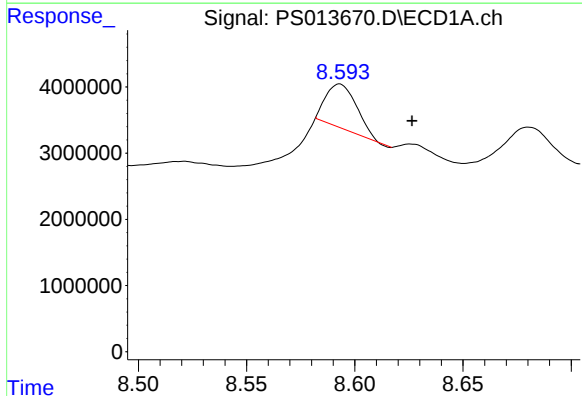


#10 Pentachlorophenol

R.T.: 8.593 min
Delta R.T.: -0.033 min
Response: 6549408
Conc: N.D.

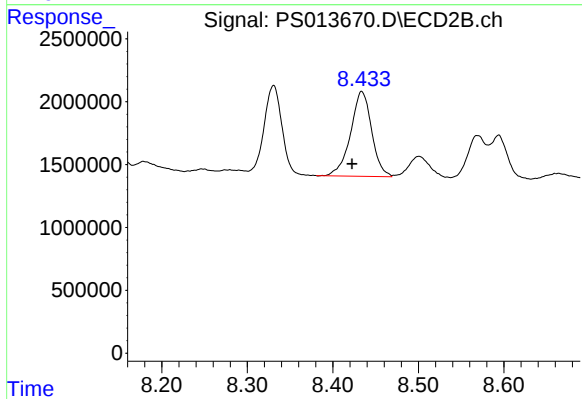

#10 Pentachlorophenol


R.T.: 8.434 min
Delta R.T.: 0.012 min
Response: 11555458
Conc: 2.00 ng/ml

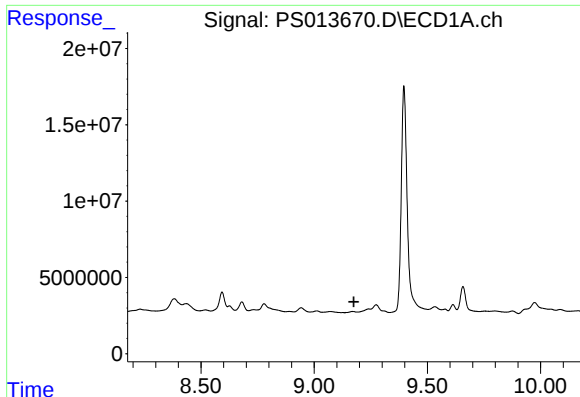

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

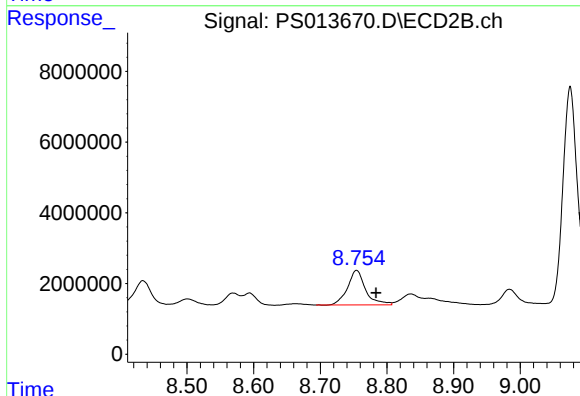


#11 2,4,5-TP (SILVEX)

R.T.: 8.754 min
Delta R.T.: -0.029 min
Response: 18430703
Conc: 7.72 ng/ml

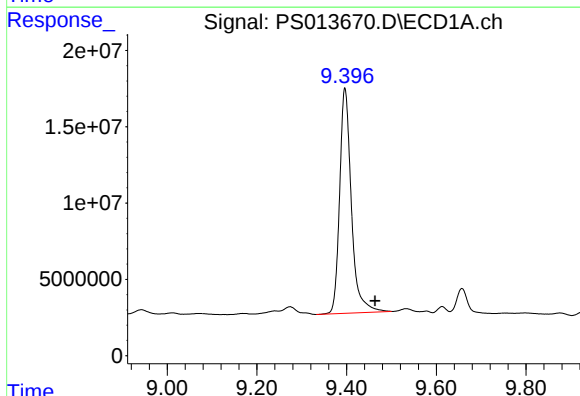


#12 2,4,5-T

R.T.: 9.396 min
Delta R.T.: -0.067 min
Response: 267986687
Conc: 47.39 ng/ml

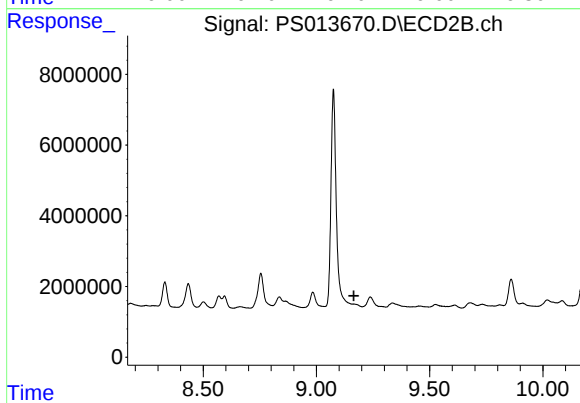

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.165 min
Response: 0
Conc: N.D.

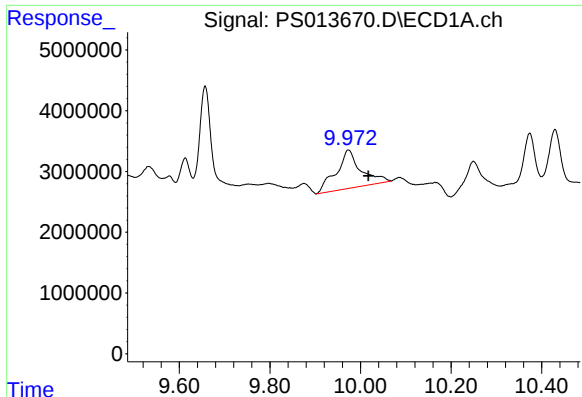

#13 2,4-DB


R.T.: 9.973 min
Delta R.T.: -0.044 min
Response: 23876017
Conc: 24.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

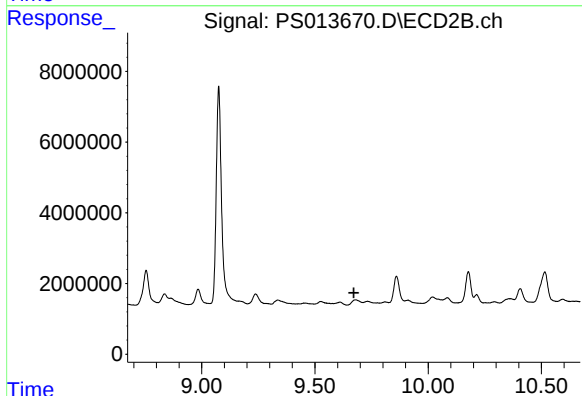


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

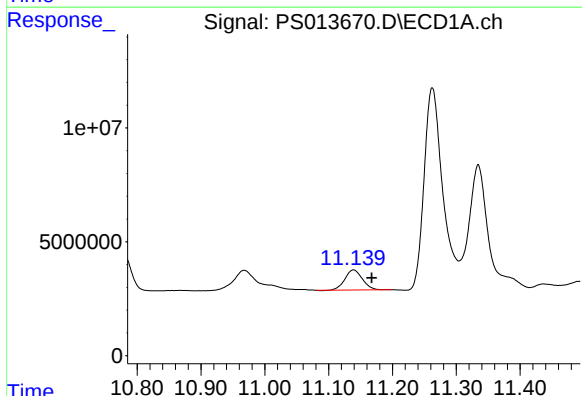


#14 DINOSEB

R.T.: 11.139 min
Delta R.T.: -0.029 min
Response: 16917971
Conc: 3.83 ng/ml

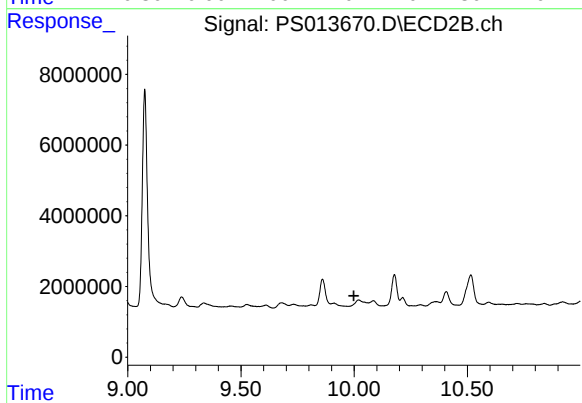

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.999 min
Response: 0
Conc: N.D.

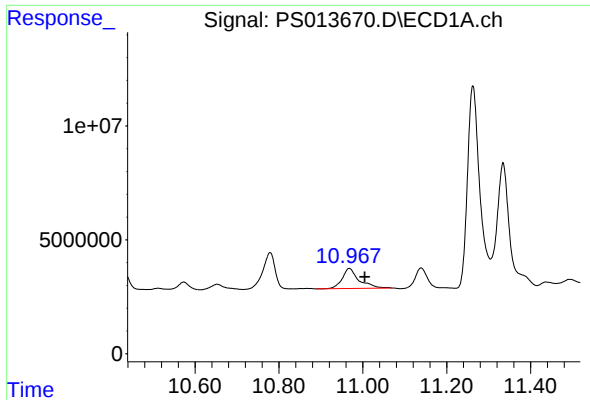

#15 Picloram

R.T.: 10.968 min
Delta R.T.: -0.036 min
Response: 24098970
Conc: 3.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

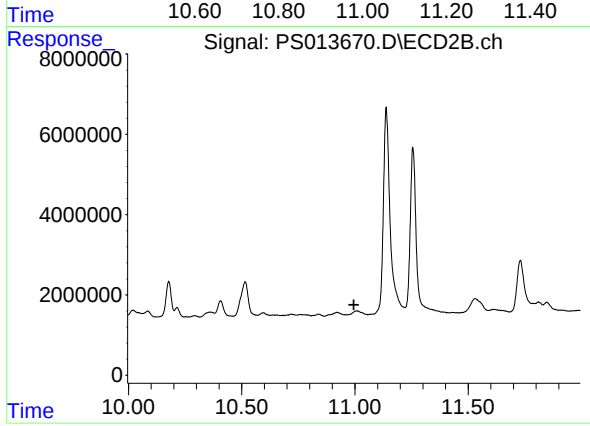

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.