

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 00:54
 Operator : DD\AJ
 Sample : L5242-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:34:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.209	6.910	633.1E6	311.7E6	662.545	775.100
Target Compounds							
1) T	Dalapon	2.986f	2.590	72451139	160.9E6	66.614	309.470 #
2) T	3,5-DICHL...	0.000	6.093	0	52777915	N.D.	83.774
5) T	DICAMBA	7.384	7.044	8571397	5554848	2.226	3.235 #
7) T	MCPA	7.715	0.000	8880482	0	2.161	N.D. #
10) T	Pentachlo...	8.681f	0.000	5627392	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.757	0	15552483	N.D.	6.511
12) T	2,4,5-T	9.400f	0.000	19556486	0	3.458	N.D. #
13) T	2,4-DB	9.979	0.000	16954687	0	17.351	N.D. #
14) T	DINOSEB	11.143	0.000	13915442	0	3.154	N.D. #
15) T	Picloram	10.977	0.000	15853491	0	2.195	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 00:54
Operator : DD\AJ
Sample : L5242-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:34:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

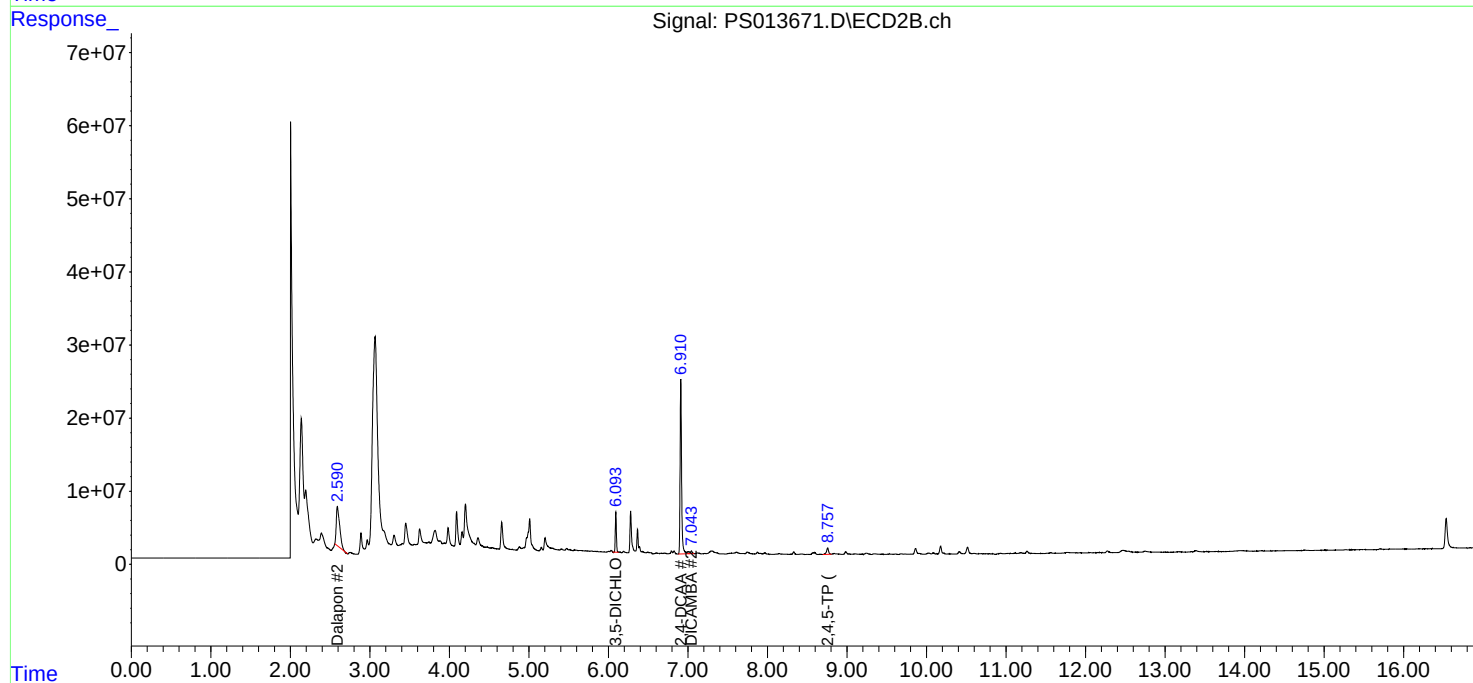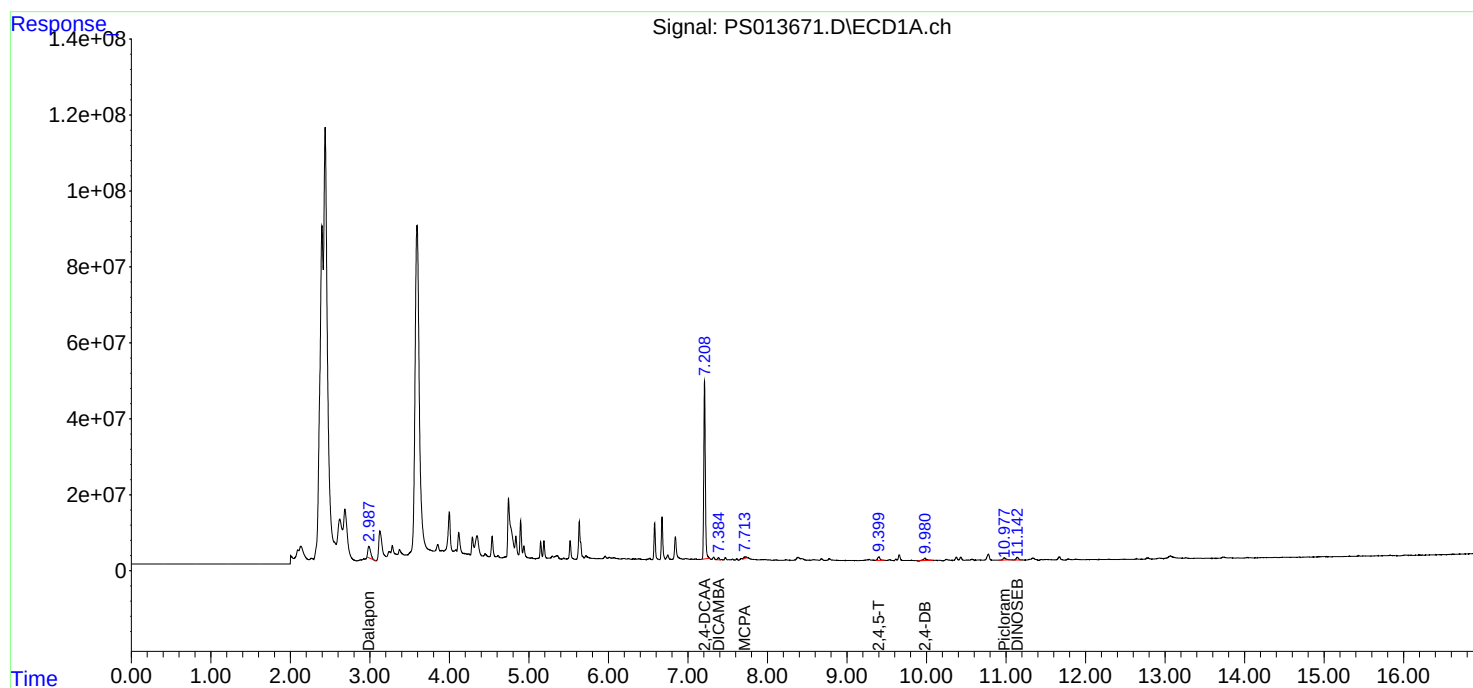


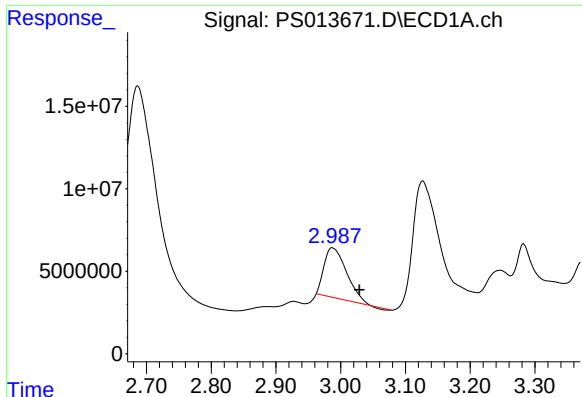

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: -0.043 min
Response: 72451139
Conc: 66.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

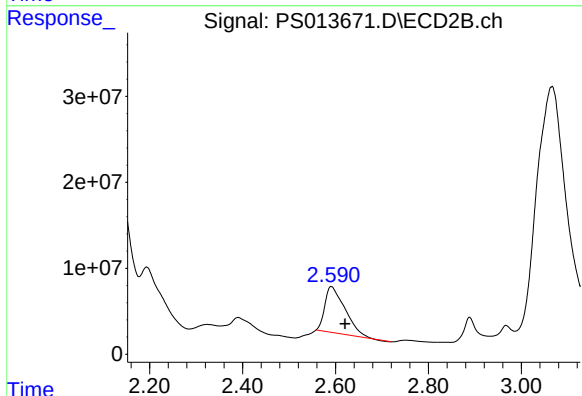


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.031 min
Response: 160908442
Conc: 309.47 ng/ml

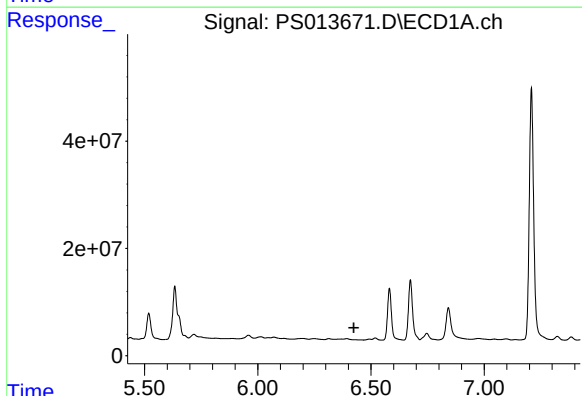


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

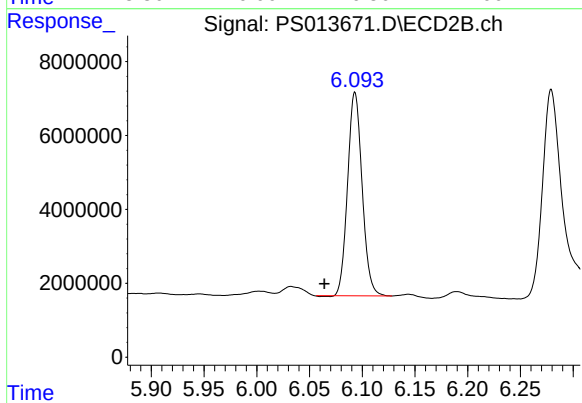

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.093 min
Delta R.T.: 0.029 min
Response: 52777915
Conc: 83.77 ng/ml

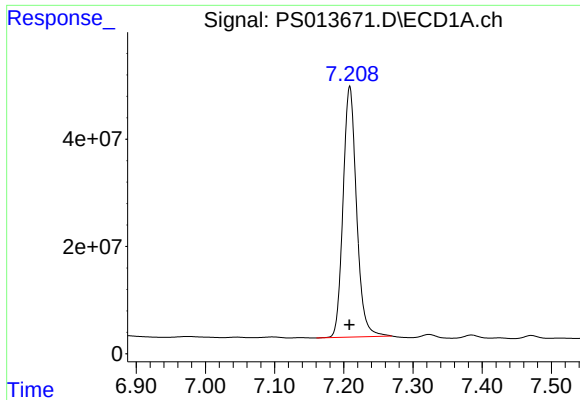

#4 2,4-DCAA


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 633122924
Conc: 662.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

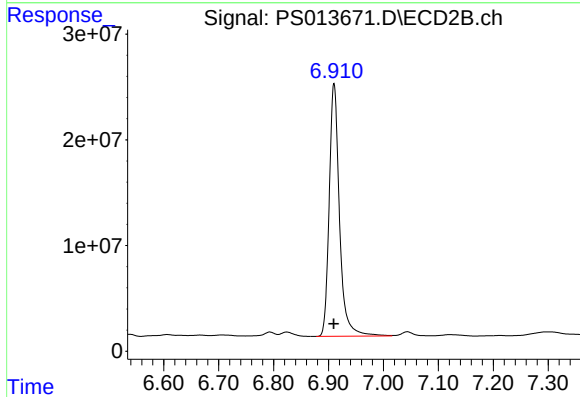


#4 2,4-DCAA

R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 311679406
Conc: 775.10 ng/ml

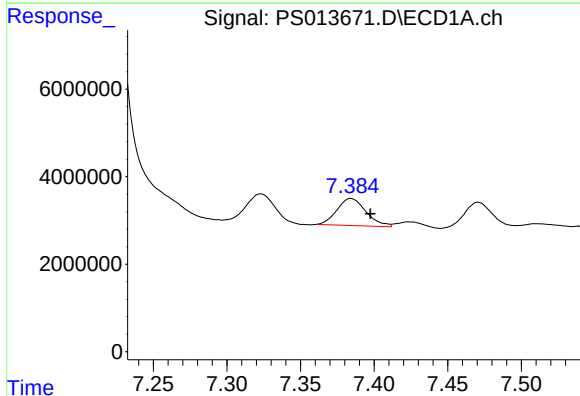


#5 DICAMBA

R.T.: 7.384 min
Delta R.T.: -0.013 min
Response: 8571397
Conc: 2.23 ng/ml

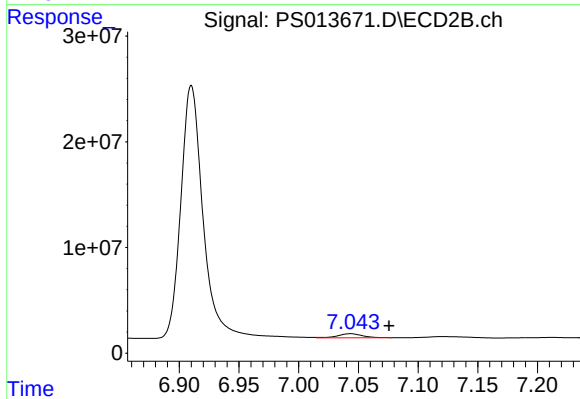

#5 DICAMBA


R.T.: 7.044 min
Delta R.T.: -0.032 min
Response: 5554848
Conc: 3.23 ng/ml

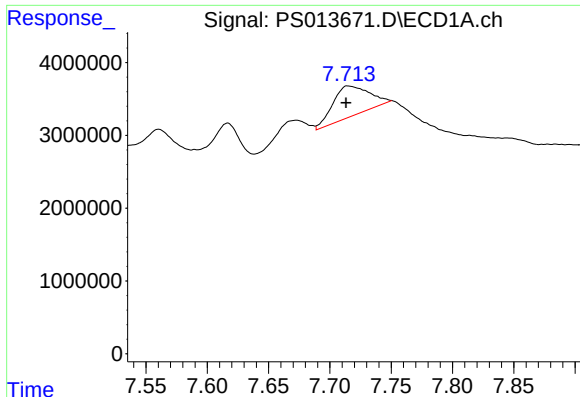

#7 MCPA


R.T.: 7.715 min
Delta R.T.: 0.002 min
Response: 8880482
Conc: 2.16 ug/ml

Instrument :
ECD_S
ClientSampleId :

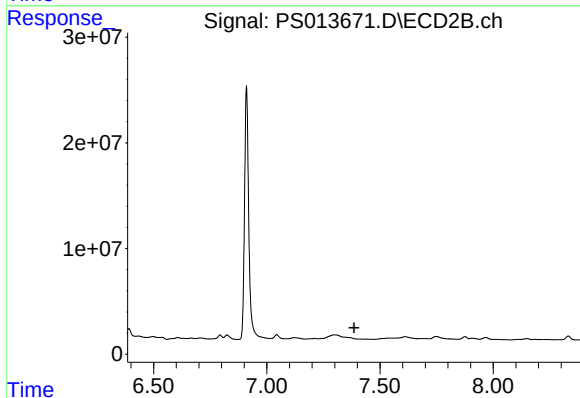


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

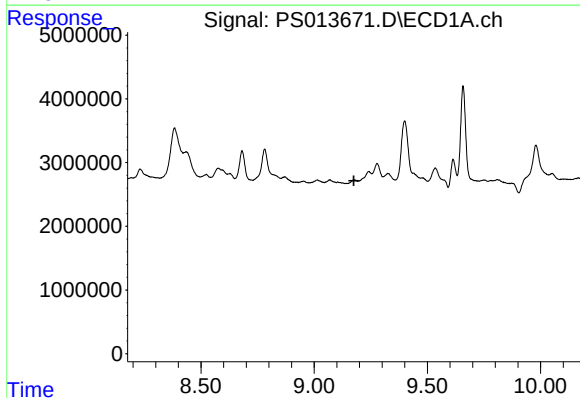


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.175 min
Response: 0
Conc: N.D.

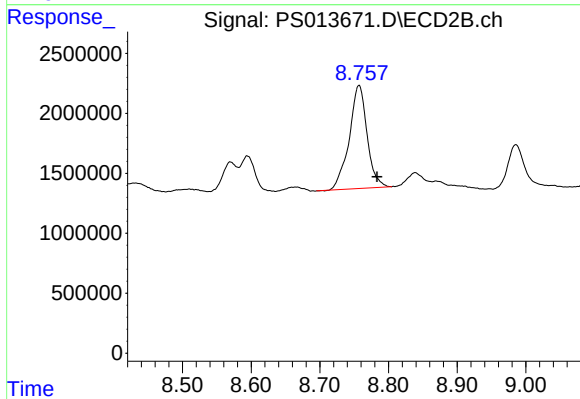

#11 2,4,5-TP (SILVEX)


R.T.: 8.757 min
Delta R.T.: -0.027 min
Response: 15552483
Conc: 6.51 ng/ml

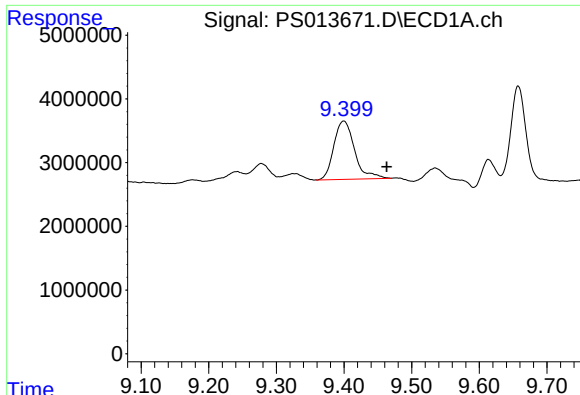

#12 2,4,5-T


R.T.: 9.400 min
Delta R.T.: -0.064 min
Response: 19556486
Conc: 3.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

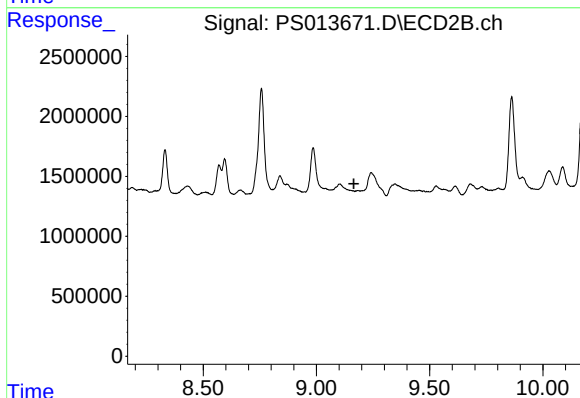


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.165 min
Response: 0
Conc: N.D.

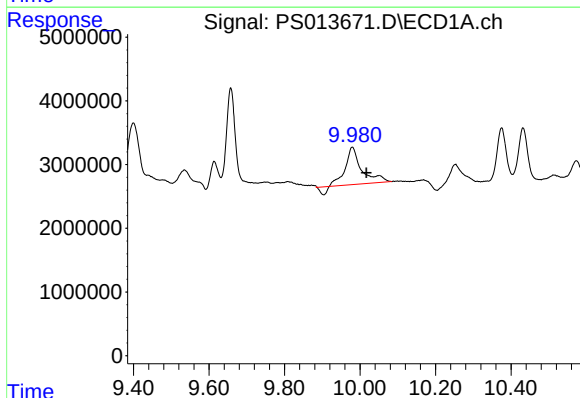


#13 2,4-DB

R.T.: 9.979 min
Delta R.T.: -0.038 min
Response: 16954687
Conc: 17.35 ng/ml

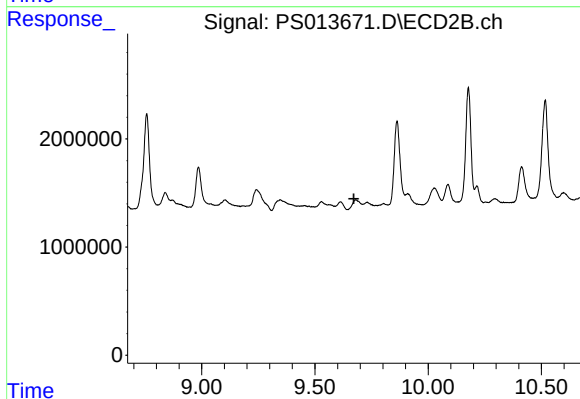

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

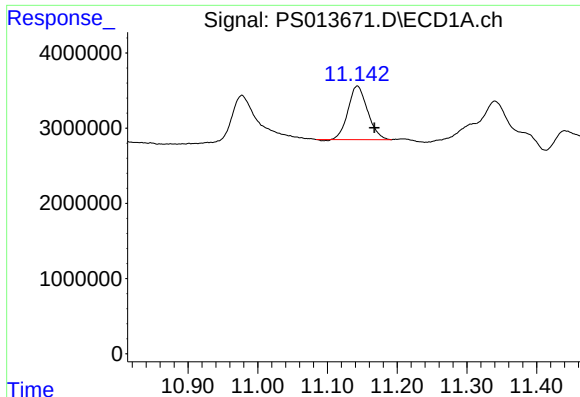

#14 DINOSEB


R.T.: 11.143 min
Delta R.T.: -0.025 min
Response: 13915442
Conc: 3.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

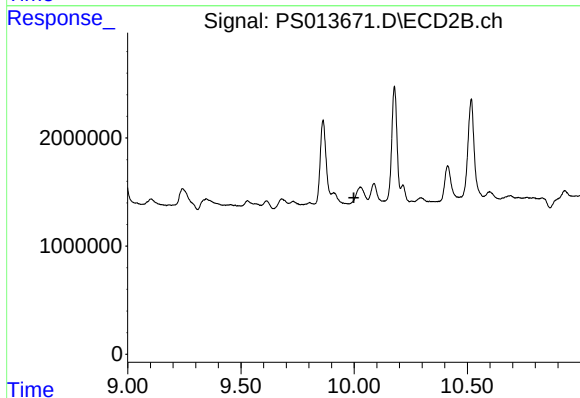


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.999 min
Response: 0
Conc: N.D.

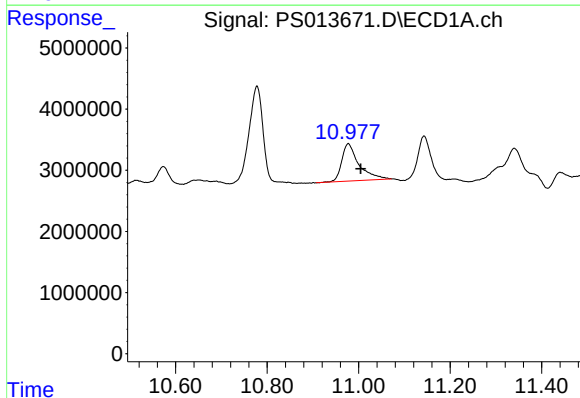

#15 Picloram

R.T.: 10.977 min
Delta R.T.: -0.027 min
Response: 15853491
Conc: 2.19 ng/ml

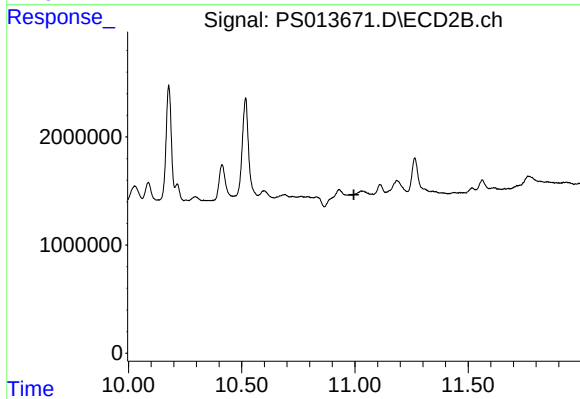

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.