

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 01:17
 Operator : DD\AJ
 Sample : L5242-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:35:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.209	6.910	324.5E6	160.6E6	339.558	399.356
Target Compounds							
1) T	Dalapon	2.985f	2.588	70869276	165.1E6	65.160	317.519 #
2) T	3,5-DICHL...	0.000	6.093	0	44926137	N.D.	71.311
5) T	DICAMBA	7.383	7.042	6840558	5721087	1.776	3.331 #
7) T	MCPA	7.704	0.000	70507835	0	17.154	N.D. #
10) T	Pentachlo...	8.681f	8.437	8304573	4428250	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.755	0	14521925	N.D.	6.079
12) T	2,4,5-T	9.399f	0.000	29456613	0	5.209	N.D. #
13) T	2,4-DB	9.977f	0.000	16269310	0	16.650	N.D. #
14) T	DINOSEB	11.142	0.000	16232839	0	3.679	N.D. #
15) T	Picloram	10.974	0.000	16415812	0	2.273	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 01:17
Operator : DD\AJ
Sample : L5242-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:35:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

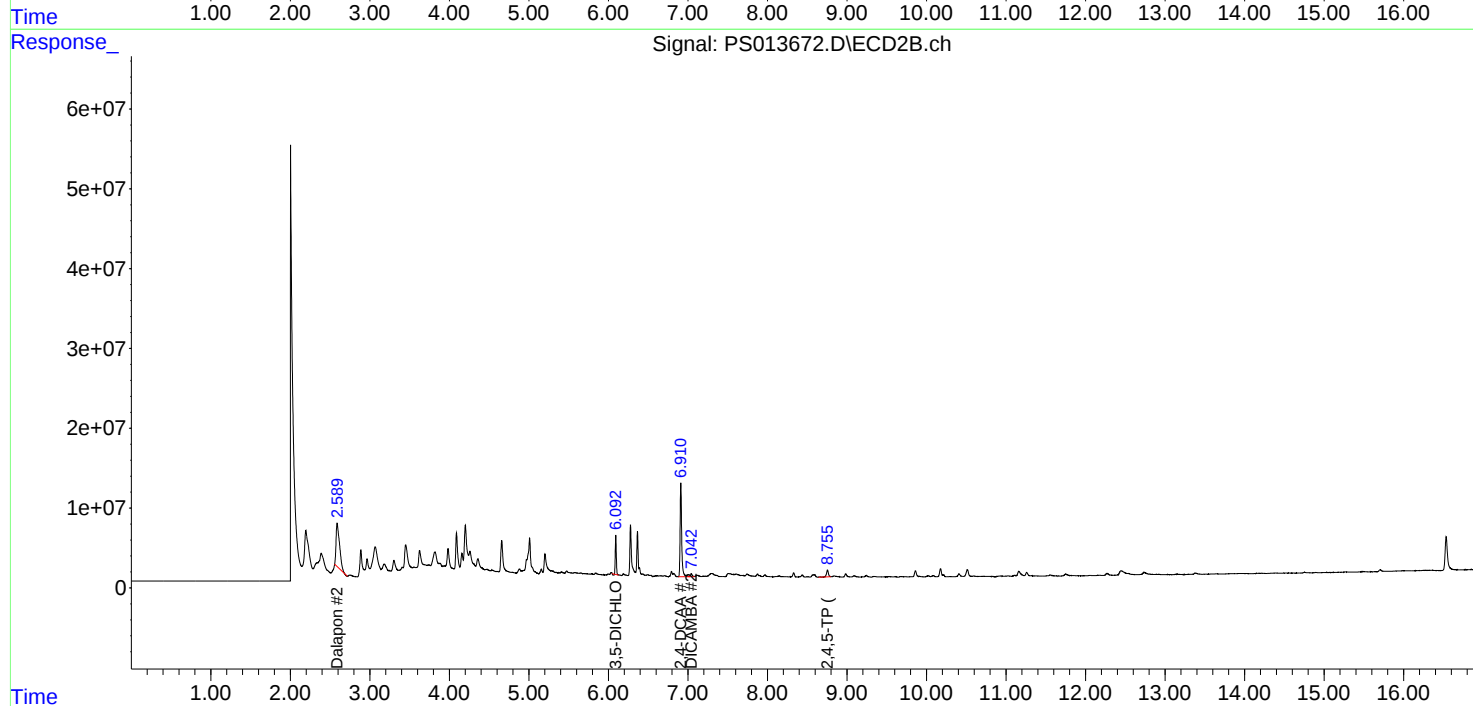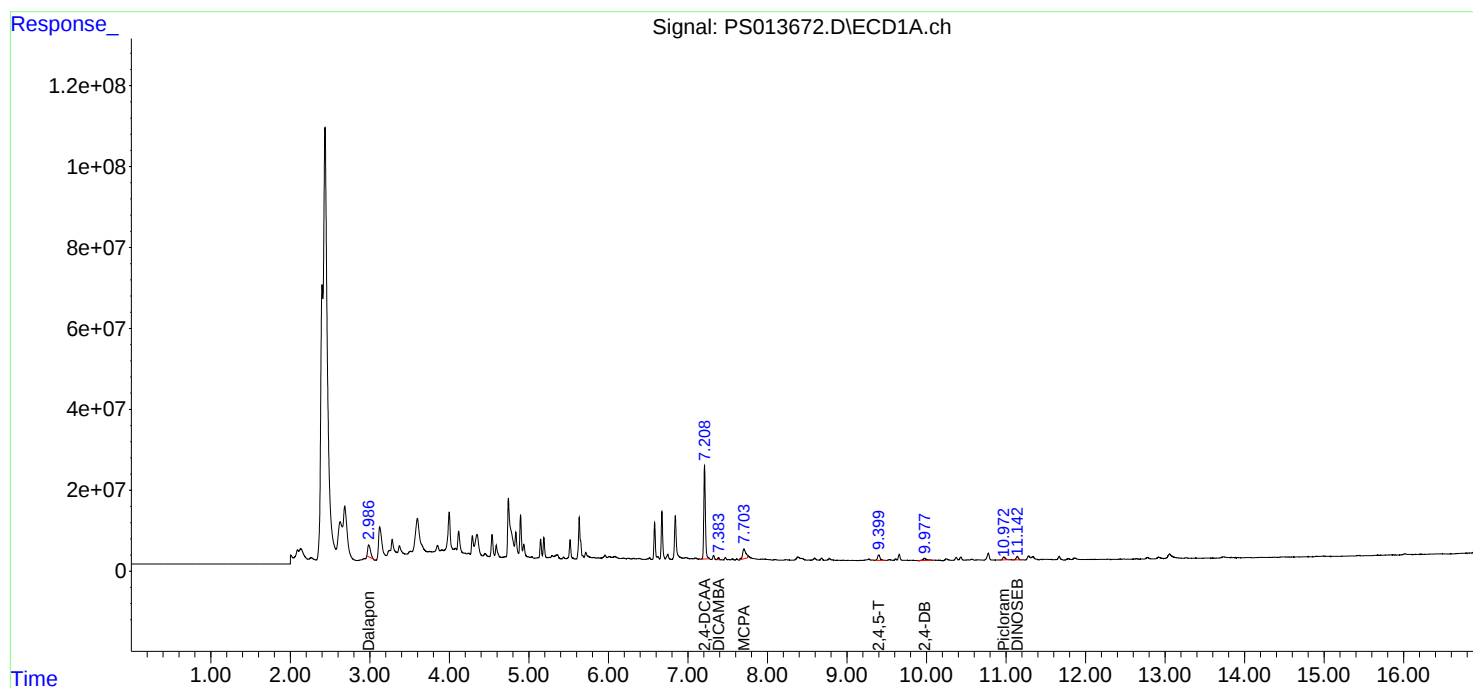


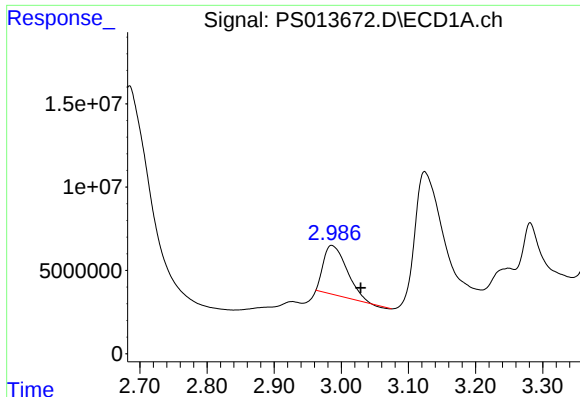

#1 Dalapon


R.T.: 2.985 min
Delta R.T.: -0.044 min
Response: 70869276
Conc: 65.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

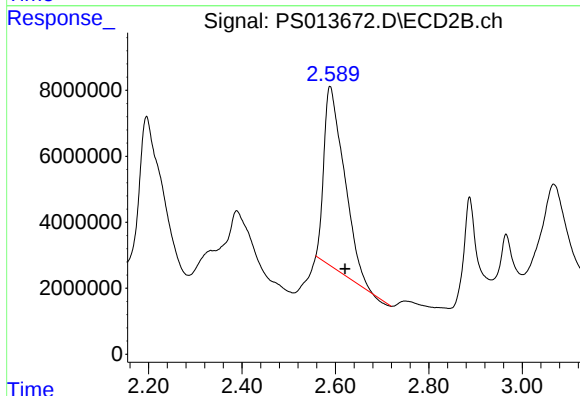


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.033 min
Response: 165093852
Conc: 317.52 ng/ml

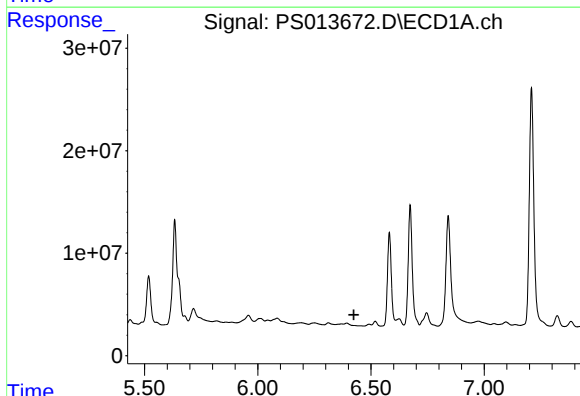


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

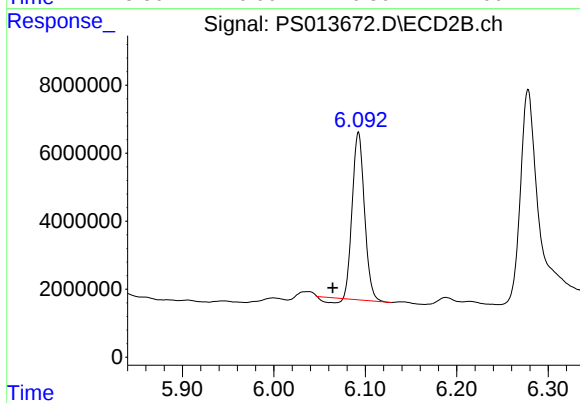

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.093 min
Delta R.T.: 0.028 min
Response: 44926137
Conc: 71.31 ng/ml

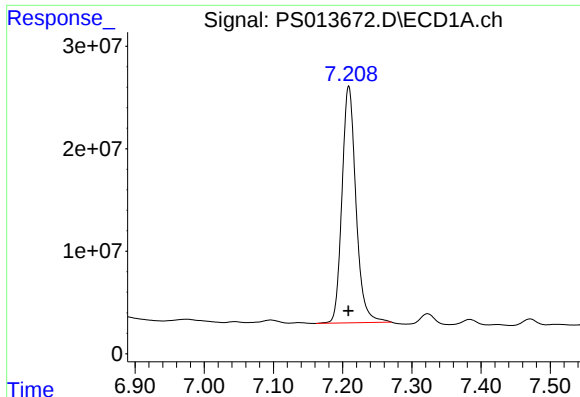

#4 2,4-DCAA


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 324479352
Conc: 339.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

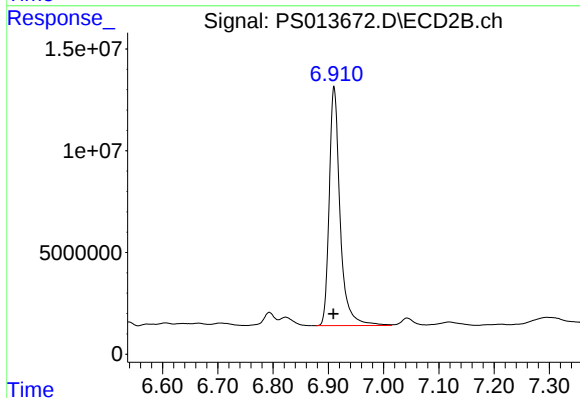


#4 2,4-DCAA

R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 160587150
Conc: 399.36 ng/ml

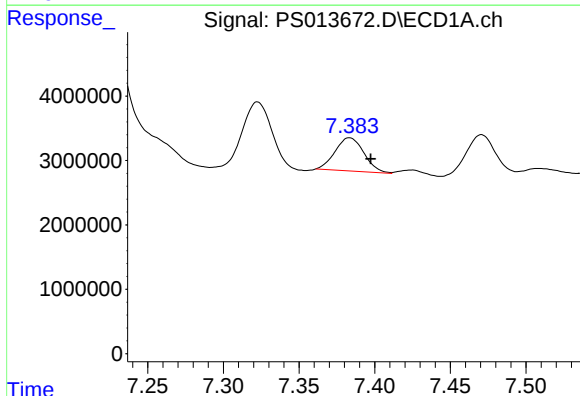


#5 DICAMBA

R.T.: 7.383 min
Delta R.T.: -0.014 min
Response: 6840558
Conc: 1.78 ng/ml

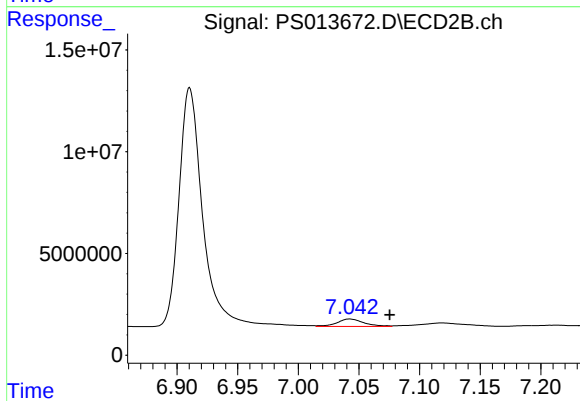

#5 DICAMBA


R.T.: 7.042 min
Delta R.T.: -0.033 min
Response: 5721087
Conc: 3.33 ng/ml

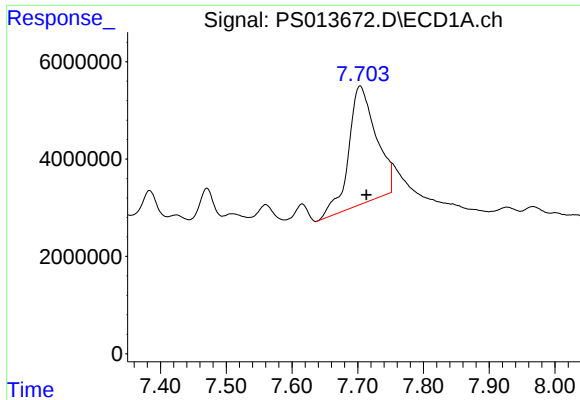

#7 MCPA


R.T.: 7.704 min
Delta R.T.: -0.010 min
Response: 70507835
Conc: 17.15 ug/ml

Instrument :
ECD_S
ClientSampleId :

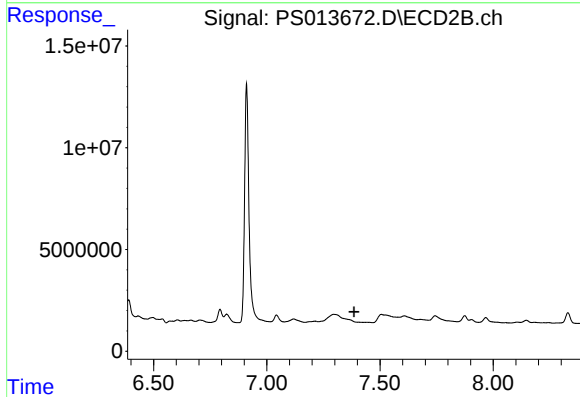


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

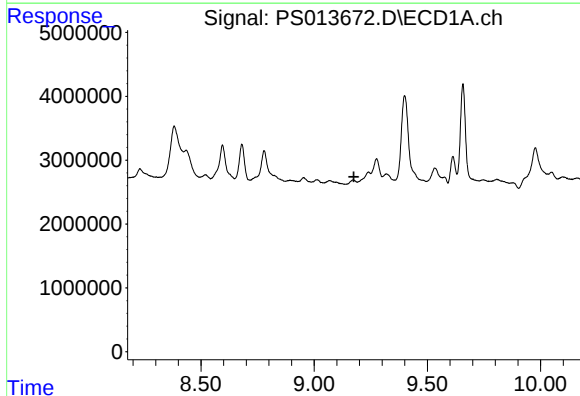


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.175 min
Response: 0
Conc: N.D.

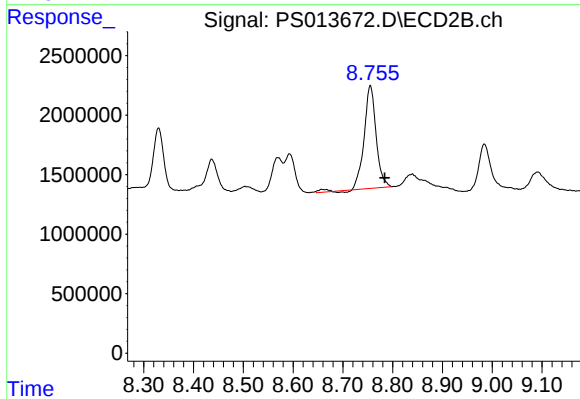

#11 2,4,5-TP (SILVEX)


R.T.: 8.755 min
Delta R.T.: -0.029 min
Response: 14521925
Conc: 6.08 ng/ml

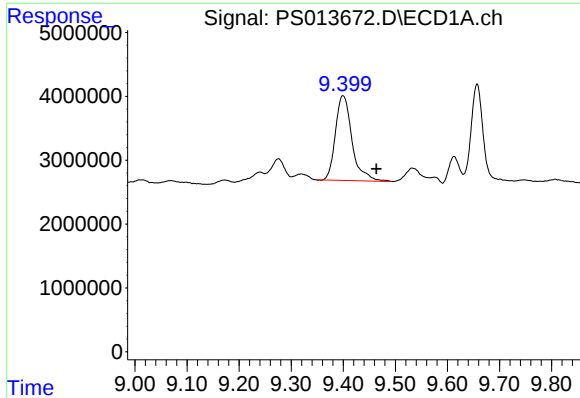

#12 2,4,5-T


R.T.: 9.399 min
Delta R.T.: -0.064 min
Response: 29456613
Conc: 5.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

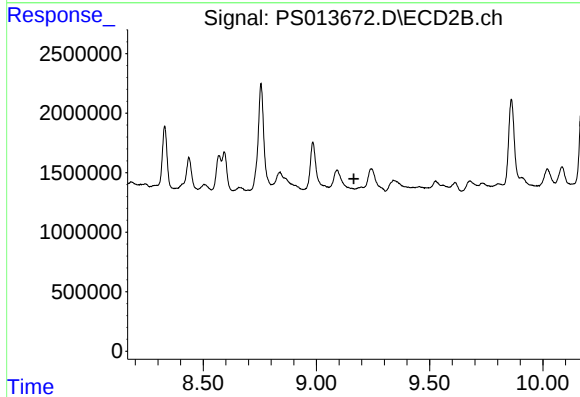


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.165 min
Response: 0
Conc: N.D.

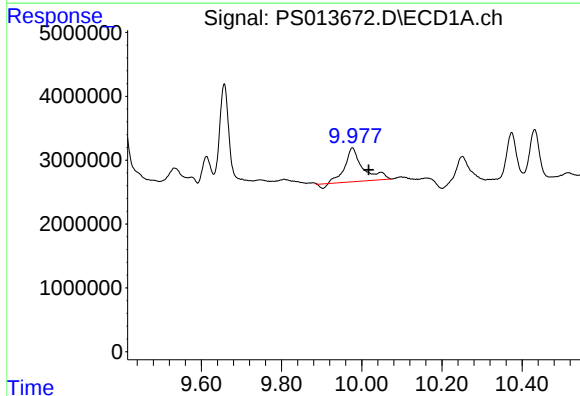


#13 2,4-DB

R.T.: 9.977 min
Delta R.T.: -0.041 min
Response: 16269310
Conc: 16.65 ng/ml

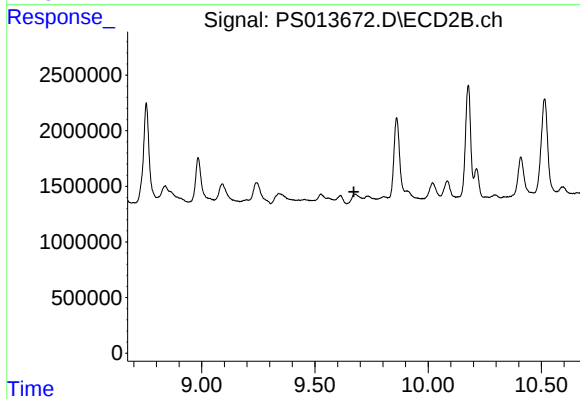

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

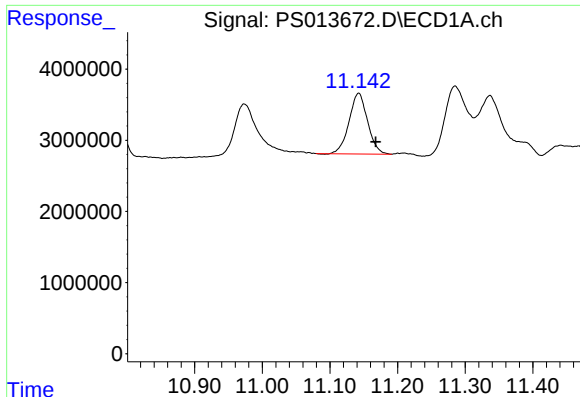

#14 DINOSEB


R.T.: 11.142 min
Delta R.T.: -0.025 min
Response: 16232839
Conc: 3.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

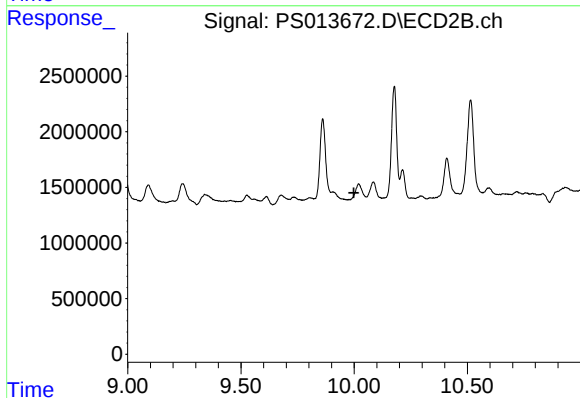


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.999 min
Response: 0
Conc: N.D.

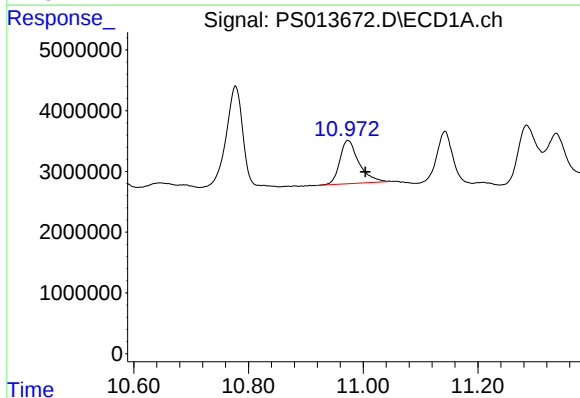

#15 Picloram

R.T.: 10.974 min
Delta R.T.: -0.031 min
Response: 16415812
Conc: 2.27 ng/ml

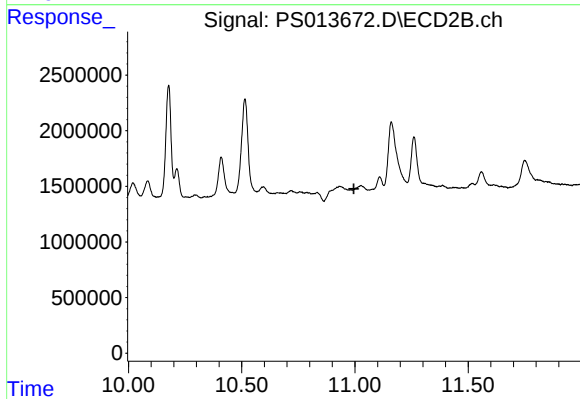

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.