

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 02:03
 Operator : DD\AJ
 Sample : L5242-21
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:35:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.209	6.911	335.2E6	165.2E6	350.790	410.783
Target Compounds							
1) T	Dalapon	2.987f	2.589	80567577	150.7E6	74.077	289.796 #
2) T	3,5-DICHL...	0.000	6.093	0	49850905	N.D.	79.128
5) T	DICAMBA	7.384	7.044	8332047	4813500	2.164	2.803 #
7) T	MCPA	7.709	0.000	43420689	0	10.564	N.D. #
10) T	Pentachlo...	8.681f	0.000	8300555	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.756	0	16652859	N.D.	6.971
12) T	2,4,5-T	9.403f	0.000	49441700	0	8.744	N.D. #
13) T	2,4-DB	9.976f	0.000	23881701	0	24.440	N.D. #
14) T	DINOSEB	11.143	0.000	17852675	0	4.047	N.D. #
15) T	Picloram	10.981	0.000	30100808	0	4.168	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 02:03
Operator : DD\AJ
Sample : L5242-21
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:35:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

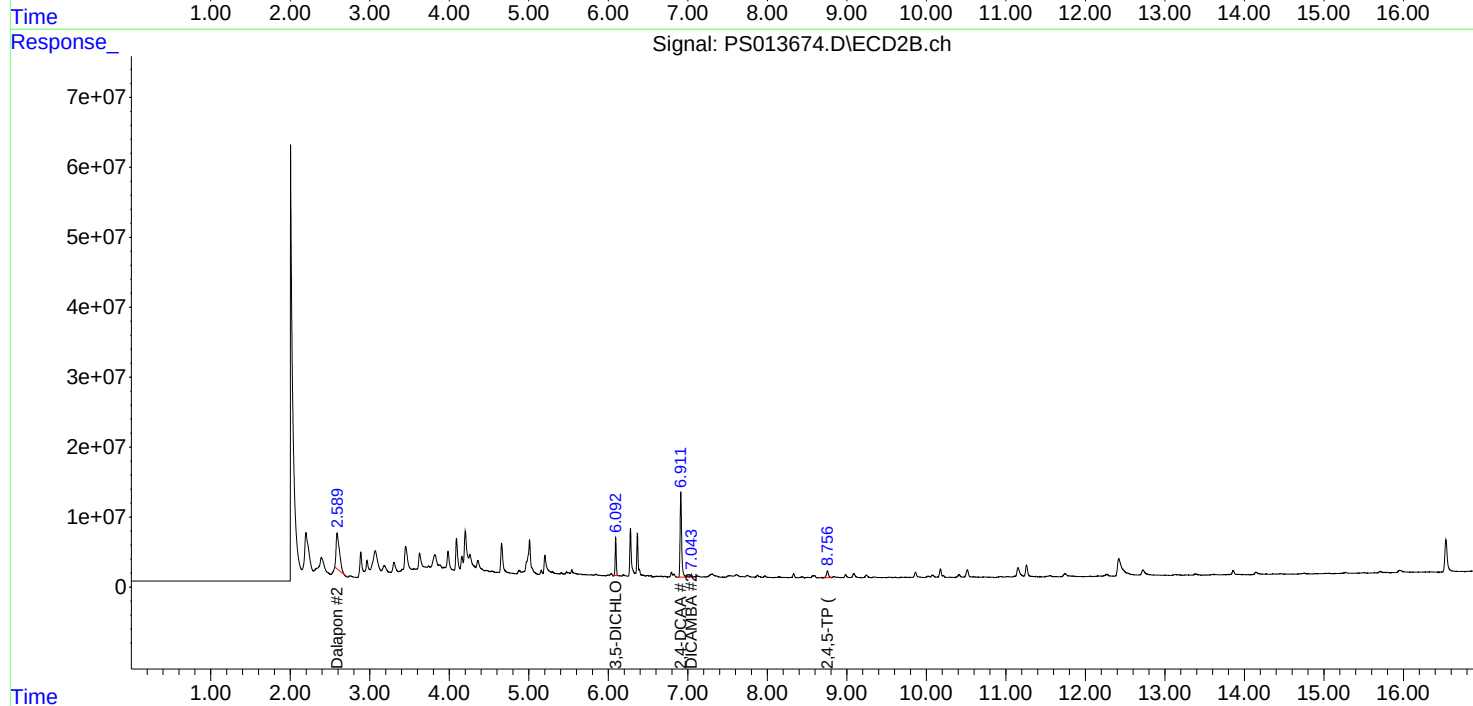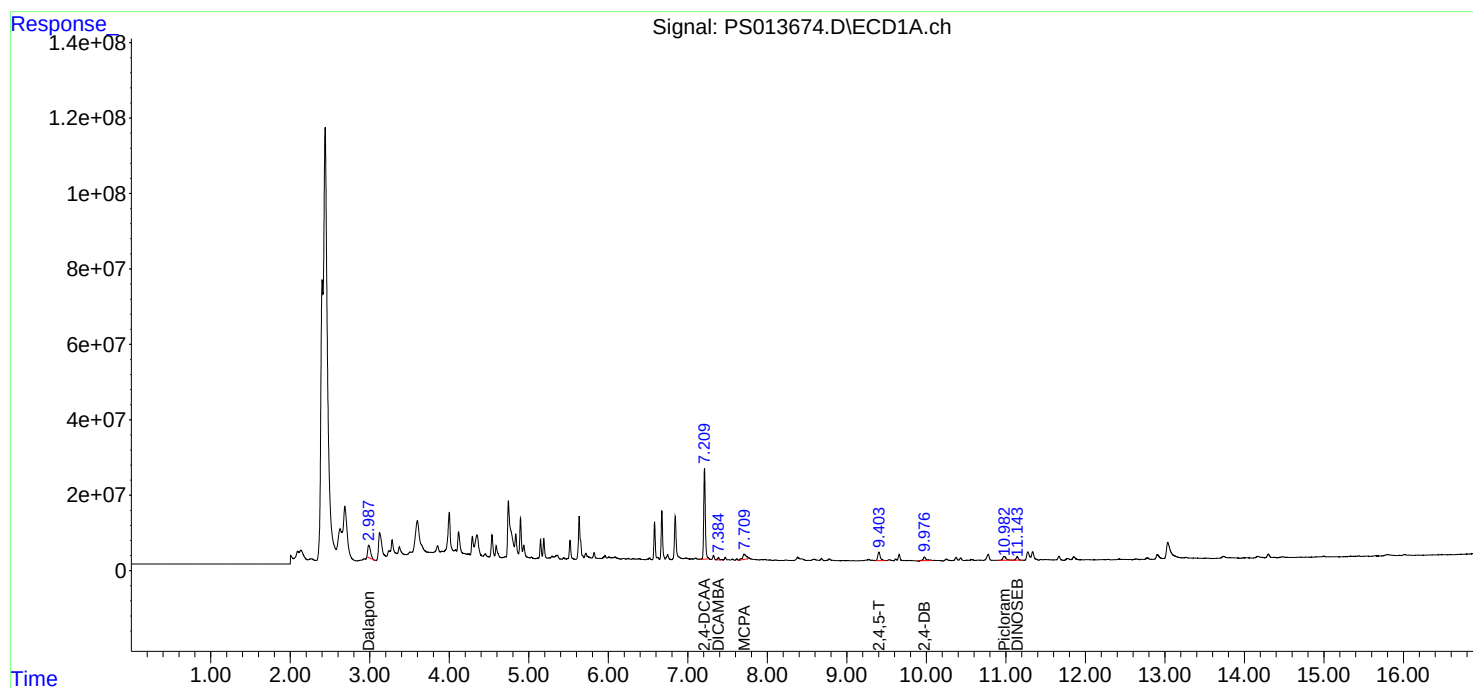


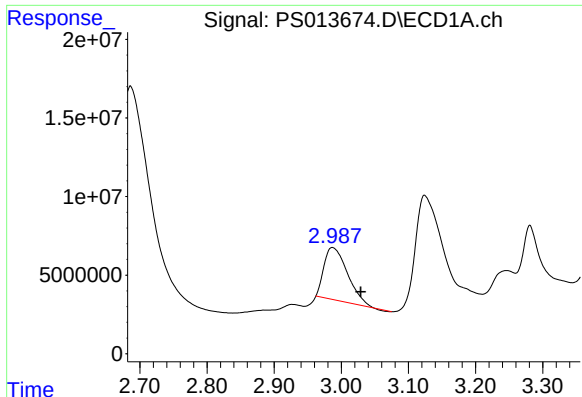

#1 Dalapon


R.T.: 2.987 min
Delta R.T.: -0.042 min
Response: 80567577
Conc: 74.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

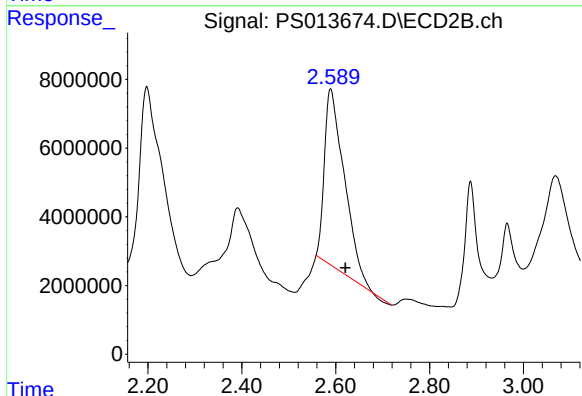


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.032 min
Response: 150679127
Conc: 289.80 ng/ml

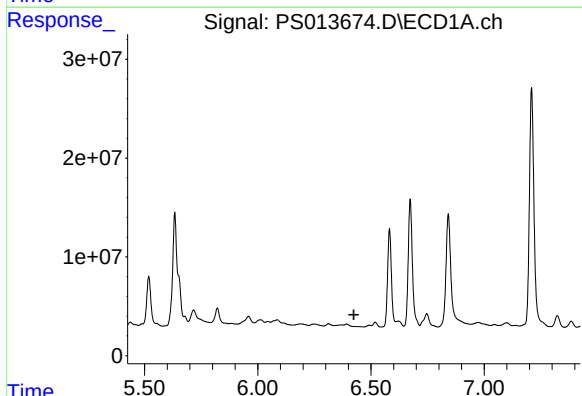


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

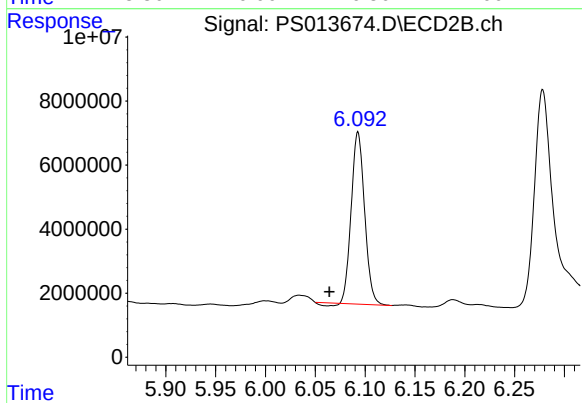

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.093 min
Delta R.T.: 0.029 min
Response: 49850905
Conc: 79.13 ng/ml

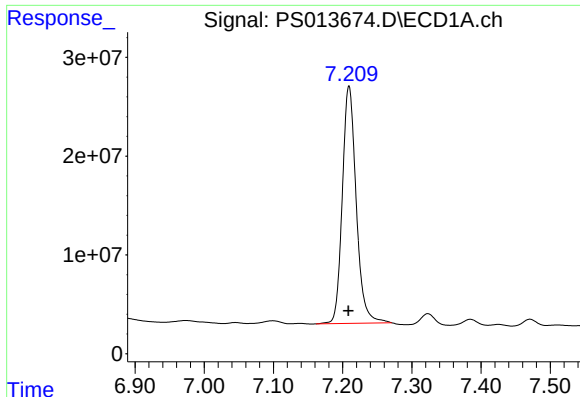

#4 2,4-DCAA


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 335212191
Conc: 350.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

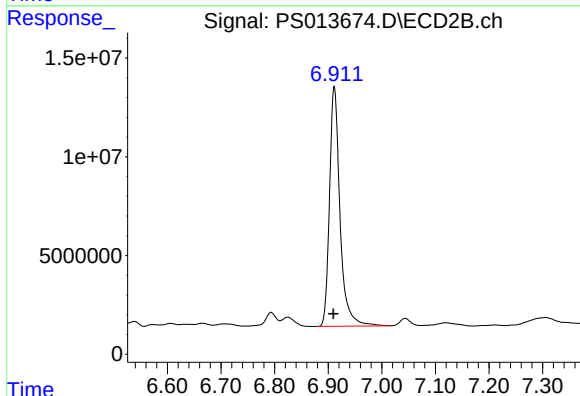


#4 2,4-DCAA

R.T.: 6.911 min
Delta R.T.: 0.002 min
Response: 165182155
Conc: 410.78 ng/ml

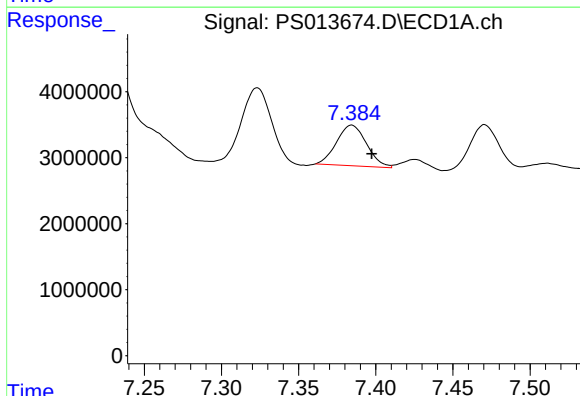


#5 DICAMBA

R.T.: 7.384 min
Delta R.T.: -0.013 min
Response: 8332047
Conc: 2.16 ng/ml

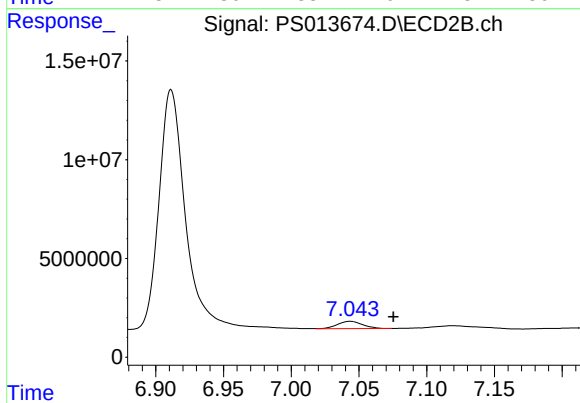

#5 DICAMBA


R.T.: 7.044 min
Delta R.T.: -0.032 min
Response: 4813500
Conc: 2.80 ng/ml

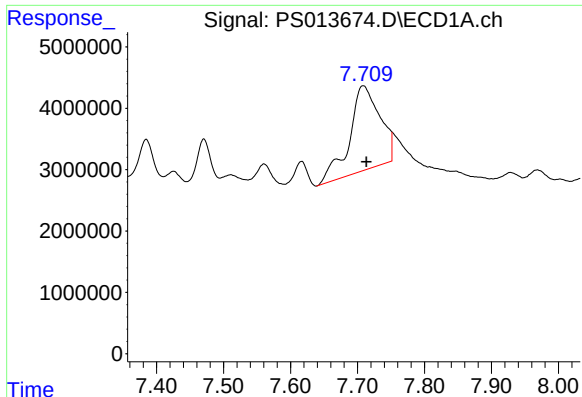

#7 MCPA


R.T.: 7.709 min
Delta R.T.: -0.005 min
Response: 43420689
Conc: 10.56 ug/ml

Instrument :
ECD_S
ClientSampleId :

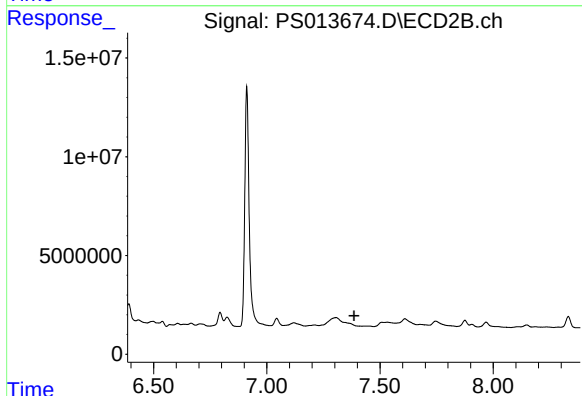


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

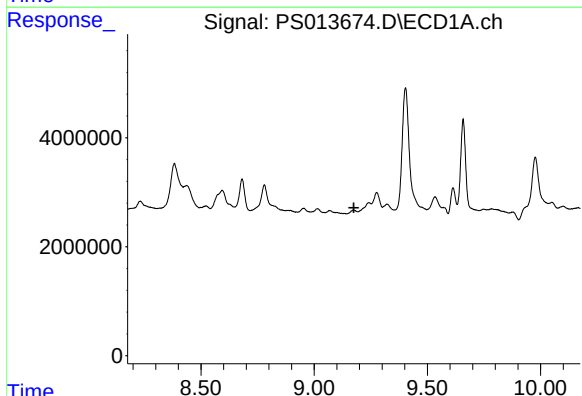


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.175 min
Response: 0
Conc: N.D.

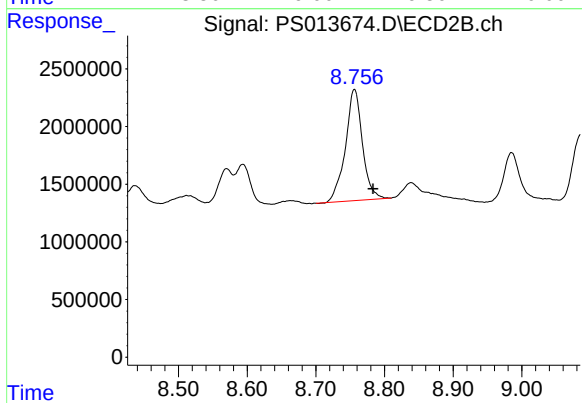

#11 2,4,5-TP (SILVEX)


R.T.: 8.756 min
Delta R.T.: -0.027 min
Response: 16652859
Conc: 6.97 ng/ml

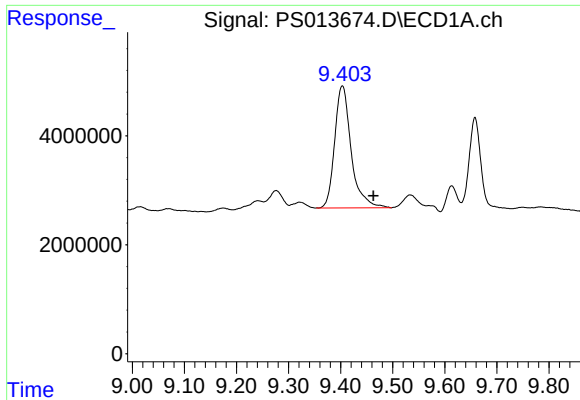

#12 2,4,5-T


R.T.: 9.403 min
Delta R.T.: -0.060 min
Response: 49441700
Conc: 8.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

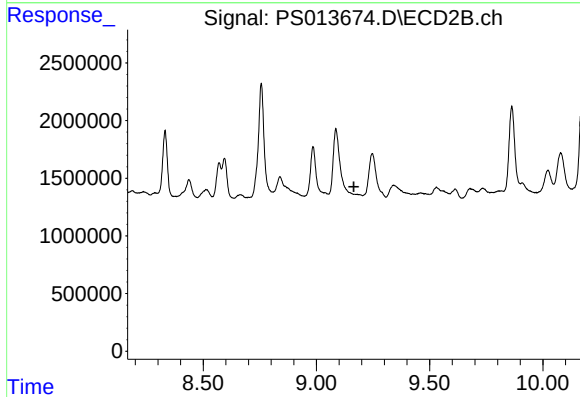


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.165 min
Response: 0
Conc: N.D.

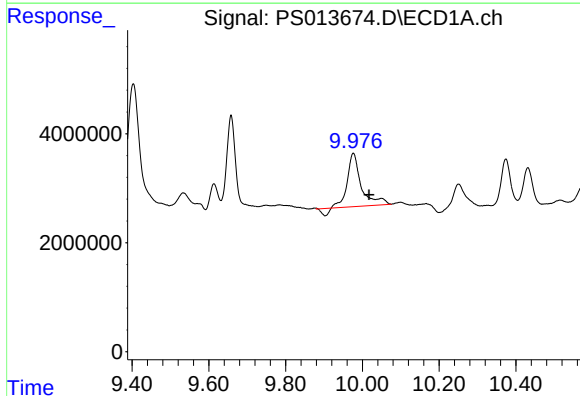


#13 2,4-DB

R.T.: 9.976 min
Delta R.T.: -0.041 min
Response: 23881701
Conc: 24.44 ng/ml

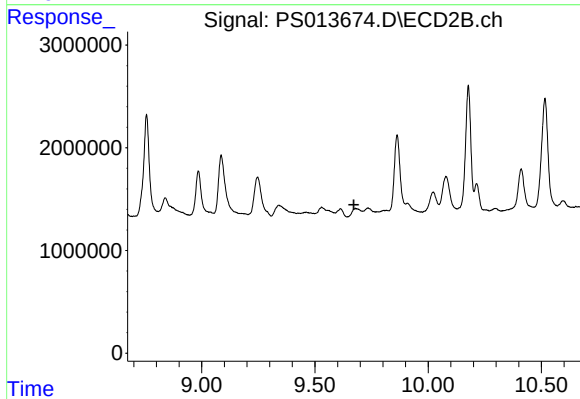

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

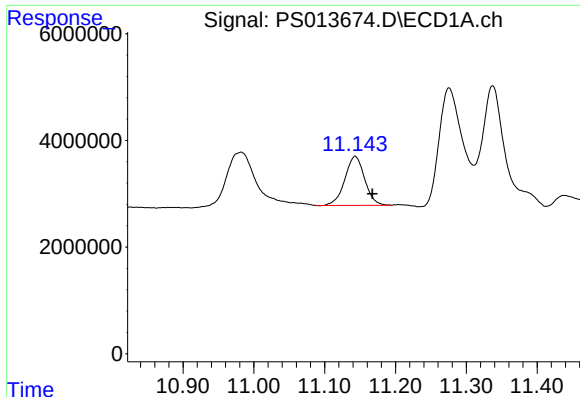

#14 DINOSEB


R.T.: 11.143 min
Delta R.T.: -0.024 min
Response: 17852675
Conc: 4.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

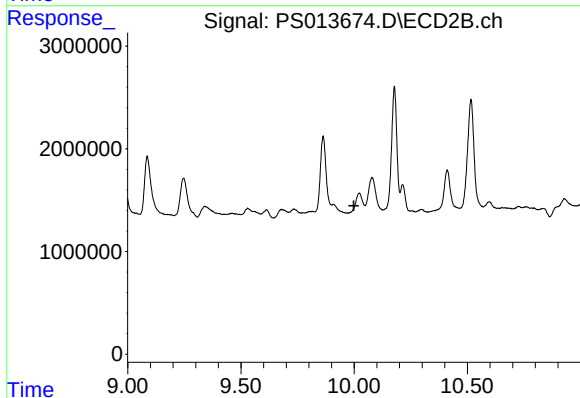


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.999 min
Response: 0
Conc: N.D.

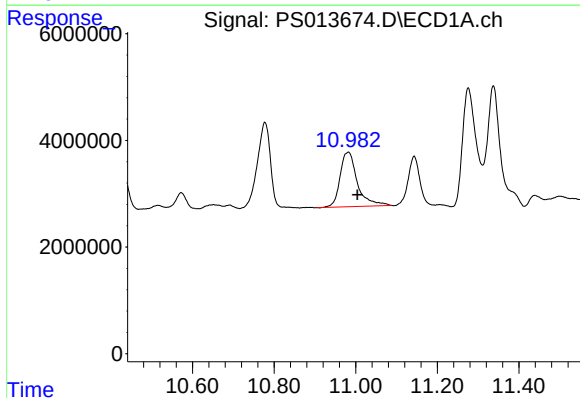

#15 Picloram

R.T.: 10.981 min
Delta R.T.: -0.023 min
Response: 30100808
Conc: 4.17 ng/ml

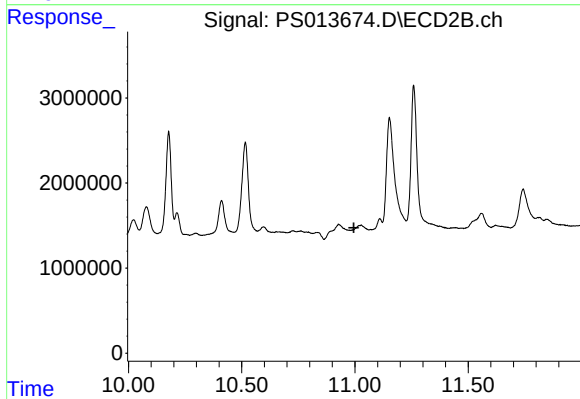

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.