

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 03:12
 Operator : DD\AJ
 Sample : L5242-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:36:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.209	6.911	533.5E6	261.9E6	558.329	651.356
Target Compounds							
1) T	Dalapon	2.986f	2.589	68339279	121.0E6	62.834	232.650 #
2) T	3,5-DICHL...	0.000	6.093	0	49197751	N.D.	78.091
5) T	DICAMBA	7.386	7.043	8878482	4355571	2.305	2.536
7) T	MCPA	7.717	0.000	14945288	0	3.636	N.D. #
8) T	DICHLORPROP	0.000	7.745f	0	2898070	N.D.	6.508
10) T	Pentachlo...	8.681f	8.436	7004638	6304917	<MDL	1.091 #
11) T	2,4,5-TP ...	0.000	8.807	0	21803886	N.D.	9.128
12) T	2,4,5-T	9.398f	0.000	24107862	0	4.263	N.D. #
13) T	2,4-DB	9.980	0.000	7075966	0	7.242	N.D. #
15) T	Picloram	10.976	11.023	20211368	9116546	2.798	2.623
16) T	DCPA	0.000	10.928	0	7654291	N.D.	2.473



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 03:12
Operator : DD\AJ
Sample : L5242-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:36:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

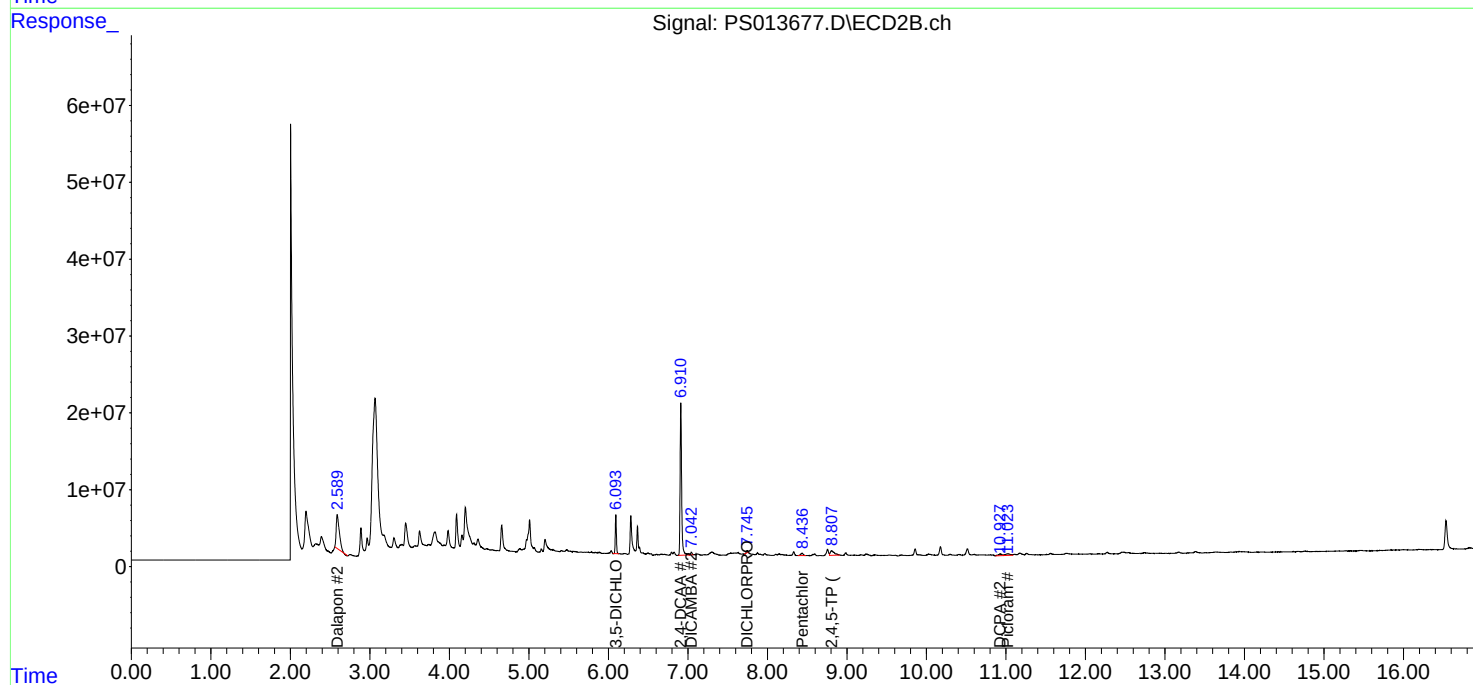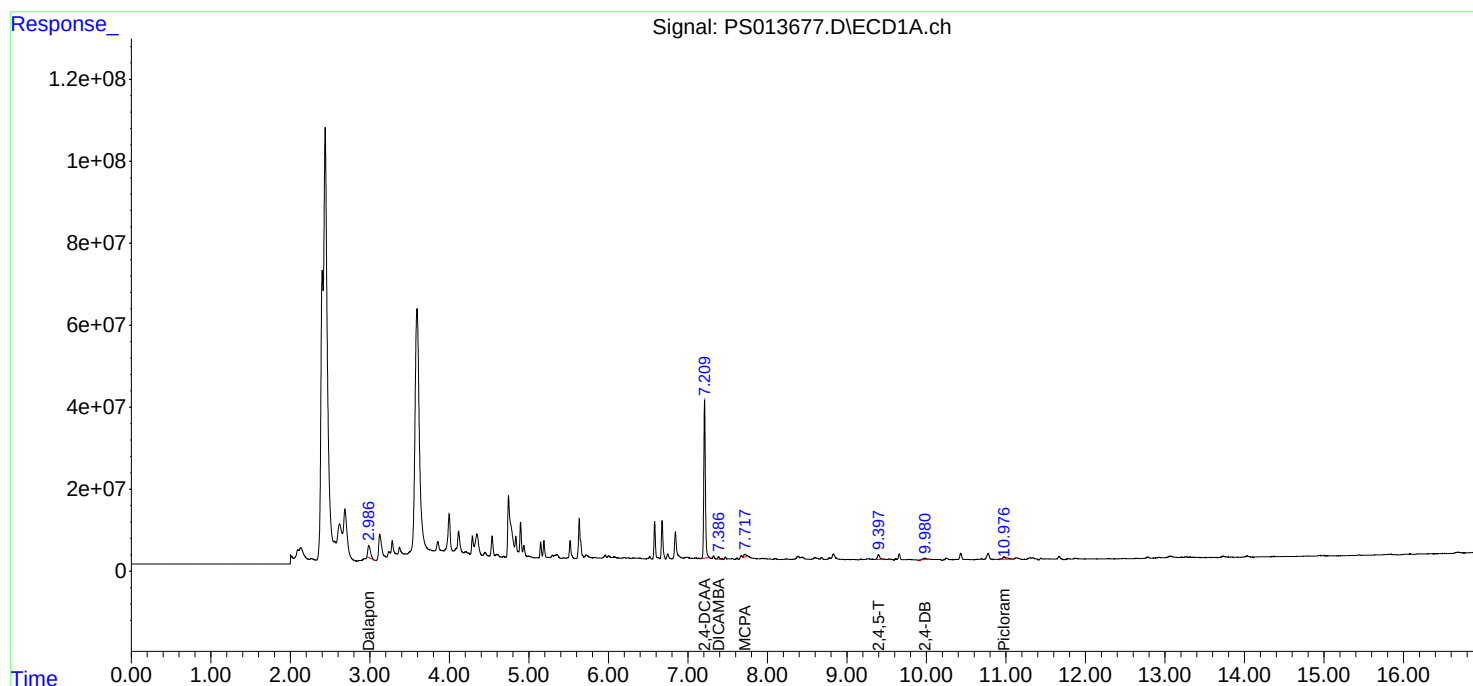


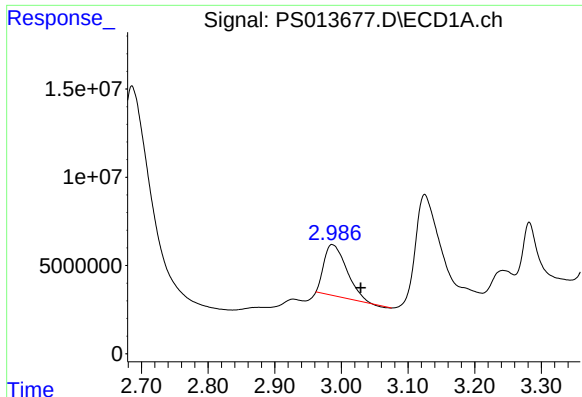

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: -0.043 min
Response: 68339279
Conc: 62.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

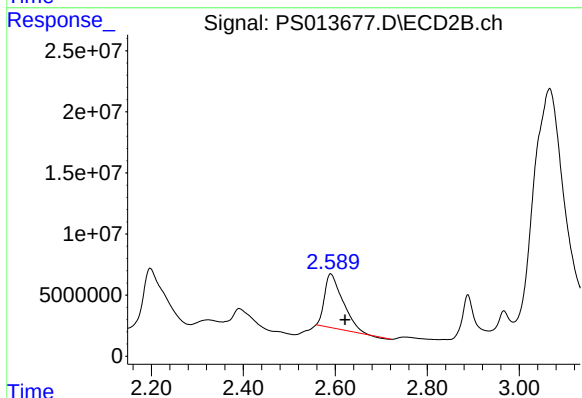


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.031 min
Response: 120966418
Conc: 232.65 ng/ml

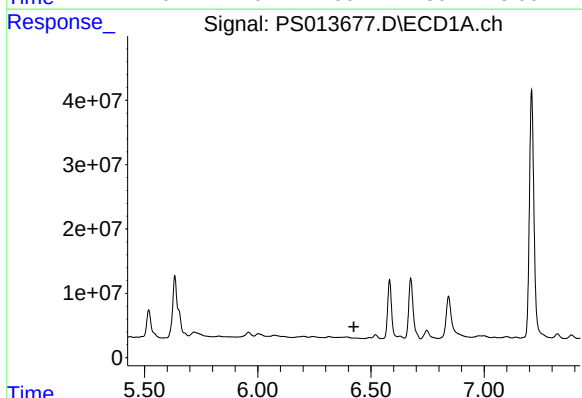


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

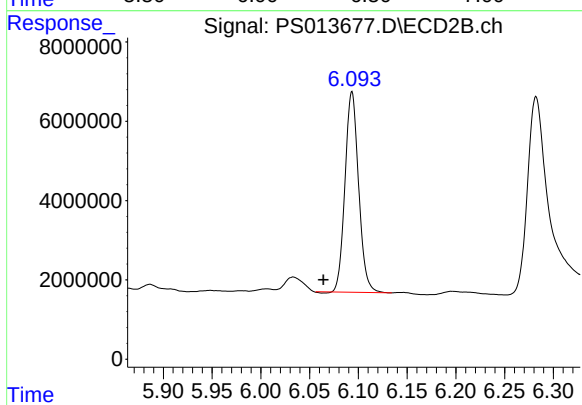

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.093 min
Delta R.T.: 0.029 min
Response: 49197751
Conc: 78.09 ng/ml

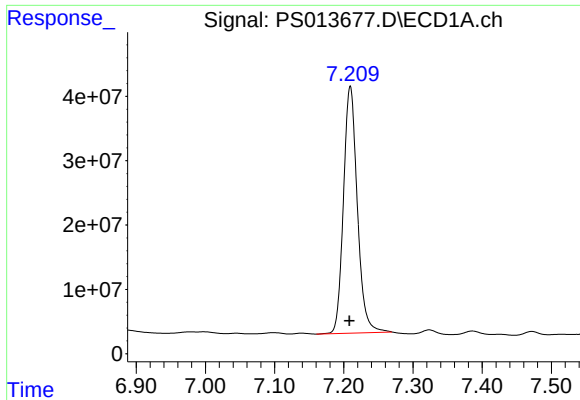

#4 2,4-DCAA


R.T.: 7.209 min
Delta R.T.: 0.001 min
Response: 533535525
Conc: 558.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

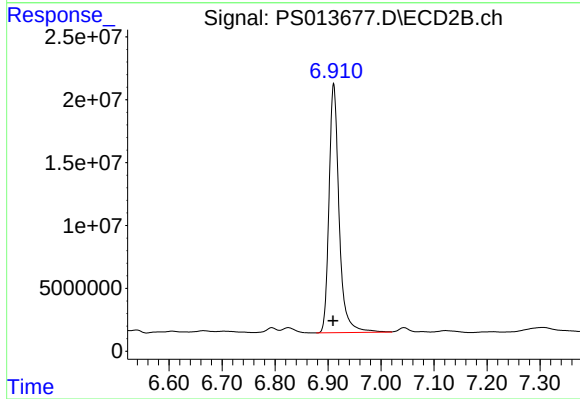


#4 2,4-DCAA

R.T.: 6.911 min
Delta R.T.: 0.001 min
Response: 261920099
Conc: 651.36 ng/ml

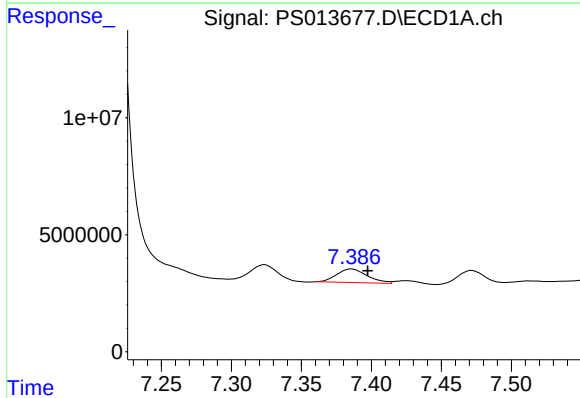


#5 DICAMBA

R.T.: 7.386 min
Delta R.T.: -0.012 min
Response: 8878482
Conc: 2.31 ng/ml

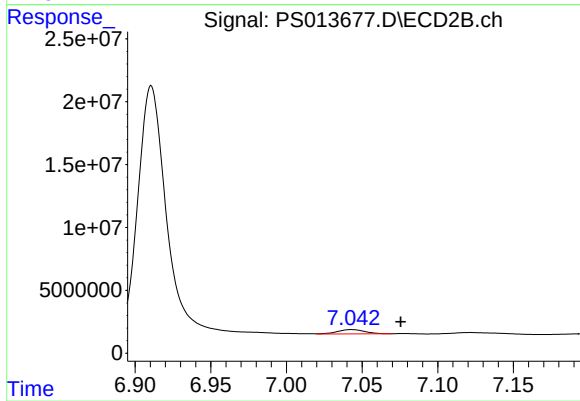

#5 DICAMBA


R.T.: 7.043 min
Delta R.T.: -0.032 min
Response: 4355571
Conc: 2.54 ng/ml

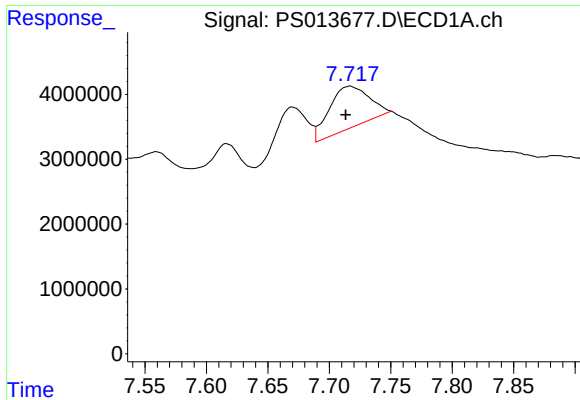

#7 MCPA


R.T.: 7.717 min
Delta R.T.: 0.003 min
Response: 14945288
Conc: 3.64 ug/ml

Instrument :
ECD_S
ClientSampleId :

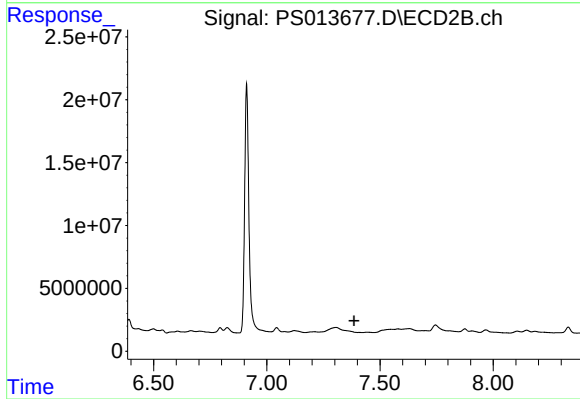


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

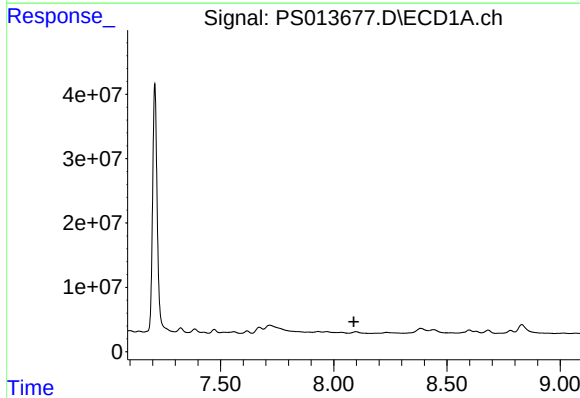


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.088 min
Response: 0
Conc: N.D.

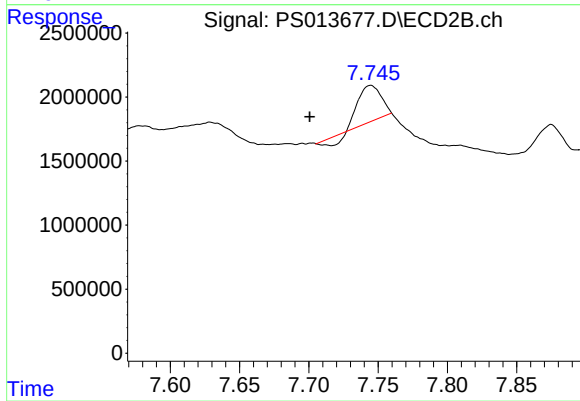

#8 DICHLORPROP


R.T.: 7.745 min
Delta R.T.: 0.044 min
Response: 2898070
Conc: 6.51 ng/ml

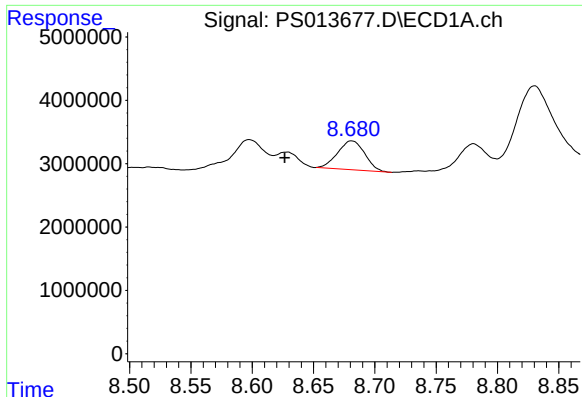

#10 Pentachlorophenol


R.T.: 8.681 min
Delta R.T.: 0.055 min
Response: 7004638
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

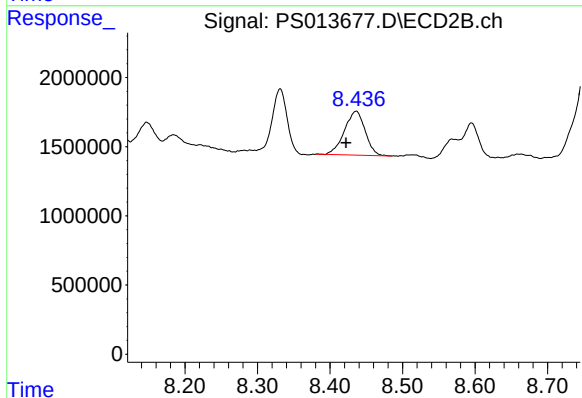


#10 Pentachlorophenol

R.T.: 8.436 min
Delta R.T.: 0.014 min
Response: 6304917
Conc: 1.09 ng/ml

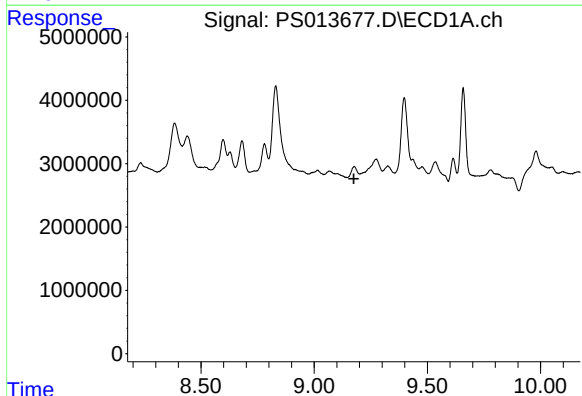


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.175 min
Response: 0
Conc: N.D.

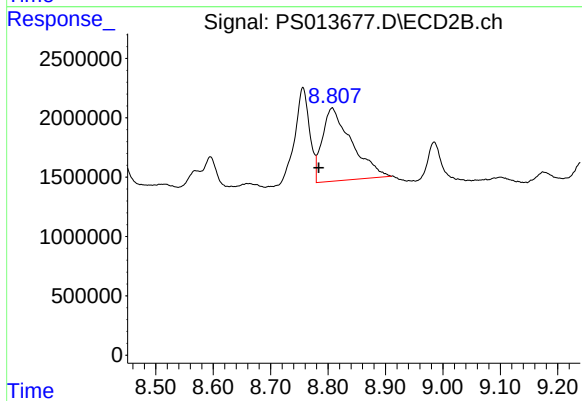

#11 2,4,5-TP (SILVEX)


R.T.: 8.807 min
Delta R.T.: 0.023 min
Response: 21803886
Conc: 9.13 ng/ml

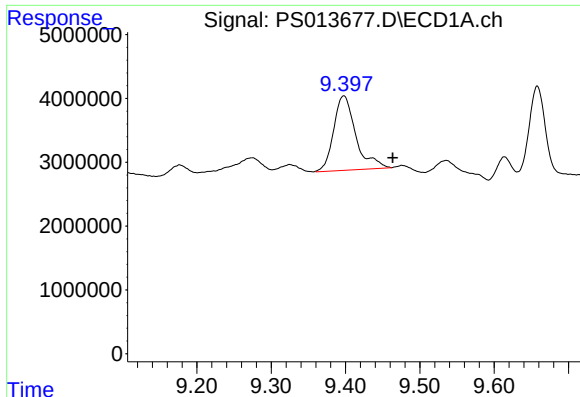

#12 2,4,5-T


R.T.: 9.398 min
Delta R.T.: -0.066 min
Response: 24107862
Conc: 4.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

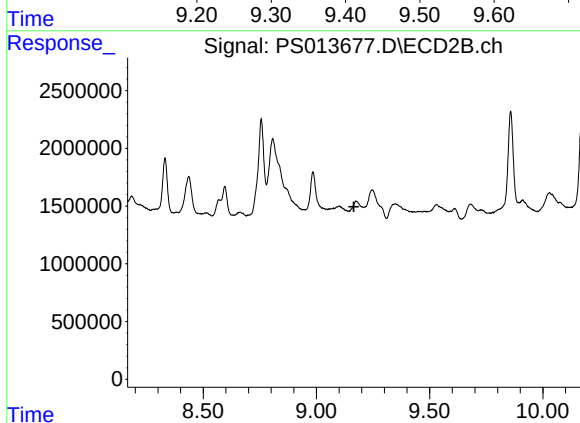


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.165 min
Response: 0
Conc: N.D.

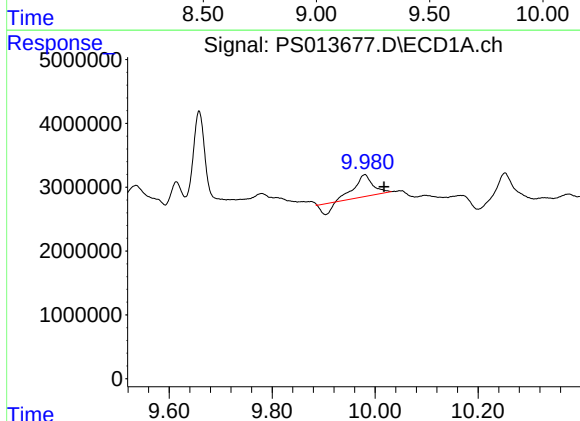


#13 2,4-DB

R.T.: 9.980 min
Delta R.T.: -0.037 min
Response: 7075966
Conc: 7.24 ng/ml

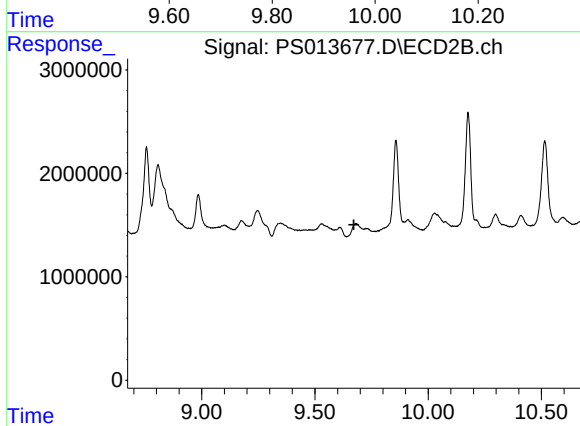

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

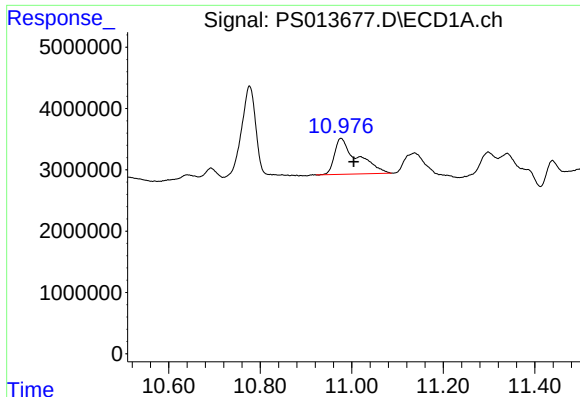

#15 Picloram


R.T.: 10.976 min
Delta R.T.: -0.028 min
Response: 20211368
Conc: 2.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

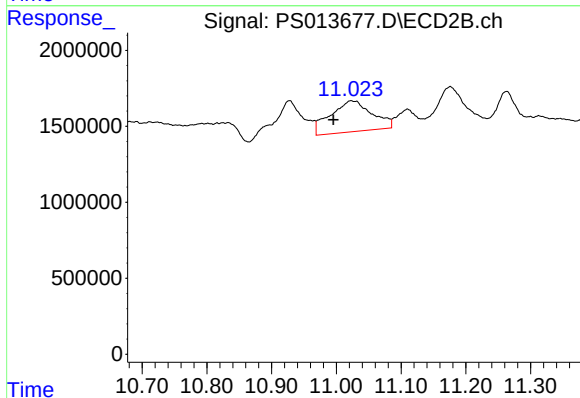


#15 Picloram

R.T.: 11.023 min
Delta R.T.: 0.027 min
Response: 9116546
Conc: 2.62 ng/ml

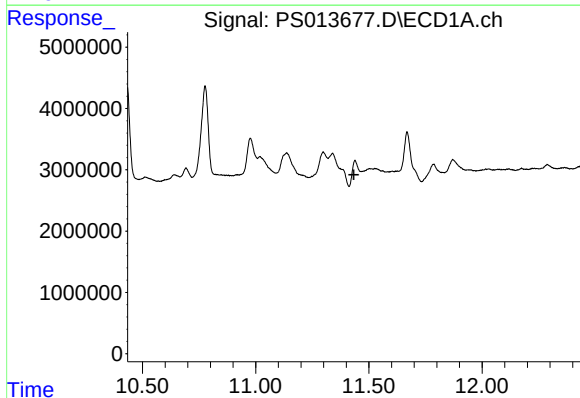

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.433 min
Response: 0
Conc: N.D.

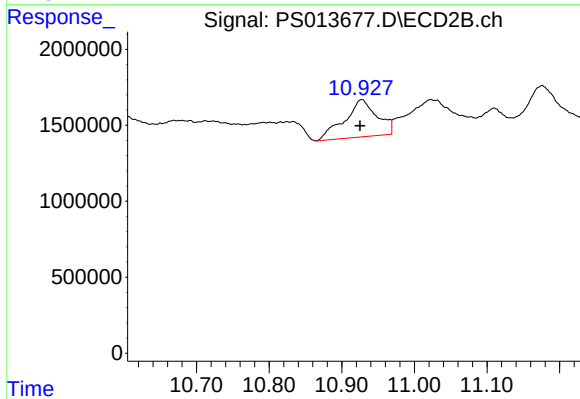

#16 DCPA

R.T.: 10.928 min
Delta R.T.: 0.002 min
Response: 7654291
Conc: 2.47 ng/ml