

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 11:20
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 12:09:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.907	397.0E6	198.3E6	415.410	493.092
Target Compounds							
5) T	DICAMBA	0.000	7.076	0	4570607	N.D.	2.661
6) T	MCPD	0.000	7.137	0	4395170	N.D.	3.110
9) T	2,4-D	8.319	0.000	32677595	0	30.848	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 11:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 12:09:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

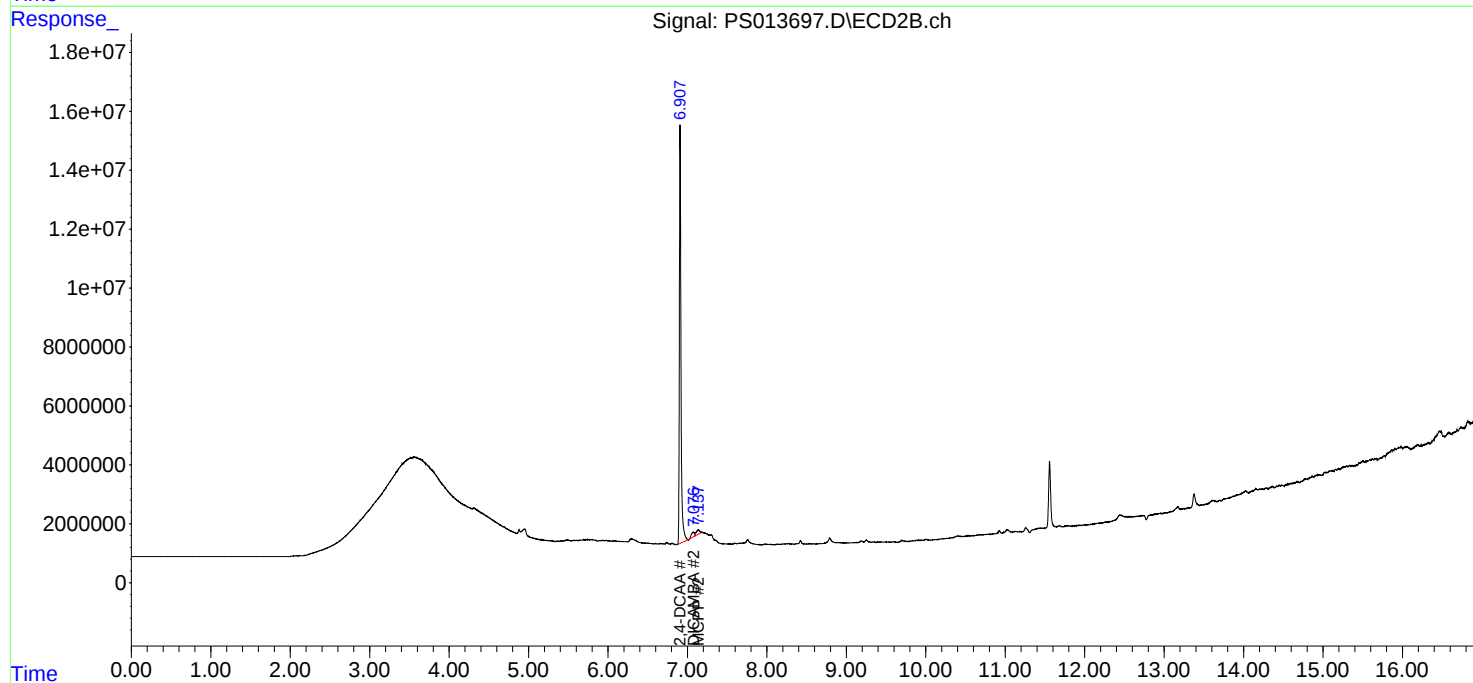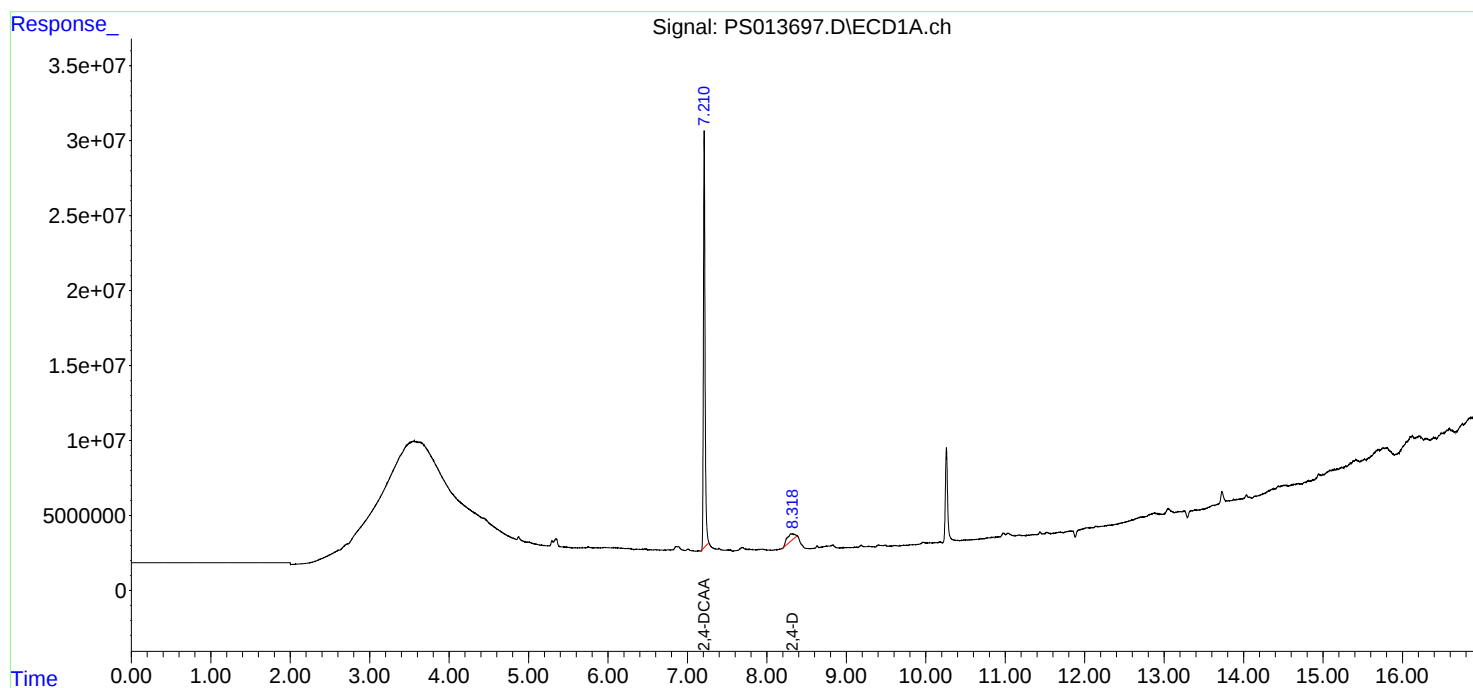


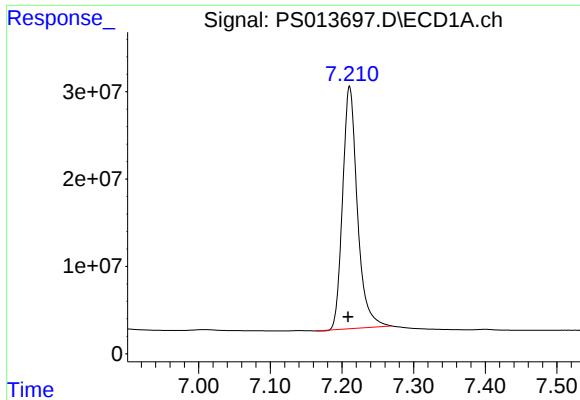

#4 2,4-DCAA


R.T.: 7.211 min
Delta R.T.: 0.002 min
Response: 396963262
Conc: 415.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

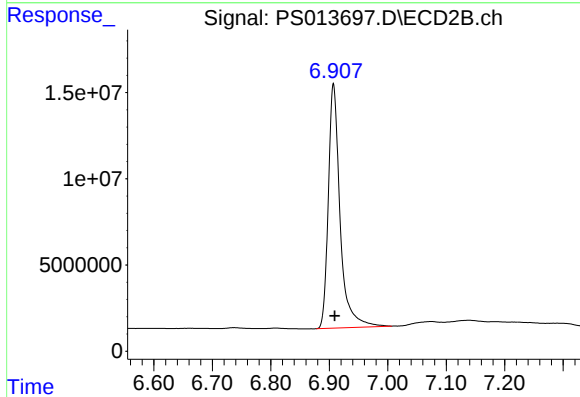


#4 2,4-DCAA

R.T.: 6.907 min
Delta R.T.: -0.002 min
Response: 198279610
Conc: 493.09 ng/ml

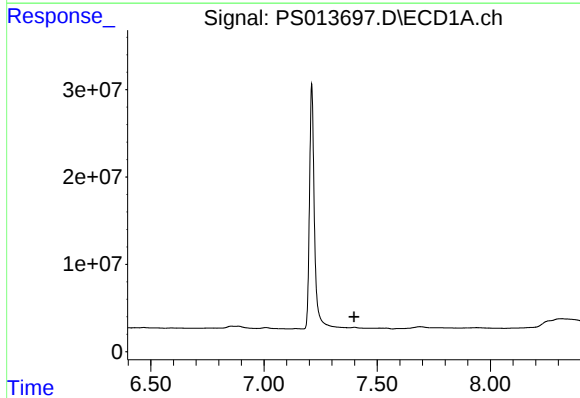


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.397 min
Response: 0
Conc: N.D.

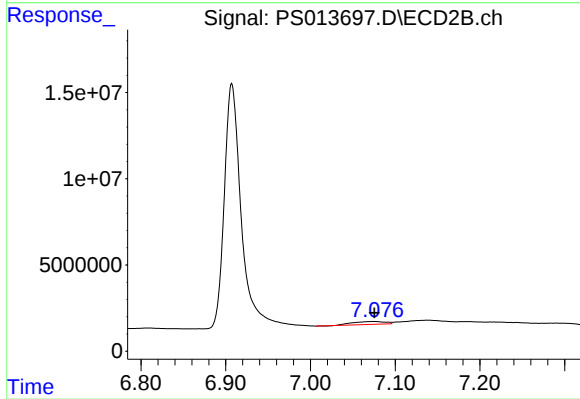

#5 DICAMBA


R.T.: 7.076 min
Delta R.T.: 0.000 min
Response: 4570607
Conc: 2.66 ng/ml

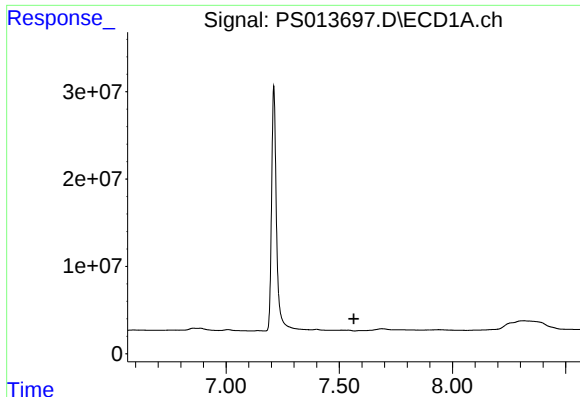

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

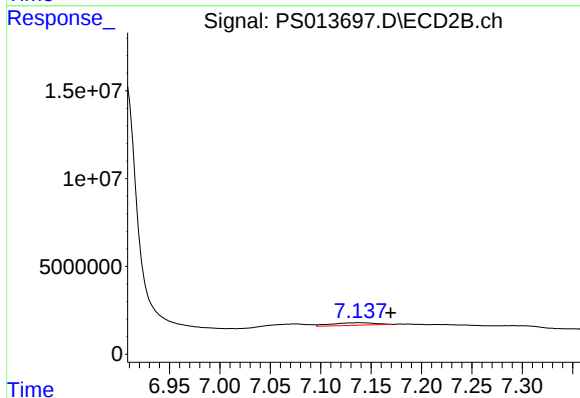


#6 MCP

R.T.: 7.137 min
Delta R.T.: -0.032 min
Response: 4395170
Conc: 3.11 ug/ml

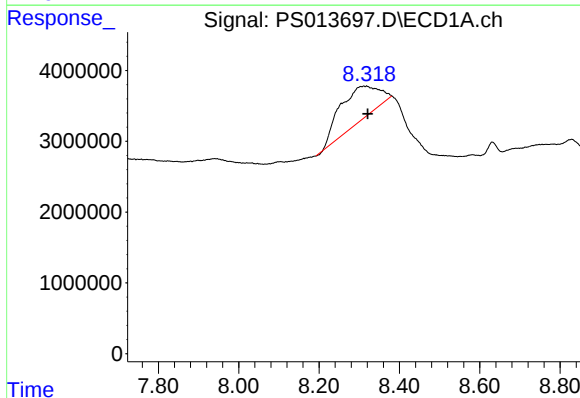

#9 2,4-D

R.T.: 8.319 min
Delta R.T.: -0.002 min
Response: 32677595
Conc: 30.85 ng/ml

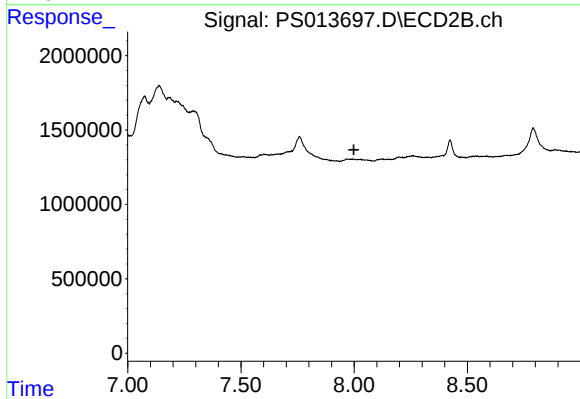

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.999 min
Response: 0
Conc: N.D.