

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 15:03
 Operator : DD\AJ
 Sample : L5242-18RE
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 16:25:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.208	6.908	713.9E6	343.6E6	747.059	854.556
Target Compounds							
1) T	Dalapon	2.986f	2.589	72334283	138.5E6	66.507	266.355 #
2) T	3,5-DICHL...	0.000	6.092	0	53268735	N.D.	84.553
5) T	DICAMBA	7.384	7.041	7786755	4840449	2.022	2.819 #
7) T	MCPA	7.703	0.000	18034173	0	4.388	N.D. #
8) T	DICHLORPROP	0.000	7.737	0	13470769	N.D.	30.249
10) T	Pentachlo...	8.681f	0.000	7060207	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.754	0	14257094	N.D.	5.968
12) T	2,4,5-T	9.399f	0.000	19788029	0	3.499	N.D. #
13) T	2,4-DB	9.976f	0.000	10351300	0	10.593	N.D. #
14) T	DINOSEB	11.141	0.000	14925584	0	3.383	N.D. #
15) T	Picloram	10.969	0.000	24961199	0	3.456	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 15:03
Operator : DD\AJ
Sample : L5242-18RE
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 16:25:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

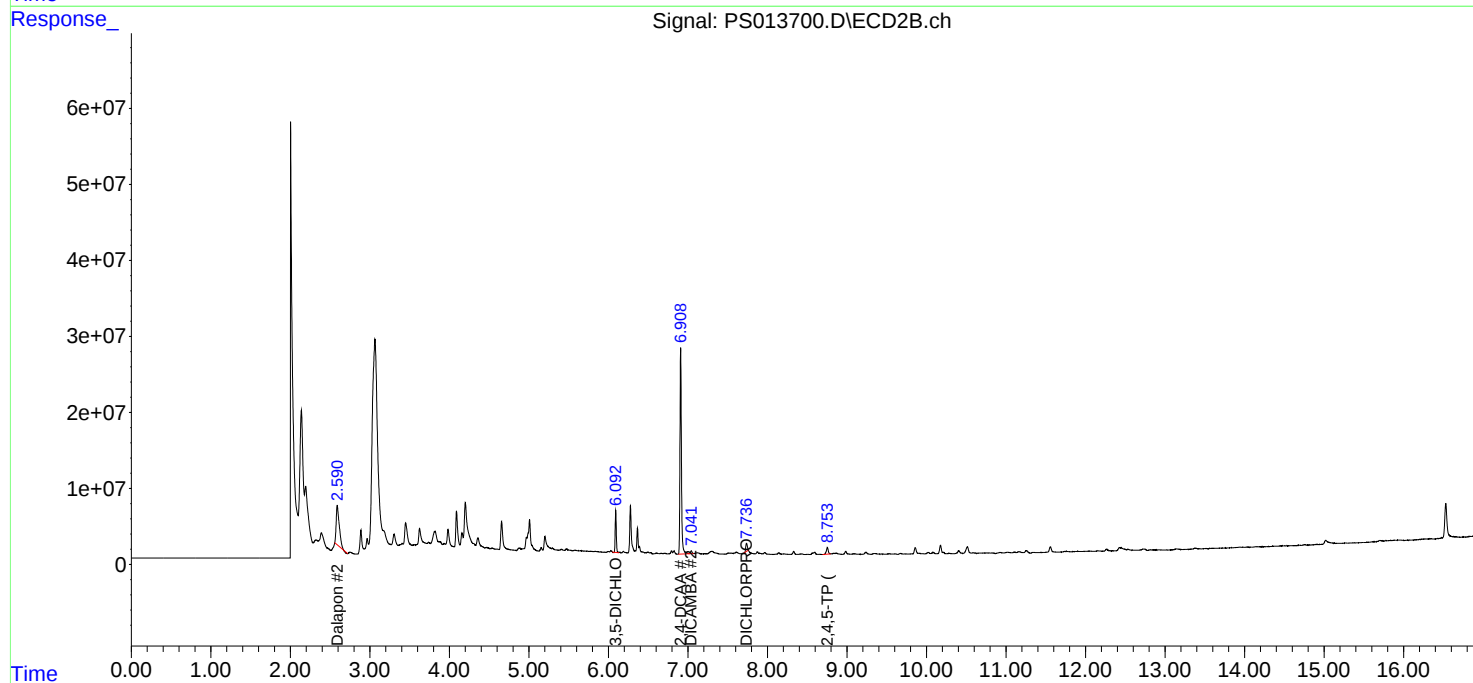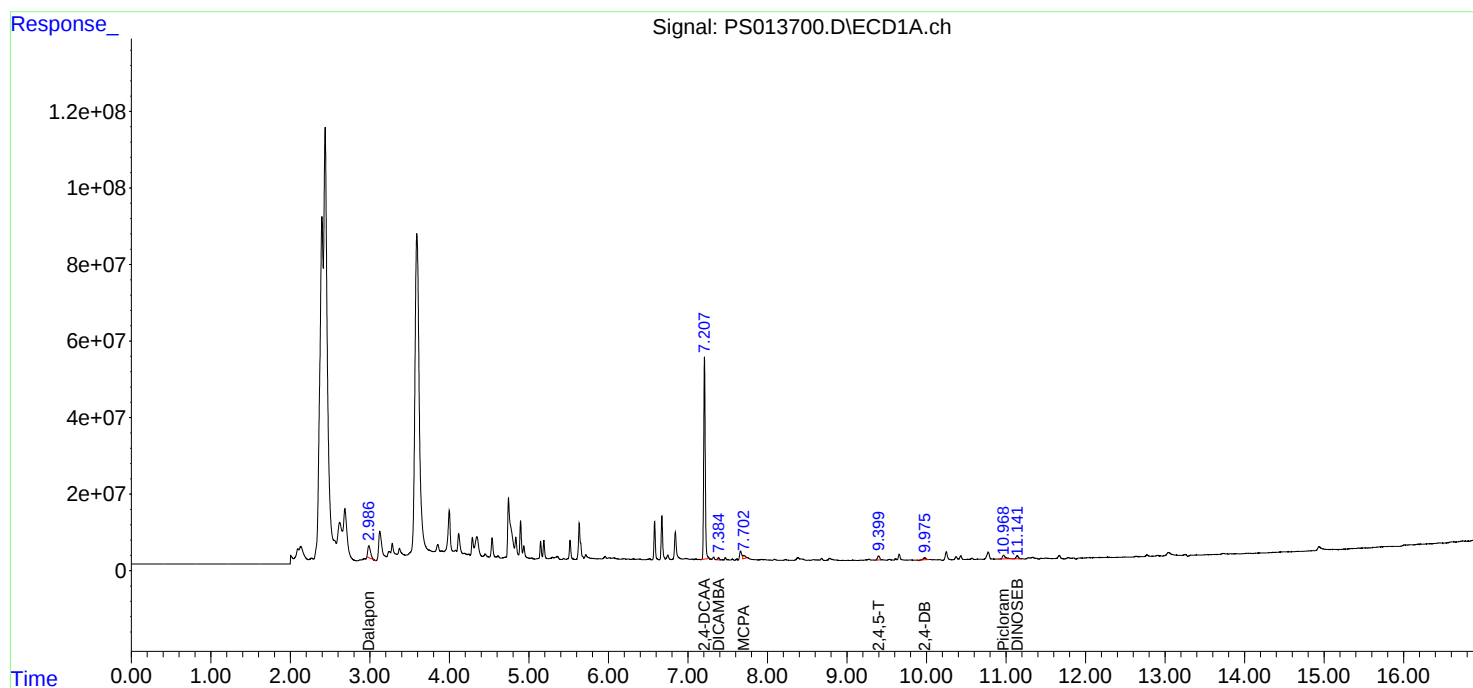


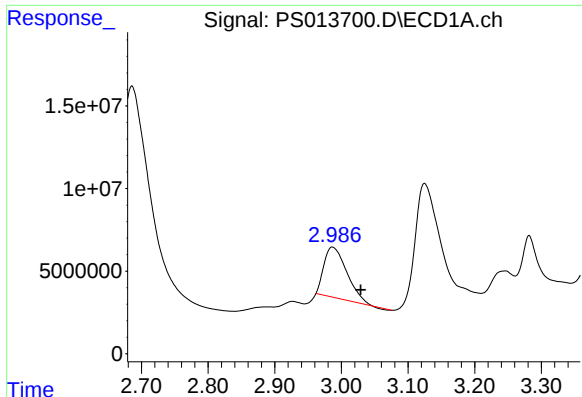

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: -0.043 min
Response: 72334283
Conc: 66.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

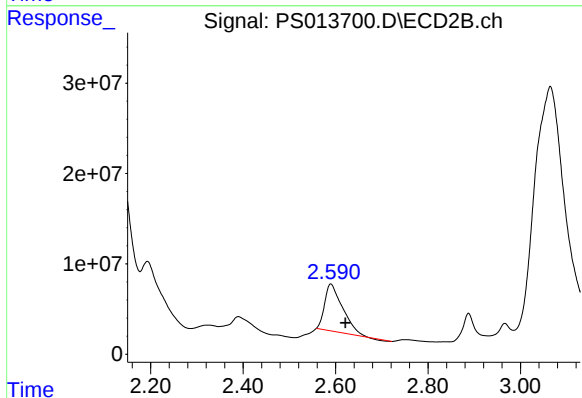


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.032 min
Response: 138491289
Conc: 266.36 ng/ml

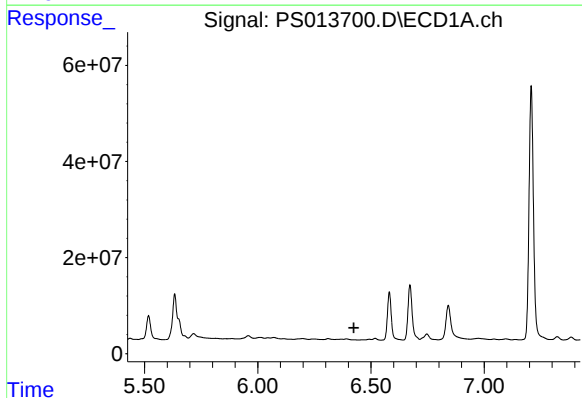


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

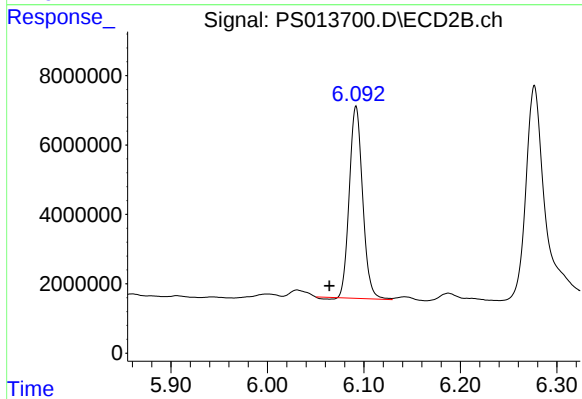

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.092 min
Delta R.T.: 0.028 min
Response: 53268735
Conc: 84.55 ng/ml

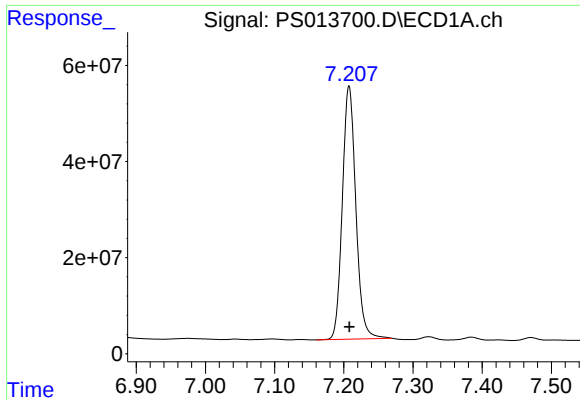

#4 2,4-DCAA


R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 713884613
Conc: 747.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

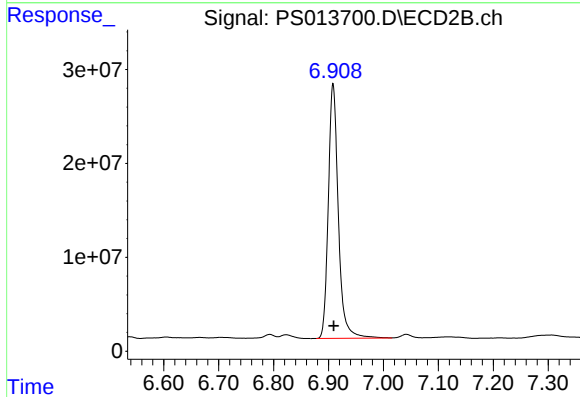


#4 2,4-DCAA

R.T.: 6.908 min
Delta R.T.: -0.001 min
Response: 343629642
Conc: 854.56 ng/ml

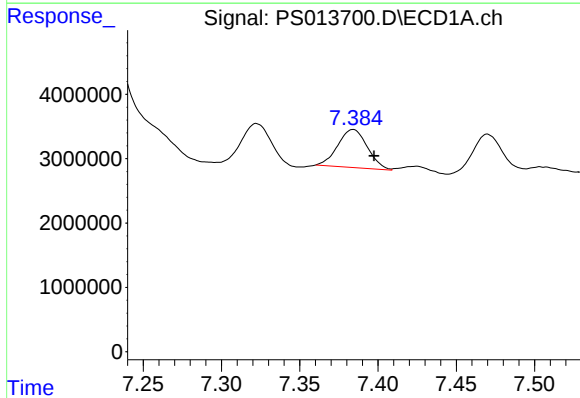


#5 DICAMBA

R.T.: 7.384 min
Delta R.T.: -0.013 min
Response: 7786755
Conc: 2.02 ng/ml

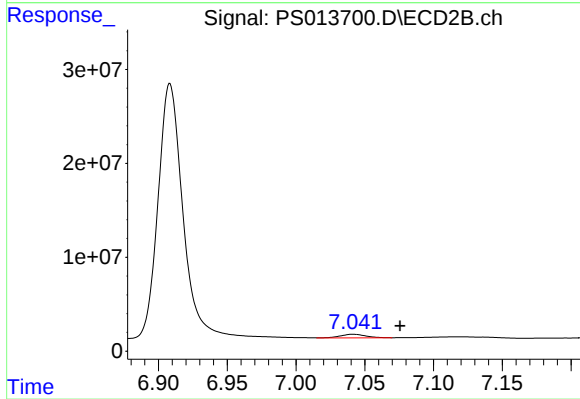

#5 DICAMBA


R.T.: 7.041 min
Delta R.T.: -0.034 min
Response: 4840449
Conc: 2.82 ng/ml

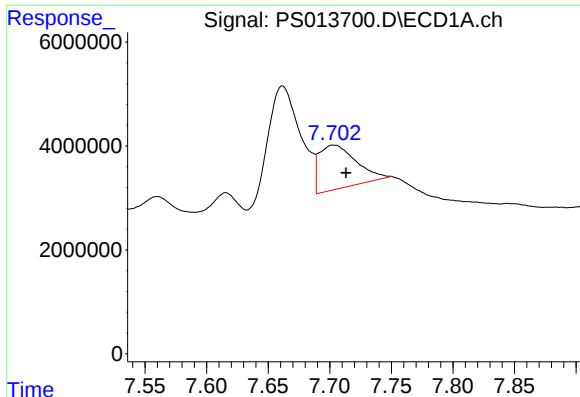

#7 MCPA


R.T.: 7.703 min
Delta R.T.: -0.010 min
Response: 18034173
Conc: 4.39 ug/ml

Instrument :
ECD_S
ClientSampleId :

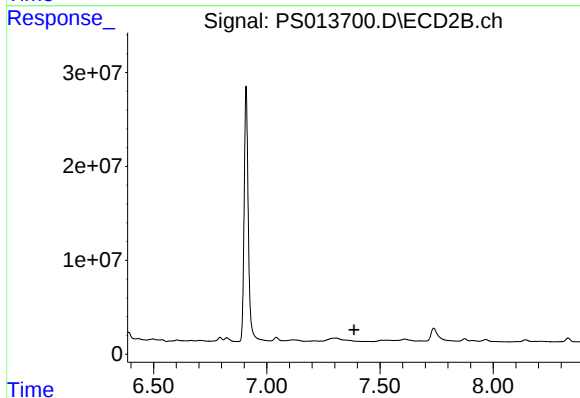


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

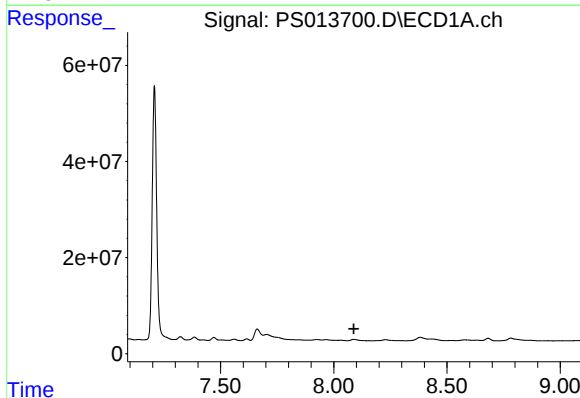


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.088 min
Response: 0
Conc: N.D.

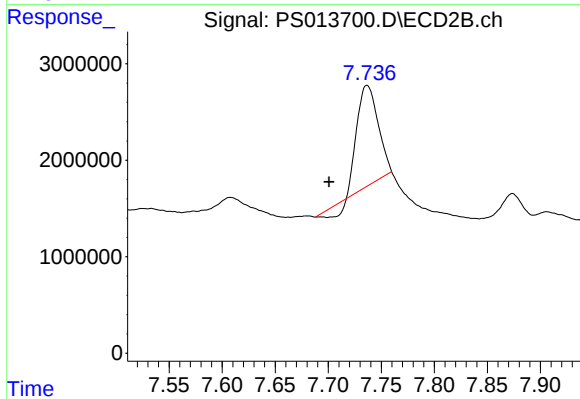

#8 DICHLORPROP


R.T.: 7.737 min
Delta R.T.: 0.036 min
Response: 13470769
Conc: 30.25 ng/ml

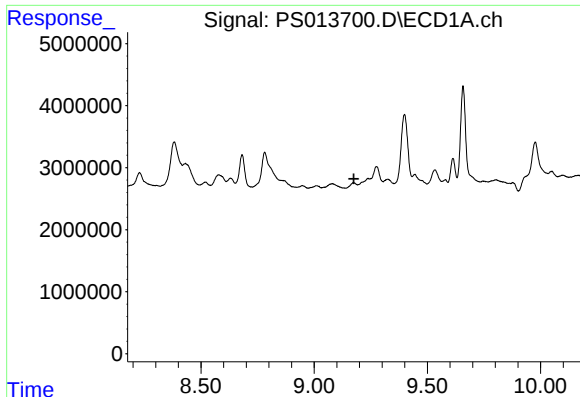

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

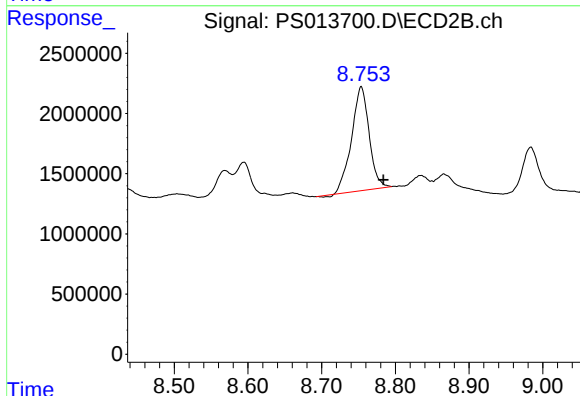


#11 2,4,5-TP (SILVEX)

R.T.: 8.754 min
Delta R.T.: -0.030 min
Response: 14257094
Conc: 5.97 ng/ml

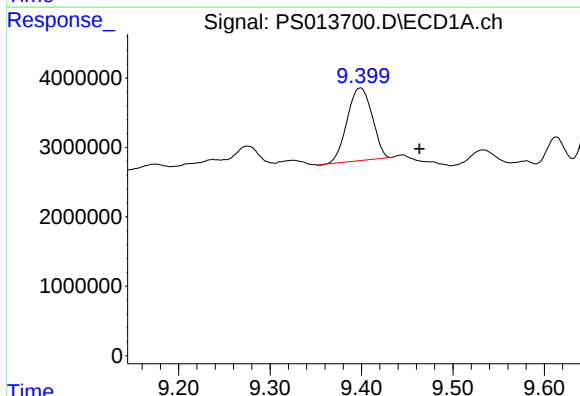


#12 2,4,5-T

R.T.: 9.399 min
Delta R.T.: -0.065 min
Response: 19788029
Conc: 3.50 ng/ml

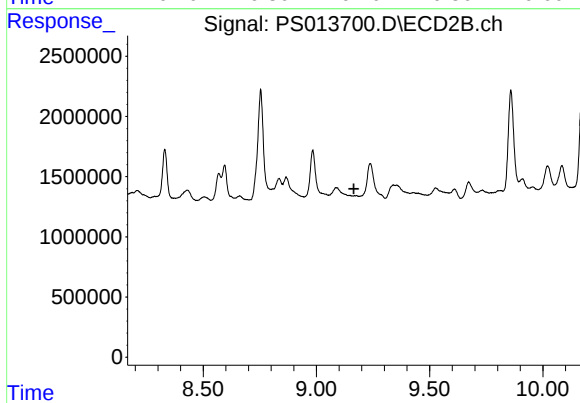

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.165 min
Response: 0
Conc: N.D.

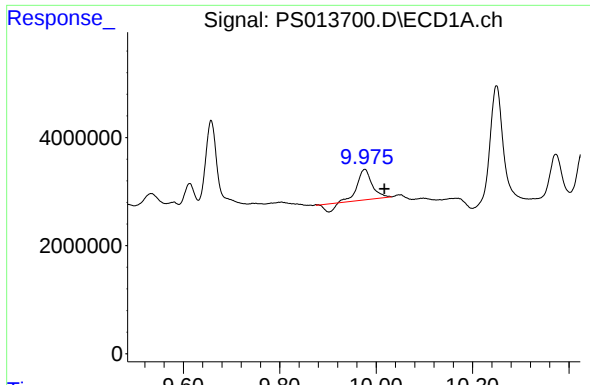

#13 2,4-DB


R.T.: 9.976 min
Delta R.T.: -0.041 min
Response: 10351300
Conc: 10.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

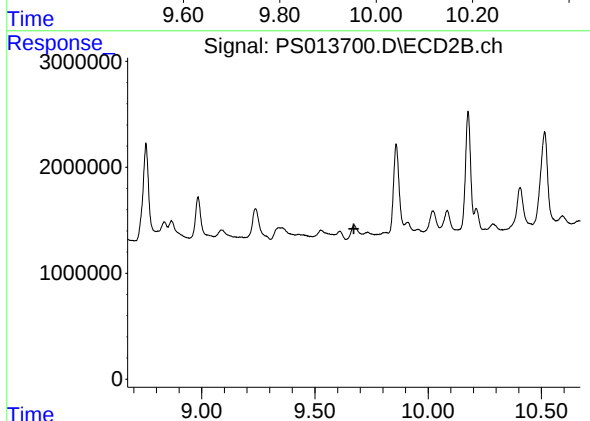


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

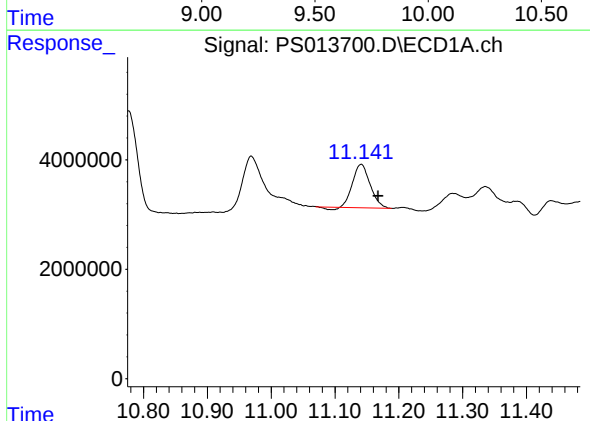


#14 DINOSEB

R.T.: 11.141 min
Delta R.T.: -0.027 min
Response: 14925584
Conc: 3.38 ng/ml

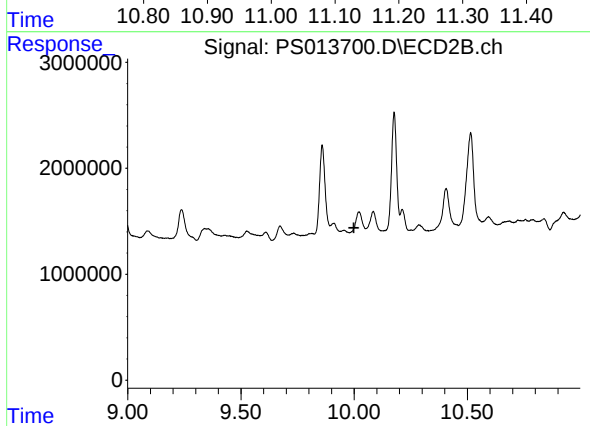

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.999 min
Response: 0
Conc: N.D.

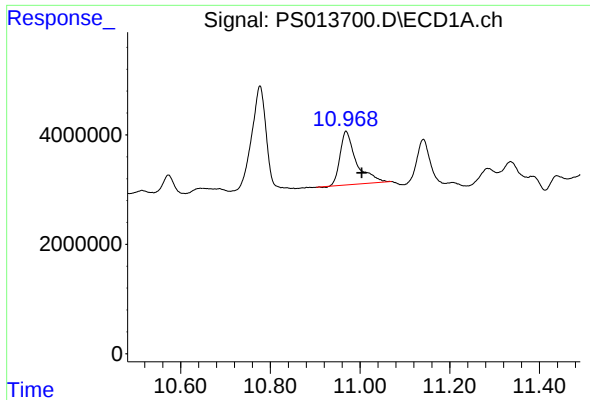

#15 Picloram

R.T.: 10.969 min
Delta R.T.: -0.035 min
Response: 24961199
Conc: 3.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

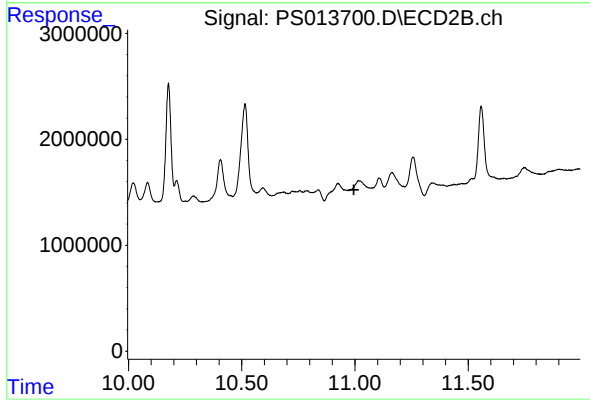

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.