

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
 Data File : PS013689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 07:48
 Operator : DD\AJ
 Sample : L5242-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SAMPLE-4(464+26)

Manual Integrations
 APPROVED

Ankita
 1/5/2021 1:51:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 12:06:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.206	6.908	299.9E6	159.0E6	313.838m	395.353 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010421\
Data File : PS013689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 07:48
Operator : DD\AJ
Sample : L5242-07
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SAMPLE-4(464+26)


Manual Integrations
APPROVED

Ankita
1/5/2021 1:51:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 12:06:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

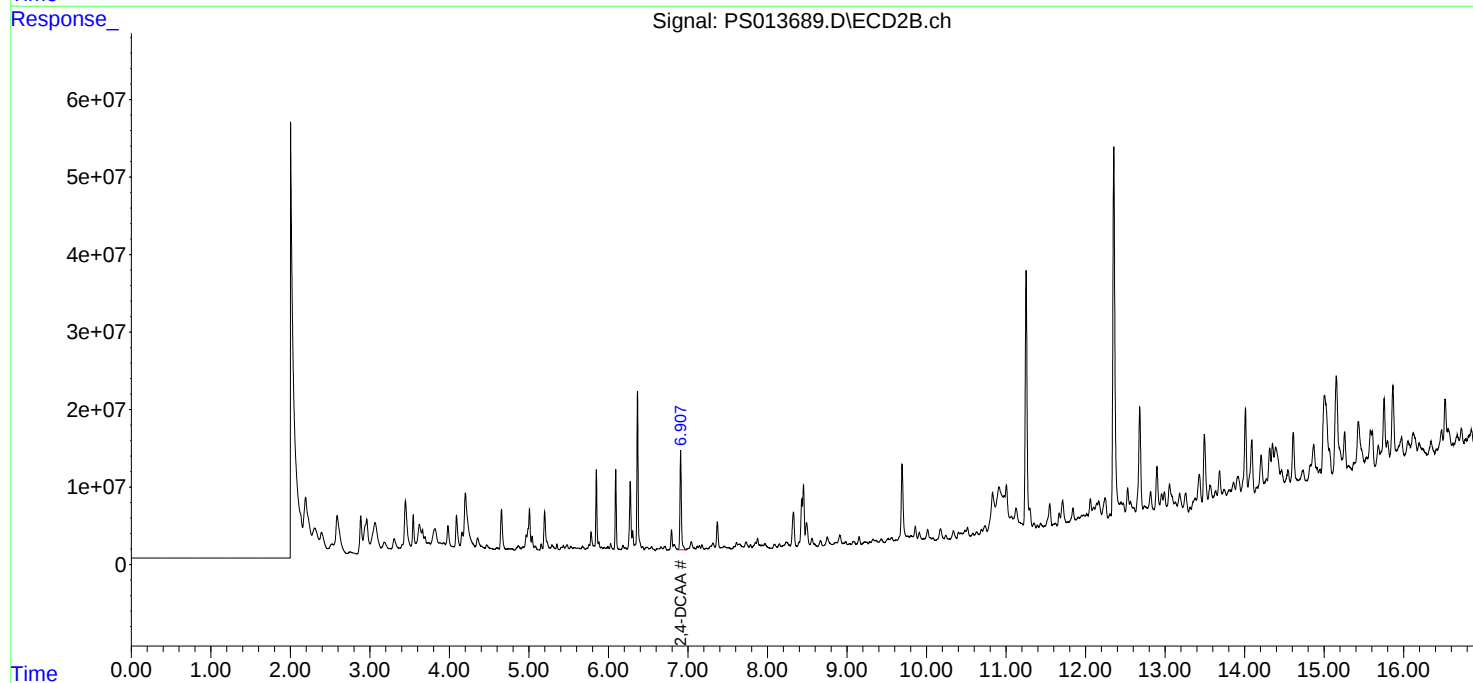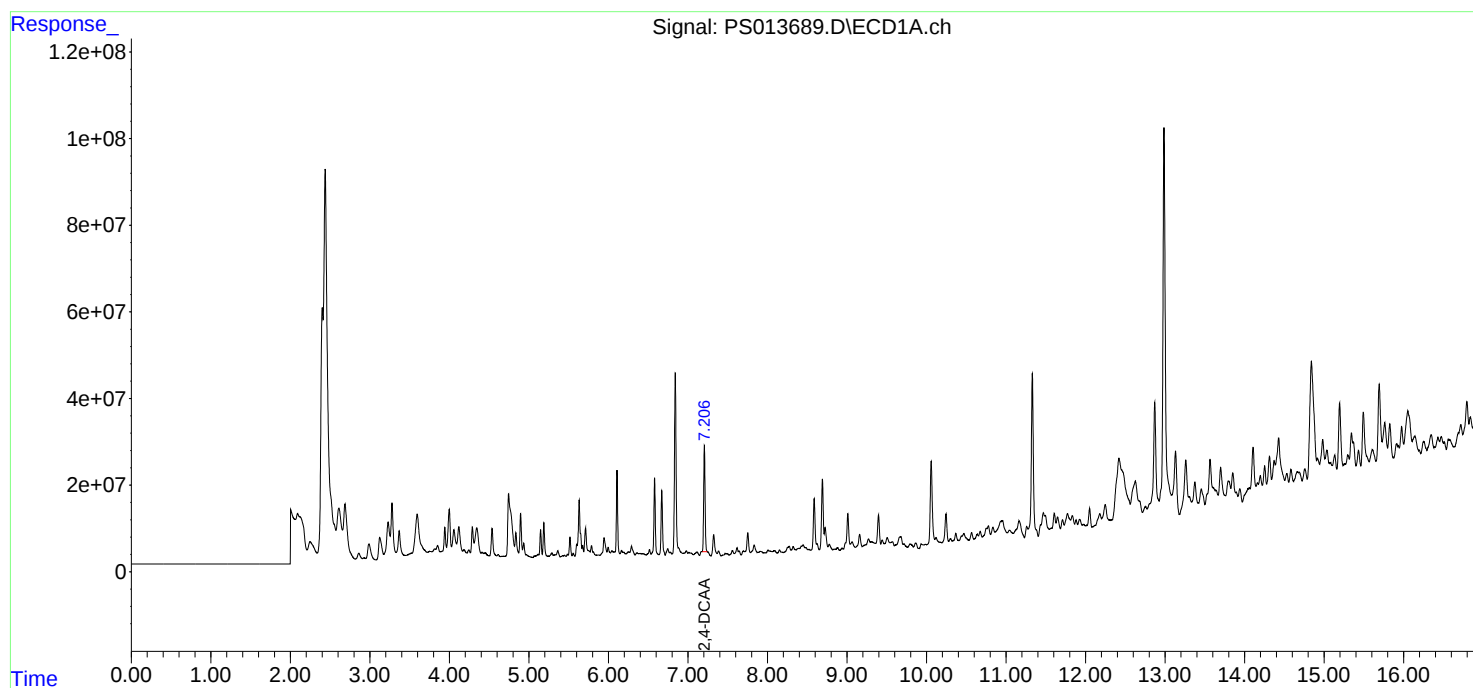

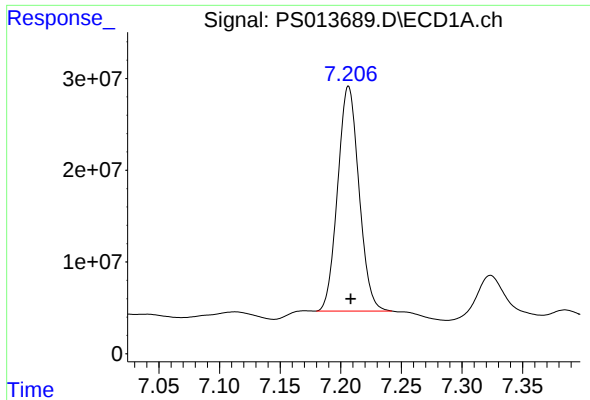


#4 2,4-DCAA

R.T.: 7.206 min
Delta R.T.: -0.002 min
Response: 299901718
Conc: 313.84 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SAMPLE-4(464+26)

Manual Integrations
APPROVED

Ankita
1/5/2021 1:51:45 PM

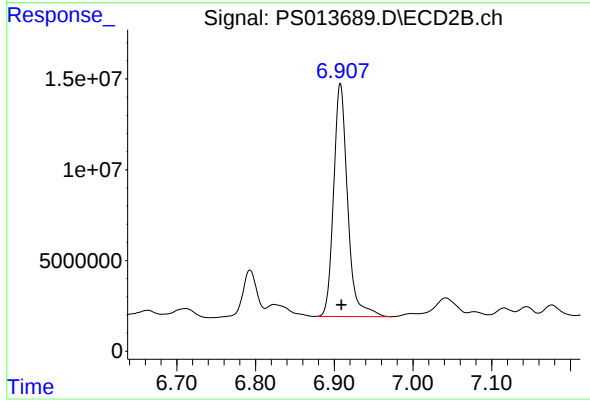

#4 2,4-DCAA

R.T.: 6.908 min
Delta R.T.: -0.002 min
Response: 158977532
Conc: 395.35 ng/ml