

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010423\
 Data File : PS021609.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2023 14:39
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 00:19:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.376	0.000	217159	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.456	0.000	858660	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.736	0.000	8828486	0	2.221	N.D. #
3) T	4-Nitroph...	6.227	0.000	207587	0	<MDL	N.D. #
5) T	DICAMBA	6.527	6.990	401581	867599	<MDL	<MDL #
6) T	MCP	6.699	7.109	903251	810603	<MDL	<MDL #
7) T	MCPA	6.806	0.000	708026	0	<MDL	N.D. #
8) T	DICHLORPROP	7.131	0.000	999210	0	<MDL	N.D. #
9) T	2,4-D	7.305	0.000	41664804	0	10.904	N.D. #
10) T	Pentachlo...	7.552	8.316	1302677	1686908	<MDL	<MDL #
11) T	2,4,5-TP ...	8.091	8.677	5013646	3986938	<MDL	<MDL #
12) T	2,4,5-T	8.370	9.078	4533247	21888292	<MDL	2.019 #
13) T	2,4-DB	8.832	9.636f	666979	1882439	<MDL	1.310 #
15) T	Picloram	9.731	10.908	21874518	43077320	<MDL	2.649 #
16) T	DCPA	10.168	0.000	1810282	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010423\
Data File : PS021609.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2023 14:39
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 00:19:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

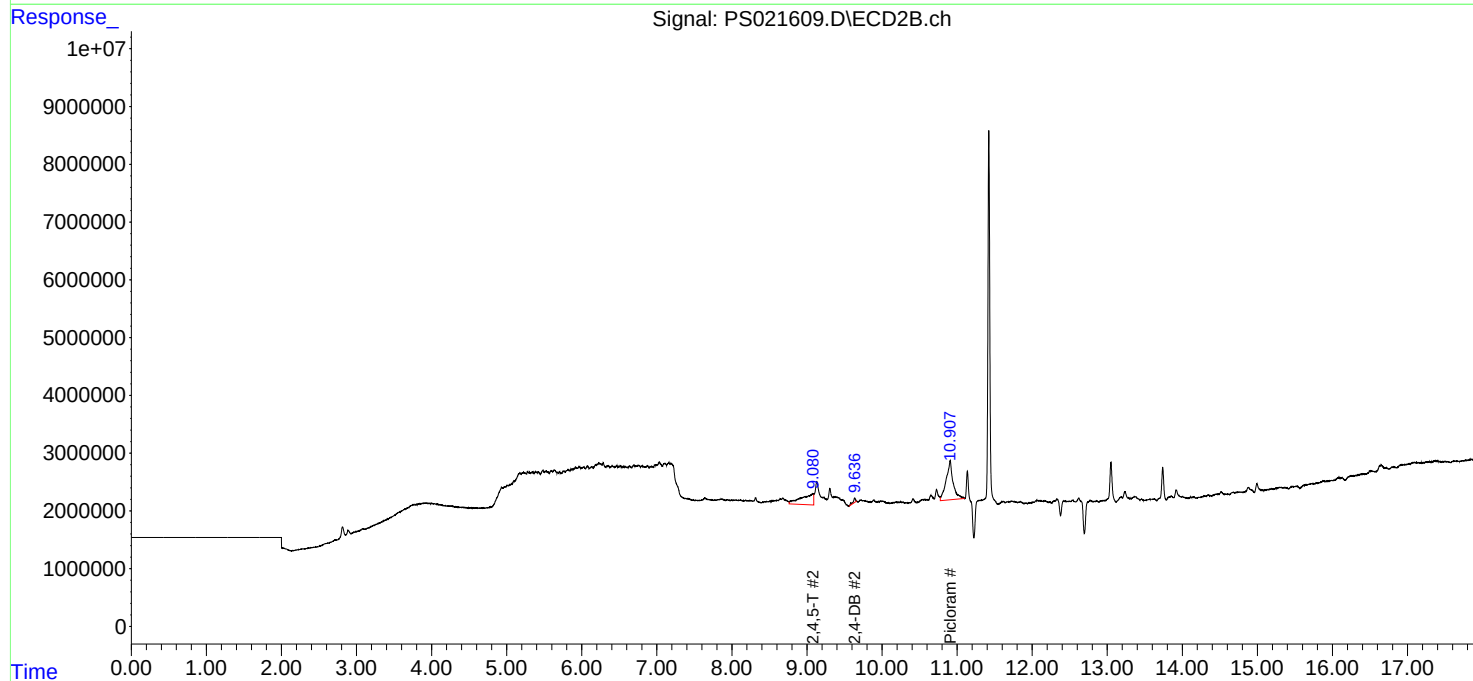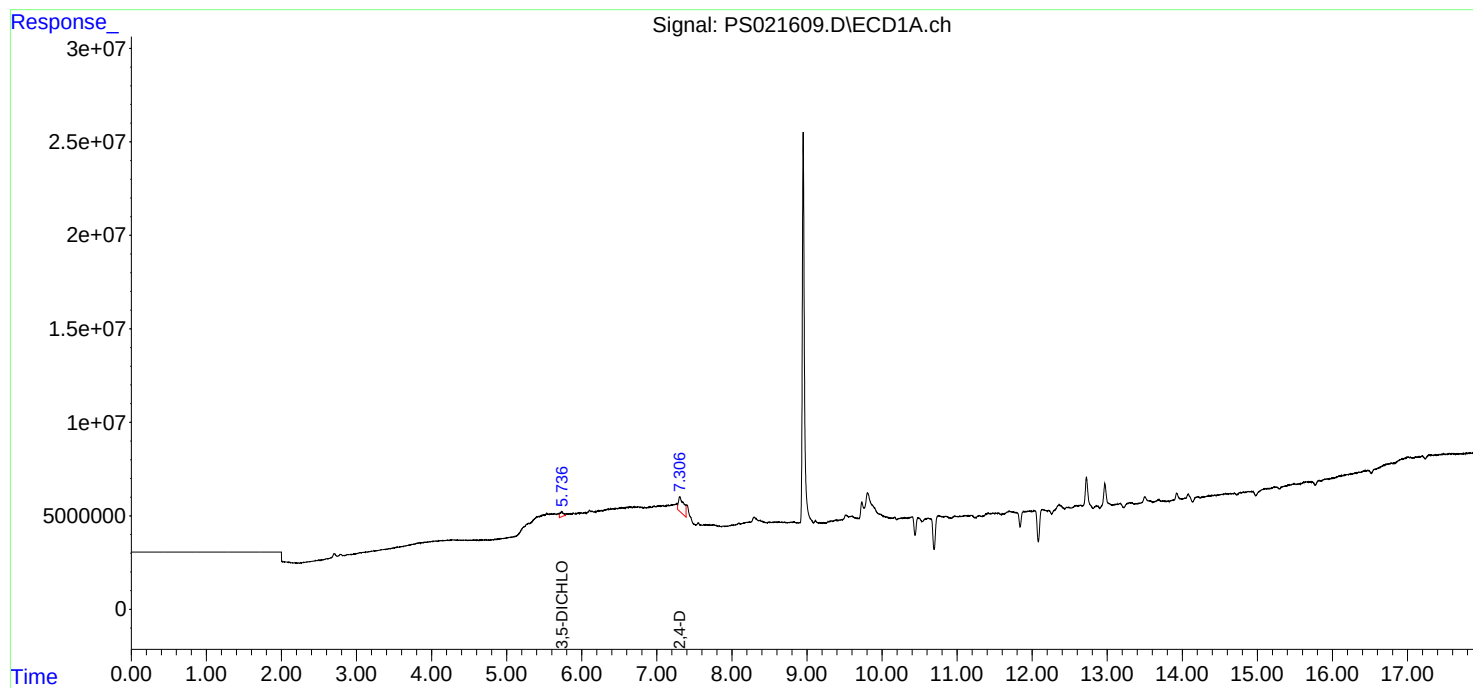


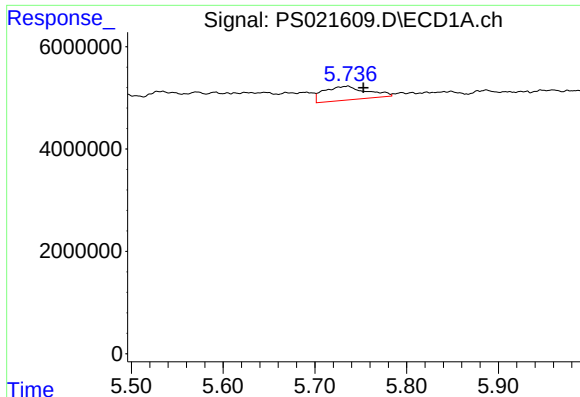

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.736 min
Delta R.T.: -0.017 min
Response: 8828486
Conc: 2.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

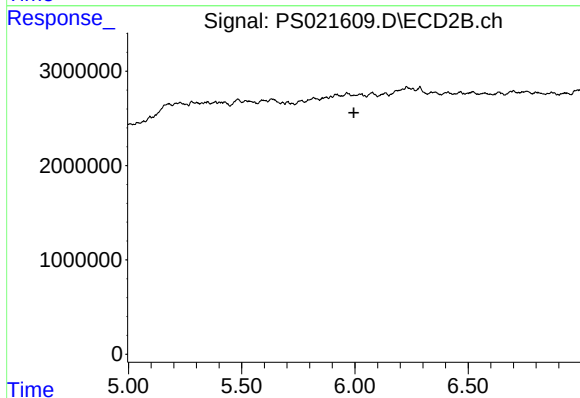


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

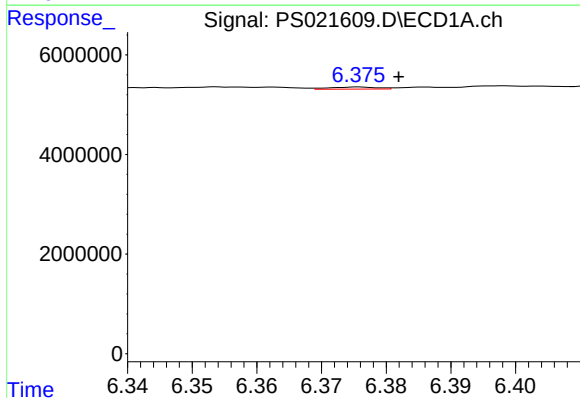


#4 2,4-DCAA

R.T.: 6.376 min
Delta R.T.: -0.006 min
Response: 217159
Conc: N.D.

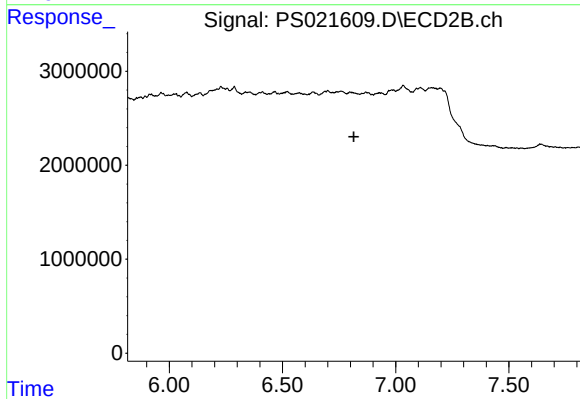

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.816 min
Response: 0
Conc: N.D.

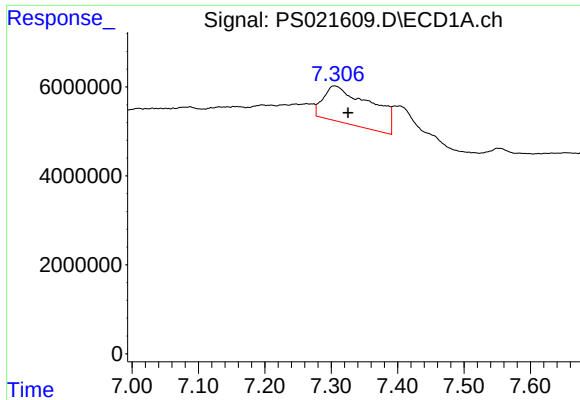

#9 2,4-D


R.T.: 7.305 min
Delta R.T.: -0.020 min
Response: 41664804
Conc: 10.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

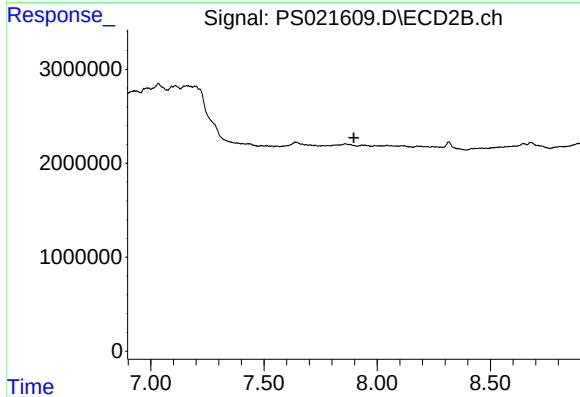


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.897 min
Response: 0
Conc: N.D.

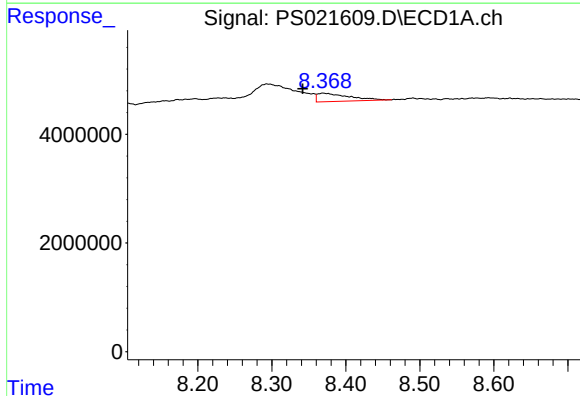


#12 2,4,5-T

R.T.: 8.370 min
Delta R.T.: 0.028 min
Response: 4533247
Conc: N.D.

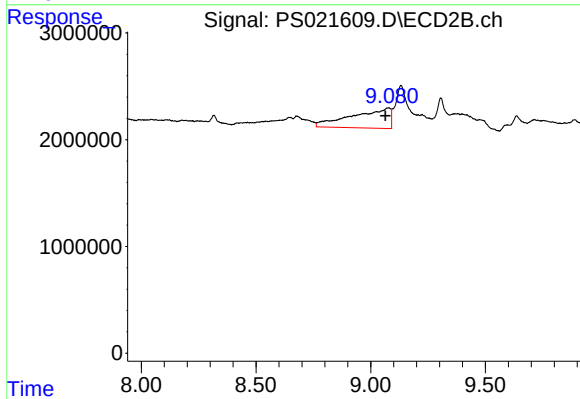

#12 2,4,5-T


R.T.: 9.078 min
Delta R.T.: 0.015 min
Response: 21888292
Conc: 2.02 ng/ml

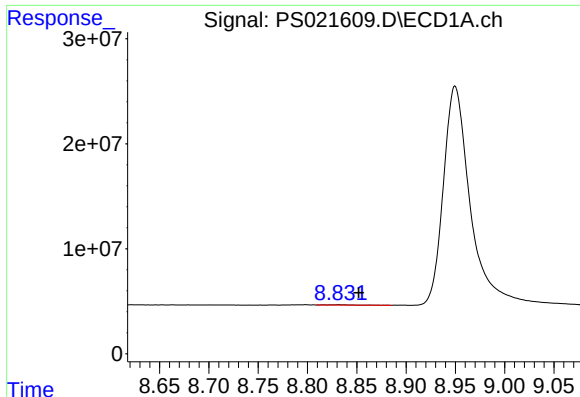

#13 2,4-DB


R.T.: 8.832 min
Delta R.T.: -0.020 min
Response: 666979
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

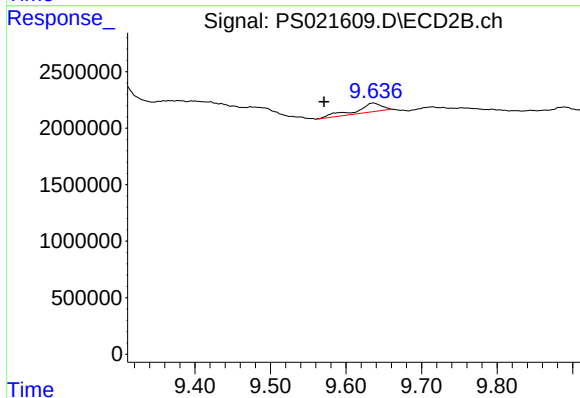


#13 2,4-DB

R.T.: 9.636 min
Delta R.T.: 0.065 min
Response: 1882439
Conc: 1.31 ng/ml

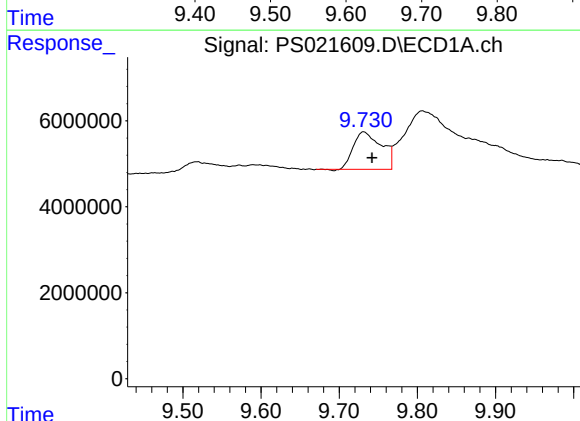

#15 Picloram

R.T.: 9.731 min
Delta R.T.: -0.011 min
Response: 21874518
Conc: N.D.

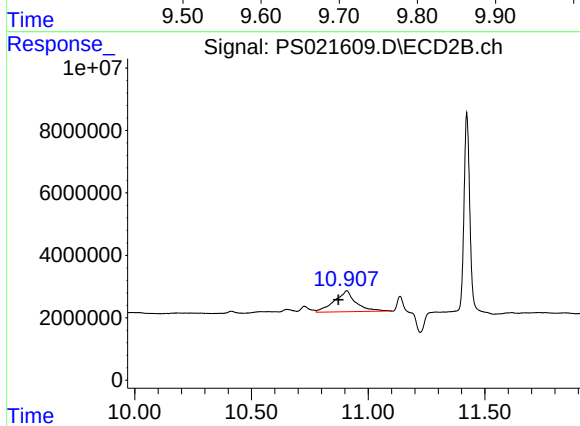

#15 Picloram

R.T.: 10.908 min
Delta R.T.: 0.036 min
Response: 43077320
Conc: 2.65 ng/ml