

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010423\
 Data File : PS021610.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2023 15:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 00:20:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.378	6.809	1323.0E6	1016.4E6	455.327	589.557	#
Target Compounds								
1) T	Dalapon	2.524f	0.000	160643	0	<MDL	N.D.	#
2) T	3,5-DICHL...	5.724	0.000	5457794	0	1.373	N.D.	#
3) T	4-Nitroph...	6.228	0.000	5463835	0	3.039	N.D.	#
6) T	MCP	0.000	7.119f	0	6127113	N.D.	1.041	
7) T	MCPA	6.761	7.215f	-2617338	50996917	N.D.	5.767	
10) T	Pentachlo...	7.551	0.000	712416	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	8.084	0.000	3389823	0	<MDL	N.D.	#
12) T	2,4,5-T	8.348	0.000	6965016	0	<MDL	N.D.	#
13) T	2,4-DB	8.875	9.505f	1049397	1197835	<MDL	<MDL	#
14) T	DINOSEB	9.883	0.000	34283207	0	2.152	N.D.	#
15) T	Picloram	9.758	10.925f	1137133	20604126	<MDL	1.267	#
16) T	DCPA	10.164	0.000	1462795	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010423\
Data File : PS021610.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2023 15:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 00:20:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

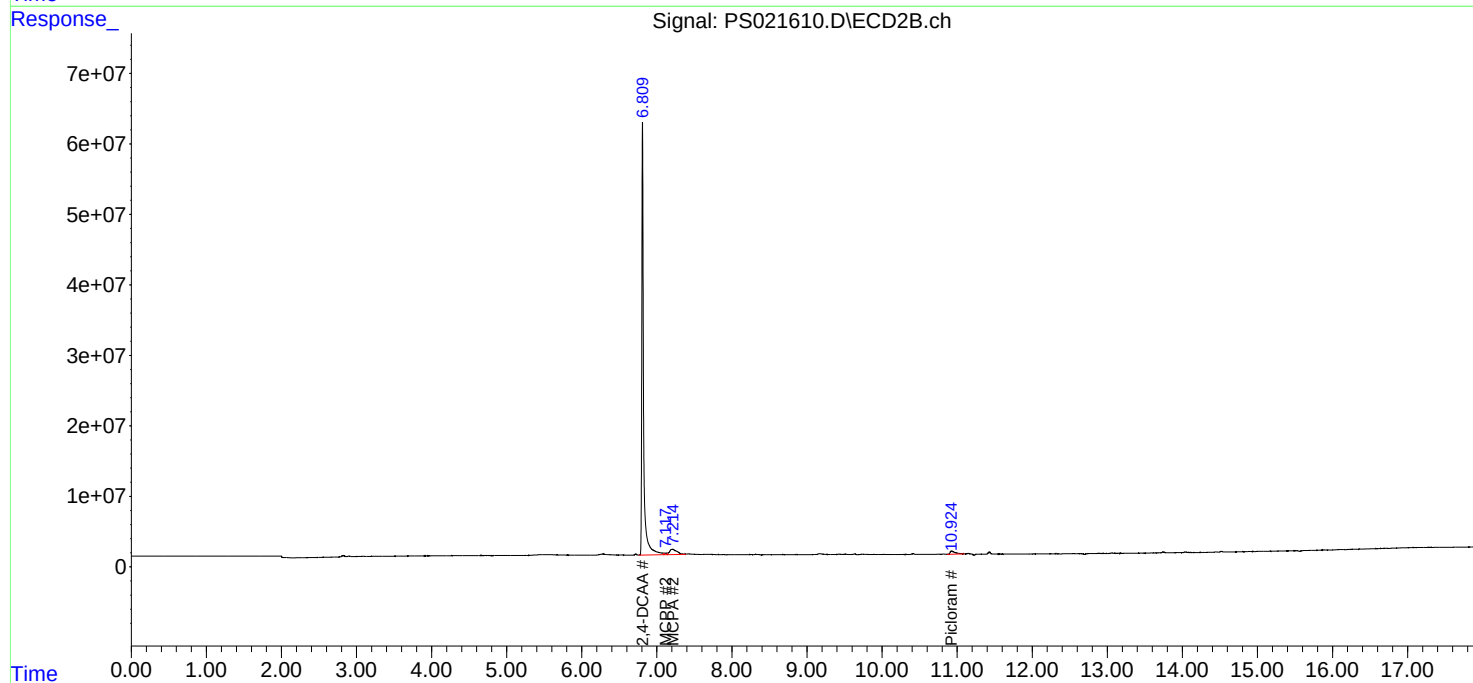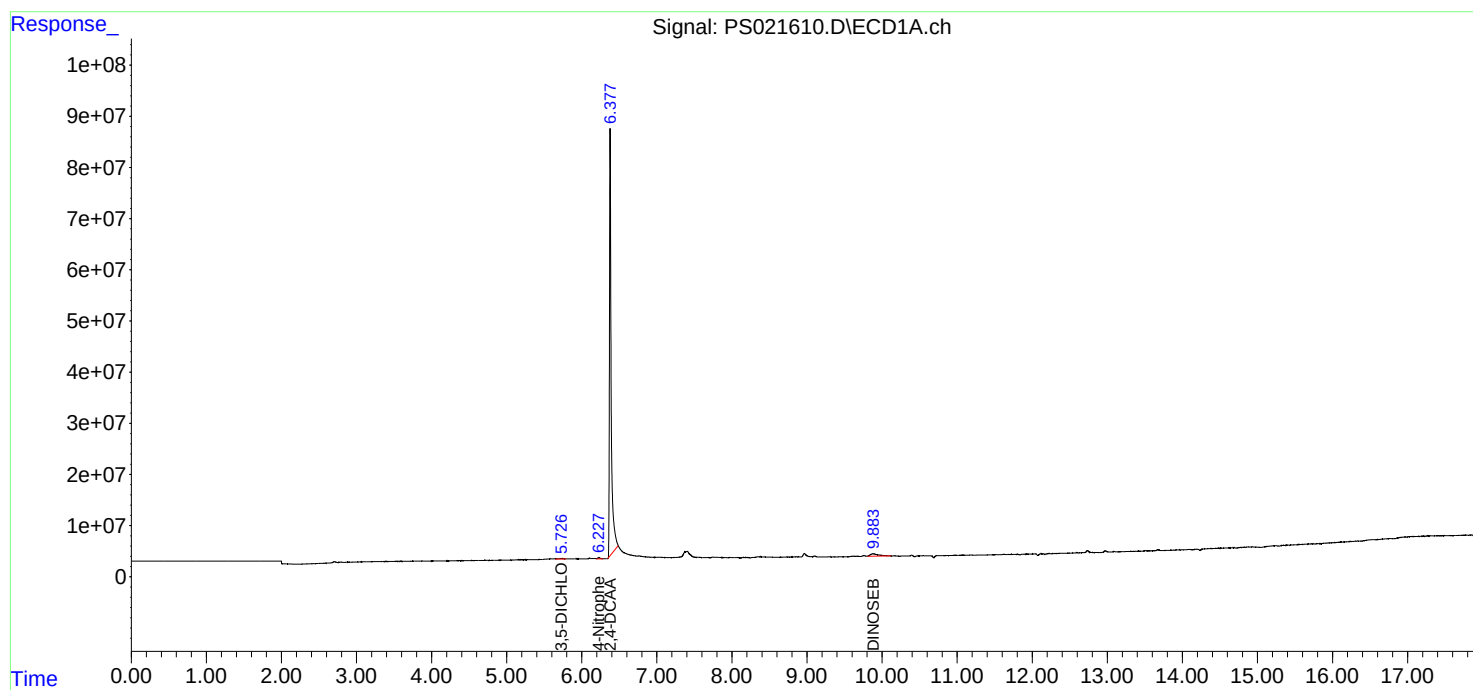


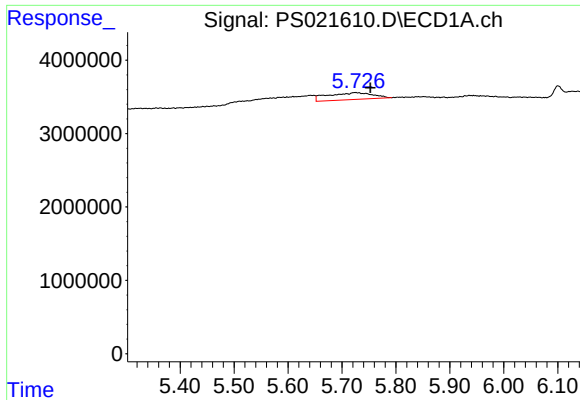

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.724 min
Delta R.T.: -0.029 min
Response: 5457794
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

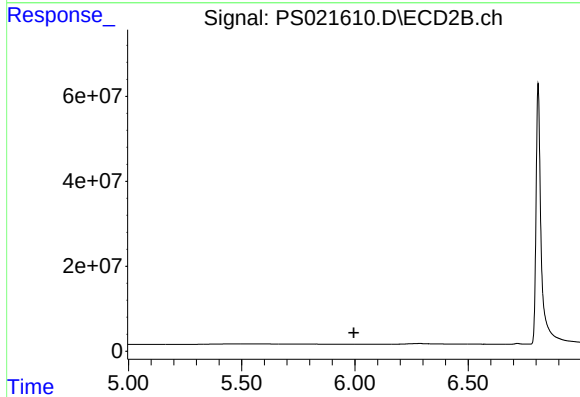


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

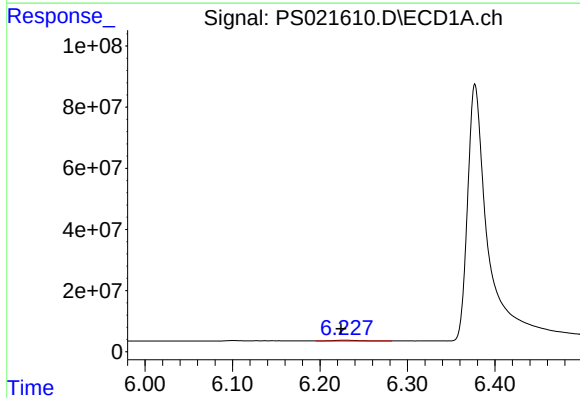


#3 4-Nitrophenol

R.T.: 6.228 min
Delta R.T.: 0.004 min
Response: 5463835
Conc: 3.04 ng/ml

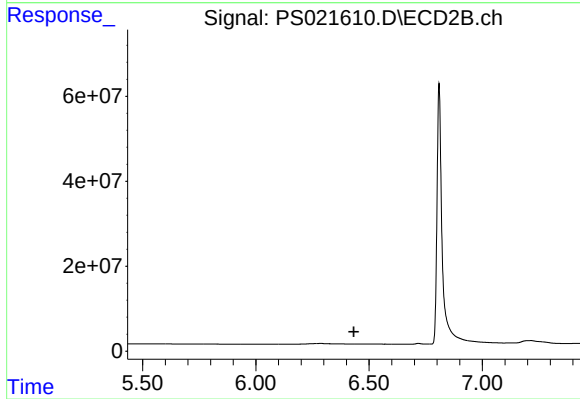

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

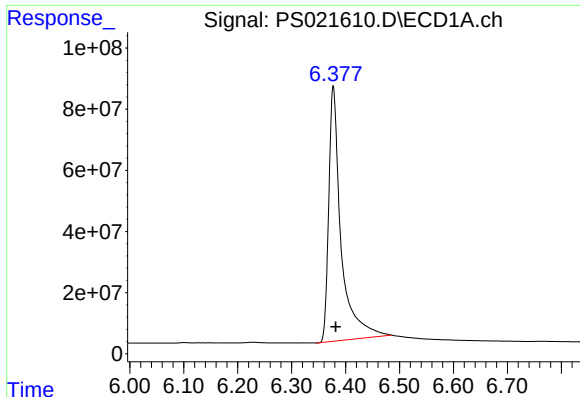

#4 2,4-DCAA


R.T.: 6.378 min
Delta R.T.: -0.004 min
Response: 1322950530
Conc: 455.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

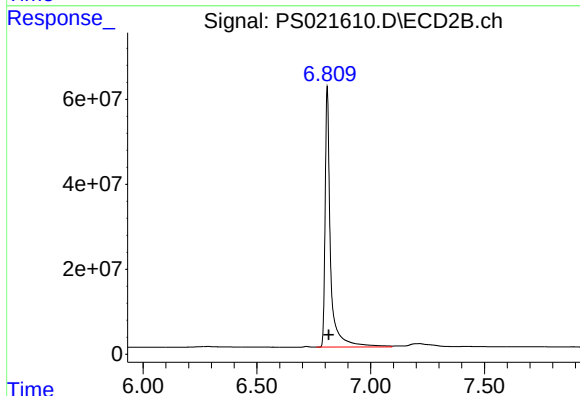


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.007 min
Response: 1016392606
Conc: 589.56 ng/ml

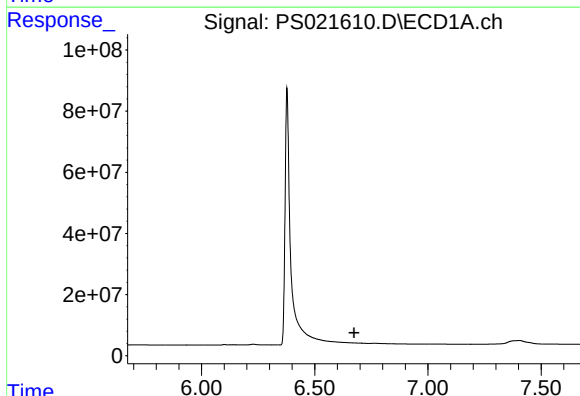


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.673 min
Response: 0
Conc: N.D.

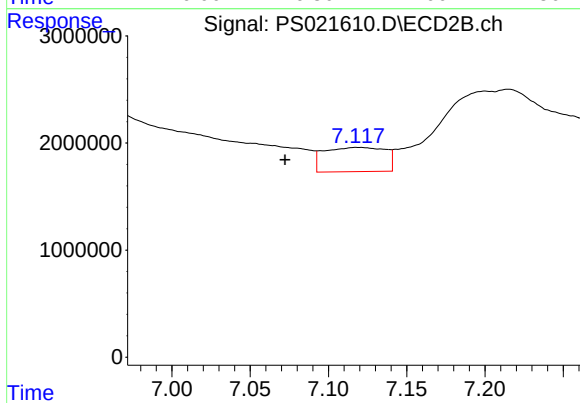

#6 MCPP


R.T.: 7.119 min
Delta R.T.: 0.047 min
Response: 6127113
Conc: 1.04 ug/ml

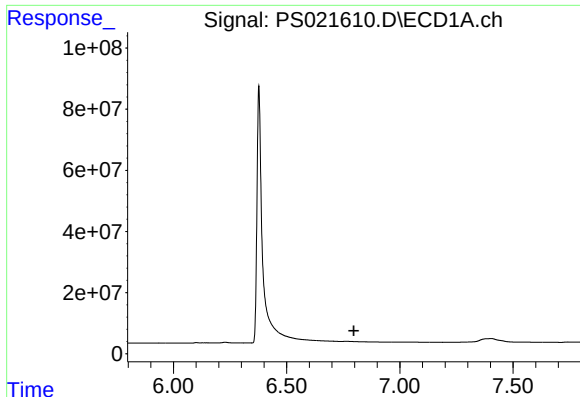

#7 MCPA


R.T.: 6.761 min
Delta R.T.: -0.036 min
Response: -2617338
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

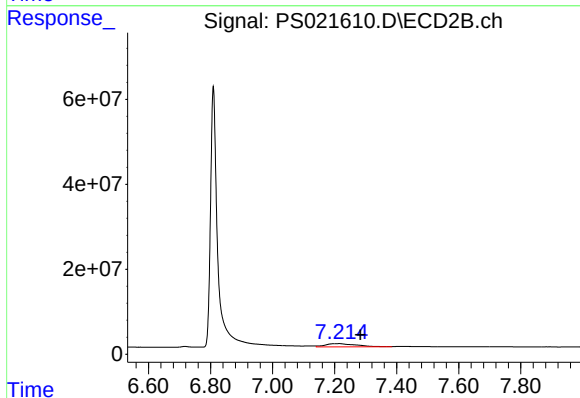


#7 MCPA

R.T.: 7.215 min
Delta R.T.: -0.068 min
Response: 50996917
Conc: 5.77 ug/ml

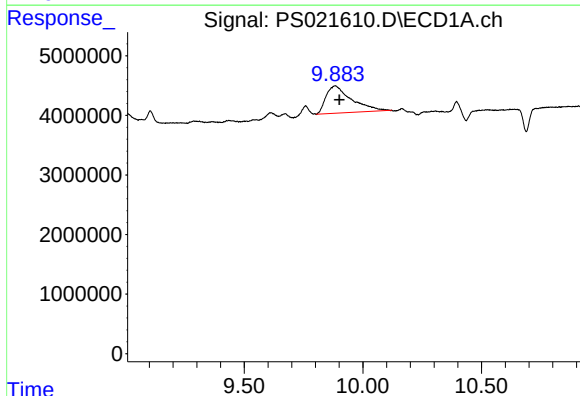


#14 DINOSEB

R.T.: 9.883 min
Delta R.T.: -0.018 min
Response: 34283207
Conc: 2.15 ng/ml

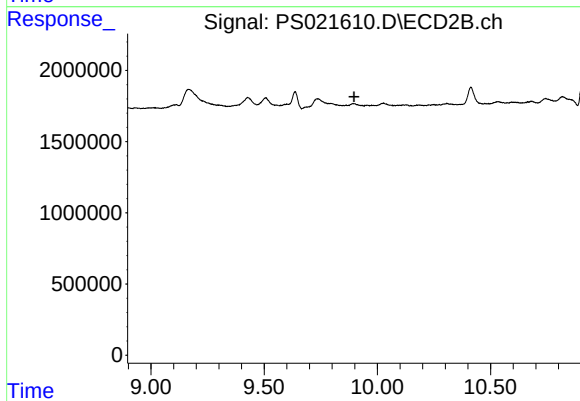

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.897 min
Response: 0
Conc: N.D.

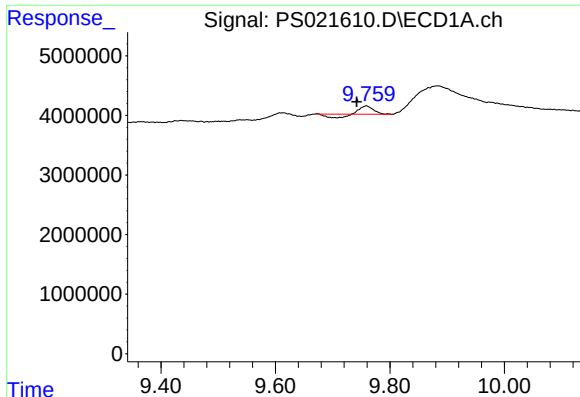

#15 Picloram

R.T.: 9.758 min
Delta R.T.: 0.016 min
Response: 1137133
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

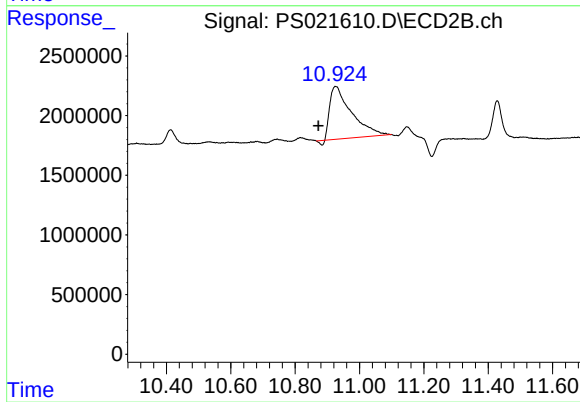

#15 Picloram

R.T.: 10.925 min
Delta R.T.: 0.053 min
Response: 20604126
Conc: 1.27 ng/ml