

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010522\
 Data File : PS017911.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2022 18:38
 Operator : AJ\MA
 Sample : HSTDICC1500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC1500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 01:56:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 01:55:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.044	6.645	2239.7E6	912.6E6	1517.224	1530.477
Target Compounds							
1) T	Dalapon	2.912	2.424	3497.7E6	1095.1E6	1396.471	1405.249
2) T	3,5-DICHL...	6.285	5.862	2963.7E6	1269.7E6	1383.274	1399.643
3) T	4-Nitroph...	6.871	6.279	1182.3E6	450.7E6	1414.290	1404.985
5) T	DICAMBA	7.230	6.800	8569.7E6	3622.5E6	1387.739	1383.794
6) T	MCP	7.406	6.902	705.7E6	320.2E6	144.838	144.614
7) T	MCPA	7.555	7.113	966.4E6	434.8E6	141.960	142.364
8) T	DICHLORPROP	7.916	7.410	2180.2E6	961.2E6	1403.283	1424.351
9) T	2,4-D	8.142	7.698	2547.2E6	1114.6E6	1408.660	1443.391
10) T	Pentachlo...	8.441	8.113	26833.3E6	10401.8E6	1341.184	1318.565
11) T	2,4,5-TP ...	8.991	8.475	11484.1E6	4902.9E6	1388.883	1390.964
12) T	2,4,5-T	9.273	8.849	11974.2E6	4646.8E6	1387.068	1405.014
13) T	2,4-DB	9.819	9.352	2524.1E6	663.3E6	1467.797	1456.436
14) T	DINOSEB	10.966	9.674	8874.6E6	3521.1E6	1384.686	1403.555
15) T	Picloram	10.788	10.648	17267.8E6	6736.1E6	1427.052	1416.346
16) T	DCPA	11.235	10.600	14492.0E6	5957.3E6	1389.574	1388.243



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010522\
Data File : PS017911.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2022 18:38
Operator : AJ\MA
Sample : HSTDICC1500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 01:56:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 01:55:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

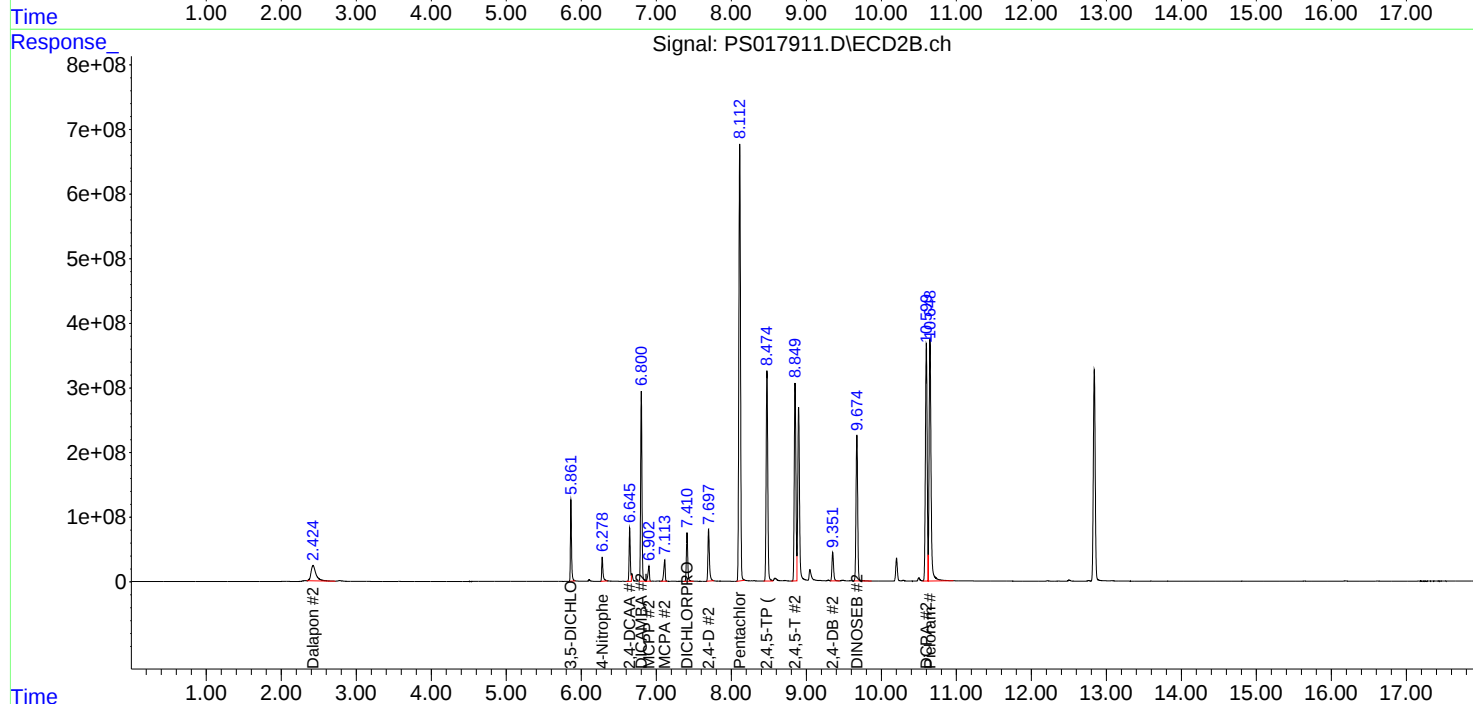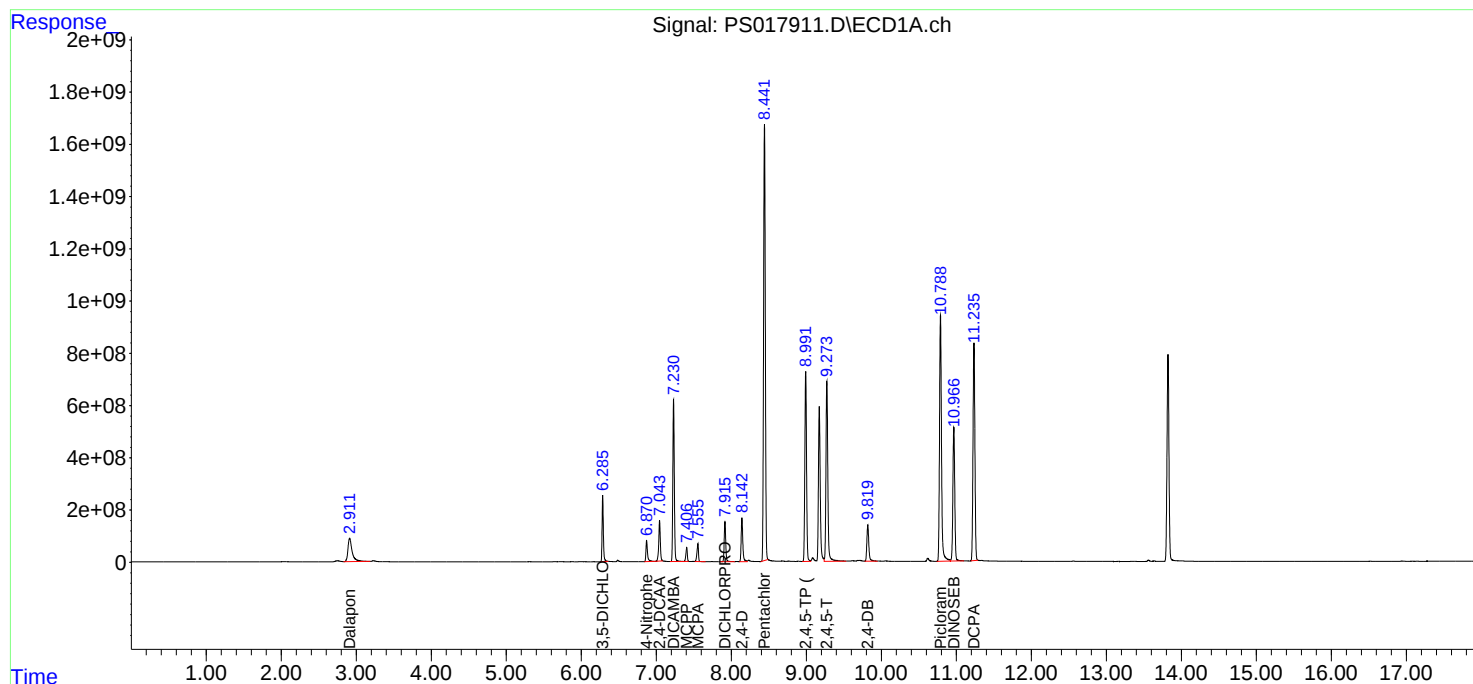


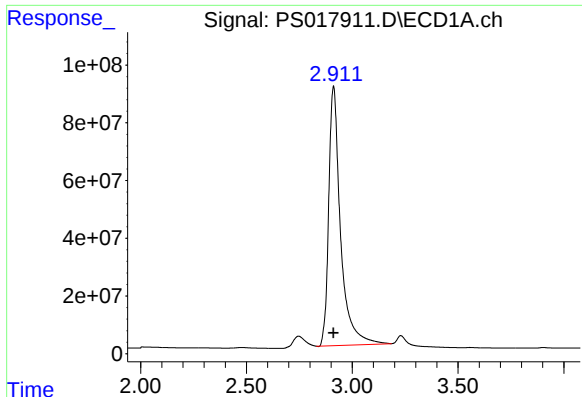

#1 Dalapon


R.T.: 2.912 min
Delta R.T.: 0.000 min
Response: 3497651207
Conc: 1396.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

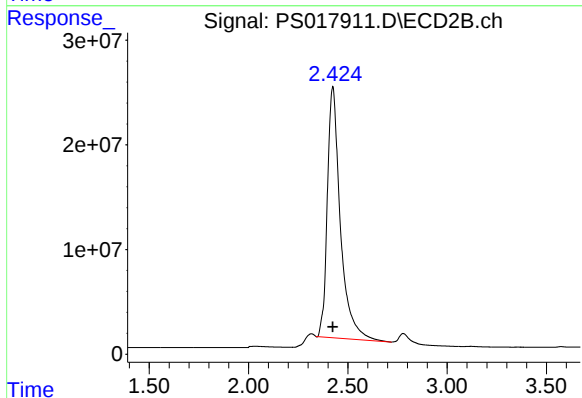


#1 Dalapon

R.T.: 2.424 min
Delta R.T.: 0.000 min
Response: 1095083201
Conc: 1405.25 ng/ml

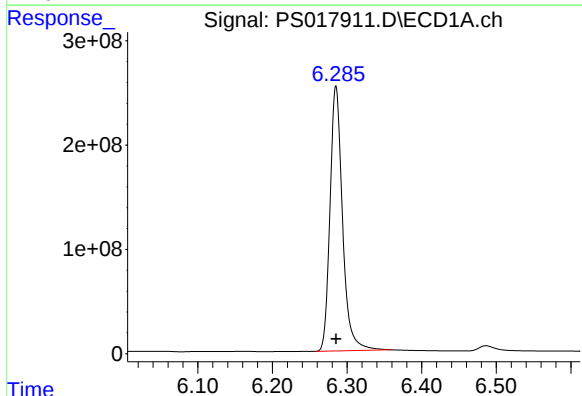


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.285 min
Delta R.T.: 0.000 min
Response: 2963740727
Conc: 1383.27 ng/ml

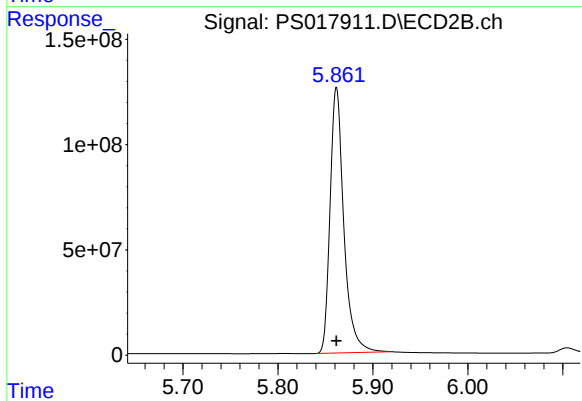

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.862 min
Delta R.T.: 0.000 min
Response: 1269673812
Conc: 1399.64 ng/ml

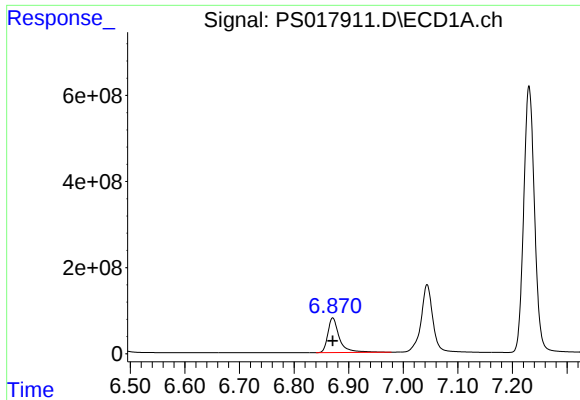

#3 4-Nitrophenol


R.T.: 6.871 min
Delta R.T.: 0.000 min
Response: 1182256871
Conc: 1414.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

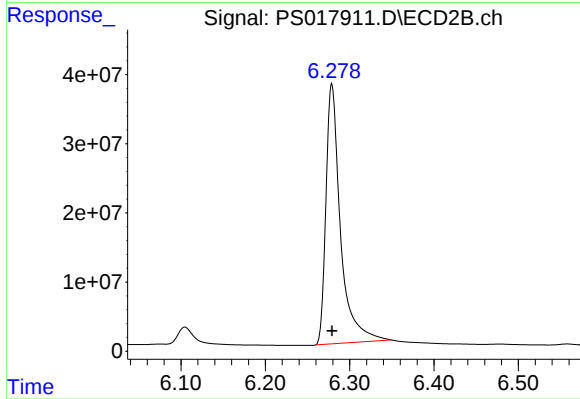


#3 4-Nitrophenol

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 450701506
Conc: 1404.98 ng/ml

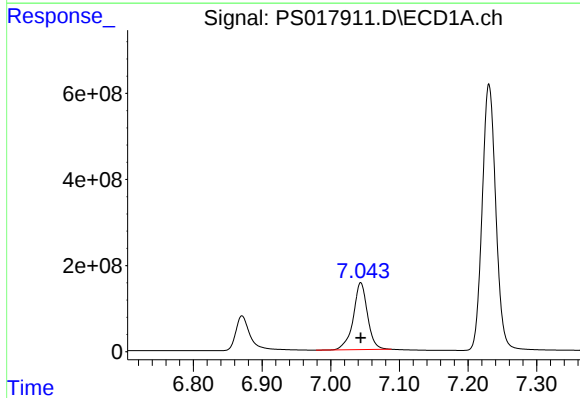


#4 2,4-DCAA

R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 2239674601
Conc: 1517.22 ng/ml

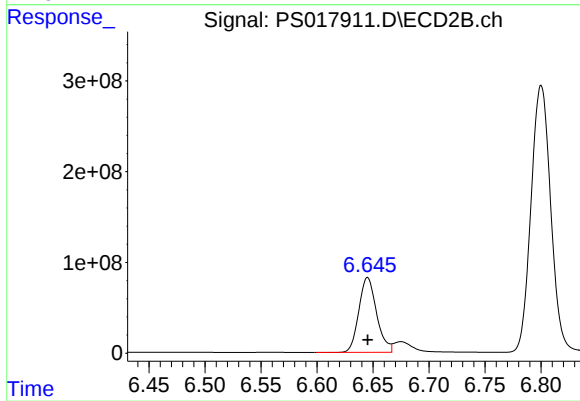

#4 2,4-DCAA


R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 912608043
Conc: 1530.48 ng/ml

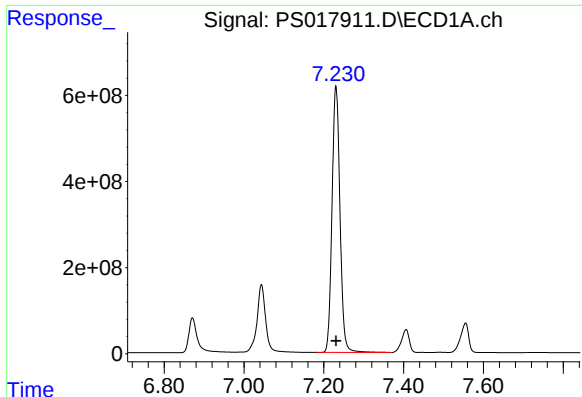

#5 DICAMBA


R.T.: 7.230 min
Delta R.T.: 0.000 min
Response: 8569670963
Conc: 1387.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

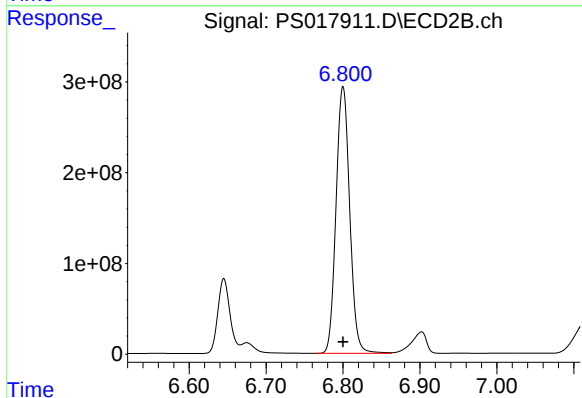


#5 DICAMBA

R.T.: 6.800 min
Delta R.T.: 0.000 min
Response: 3622509880
Conc: 1383.79 ng/ml

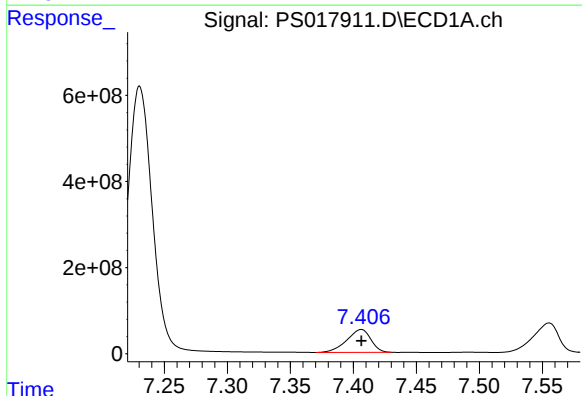


#6 MCP

R.T.: 7.406 min
Delta R.T.: 0.000 min
Response: 705710090
Conc: 144.84 ug/ml

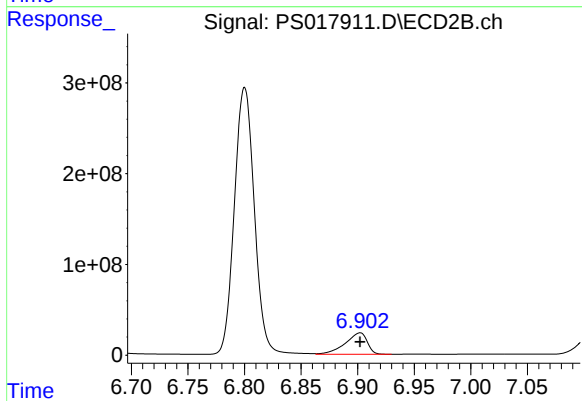

#6 MCP


R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 320227045
Conc: 144.61 ug/ml

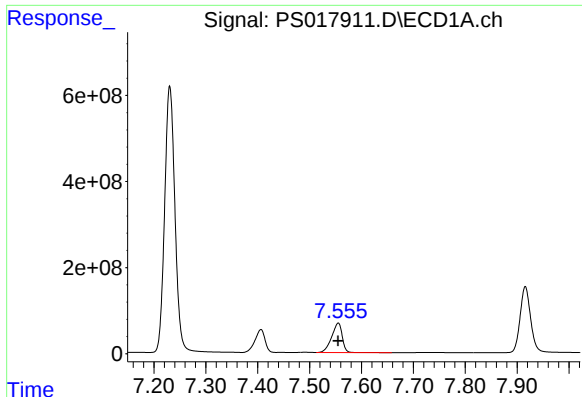

#7 MCPA


R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 966423975
Conc: 141.96 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

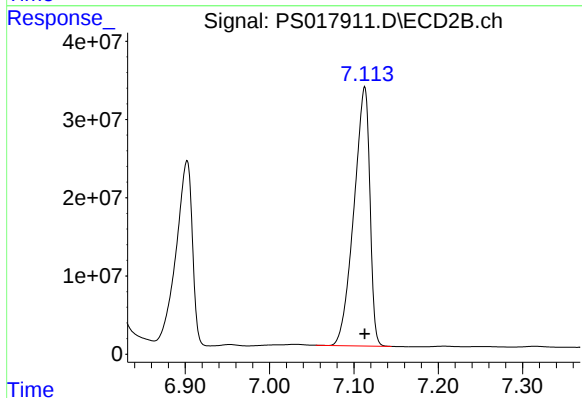


#7 MCPA

R.T.: 7.113 min
Delta R.T.: 0.000 min
Response: 434764645
Conc: 142.36 ug/ml

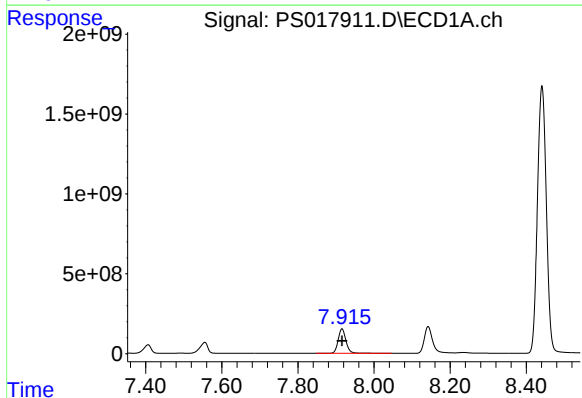


#8 DICHLORPROP

R.T.: 7.916 min
Delta R.T.: 0.000 min
Response: 2180167470
Conc: 1403.28 ng/ml

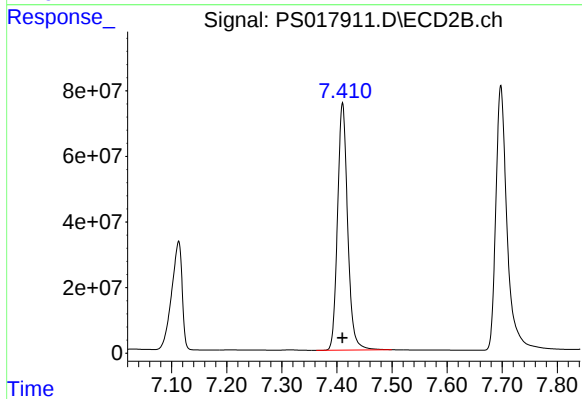

#8 DICHLORPROP


R.T.: 7.410 min
Delta R.T.: 0.000 min
Response: 961161420
Conc: 1424.35 ng/ml

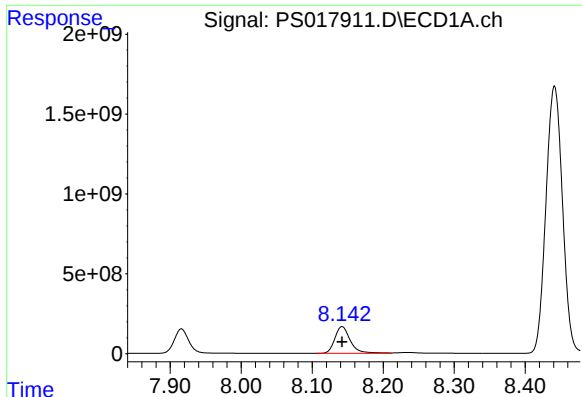

#9 2,4-D


R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 2547235479
Conc: 1408.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

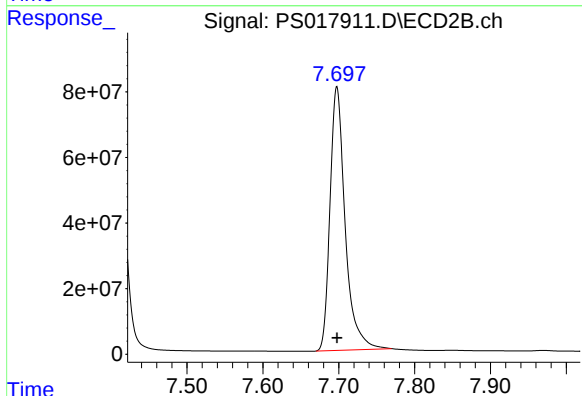


#9 2,4-D

R.T.: 7.698 min
Delta R.T.: 0.000 min
Response: 1114625810
Conc: 1443.39 ng/ml

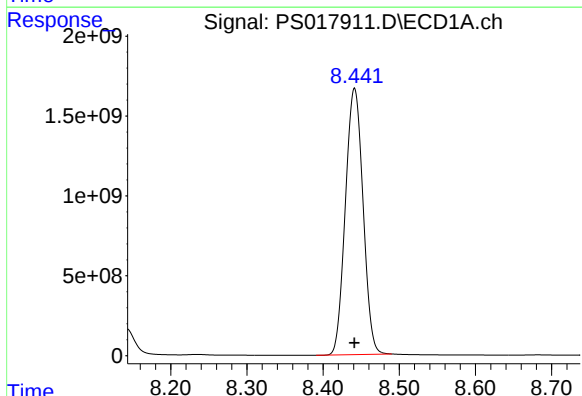


#10 Pentachlorophenol

R.T.: 8.441 min
Delta R.T.: 0.000 min
Response: 26833317107
Conc: 1341.18 ng/ml

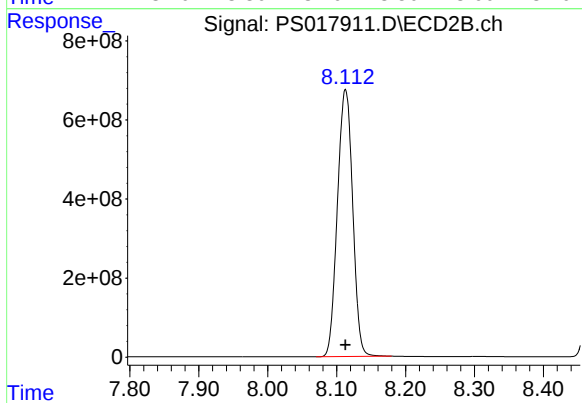

#10 Pentachlorophenol


R.T.: 8.113 min
Delta R.T.: 0.000 min
Response: 10401826917
Conc: 1318.56 ng/ml

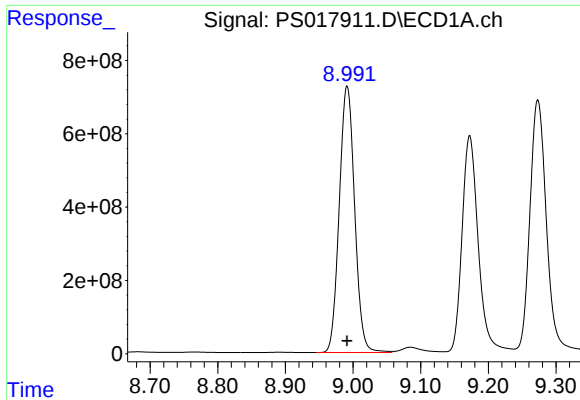

#11 2,4,5-TP (SILVEX)


R.T.: 8.991 min
Delta R.T.: 0.000 min
Response: 11484076557
Conc: 1388.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

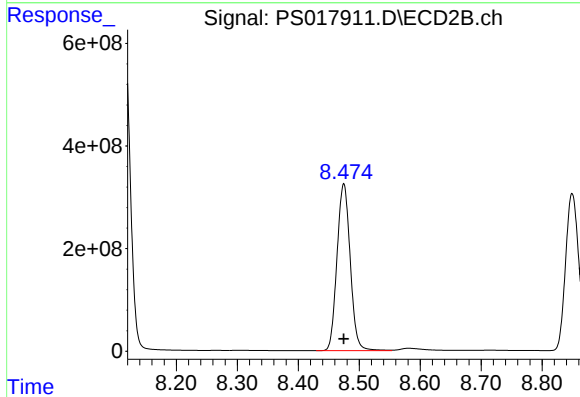


#11 2,4,5-TP (SILVEX)

R.T.: 8.475 min
Delta R.T.: 0.000 min
Response: 4902880873
Conc: 1390.96 ng/ml

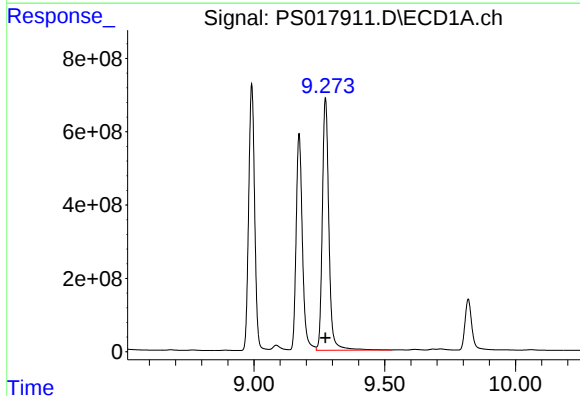


#12 2,4,5-T

R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 11974210454
Conc: 1387.07 ng/ml

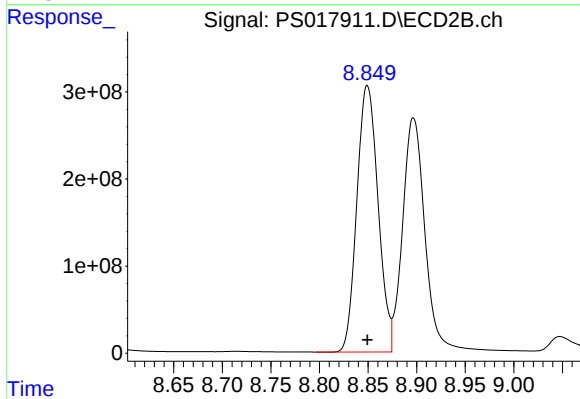

#12 2,4,5-T


R.T.: 8.849 min
Delta R.T.: 0.000 min
Response: 4646787416
Conc: 1405.01 ng/ml

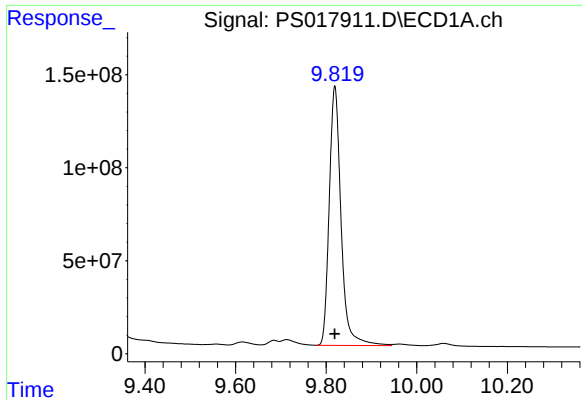

#13 2,4-DB


R.T.: 9.819 min
Delta R.T.: 0.000 min
Response: 2524136971
Conc: 1467.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

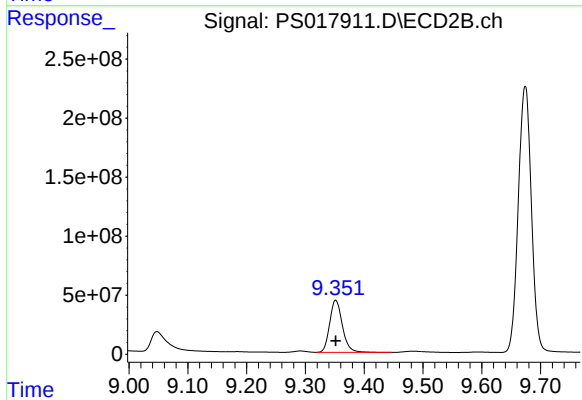


#13 2,4-DB

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 663304932
Conc: 1456.44 ng/ml

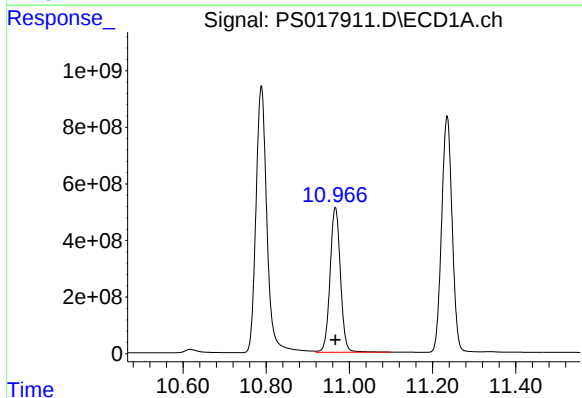


#14 DINOSEB

R.T.: 10.966 min
Delta R.T.: 0.000 min
Response: 8874641930
Conc: 1384.69 ng/ml

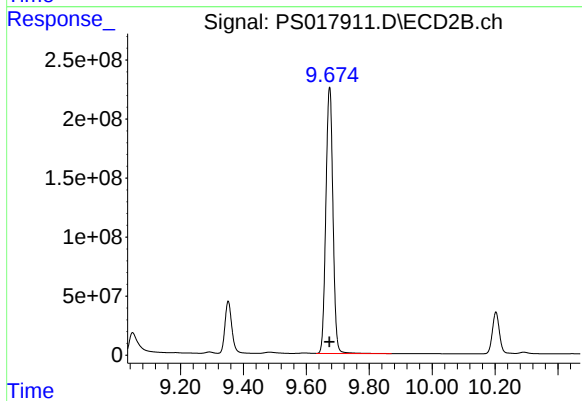

#14 DINOSEB


R.T.: 9.674 min
Delta R.T.: 0.000 min
Response: 3521145114
Conc: 1403.56 ng/ml

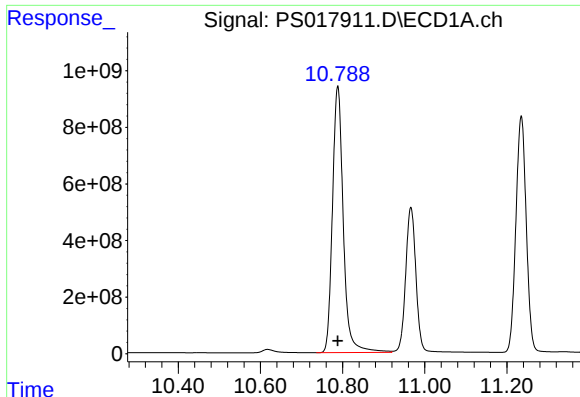

#15 Picloram


R.T.: 10.788 min
Delta R.T.: 0.000 min
Response: 17267809244
Conc: 1427.05 ng/m

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

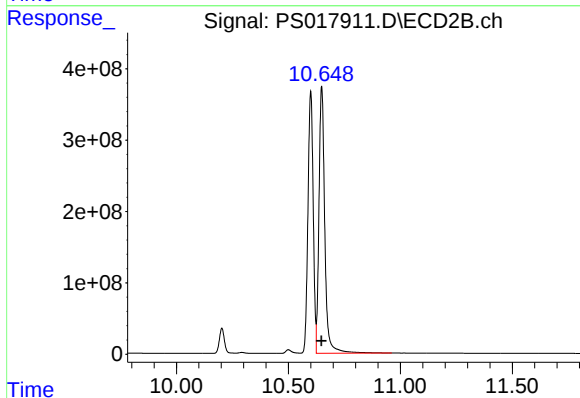


#15 Picloram

R.T.: 10.648 min
Delta R.T.: 0.000 min
Response: 6736084355
Conc: 1416.35 ng/ml

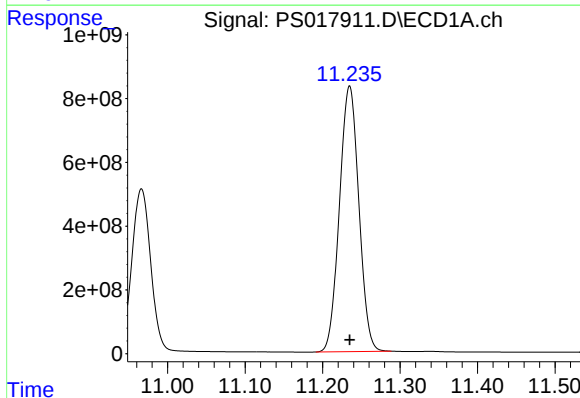

#16 DCPA

R.T.: 11.235 min
Delta R.T.: 0.000 min
Response: 14492034911
Conc: 1389.57 ng/ml

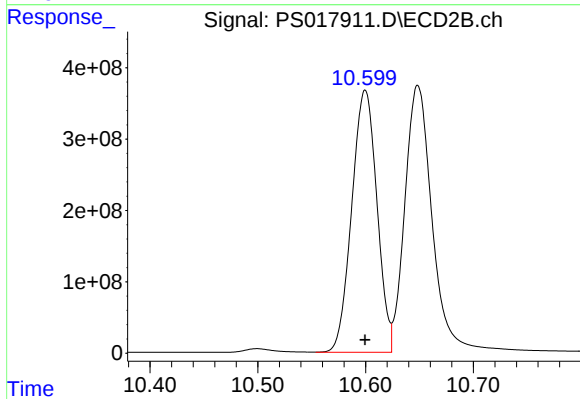

#16 DCPA

R.T.: 10.600 min
Delta R.T.: 0.000 min
Response: 5957276507
Conc: 1388.24 ng/ml