

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010524\
 Data File : PS025449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2024 09:33
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 23:25:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1) T	Dalapon	0.000	2.555	0	2377937	N.D.	2.069
2) T	3,5-DICHL...	5.693	0.000	3708863	0	1.091	N.D. #
5) T	DICAMBA	0.000	6.960	0	27070732	N.D.	8.944
6) T	MCPP	0.000	7.065f	0	292778	N.D.	<MDL
7) T	MCPA	0.000	7.165f	0	11396411	N.D.	3.626
8) T	DICHLORPROP	0.000	7.567	0	1153973	N.D.	1.492
9) T	2,4-D	7.247	0.000	210.9E6	0	68.084	N.D. #
15) T	Picloram	9.669	10.784	13741027	2927559	<MDL	<MDL #
16) T	DCPA	0.000	10.784f	0	2927559	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010524\
Data File : PS025449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2024 09:33
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 23:25:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

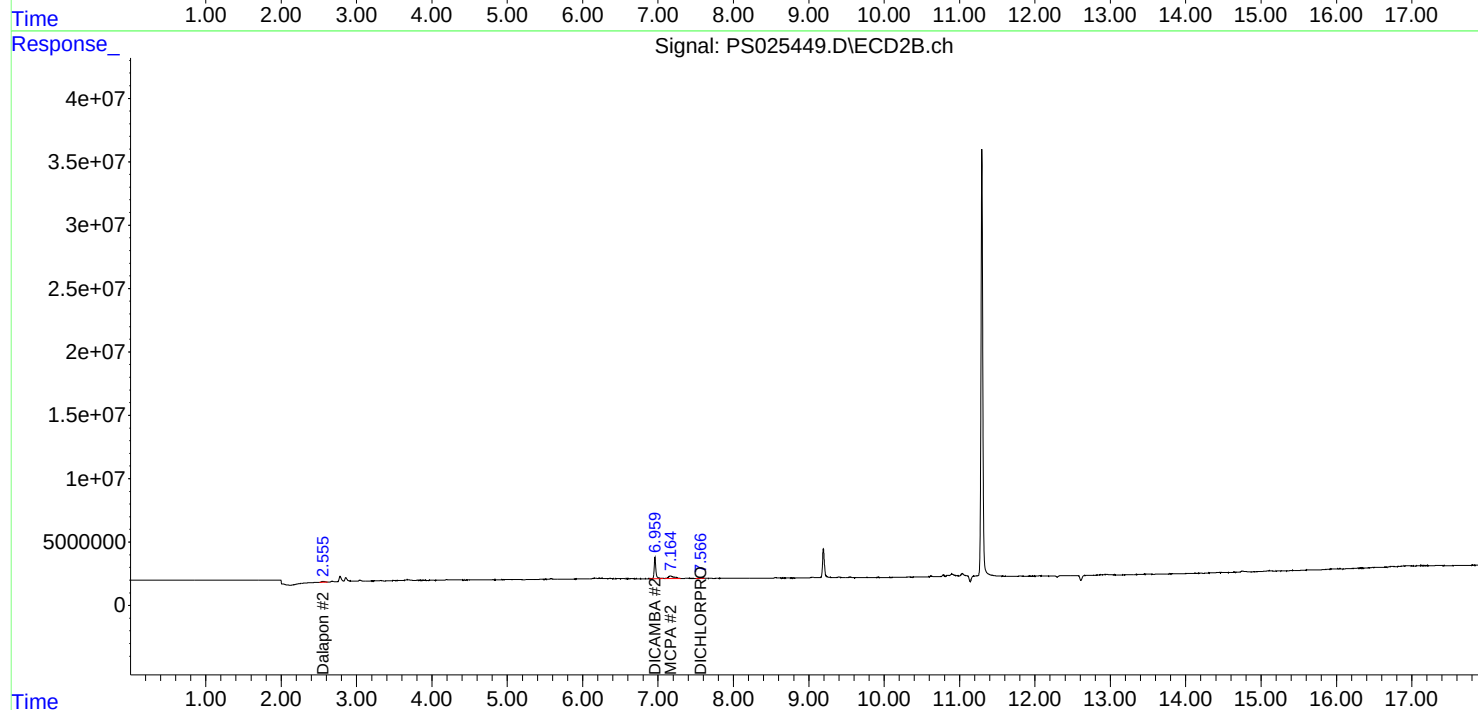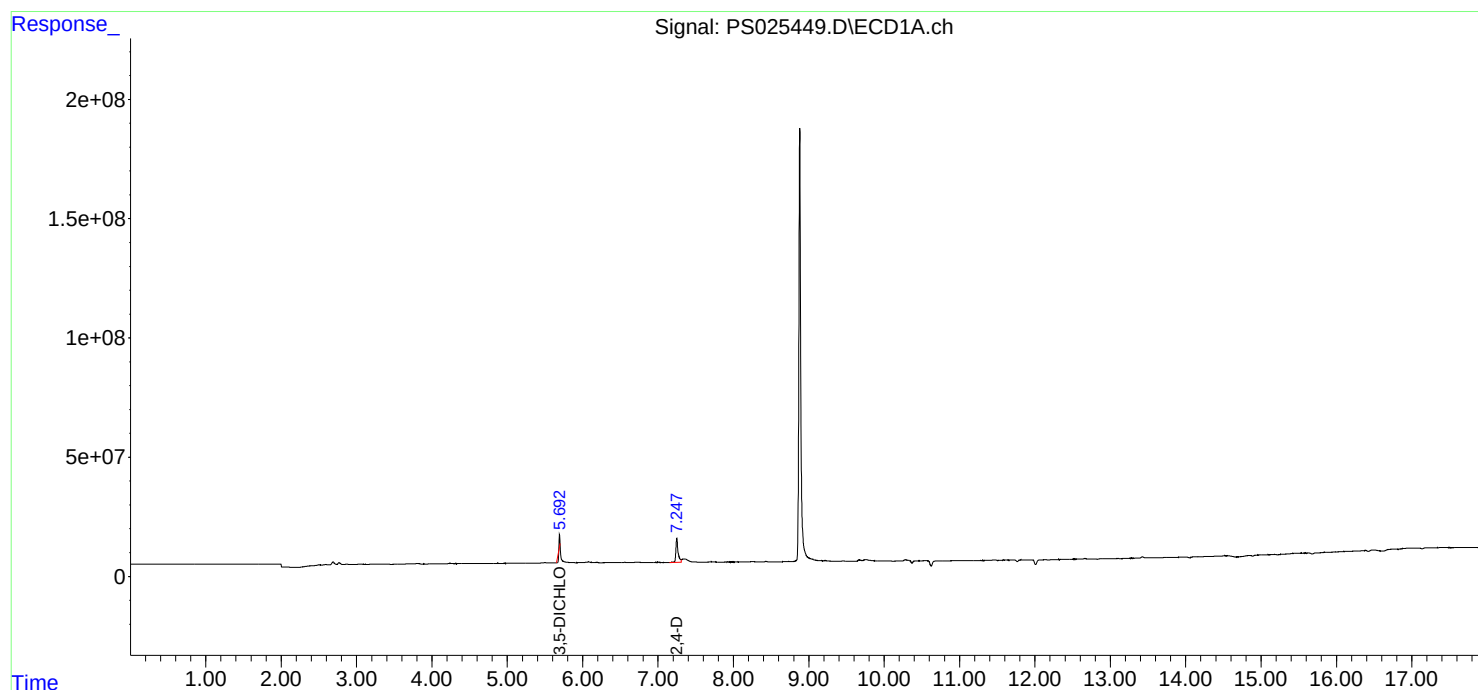


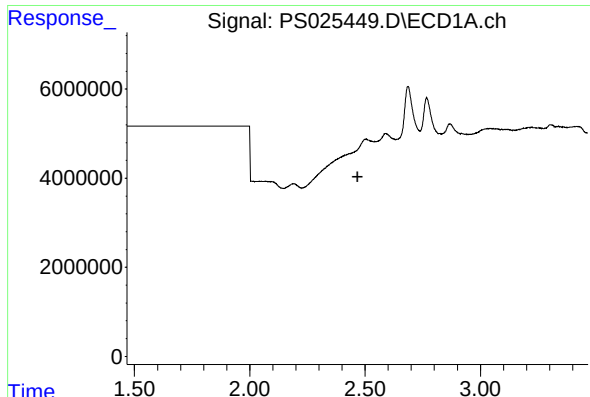

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

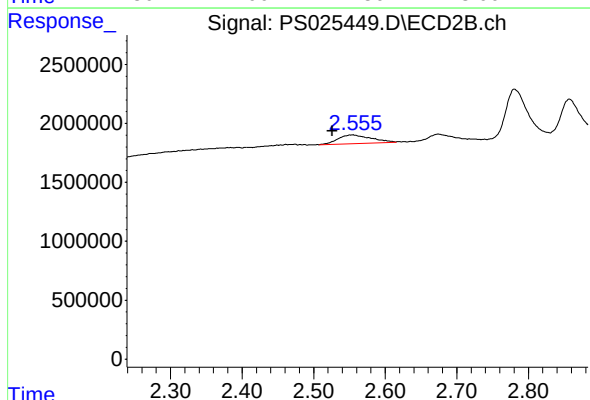


#1 Dalapon

R.T.: 2.555 min
Delta R.T.: 0.029 min
Response: 2377937
Conc: 2.07 ng/ml

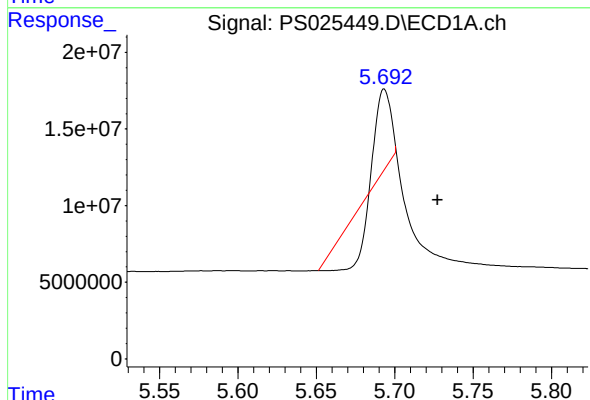


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.693 min
Delta R.T.: -0.034 min
Response: 3708863
Conc: 1.09 ng/ml

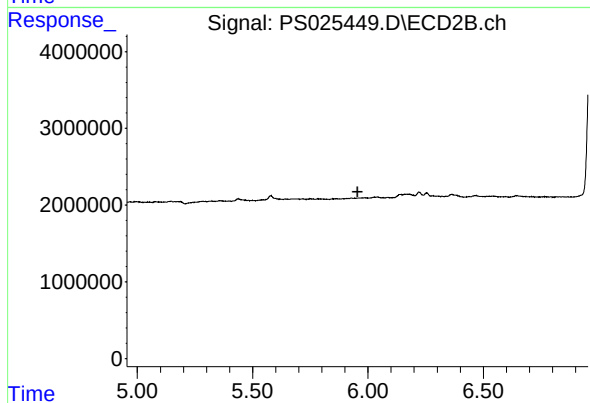

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

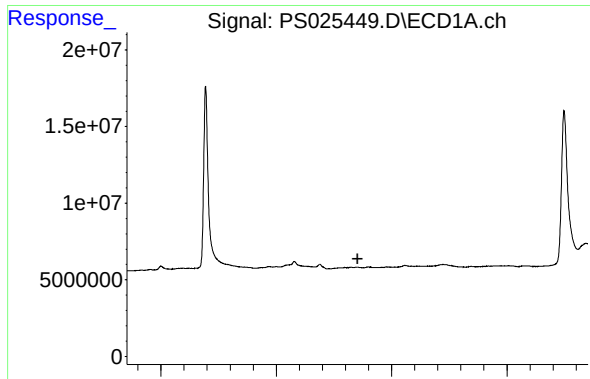

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

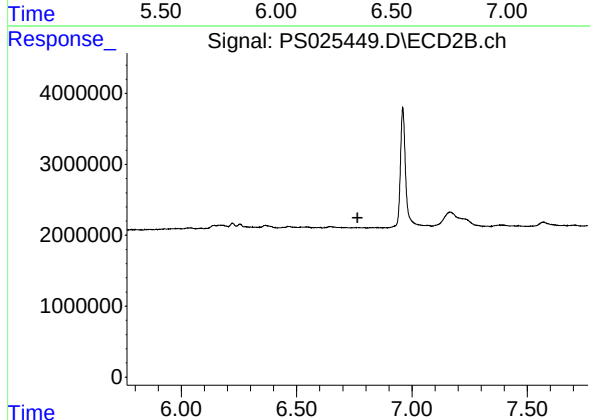


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

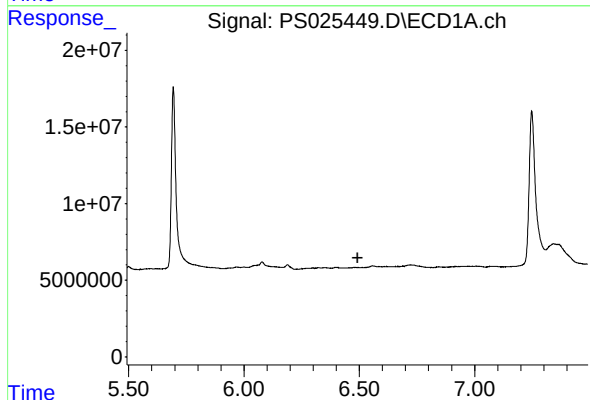


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

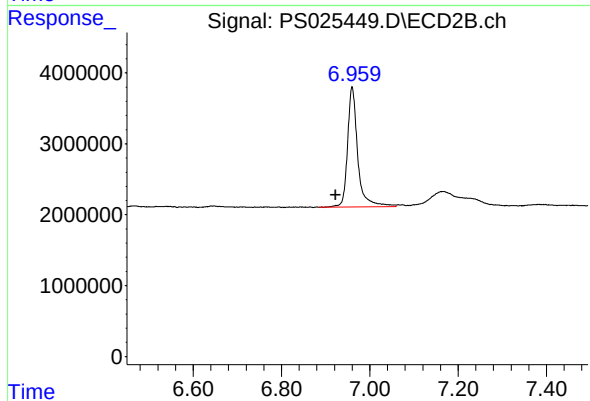

#5 DICAMBA


R.T.: 6.960 min
Delta R.T.: 0.037 min
Response: 27070732
Conc: 8.94 ng/ml

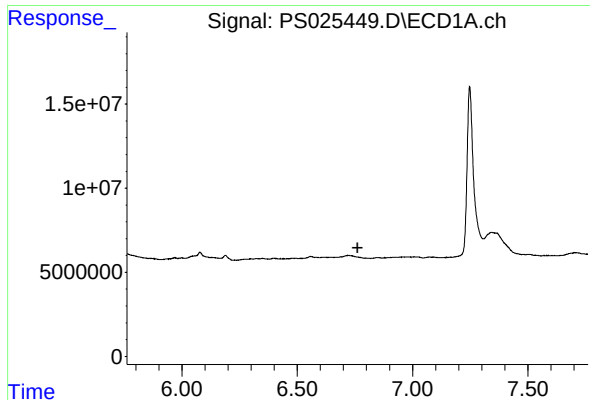

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

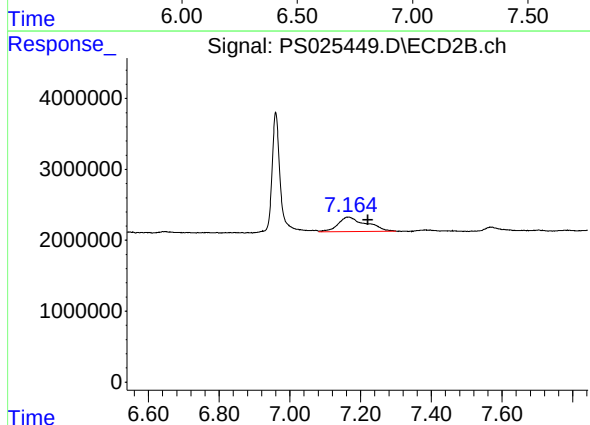


#7 MCPA

R.T.: 7.165 min
Delta R.T.: -0.056 min
Response: 11396411
Conc: 3.63 ug/ml

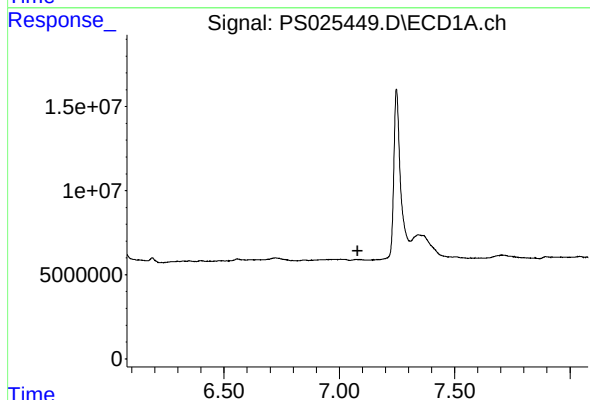


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

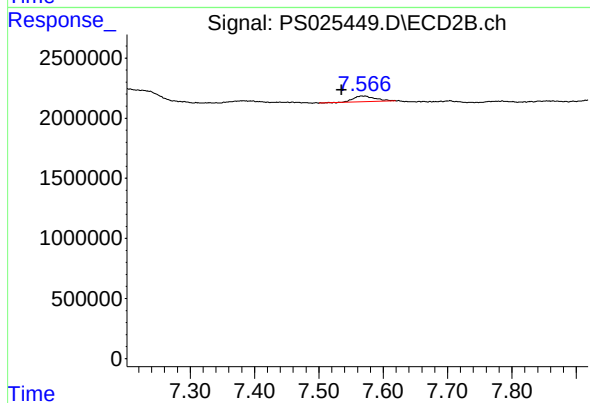

#8 DICHLORPROP


R.T.: 7.567 min
Delta R.T.: 0.032 min
Response: 1153973
Conc: 1.49 ng/ml

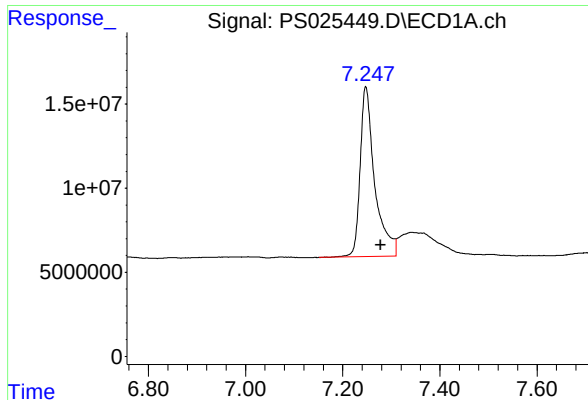

#9 2,4-D

R.T.: 7.247 min
Delta R.T.: -0.030 min
Response: 210917837
Conc: 68.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

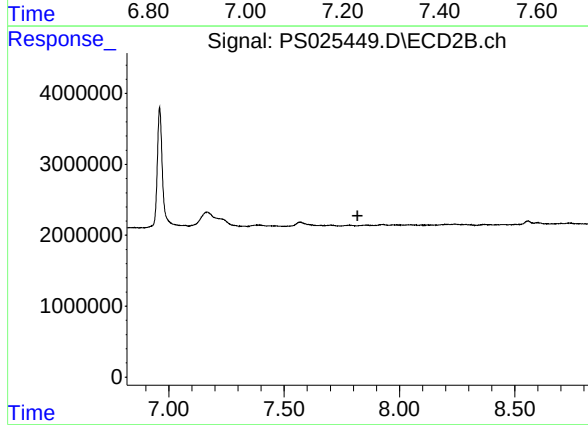

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.818 min
Response: 0
Conc: N.D.