

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010524\
 Data File : PS025450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2024 09:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 23:25:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.352	6.762	1094.3E6	350.4E6	488.350	493.620
Target Compounds						
1) T Dalapon	2.502	2.557	8171786	3085343	2.641	2.684
2) T 3,5-DICHL...	5.693	0.000	1497097	0	<MDL	N.D. #
3) T 4-Nitroph...	0.000	6.362	0	675366	N.D.	1.360
5) T DICAMBA	0.000	6.960	0	2189643	N.D.	<MDL
6) T MCPP	0.000	6.960f	0	2189643	N.D.	1.097
7) T MCPA	0.000	7.156f	0	11871786	N.D.	3.777
8) T DICHLORPROP	0.000	7.563	0	1194239	N.D.	1.544
9) T 2,4-D	7.250	0.000	21047537	0	6.794	N.D. #
13) T 2,4-DB	0.000	9.404f	0	1050616	N.D.	1.915
15) T Picloram	0.000	10.798f	0	3297437	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010524\
Data File : PS025450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2024 09:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 23:25:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

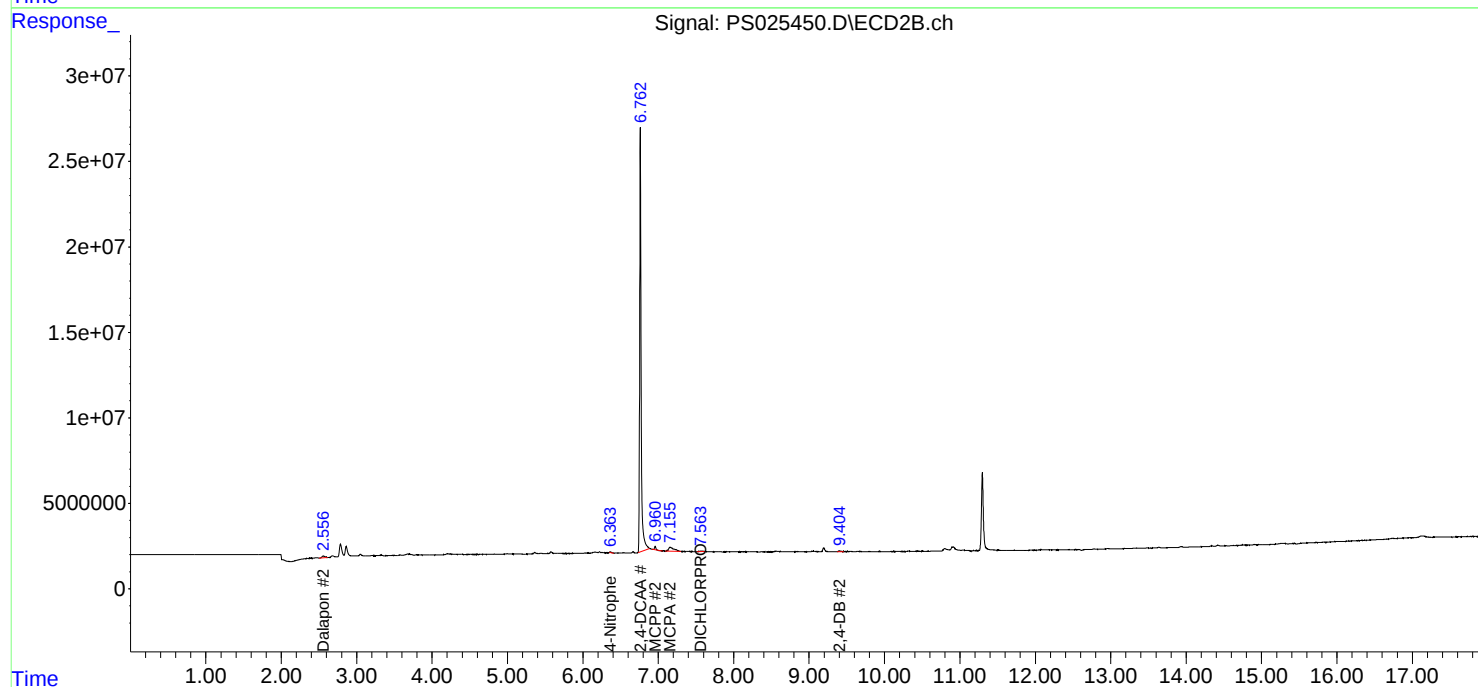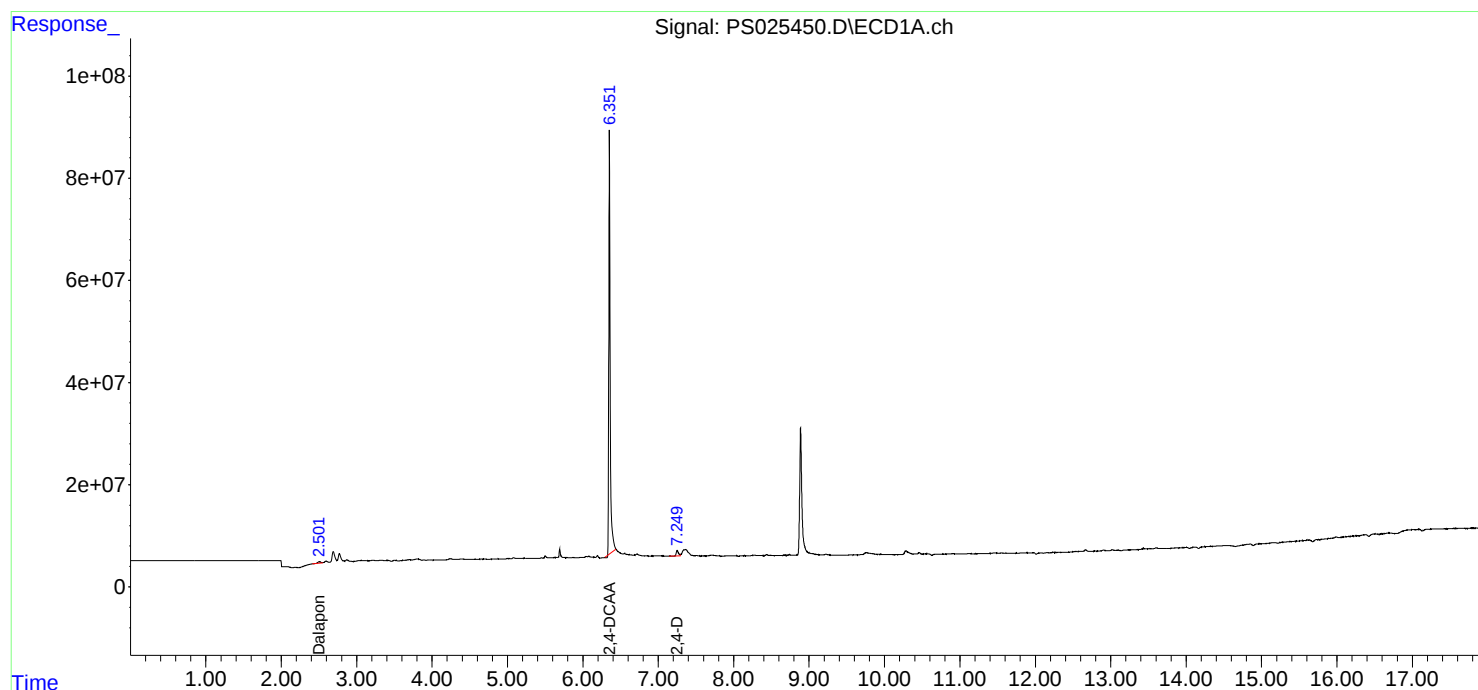


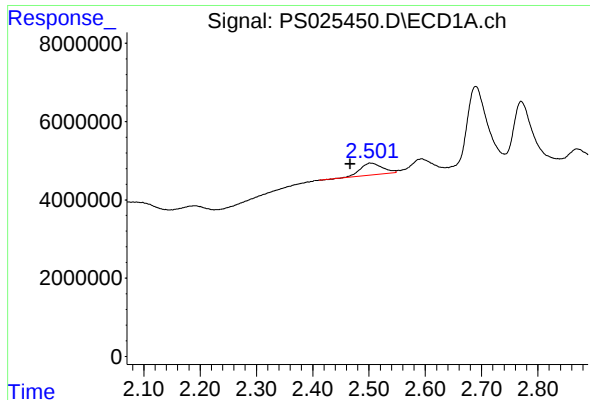

#1 Dalapon


R.T.: 2.502 min
Delta R.T.: 0.035 min
Response: 8171786
Conc: 2.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

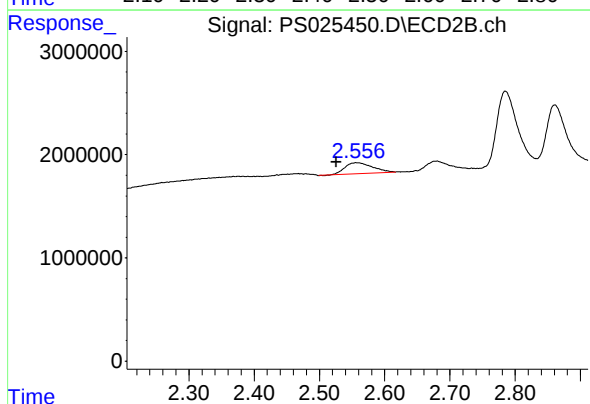


#1 Dalapon

R.T.: 2.557 min
Delta R.T.: 0.031 min
Response: 3085343
Conc: 2.68 ng/ml

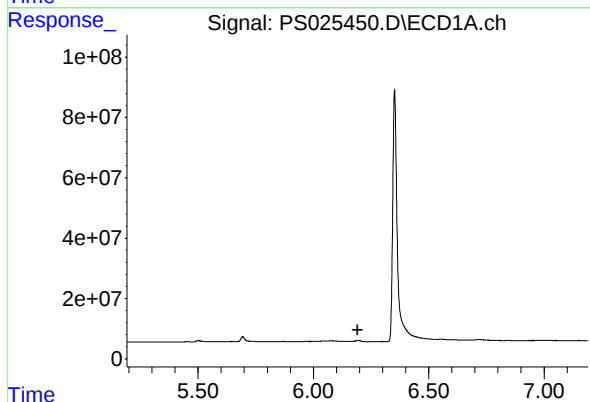


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

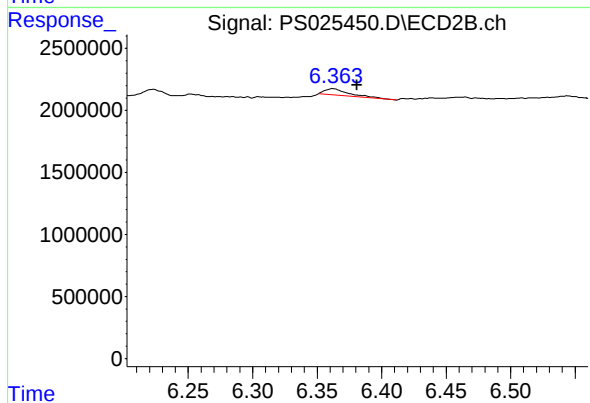

#3 4-Nitrophenol


R.T.: 6.362 min
Delta R.T.: -0.018 min
Response: 675366
Conc: 1.36 ng/ml

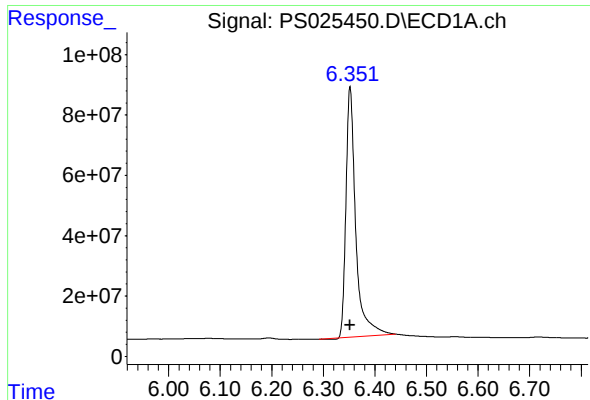

#4 2,4-DCAA


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 1094296680
Conc: 488.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

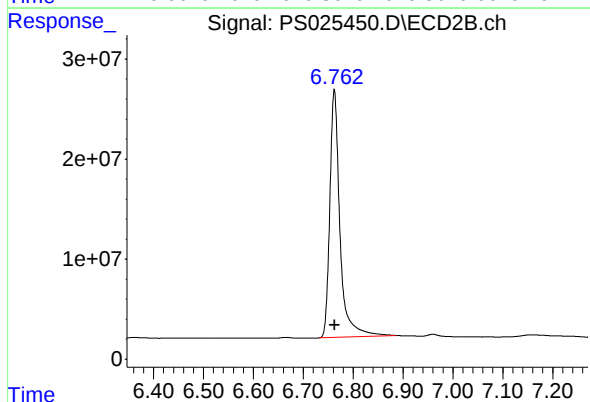


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 350358485
Conc: 493.62 ng/ml

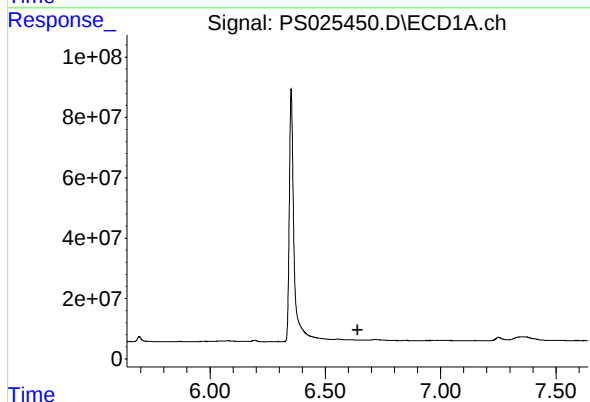


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

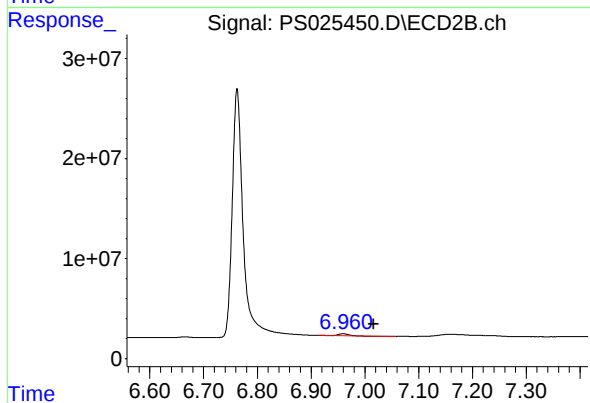

#6 MCPP


R.T.: 6.960 min
Delta R.T.: -0.057 min
Response: 2189643
Conc: 1.10 ug/ml

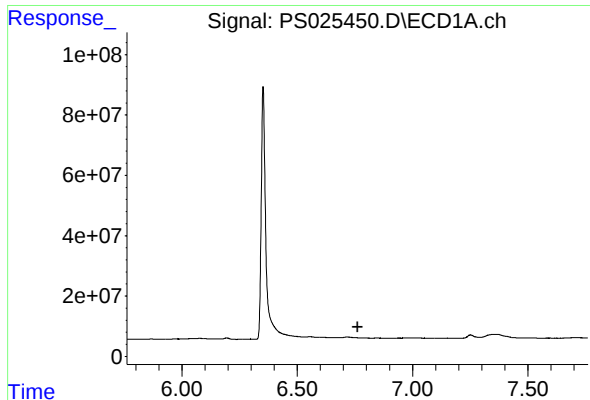

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

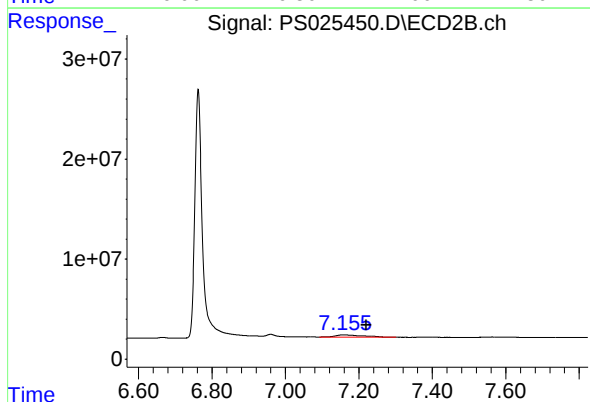


#7 MCPA

R.T.: 7.156 min
Delta R.T.: -0.065 min
Response: 11871786
Conc: 3.78 ug/ml

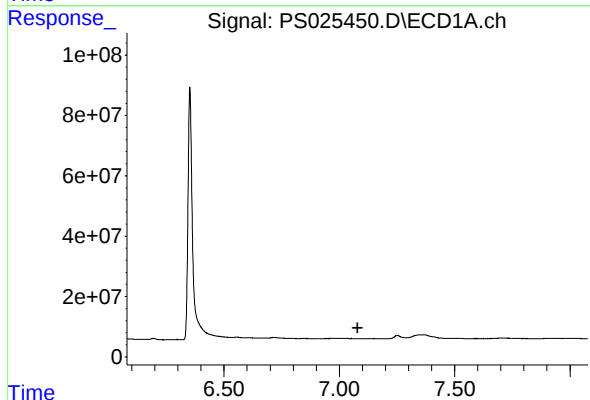


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

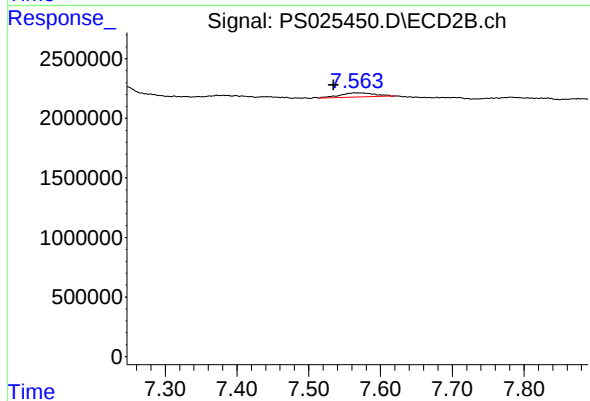

#8 DICHLORPROP


R.T.: 7.563 min
Delta R.T.: 0.028 min
Response: 1194239
Conc: 1.54 ng/ml

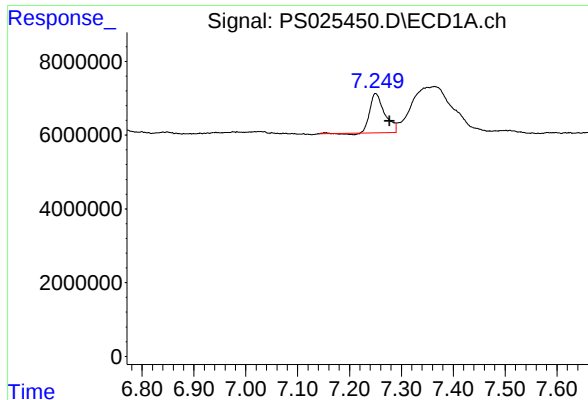

#9 2,4-D


R.T.: 7.250 min
Delta R.T.: -0.027 min
Response: 21047537
Conc: 6.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

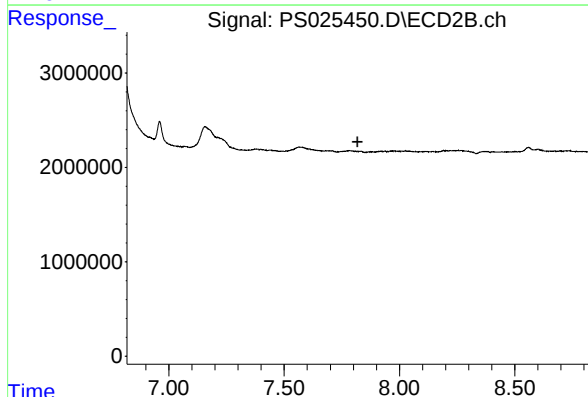


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.818 min
Response: 0
Conc: N.D.

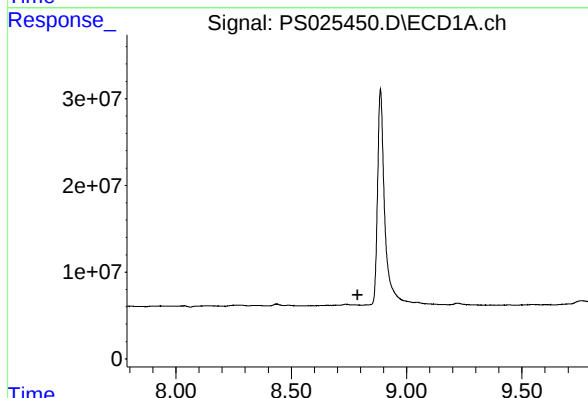

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.787 min
Response: 0
Conc: N.D.

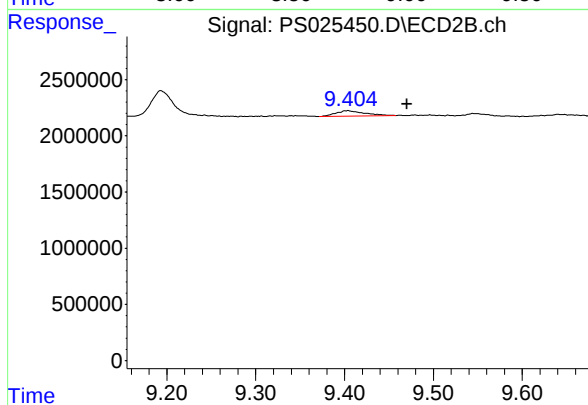

#13 2,4-DB

R.T.: 9.404 min
Delta R.T.: -0.067 min
Response: 1050616
Conc: 1.92 ng/ml