

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010524\
 Data File : PS025470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2024 22:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 23:31:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 28 17:23:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.352	6.762	1135.4E6	365.8E6	506.685	515.426
Target Compounds							
1) T	Dalapon	0.000	2.559	0	2778334	N.D.	2.417
3) T	4-Nitroph...	0.000	6.362	0	547157	N.D.	1.102
5) T	DICAMBA	0.000	6.960	0	3761097	N.D.	1.243
6) T	MCPD	0.000	6.960f	0	3761097	N.D.	1.884
7) T	MCPA	0.000	7.156f	0	12099862	N.D.	3.850
8) T	DICHLORPROP	0.000	7.565	0	2689326	N.D.	3.477
9) T	2,4-D	7.252	0.000	31341489	0	10.117	N.D. #
10) T	Pentachlo...	0.000	8.238	0	1130200	N.D.	<MDL
12) T	2,4,5-T	0.000	8.993	0	724507	N.D.	<MDL
13) T	2,4-DB	0.000	9.404f	0	1308273	N.D.	2.385
15) T	Picloram	0.000	10.715	0	437612	N.D.	<MDL
16) T	DCPA	0.000	10.715	0	437612	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010524\
Data File : PS025470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2024 22:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 23:31:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122823.M
Quant Title : 8080.M
QLast Update : Thu Dec 28 17:23:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

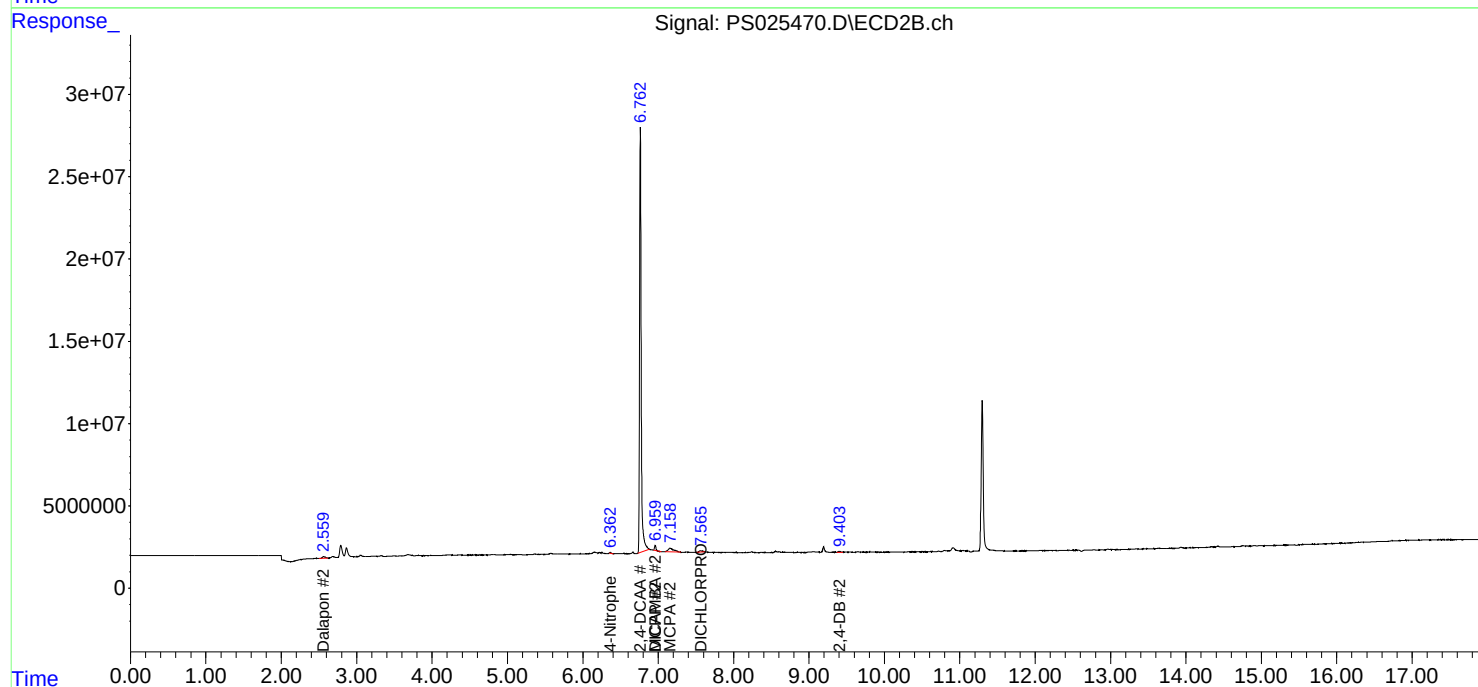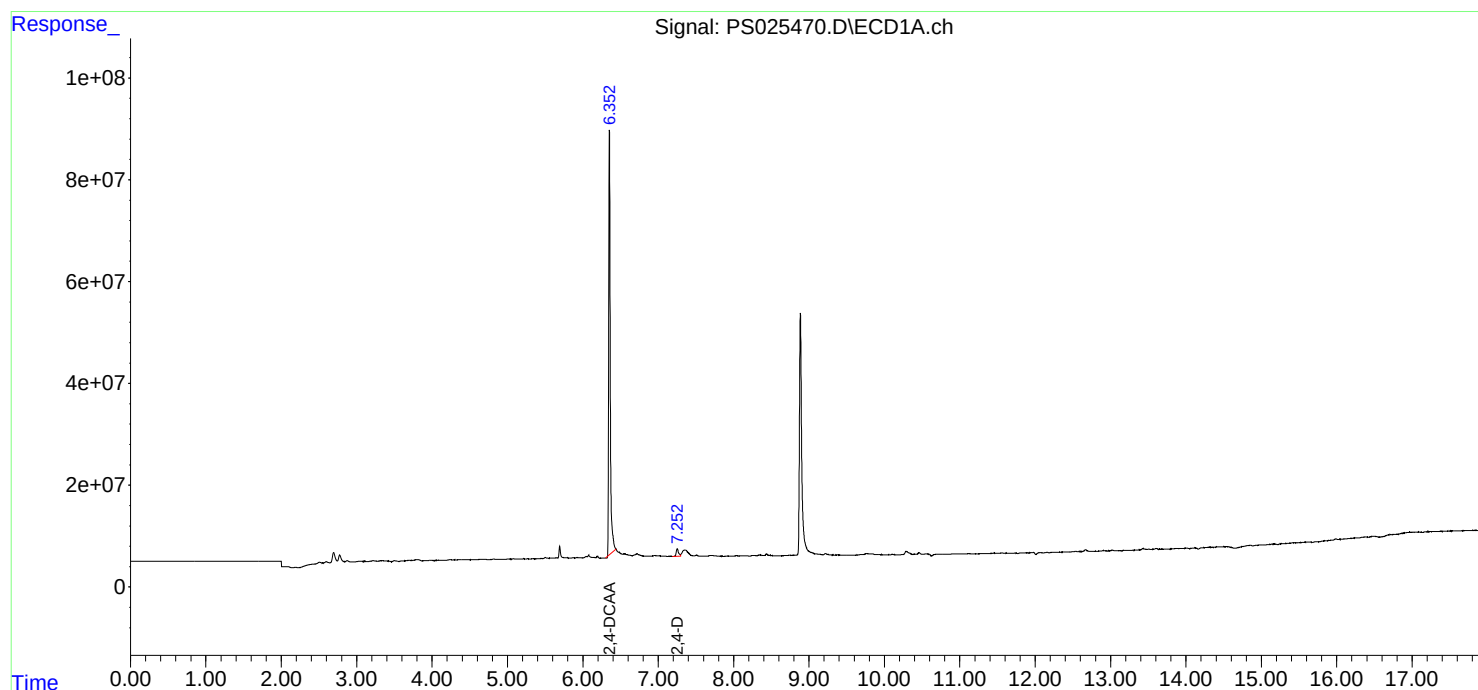


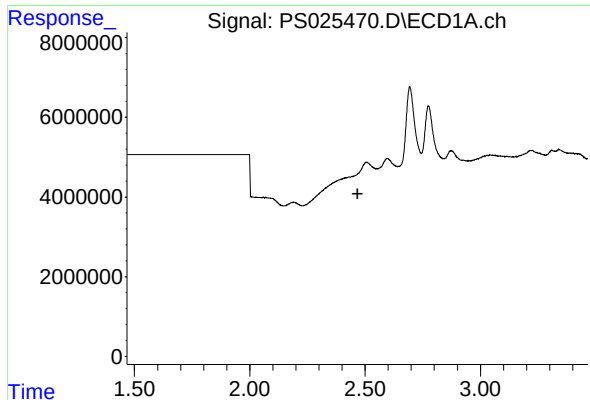

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

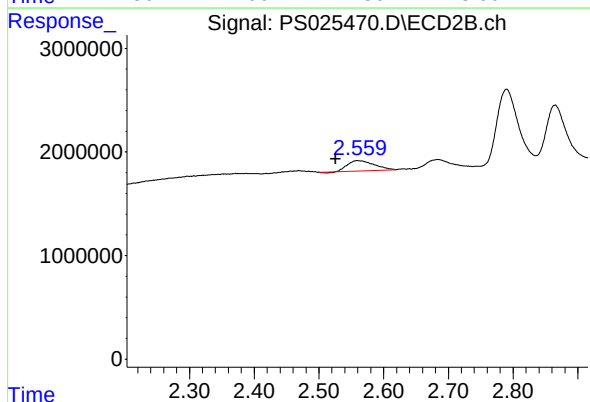


#1 Dalapon

R.T.: 2.559 min
Delta R.T.: 0.034 min
Response: 2778334
Conc: 2.42 ng/ml

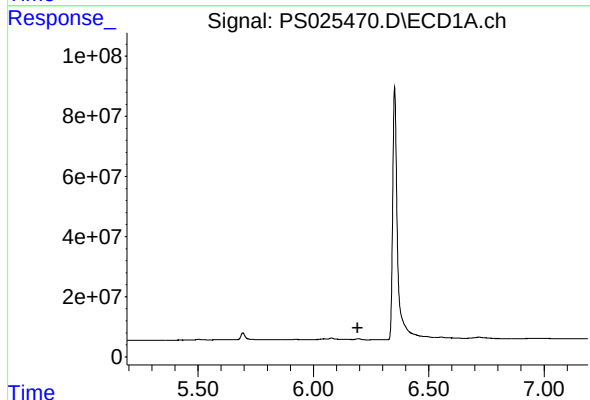


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

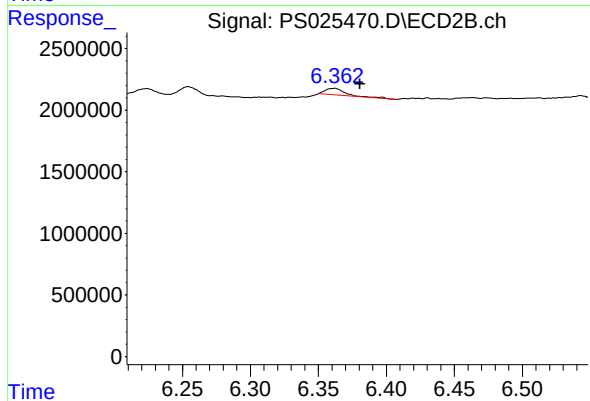

#3 4-Nitrophenol


R.T.: 6.362 min
Delta R.T.: -0.019 min
Response: 547157
Conc: 1.10 ng/ml

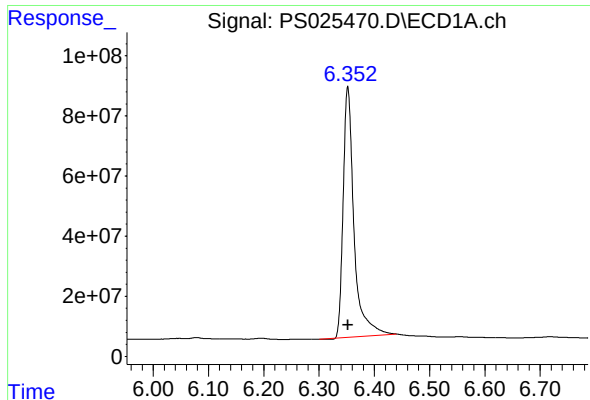

#4 2,4-DCAA


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 1135381503
Conc: 506.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

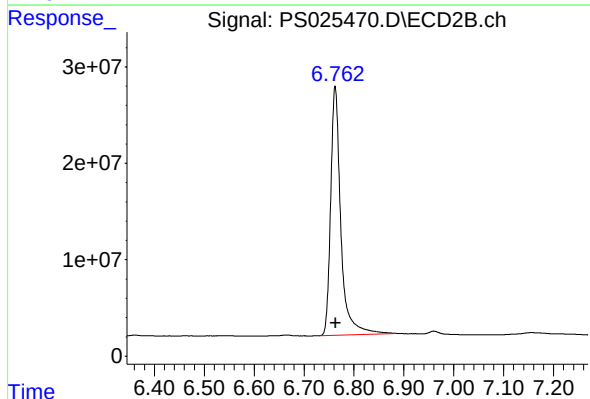


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 365835769
Conc: 515.43 ng/ml

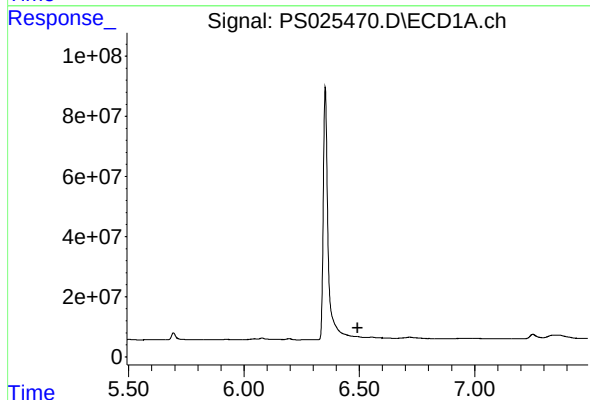


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.492 min
Response: 0
Conc: N.D.

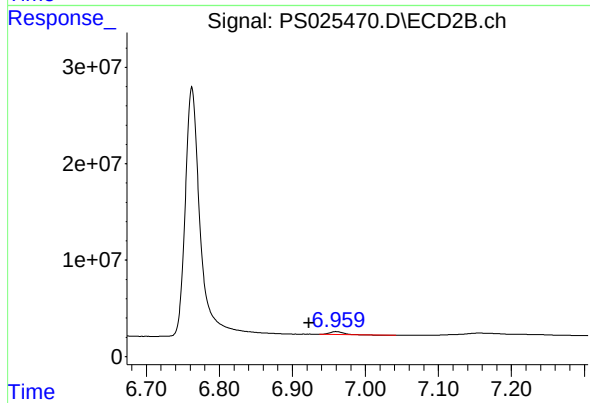

#5 DICAMBA


R.T.: 6.960 min
Delta R.T.: 0.037 min
Response: 3761097
Conc: 1.24 ng/ml

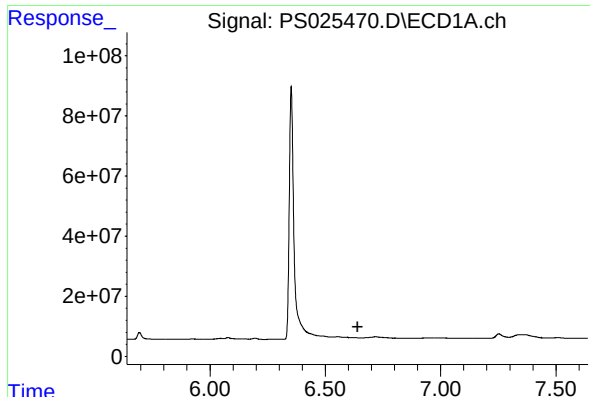

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

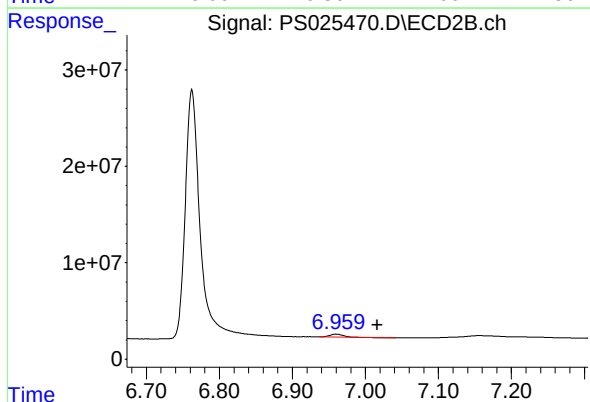


#6 MCPP

R.T.: 6.960 min
Delta R.T.: -0.057 min
Response: 3761097
Conc: 1.88 ug/ml

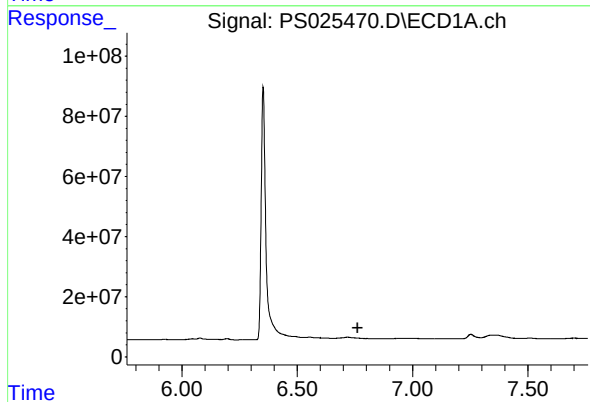


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

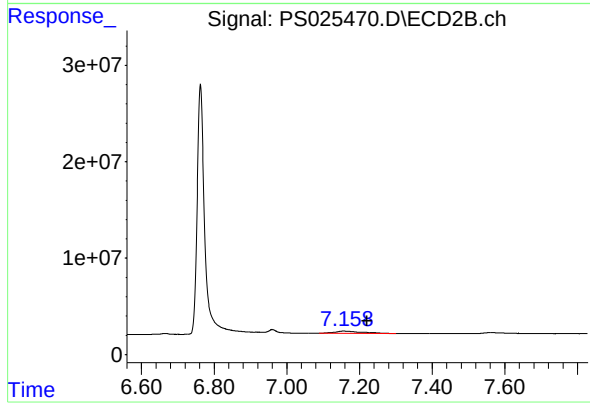

#7 MCPA


R.T.: 7.156 min
Delta R.T.: -0.065 min
Response: 12099862
Conc: 3.85 ug/ml

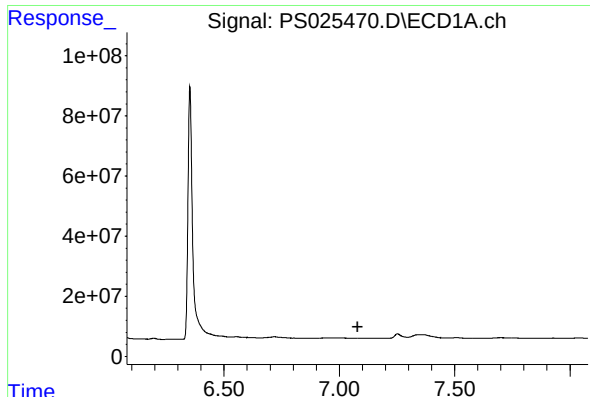

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

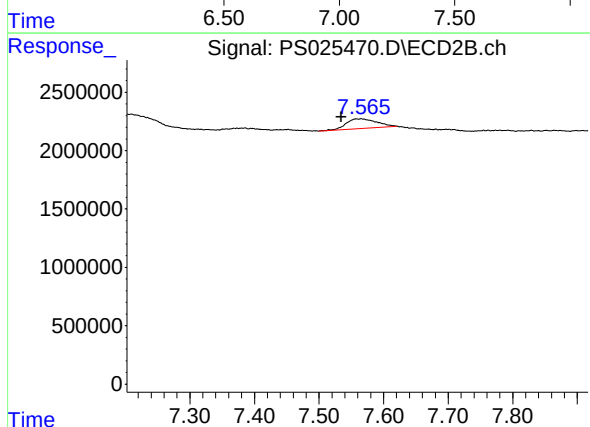


#8 DICHLORPROP

R.T.: 7.565 min
Delta R.T.: 0.030 min
Response: 2689326
Conc: 3.48 ng/ml

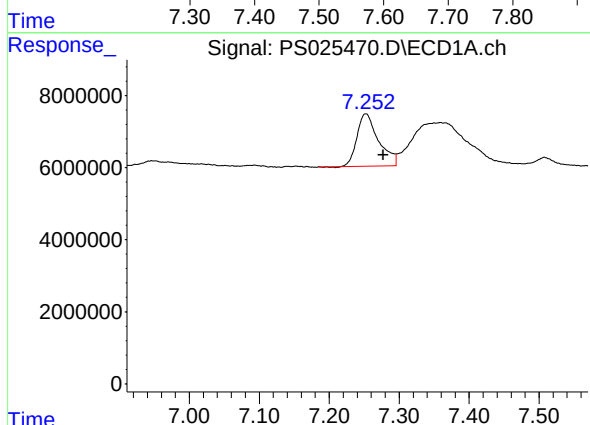


#9 2,4-D

R.T.: 7.252 min
Delta R.T.: -0.025 min
Response: 31341489
Conc: 10.12 ng/ml

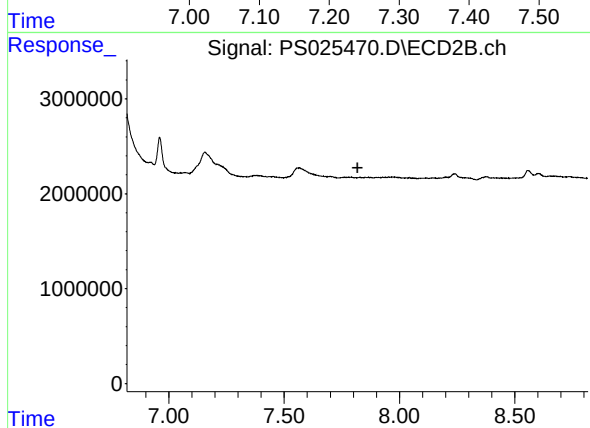

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.818 min
Response: 0
Conc: N.D.

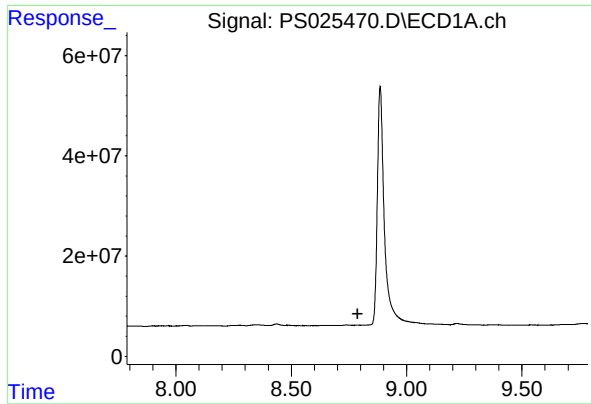

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.787 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

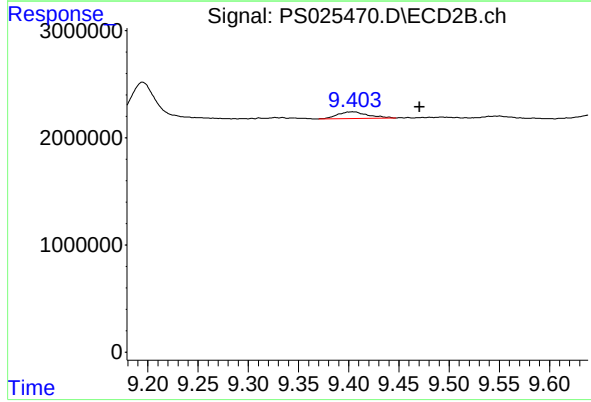

#13 2,4-DB

R.T.: 9.404 min
Delta R.T.: -0.067 min
Response: 1308273
Conc: 2.38 ng/ml