

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS010622\  
 Data File : PS017930.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 06 Jan 2022 18:54  
 Operator : AJ\MA  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 07 00:11:43 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS010522.M  
 Quant Title : 8080.M  
 QLast Update : Thu Jan 06 10:21:08 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|-------|----------|---------|---------|---------|
| -----                       |              |        |       |          |         |         |         |
| System Monitoring Compounds |              |        |       |          |         |         |         |
| 4) S                        | 2,4-DCAA     | 7.050  | 6.644 | 617.3E6  | 288.4E6 | 427.067 | 497.100 |
| Target Compounds            |              |        |       |          |         |         |         |
| 2) T                        | 3,5-DICHL... | 6.320  | 0.000 | 3007139  | 0       | 1.398   | N.D. #  |
| 7) T                        | MCPA         | 7.499f | 0.000 | 6607271  | 0       | <MDL    | N.D. #  |
| 9) T                        | 2,4-D        | 8.207f | 0.000 | 16294611 | 0       | 8.948   | N.D. #  |
| 15) T                       | Picloram     | 10.775 | 0.000 | 49477272 | 0       | 4.145   | N.D. #  |
| -----                       |              |        |       |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS010622\  
Data File : PS017930.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 06 Jan 2022 18:54  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 07 00:11:43 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS010522.M  
Quant Title : 8080.M  
QLast Update : Thu Jan 06 10:21:08 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

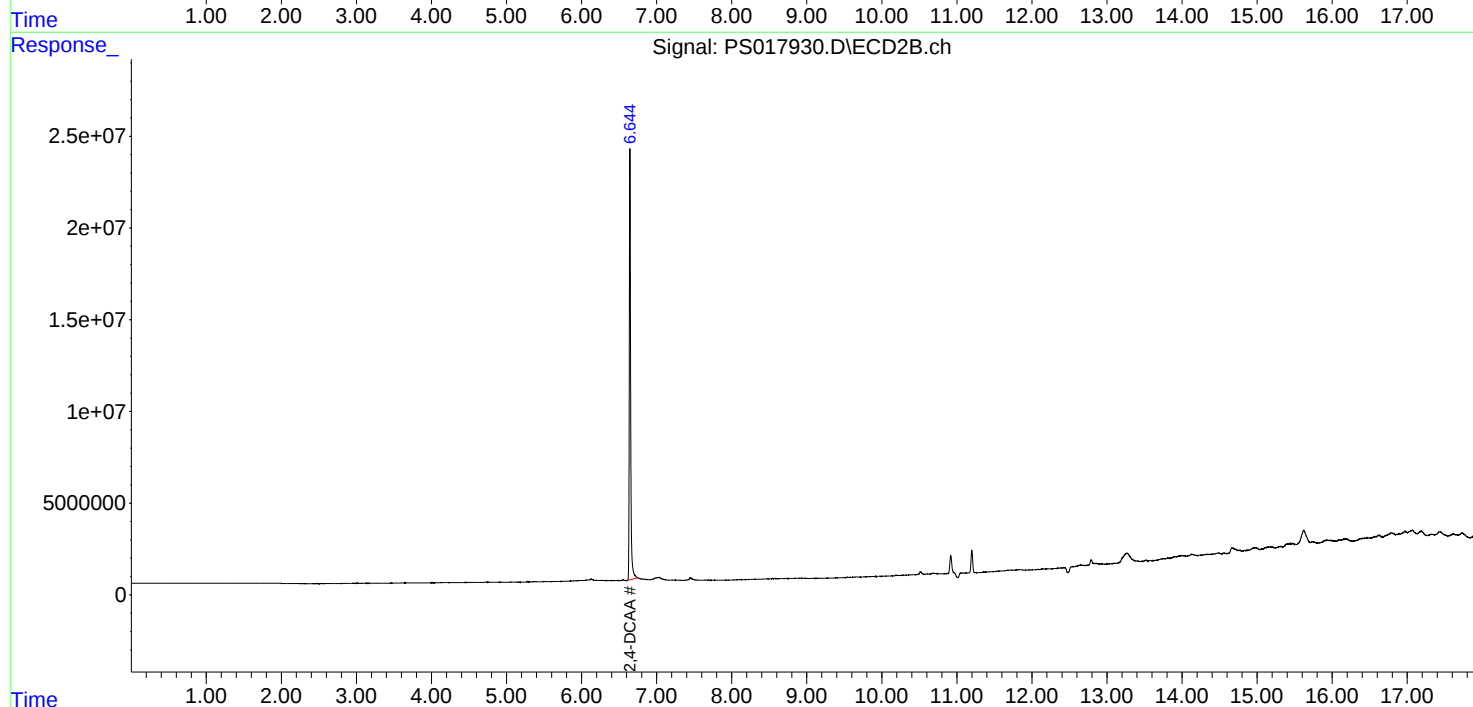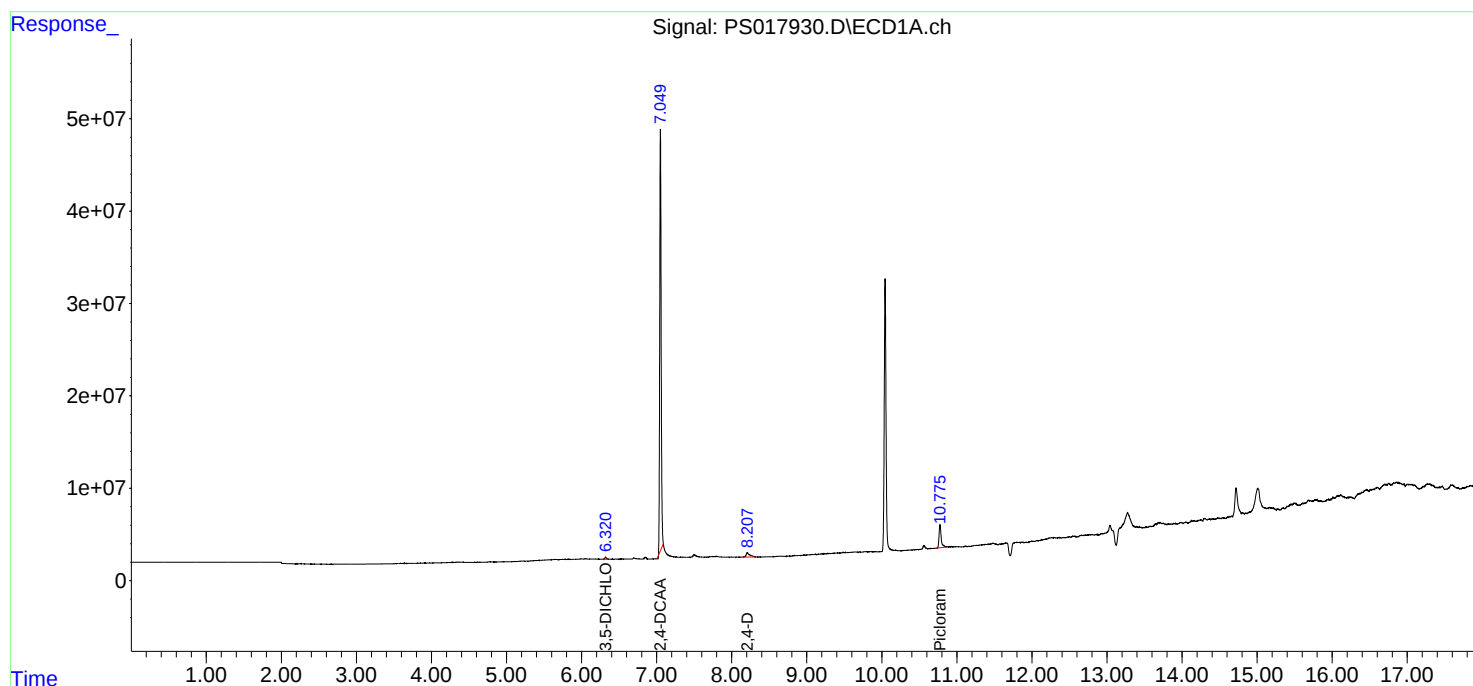


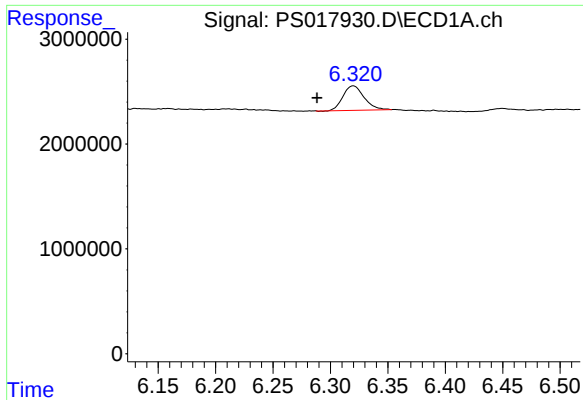

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.320 min  
Delta R.T.: 0.032 min  
Response: 3007139  
Conc: 1.40 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

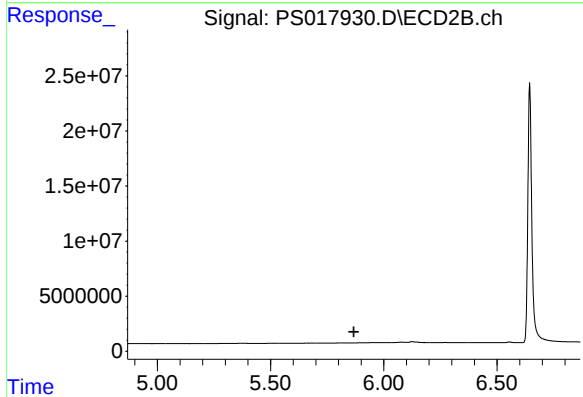


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T. : 5.868 min  
Response: 0  
Conc: N.D.

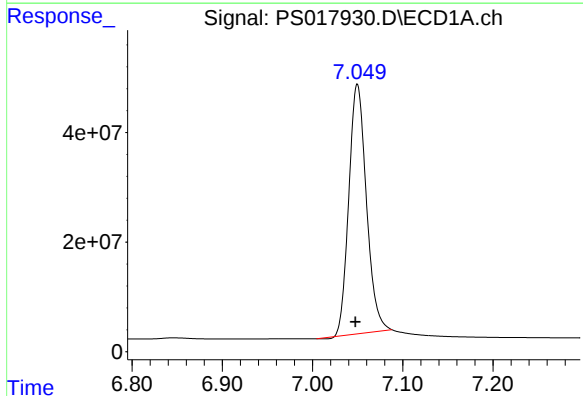


#4 2,4-DCAA

R.T.: 7.050 min  
Delta R.T.: 0.002 min  
Response: 617320032  
Conc: 427.07 ng/ml

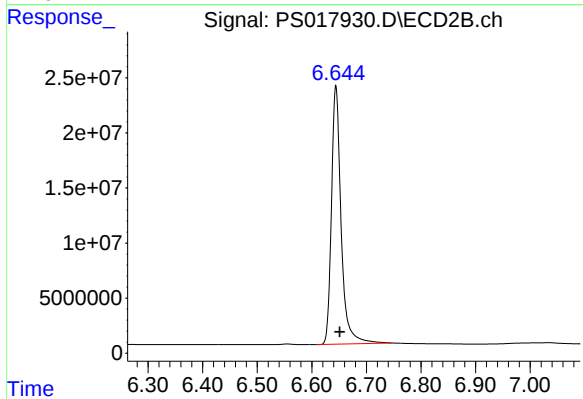

#4 2,4-DCAA


R.T.: 6.644 min  
Delta R.T.: -0.007 min  
Response: 288441631  
Conc: 497.10 ng/ml

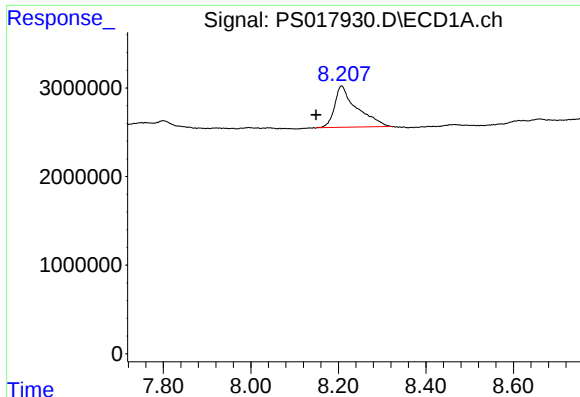

#9 2,4-D


R.T.: 8.207 min  
Delta R.T.: 0.058 min  
Response: 16294611  
Conc: 8.95 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

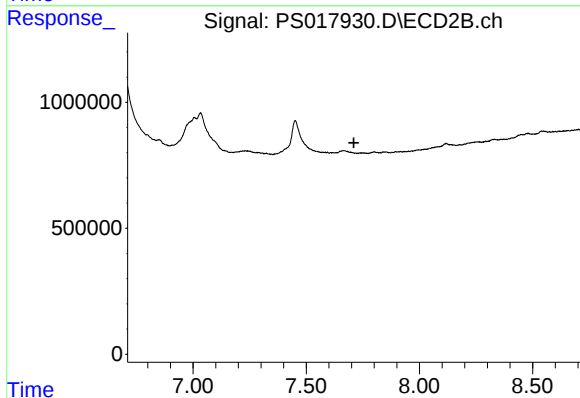


#9 2,4-D

R.T.: 0.000 min  
Exp R.T. : 7.710 min  
Response: 0  
Conc: N.D.

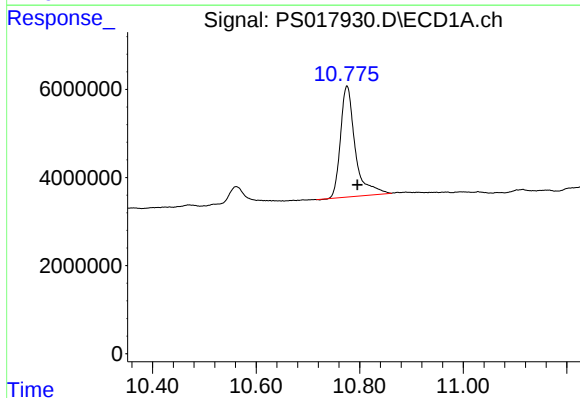

#15 Picloram

R.T.: 10.775 min  
Delta R.T.: -0.021 min  
Response: 49477272  
Conc: 4.15 ng/ml

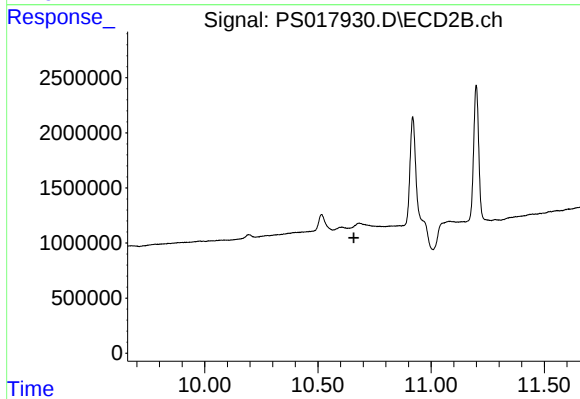

#15 Picloram

R.T.: 0.000 min  
Exp R.T. : 10.659 min  
Response: 0  
Conc: N.D.