

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010819\
 Data File : PS002755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2019 09:46
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 23:51:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010419.M
 Quant Title : 8080.M
 QLast Update : Sat Jan 05 06:20:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.864	0	193409	N.D.	0.509 #
Target Compounds							
3) T	4-Nitroph...	0.000	10.030	0	574474	N.D.	3.307 #
9) T	2,4-D	0.000	12.739	0	233656	N.D.	0.584 #
13) T	2,4-DB	0.000	15.203	0	630183	N.D.	3.346 #
15) T	Picloram	0.000	16.814	0	10936916	N.D.	4.084 #
16) T	DCPA	0.000	16.814	0	10936916	N.D.	4.223 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010819\
Data File : PS002755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2019 09:46
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 23:51:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010419.M
Quant Title : 8080.M
QLast Update : Sat Jan 05 06:20:43 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

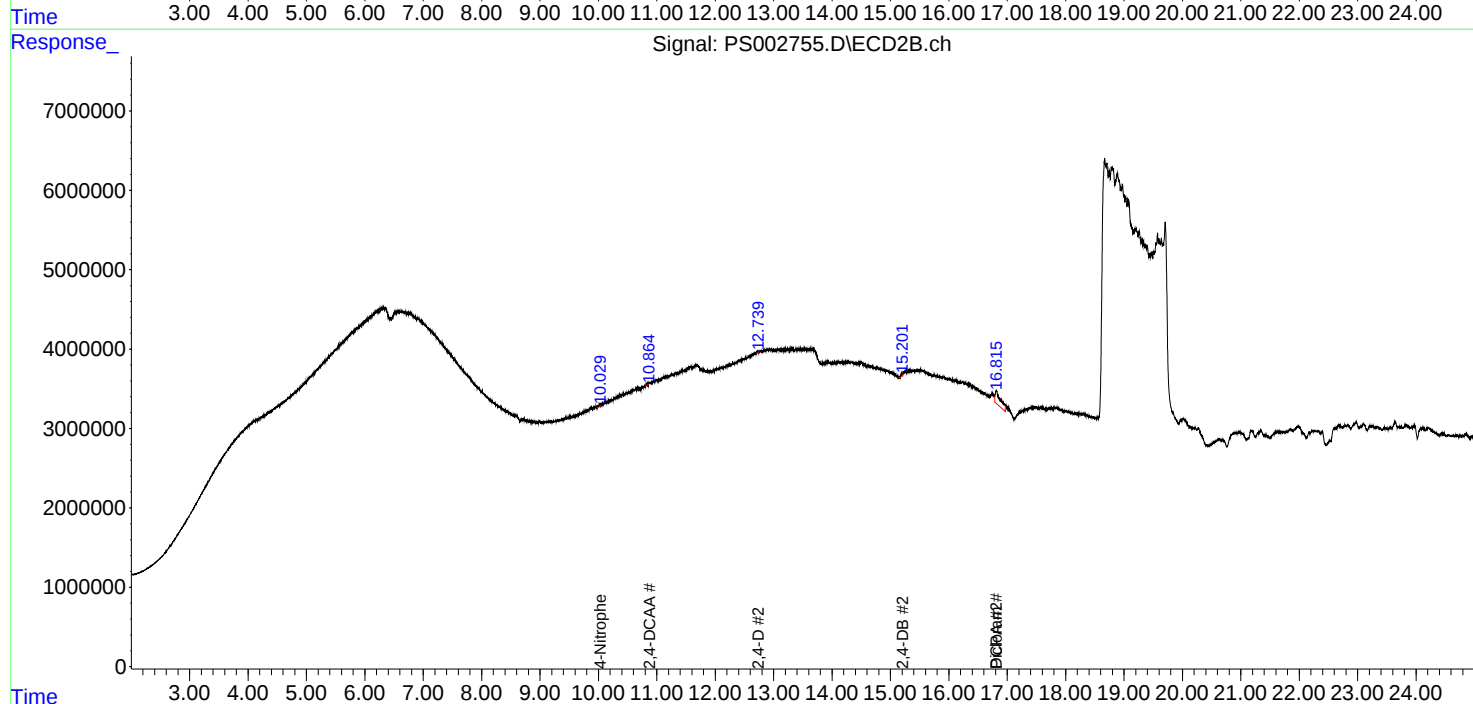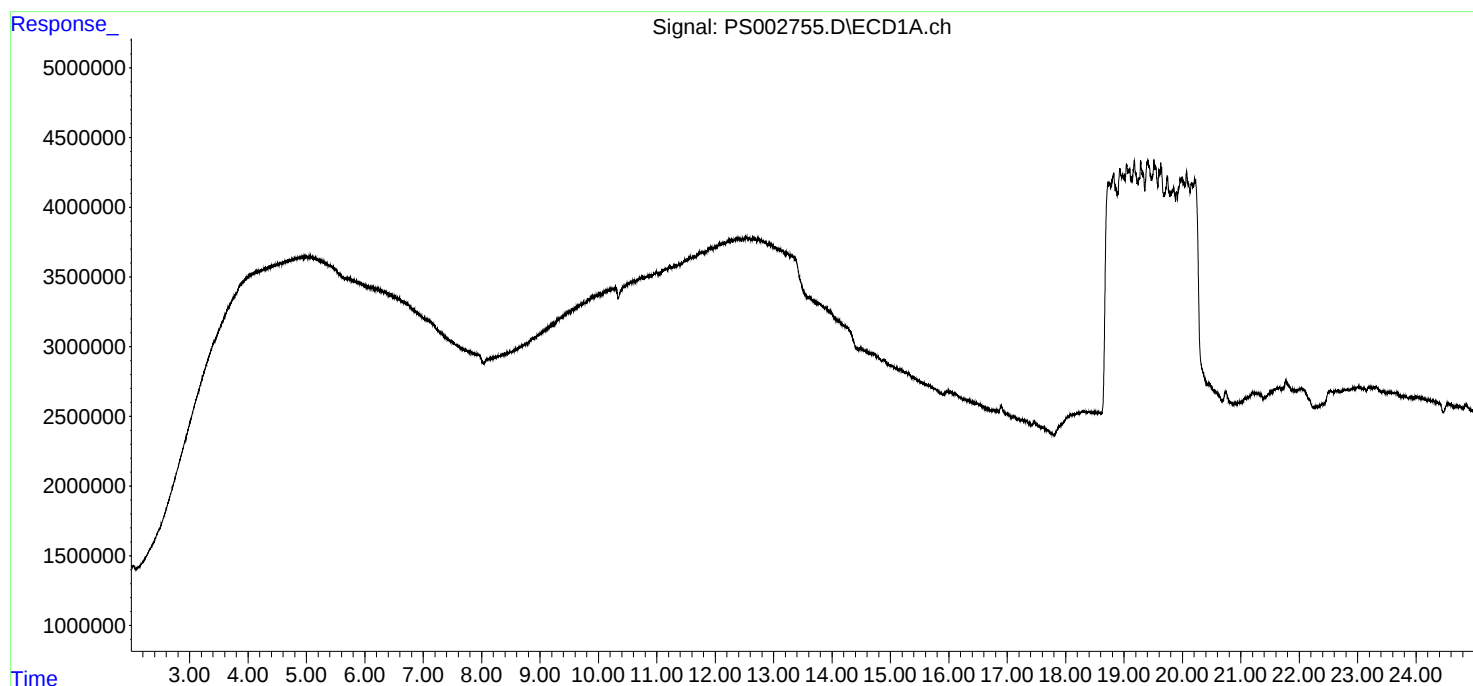


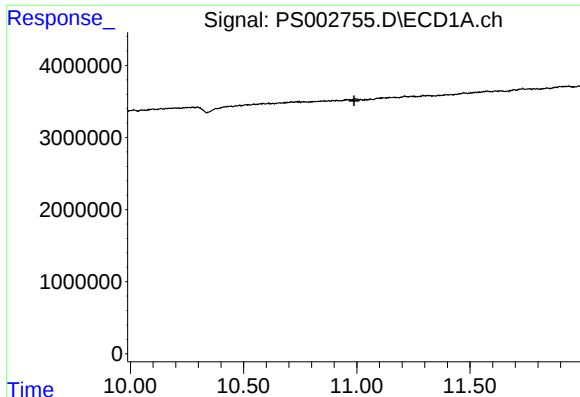

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.987 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

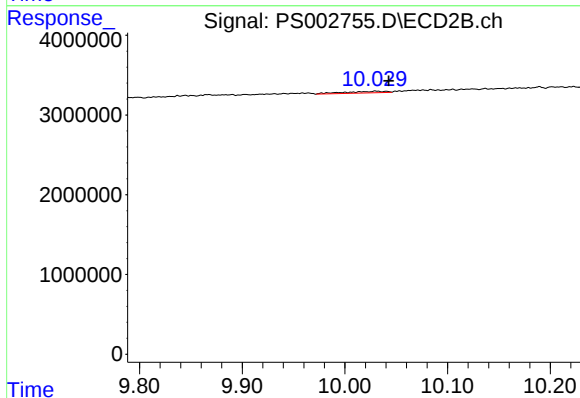


#3 4-Nitrophenol

R.T.: 10.030 min
Delta R.T.: -0.012 min
Response: 574474
Conc: 3.31 ng/ml

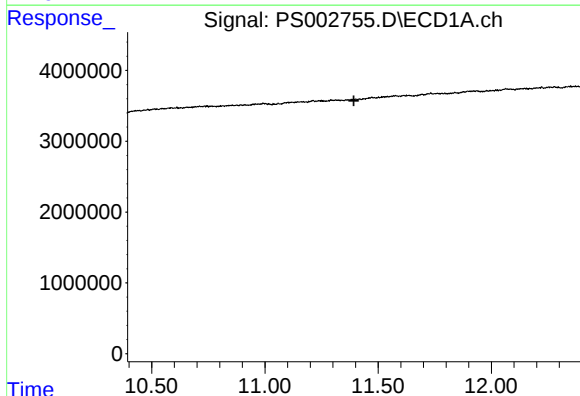


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.393 min
Response: 0
Conc: N.D.

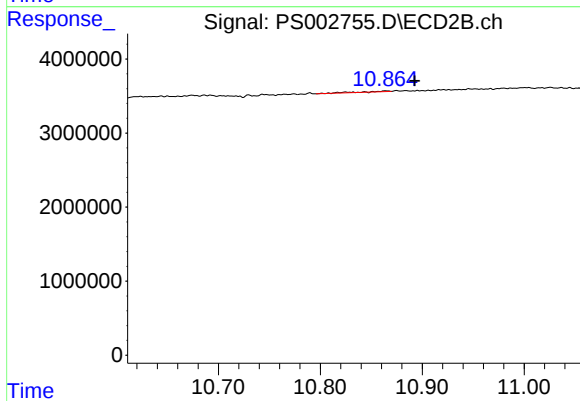

#4 2,4-DCAA


R.T.: 10.864 min
Delta R.T.: -0.028 min
Response: 193409
Conc: 0.51 ng/ml

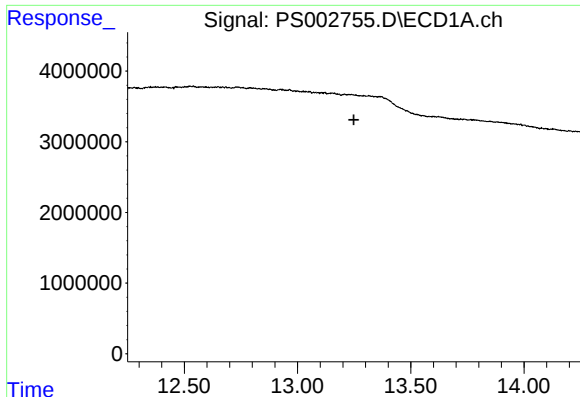

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.248 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

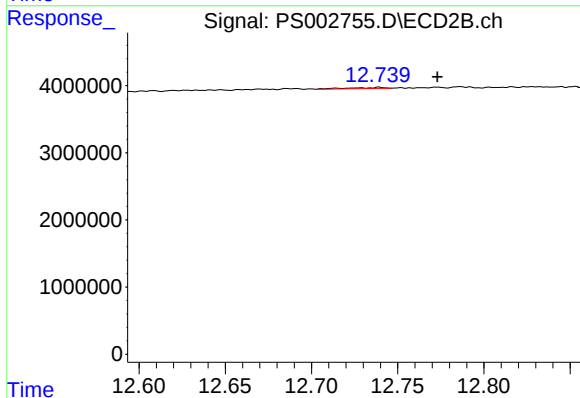


#9 2,4-D

R.T.: 12.739 min
Delta R.T.: -0.034 min
Response: 233656
Conc: 0.58 ng/ml

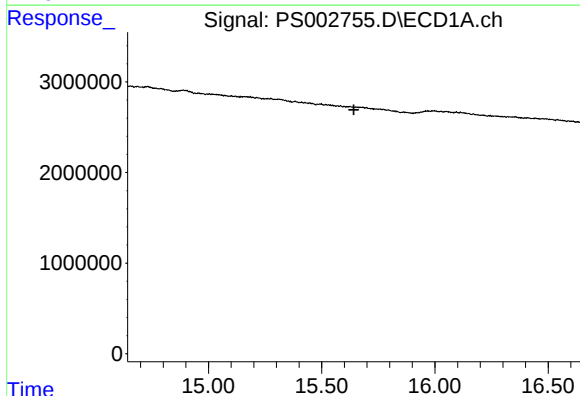


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.642 min
Response: 0
Conc: N.D.

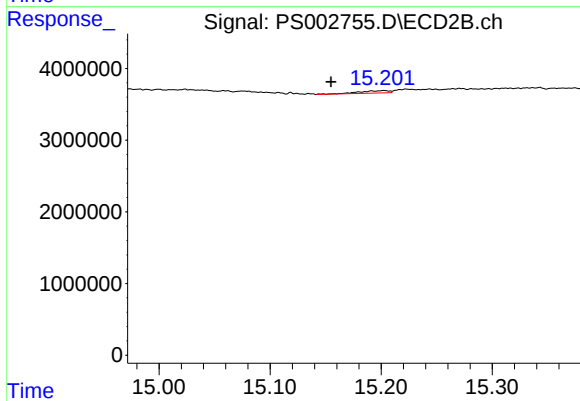

#13 2,4-DB


R.T.: 15.203 min
Delta R.T.: 0.048 min
Response: 630183
Conc: 3.35 ng/ml

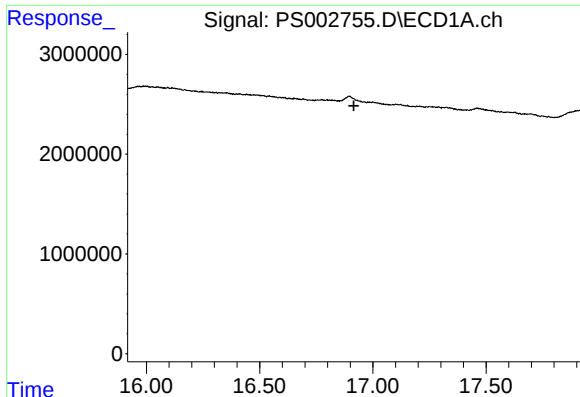

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.916 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

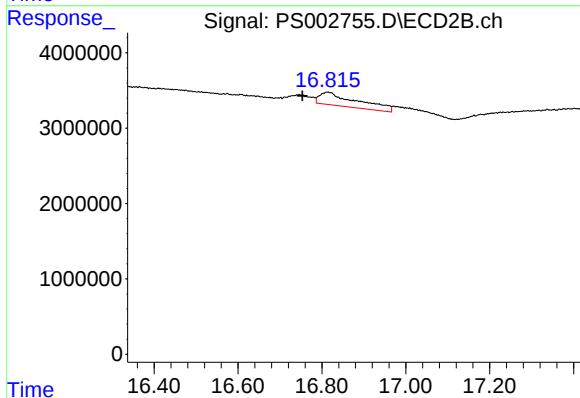


#15 Picloram

R.T.: 16.814 min
Delta R.T.: 0.061 min
Response: 10936916
Conc: 4.08 ng/ml

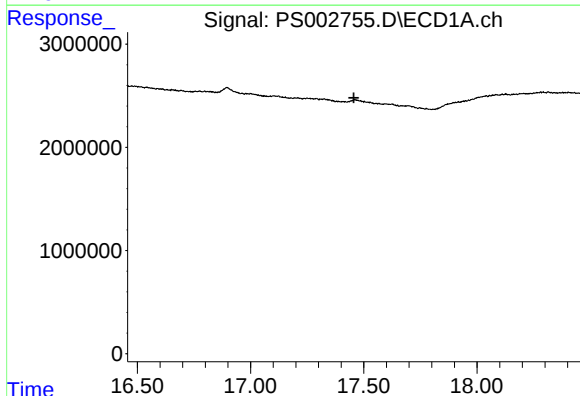

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.456 min
Response: 0
Conc: N.D.

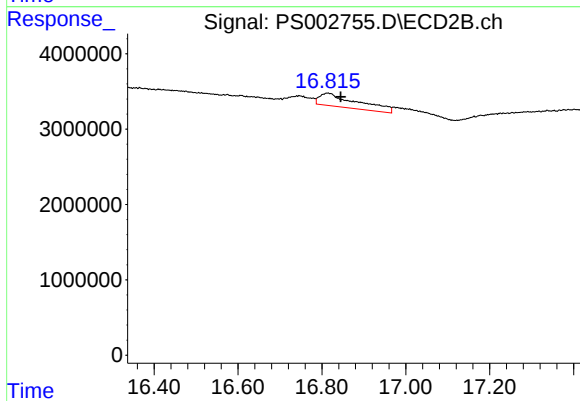

#16 DCPA

R.T.: 16.814 min
Delta R.T.: -0.031 min
Response: 10936916
Conc: 4.22 ng/ml