

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010819\
 Data File : PS002758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2019 16:29
 Operator : EI\SJ
 Sample : PB116224BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116224BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 23:52:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010419.M
 Quant Title : 8080.M
 QLast Update : Sat Jan 05 06:20:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.420	10.919	139.2E6	164.5E6	445.092	432.690
Target Compounds							
1) T	Dalapon	2.886	0.000	3061591	0	9.097	N.D. #
6) T	MCP	12.098	0.000	54068579	0	54.699	N.D. #
10) T	Pentachlo...	13.653	0.000	3539675	0	0.673	N.D. #
11) T	2,4,5-TP ...	0.000	13.876	0 10811200	N.D.	5.194	#
12) T	2,4,5-T	0.000	14.541	0 28202568	N.D.	13.904	#
15) T	Picloram	0.000	16.691	0 7536872	N.D.	2.815	#
16) T	DCPA	17.427	0.000	10297451	0	4.348	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010819\
Data File : PS002758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2019 16:29
Operator : EI\SJ
Sample : PB116224BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB116224BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 23:52:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010419.M
Quant Title : 8080.M
QLast Update : Sat Jan 05 06:20:43 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

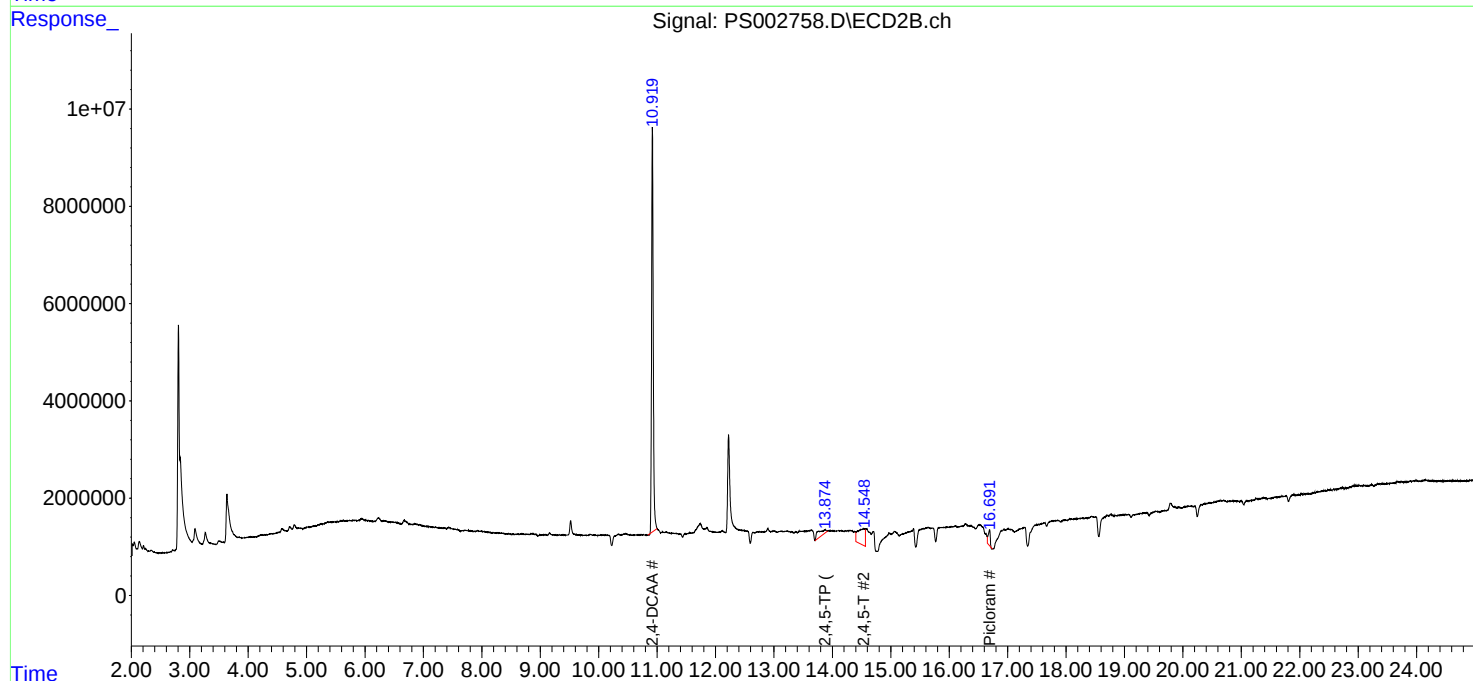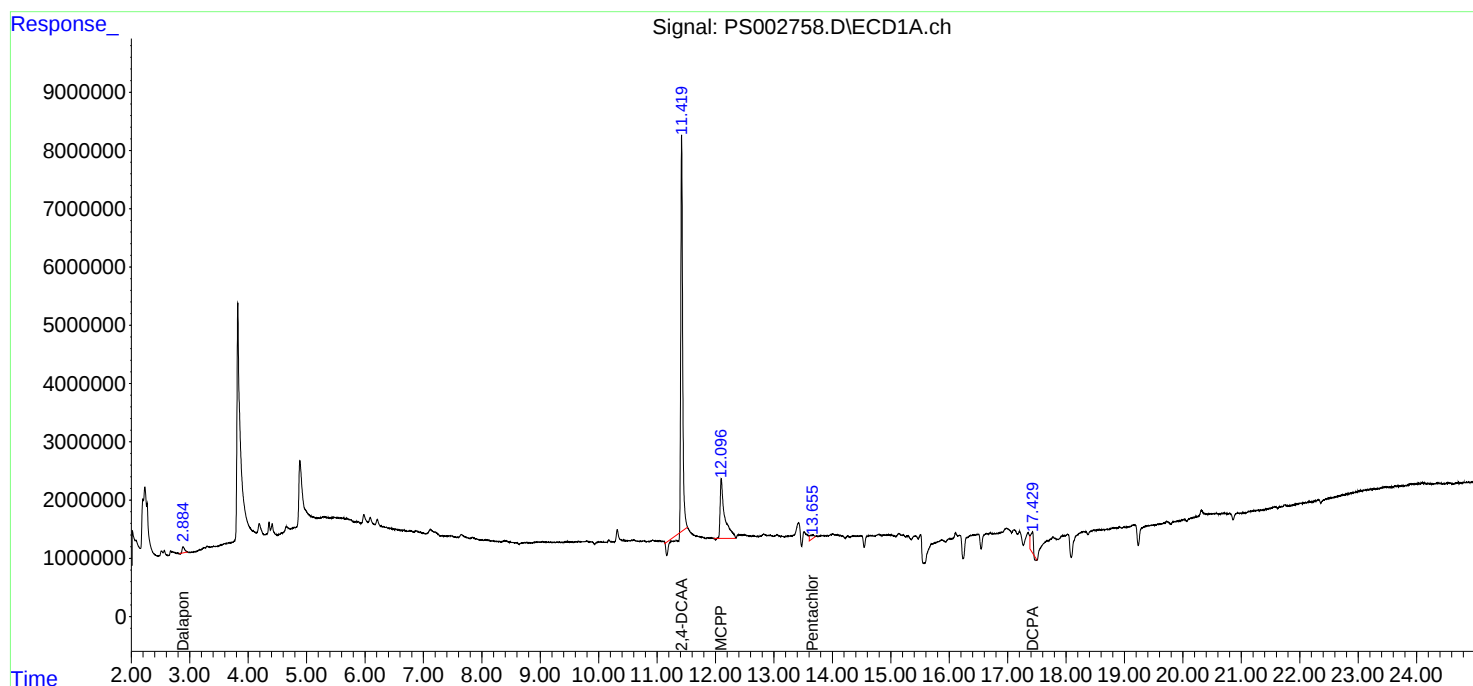


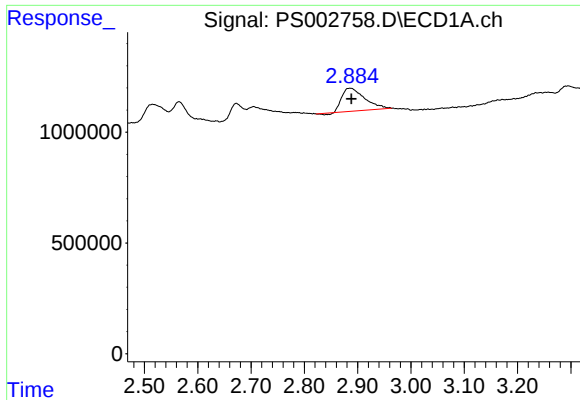

#1 Dalapon


R.T.: 2.886 min
Delta R.T.: -0.002 min
Response: 3061591
Conc: 9.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116224BL

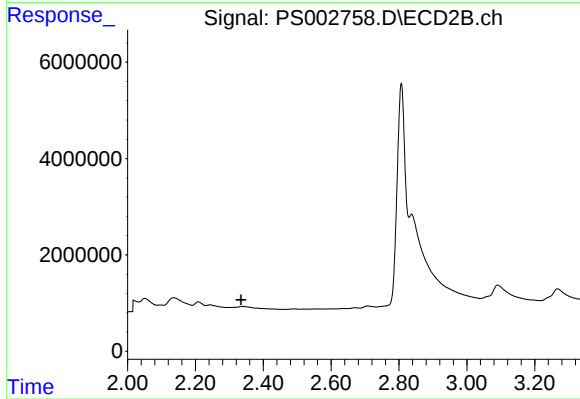


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.335 min
Response: 0
Conc: N.D.

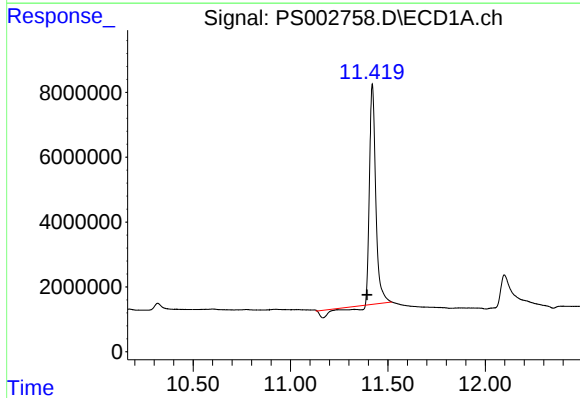


#4 2,4-DCAA

R.T.: 11.420 min
Delta R.T.: 0.026 min
Response: 139199200
Conc: 445.09 ng/ml

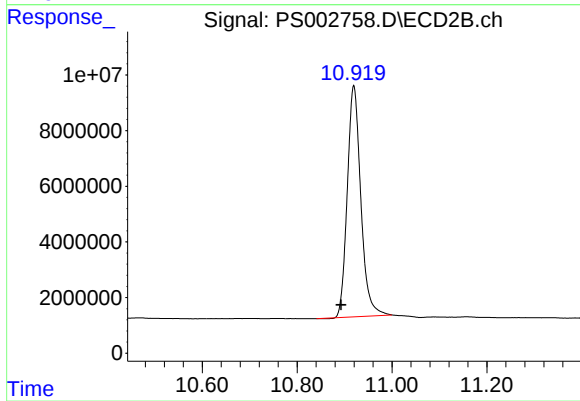

#4 2,4-DCAA


R.T.: 10.919 min
Delta R.T.: 0.027 min
Response: 164546207
Conc: 432.69 ng/ml

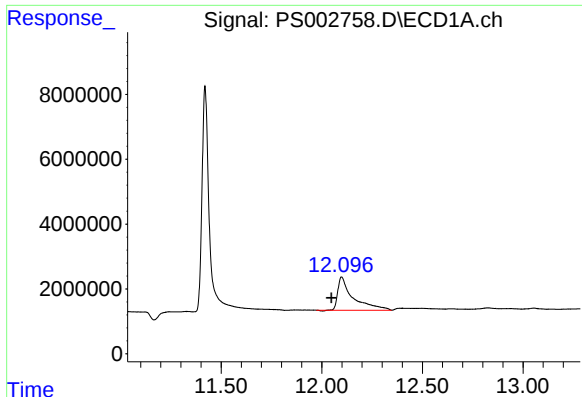

#6 MCP


R.T.: 12.098 min
Delta R.T.: 0.050 min
Response: 54068579
Conc: 54.70 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB116224BL

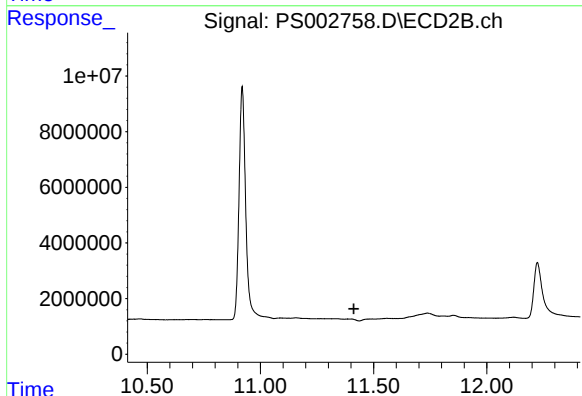


#6 MCP

R.T.: 0.000 min
Exp R.T.: 11.413 min
Response: 0
Conc: N.D.

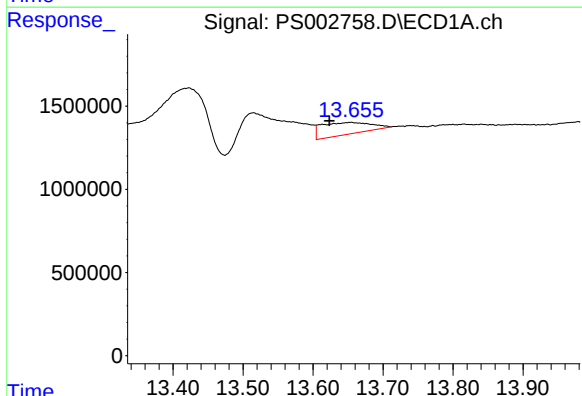


#10 Pentachlorophenol

R.T.: 13.653 min
Delta R.T.: 0.030 min
Response: 3539675
Conc: 0.67 ng/ml

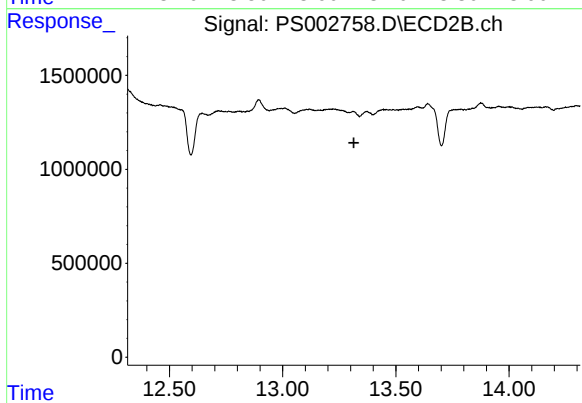

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.315 min
Response: 0
Conc: N.D.

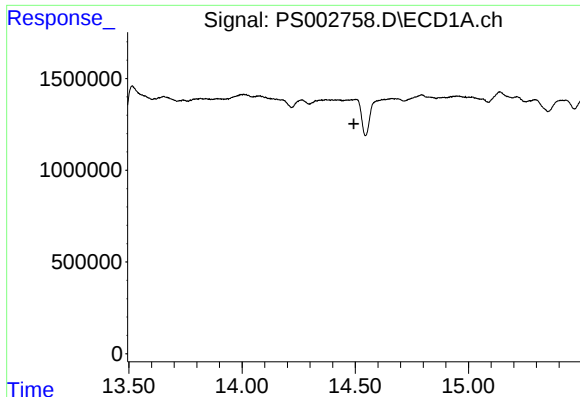

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116224BL

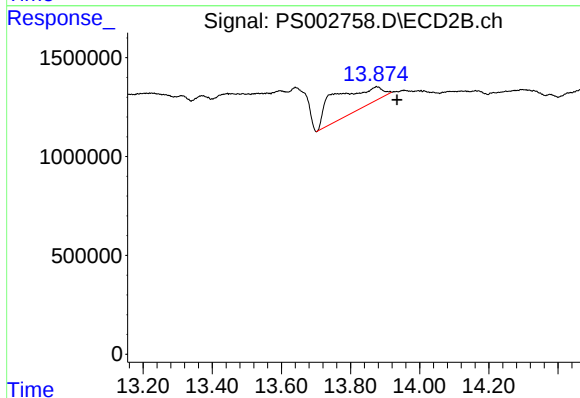


#11 2,4,5-TP (SILVEX)

R.T.: 13.876 min
Delta R.T.: -0.060 min
Response: 10811200
Conc: 5.19 ng/ml

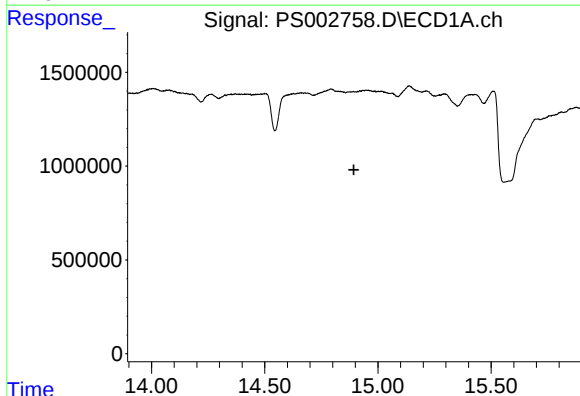


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.894 min
Response: 0
Conc: N.D.

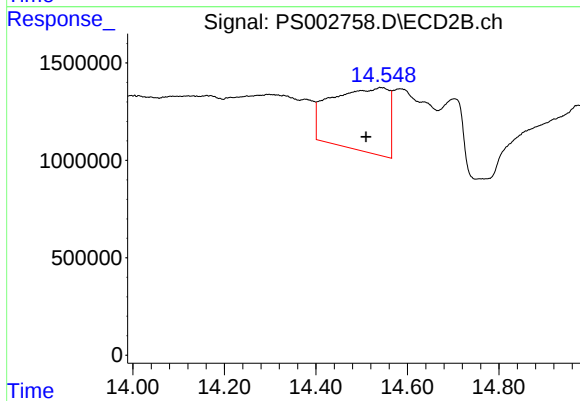

#12 2,4,5-T


R.T.: 14.541 min
Delta R.T.: 0.032 min
Response: 28202568
Conc: 13.90 ng/ml

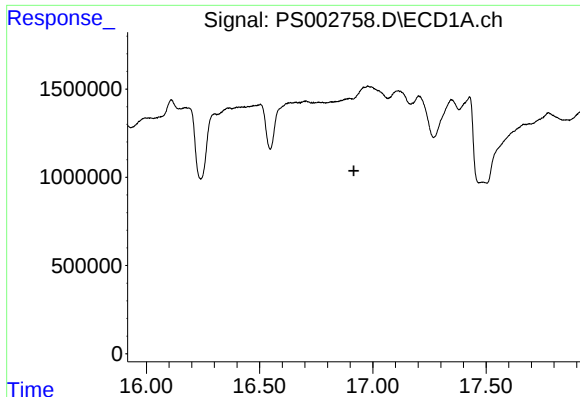

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.916 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116224BL

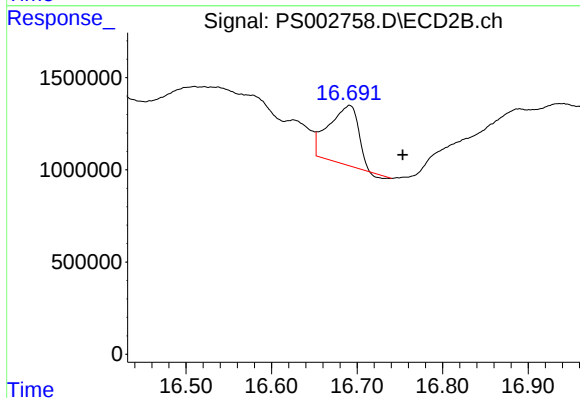


#15 Picloram

R.T.: 16.691 min
Delta R.T.: -0.063 min
Response: 7536872
Conc: 2.81 ng/ml

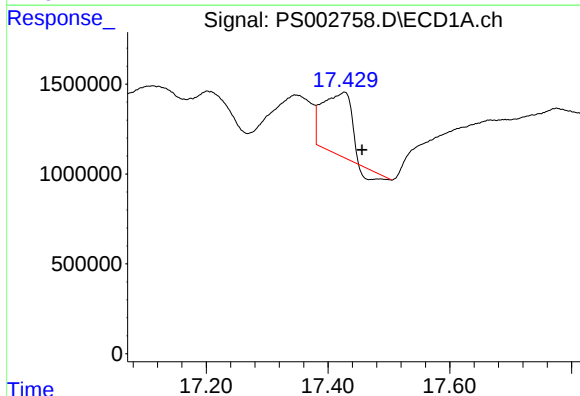

#16 DCPA

R.T.: 17.427 min
Delta R.T.: -0.029 min
Response: 10297451
Conc: 4.35 ng/ml

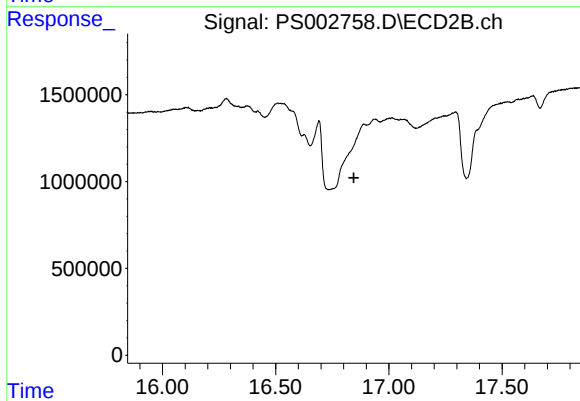

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 16.845 min
Response: 0
Conc: N.D.