

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010819\
 Data File : PS002760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2019 17:31
 Operator : EI\SJ
 Sample : K1074-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 W12-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 23:53:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010419.M
 Quant Title : 8080.M
 QLast Update : Sat Jan 05 06:20:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.407	10.907	89419838	93325914	285.922	245.409
Target Compounds							
3) T	4-Nitroph...	0.000	10.040	0	16620020	N.D.	95.674 #
5) T	DICAMBA	11.714	11.188	13319959	10475529	9.164	7.258
6) T	MCP	12.076	0.000	52101636	0	52.709	N.D. #
8) T	DICHLORPROP	0.000	12.310	0	2304014	N.D.	6.461 #
9) T	2,4-D	0.000	12.705	0	11393928	N.D.	28.471 #
10) T	Pentachlo...	13.638	13.326	13142055	3838558	2.500	0.690 #
11) T	2,4,5-TP ...	0.000	13.939	0	2533445	N.D.	1.217 #
12) T	2,4,5-T	0.000	14.482	0	31351811	N.D.	15.456 #
13) T	2,4-DB	0.000	15.164	0	6731019	N.D.	35.741 #
14) T	DINOSEB	0.000	15.617	0	9222815	N.D.	8.844 #
15) T	Picloram	16.931	0.000	8220749	0	6.976	N.D. #
16) T	DCPA	17.417	16.870	10337835	13622878	4.365	5.260



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010819\
Data File : PS002760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2019 17:31
Operator : EI\SJ
Sample : K1074-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
W12-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 23:53:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010419.M
Quant Title : 8080.M
QLast Update : Sat Jan 05 06:20:43 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

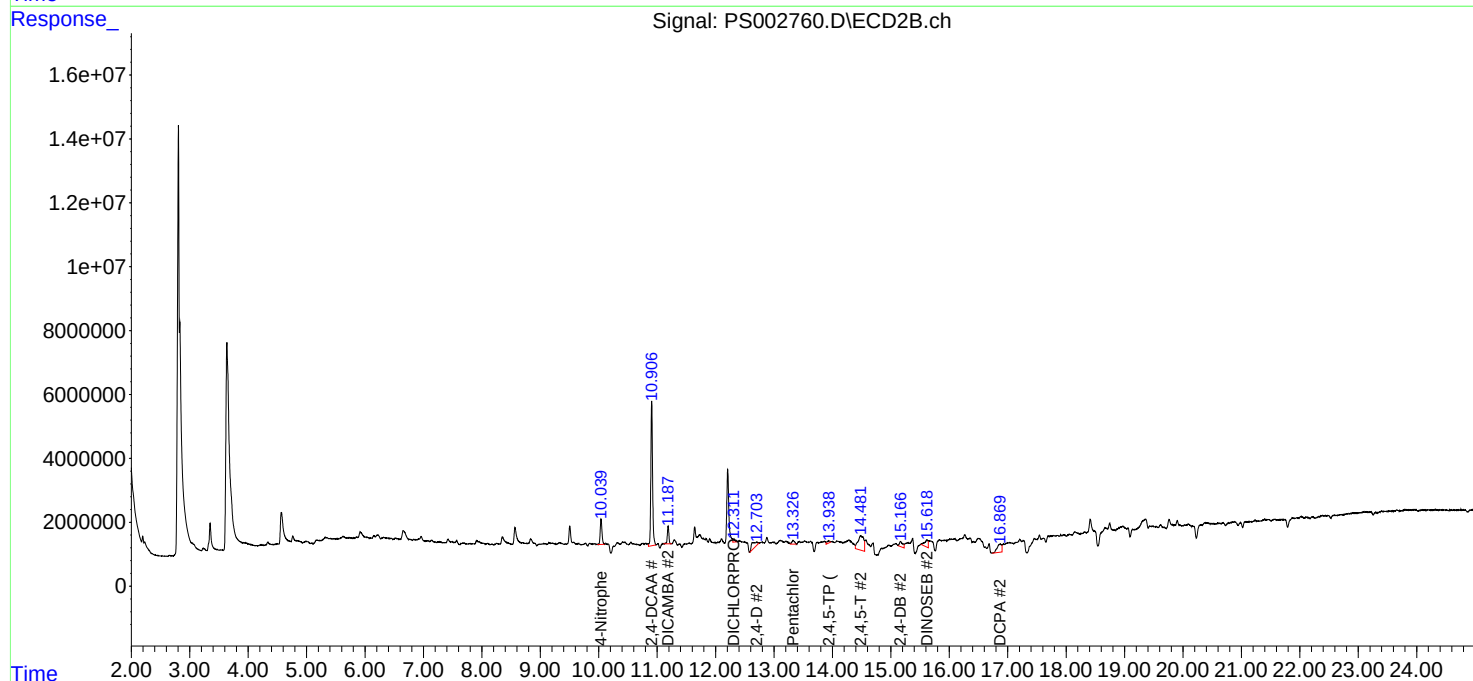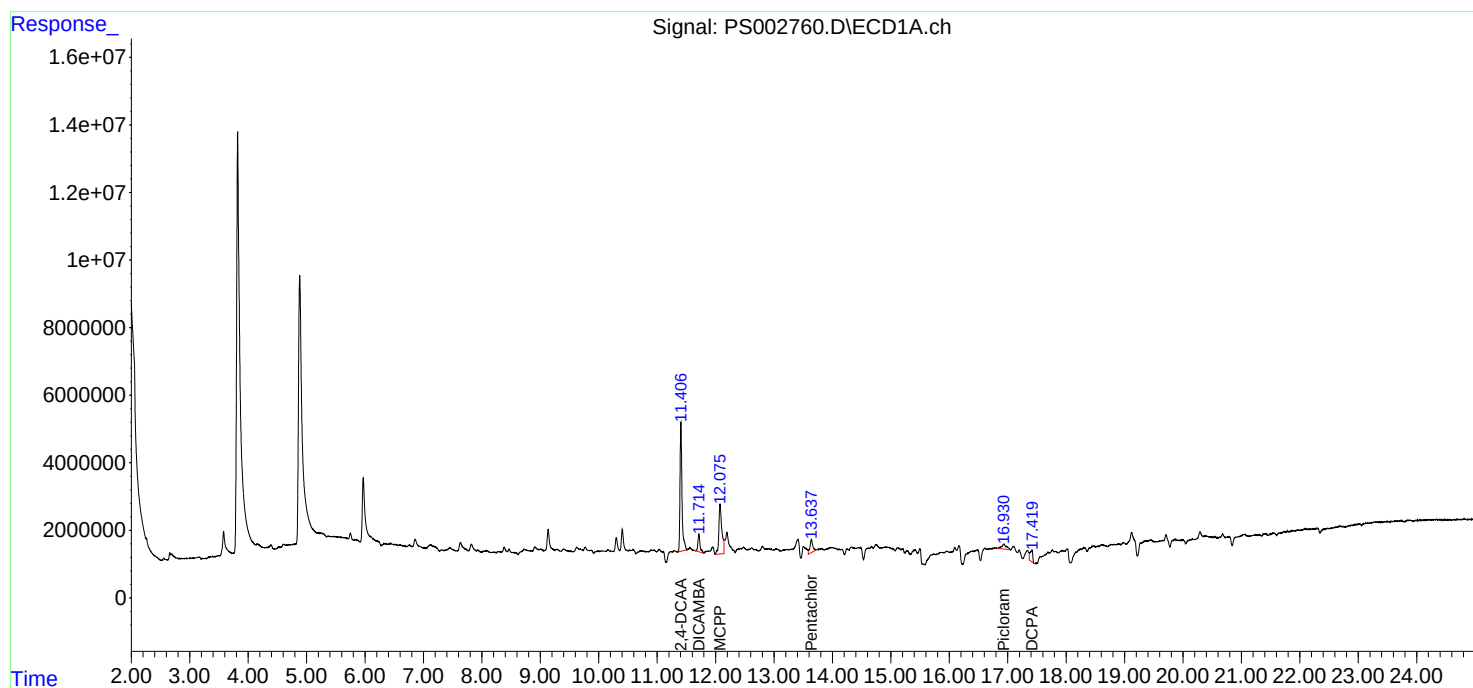


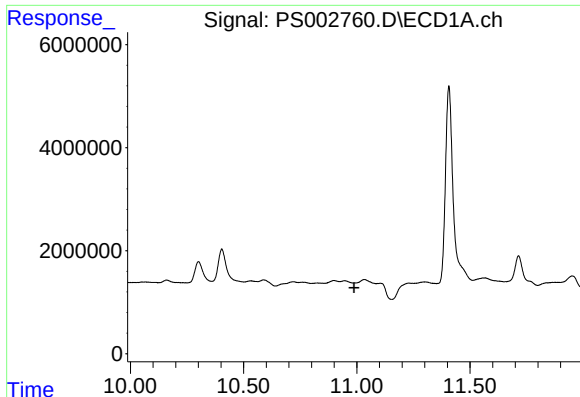

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.987 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
W12-1

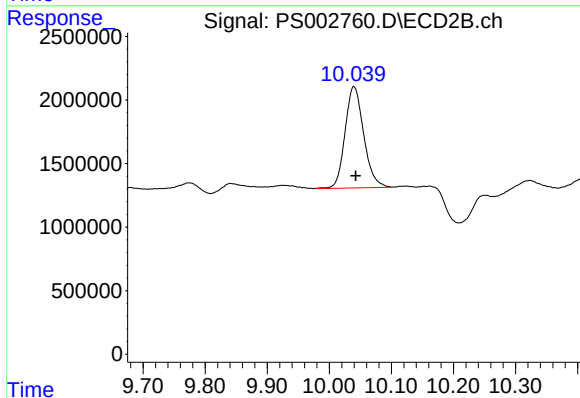


#3 4-Nitrophenol

R.T.: 10.040 min
Delta R.T.: -0.003 min
Response: 16620020
Conc: 95.67 ng/ml

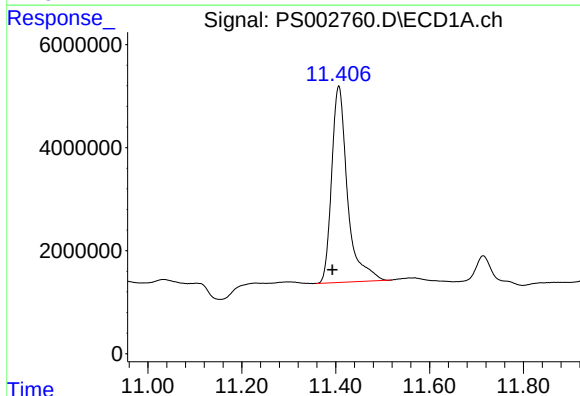


#4 2,4-DCAA

R.T.: 11.407 min
Delta R.T.: 0.013 min
Response: 89419838
Conc: 285.92 ng/ml

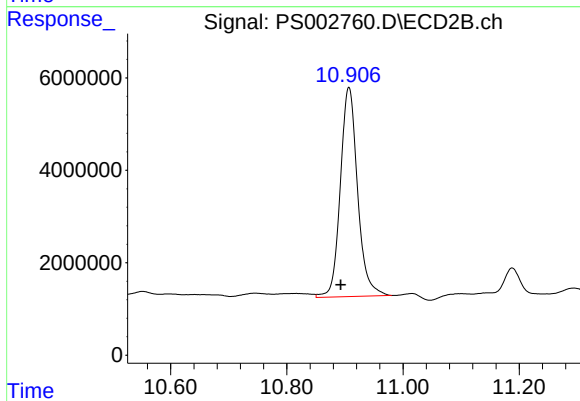

#4 2,4-DCAA


R.T.: 10.907 min
Delta R.T.: 0.014 min
Response: 93325914
Conc: 245.41 ng/ml

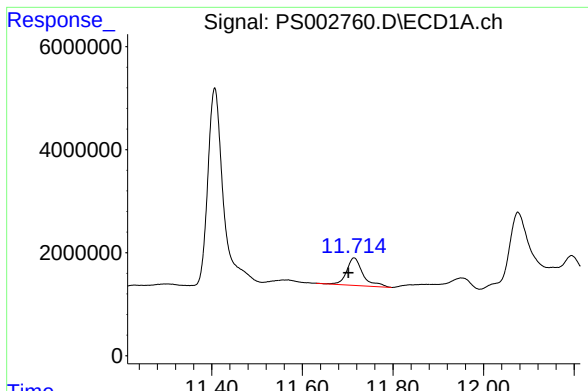

#5 DICAMBA


R.T.: 11.714 min
Delta R.T.: 0.013 min
Response: 13319959
Conc: 9.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
W12-1

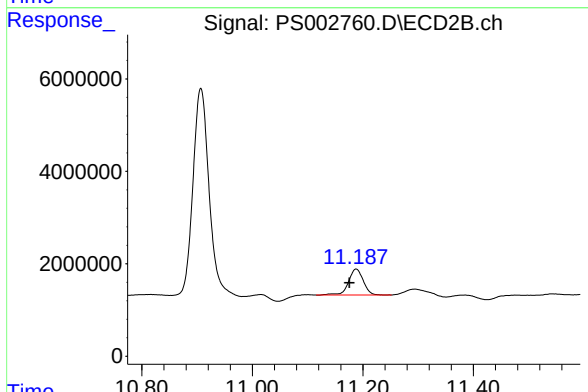


#5 DICAMBA

R.T.: 11.188 min
Delta R.T.: 0.012 min
Response: 10475529
Conc: 7.26 ng/ml

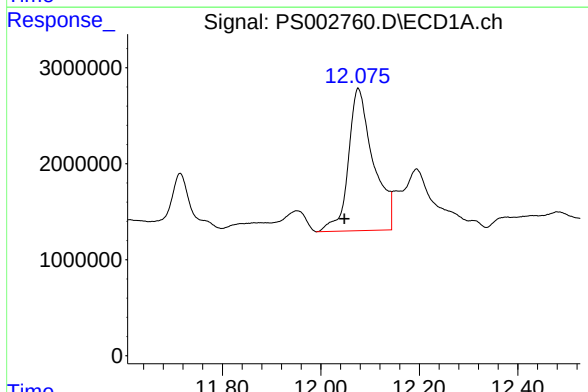


#6 MCPP

R.T.: 12.076 min
Delta R.T.: 0.028 min
Response: 52101636
Conc: 52.71 ug/ml

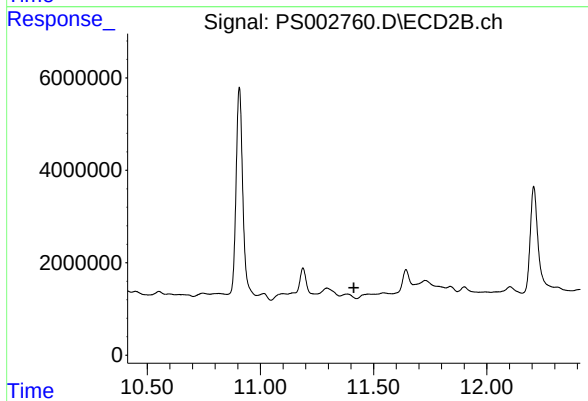

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.413 min
Response: 0
Conc: N.D.

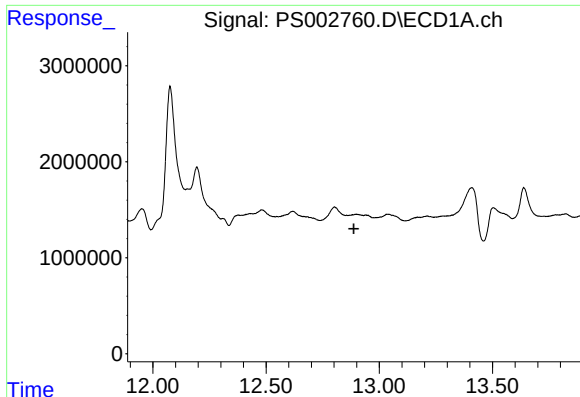

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.888 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
W12-1

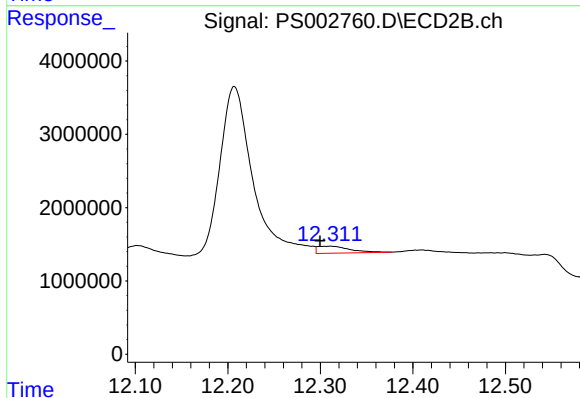


#8 DICHLORPROP

R.T.: 12.310 min
Delta R.T.: 0.010 min
Response: 2304014
Conc: 6.46 ng/ml

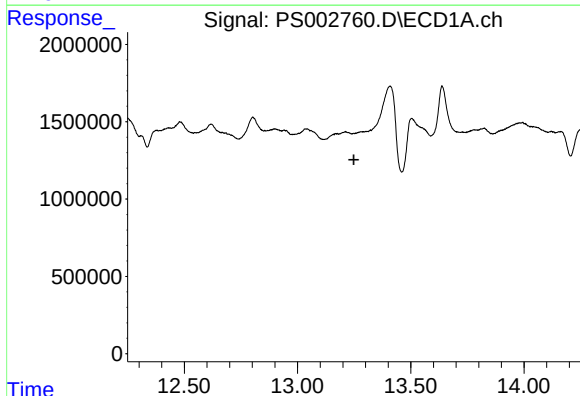


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.248 min
Response: 0
Conc: N.D.

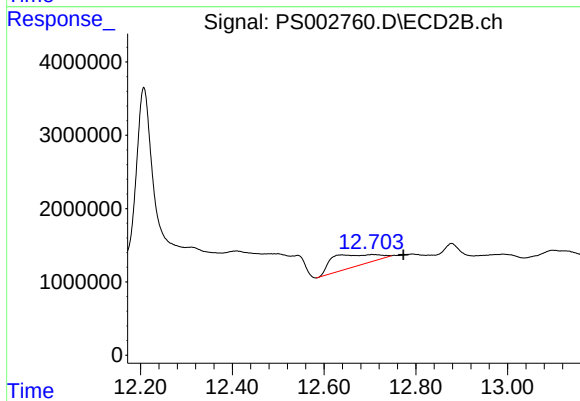

#9 2,4-D


R.T.: 12.705 min
Delta R.T.: -0.068 min
Response: 11393928
Conc: 28.47 ng/ml

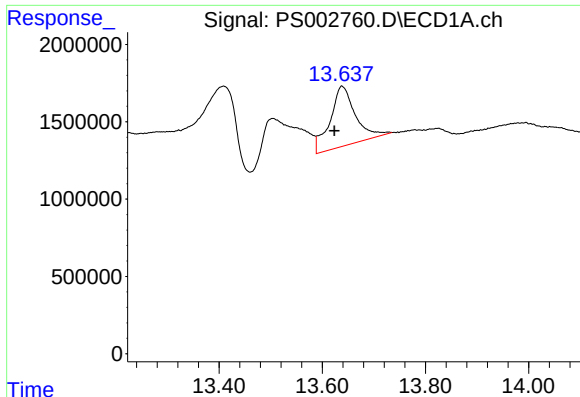

#10 Pentachlorophenol


R.T.: 13.638 min
Delta R.T.: 0.015 min
Response: 13142055
Conc: 2.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
W12-1

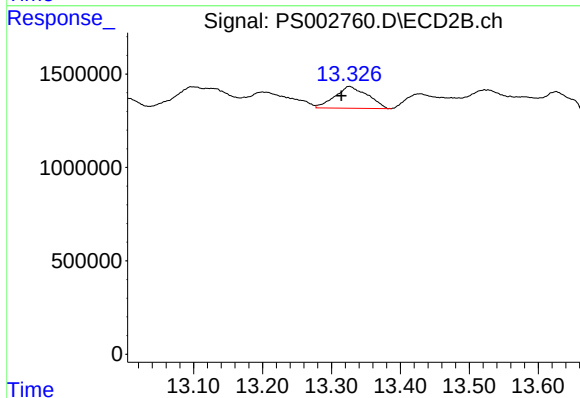


#10 Pentachlorophenol

R.T.: 13.326 min
Delta R.T.: 0.011 min
Response: 3838558
Conc: 0.69 ng/ml

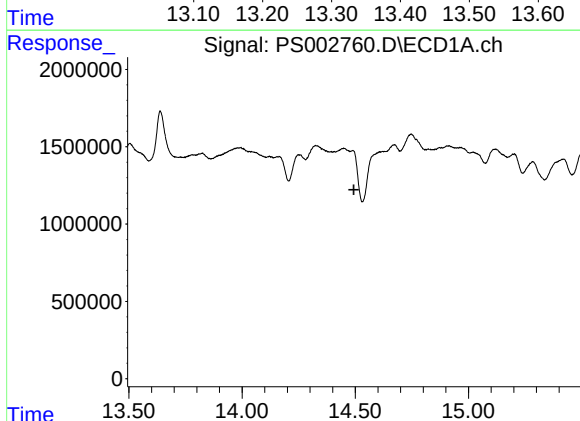


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.494 min
Response: 0
Conc: N.D.

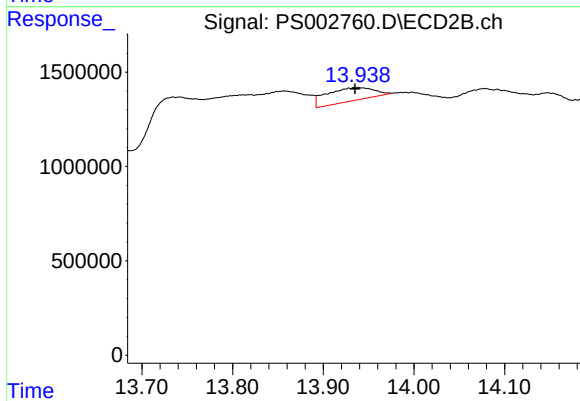

#11 2,4,5-TP (SILVEX)


R.T.: 13.939 min
Delta R.T.: 0.003 min
Response: 2533445
Conc: 1.22 ng/ml

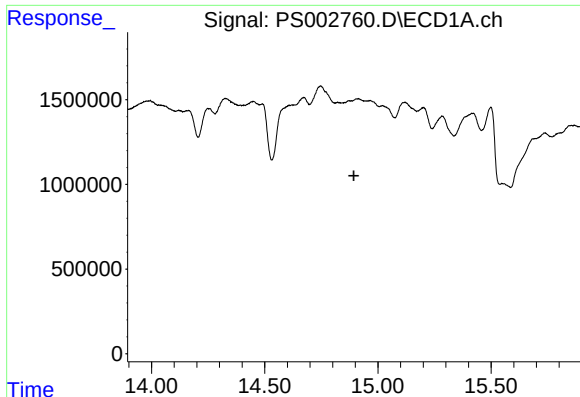

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.894 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
W12-1

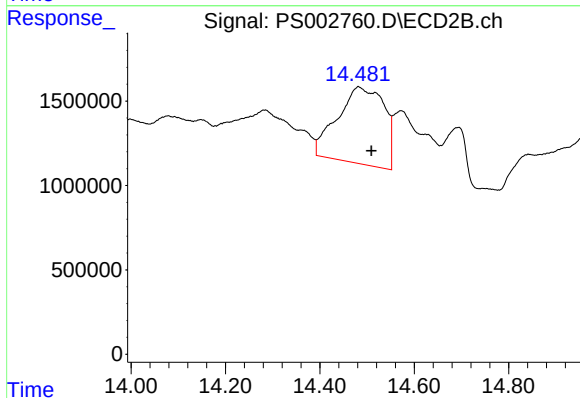


#12 2,4,5-T

R.T.: 14.482 min
Delta R.T.: -0.028 min
Response: 31351811
Conc: 15.46 ng/ml

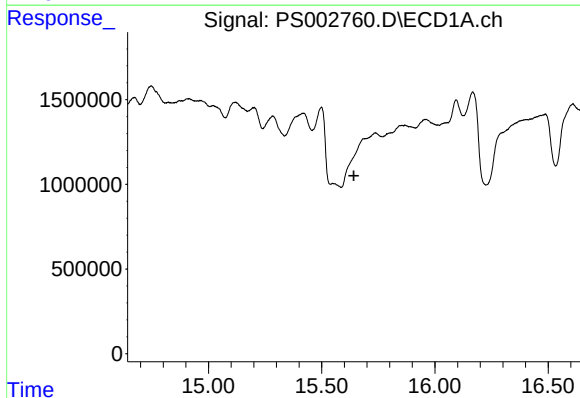


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.642 min
Response: 0
Conc: N.D.

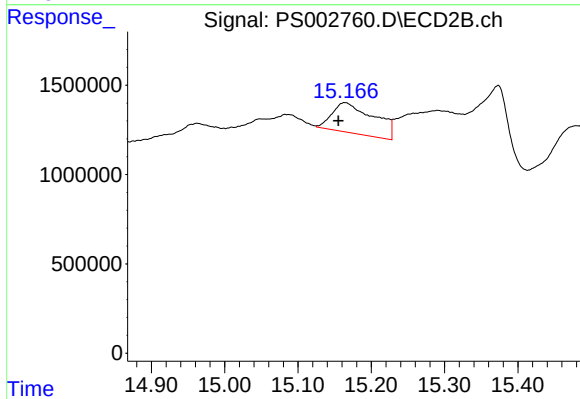

#13 2,4-DB


R.T.: 15.164 min
Delta R.T.: 0.009 min
Response: 6731019
Conc: 35.74 ng/ml

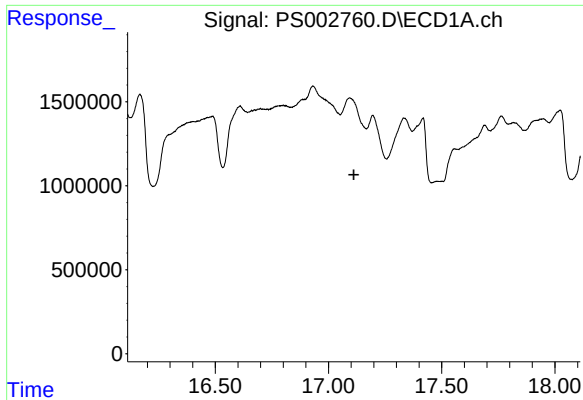

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
W12-1

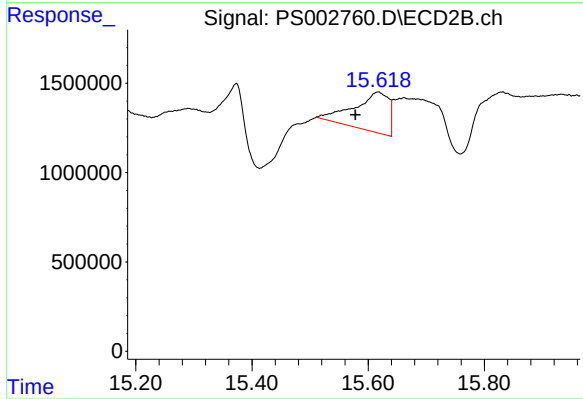


#14 DINOSEB

R.T.: 15.617 min
Delta R.T.: 0.039 min
Response: 9222815
Conc: 8.84 ng/ml

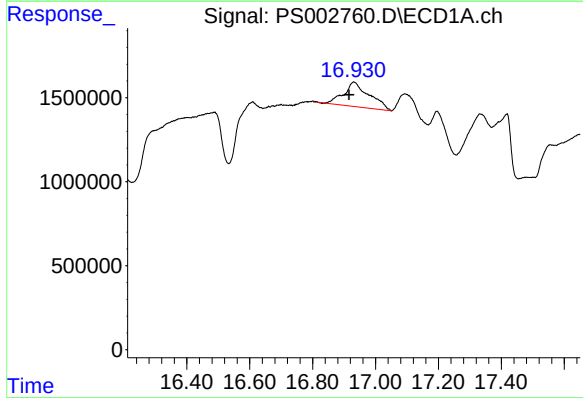


#15 Picloram

R.T.: 16.931 min
Delta R.T.: 0.015 min
Response: 8220749
Conc: 6.98 ng/ml

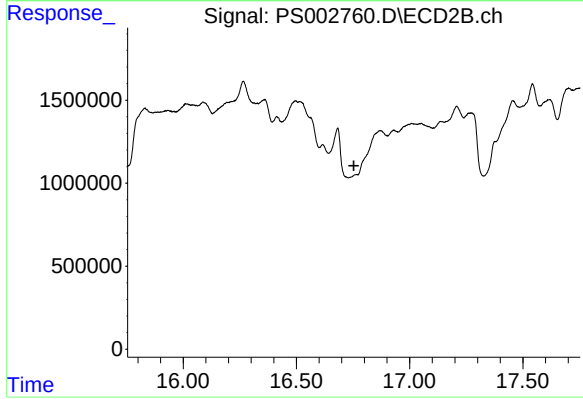

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.754 min
Response: 0
Conc: N.D.

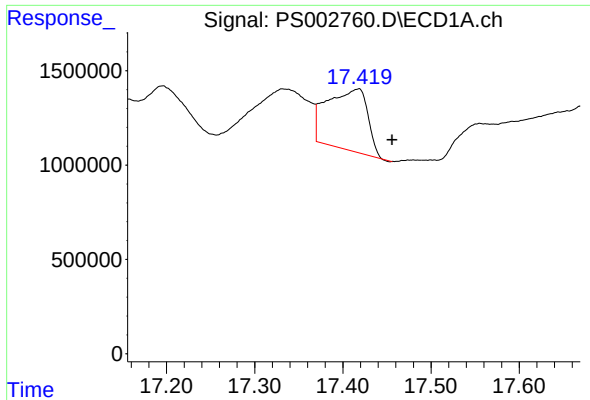

#16 DCPA

R.T.: 17.417 min
Delta R.T.: -0.039 min
Response: 10337835
Conc: 4.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
W12-1

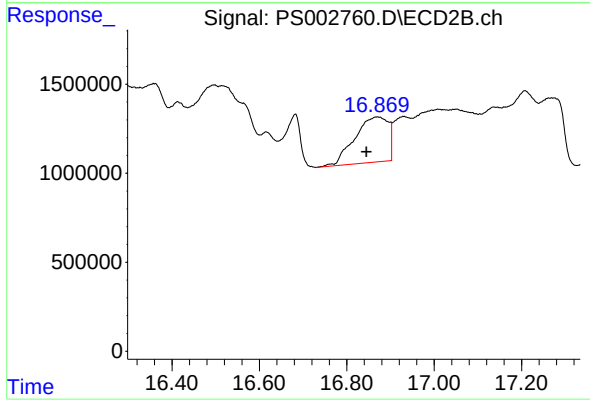

#16 DCPA

R.T.: 16.870 min
Delta R.T.: 0.024 min
Response: 13622878
Conc: 5.26 ng/ml