

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010819\
 Data File : PS002764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2019 19:36
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 23:55:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010419.M
 Quant Title : 8080.M
 QLast Update : Sat Jan 05 06:20:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.399	10.895	104.6E6	113.2E6	334.432	297.696
Target Compounds							
15) T	Picloram	0.000	16.730	0	1213992	N.D.	0.453 #
16) T	DCPA	0.000	16.914	0	2687444	N.D.	1.038 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010819\
Data File : PS002764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2019 19:36
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 23:55:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010419.M
Quant Title : 8080.M
QLast Update : Sat Jan 05 06:20:43 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

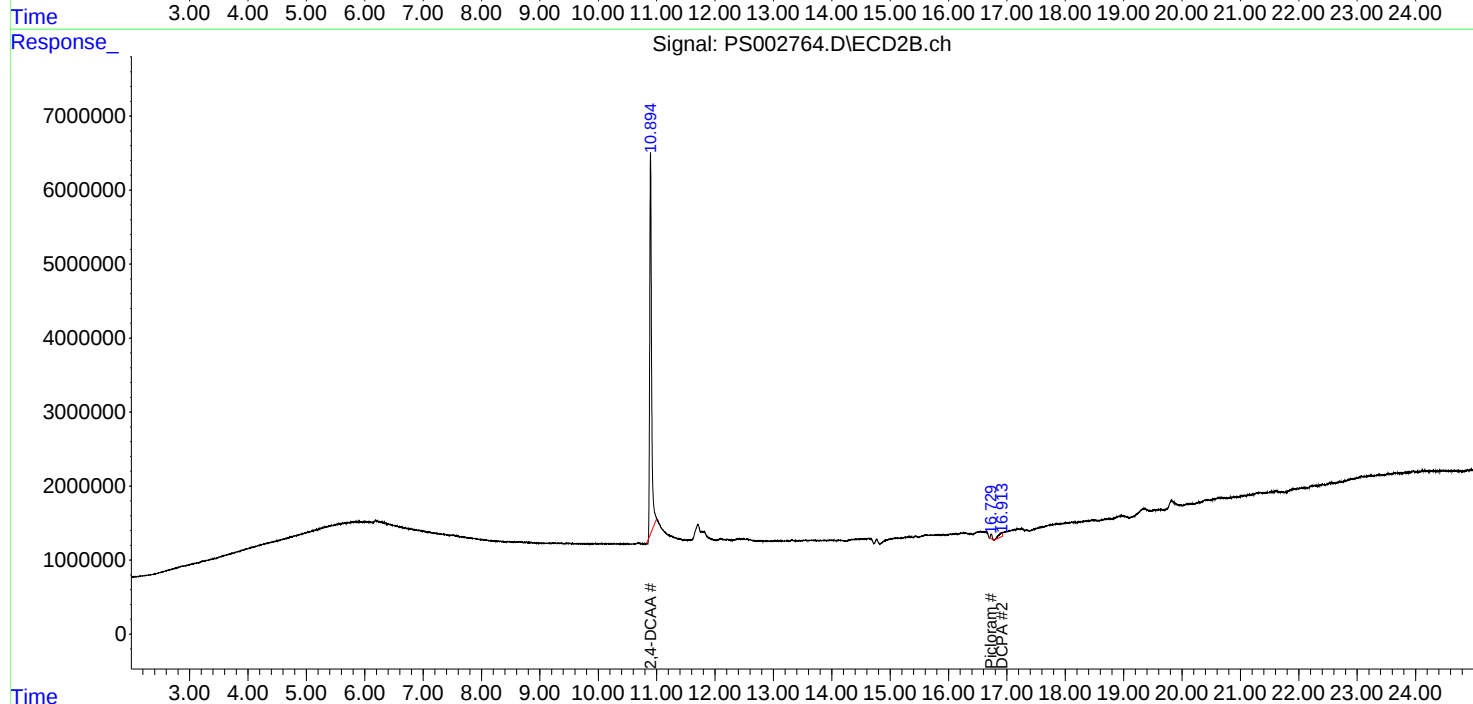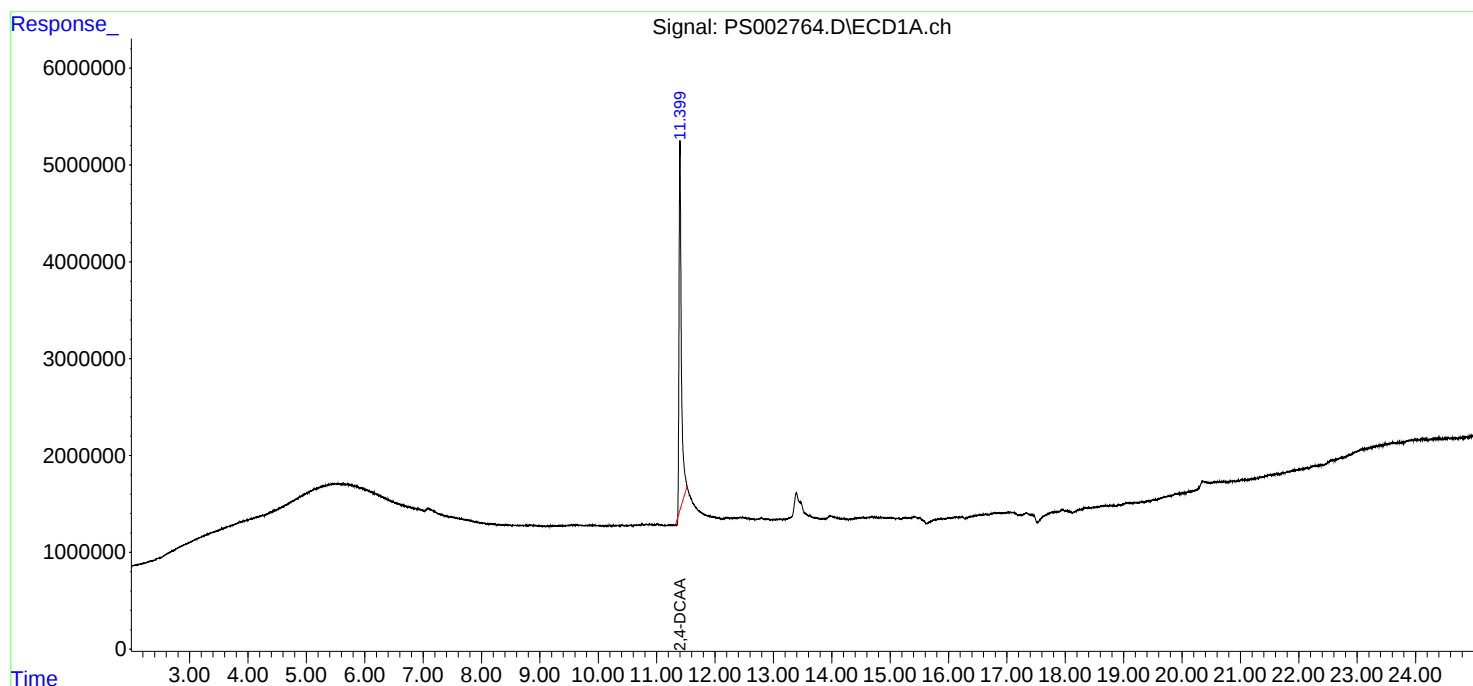


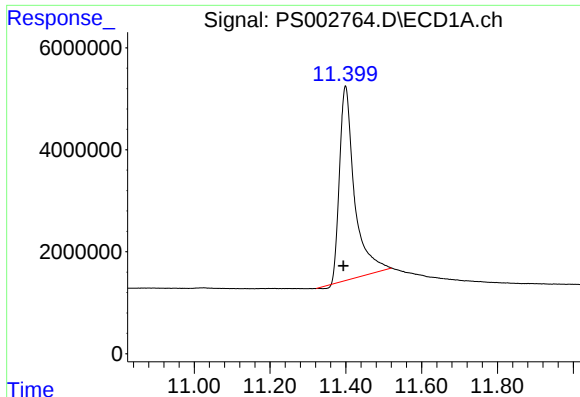

#4 2,4-DCAA


R.T.: 11.399 min
Delta R.T.: 0.006 min
Response: 104591093
Conc: 334.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

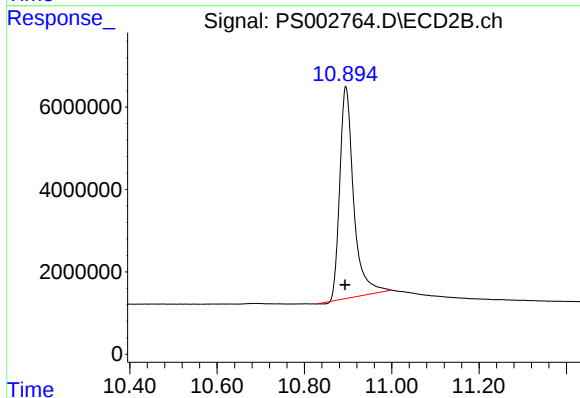


#4 2,4-DCAA

R.T.: 10.895 min
Delta R.T.: 0.002 min
Response: 113209961
Conc: 297.70 ng/ml

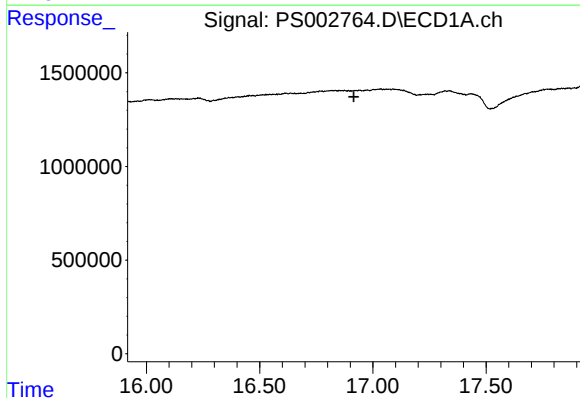


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.916 min
Response: 0
Conc: N.D.

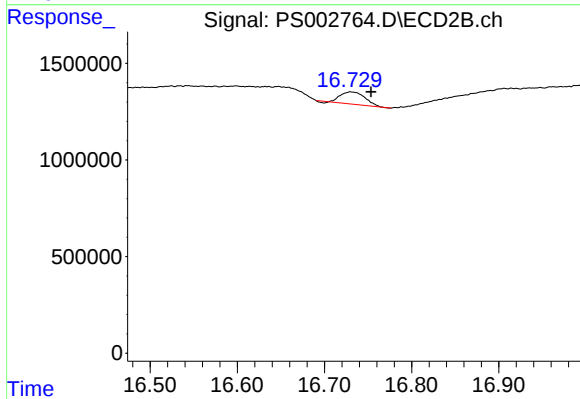

#15 Picloram


R.T.: 16.730 min
Delta R.T.: -0.024 min
Response: 1213992
Conc: 0.45 ng/ml

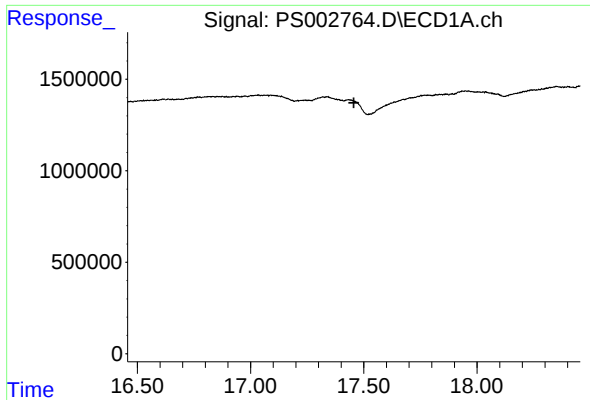

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

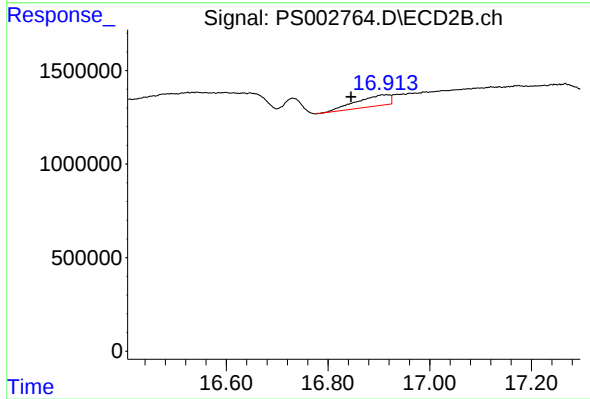

#16 DCPA

R.T.: 16.914 min
Delta R.T.: 0.069 min
Response: 2687444
Conc: 1.04 ng/ml