

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010820\
 Data File : PS008339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2020 16:55
 Operator : DD\AJ
 Sample : PB125953TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 03:07:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.277	5.972	776.1E6	391.4E6	439.566	413.115
Target Compounds							
1) T	Dalapon	2.505	2.190	118.4E6	38191757	46.194	30.126 #
2) T	3,5-DICHL...	0.000	5.157	0	119.8E6	N.D.	85.715
3) T	4-Nitroph...	6.147	5.633	14834067	8884661	15.231	14.964
8) T	DICHLORPROP	0.000	6.792	0	13046982	N.D.	13.504
10) T	Pentachlo...	7.762	0.000	21792636	0	<MDL	N.D. #
12) T	2,4,5-T	8.477	8.302	250.3E6	12367504	27.132	2.339 #
13) T	2,4-DB	9.040	0.000	13065658	0	9.425	N.D. #
14) T	DINOSEB	10.219	9.126	34425409	74249575	4.798	19.655 #
15) T	Picloram	10.044	0.000	78228897	0	6.267	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010820\
Data File : PS008339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2020 16:55
Operator : DD\AJ
Sample : PB125953TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 03:07:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

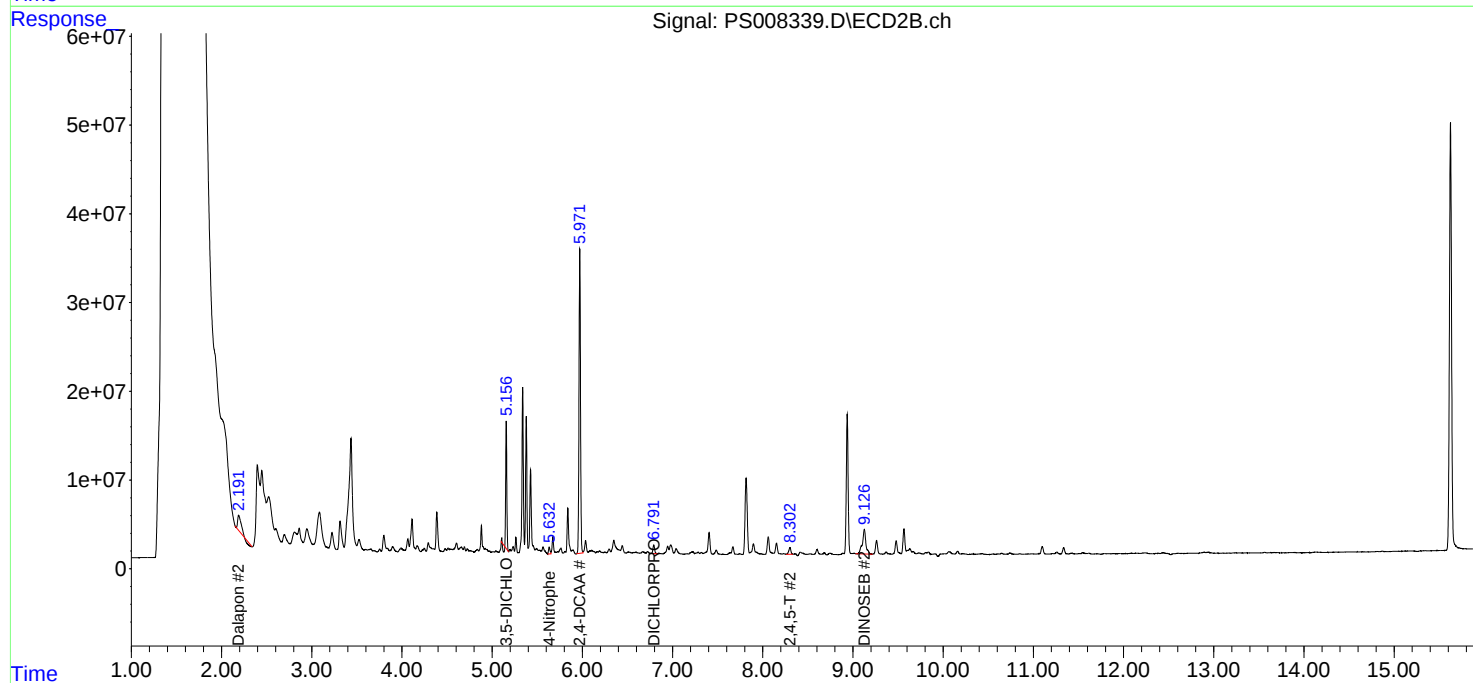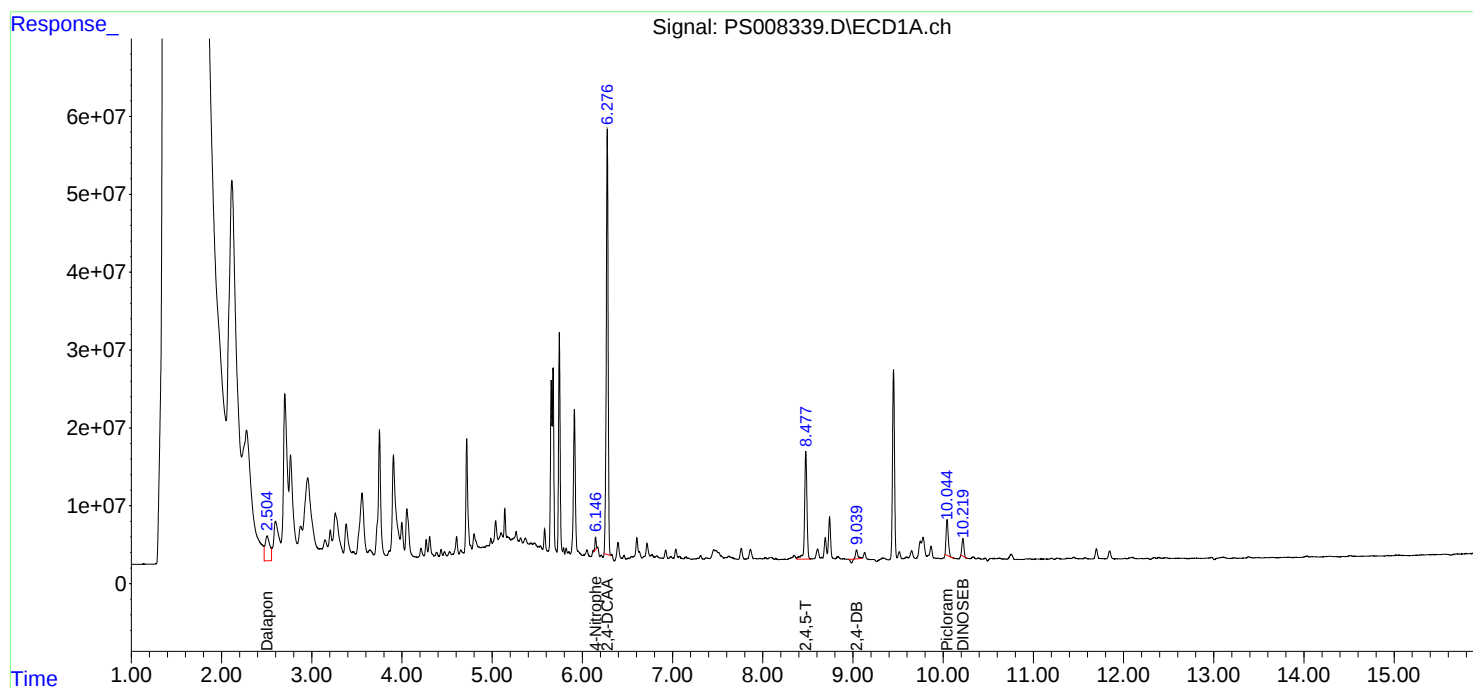


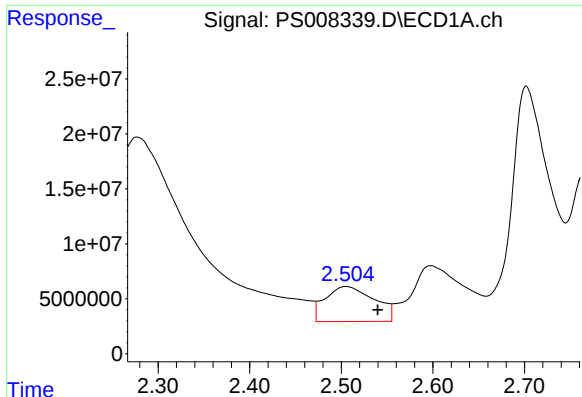

#1 Dalapon


R.T.: 2.505 min
Delta R.T.: -0.035 min
Response: 118434450
Conc: 46.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

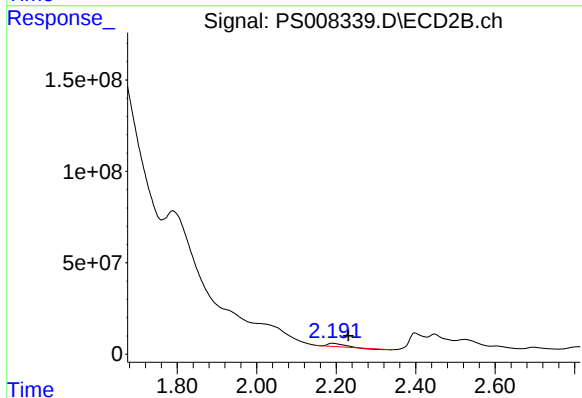


#1 Dalapon

R.T.: 2.190 min
Delta R.T.: -0.041 min
Response: 38191757
Conc: 30.13 ng/ml

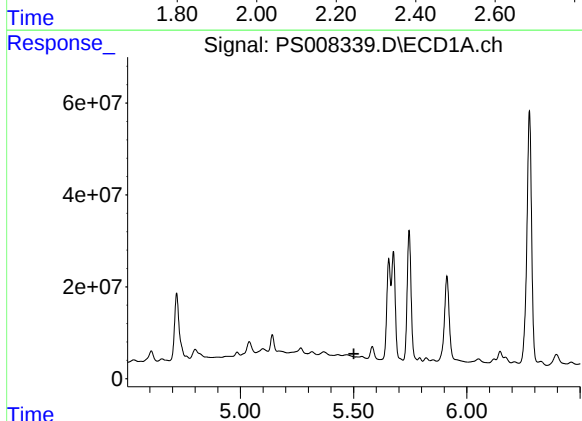


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

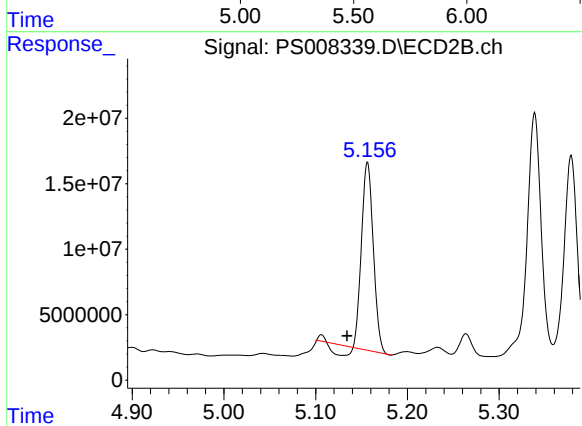

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.157 min
Delta R.T.: 0.022 min
Response: 119758507
Conc: 85.71 ng/ml

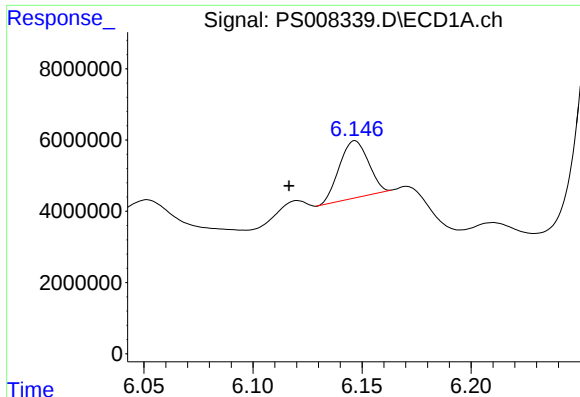

#3 4-Nitrophenol


R.T.: 6.147 min
Delta R.T.: 0.030 min
Response: 14834067
Conc: 15.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

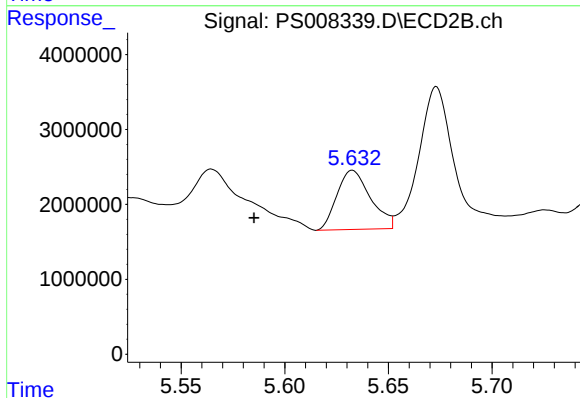


#3 4-Nitrophenol

R.T.: 5.633 min
Delta R.T.: 0.048 min
Response: 8884661
Conc: 14.96 ng/ml

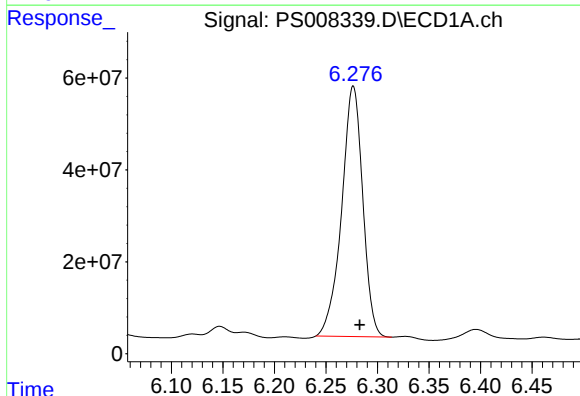


#4 2,4-DCAA

R.T.: 6.277 min
Delta R.T.: -0.006 min
Response: 776143887
Conc: 439.57 ng/ml

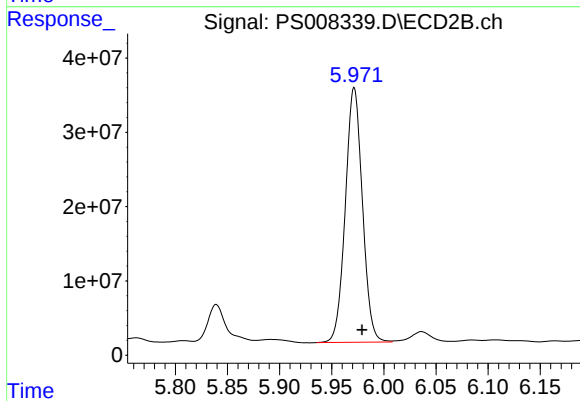

#4 2,4-DCAA


R.T.: 5.972 min
Delta R.T.: -0.008 min
Response: 391411316
Conc: 413.12 ng/ml

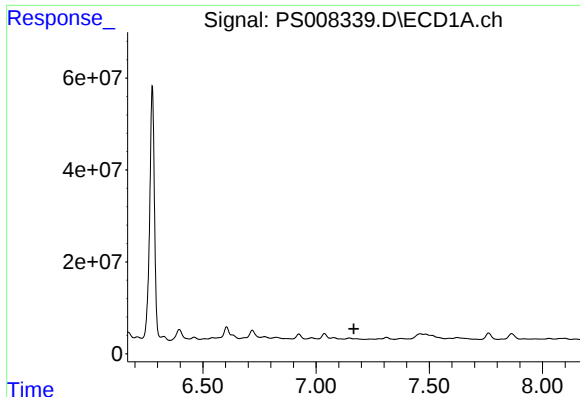

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

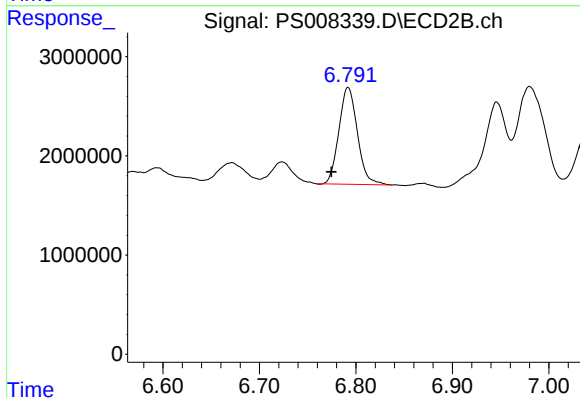


#8 DICHLORPROP

R.T.: 6.792 min
Delta R.T.: 0.017 min
Response: 13046982
Conc: 13.50 ng/ml

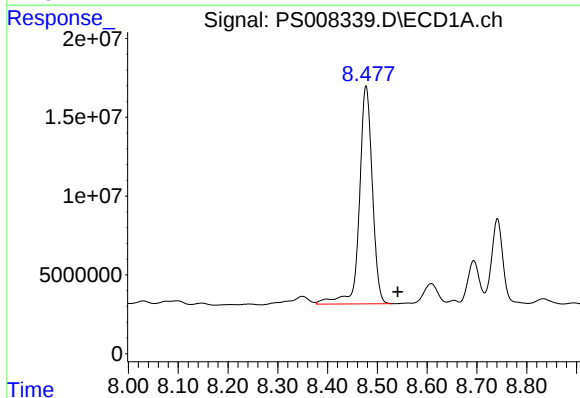


#12 2,4,5-T

R.T.: 8.477 min
Delta R.T.: -0.064 min
Response: 250337879
Conc: 27.13 ng/ml

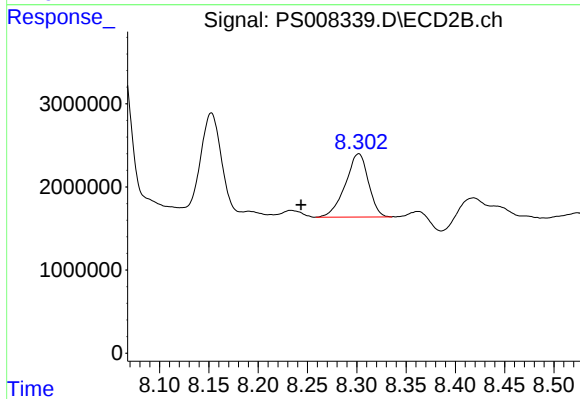

#12 2,4,5-T


R.T.: 8.302 min
Delta R.T.: 0.058 min
Response: 12367504
Conc: 2.34 ng/ml

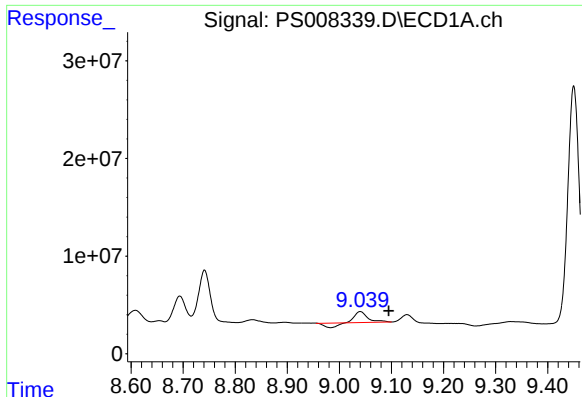

#13 2,4-DB


R.T.: 9.040 min
Delta R.T.: -0.055 min
Response: 13065658
Conc: 9.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

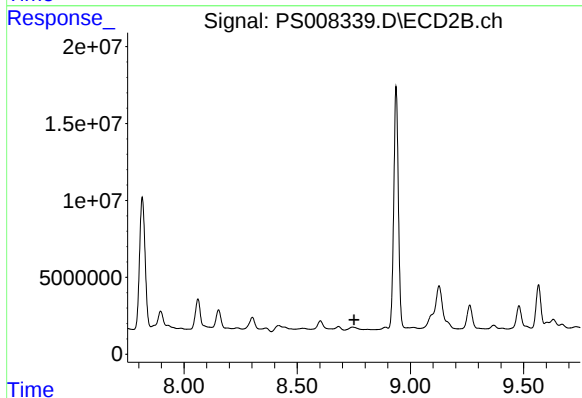


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

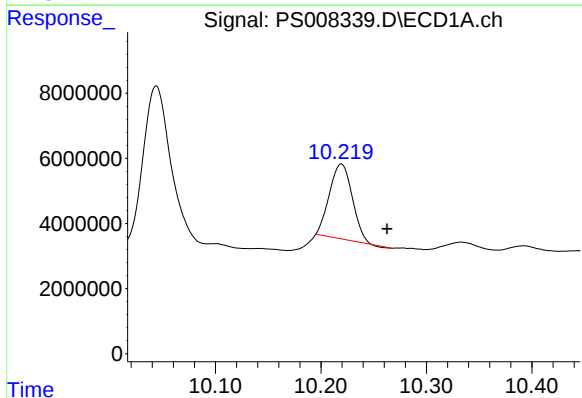


#14 DINOSEB

R.T.: 10.219 min
Delta R.T.: -0.043 min
Response: 34425409
Conc: 4.80 ng/ml

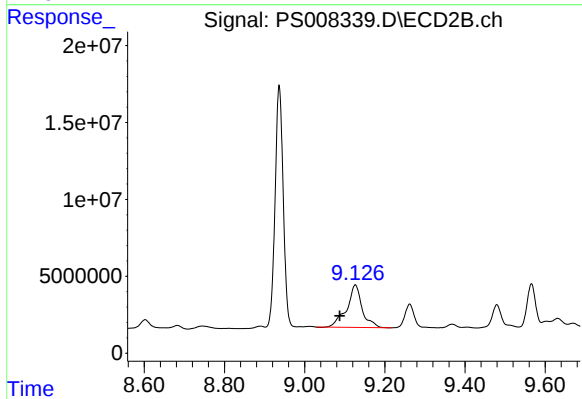

#14 DINOSEB


R.T.: 9.126 min
Delta R.T.: 0.039 min
Response: 74249575
Conc: 19.65 ng/ml

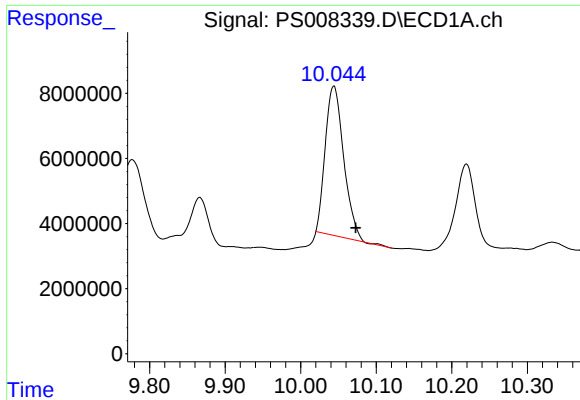

#15 Picloram

R.T.: 10.044 min
Delta R.T.: -0.029 min
Response: 78228897
Conc: 6.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

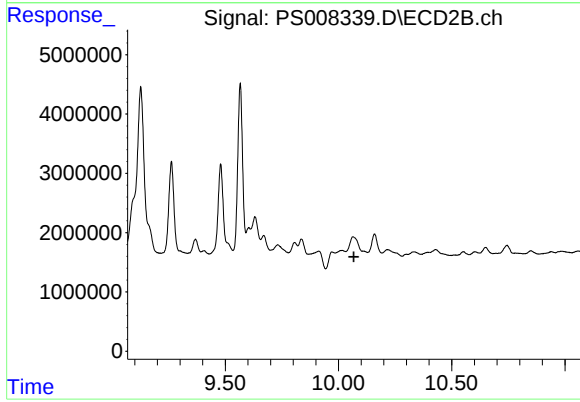

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.068 min
Response: 0
Conc: N.D.