

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010820\
 Data File : PS008341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2020 17:39
 Operator : DD\AJ
 Sample : K6456-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 03:07:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.277	5.973	1211.4E6	629.7E6	686.089	664.586
Target Compounds							
1) T	Dalapon	2.506	2.191	102.3E6	32288707	39.899	25.469 #
2) T	3,5-DICHL...	0.000	5.158	0	132.5E6	N.D.	94.809
3) T	4-Nitroph...	6.147	5.634	17766862	11777344	18.242	19.836
7) T	MCPA	0.000	6.503	0	8294300	N.D.	1.943
8) T	DICHLORPROP	0.000	6.793	0	10189393	N.D.	10.546
9) T	2,4-D	0.000	7.042	0	12284279	N.D.	10.479
10) T	Pentachlo...	7.762	0.000	28286917	0	1.164	N.D. #
12) T	2,4,5-T	8.478	0.000	277.3E6	0	30.059	N.D. #
14) T	DINOSEB	10.219	9.128	34103530	70602753	4.753	18.689 #
15) T	Picloram	10.043	0.000	69862174	0	5.597	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010820\
Data File : PS008341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2020 17:39
Operator : DD\AJ
Sample : K6456-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 03:07:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

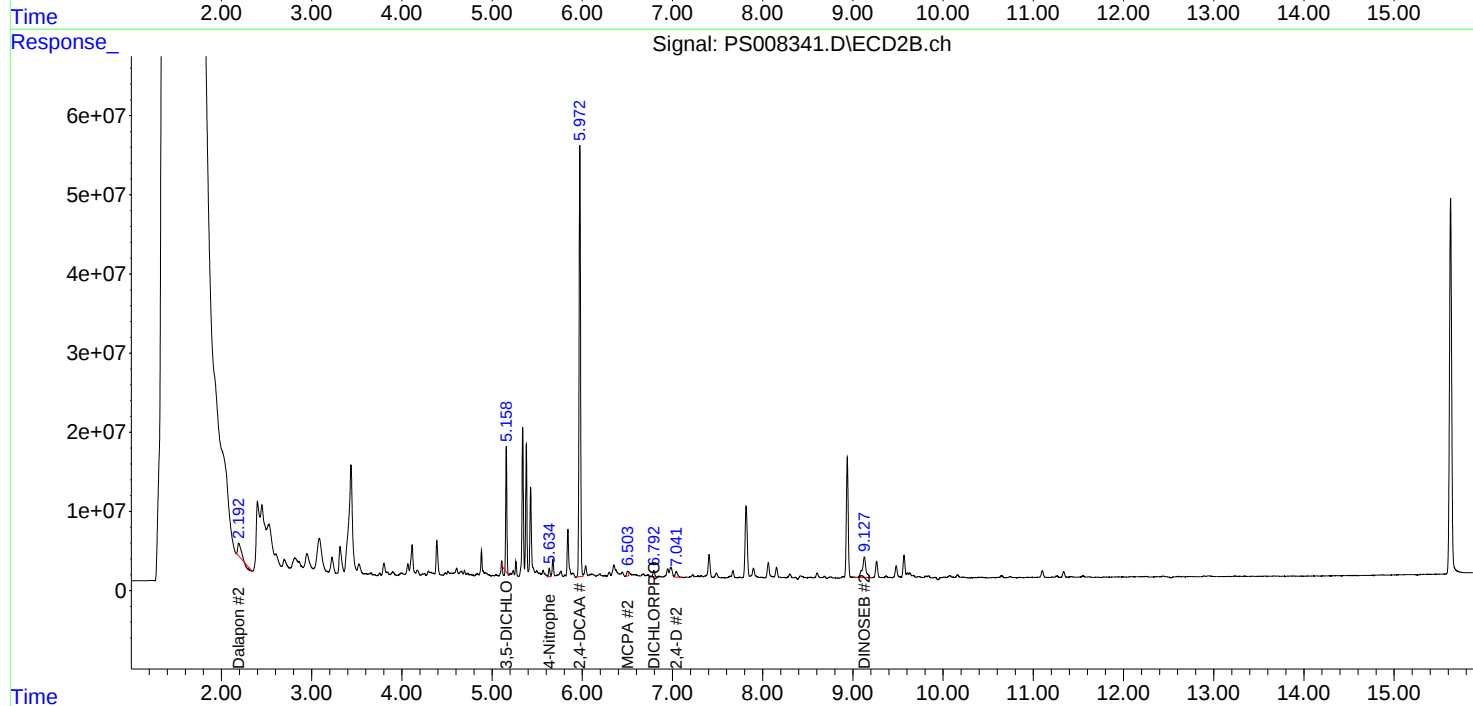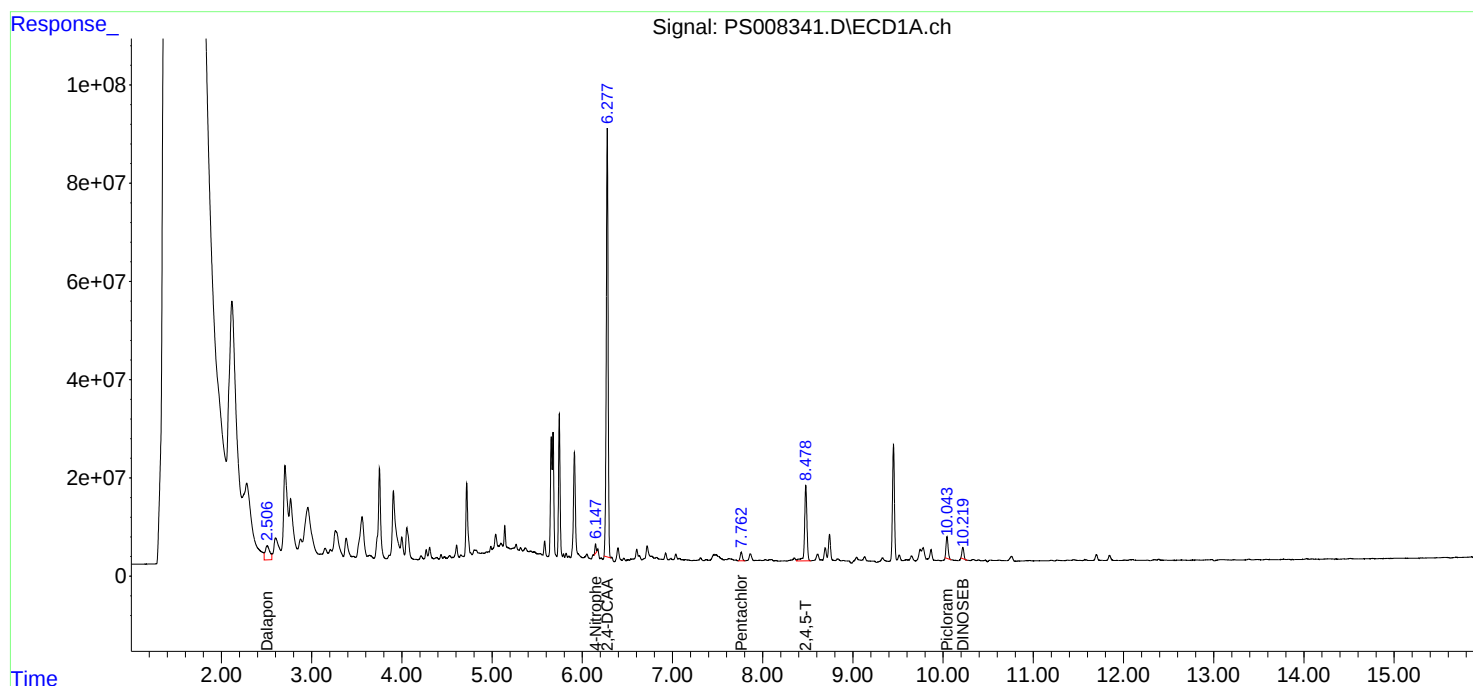


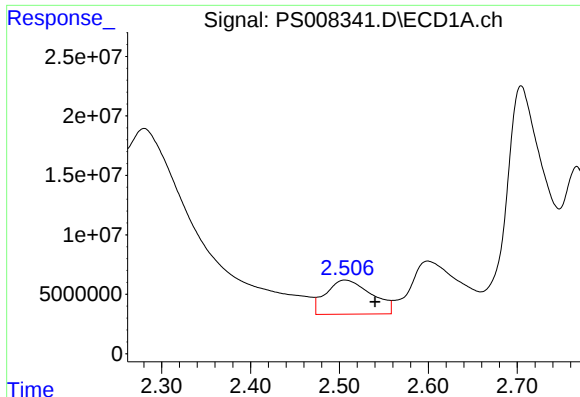

#1 Dalapon


R.T.: 2.506 min
Delta R.T.: -0.034 min
Response: 102295303
Conc: 39.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

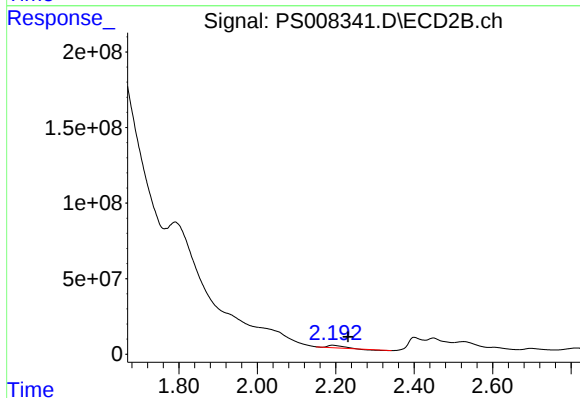


#1 Dalapon

R.T.: 2.191 min
Delta R.T.: -0.040 min
Response: 32288707
Conc: 25.47 ng/ml

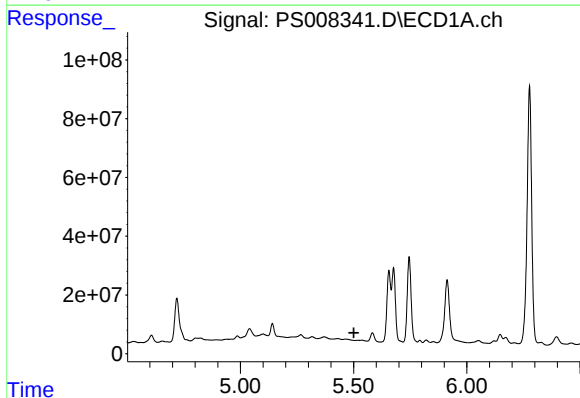


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

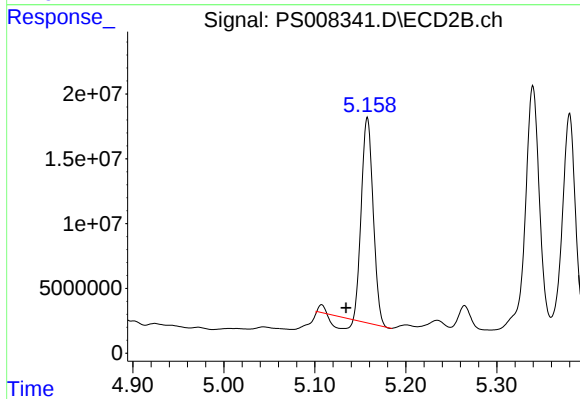

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.158 min
Delta R.T.: 0.023 min
Response: 132464372
Conc: 94.81 ng/ml

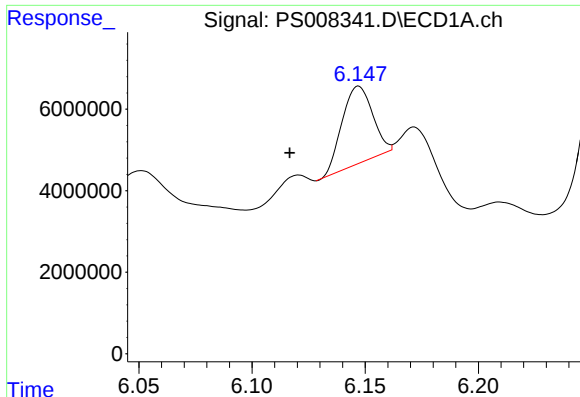

#3 4-Nitrophenol


R.T.: 6.147 min
Delta R.T.: 0.030 min
Response: 17766862
Conc: 18.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

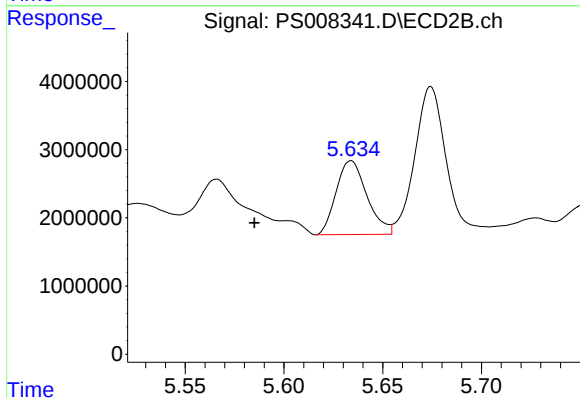


#3 4-Nitrophenol

R.T.: 5.634 min
Delta R.T.: 0.049 min
Response: 11777344
Conc: 19.84 ng/ml

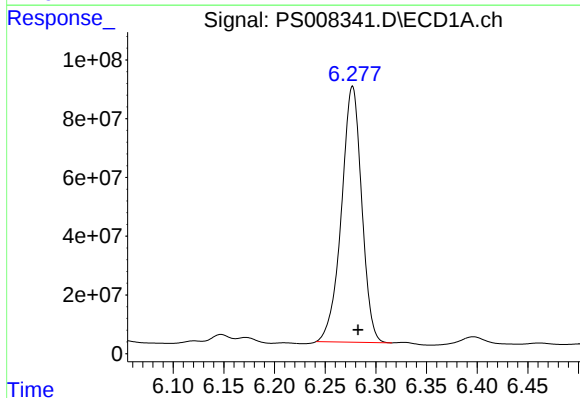


#4 2,4-DCAA

R.T.: 6.277 min
Delta R.T.: -0.006 min
Response: 1211429960
Conc: 686.09 ng/ml

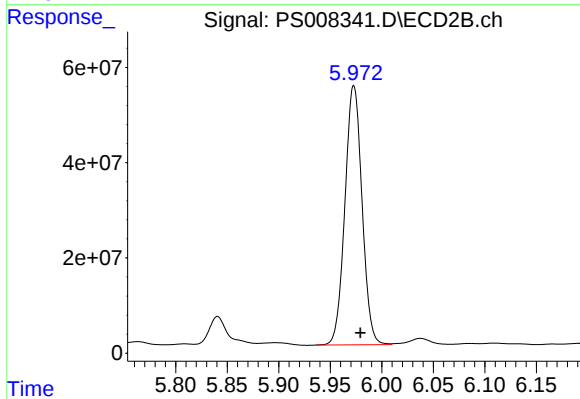

#4 2,4-DCAA


R.T.: 5.973 min
Delta R.T.: -0.006 min
Response: 629670961
Conc: 664.59 ng/ml

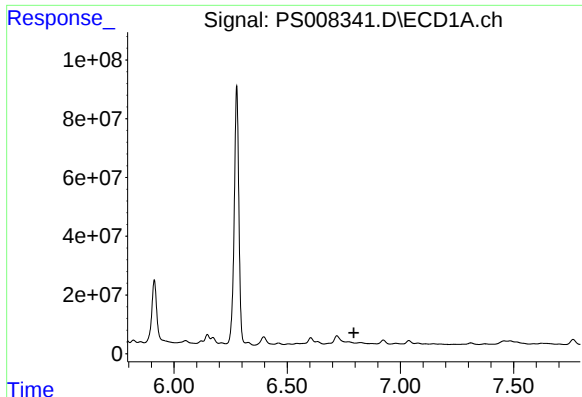

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

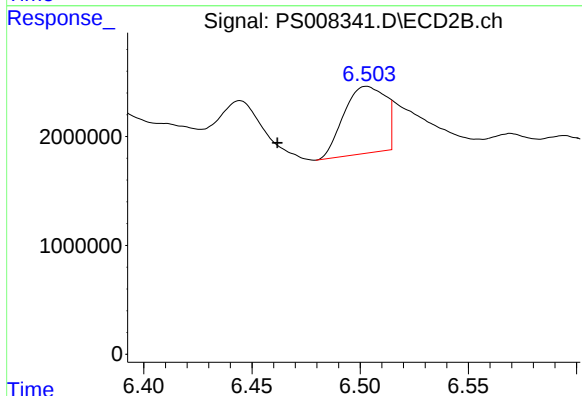


#7 MCPA

R.T.: 6.503 min
Delta R.T.: 0.042 min
Response: 8294300
Conc: 1.94 ug/ml

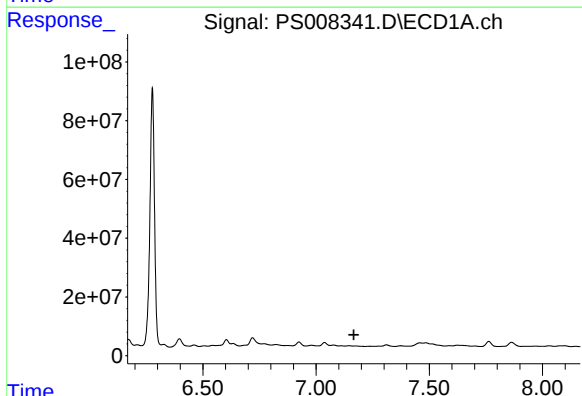


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

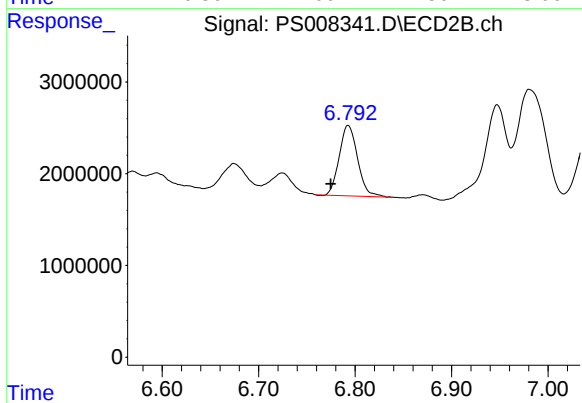

#8 DICHLORPROP


R.T.: 6.793 min
Delta R.T.: 0.018 min
Response: 10189393
Conc: 10.55 ng/ml

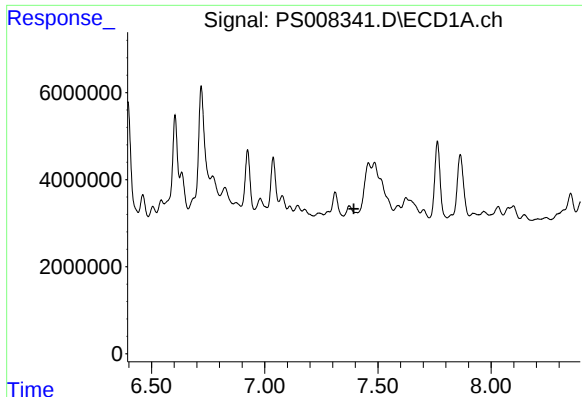

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

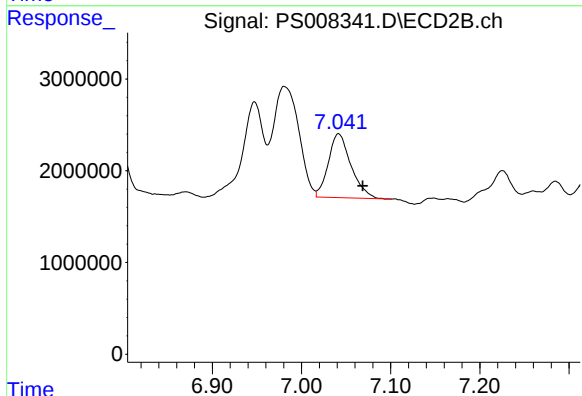


#9 2,4-D

R.T.: 7.042 min
Delta R.T.: -0.027 min
Response: 12284279
Conc: 10.48 ng/ml

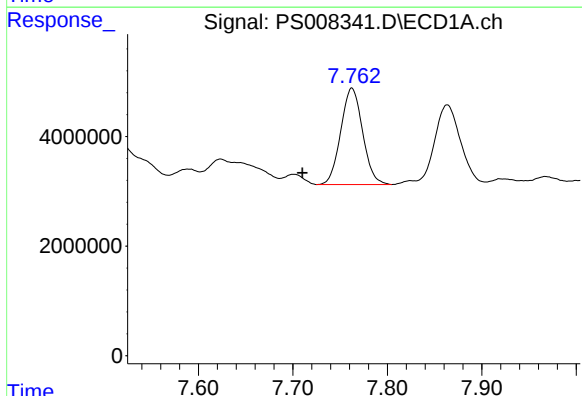


#10 Pentachlorophenol

R.T.: 7.762 min
Delta R.T.: 0.052 min
Response: 28286917
Conc: 1.16 ng/ml

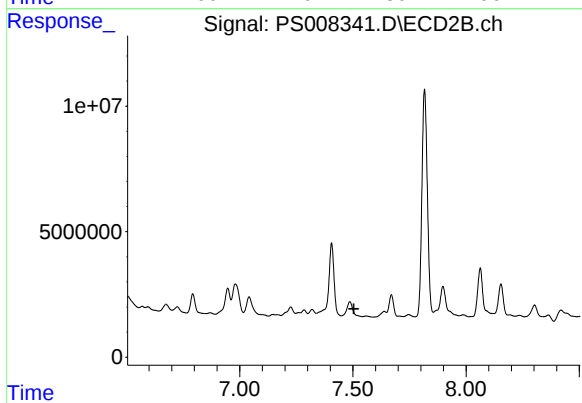

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 7.505 min
Response: 0
Conc: N.D.

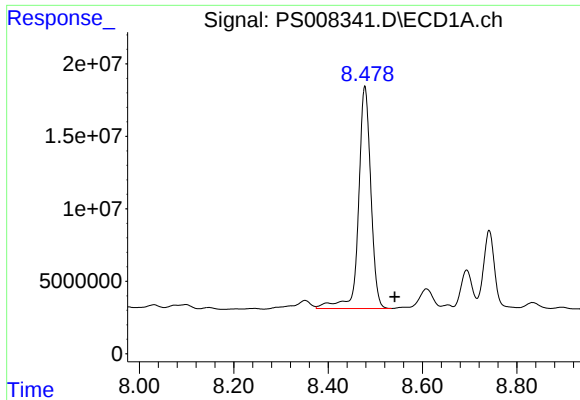

#12 2,4,5-T


R.T.: 8.478 min
Delta R.T.: -0.063 min
Response: 277340408
Conc: 30.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

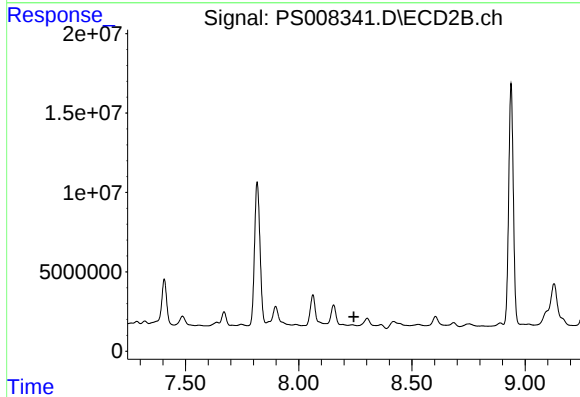


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.243 min
Response: 0
Conc: N.D.

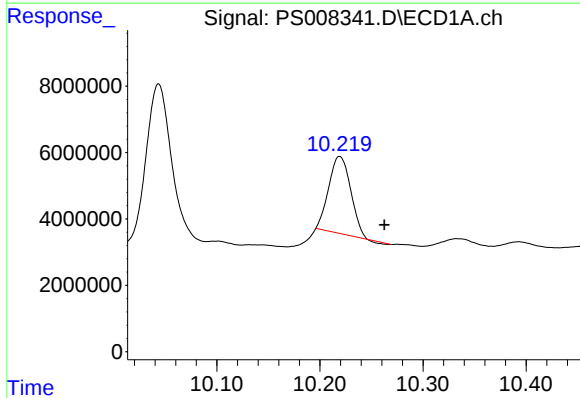


#14 DINOSEB

R.T.: 10.219 min
Delta R.T.: -0.043 min
Response: 34103530
Conc: 4.75 ng/ml

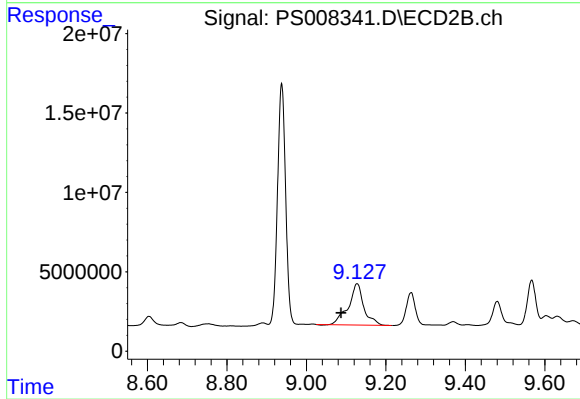

#14 DINOSEB


R.T.: 9.128 min
Delta R.T.: 0.040 min
Response: 70602753
Conc: 18.69 ng/ml

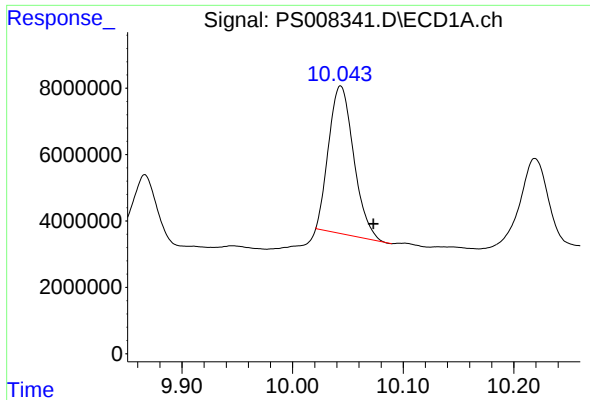

#15 Picloram

R.T.: 10.043 min
Delta R.T.: -0.030 min
Response: 69862174
Conc: 5.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

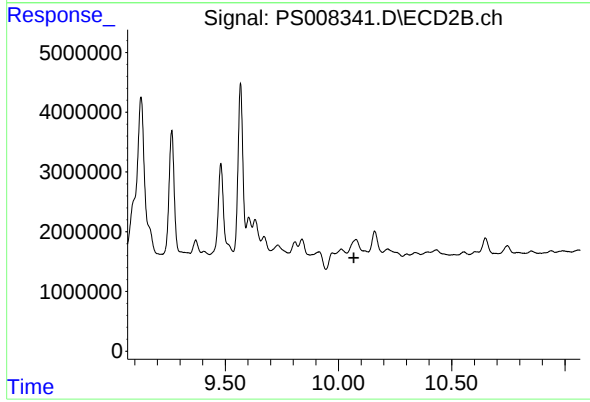

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.068 min
Response: 0
Conc: N.D.