

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010820\
 Data File : PS008346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2020 19:29
 Operator : DD\AJ
 Sample : L1039-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 03:09:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.289	5.969	1277.9E6	658.0E6	723.718	694.471
Target Compounds							
1) T	Dalapon	2.519	2.188	105.4E6	44480877	41.117	35.087
2) T	3,5-DICHL...	0.000	5.154	0	138.3E6	N.D.	98.956
3) T	4-Nitroph...	6.159	5.630	10637497	8345050	10.922	14.055 #
7) T	MCPA	6.730	6.496	24478957	2500223	3.350	<MDL #
8) T	DICHLORPROP	0.000	6.789	0	8718628	N.D.	9.024
10) T	Pentachlo...	7.774	0.000	26431663	0	1.087	N.D. #
12) T	2,4,5-T	8.489	0.000	259.9E6	0	28.168	N.D. #
13) T	2,4-DB	9.052	0.000	14560045	0	10.503	N.D. #
14) T	DINOSEB	10.231	9.123	47131271	74814519	6.569	19.804 #
15) T	Picloram	10.055	0.000	83725619	0	6.708	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010820\
Data File : PS008346.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2020 19:29
Operator : DD\AJ
Sample : L1039-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 03:09:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

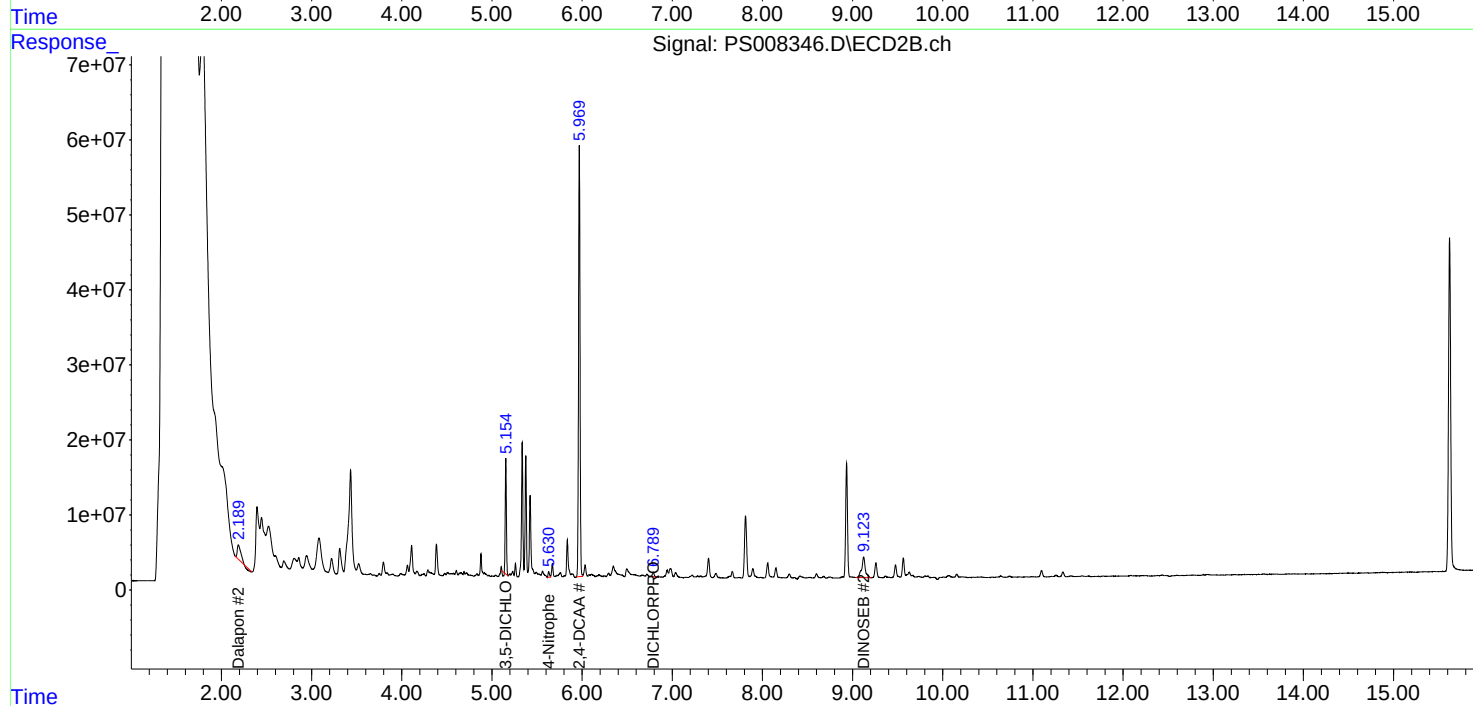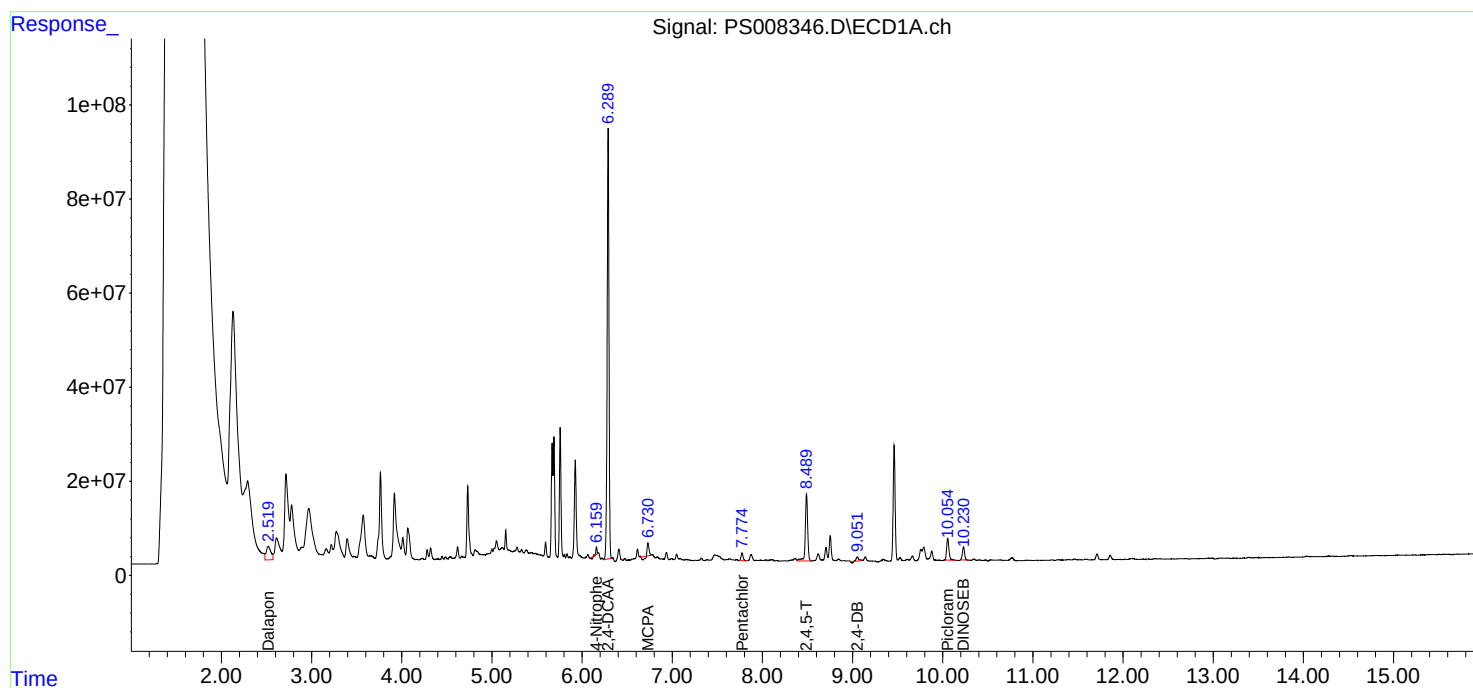


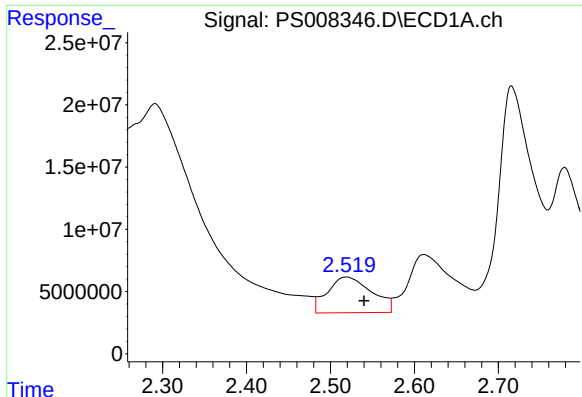

#1 Dalapon


R.T.: 2.519 min
Delta R.T.: -0.021 min
Response: 105418552
Conc: 41.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

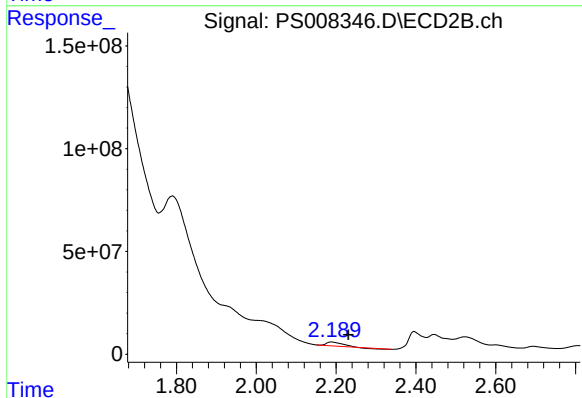


#1 Dalapon

R.T.: 2.188 min
Delta R.T.: -0.043 min
Response: 44480877
Conc: 35.09 ng/ml

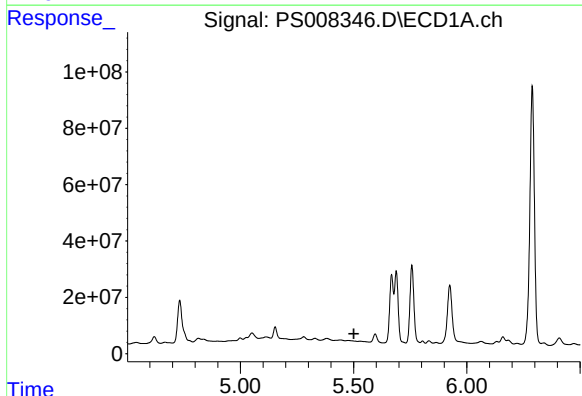


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

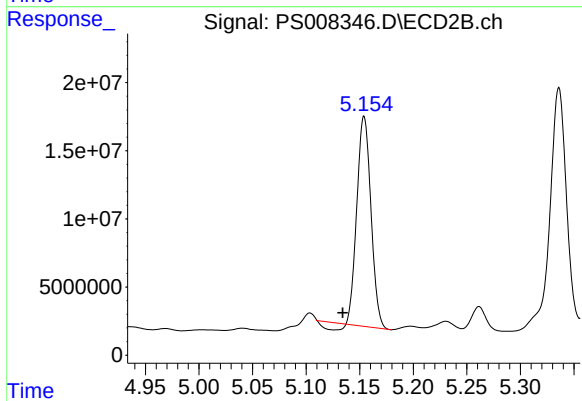

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.154 min
Delta R.T.: 0.020 min
Response: 138258428
Conc: 98.96 ng/ml

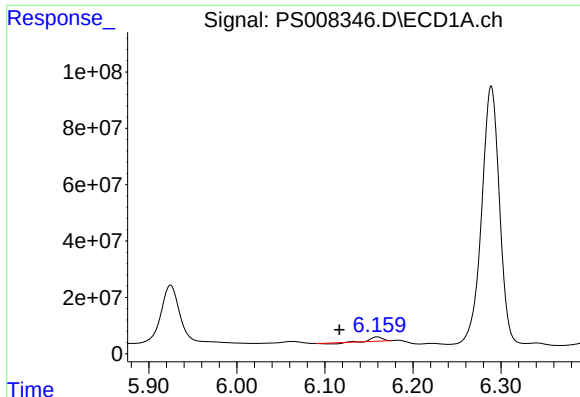

#3 4-Nitrophenol


R.T.: 6.159 min
Delta R.T.: 0.043 min
Response: 10637497
Conc: 10.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

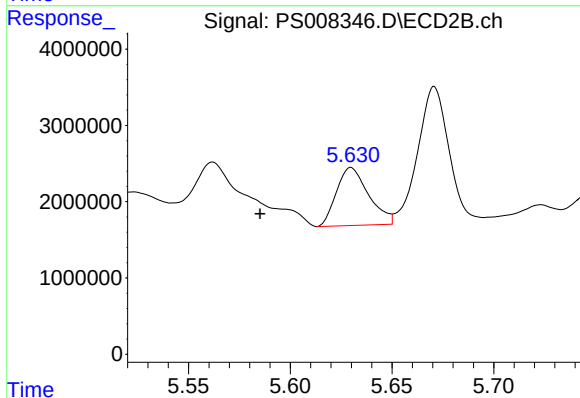


#3 4-Nitrophenol

R.T.: 5.630 min
Delta R.T.: 0.045 min
Response: 8345050
Conc: 14.05 ng/ml

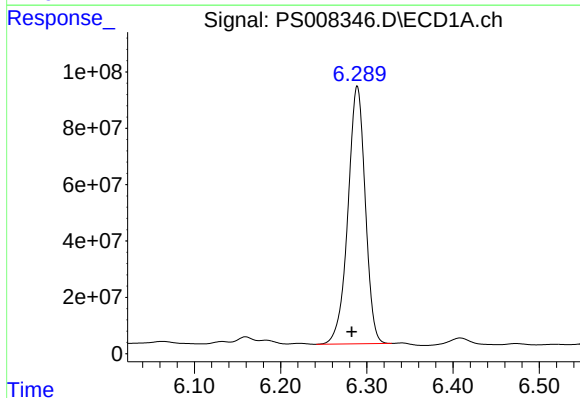


#4 2,4-DCAA

R.T.: 6.289 min
Delta R.T.: 0.006 min
Response: 1277871117
Conc: 723.72 ng/ml

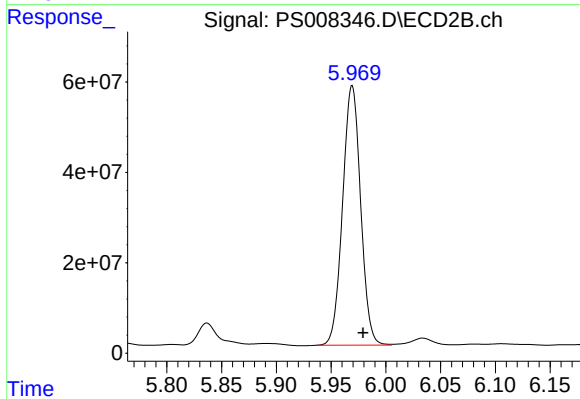

#4 2,4-DCAA


R.T.: 5.969 min
Delta R.T.: -0.010 min
Response: 657985667
Conc: 694.47 ng/ml

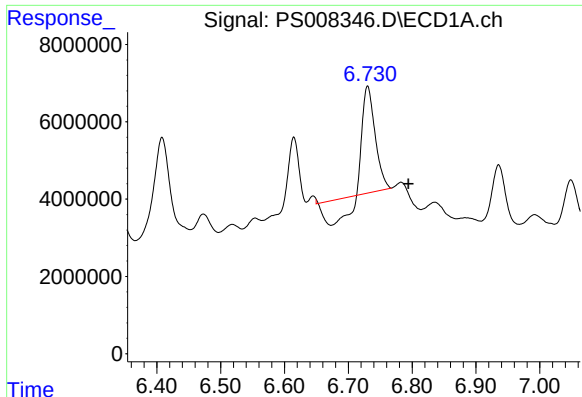

#7 MCPA


R.T.: 6.730 min
Delta R.T.: -0.064 min
Response: 24478957
Conc: 3.35 ug/ml

Instrument :
ECD_S
ClientSampleId :

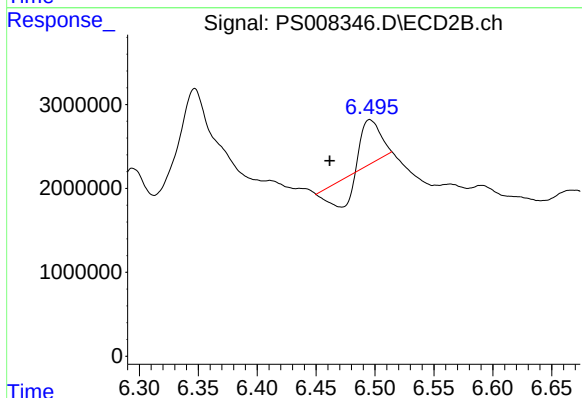


#7 MCPA

R.T.: 6.496 min
Delta R.T.: 0.034 min
Response: 2500223
Conc: N.D.

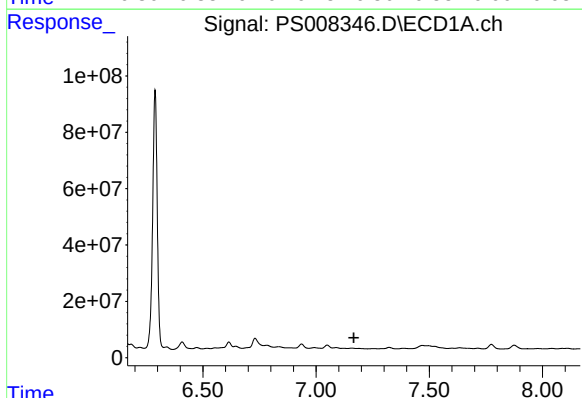


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

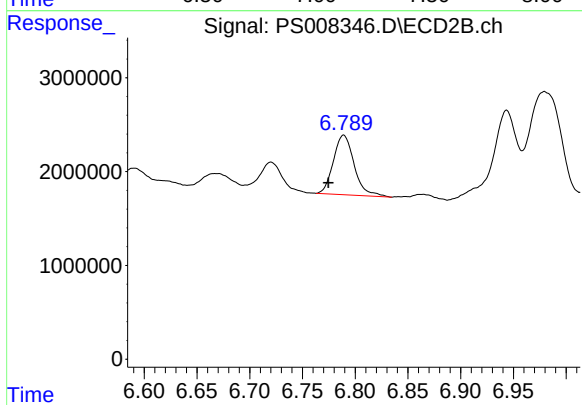

#8 DICHLORPROP


R.T.: 6.789 min
Delta R.T.: 0.014 min
Response: 8718628
Conc: 9.02 ng/ml

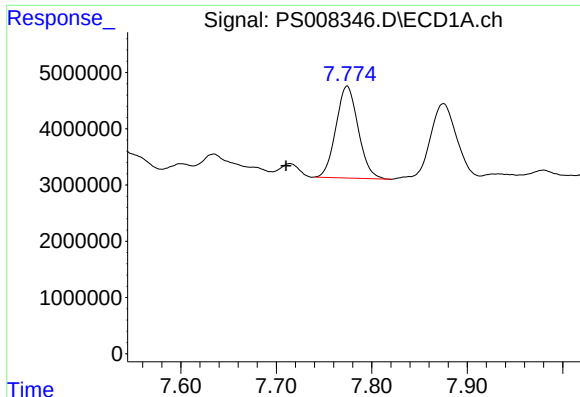

#10 Pentachlorophenol


R.T.: 7.774 min
Delta R.T.: 0.064 min
Response: 26431663
Conc: 1.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

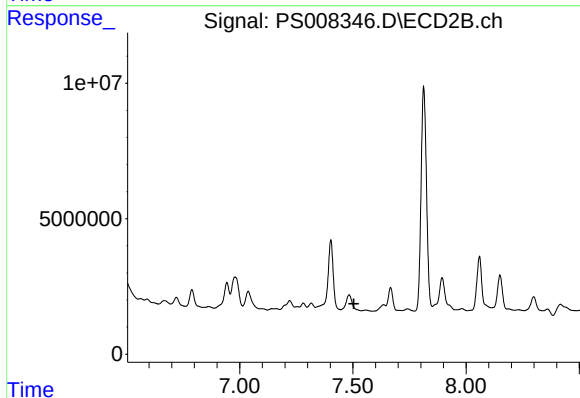


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

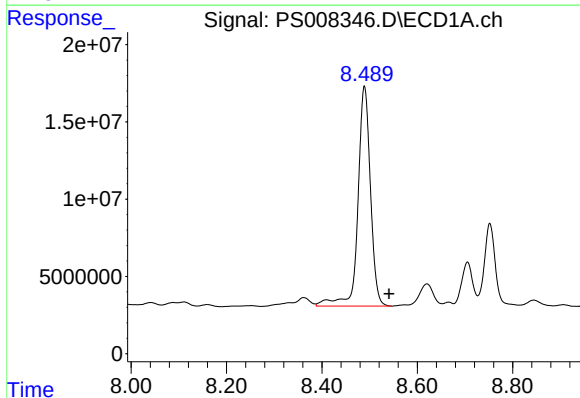


#12 2,4,5-T

R.T.: 8.489 min
Delta R.T.: -0.052 min
Response: 259889306
Conc: 28.17 ng/ml

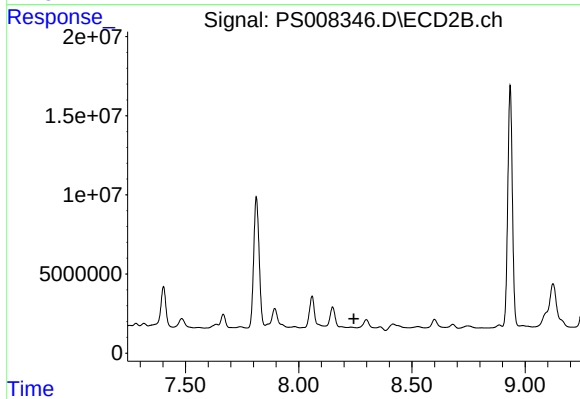

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.243 min
Response: 0
Conc: N.D.

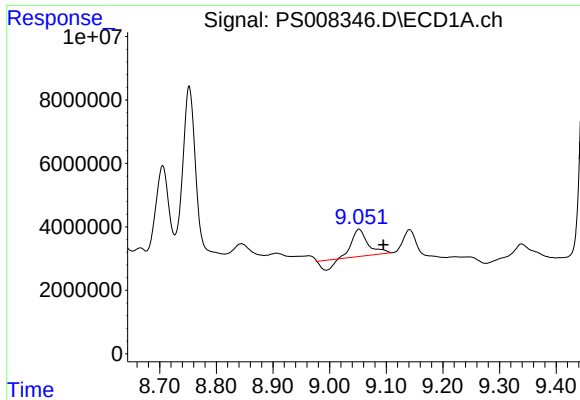

#13 2,4-DB


R.T.: 9.052 min
Delta R.T.: -0.043 min
Response: 14560045
Conc: 10.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

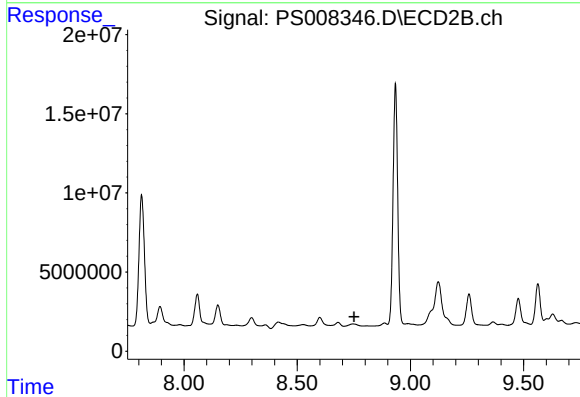


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

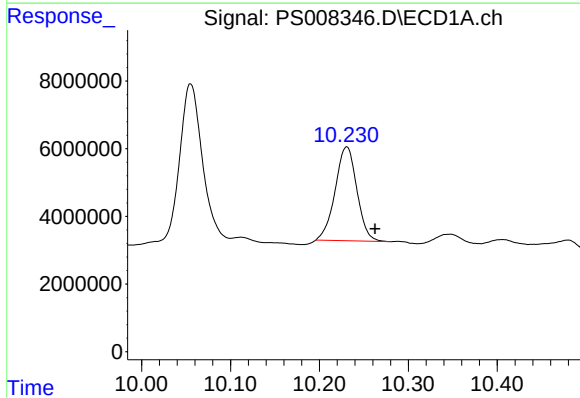


#14 DINOSEB

R.T.: 10.231 min
Delta R.T.: -0.032 min
Response: 47131271
Conc: 6.57 ng/ml

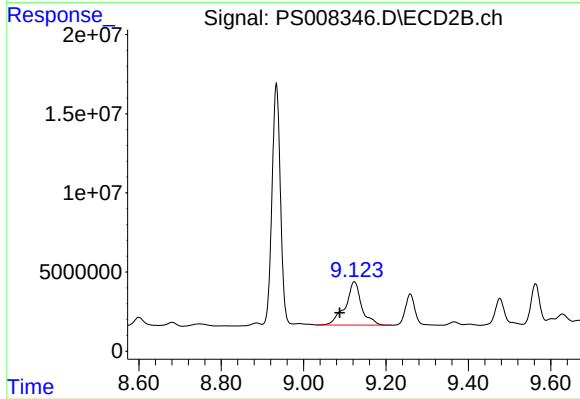

#14 DINOSEB


R.T.: 9.123 min
Delta R.T.: 0.035 min
Response: 74814519
Conc: 19.80 ng/ml

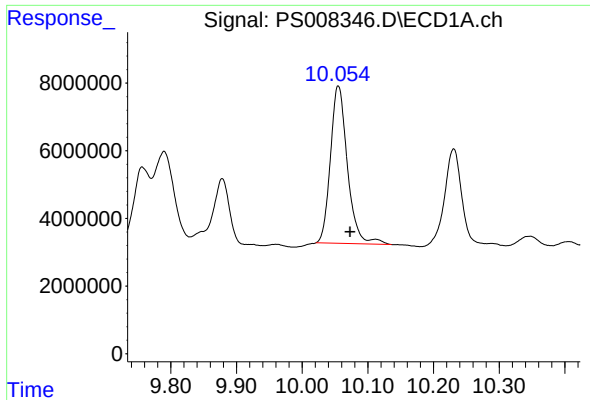

#15 Picloram

R.T.: 10.055 min
Delta R.T.: -0.018 min
Response: 83725619
Conc: 6.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

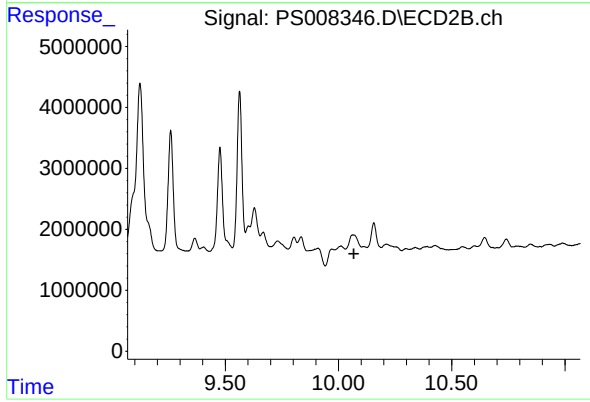

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.068 min
Response: 0
Conc: N.D.