

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010820\
 Data File : PS008331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2020 09:59
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 10:23:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 10:23:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.283	5.979	1357.8E6	731.5E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.540	2.231	1822.6E6	911.3E6	682.500	682.500
2) T	3,5-DICHL...	5.501	5.134	1716.2E6	1007.4E6	697.500	697.500
3) T	4-Nitroph...	6.117	5.585	689.2E6	421.0E6	682.500	682.500
5) T	DICAMBA	6.476	6.150	5000.6E6	2929.8E6	705.000	705.000
6) T	MCPD	6.645	6.246	379.0E6	224.1E6	70.500	70.500
7) T	MCPA	6.794	6.462	533.9E6	312.0E6	69.750	69.750
8) T	DICHLORPROP	7.167	6.775	1185.5E6	701.0E6	705.000	705.000
9) T	2,4-D	7.394	7.069	1314.7E6	852.4E6	705.000	705.000
10) T	Pentachlo...	7.710	7.505	17761.9E6	9894.8E6	712.500	712.500
11) T	2,4,5-TP ...	8.258	7.864	6839.3E6	3863.6E6	712.500	712.500
12) T	2,4,5-T	8.541	8.243	6792.3E6	3908.6E6	712.500	712.500
13) T	2,4-DB	9.095	8.751	1024.6E6	523.0E6	712.500	712.500
14) T	DINOSEB	10.263	9.088	5200.8E6	2771.3E6	705.000	705.000
15) T	Picloram	10.073	10.068	9492.2E6	5672.5E6	712.500	712.500
16) T	DCPA	10.527	10.019	8816.9E6	4855.0E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010820\
Data File : PS008331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2020 09:59
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 10:23:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 10:23:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

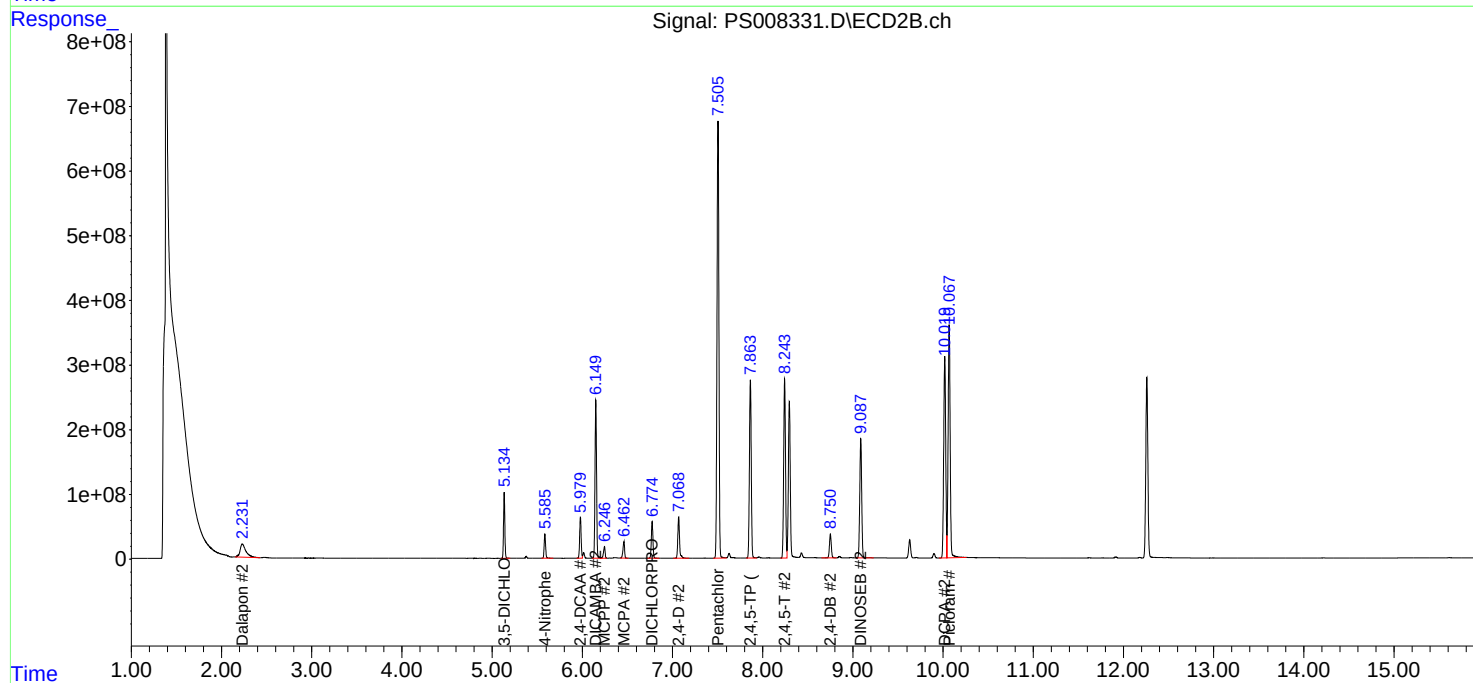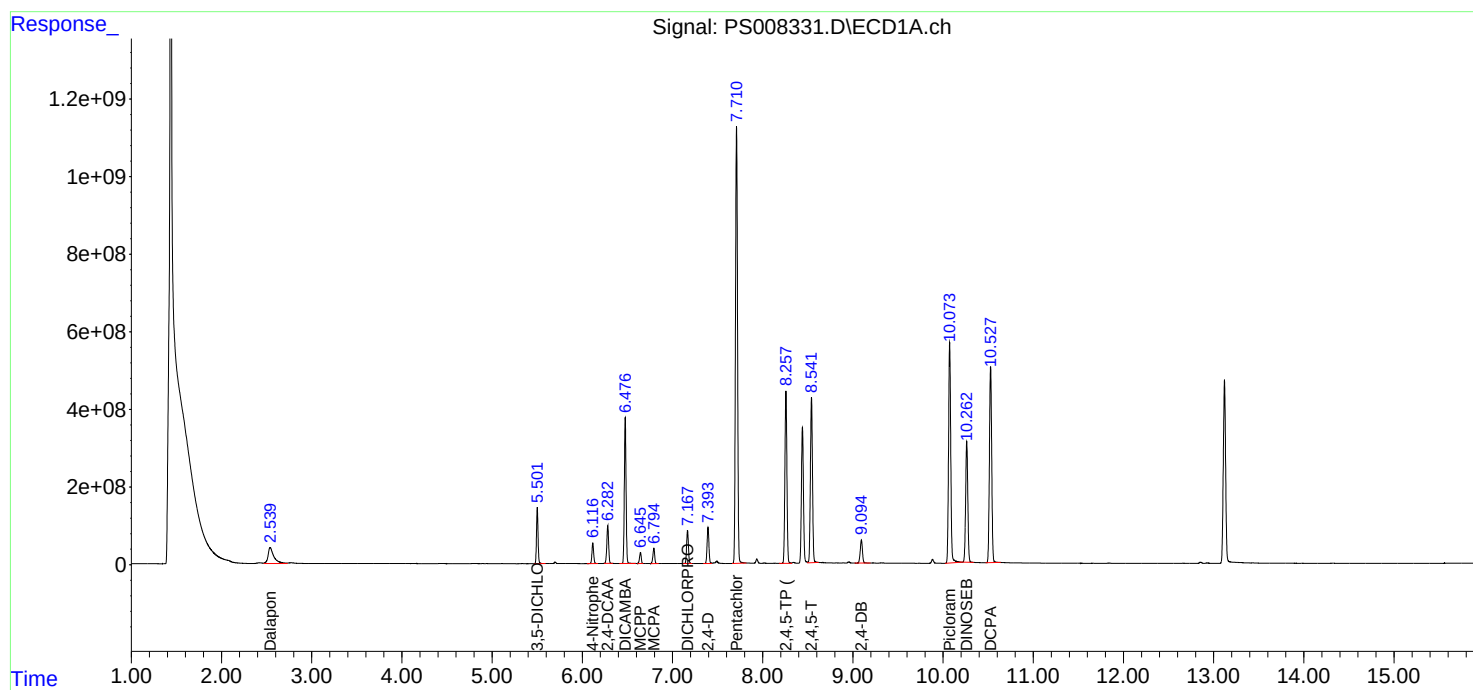


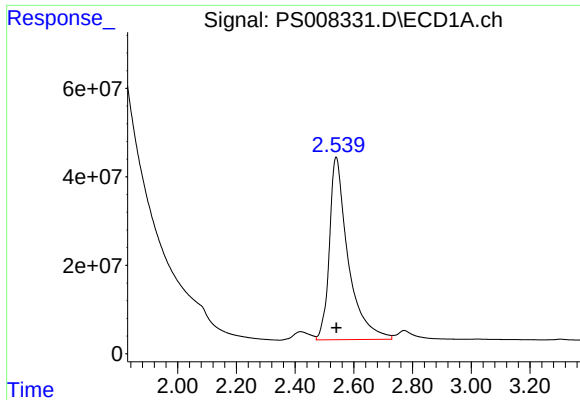

#1 Dalapon


R.T.: 2.540 min
Delta R.T.: 0.000 min
Response: 1822635957
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

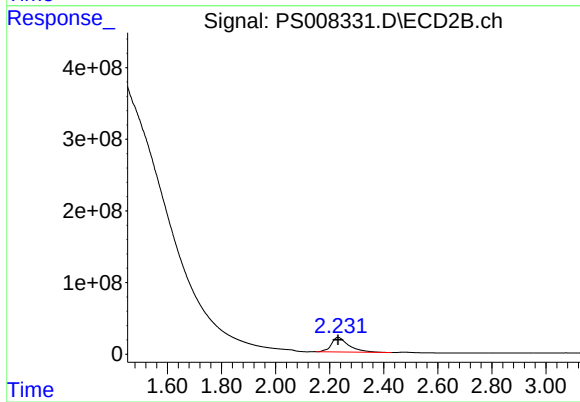


#1 Dalapon

R.T.: 2.231 min
Delta R.T.: 0.000 min
Response: 911277476
Conc: 682.50 ng/ml

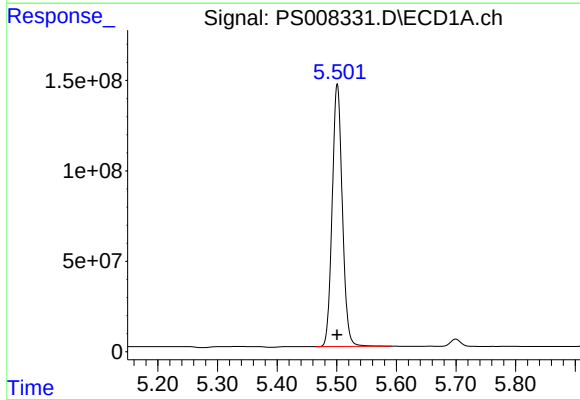


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 1716195661
Conc: 697.50 ng/ml

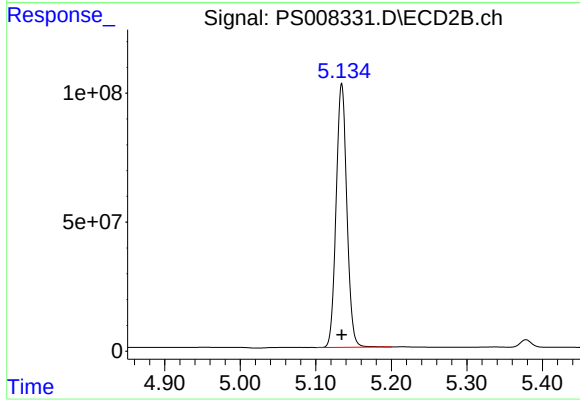

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.134 min
Delta R.T.: 0.000 min
Response: 1007368790
Conc: 697.50 ng/ml

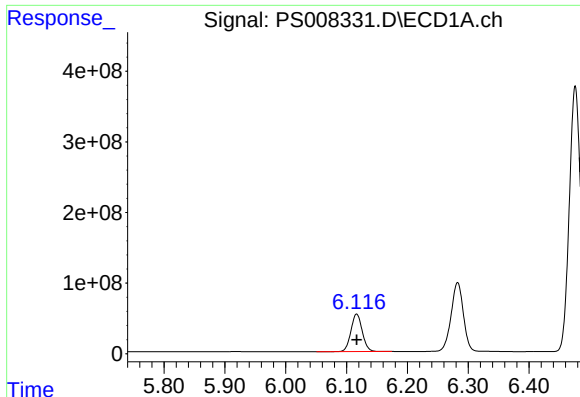

#3 4-Nitrophenol


R.T.: 6.117 min
Delta R.T.: 0.000 min
Response: 689166934
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

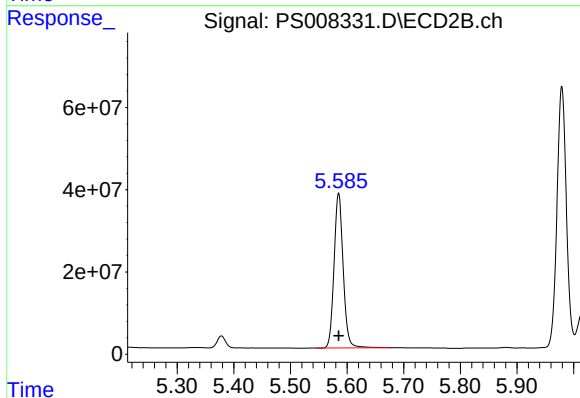


#3 4-Nitrophenol

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 420971956
Conc: 682.50 ng/ml

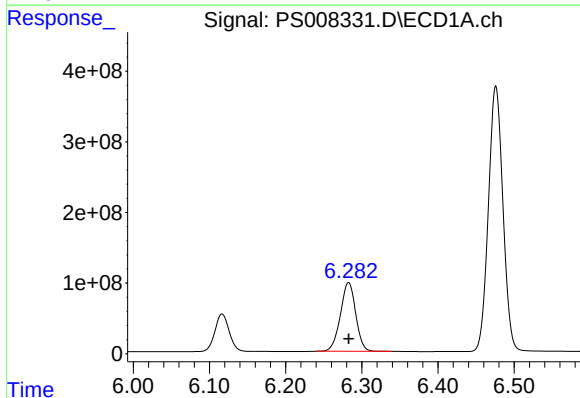


#4 2,4-DCAA

R.T.: 6.283 min
Delta R.T.: 0.000 min
Response: 1357839913
Conc: 750.00 ng/ml

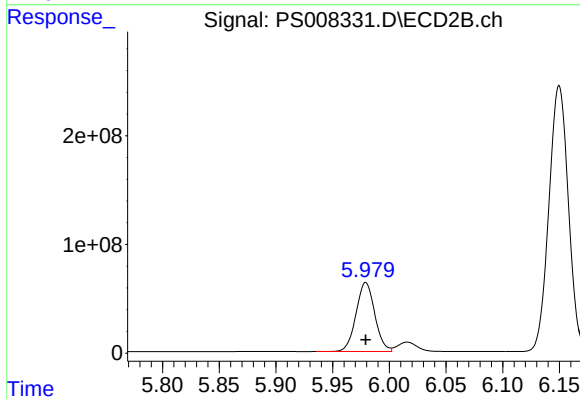

#4 2,4-DCAA


R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 731505900
Conc: 750.00 ng/ml

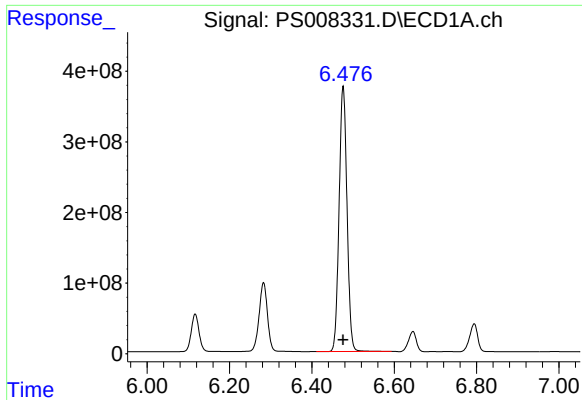

#5 DICAMBA


R.T.: 6.476 min
Delta R.T.: 0.000 min
Response: 5000630278
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

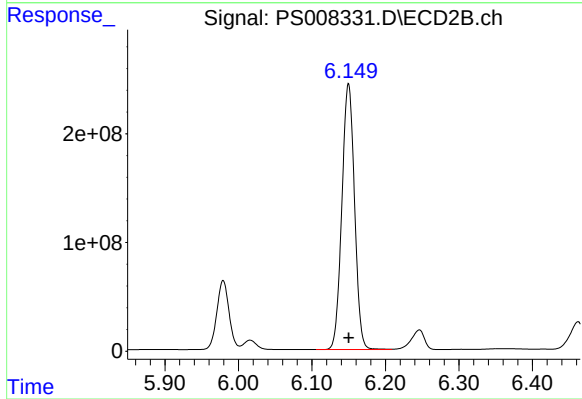


#5 DICAMBA

R.T.: 6.150 min
Delta R.T.: 0.000 min
Response: 2929799031
Conc: 705.00 ng/ml

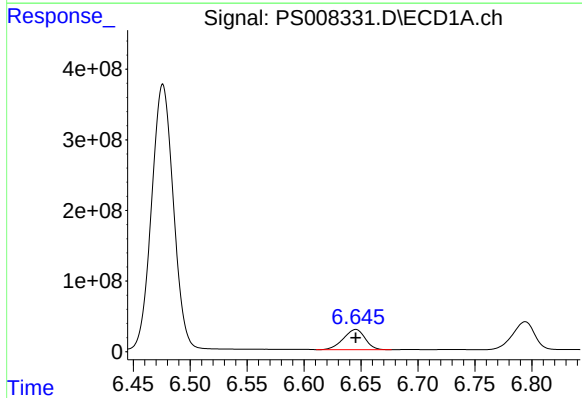


#6 MCP

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 378960311
Conc: 70.50 ug/ml

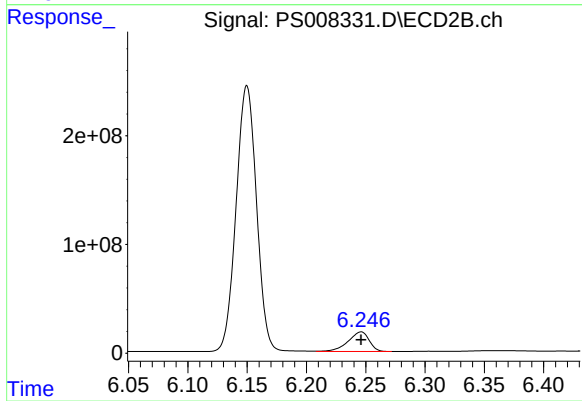

#6 MCP


R.T.: 6.246 min
Delta R.T.: 0.000 min
Response: 224147286
Conc: 70.50 ug/ml

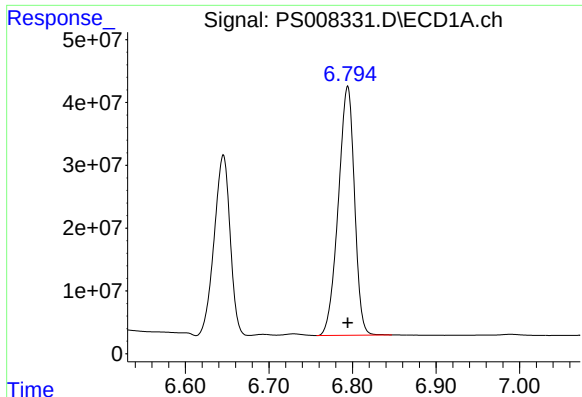

#7 MCPA


R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 533871349
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

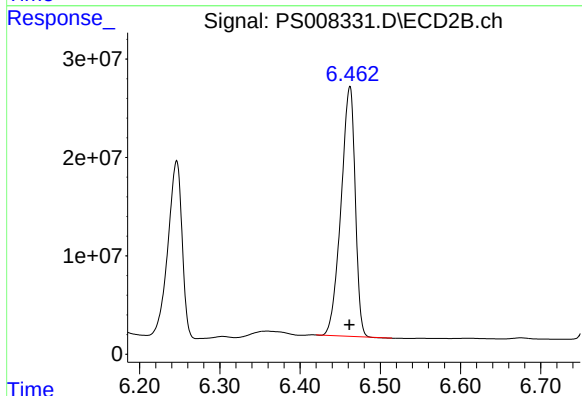


#7 MCPA

R.T.: 6.462 min
Delta R.T.: 0.000 min
Response: 312014739
Conc: 69.75 ug/ml

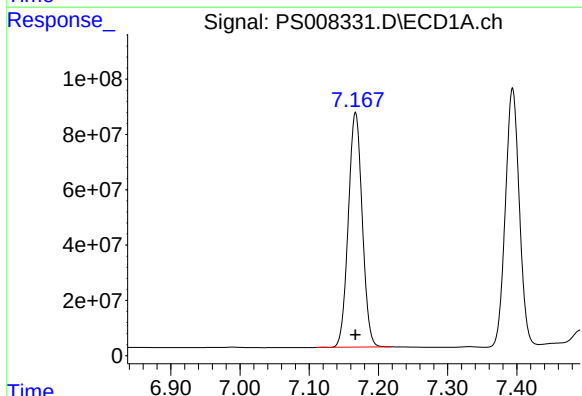


#8 DICHLORPROP

R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 1185504146
Conc: 705.00 ng/ml

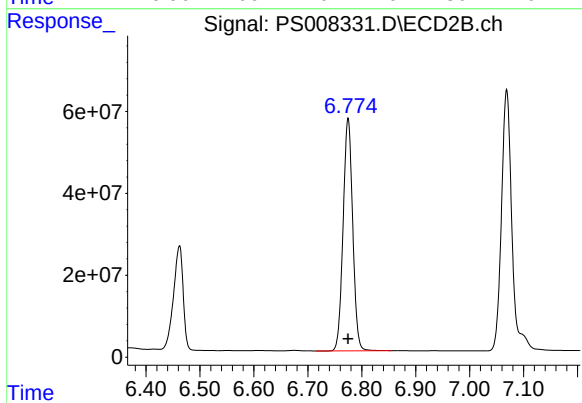

#8 DICHLORPROP


R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 701016144
Conc: 705.00 ng/ml

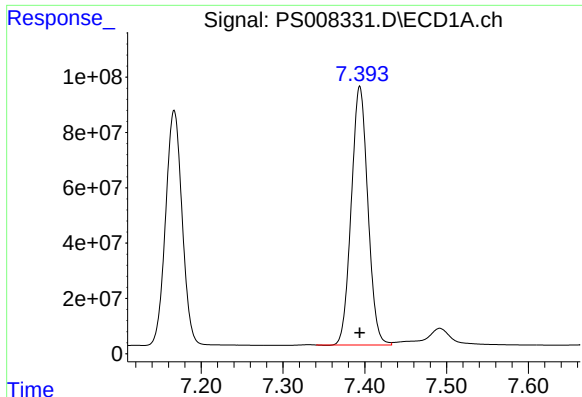

#9 2,4-D


R.T.: 7.394 min
Delta R.T.: 0.000 min
Response: 1314725726
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

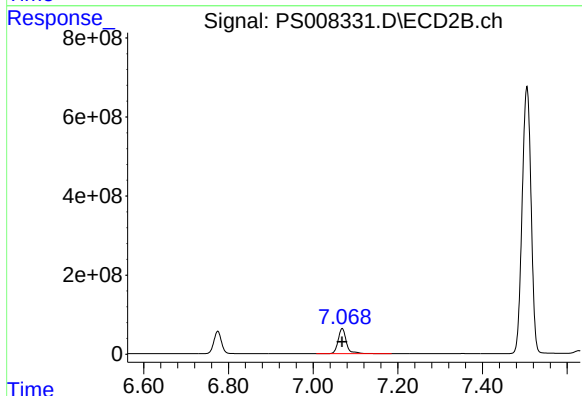


#9 2,4-D

R.T.: 7.069 min
Delta R.T.: 0.000 min
Response: 852387441
Conc: 705.00 ng/ml

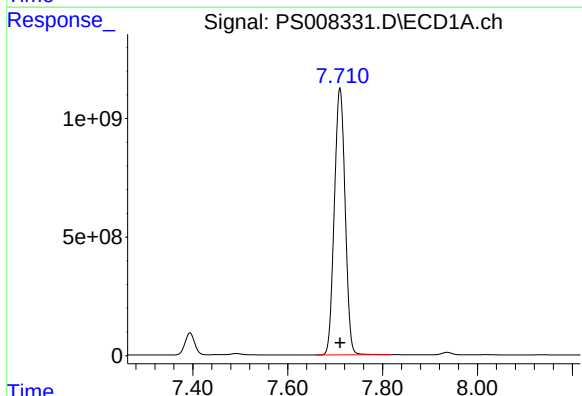


#10 Pentachlorophenol

R.T.: 7.710 min
Delta R.T.: 0.000 min
Response: 17761935514
Conc: 712.50 ng/ml

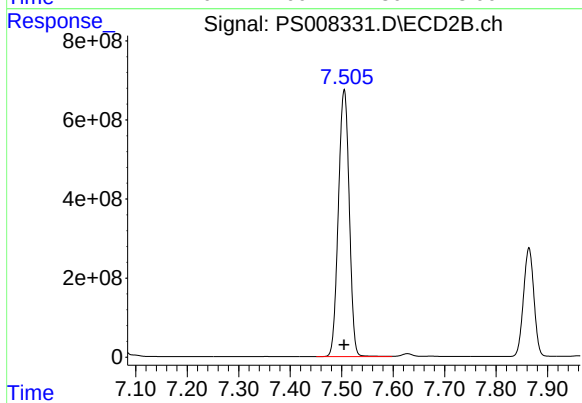

#10 Pentachlorophenol


R.T.: 7.505 min
Delta R.T.: 0.000 min
Response: 9894757110
Conc: 712.50 ng/ml

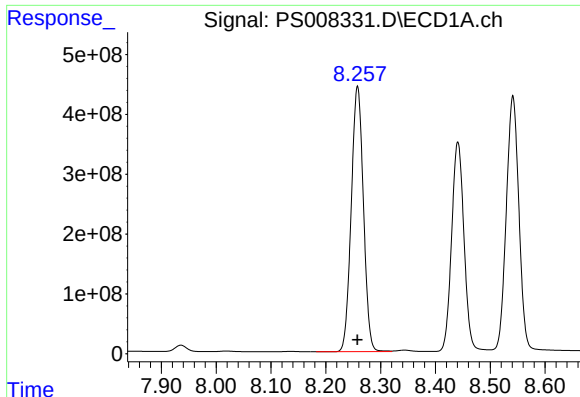

#11 2,4,5-TP (SILVEX)


R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 6839310825
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

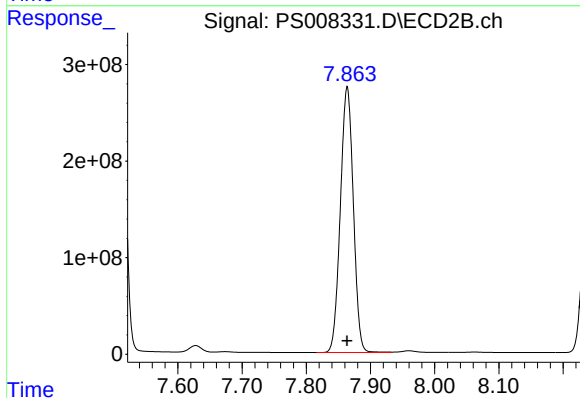


#11 2,4,5-TP (SILVEX)

R.T.: 7.864 min
Delta R.T.: 0.000 min
Response: 3863624059
Conc: 712.50 ng/ml

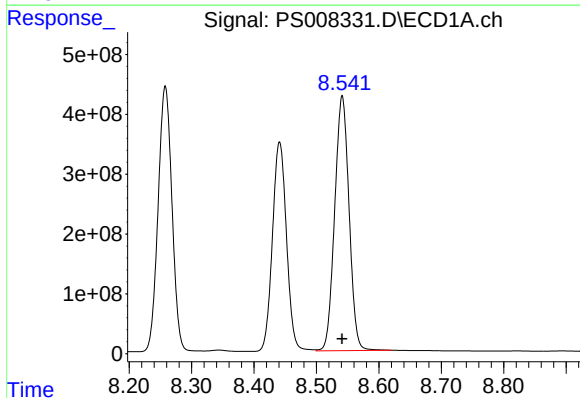


#12 2,4,5-T

R.T.: 8.541 min
Delta R.T.: 0.000 min
Response: 6792336002
Conc: 712.50 ng/ml

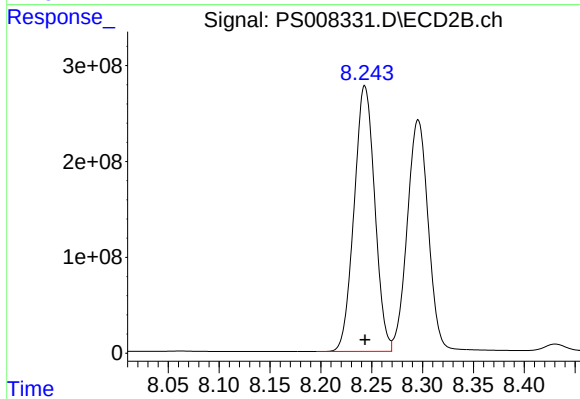

#12 2,4,5-T


R.T.: 8.243 min
Delta R.T.: 0.000 min
Response: 3908627558
Conc: 712.50 ng/ml

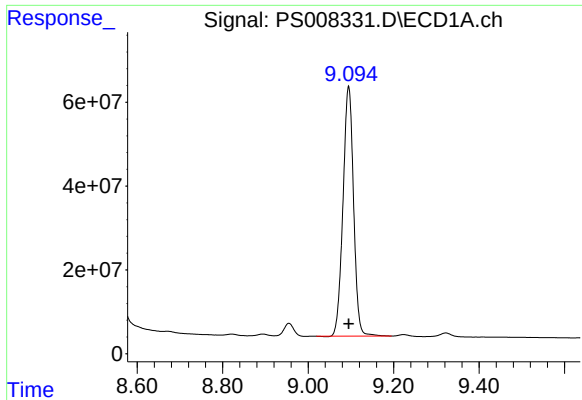

#13 2,4-DB


R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 1024557894
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

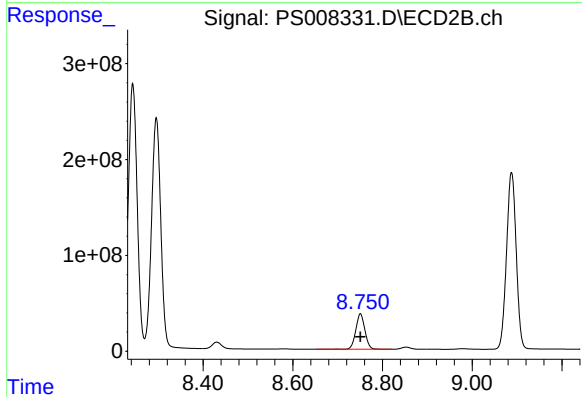


#13 2,4-DB

R.T.: 8.751 min
Delta R.T.: 0.000 min
Response: 522972496
Conc: 712.50 ng/ml

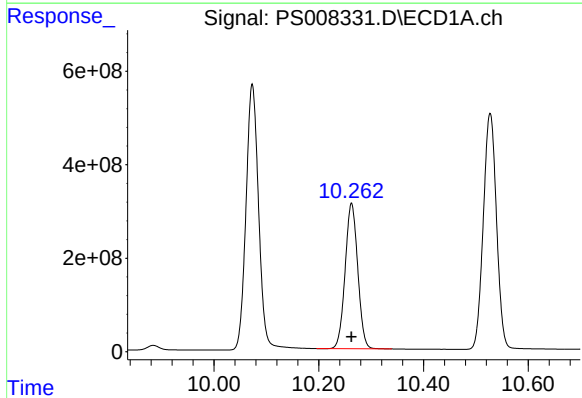


#14 DINOSEB

R.T.: 10.263 min
Delta R.T.: 0.000 min
Response: 5200799055
Conc: 705.00 ng/ml

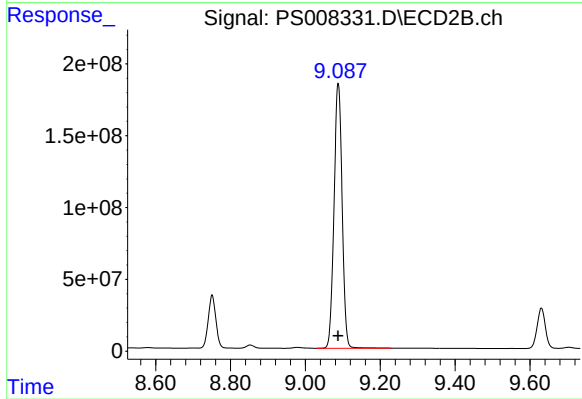

#14 DINOSEB


R.T.: 9.088 min
Delta R.T.: 0.000 min
Response: 2771348699
Conc: 705.00 ng/ml

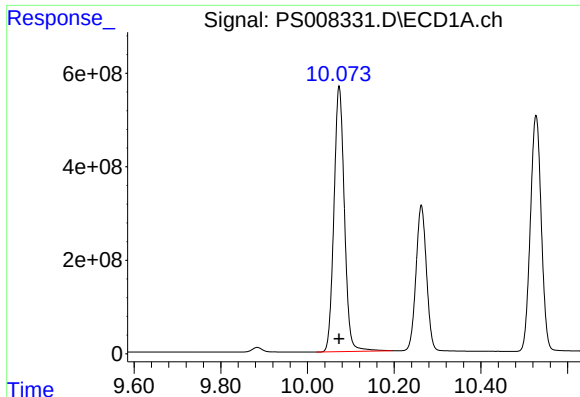

#15 Picloram


R.T.: 10.073 min
Delta R.T.: 0.000 min
Response: 9492199215
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

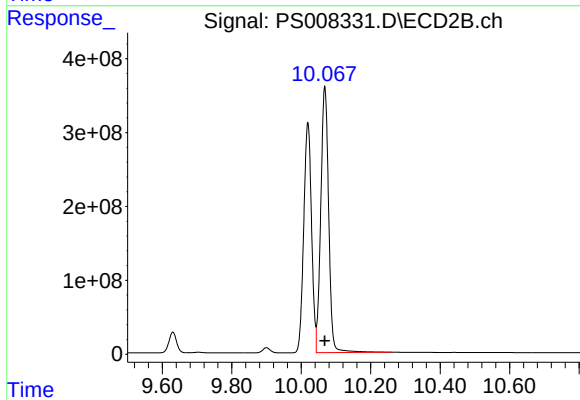


#15 Picloram

R.T.: 10.068 min
Delta R.T.: 0.000 min
Response: 5672452109
Conc: 712.50 ng/ml

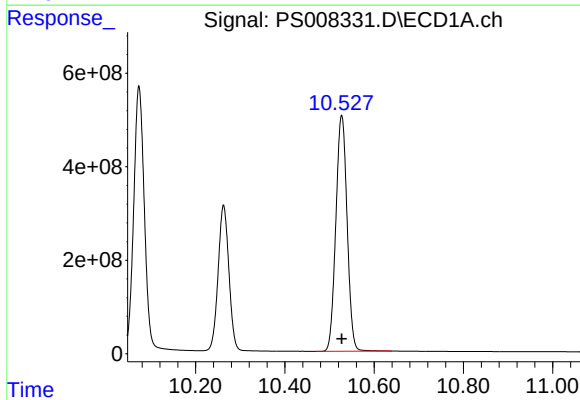

#16 DCPA

R.T.: 10.527 min
Delta R.T.: 0.000 min
Response: 8816879923
Conc: 720.00 ng/ml

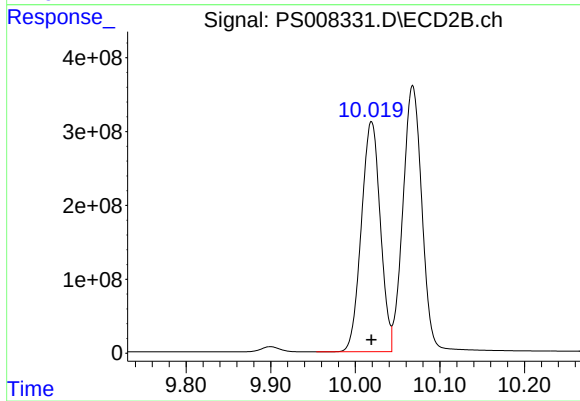

#16 DCPA

R.T.: 10.019 min
Delta R.T.: 0.000 min
Response: 4855006073
Conc: 720.00 ng/ml